

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
 Data File : BN015103.D
 Acq On : 26 Jun 2021 06:51
 Operator : CG/JU
 Sample : M2704-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGDB7

Quant Time: Jun 26 07:28:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 24 14:43:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	171802	20.000	ng/ul	0.00
20) Naphthalene-d8	10.499	136	705421	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.351	164	427961	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	863761	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	824272	20.000	ng/ul	0.00
88) Perylene-d12	23.539	264	885605	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	16710	3.785	ng/uL	0.00
4) Pyridine-d5	3.675	84	170396	14.315	ng/ul	0.00
7) Phenol-d5	6.893	99	295678	19.829	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	173435	19.805	ng/ul	0.00
11) 2-Chlorophenol-d4	7.258	132	238510	21.095	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	219916	19.109	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	110614	22.923	ng/ul	0.00
24) 2-Nitrophenol-d4	9.587	143	104584	24.331	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	208853	20.586	ng/ul	0.00
31) 4-Chloroaniline-d4	10.628	131	291983	18.570	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	625844	21.297	ng/ul	0.00
49) Acenaphthylene-d8	14.040	160	802747	21.043	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	74906	14.613	ng/ul	0.00
60) Fluorene-d10	15.345	176	552734	21.620	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	40664	11.399	ng/ul	0.00
73) Anthracene-d10	17.192	188	872746	22.076	ng/ul	0.00
81) Pyrene-d10	19.498	212	986792	22.840	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.392	264	1002602	22.933	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.222	149	96290	3.103	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015103.D
Acq On : 26 Jun 2021 06:51
Operator : CG/JU
Sample : M2704-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGDB7


Quant Time: Jun 26 07:28:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 24 14:43:13 2021
Response via : Initial Calibration

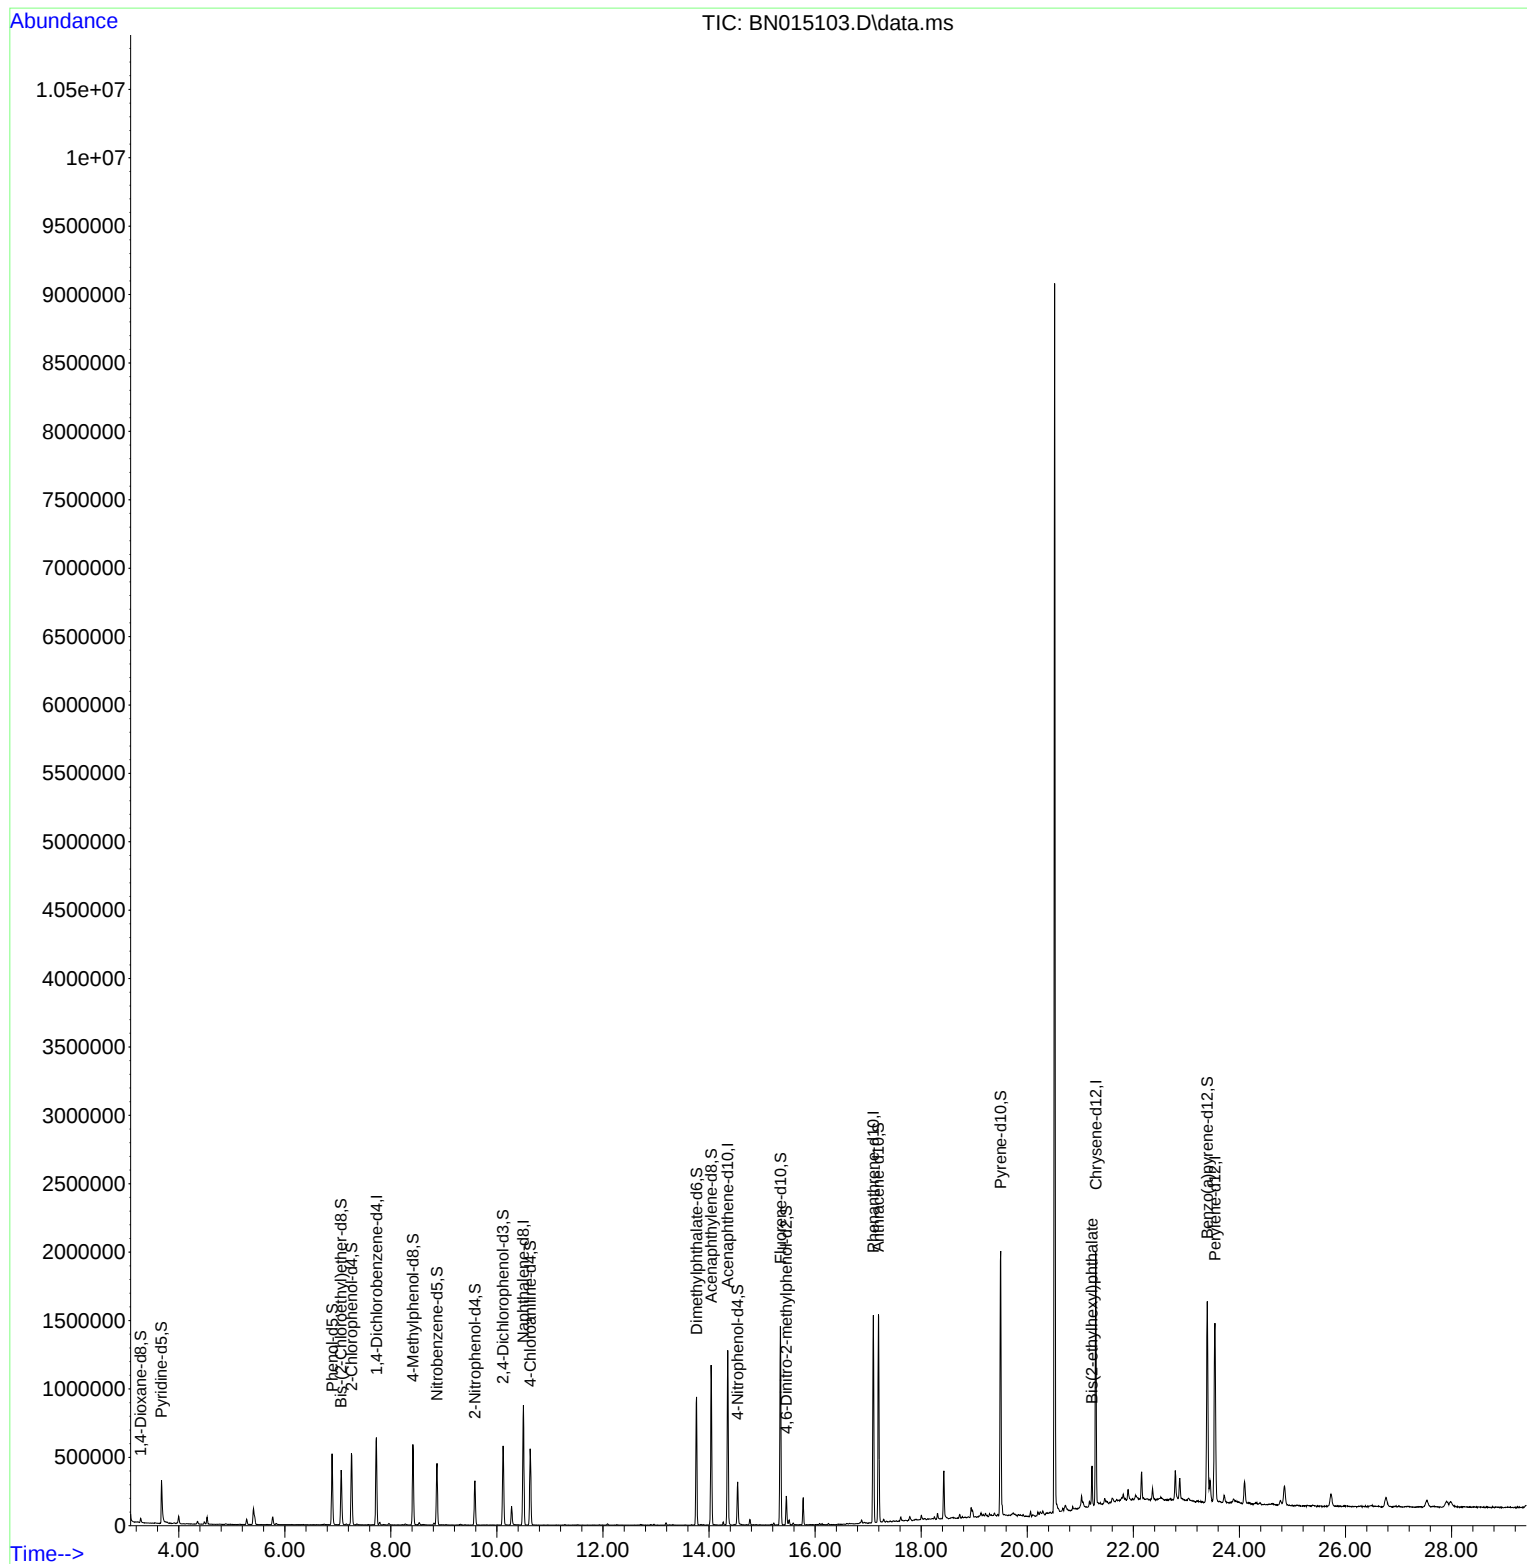

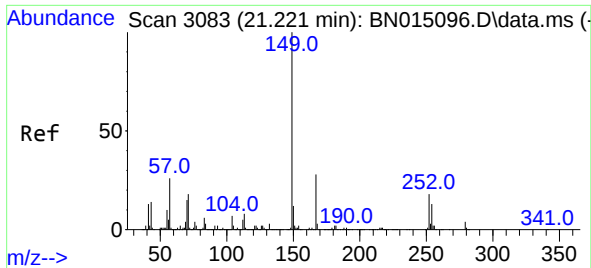

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.103 ng/ul
RT: 21.222 min Scan# 3083
Delta R.T. -0.006 min
Lab File: BN015103.D
Acq: 26 Jun 2021 06:51

Instrument :
BNA_N
ClientSampleId :
BGDB7

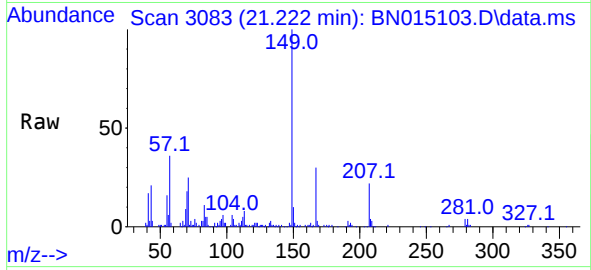

Tgt Ion:149 Resp: 96290
Ion Ratio Lower Upper
149 100
167 29.7 23.4 35.0
279 4.3 3.4 5.2

