

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
 Data File : BN015106.D
 Acq On : 26 Jun 2021 08:38
 Operator : CG/JU
 Sample : M2704-09
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGDB8

Quant Time: Jun 26 23:58:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 24 14:43:13 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	184298	20.000	ng/ul	0.00
20) Naphthalene-d8	10.499	136	761432	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.351	164	466291	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	963776	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	957875	20.000	ng/ul	0.00
88) Perylene-d12	23.539	264	992001	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	19260	4.066	ng/uL	0.00
4) Pyridine-d5	3.675	84	146102	11.442	ng/ul	0.00
7) Phenol-d5	6.893	99	333074	20.822	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.064	67	192846	20.529	ng/ul	0.00
11) 2-Chlorophenol-d4	7.263	132	262877	21.673	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	254802	20.639	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	121216	23.272	ng/ul	0.00
24) 2-Nitrophenol-d4	9.587	143	119806	25.822	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	236321	21.580	ng/ul	0.00
31) 4-Chloroaniline-d4	10.628	131	309555	18.240	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	727833	22.731	ng/ul	0.00
49) Acenaphthylene-d8	14.040	160	952488	22.915	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	84394	15.111	ng/ul	0.00
60) Fluorene-d10	15.345	176	652857	23.437	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	52581	13.210	ng/ul	0.00
73) Anthracene-d10	17.192	188	1032790	23.413	ng/ul	0.00
81) Pyrene-d10	19.492	212	1198231	23.866	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	1199650	24.497	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.222	149	138476	3.840	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015106.D
Acq On : 26 Jun 2021 08:38
Operator : CG/JU
Sample : M2704-09
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGDB8


Quant Time: Jun 26 23:58:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 24 14:43:13 2021
Response via : Initial Calibration

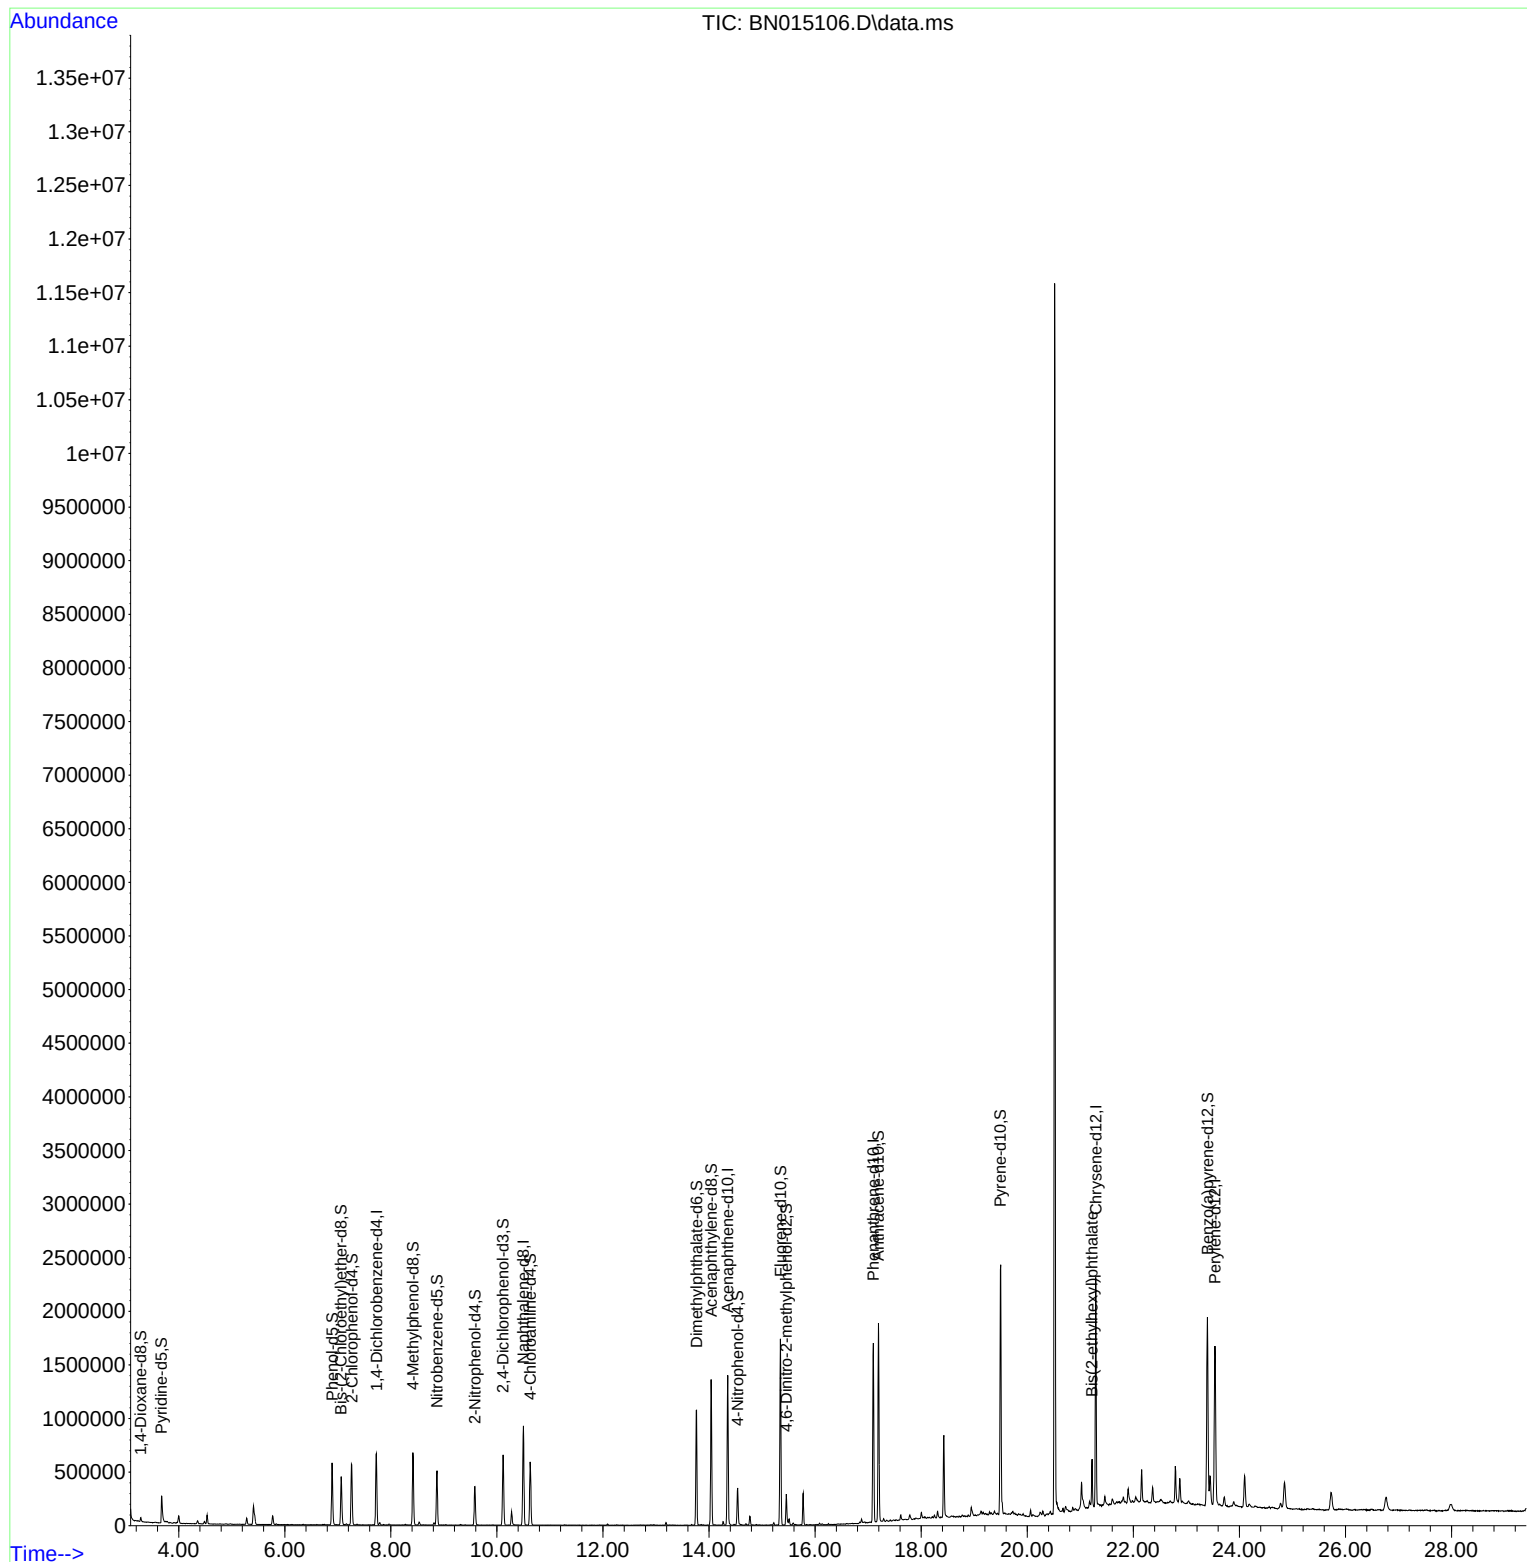

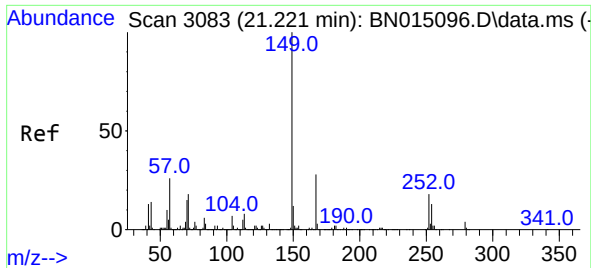

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.840 ng/ul
RT: 21.222 min Scan# 3083
Delta R.T. -0.006 min
Lab File: BN015106.D
Acq: 26 Jun 2021 08:38

Instrument :
BNA_N
ClientSampleId :
BGDB8

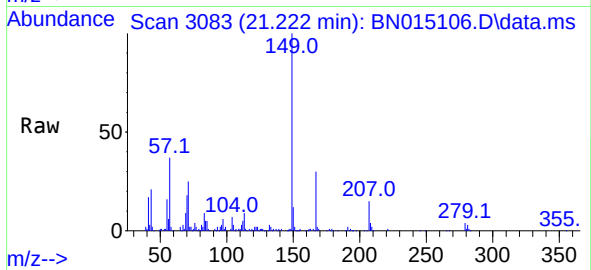

Tgt Ion:149 Resp: 138476
Ion Ratio Lower Upper
149 100
167 30.1 23.4 35.0
279 4.1 3.4 5.2

