

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
 Data File : BN015097.D
 Acq On : 26 Jun 2021 03:17
 Operator : CG/JU
 Sample : PB137260BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015097.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	40	rVB	66451	86571	1.92%	0.171%
2	3.676	97	100	119	rBV	800873	1206197	26.70%	2.376%
3	4.005	152	156	160	rBV	12320	15940	0.35%	0.031%
4	6.893	640	647	659	rBV	959842	1479123	32.75%	2.914%
5	7.064	670	676	686	rVB	757027	1168850	25.88%	2.303%
6	7.264	703	710	723	rVB	968366	1548290	34.28%	3.050%
7	7.728	781	789	797	rVB	738268	1168157	25.86%	2.301%
8	8.416	899	906	914	rBV	1103190	1801636	39.89%	3.549%
9	8.869	976	983	997	rVB	847393	1371641	30.37%	2.702%
10	9.587	1097	1105	1114	rBV	622785	1013577	22.44%	1.997%
11	10.116	1188	1195	1204	rBV	1087451	1775073	39.30%	3.497%
12	10.499	1252	1260	1267	rBV	1020634	1663734	36.83%	3.278%
13	10.628	1274	1282	1294	rBV	1102109	1861387	41.21%	3.667%
14	12.087	1524	1530	1535	rVB	18679	27473	0.61%	0.054%
15	13.763	1808	1815	1827	rVB	1770553	2456401	54.38%	4.839%
16	14.040	1855	1862	1870	rBV	2126919	3143664	69.60%	6.193%
17	14.351	1908	1915	1922	rBV	1462299	2089832	46.27%	4.117%
18	14.540	1941	1947	1956	rBV	778775	1117198	24.73%	2.201%
19	15.257	2066	2069	2075	rBV4	4237	8200	0.18%	0.016%
20	15.346	2075	2084	2095	rVB	2583868	3727068	82.52%	7.343%
21	15.457	2097	2103	2113	rBV	484423	647383	14.33%	1.275%
22	15.587	2120	2125	2134	rVB	28656	41229	0.91%	0.081%
23	16.128	2212	2217	2222	rVB4	8460	11327	0.25%	0.022%
24	16.610	2294	2299	2304	rBV6	3897	9094	0.20%	0.018%
25	16.663	2304	2308	2315	rVB2	9803	17662	0.39%	0.035%
26	16.881	2340	2345	2348	rBV3	5474	7806	0.17%	0.015%
27	17.098	2375	2382	2388	rBV	1725218	2402561	53.19%	4.733%
28	17.198	2392	2399	2406	rBV2	2734850	3930124	87.01%	7.743%
29	17.787	2494	2499	2502	rBV5	4034	5984	0.13%	0.012%
30	17.904	2517	2519	2525	rVB3	3375	5378	0.12%	0.011%
31	17.981	2526	2532	2533	rBV2	4563	5436	0.12%	0.011%
32	19.128	2723	2727	2732	rBV	31523	40839	0.90%	0.080%
33	19.381	2766	2770	2776	rBV	22040	29967	0.66%	0.059%
34	19.498	2783	2790	2797	rBV	3239044	4510759	99.87%	8.887%
35	20.433	2946	2949	2953	rBV4	5954	9624	0.21%	0.019%
36	20.516	2960	2963	2967	rBV4	9365	10730	0.24%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
 Data File : BN015097.D
 Acq On : 26 Jun 2021 03:17
 Operator : CG/JU
 Sample : PB137260BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Title : SVOA CALIBRATION

37	21.216	3080	3082	3086	rBV3	13688	15741	0.35%	0.031%
38	21.292	3089	3095	3104	rVV	2086316	2574520	57.00%	5.072%
39	22.363	3274	3277	3281	rVB2	38835	46334	1.03%	0.091%
40	22.875	3360	3364	3371	rVB	67552	97445	2.16%	0.192%
41	23.398	3445	3453	3459	rBV2	2473391	4516786	100.00%	8.899%
42	23.539	3469	3477	3486	rVB2	1436957	2687639	59.50%	5.295%
43	24.098	3567	3572	3580	rVB	103754	186698	4.13%	0.368%
44	24.851	3695	3700	3709	rVB3	98189	216854	4.80%	0.427%




Sum of corrected areas: 50757932

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015097.D
Acq On : 26 Jun 2021 03:17
Operator : CG/JU
Sample : PB137260BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK260

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

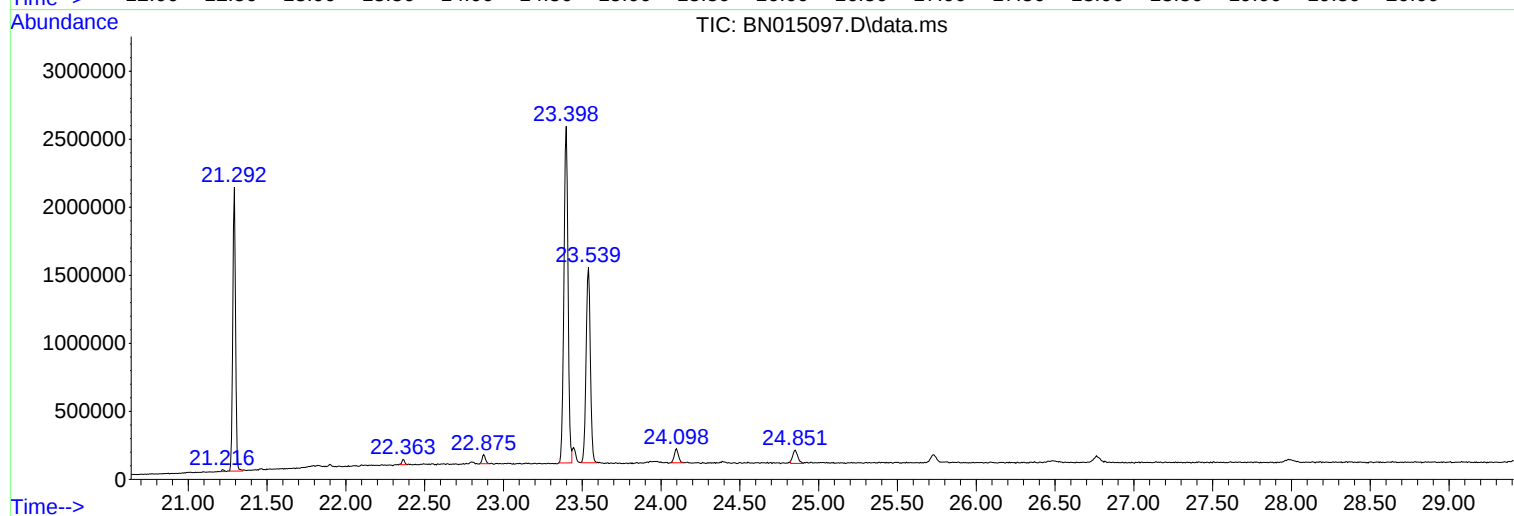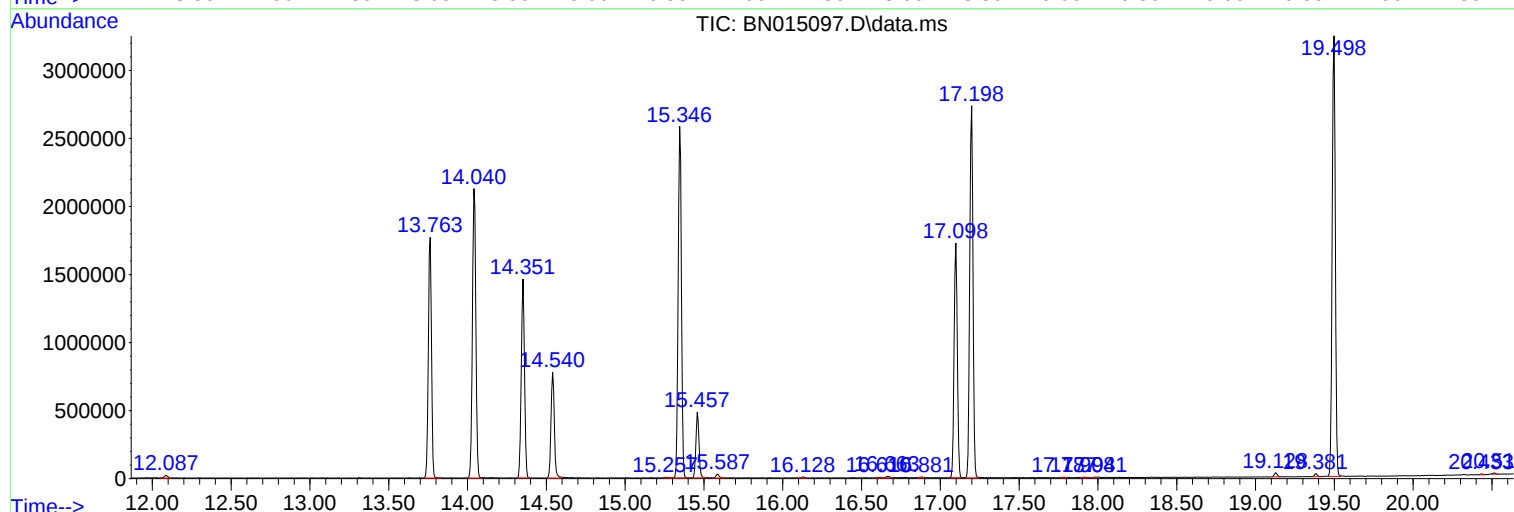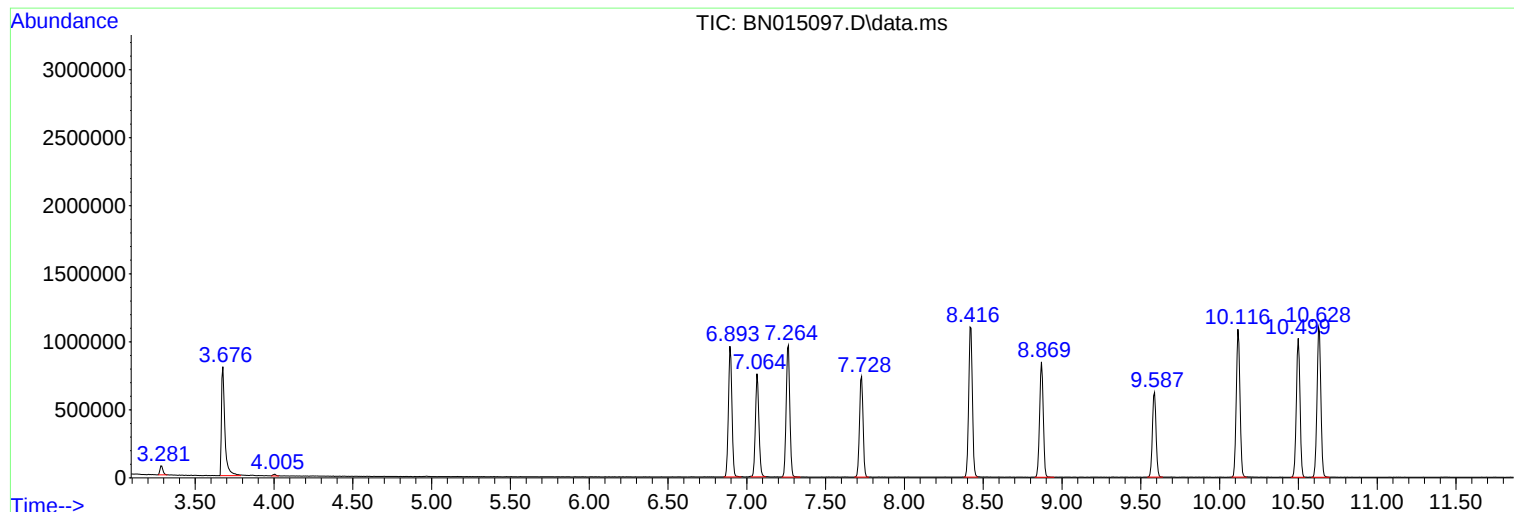

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015097.D
Acq On : 26 Jun 2021 03:17
Operator : CG/JU
Sample : PB137260BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK260

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015097.D
Acq On : 26 Jun 2021 03:17
Operator : CG/JU
Sample : PB137260BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK260

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
