

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
 Data File : BN015111.D
 Acq On : 26 Jun 2021 11:37
 Operator : CG/JU
 Sample : PB137260BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK260

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015111.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	39	rBV	60790	80796	1.96%	0.178%
2	3.675	97	100	123	rBV	749626	1117090	27.12%	2.467%
3	4.005	152	156	162	rVB	9957	13115	0.32%	0.029%
4	6.893	640	647	662	rBV	896834	1376918	33.42%	3.040%
5	7.063	670	676	686	rBV	688664	1076388	26.13%	2.377%
6	7.263	703	710	719	rBV	894345	1431915	34.76%	3.162%
7	7.728	782	789	798	rVB	593544	937051	22.75%	2.069%
8	8.416	899	906	918	rBV	1072257	1678369	40.74%	3.706%
9	8.869	976	983	991	rVB	802173	1271130	30.86%	2.807%
10	9.587	1097	1105	1117	rBV	565516	948125	23.02%	2.094%
11	10.116	1187	1195	1207	rBV	1000575	1662860	40.37%	3.672%
12	10.498	1252	1260	1267	rBV	790598	1336293	32.44%	2.951%
13	10.628	1273	1282	1296	rBV	1034104	1729385	41.98%	3.819%
14	12.087	1525	1530	1536	rVB	18272	26712	0.65%	0.059%
15	13.763	1808	1815	1825	rBV	1602333	2256095	54.77%	4.982%
16	14.039	1854	1862	1872	rBV	1935477	2884182	70.01%	6.368%
17	14.351	1908	1915	1926	rBV	1155416	1696038	41.17%	3.745%
18	14.539	1941	1947	1963	rBV	736110	1063462	25.82%	2.348%
19	15.263	2065	2070	2072	rBV4	2478	4281	0.10%	0.009%
20	15.345	2075	2084	2091	rVV	2374803	3421095	83.05%	7.554%
21	15.457	2097	2103	2111	rBV	469384	631345	15.33%	1.394%
22	15.586	2121	2125	2129	rVB	26757	32881	0.80%	0.073%
23	16.128	2215	2217	2221	rVB	5682	6858	0.17%	0.015%
24	16.669	2306	2309	2314	rVV5	4274	6965	0.17%	0.015%
25	16.880	2339	2345	2350	rBV4	6687	12487	0.30%	0.028%
26	17.098	2375	2382	2388	rBV	1352274	1918956	46.58%	4.237%
27	17.198	2392	2399	2409	rBV	2506526	3644609	88.47%	8.048%
28	19.127	2723	2727	2732	rVB2	27116	35487	0.86%	0.078%
29	19.380	2765	2770	2776	rBV	21156	30121	0.73%	0.067%
30	19.445	2776	2781	2783	rBV6	3658	5446	0.13%	0.012%
31	19.498	2783	2790	2797	rBV	2977107	4107677	99.71%	9.070%
32	20.515	2961	2963	2969	rVB4	11954	12409	0.30%	0.027%
33	21.298	3090	3096	3103	rBV	1576589	2071651	50.29%	4.574%
34	22.374	3276	3279	3284	rVB3	38339	44814	1.09%	0.099%
35	22.880	3361	3365	3372	rVB2	68809	99643	2.42%	0.220%
36	23.404	3446	3454	3460	rBV2	2215594	4119441	100.00%	9.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015111.D
Acq On : 26 Jun 2021 11:37
Operator : CG/JU
Sample : PB137260BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK260

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Title : SVOA CALIBRATION

37	23.545	3470	3478	3489	rVB2	1085697	2151375	52.22%	4.750%
38	24.104	3568	3573	3580	rVB	98471	177389	4.31%	0.392%
39	24.856	3697	3701	3708	rVB2	85804	167847	4.07%	0.371%




Sum of corrected areas: 45288701

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015111.D
Acq On : 26 Jun 2021 11:37
Operator : CG/JU
Sample : PB137260BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK260

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

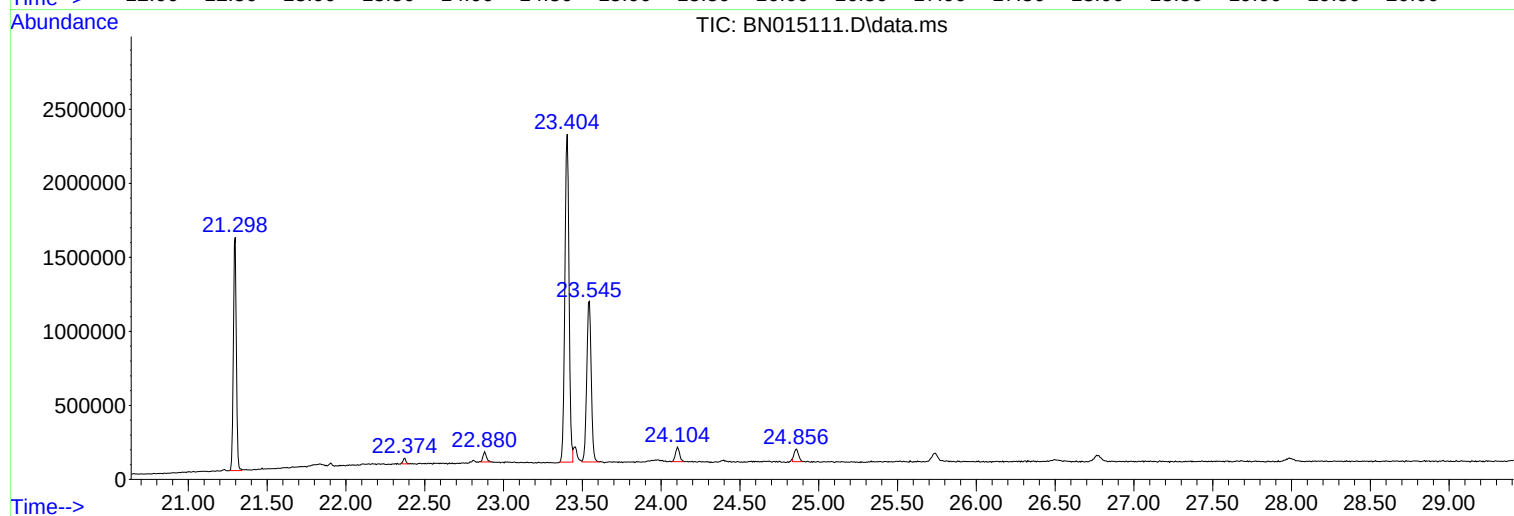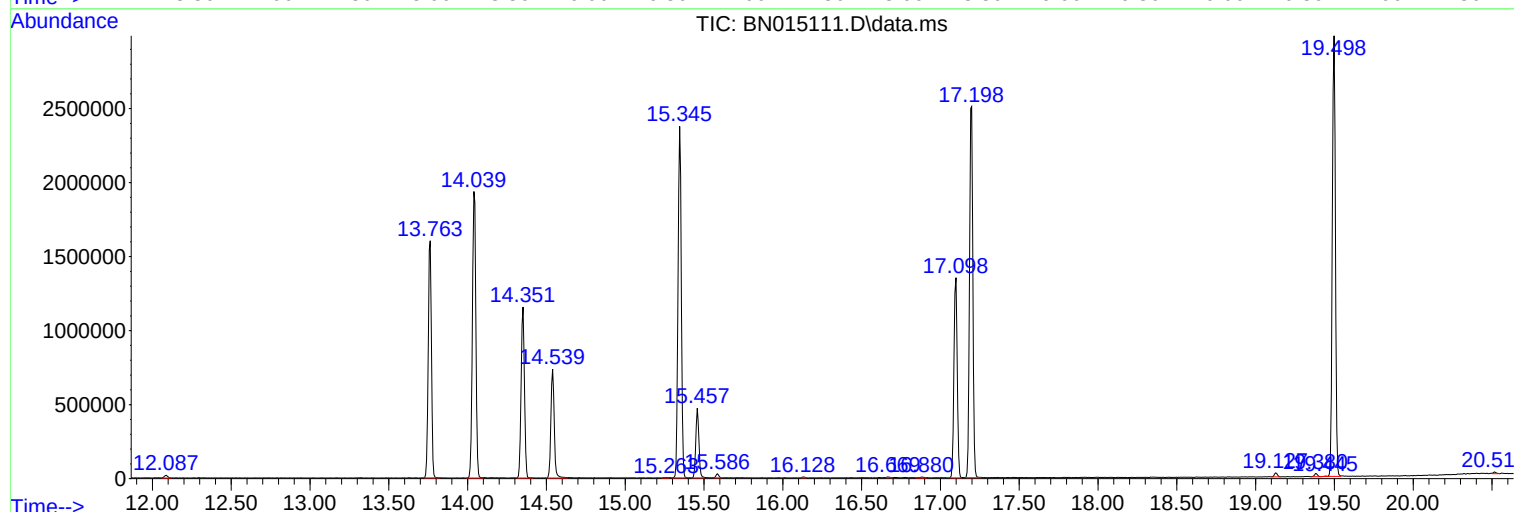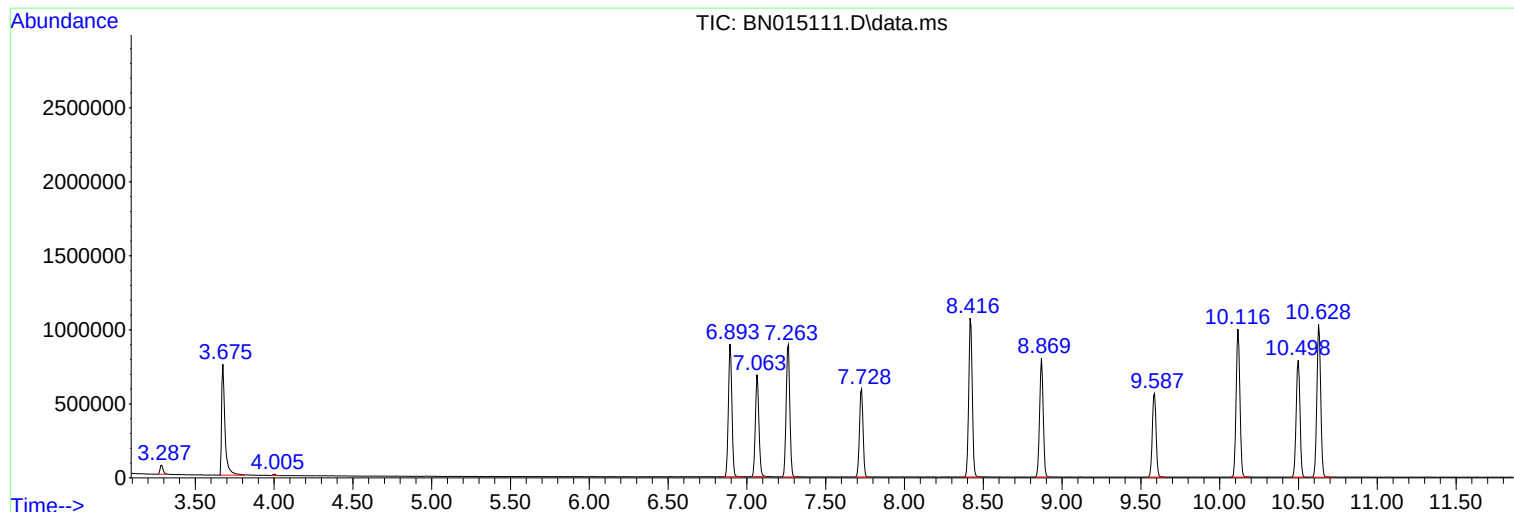

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015111.D
Acq On : 26 Jun 2021 11:37
Operator : CG/JU
Sample : PB137260BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK260

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062621\
Data File : BN015111.D
Acq On : 26 Jun 2021 11:37
Operator : CG/JU
Sample : PB137260BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK260

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
