

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062623\
 Data File : BN026020.D
 Acq On : 26 Jun 2023 10:53
 Operator : MA/JU
 Sample : PB153447BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK447

Quant Time: Jun 27 01:37:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 22 01:27:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	7259	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.786	136	23470	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.612	164	14903	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.359	188	32497	0.400	ng/ul	0.00
17) Chrysene-d12	21.549	240	19169	0.400	ng/ul	0.00
23) Perylene-d12	24.001	264	19886	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	46221	5.654	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.376	152	11944	0.331	ng/ul	0.00
18) Fluoranthene-d10	19.386	212	28047	0.384	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.606	166	4705	0.072	ng/ul#	11
20) Pyrene	19.748	202	4316	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.849	252	6711	0.091	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062623\
Data File : BN026020.D
Acq On : 26 Jun 2023 10:53
Operator : MA/JU
Sample : PB153447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK447

Quant Time: Jun 27 01:37:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 22 01:27:41 2023
Response via : Initial Calibration




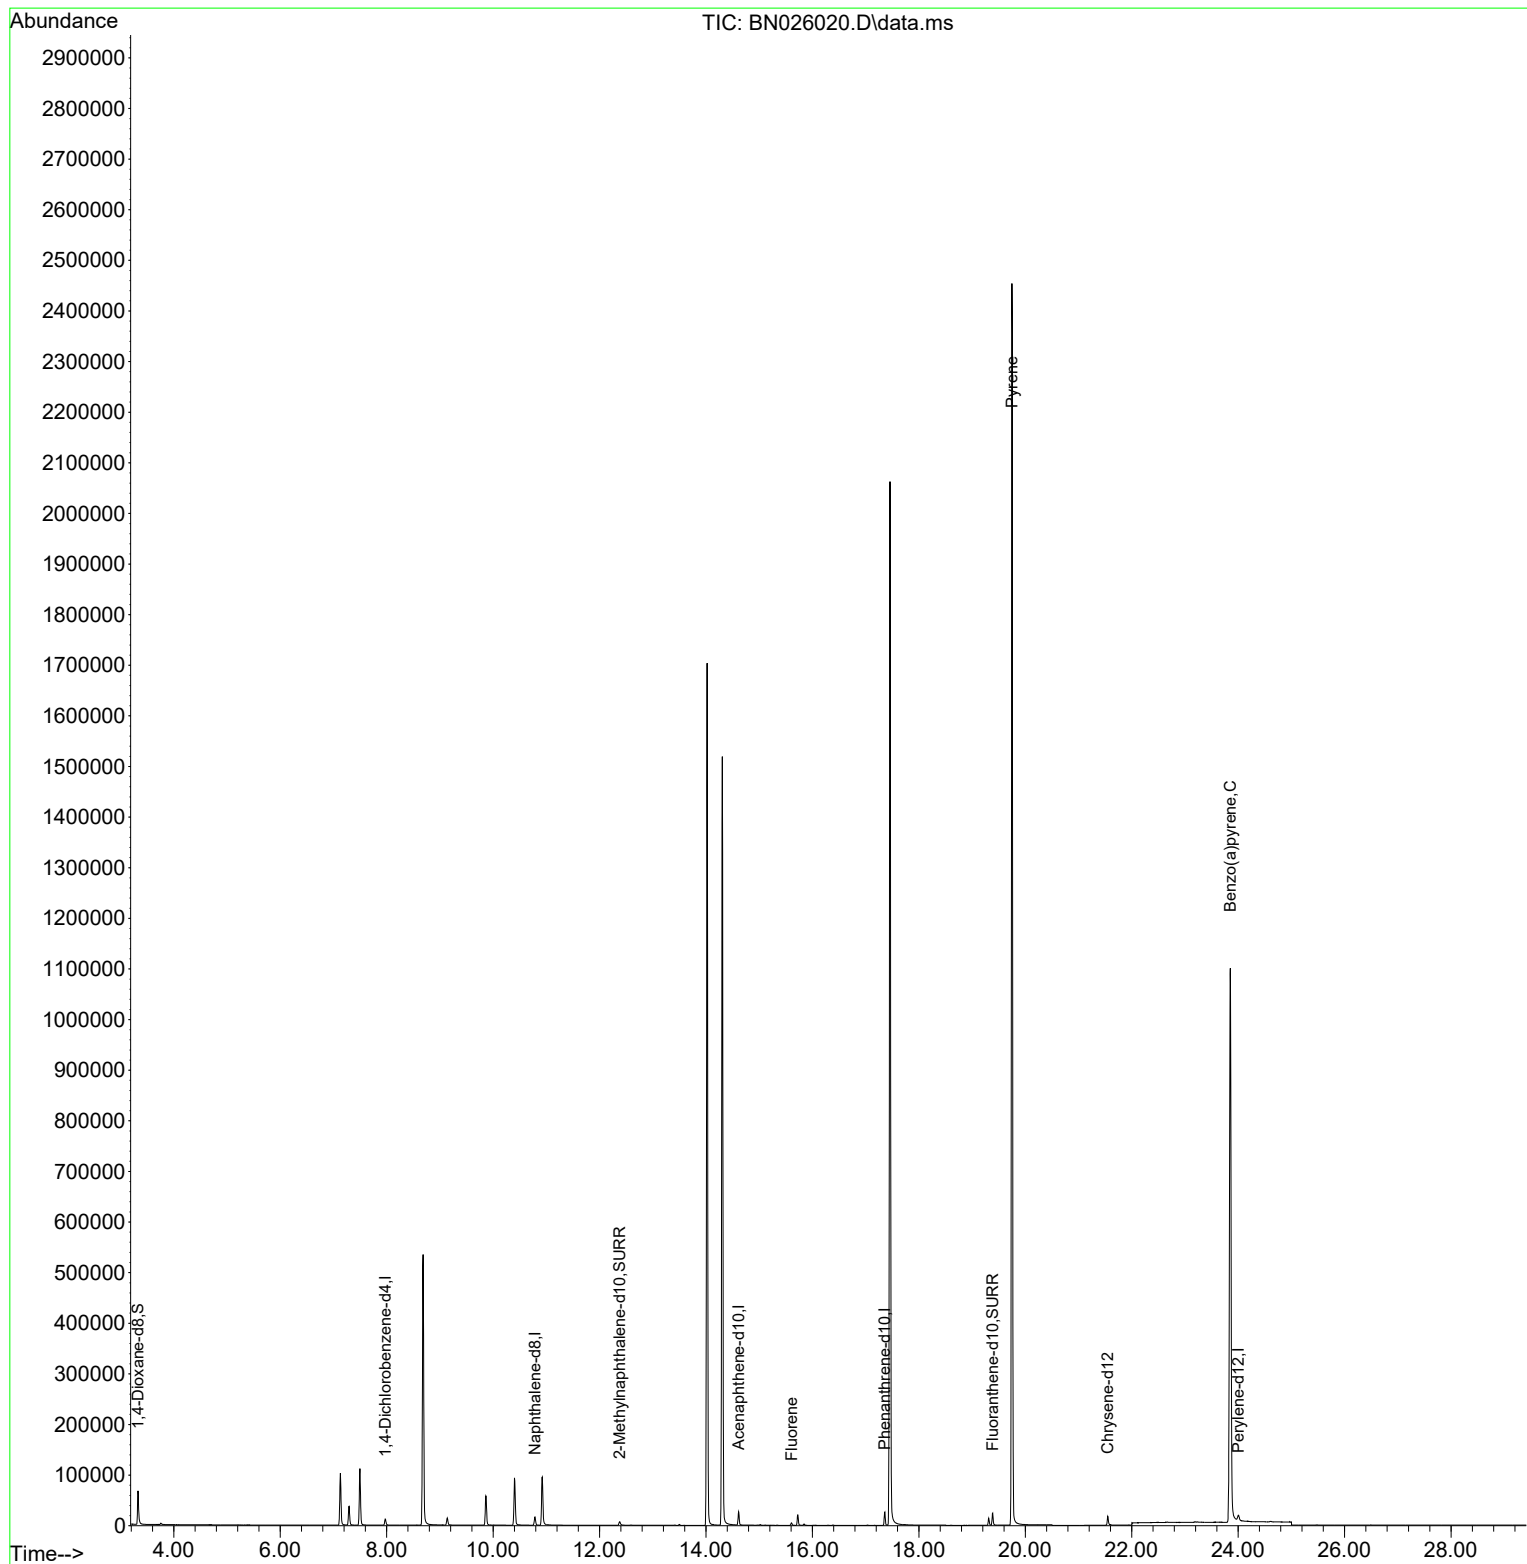


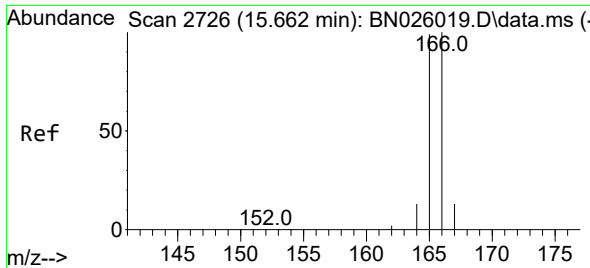

#12
Fluorene
Concen: 0.072 ng/ul
RT: 15.606 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN026020.D
Acq: 26 Jun 2023 10:53




Instrument :
BNA_N
ClientSampleId :
SBLK447


Tgt Ion:166 Resp: 4705
Ion Ratio Lower Upper
166 100
165 6.5 79.9 119.9#
167 34.9 10.8 16.2#

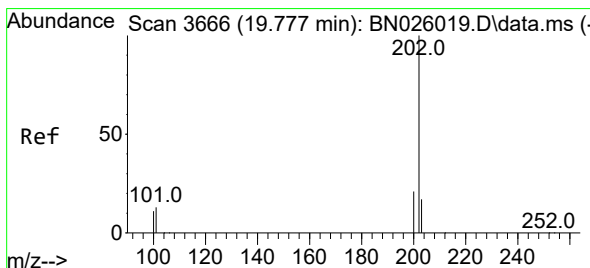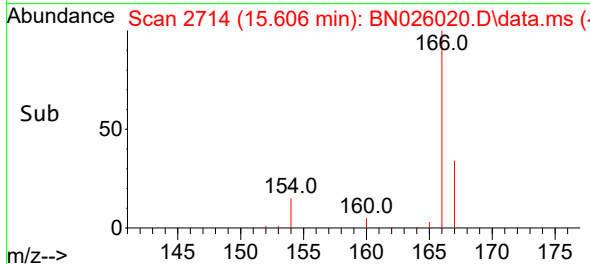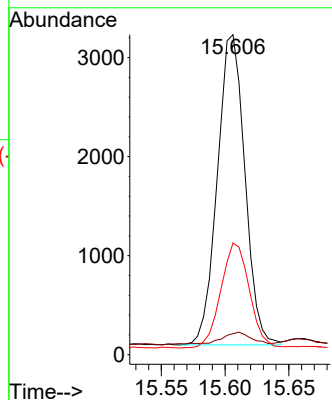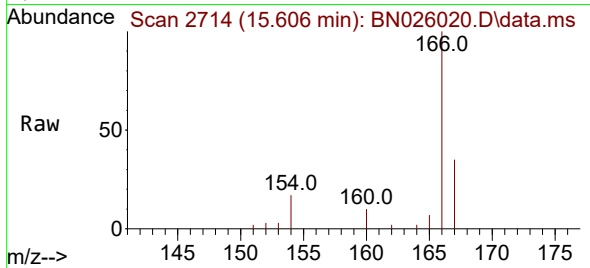

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.748 min Scan# 3660
Delta R.T. -0.033 min
Lab File: BN026020.D
Acq: 26 Jun 2023 10:53


Tgt Ion:202 Resp: 4316
Ion Ratio Lower Upper
202 100
101 181.5 11.4 17.0#
100 1432.6 9.1 13.7#

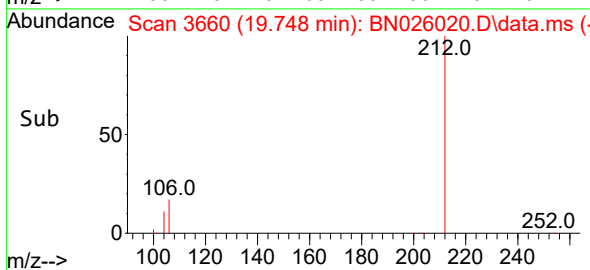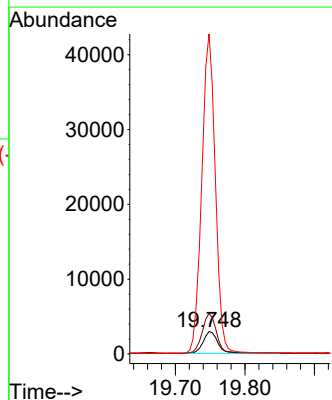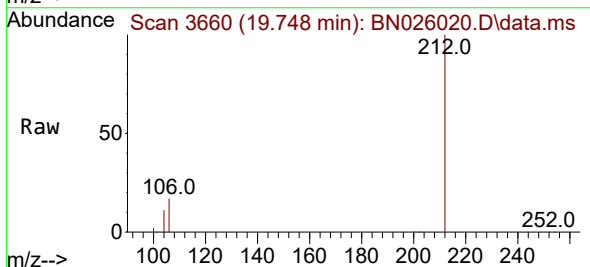

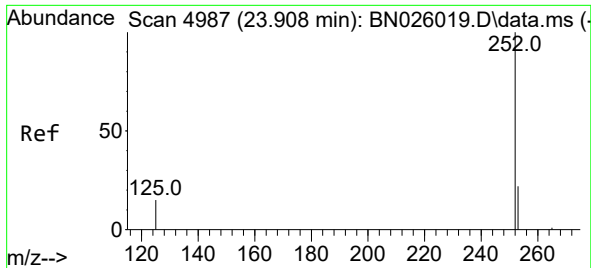

#26
Benzo(a)pyrene
Concen: 0.091 ng/ul
RT: 23.849 min Scan# 4987
Delta R.T. -0.059 min
Lab File: BN026020.D
Acq: 26 Jun 2023 10:53

Instrument :
BNA_N
ClientSampleId :
SBLK447

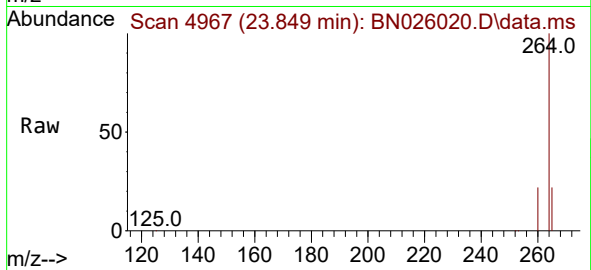

Tgt Ion:252 Resp: 6711
Ion Ratio Lower Upper
252 100
253 53.3 26.0 39.0#
125 49.7 17.3 25.9#

