


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062721\
Data File : BN015121.D
Acq On : 26 Jun 2021 17:36
Operator : CG/JU
Sample : PB137232BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK232

Quant Time: Jun 27 06:57:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 22 11:53:52 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/28/2021 1:27:16 PM

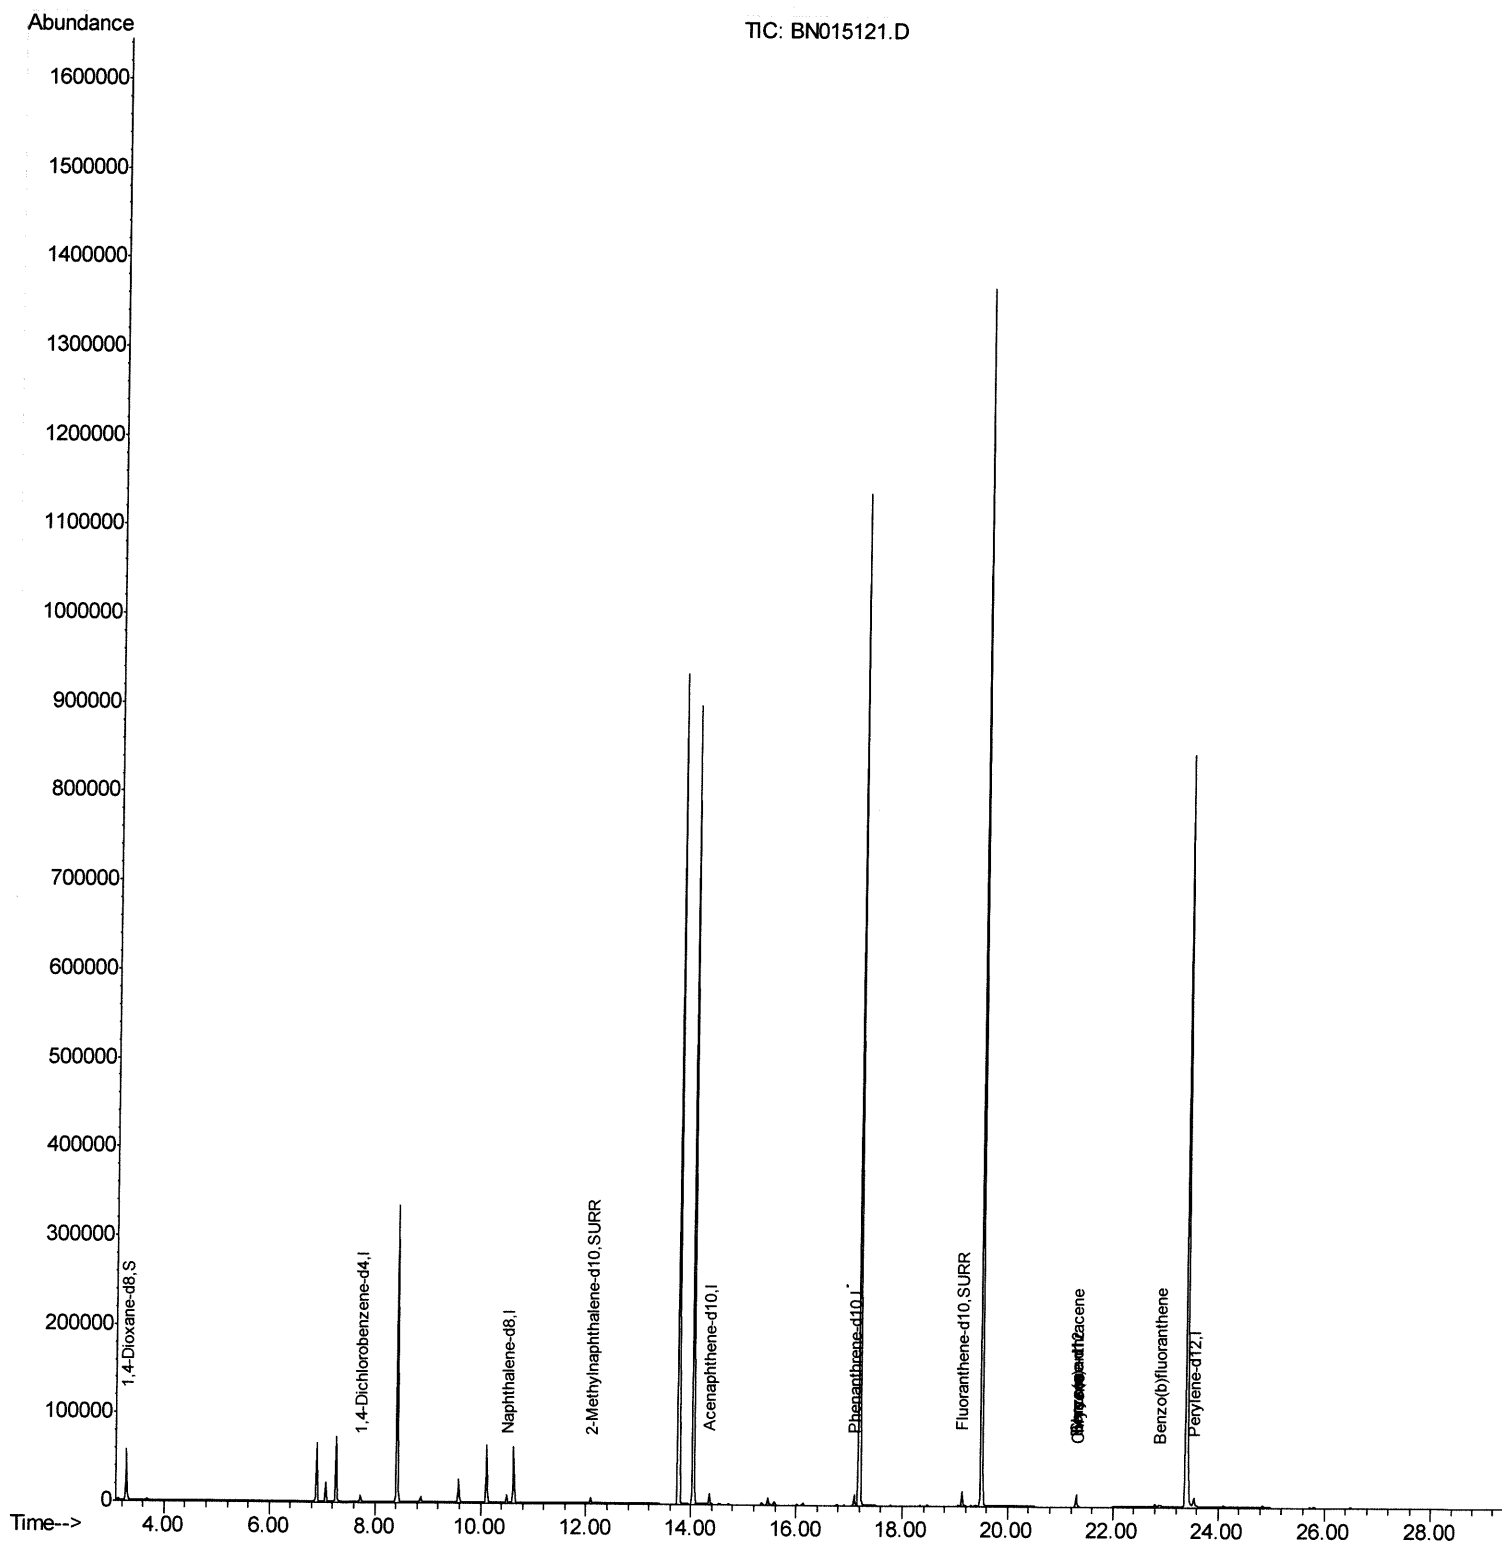

Instrument :
BNA_N
ClientSampleId :
SBLK232

Manual Integrations
APPROVED

mohammad
6/28/2021 1:27:16 PM



response 0




Ion	Exp%	Act%
188.00	100	0.00
94.00	14.10	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062721\
 Data File : BN015121.D
 Acq On : 26 Jun 2021 17:36
 Operator : CG/JU
 Sample : PB137232BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK232

Quant Time: Jun 27 06:41:14 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 22 11:53:52 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED
 mohammad
 6/28/2021 1:27:16 PM

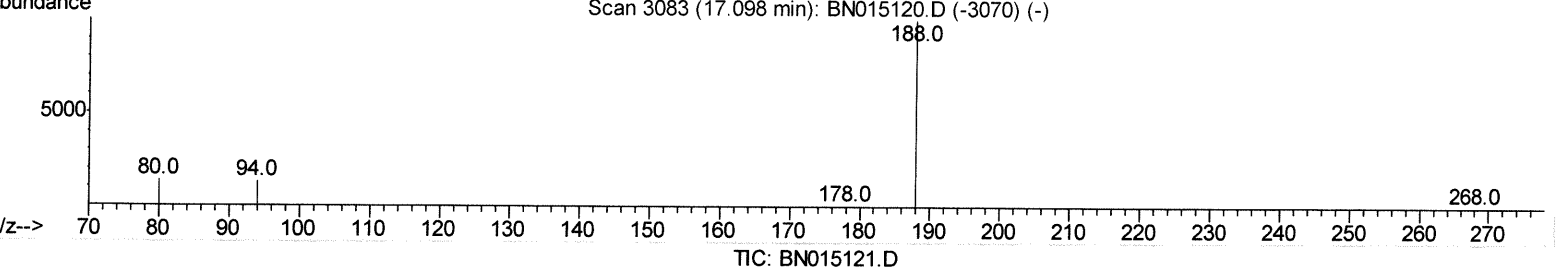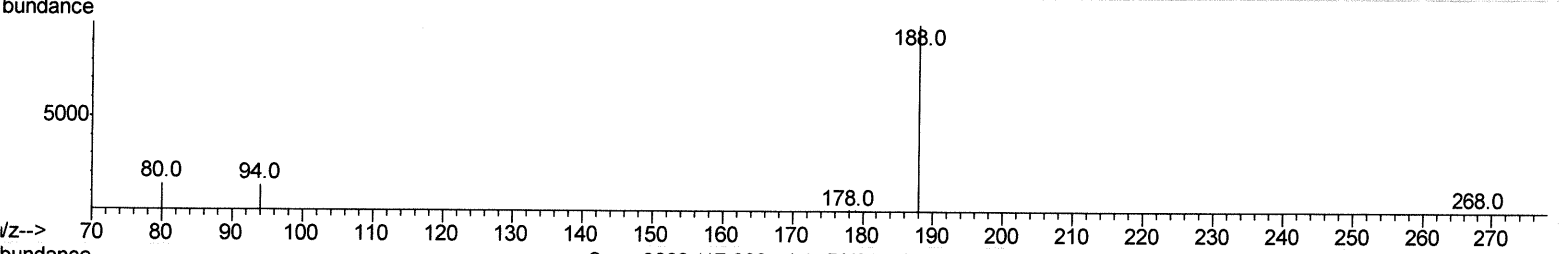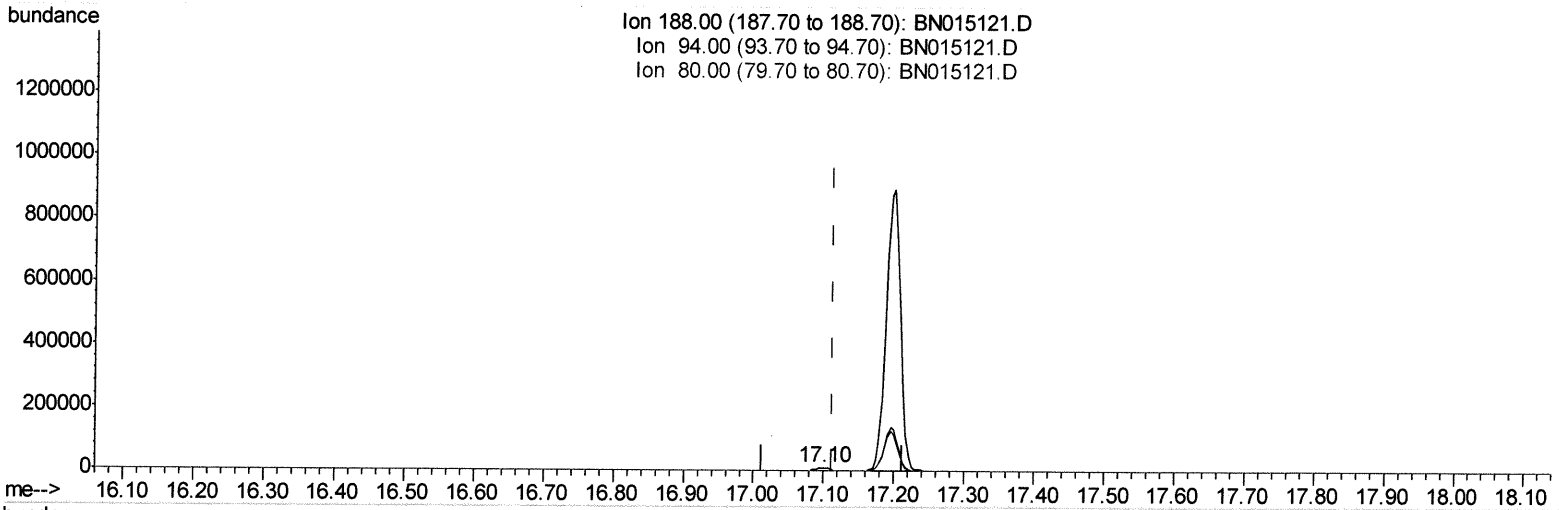

(13) Phenanthrene-d10 (I)

17.098min (-0.015) 0.40ng/ul m

response 13570

Handwritten: 7/6/2021

Ion	Exp%	Act%
188.00	100	100
94.00	14.10	13.58
80.00	14.40	14.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062721\
 Data File : BN015121.D
 Acq On : 26 Jun 2021 17:36
 Operator : CG/JU
 Sample : PB137232BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK232

Quant Time: Jun 27 06:57:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 22 11:53:52 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/28/2021 1:27:16 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	3549	0.40	ng/ul	-0.01
4) Naphthalene-d8	10.50	136	12447	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.35	164	7037	0.40	ng/ul	-0.01
13) Phenanthrene-d10	17.10	188	13570m	0.40	ng/ul	-0.01
17) Chrysene-d12	21.30	240	12340	0.40	ng/ul	-0.02
23) Perylene-d12	23.54	264	11616	0.40	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.28	96	34656	8.66	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.09	152	8685	0.44	ng/ul	-0.01
18) Fluoranthene-d10	19.13	212	16525	0.41	ng/ul	-0.02
Target Compounds						
21) Benzo(a)anthracene	21.28	228	1199	0.026	ng/ul#	81
22) Chrysene	21.33	228	1524	0.028	ng/ul#	90
24) Benzo(b)fluoranthene	22.87	252	1474	0.027	ng/ul#	29

(#) = qualifier out of range (m) = manual integration (+) = signals summed