
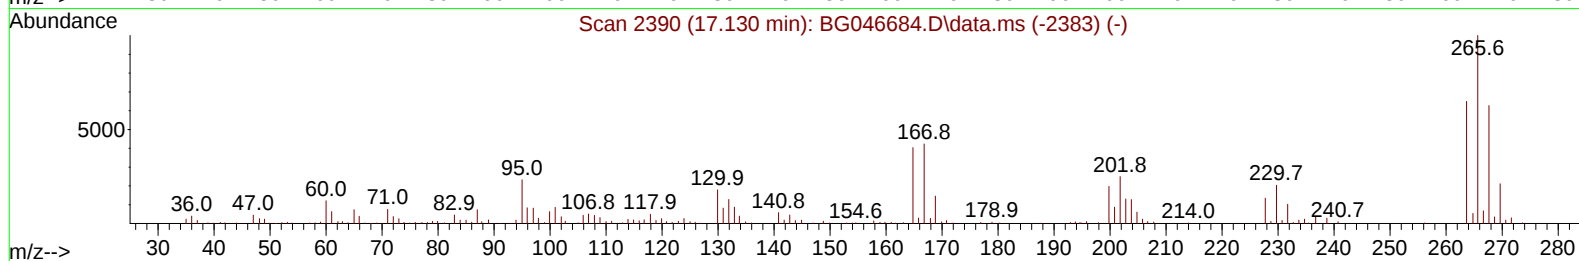
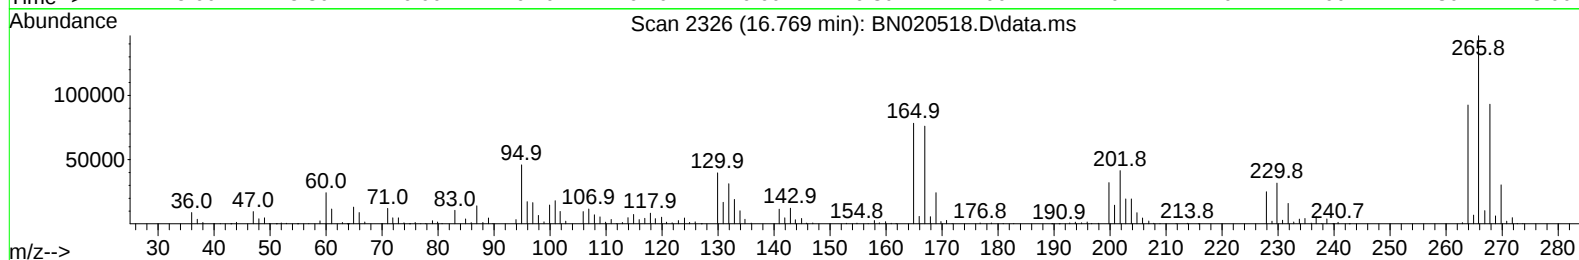


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062722\
Data File : BN020518.D
Acq On : 28 Jun 2022 04:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 08:03:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 28 08:02:00 2022
Response via : Initial Calibration

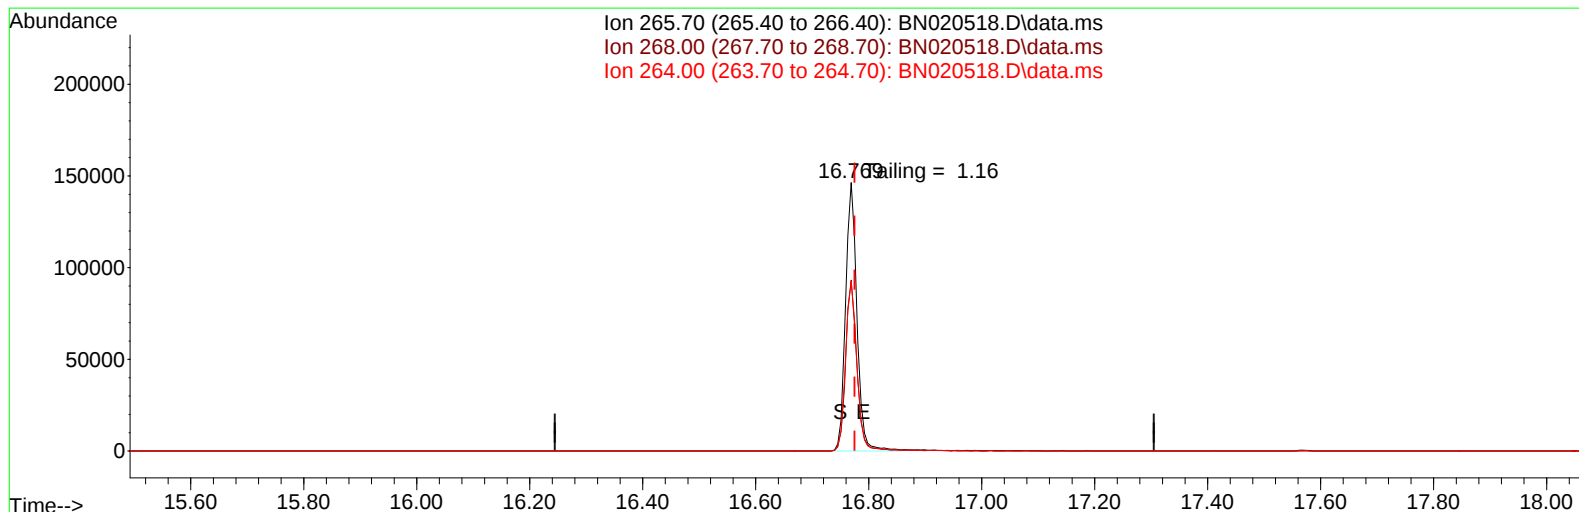

TIC: BN020518.D\data.ms

(70) Pentachlorophenol (C)




16.769min (-0.006) 18846.12 ng

response 206172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.65
264.00	61.60	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062722\
Data File : BN020518.D
Acq On : 28 Jun 2022 04:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 08:03:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 28 08:02:00 2022
Response via : Initial Calibration

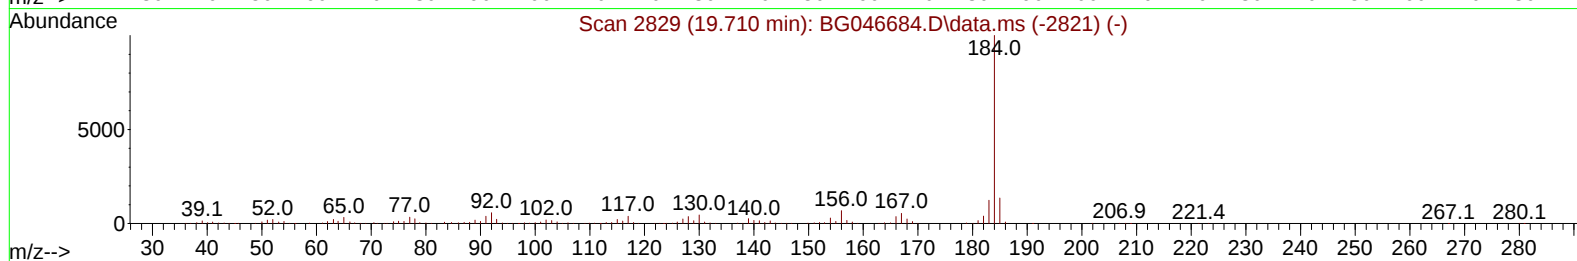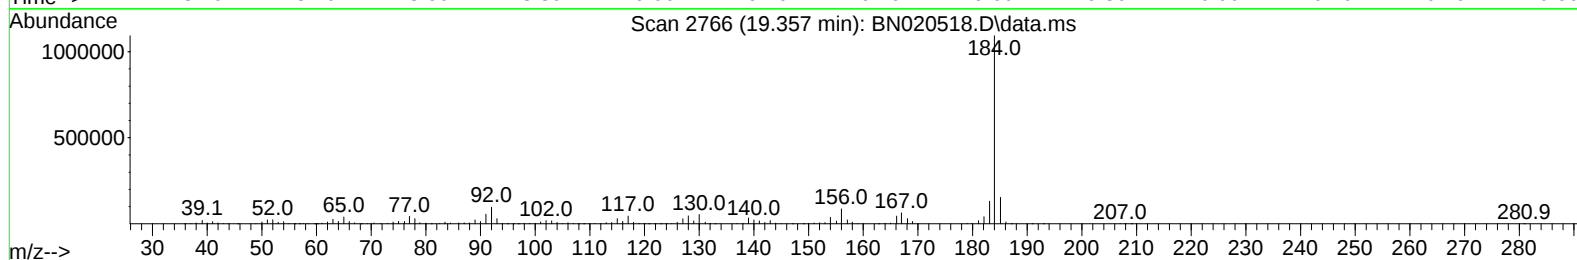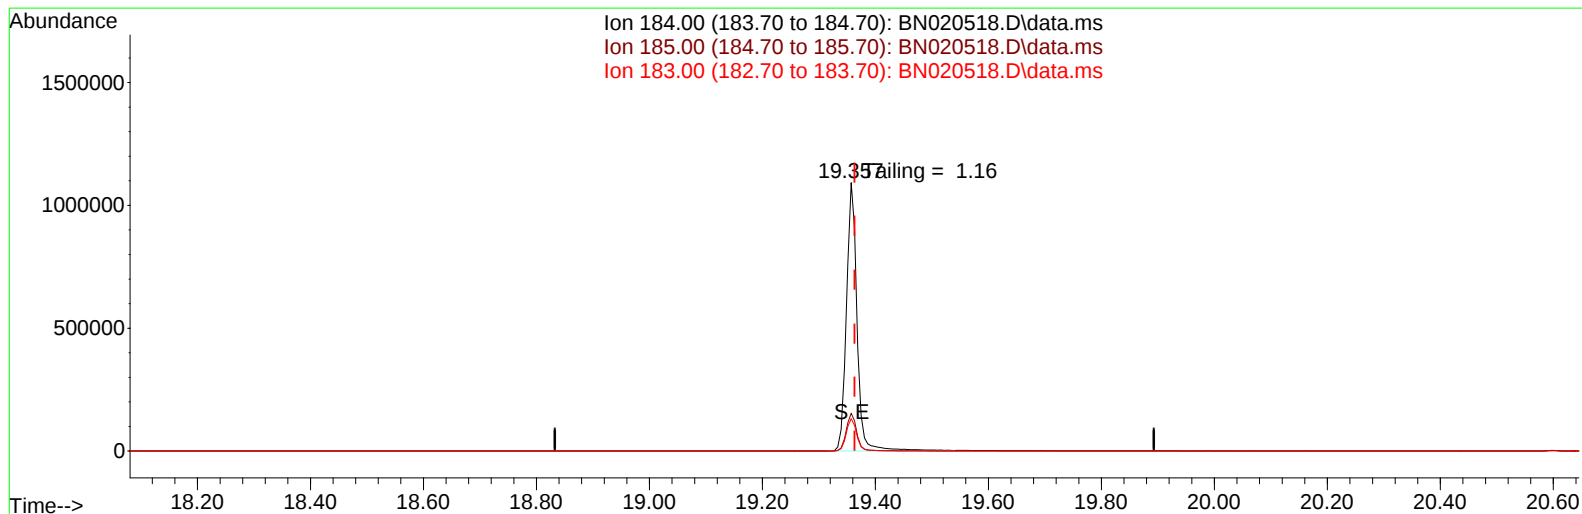

TIC: BN020518.D\data.ms

(77) Benzidine

19.357min (-0.006) 0.00 ng

response 1427506

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	12.04
0.00	0.00	0.00