


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062722\
 Data File : BN020500.D
 Acq On : 27 Jun 2022 14:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 02 03:10:12 2022

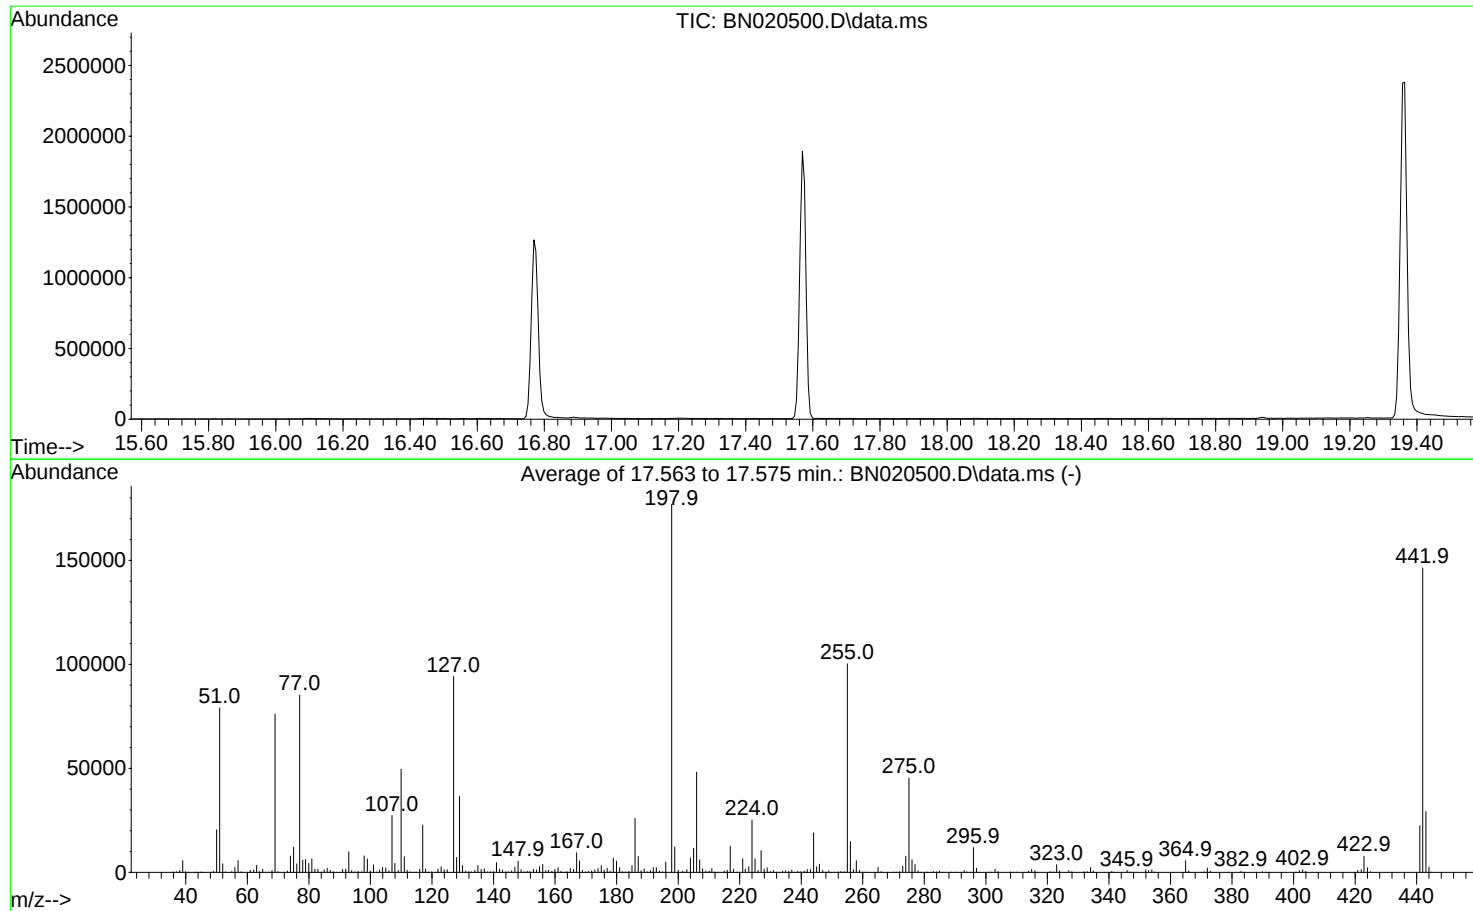

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	79085	PASS
68	69	0.00	2	1.2	942	PASS
69	198	0.00	100	43.0	76093	PASS
70	69	0.00	2	0.6	424	PASS
127	198	10	80	53.2	94115	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	176832	PASS
199	198	5	9	6.9	12224	PASS
275	198	10	60	25.6	45309	PASS
365	198	1	100	3.2	5597	PASS
441	198	0.01	100	12.7	22439	PASS
442	442	50	100	100.0	146323	PASS
443	442	15	24	20.0	29245	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/27/2022	BNA_N	<u>BN020500.D</u>
Compound Name	Response	Retention Time
DDT	626214	20.604
DDD	20541	20.163
DDE	1629	19.657
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22170	648384	3.42

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062722\
Data File : BN020500.D
Acq On : 27 Jun 2022 14:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 28 08:02:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 28 08:02:00 2022
Response via : Initial Calibration

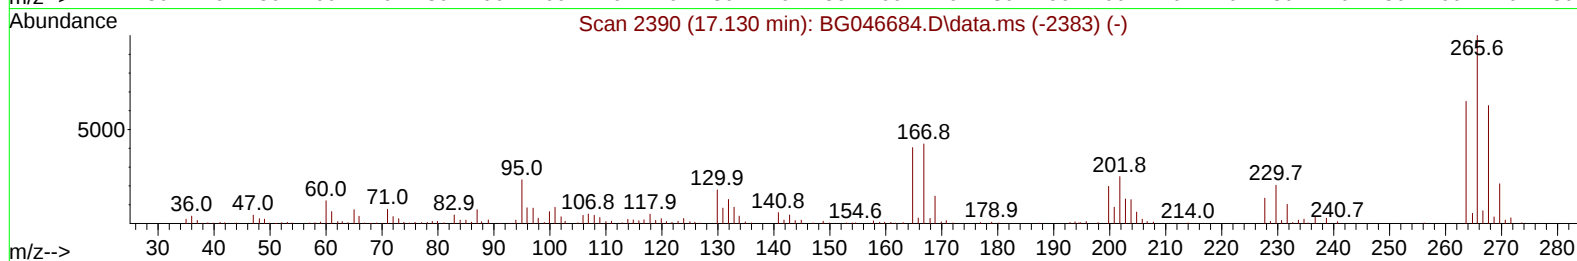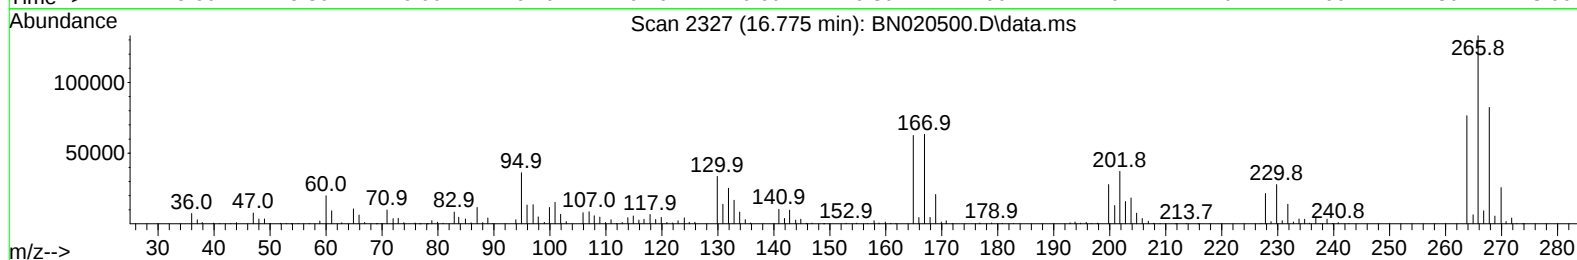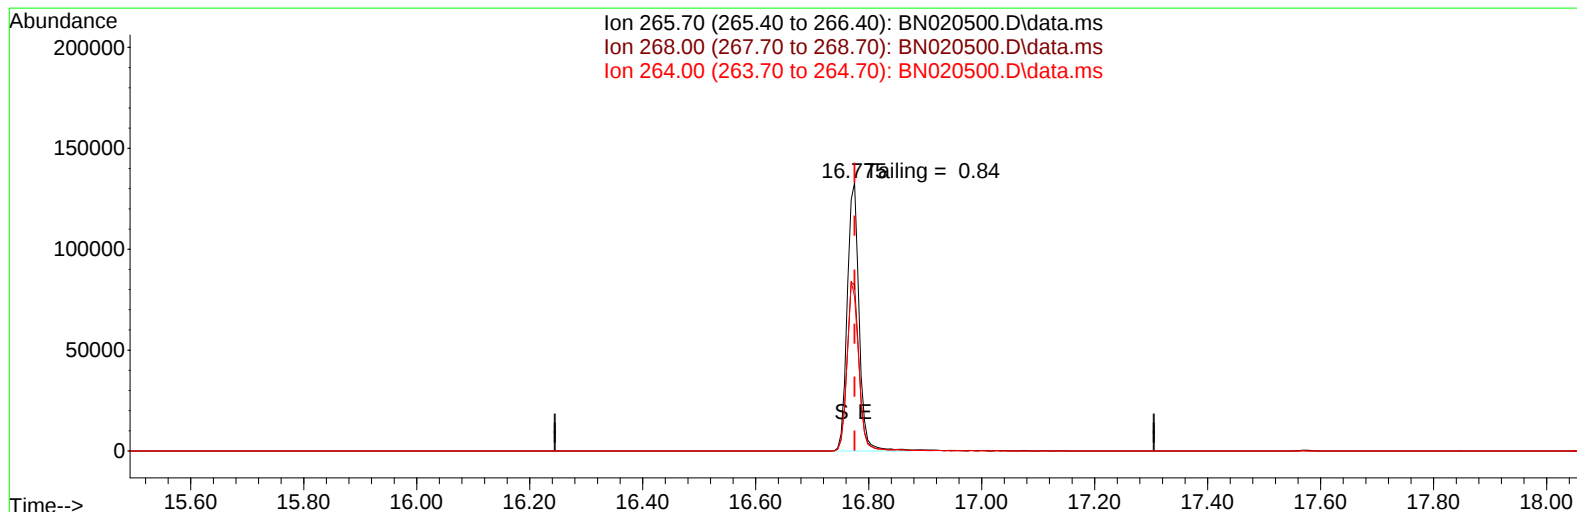

TIC: BN020500.D\data.ms

(70) Pentachlorophenol (C)

16.775min (0.000) 20457.99 ng




response 192659

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.92
264.00	61.60	57.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062722\
 Data File : BN020500.D
 Acq On : 27 Jun 2022 14:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 28 08:02:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 28 08:02:00 2022
 Response via : Initial Calibration

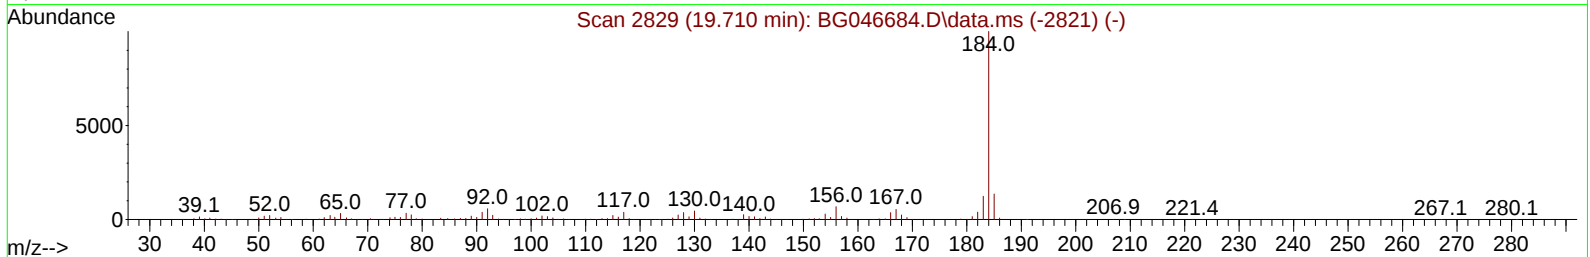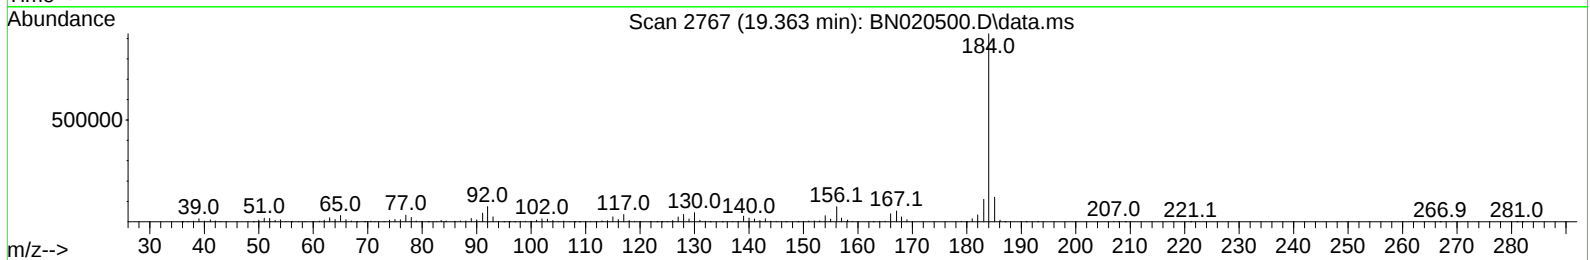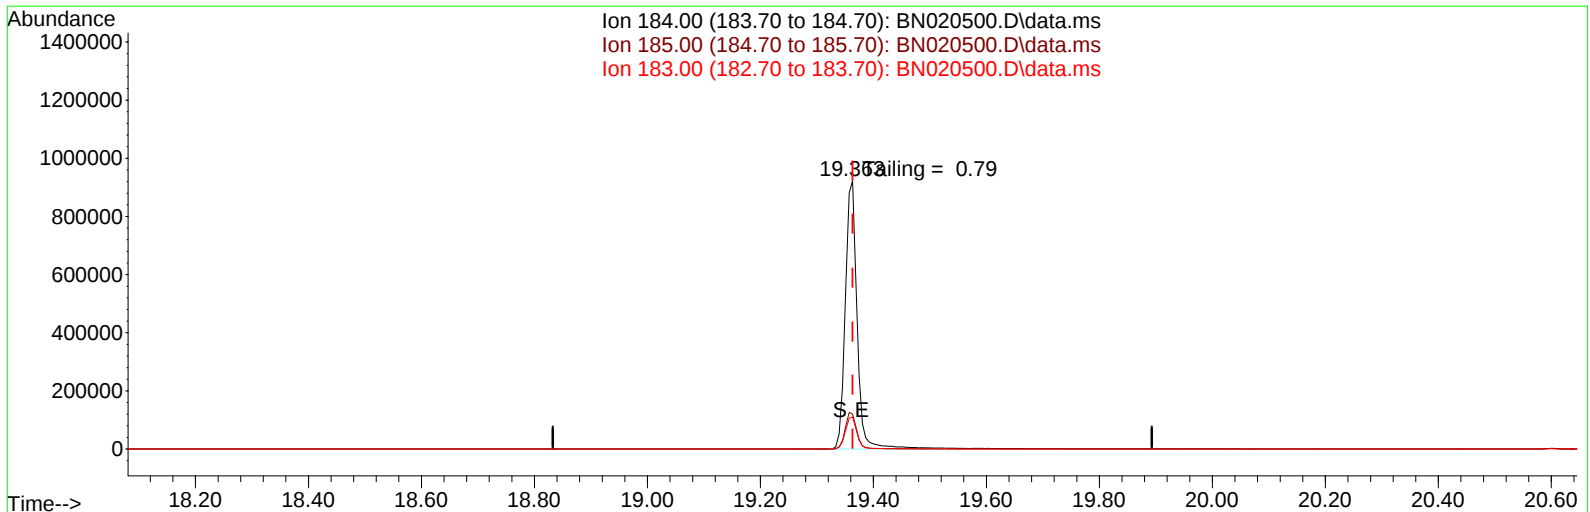

TIC: BN020500.D\data.ms

(77) Benzidine

19.363min (0.000) 0.00 ng

response 1345564

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.03
183.00	13.20	11.96
0.00	0.00	0.00