


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062722\
Data File : BN020518.D
Acq On : 28 Jun 2022 04:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jul 02 03:10:12 2022

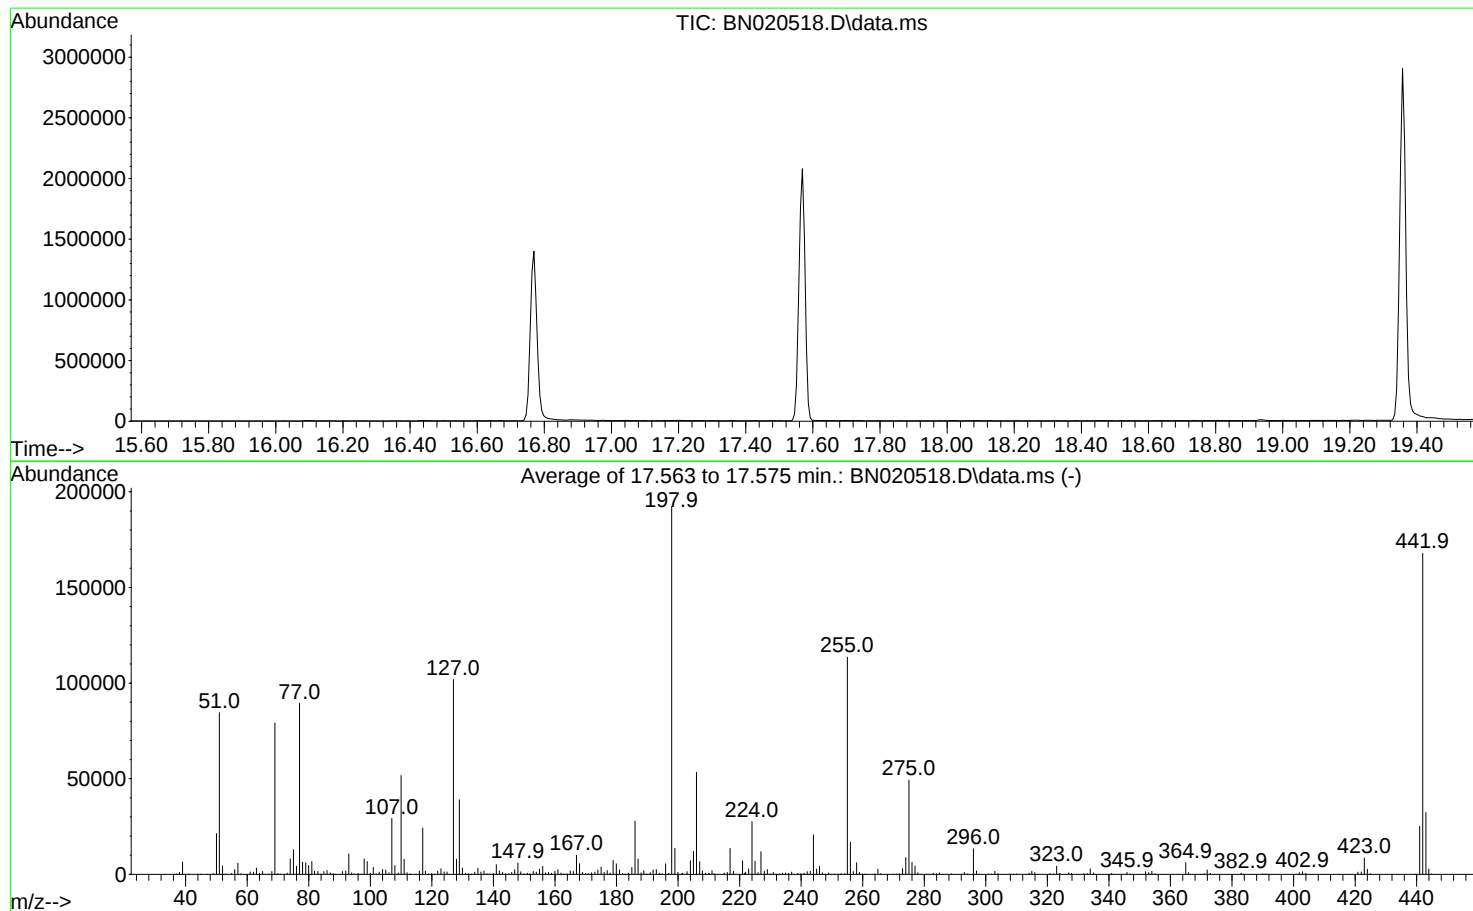

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	44.0	84546	PASS
68	69	0.00	2	1.9	1529	PASS
69	198	0.00	100	41.1	79133	PASS
70	69	0.00	2	0.6	483	PASS
127	198	10	80	53.0	101907	PASS
197	198	0.00	2	0.3	556	PASS
198	198	100	100	100.0	192320	PASS
199	198	5	9	7.1	13625	PASS
275	198	10	60	25.6	49240	PASS
365	198	1	100	3.2	6080	PASS
441	198	0.01	100	13.0	25091	PASS
442	442	50	100	100.0	167893	PASS
443	442	15	24	19.3	32360	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/27/2022	BNA_N	<u>BN020518.D</u>
Compound Name	Response	Retention Time
DDT	665538	20.598
DDD	37769	20.163
DDE	1294	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39063	704601	5.54

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062722\
 Data File : BN020518.D
 Acq On : 28 Jun 2022 04:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 28 08:03:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 28 08:02:00 2022
 Response via : Initial Calibration

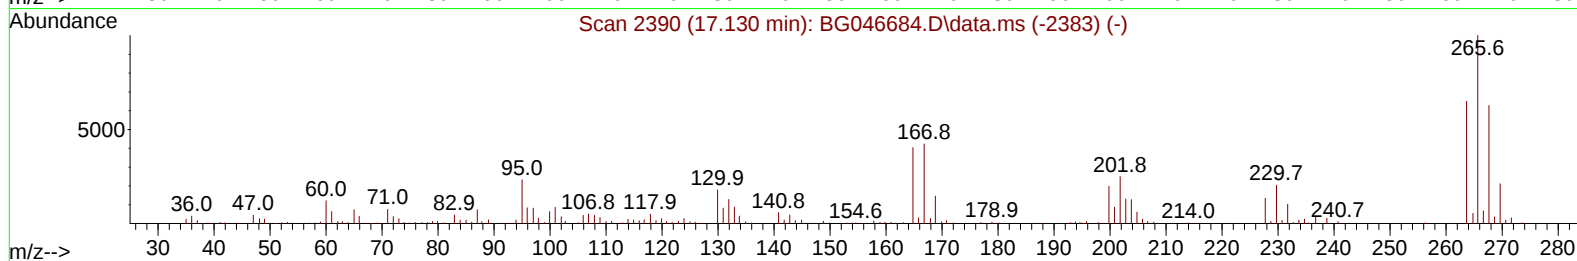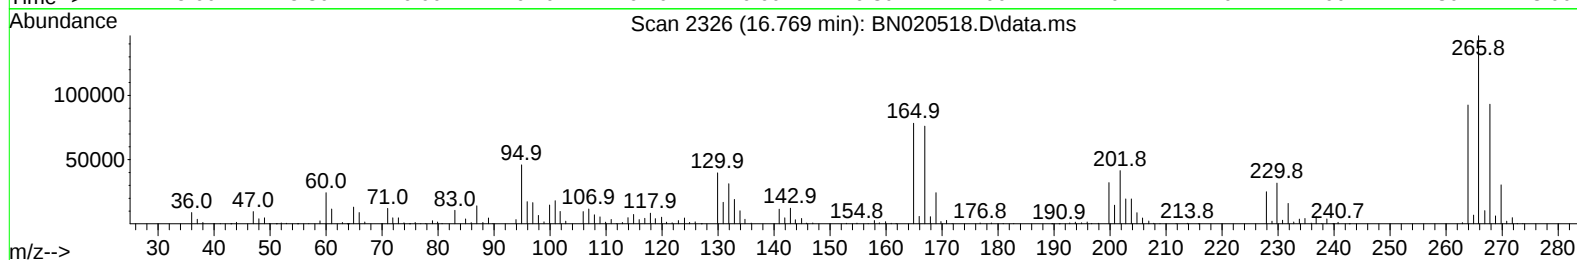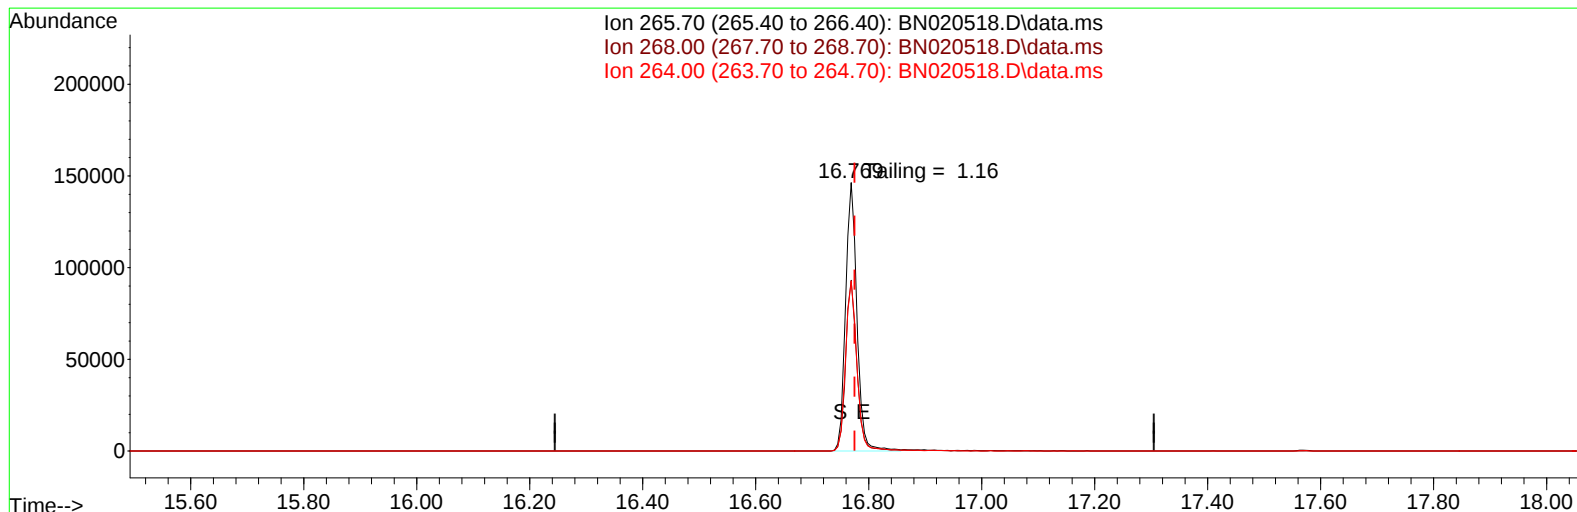

TIC: BN020518.D\data.ms

(70) Pentachlorophenol (C)

16.769min (-0.006) 18846.12 ng




response 206172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.65
264.00	61.60	63.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062722\
Data File : BN020518.D
Acq On : 28 Jun 2022 04:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 28 08:03:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 28 08:02:00 2022
Response via : Initial Calibration

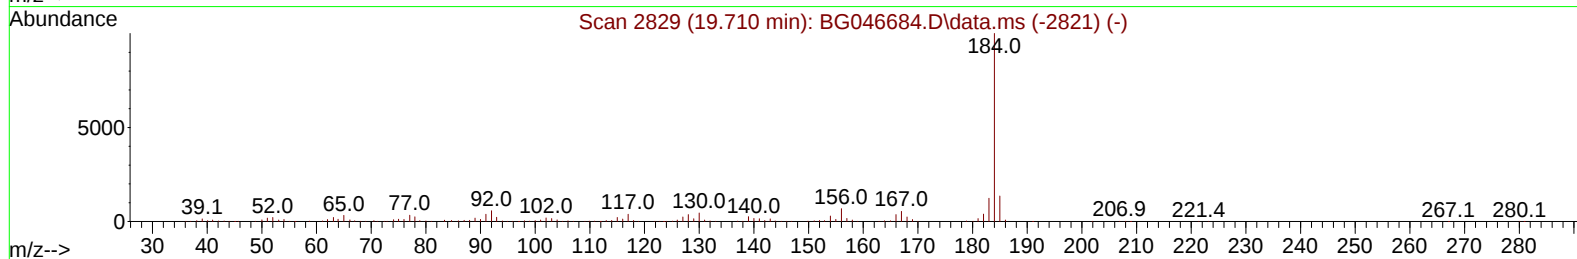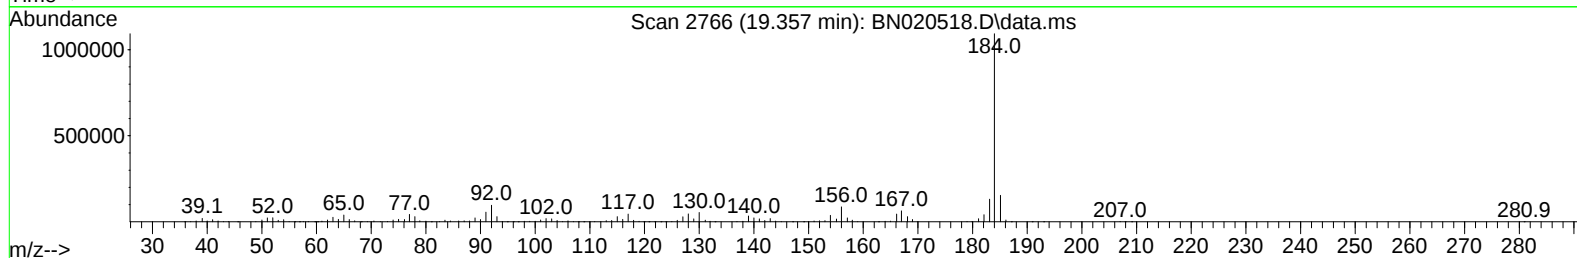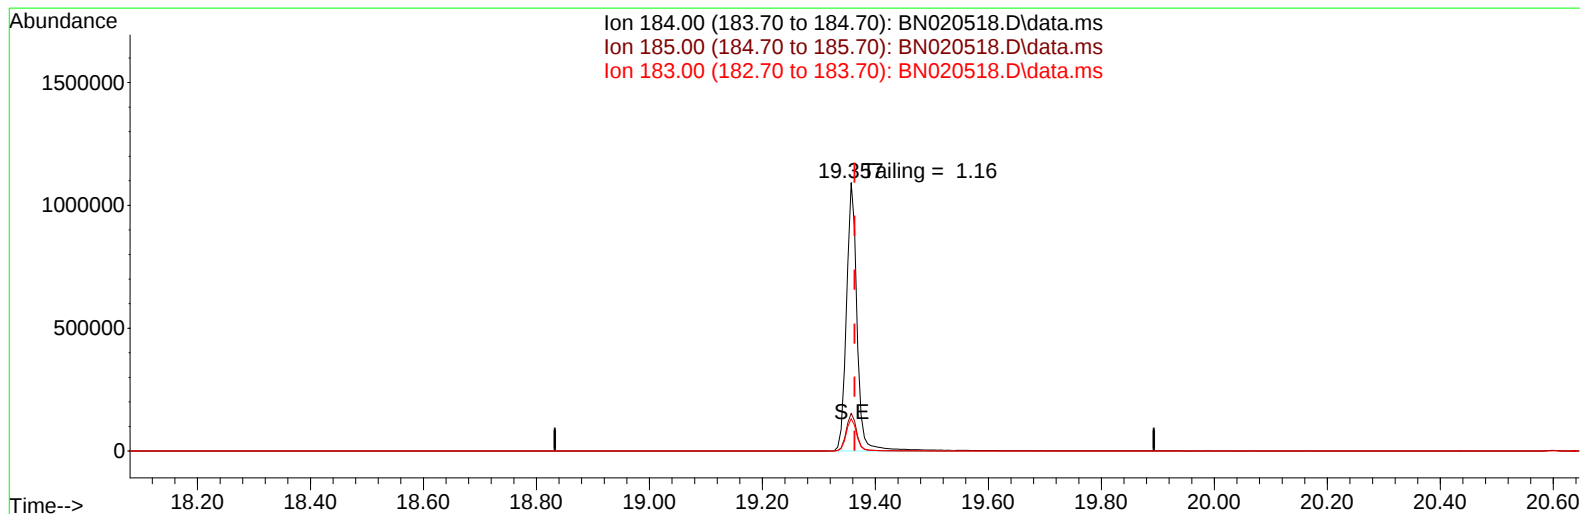

TIC: BN020518.D\data.ms

(77) Benzidine

19.357min (-0.006) 0.00 ng

response 1427506

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.06
183.00	13.20	12.04
0.00	0.00	0.00