
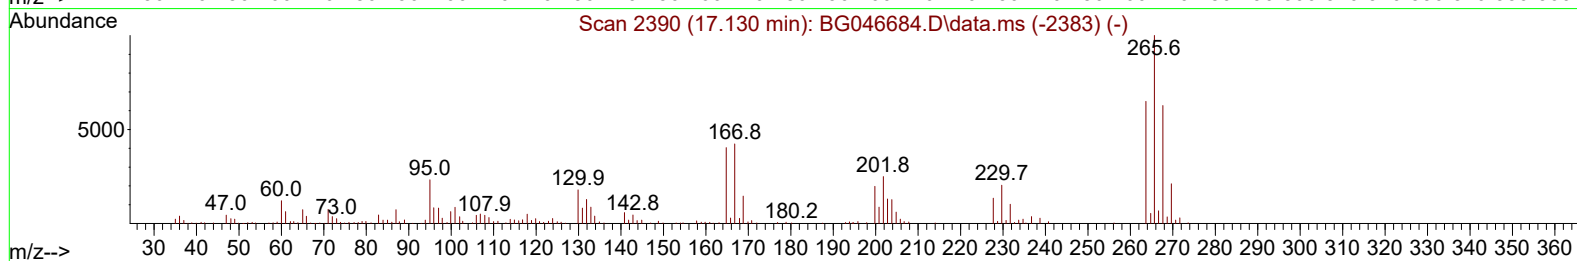
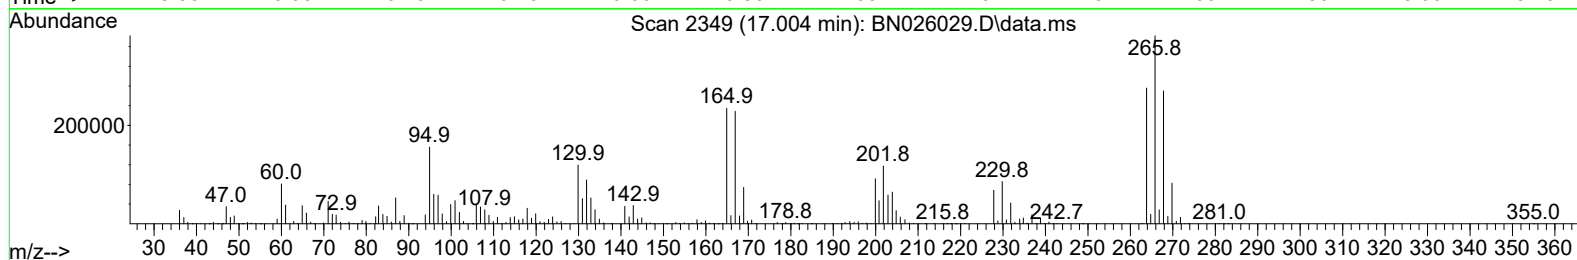


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062723\
Data File : BN026029.D
Acq On : 27 Jun 2023 10:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:19:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 07:19:03 2023
Response via : Initial Calibration

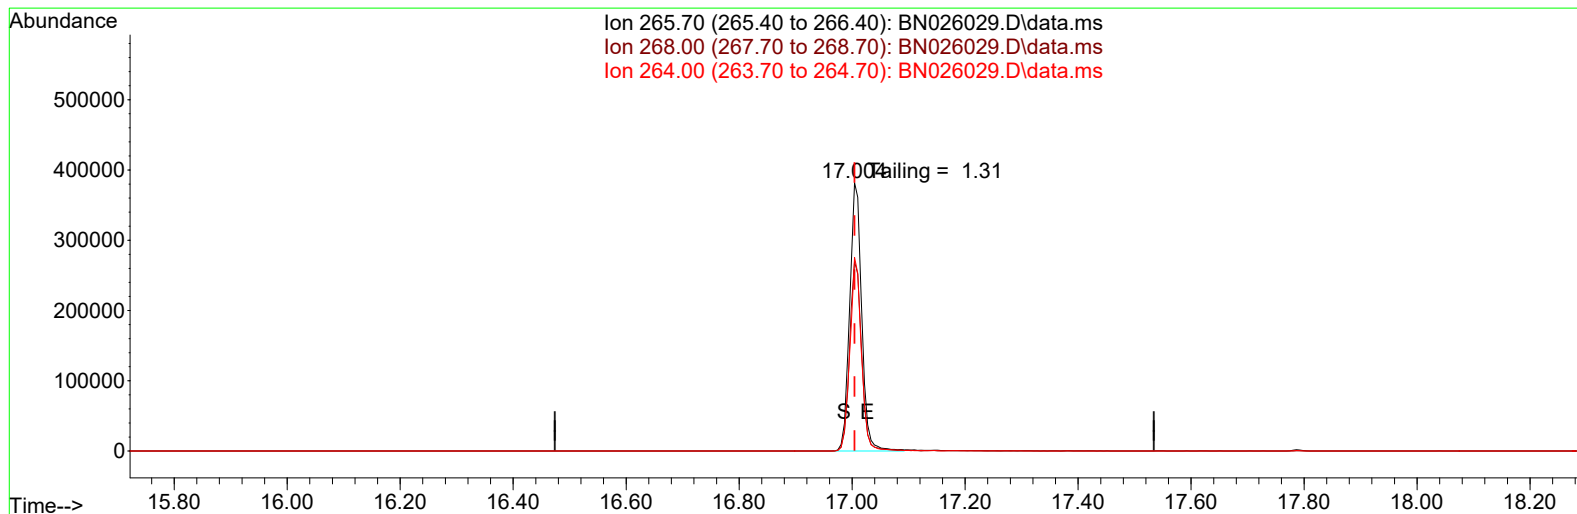

TIC: BN026029.D\data.ms

(70) Pentachlorophenol (C)




17.004min (0.000) 18842.49 ng

response 569008

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.61
264.00	61.60	72.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062723\
Data File : BN026029.D
Acq On : 27 Jun 2023 10:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:19:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 07:19:03 2023
Response via : Initial Calibration

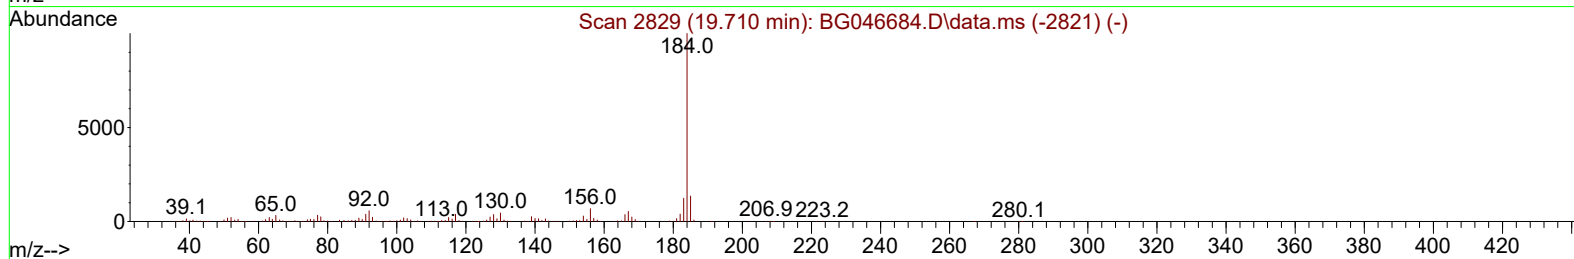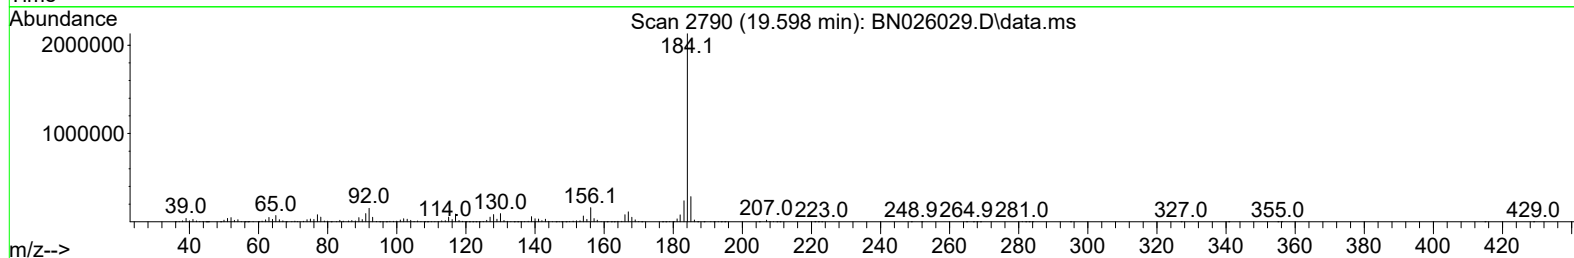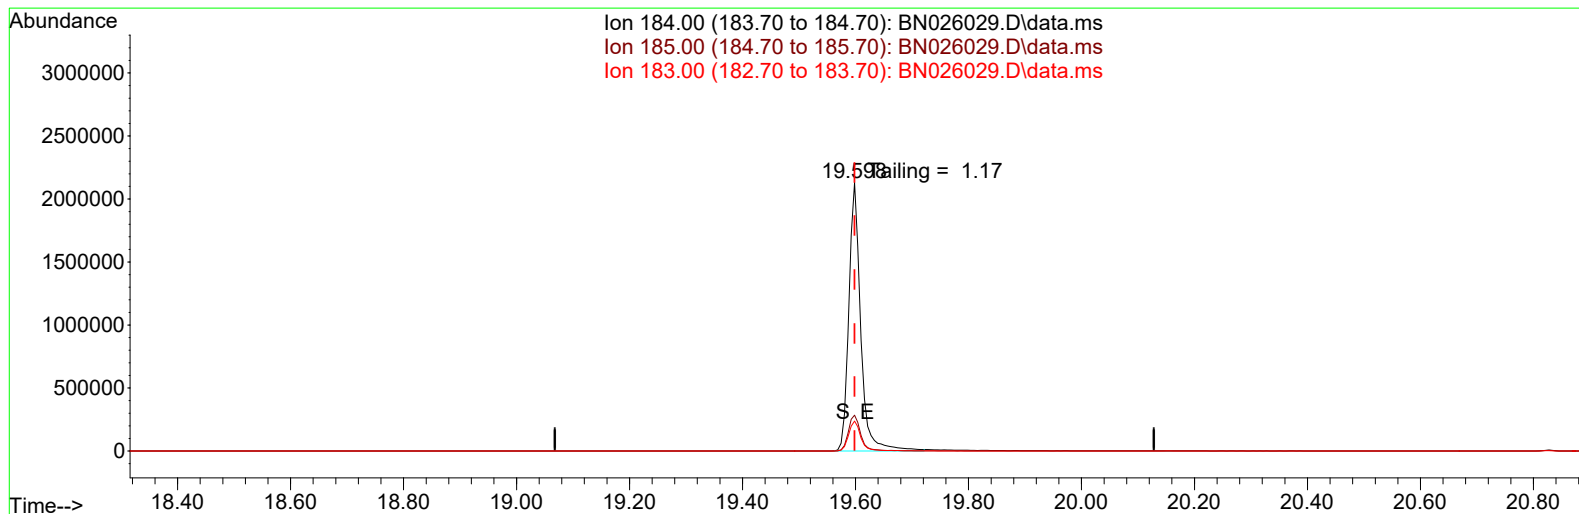

TIC: BN026029.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 3153464

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.34
183.00	13.20	11.16
0.00	0.00	0.00