
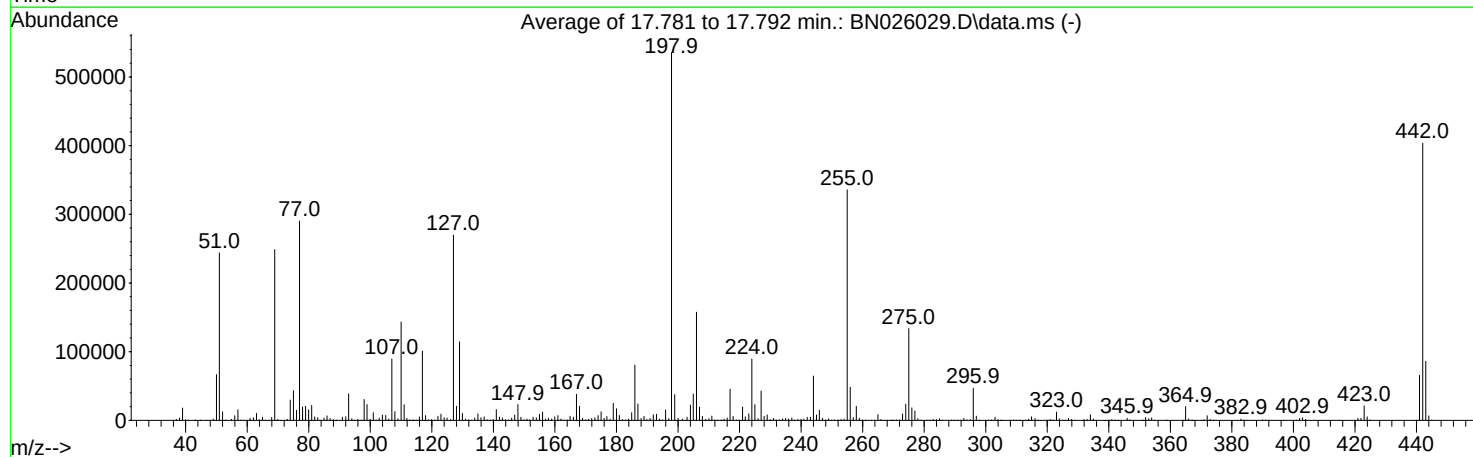


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062723\
Data File : BN026029.D
Acq On : 27 Jun 2023 10:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 28 05:23:31 2023

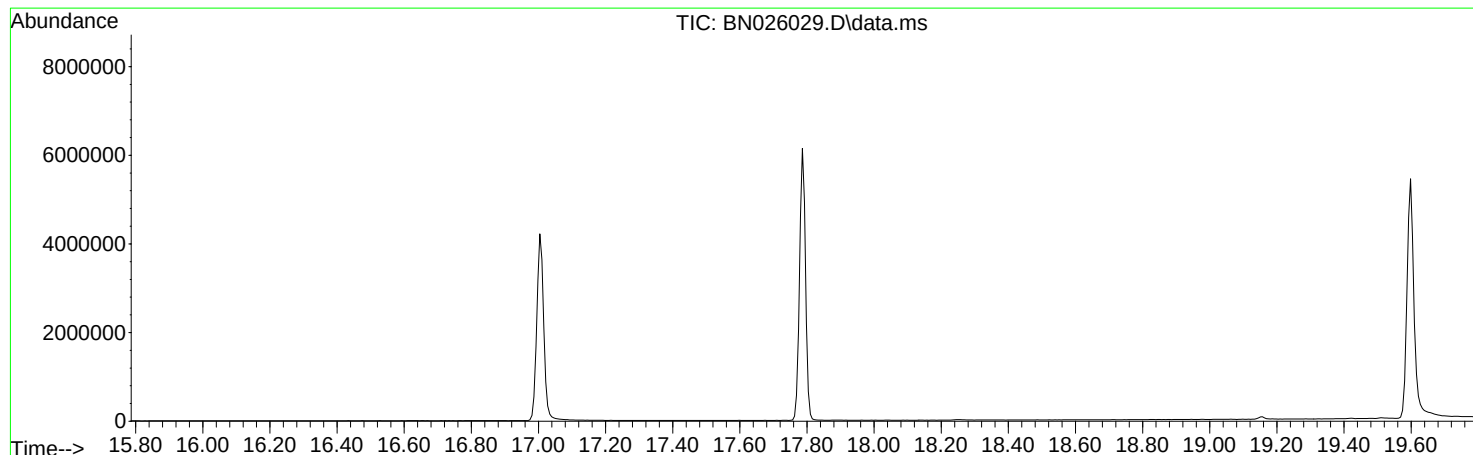

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	45.5	243918	PASS
68	69	0.00	2	1.7	4282	PASS
69	198	0.00	100	46.4	248597	PASS
70	69	0.00	2	0.6	1456	PASS
127	198	10	80	50.4	269845	PASS
197	198	0.00	2	0.5	2615	PASS
198	198	100	100	100.0	535616	PASS
199	198	5	9	7.0	37509	PASS
275	198	10	60	25.0	133693	PASS
365	198	1	100	3.7	19945	PASS
441	198	0.01	100	12.3	65699	PASS
442	442	50	100	100.0	403584	PASS
443	442	15	24	21.3	86029	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/27/2023	BNA_N	<u>BN026029.D</u>
Compound Name	Response	Retention Time
DDT	1715212	20.827
DDD	129184	20.386
DDE	3533	19.875
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
132717	1847929	7.18

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062723\
Data File : BN026029.D
Acq On : 27 Jun 2023 10:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 28 07:19:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 07:19:03 2023
Response via : Initial Calibration

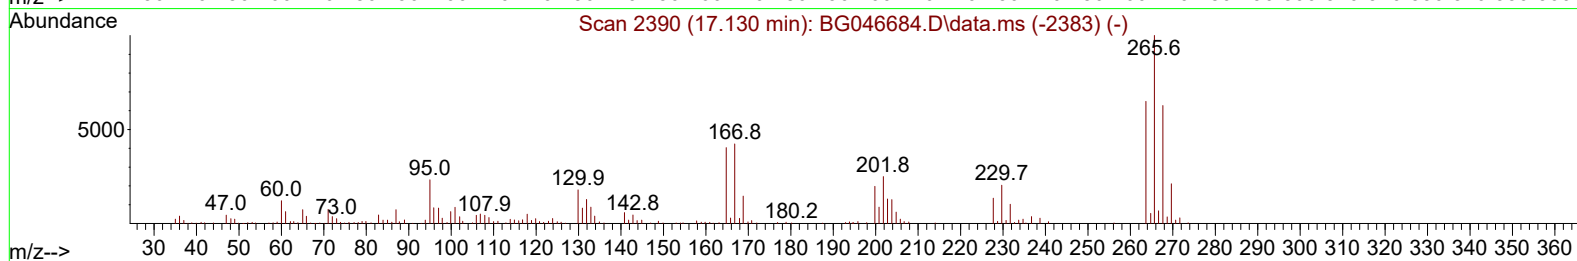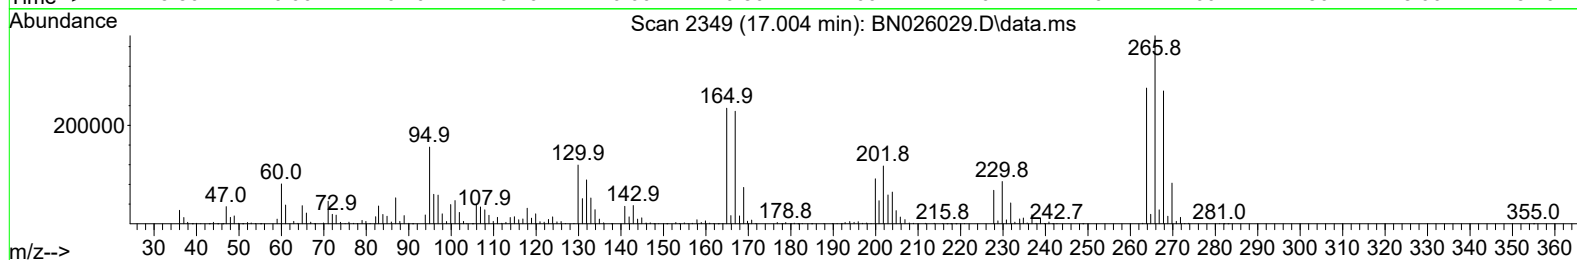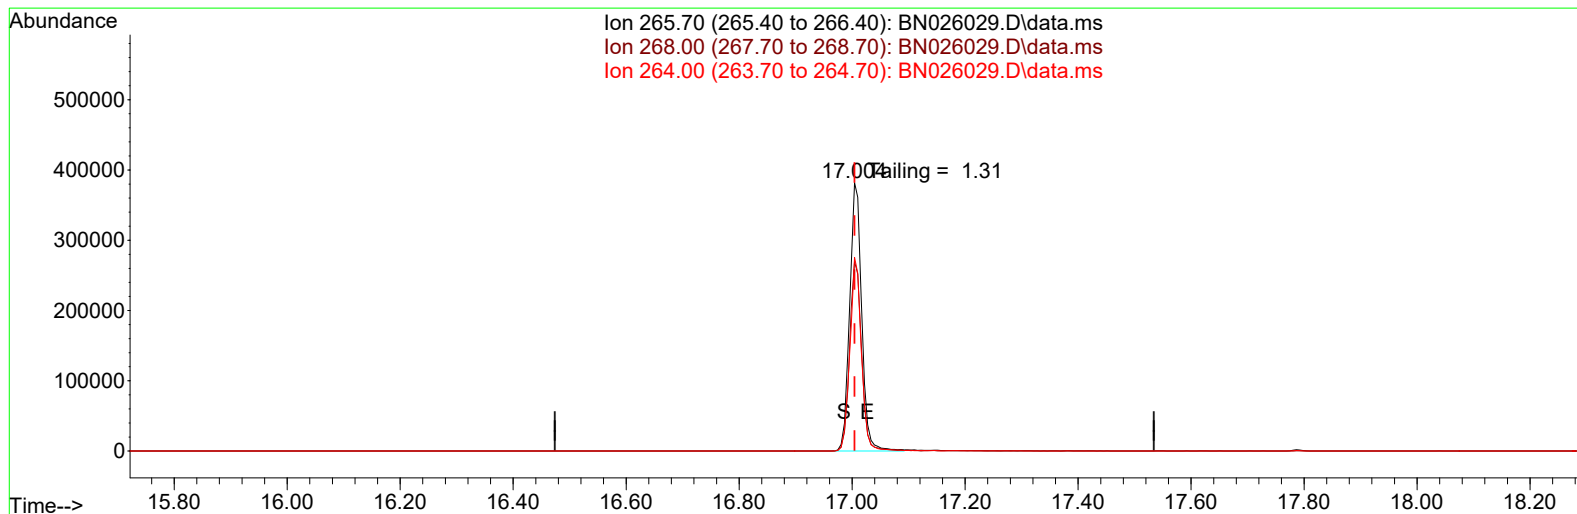

TIC: BN026029.D\data.ms

(70) Pentachlorophenol (C)

17.004min (0.000) 18842.49 ng




response 569008

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.61
264.00	61.60	72.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062723\
Data File : BN026029.D
Acq On : 27 Jun 2023 10:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 28 07:19:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 07:19:03 2023
Response via : Initial Calibration

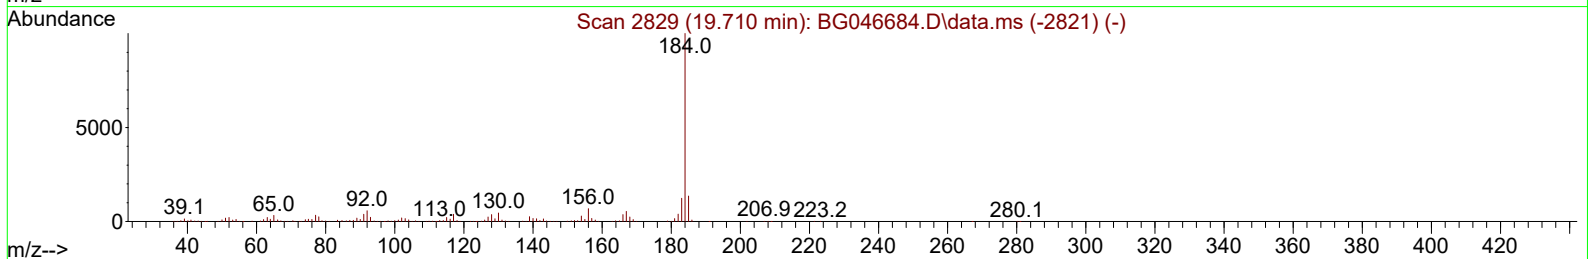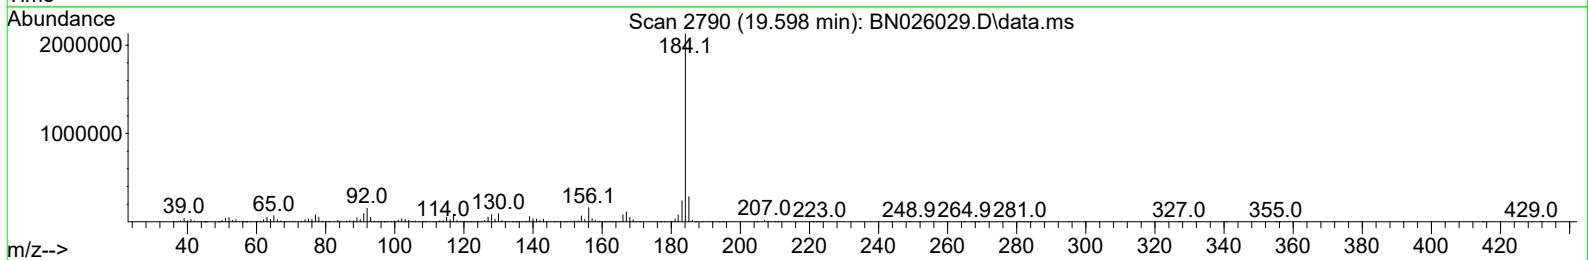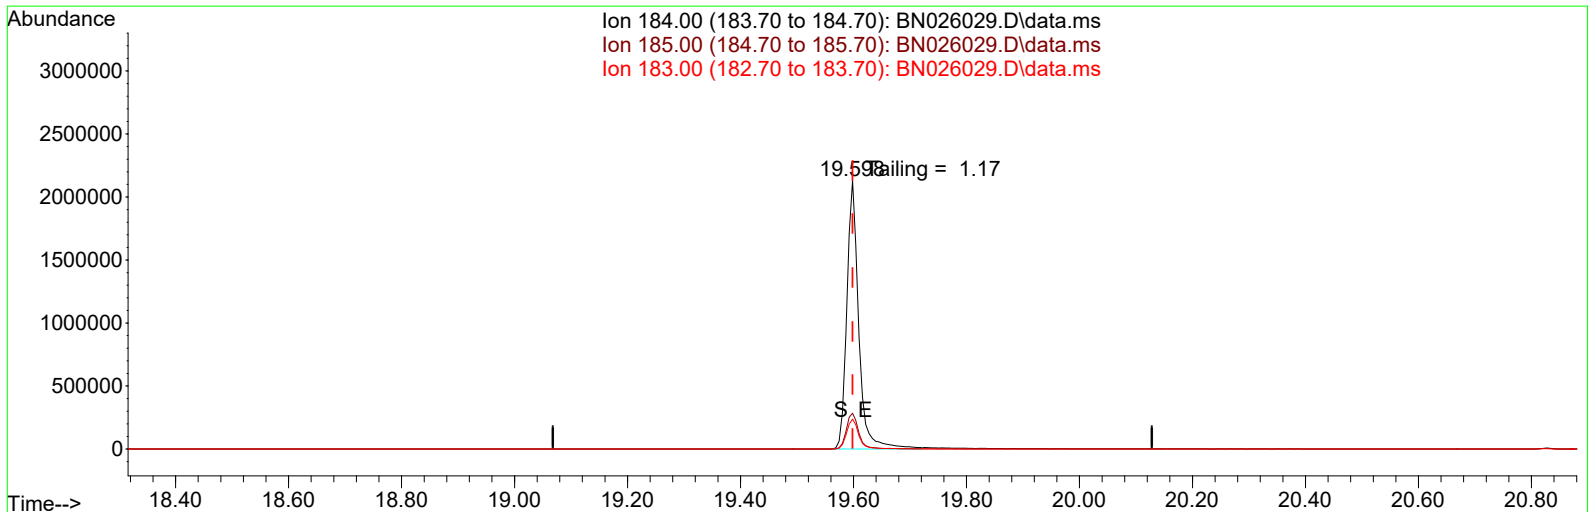

TIC: BN026029.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 3153464

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.34
183.00	13.20	11.16
0.00	0.00	0.00