
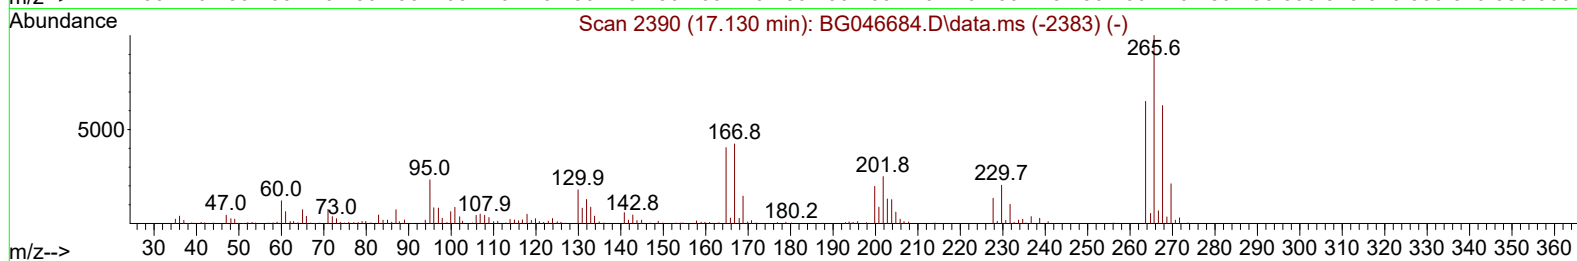
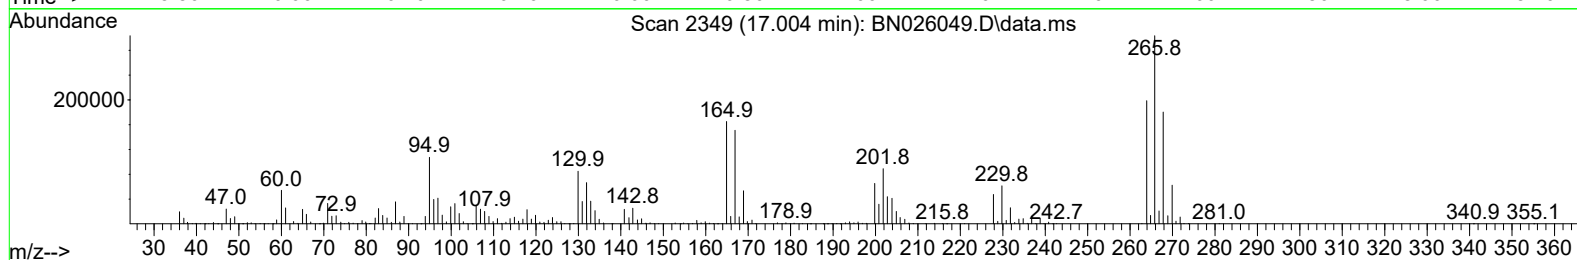


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062823\
Data File : BN026049.D
Acq On : 28 Jun 2023 09:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 06:03:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 29 06:03:22 2023
Response via : Initial Calibration

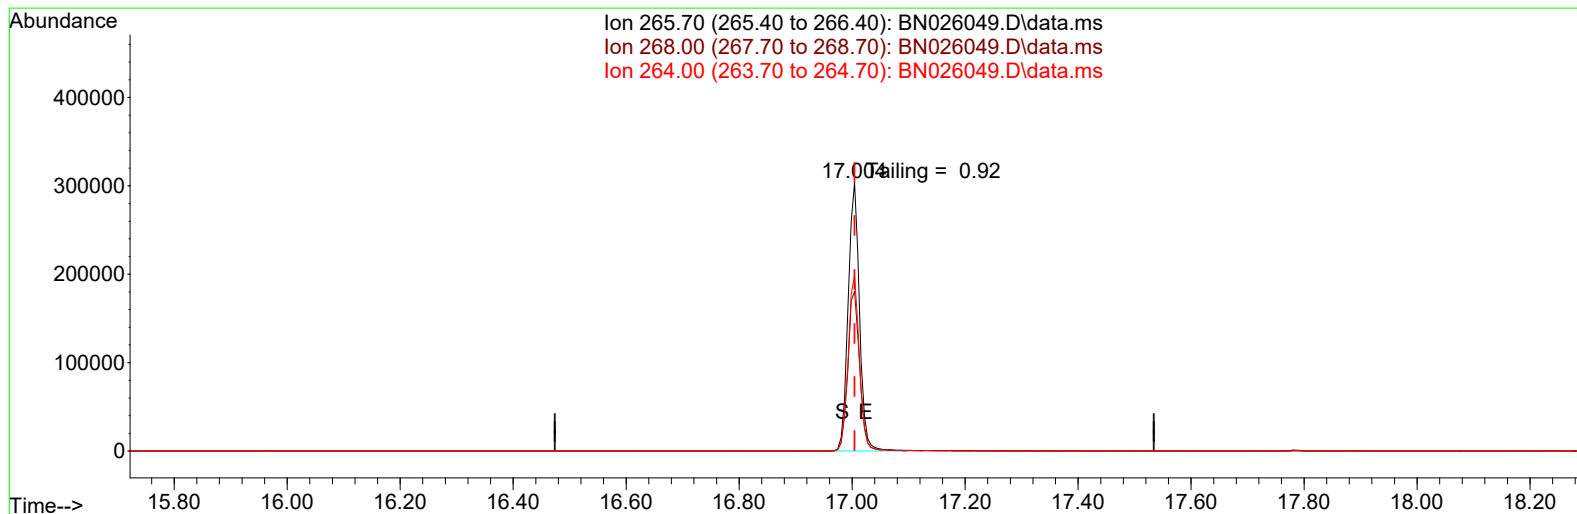

TIC: BN026049.D\data.ms

(70) Pentachlorophenol (C)




17.004min (0.000) 19797.32 ng

response 425543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.42
264.00	61.60	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062823\
Data File : BN026049.D
Acq On : 28 Jun 2023 09:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 06:03:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 29 06:03:22 2023
Response via : Initial Calibration

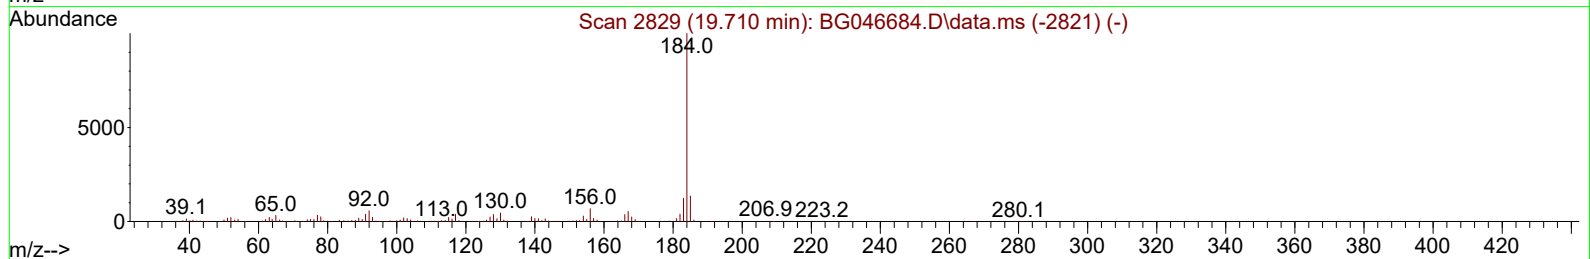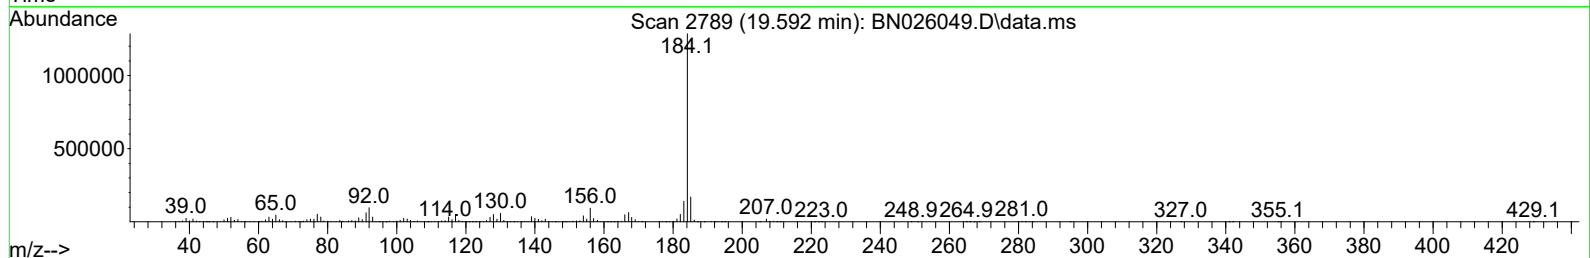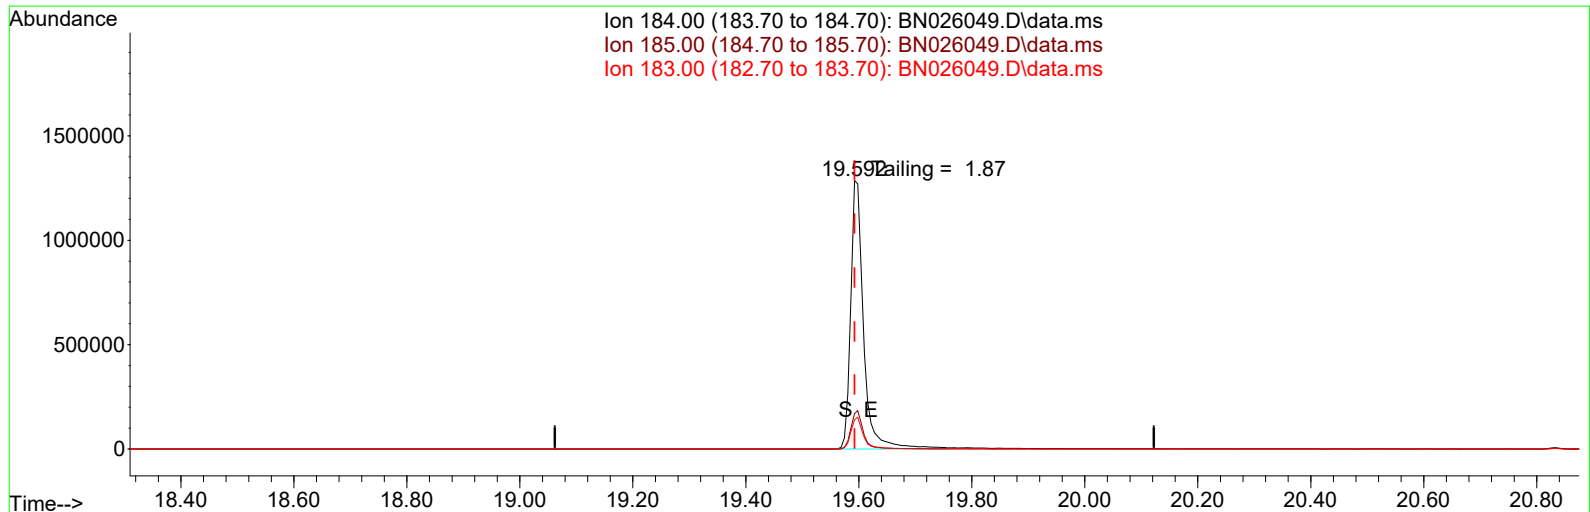

TIC: BN026049.D\data.ms

(77) Benzidine

19.592min (0.000) 0.00 ng

response 2056241

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.24
183.00	13.20	10.91
0.00	0.00	0.00