
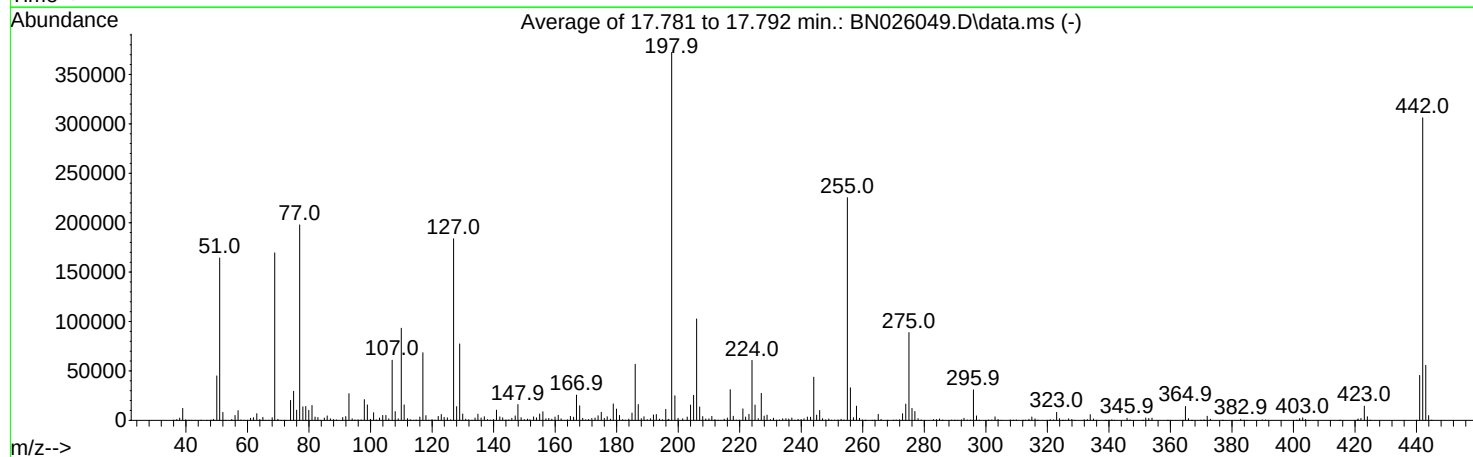


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062823\
 Data File : BN026049.D
 Acq On : 28 Jun 2023 09:06
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 05:23:31 2023

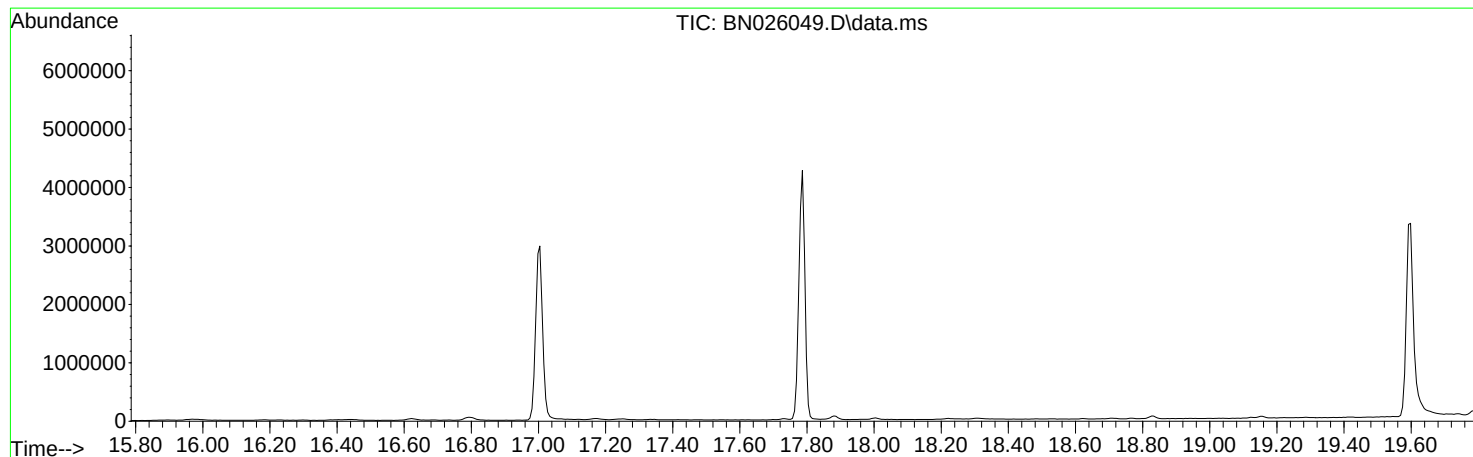

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	164392	PASS
68	69	0.00	2	1.7	2816	PASS
69	198	0.00	100	45.5	169513	PASS
70	69	0.00	2	0.7	1212	PASS
127	198	10	80	49.4	183723	PASS
197	198	0.00	2	0.3	1225	PASS
198	198	100	100	100.0	372203	PASS
199	198	5	9	6.7	24995	PASS
275	198	10	60	23.9	88880	PASS
365	198	1	100	3.8	14109	PASS
441	198	0.01	100	12.2	45512	PASS
442	442	50	100	100.0	306091	PASS
443	442	15	24	18.2	55733	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/28/2023	BNA_N	<u>BN026049.D</u>
Compound Name	Response	Retention Time
DDT	1247900	20.833
DDD	63994	20.392
DDE	3361	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
67355	1315255	5.12

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062823\
Data File : BN026049.D
Acq On : 28 Jun 2023 09:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 29 06:03:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 29 06:03:22 2023
Response via : Initial Calibration

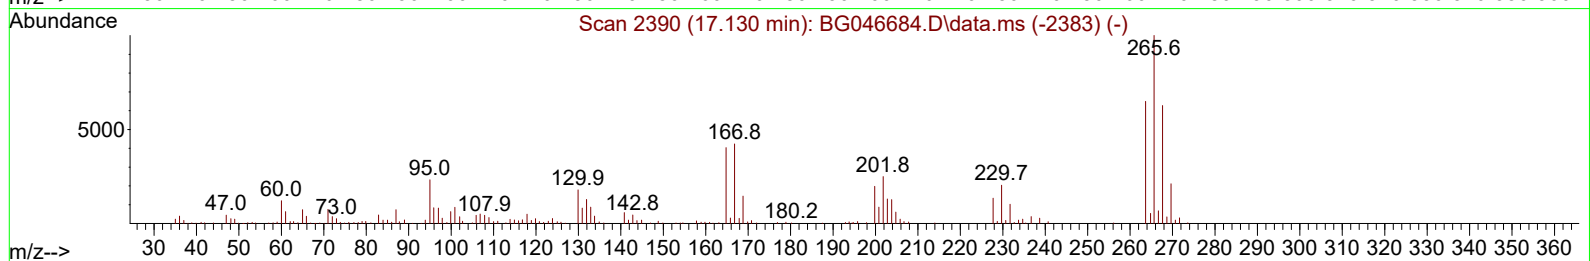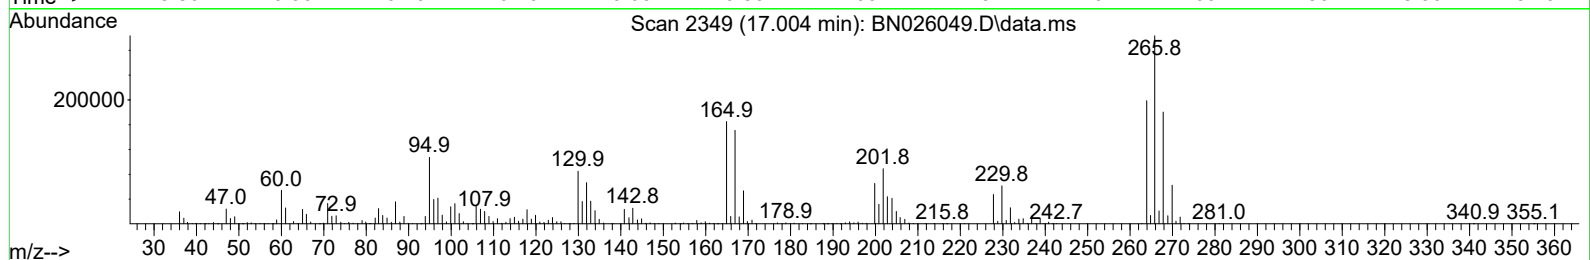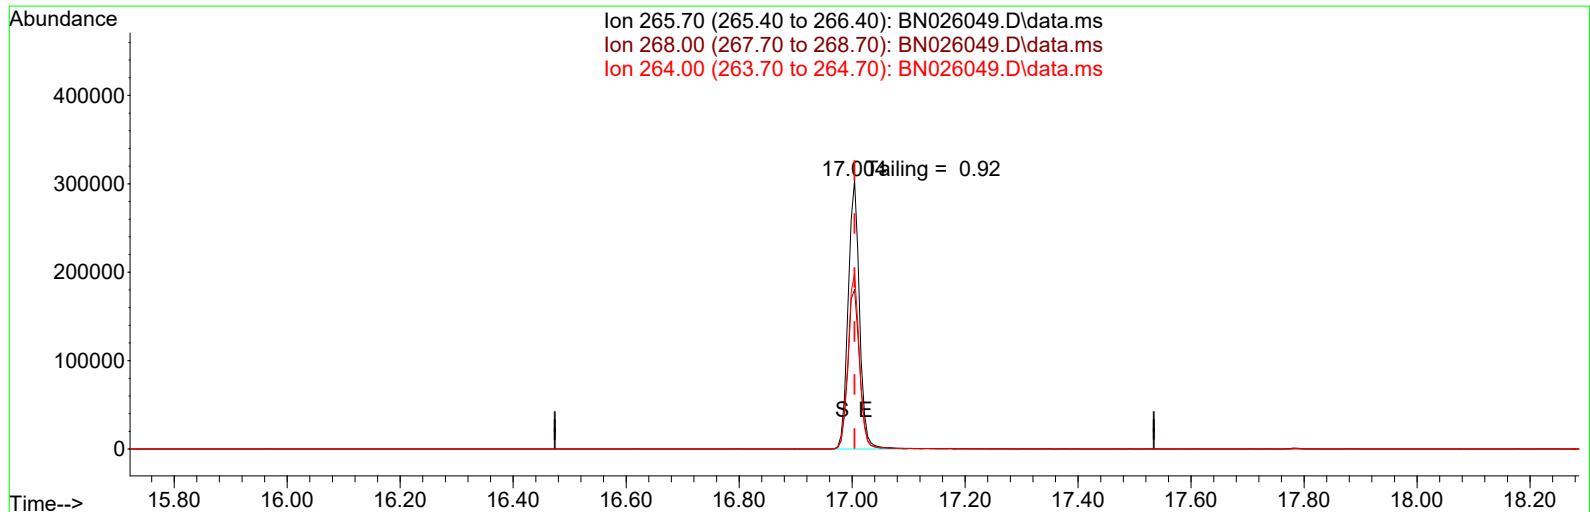

TIC: BN026049.D\data.ms

(70) Pentachlorophenol (C)

17.004min (0.000) 19797.32 ng




response 425543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.42
264.00	61.60	65.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062823\
Data File : BN026049.D
Acq On : 28 Jun 2023 09:06
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 29 06:03:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 29 06:03:22 2023
Response via : Initial Calibration

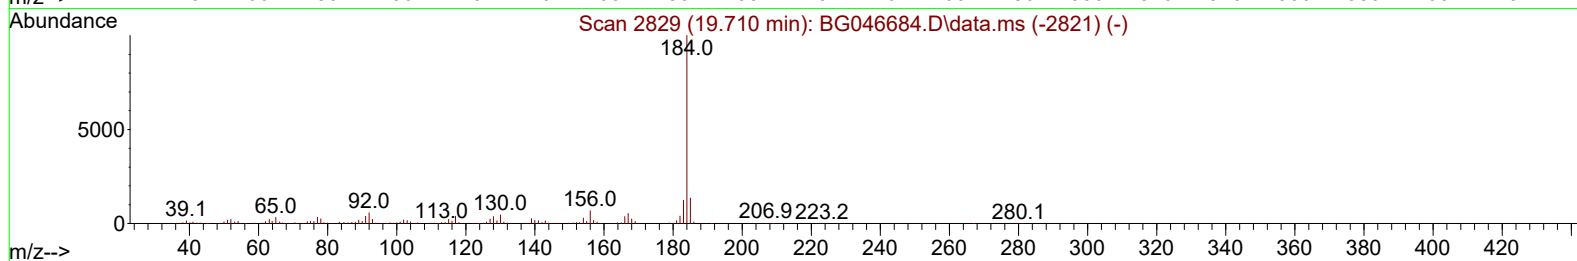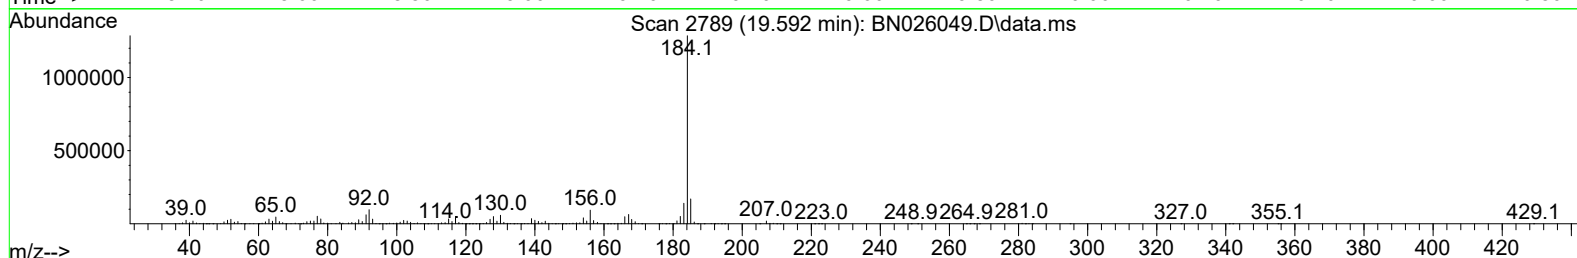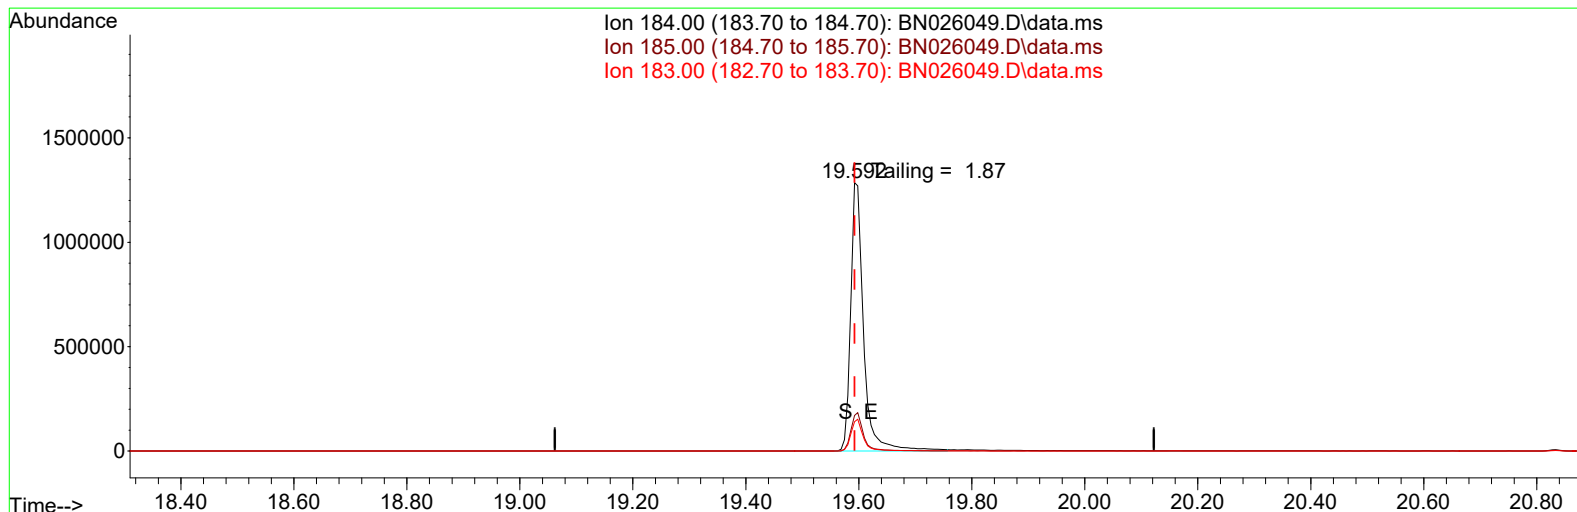

TIC: BN026049.D\data.ms

(77) Benzidine

19.592min (0.000) 0.00 ng

response 2056241

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.24
183.00	13.20	10.91
0.00	0.00	0.00