

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
 Data File : BN032339.D
 Acq On : 29 Jun 2024 07:29
 Operator : MA/JU
 Sample : PB161564BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK564

Quant Time: Jun 30 23:03:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 27 13:23:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.612	152	9651	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	31546	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.258	164	17680	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.109	188	1933891	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.23
23) Perylene-d12	23.430	264	31310	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.148	96	59911	5.585	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.993	152	12936	0.273	ng/ul	0.00
18) Fluoranthene-d10	19.050	212	20528	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.257	166	3754	0.055	ng/ul#	13
26) Benzo(a)pyrene	23.283	252	6847	0.072	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
Data File : BN032339.D
Acq On : 29 Jun 2024 07:29
Operator : MA/JU
Sample : PB161564BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK564

Quant Time: Jun 30 23:03:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

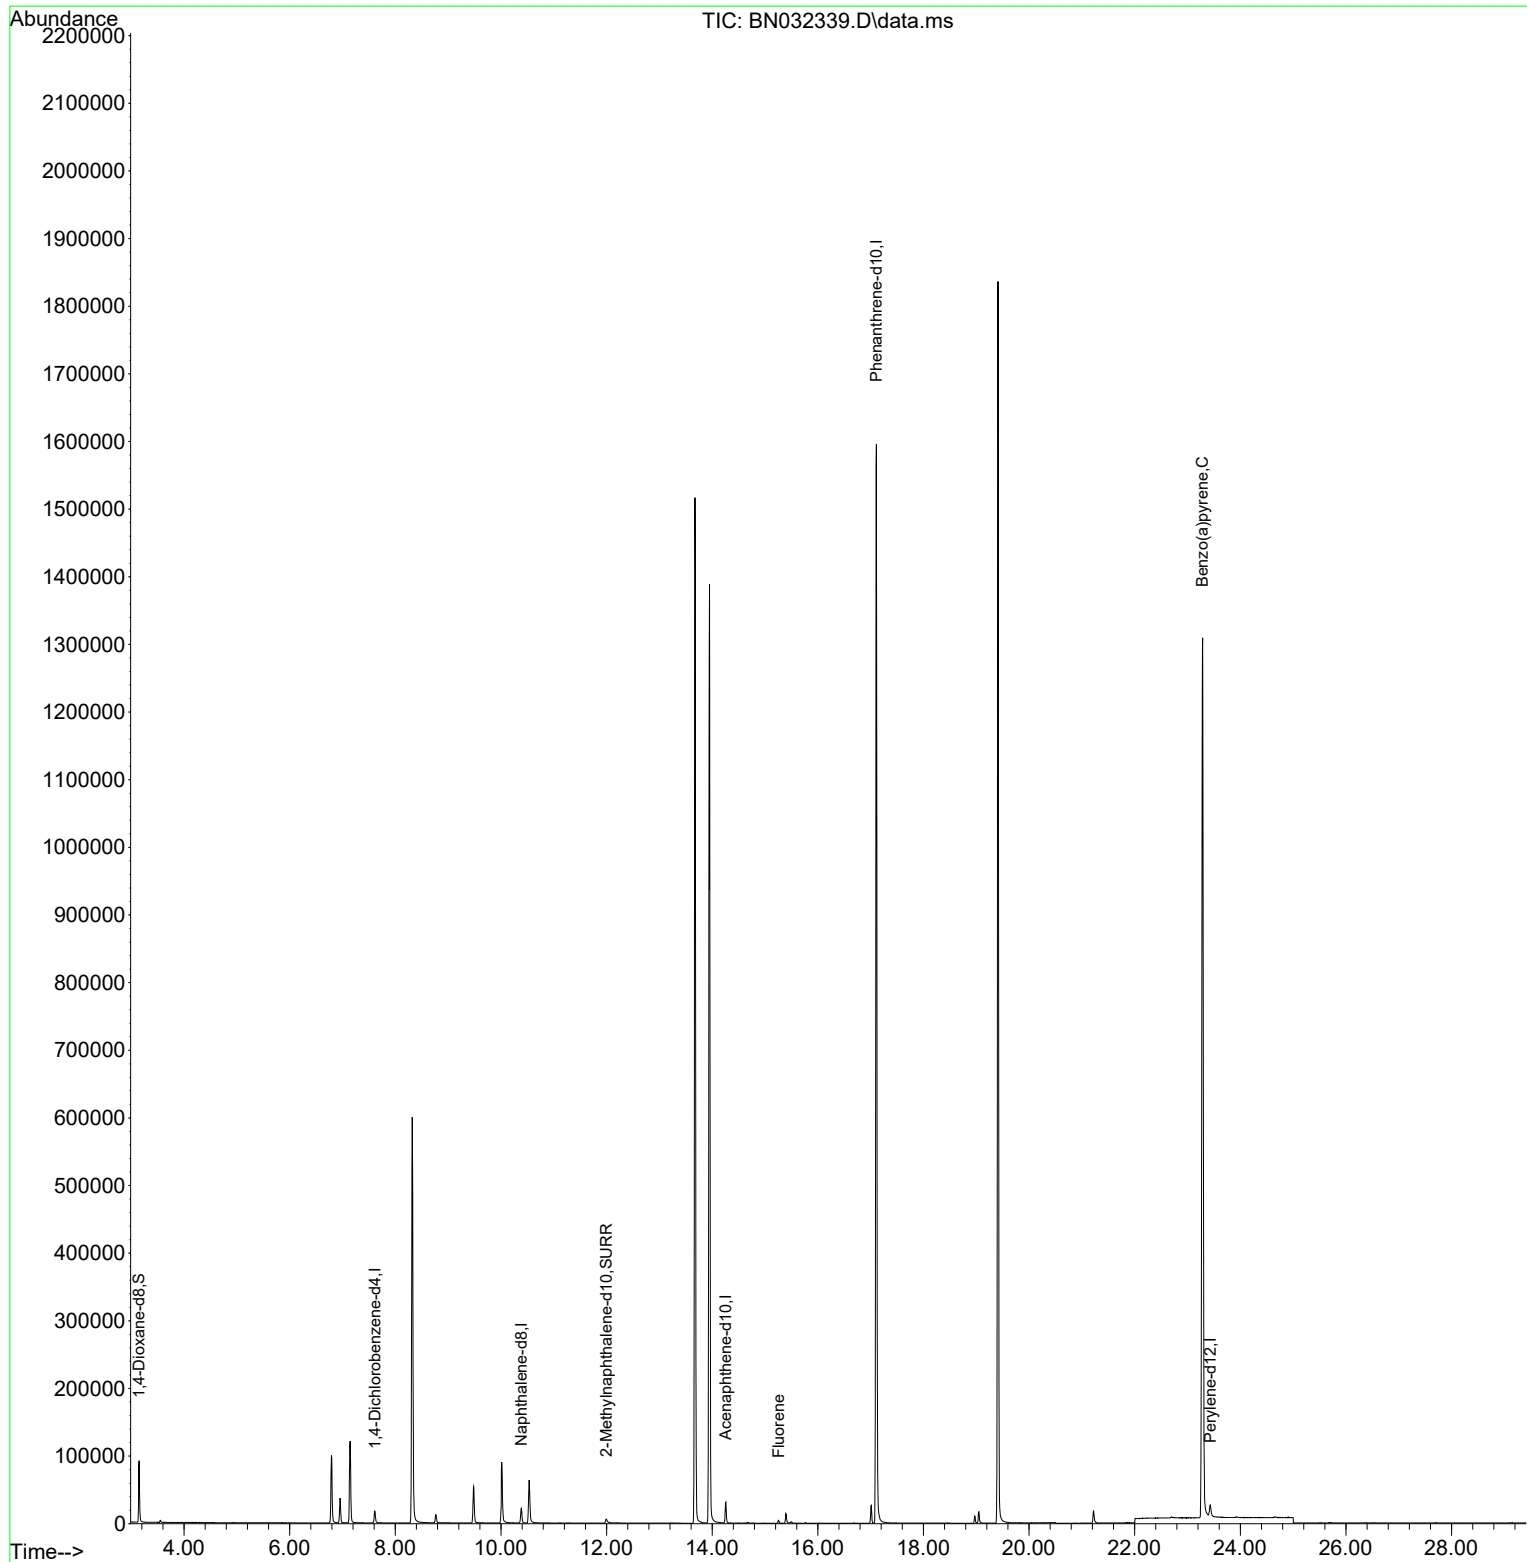

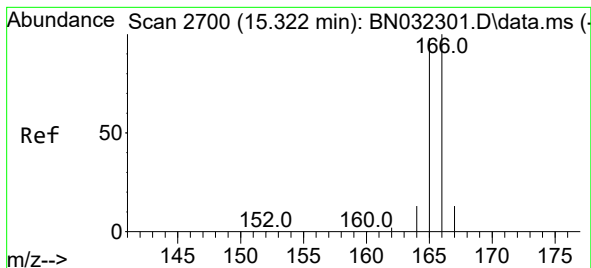

#12

Fluorene

Concen: 0.055 ng/ul

RT: 15.257 min Scan# 2

Delta R.T. -0.070 min

Lab File: BN032339.D

Acq: 29 Jun 2024 07:29

Instrument :

BNA_N

ClientSampleId :

SBLK564





Tgt Ion:166 Resp: 3754

Ion Ratio Lower Upper

166 100

165 7.3 79.0 118.6#

167 34.7 11.0 16.6#

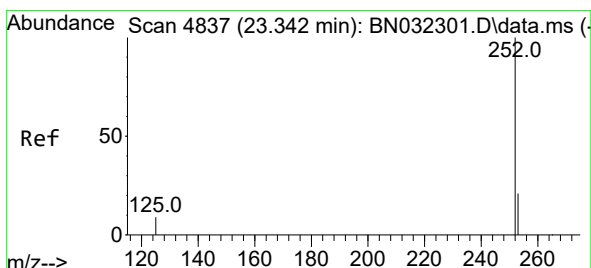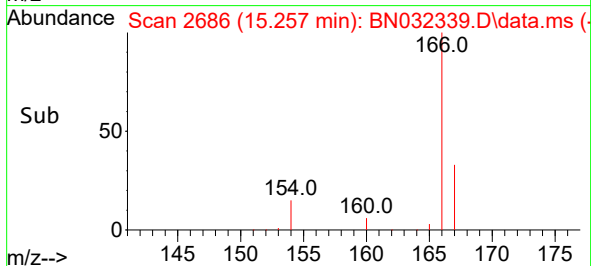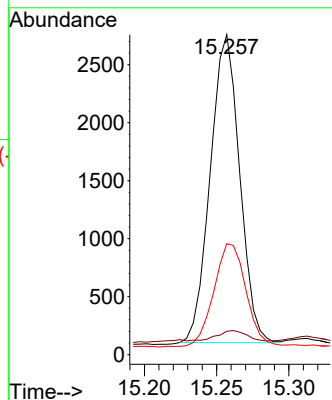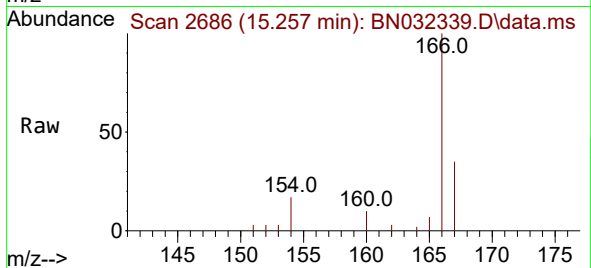

#26

Benzo(a)pyrene

Concen: 0.072 ng/ul

RT: 23.283 min Scan# 4817

Delta R.T. -0.076 min

Lab File: BN032339.D

Acq: 29 Jun 2024 07:29

Tgt Ion:252 Resp: 6847

Ion Ratio Lower Upper

252 100

253 48.7 22.2 33.2#

125 55.5 16.4 24.6#

