

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
 Data File : BN032340.D
 Acq On : 29 Jun 2024 08:05
 Operator : MA/JU
 Sample : PB161631BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK631

Quant Time: Jun 30 23:03:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 27 13:23:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.612	152	9798	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	32111	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.258	164	18356	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.109	188	1646106	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.23
23) Perylene-d12	23.433	264	30004	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.148	96	50562	4.643	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.993	152	10846	0.225	ng/ul	0.00
18) Fluoranthene-d10	19.050	212	16610	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.257	166	3218	0.046	ng/ul#	13
26) Benzo(a)pyrene	23.283	252	5223	0.058	ng/ul#	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
Data File : BN032340.D
Acq On : 29 Jun 2024 08:05
Operator : MA/JU
Sample : PB161631BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK631

Quant Time: Jun 30 23:03:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

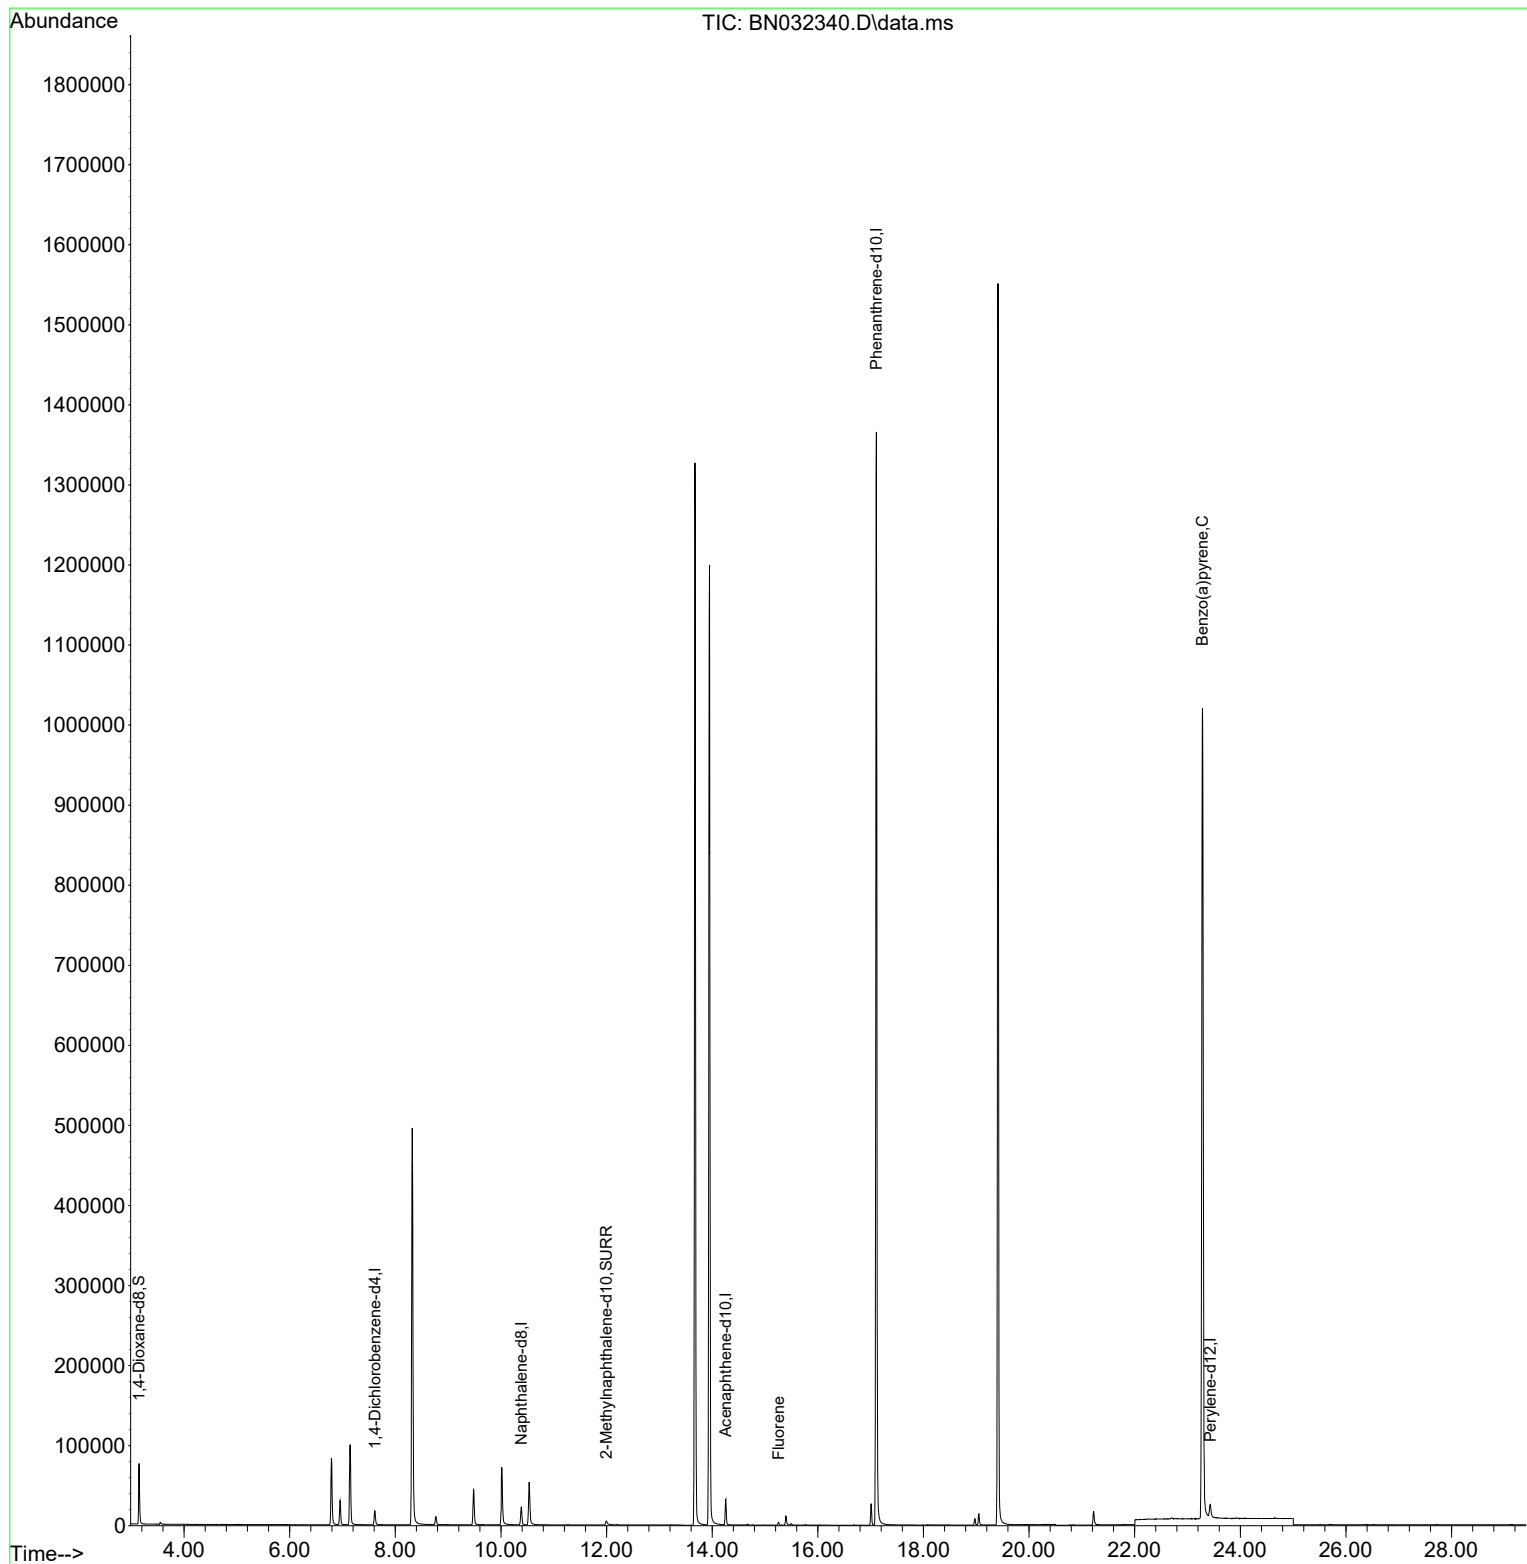

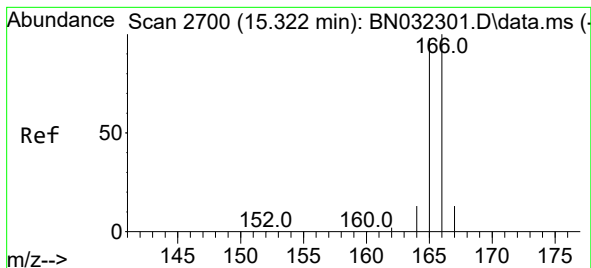

#12

Fluorene

Concen: 0.046 ng/ul

RT: 15.257 min Scan# 2

Delta R.T. -0.070 min

Lab File: BN032340.D

Acq: 29 Jun 2024 08:05

Instrument :

BNA_N

ClientSampleId :

SBLK631





Tgt Ion:166 Resp: 3218

Ion Ratio Lower Upper

166 100

165 7.8 79.0 118.6#

167 36.1 11.0 16.6#

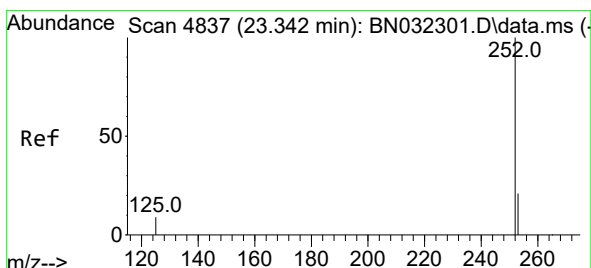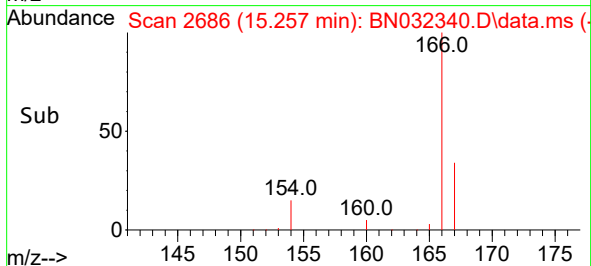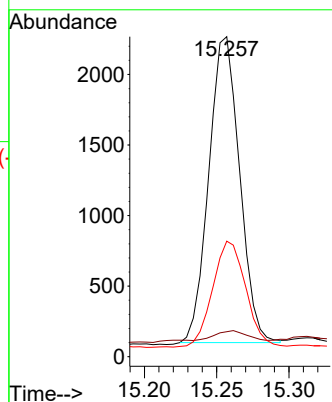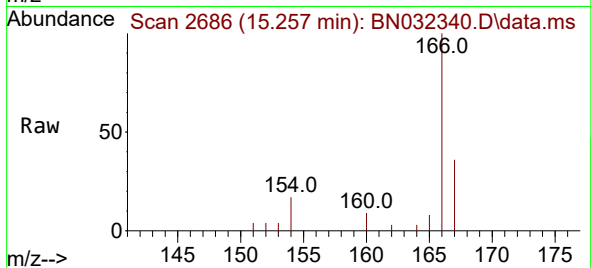

#26

Benzo(a)pyrene

Concen: 0.058 ng/ul

RT: 23.283 min Scan# 4817

Delta R.T. -0.076 min

Lab File: BN032340.D

Acq: 29 Jun 2024 08:05

Tgt Ion:252 Resp: 5223

Ion Ratio Lower Upper

252 100

253 52.9 22.2 33.2#

125 59.9 16.4 24.6#

