

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
 Data File : BN032310.D
 Acq On : 28 Jun 2024 12:49
 Operator : MA/JU
 Sample : P2898-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1G83

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jun 28 15:07:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 27 13:23:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	9225	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	29529	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.262	164	17018	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.012	188	30183m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.220	240	20247m	0.400	ng/ul	0.00
23) Perylene-d12	23.439	264	19966m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.148	96	44037	4.295	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.988	152	14975	0.338	ng/ul	-0.01
18) Fluoranthene-d10	19.050	212	24995	0.410	ng/ul	0.00
Target Compounds						Qvalue
27) Indeno(1,2,3-cd)pyrene	25.693	276	2064	0.022	ng/ul#	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
Data File : BN032310.D
Acq On : 28 Jun 2024 12:49
Operator : MA/JU
Sample : P2898-05
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1G83

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 07/04/2024


Quant Time: Jun 28 15:07:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

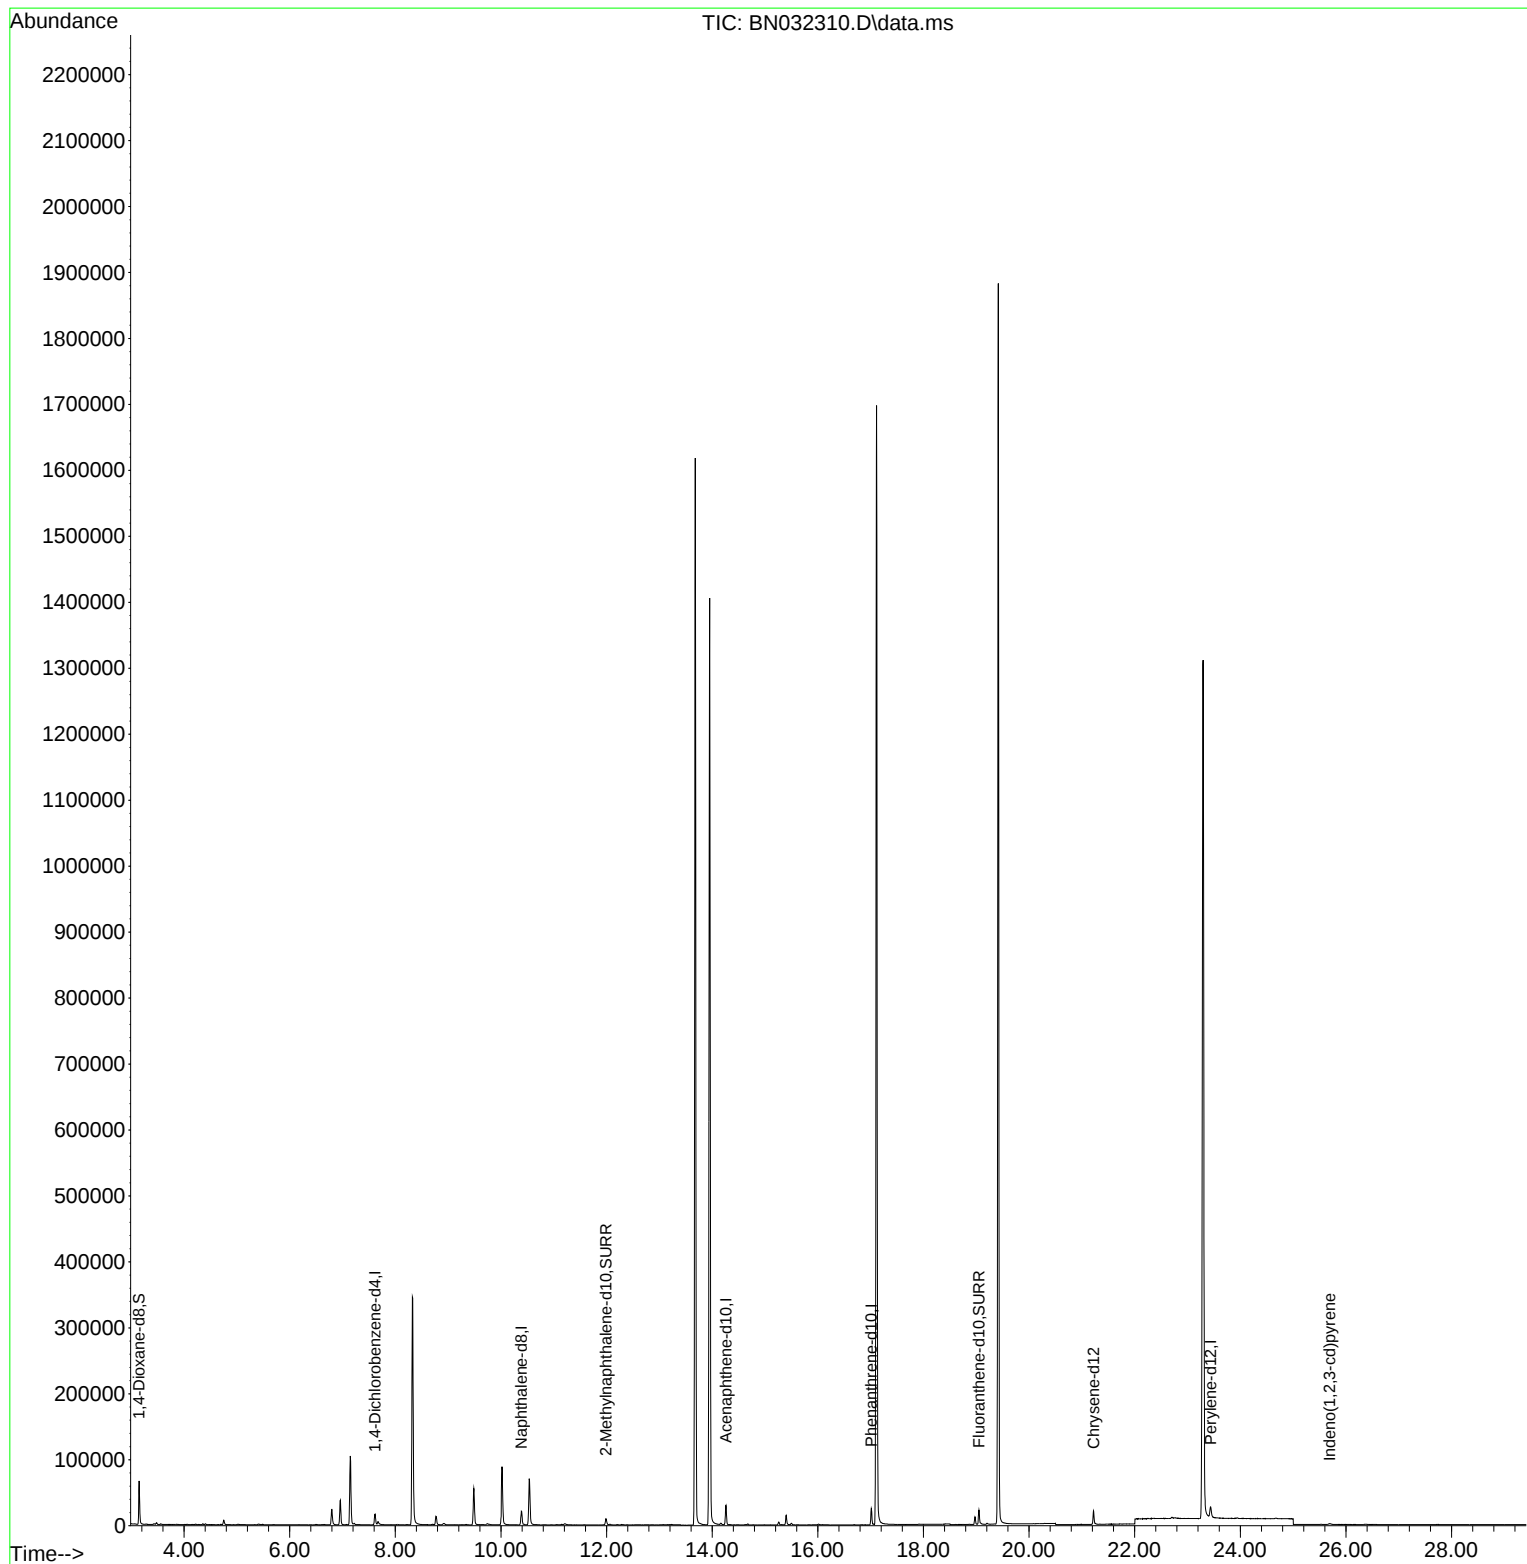

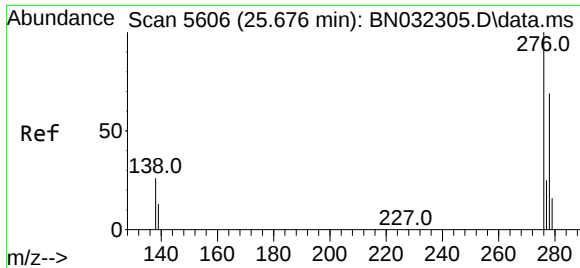

#27
 Indeno(1,2,3-cd)pyrene
 Concen: 0.022 ng/ul
 RT: 25.693 min Scan# 50
 Delta R.T. -0.007 min
 Lab File: BN032310.D
 Acq: 28 Jun 2024 12:49

Instrument :
 BNA_N
 ClientSampleId :
 E1G83

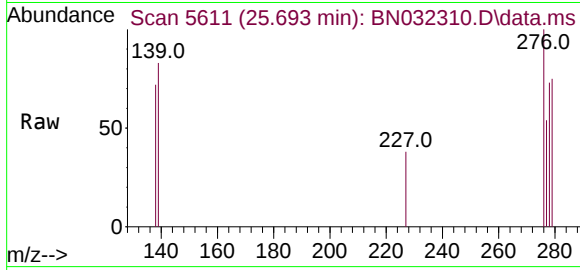

Tgt Ion: 276 Resp: 2064
 Ion Ratio Lower Upper
 276 100
 138 25.9 21.3 31.9
 227 0.2 0.1 0.1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 07/04/2024

