

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
 Data File : BN032316.D
 Acq On : 28 Jun 2024 16:26
 Operator : MA/JU
 Sample : P2898-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GD7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jun 28 17:07:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 27 13:23:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	8276	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	26419	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.262	164	15289	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.012	188	26402m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.223	240	17249m	0.400	ng/ul	0.00
23) Perylene-d12	23.438	264	16762m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.148	96	37430	4.069	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.988	152	11563	0.292	ng/ul	-0.01
18) Fluoranthene-d10	19.050	212	19020	0.366	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.437	128	5700	0.082	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
Data File : BN032316.D
Acq On : 28 Jun 2024 16:26
Operator : MA/JU
Sample : P2898-14
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GD7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 07/04/2024


Quant Time: Jun 28 17:07:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

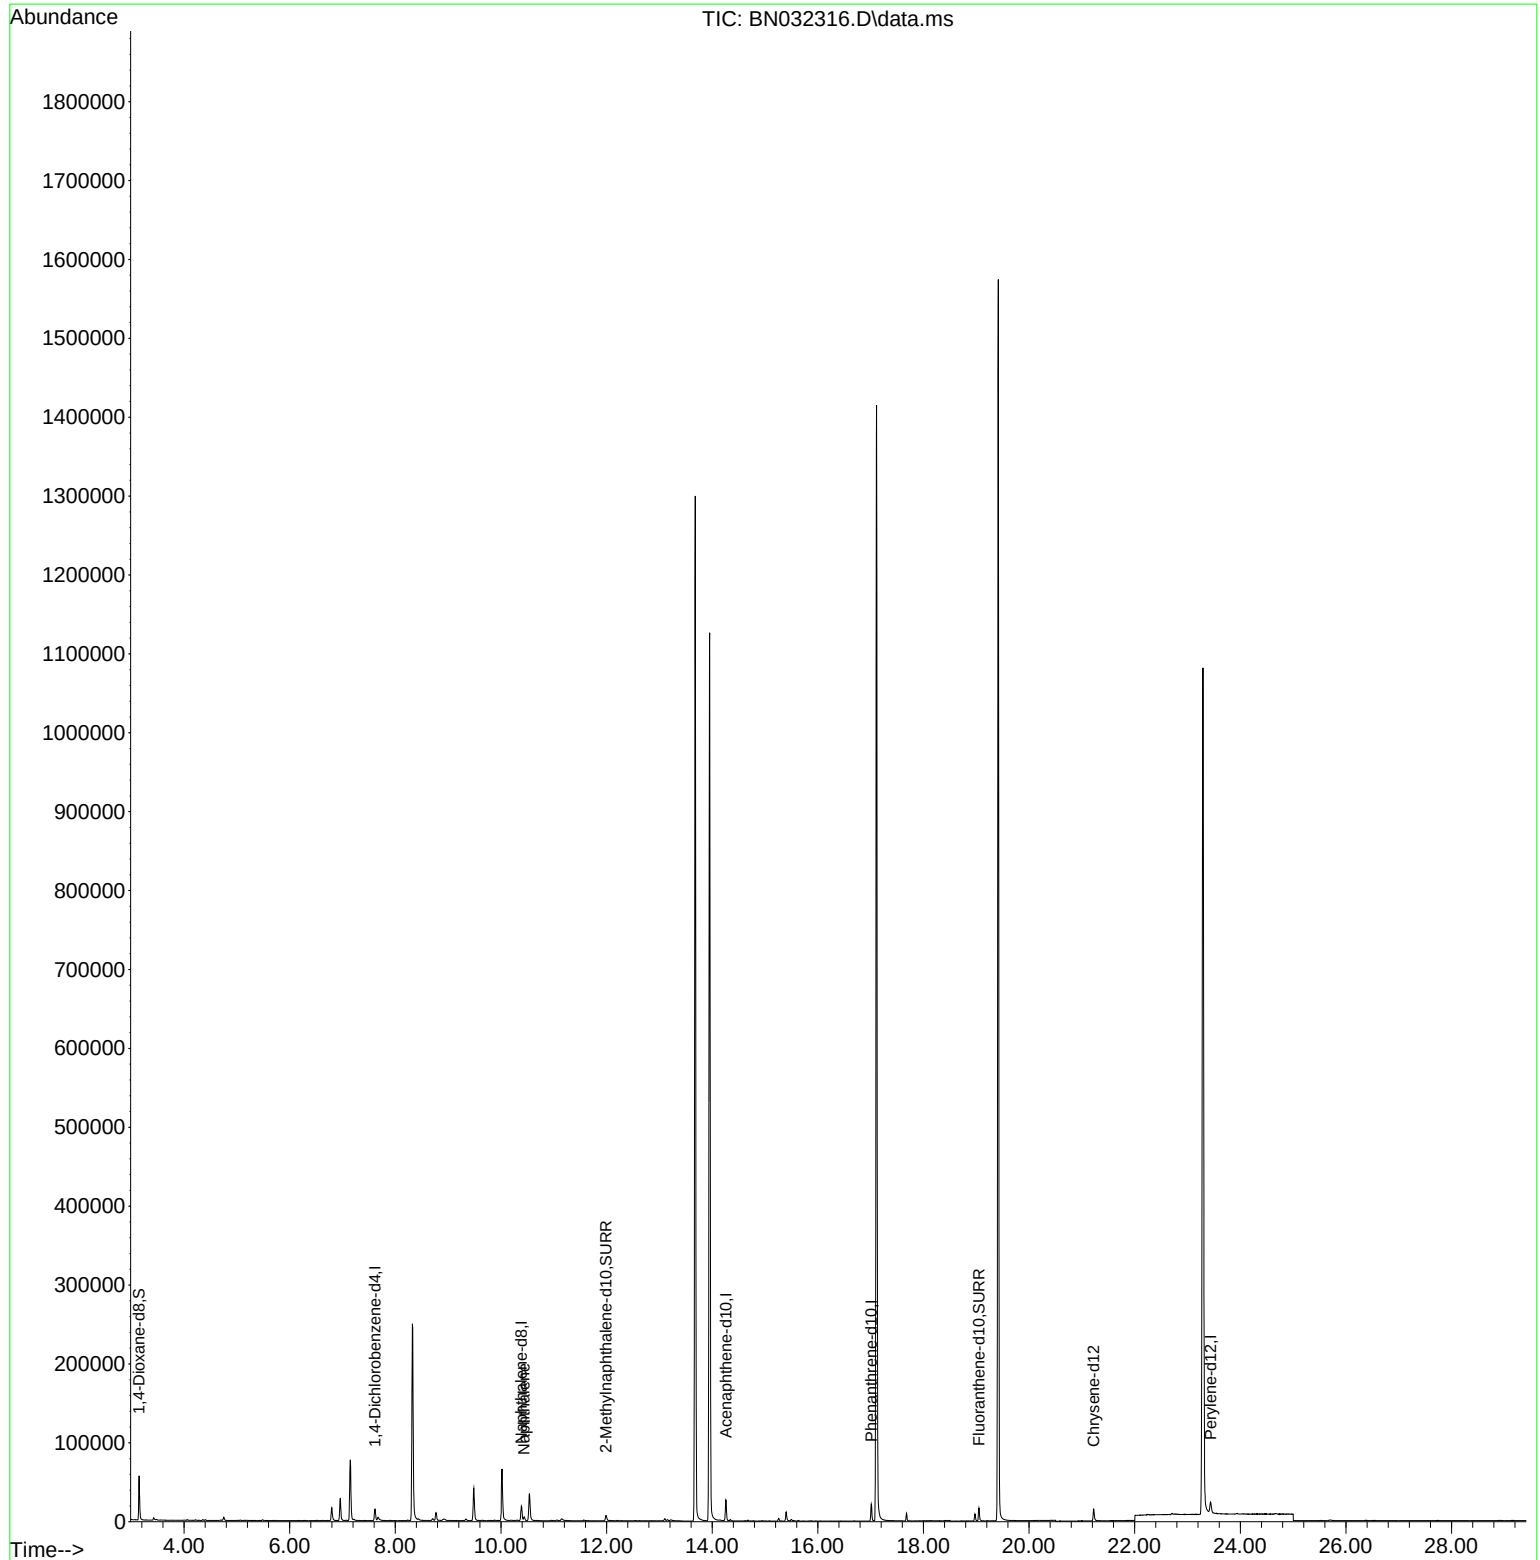

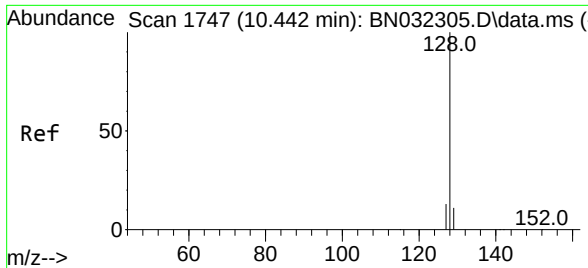

#5
Naphthalene
Concen: 0.082 ng/ul
RT: 10.437 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN032316.D
Acq: 28 Jun 2024 16:26

Instrument :
BNA_N
ClientSampleId :
E1GD7

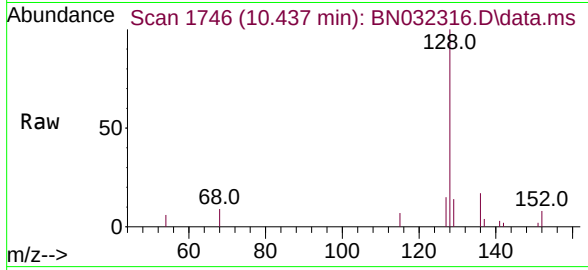

Tgt Ion:128 Resp: 5700

Ion	Ratio	Lower	Upper
128	100		
129	14.4	9.2	13.8
127	14.6	10.8	16.2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 07/04/2024

