

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
 Data File : BN032324.D
 Acq On : 28 Jun 2024 21:52
 Operator : MA/JU
 Sample : P2898-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GD9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/29/2024
 Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jun 28 23:06:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 27 13:23:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.612	152	8937	0.400	ng/ul	0.00
4) Naphthalene-d8	10.386	136	29097	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.256	164	17439	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.011	188	30261m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.219	240	18359m	0.400	ng/ul	0.00
23) Perylene-d12	23.429	264	17366m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.148	96	38017	3.827	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.986	152	13512	0.310	ng/ul	-0.01
18) Fluoranthene-d10	19.049	212	22451	0.406	ng/ul	-0.01
Target Compounds						Qvalue
5) Naphthalene	10.436	128	7155	0.093	ng/ul#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062824\
Data File : BN032324.D
Acq On : 28 Jun 2024 21:52
Operator : MA/JU
Sample : P2898-16
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GD9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 07/04/2024


Quant Time: Jun 28 23:06:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

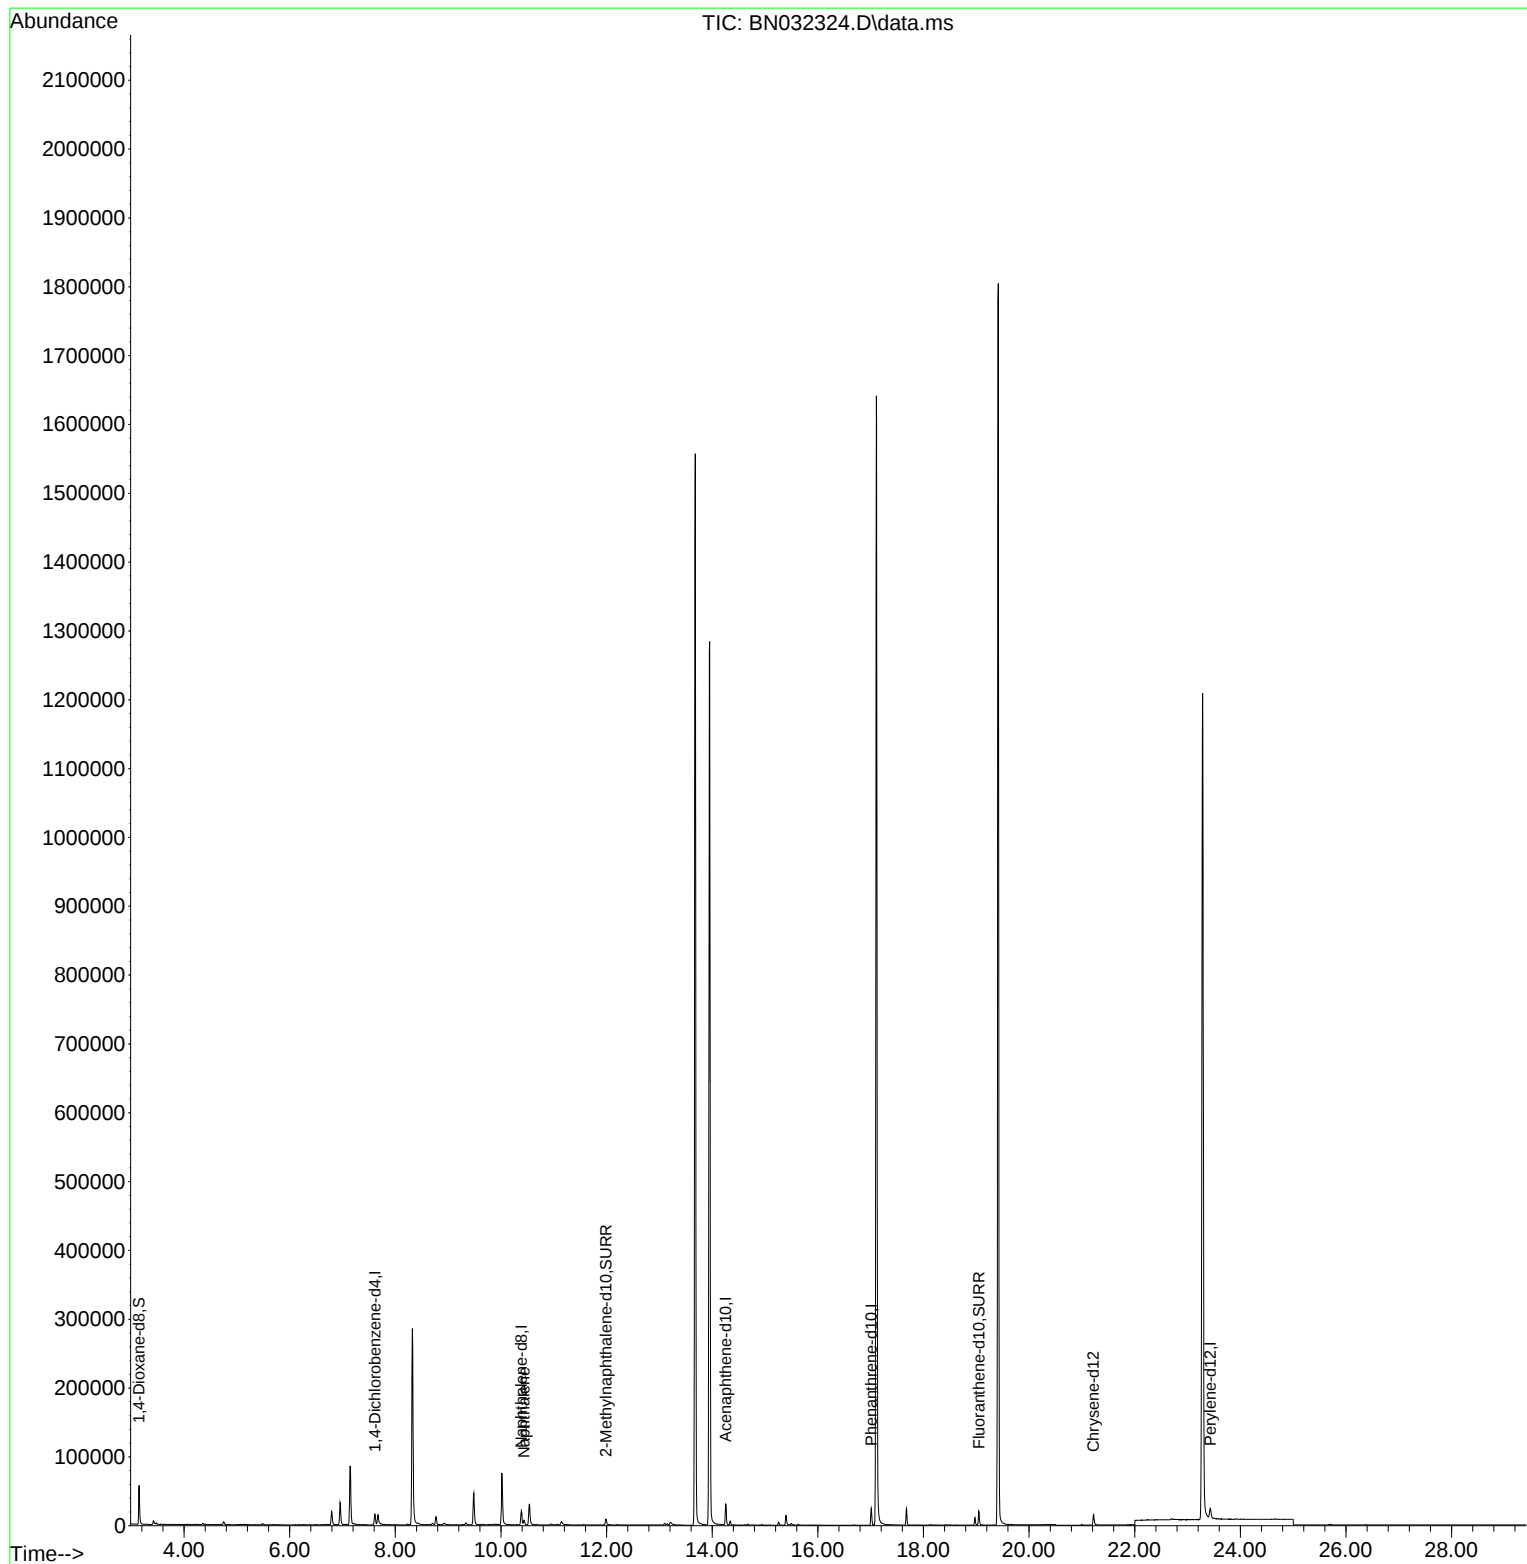

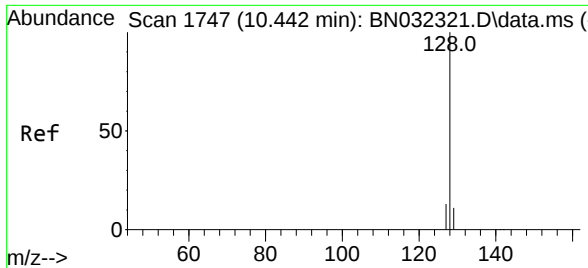

#5
Naphthalene
Concen: 0.093 ng/ul
RT: 10.436 min Scan# 11
Delta R.T. -0.012 min
Lab File: BN032324.D
Acq: 28 Jun 2024 21:52

Instrument :
BNA_N
ClientSampleId :
E1GD9

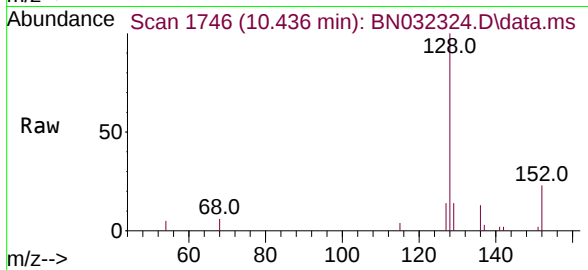

Tgt Ion:128 Resp: 715
Ion Ratio Lower Upper
128 100
129 13.9 9.2 13.8
127 14.5 10.8 16.2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/29/2024
Supervised By :mohammad ahmed 07/04/2024

