

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062920\
 Data File : BN011070.D
 Acq On : 29 Jun 2020 16:56
 Operator : CG/JU
 Sample : L3117-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 KY038PS037-200624

Quant Time: Jun 29 17:27:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN062320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 26 11:59:47 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	2252	0.40	ng	0.00
7) Naphthalene-d8	10.27	136	7523	0.40	ng	0.00
13) Acenaphthene-d10	14.13	164	4135	0.40	ng	-0.01
19) Phenanthrene-d10	16.90	188	8718	0.40	ng	0.00
29) Chrysene-d12	21.10	240	7881	0.40	ng	-0.01
36) Perylene-d12	23.25	264	7959	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.19	112	965	0.15	ng	0.00
5) Phenol-d6	6.73	99	564	0.08	ng	0.00
8) Nitrobenzene-d5	8.66	82	2566	0.37	ng	0.00
11) 2-Methylnaphthalene-d10	11.86	152	3834	0.29	ng	0.00
14) 2,4,6-Tribromophenol	15.64	330	624	0.34	ng	-0.01
15) 2-Fluorobiphenyl	12.76	172	7932	0.41	ng	0.00
27) Fluoranthene-d10	18.93	212	9339	0.34	ng	0.00
31) Terphenyl-d14	19.55	244	10659	0.50	ng	0.00
Target Compounds						Qvalue
34) Bis(2-ethylhexyl)phthalate	21.05	149	2546	0.232	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN062920\
Data File : BN011070.D
Acq On : 29 Jun 2020 16:56
Operator : CG/JU
Sample : L3117-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
KY038PS037-200624

Quant Time: Jun 29 17:27:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN062320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 26 11:59:47 2020
Response via : Initial Calibration

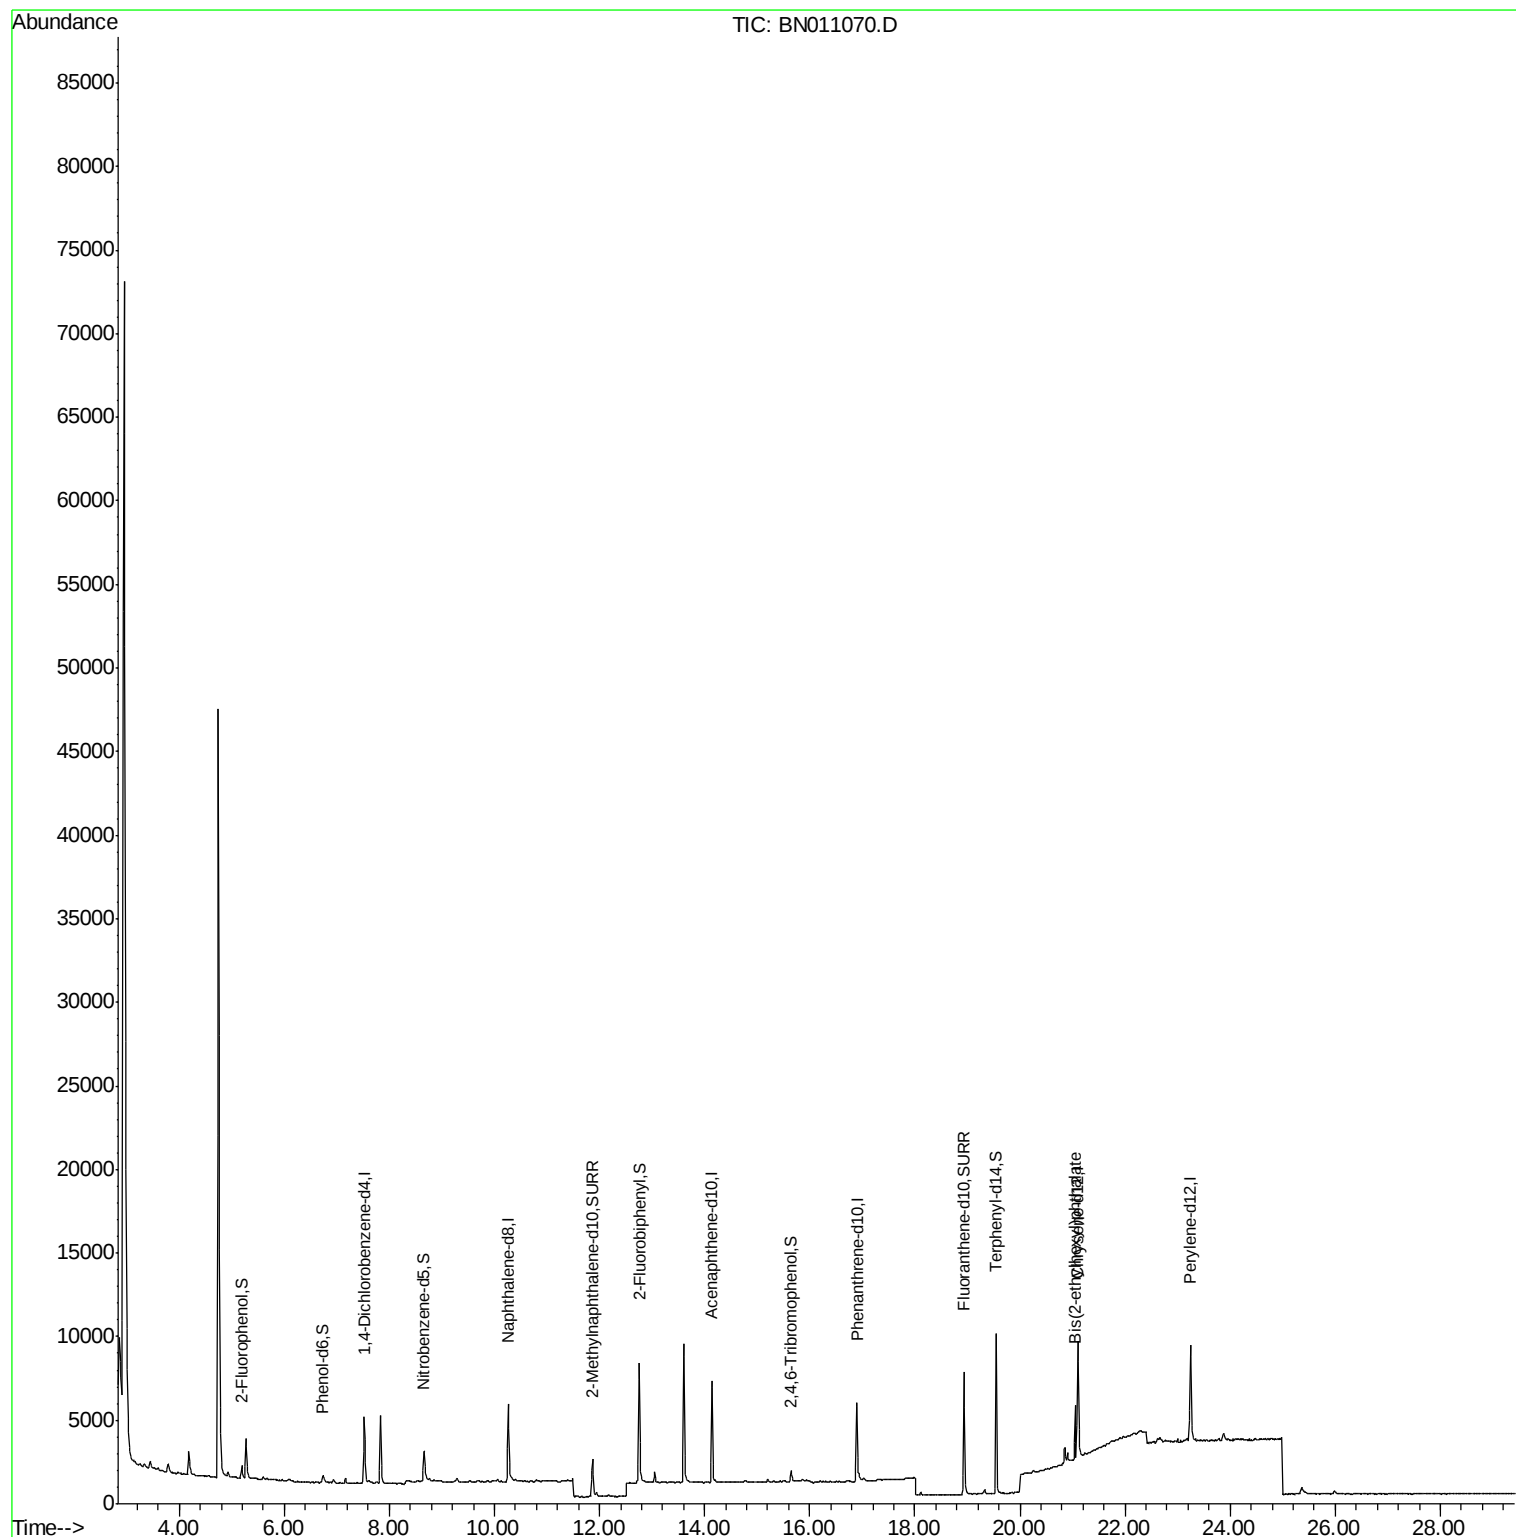

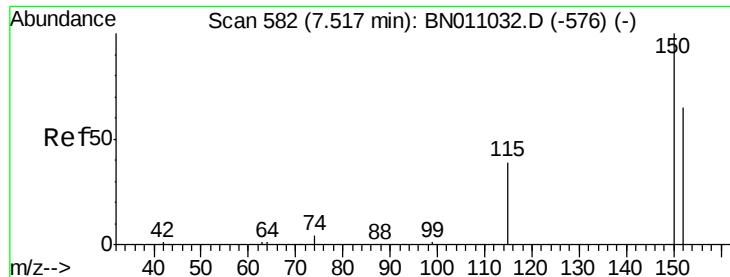


#1




1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.52 min Scan# 583
 Delta R.T. -0.00 min
 Lab File: BN011070.D
 Acq: 29 Jun 2020 16:56

Instrument :
 BNA_N
 ClientSampleId :
 KY038PS037-200624

Tot Ion:152 Resp: 2252
 Ion Ratio Lower Upper
 152 100
 150 150.6 121.8 182.8
 115 60.5 50.2 75.2

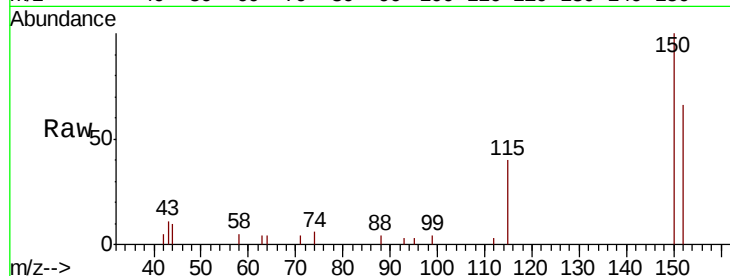


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

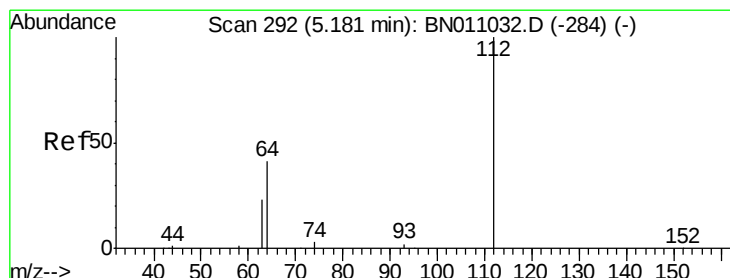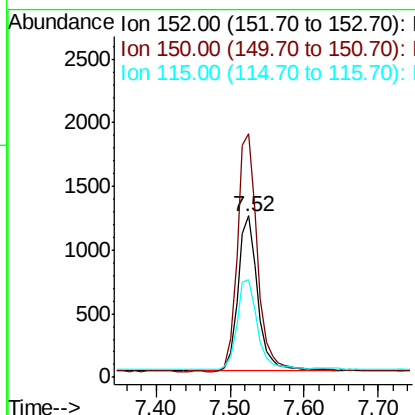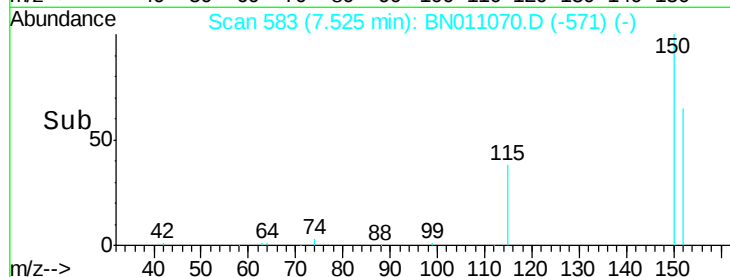



#4


2-Fluorophenol
 Concen: 0.152 ng
 RT: 5.19 min Scan# 293
 Delta R.T. -0.00 min
 Lab File: BN011070.D
 Acq: 29 Jun 2020 16:56

Tgt Ion:112 Resp: 965
 Ion Ratio Lower Upper
 112 100
 64 46.5 37.3 55.9
 63 24.6 20.4 30.6

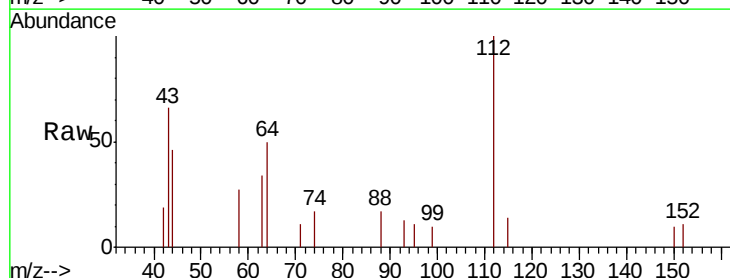

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BNC
 Ion 63.00 (62.70 to 63.70): BNC

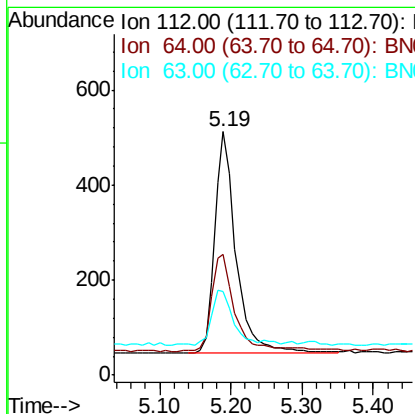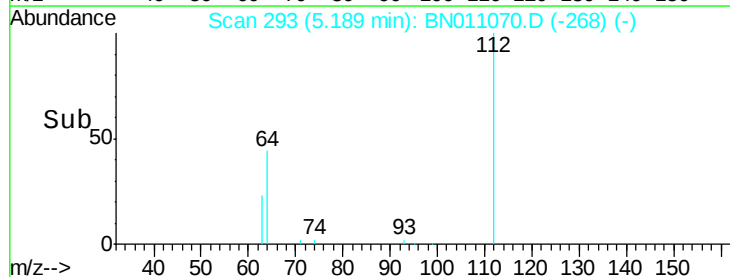

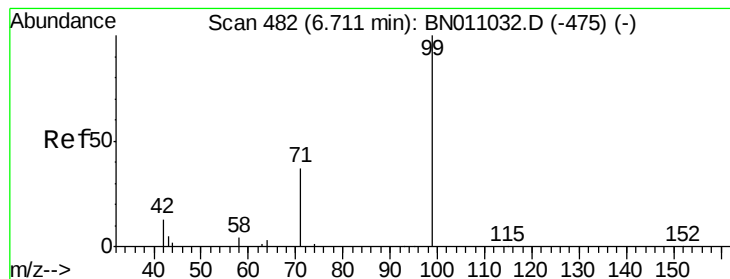

#5

Phenol-d6

Concen: 0.075 ng

RT: 6.73 min Scan# 484

Delta R.T. -0.00 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56

Instrument :

BNA_N

ClientSampleId :

KY038PS037-200624


Tot Ion: 99 Resp: 564

Ion Ratio Lower Upper

99 100

42 13.3 10.6 16.0

71 43.3 28.7 43.1#

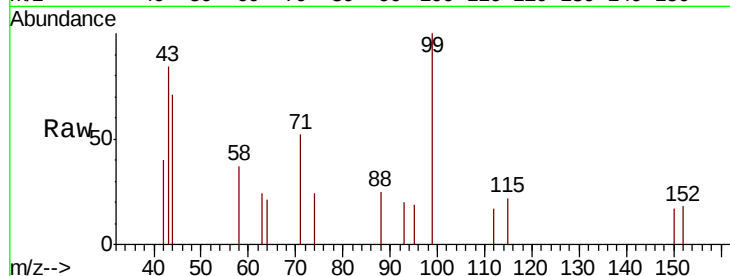

Abundance Ion 99.00 (98.70 to 99.70): BN011032.D (-475) (-)

Ion 42.00 (41.70 to 42.70): BN011032.D (-475) (-)

Ion 71.00 (70.70 to 71.70): BN011032.D (-475) (-)

6.73

300



200

100

0

6.60 6.70 6.80 6.90

Time-->

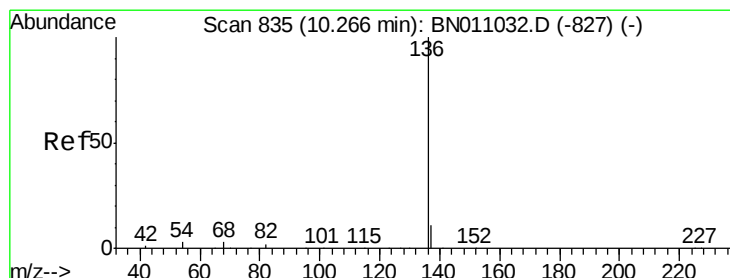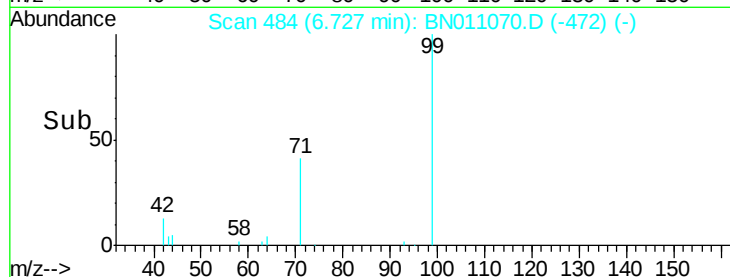

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.27 min Scan# 835

Delta R.T. -0.00 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56

Tgt Ion: 136 Resp: 7523


Ion Ratio Lower Upper

136 100

137 12.0 9.6 14.4

54 5.3 3.0 4.4#

68 5.8 3.4 5.2#

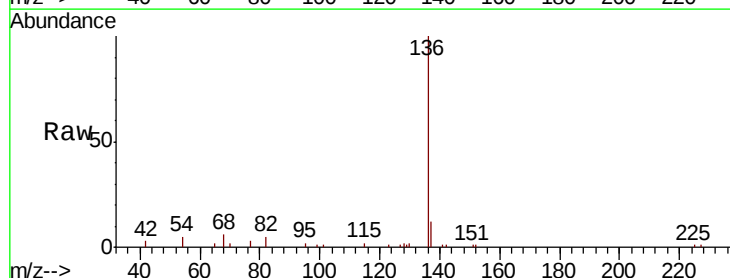

Abundance Ion 136.00 (135.70 to 136.70): BN011032.D (-827) (-)

Ion 137.00 (136.70 to 137.70): BN011032.D (-827) (-)

Ion 54.00 (53.70 to 54.70): BN011032.D (-827) (-)

Ion 68.00 (67.70 to 68.70): BN011032.D (-827) (-)

10.27

5000

4000

3000


2000


1000

0

10.20 10.40

Time-->

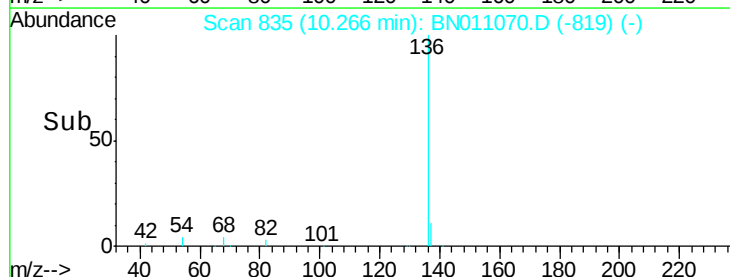

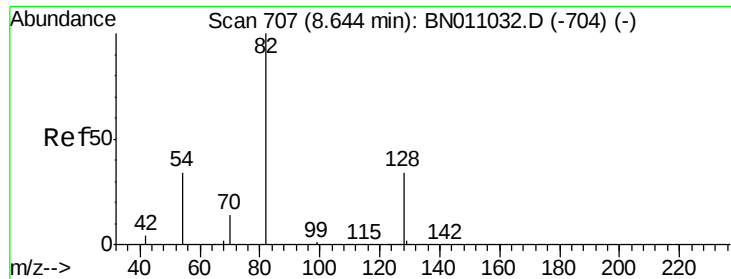

#8

Nitrobenzene-d5

Concen: 0.374 ng

RT: 8.66 min Scan# 708

Delta R.T. -0.00 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56

Instrument :

BNA_N

ClientSampleId :

KY038PS037-200624


Tot Ion: 82 Resp: 2566

Ion Ratio Lower Upper

82 100

128 39.4 29.4 44.2




54 37.2 28.8 43.2

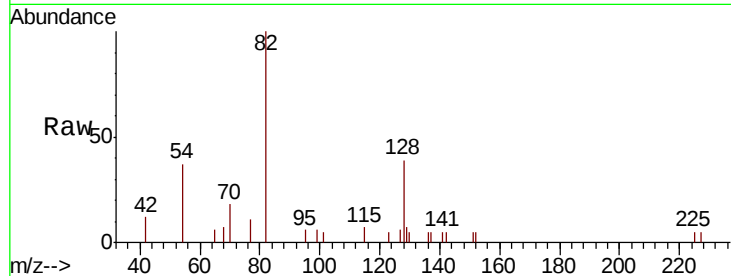

Abundance Ion 82.00 (81.70 to 82.70): BN011032.D (-704) (-)

Ion 128.00 (127.70 to 128.70): BN011032.D (-704) (-)

Ion 54.00 (53.70 to 54.70): BN011032.D (-704) (-)

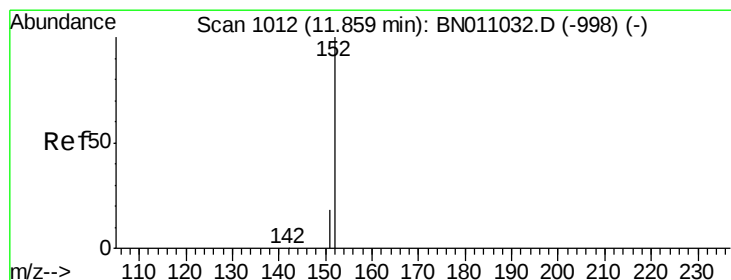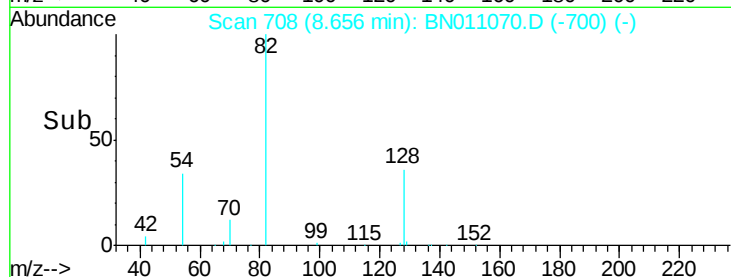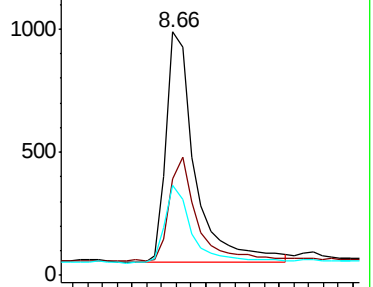

#11

2-Methylnaphthalene-d10

Concen: 0.289 ng

RT: 11.86 min Scan# 1013

Delta R.T. -0.00 min

Lab File: BN011070.D


Acq: 29 Jun 2020 16:56

Tgt Ion: 152 Resp: 3834

Ion Ratio Lower Upper



152 100


151 19.2 16.2 24.4

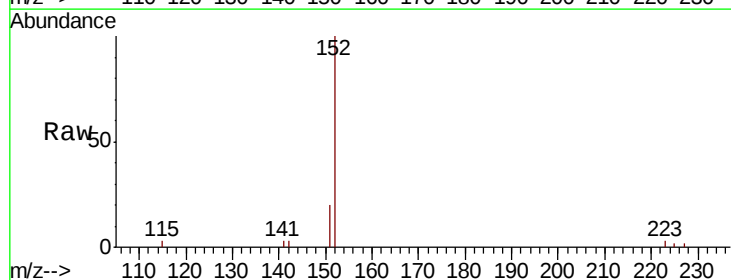

Abundance Ion 152.00 (151.70 to 152.70): BN011032.D (-998) (-)

Ion 151.00 (150.70 to 151.70): BN011032.D (-998) (-)

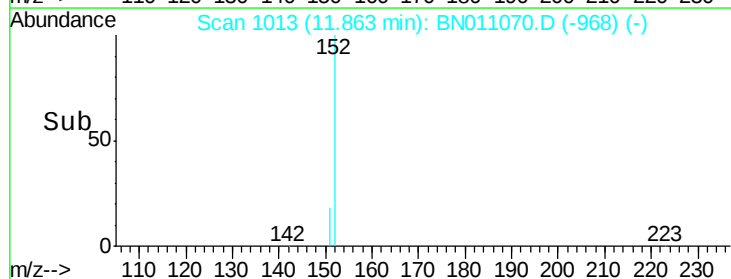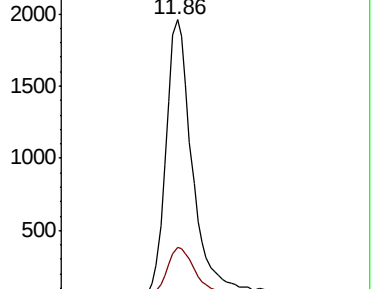

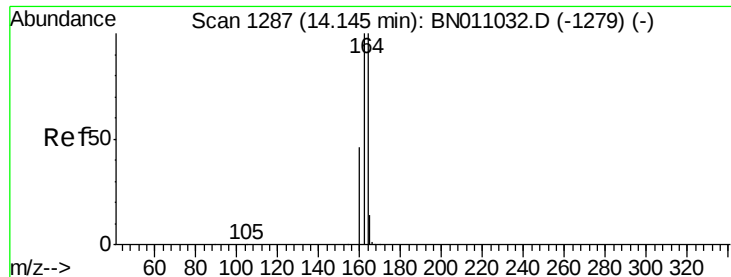

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.13 min Scan# 1286

Delta R.T. -0.01 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56

Instrument :

BNA_N

ClientSampleId :

KY038PS037-200624





Tot Ion:164 Resp: 4135

Ion Ratio Lower Upper

164 100

162 105.2 80.2 120.4

160 51.2 37.7 56.5

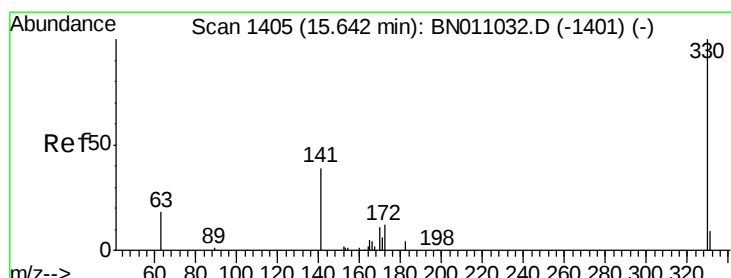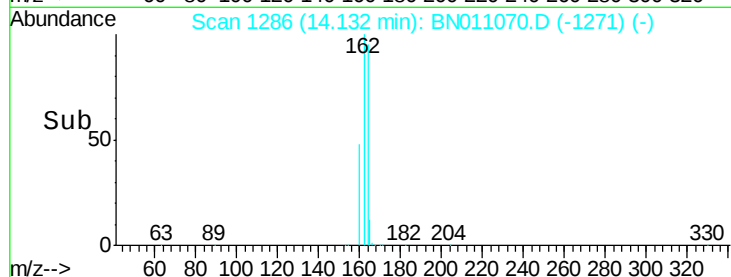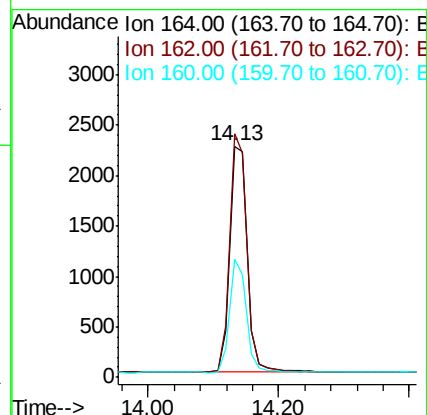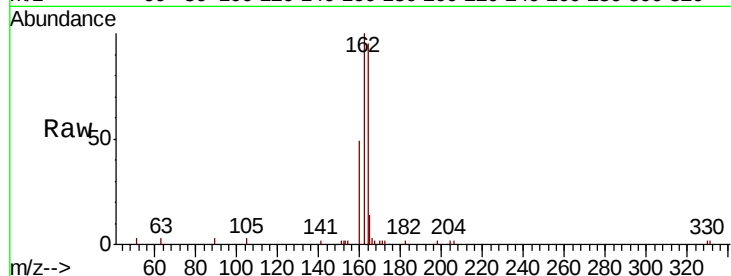

#14

2,4,6-Tribromophenol

Concen: 0.343 ng

RT: 15.64 min Scan# 1405

Delta R.T. -0.01 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56




Tgt Ion:330 Resp: 624


Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0

141 41.7 34.5 51.7


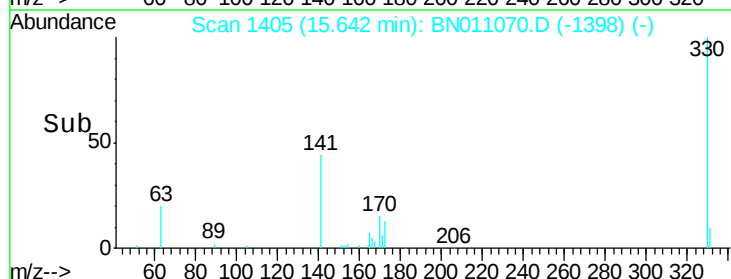
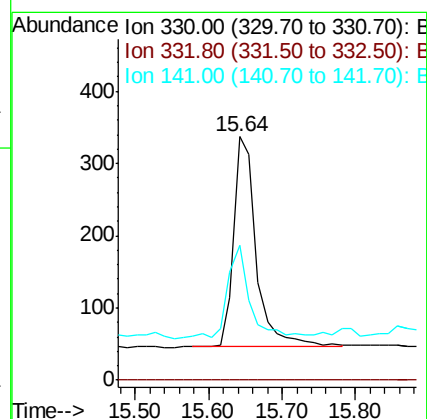
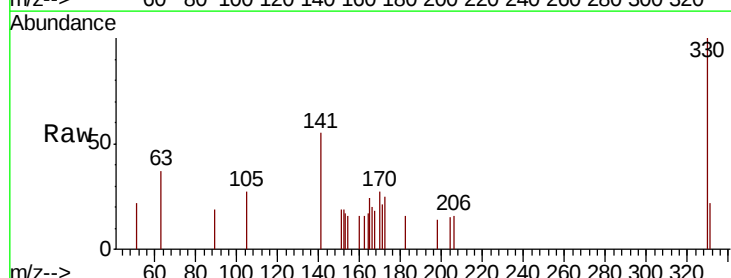


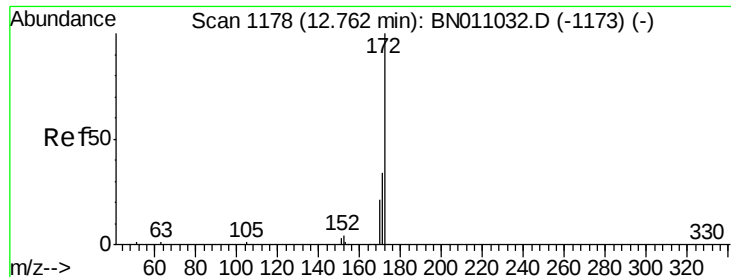

#15
2-Fluorobiphenyl
Concen: 0.411 ng
RT: 12.76 min Scan# 1178
Delta R.T. -0.00 min
Lab File: BN011070.D
Acq: 29 Jun 2020 16:56




Instrument :
BNA_N
ClientSampleId :
KY038PS037-200624


Tot Ion:172 Resp: 7932
Ion Ratio Lower Upper
172 100
171 35.4 27.4 41.2
170 23.4 17.5 26.3

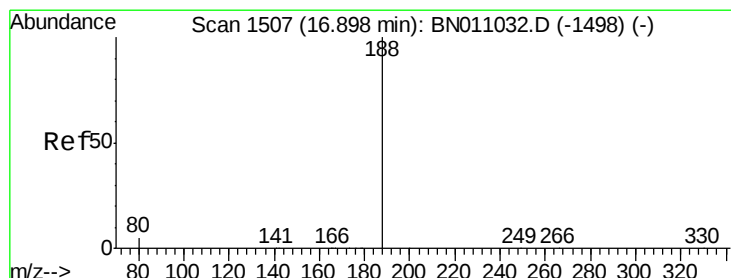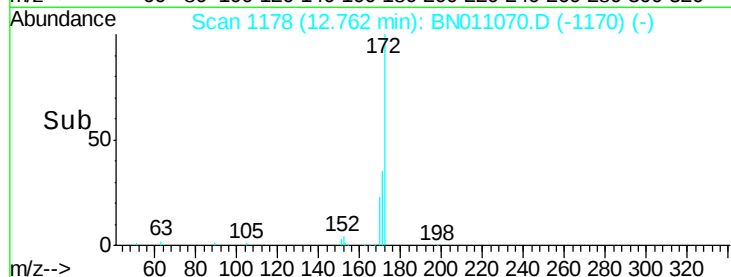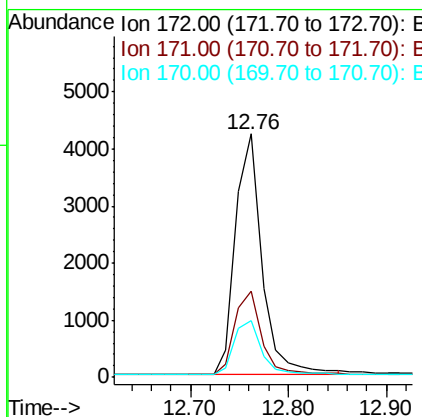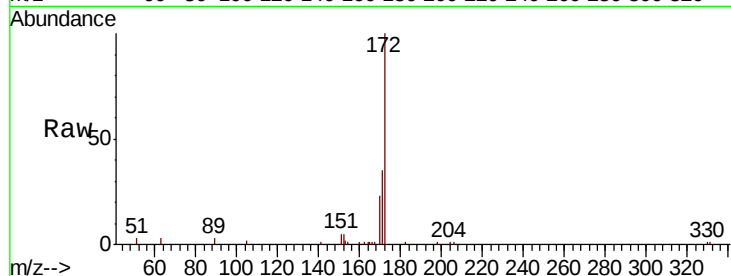

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.90 min Scan# 1507
Delta R.T. -0.00 min
Lab File: BN011070.D
Acq: 29 Jun 2020 16:56

Tgt Ion:188 Resp: 8718
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.5 4.6 7.0

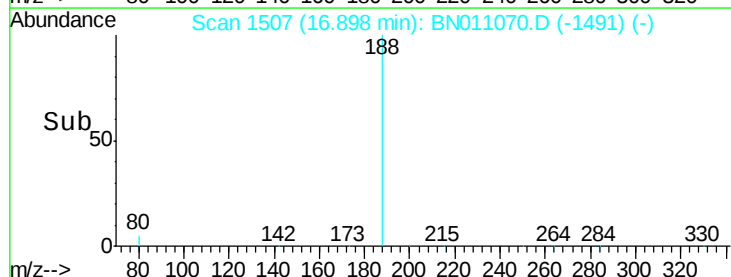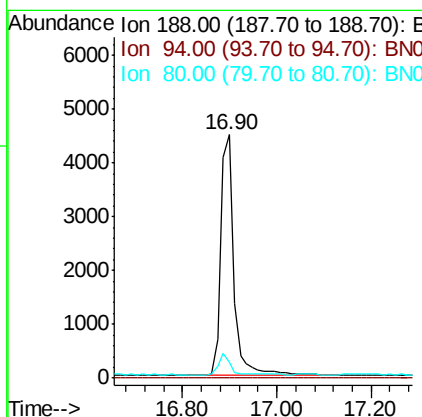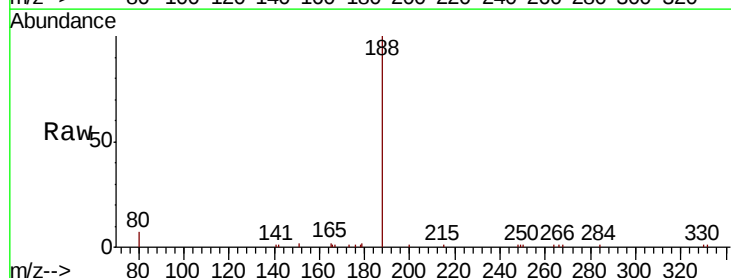

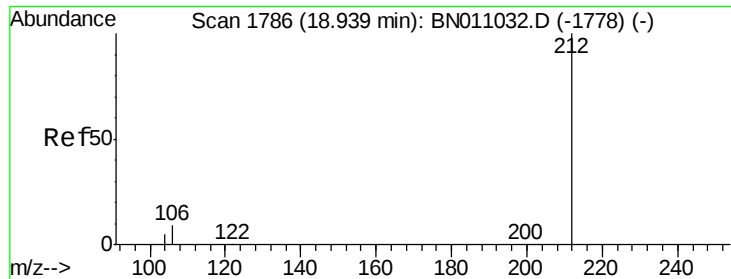

#27

Fluoranthene-d10

Concen: 0.339 ng

RT: 18.93 min Scan# 1783

Delta R.T. -0.01 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56

Instrument :

BNA_N

ClientSampleId :

KY038PS037-200624


Tot Ion:212 Resp: 9339

Ion Ratio Lower Upper

212 100

106 9.2 7.7 11.5




104 5.3 4.6 6.8

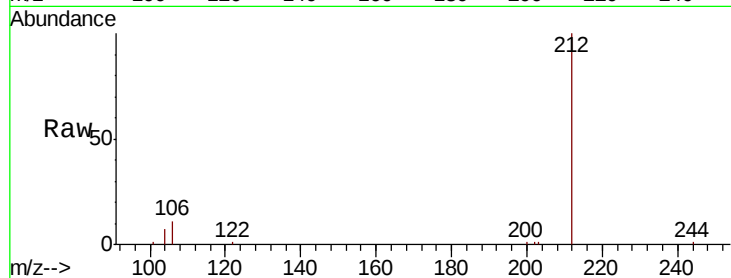

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

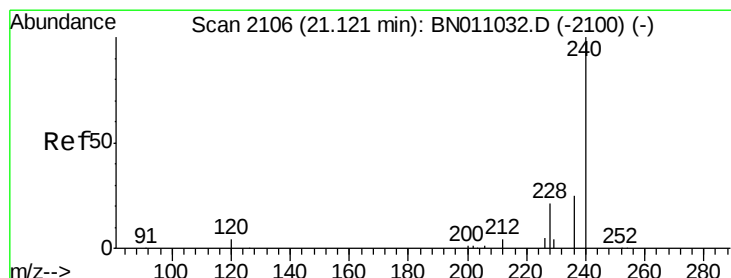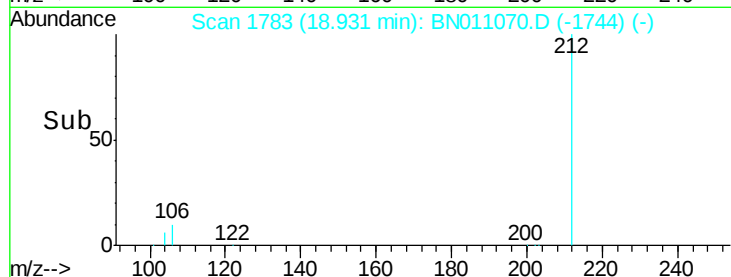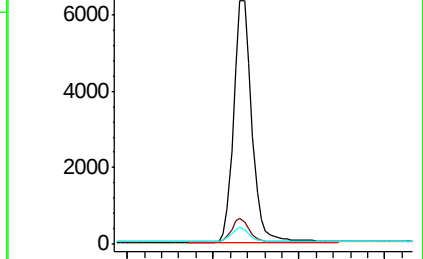

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.10 min Scan# 2103

Delta R.T. -0.01 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56


Tgt Ion:240 Resp: 7881

Ion Ratio Lower Upper

240 100

120 12.8 5.4 8.0#



236 29.3 21.4 32.2

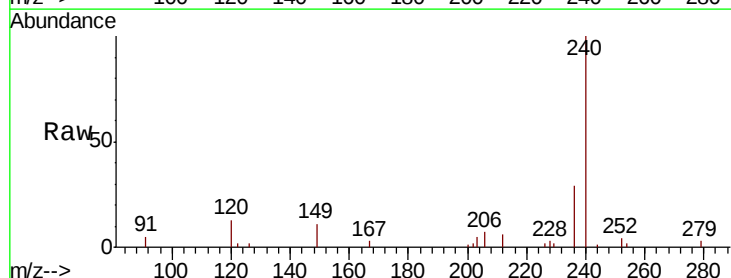


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

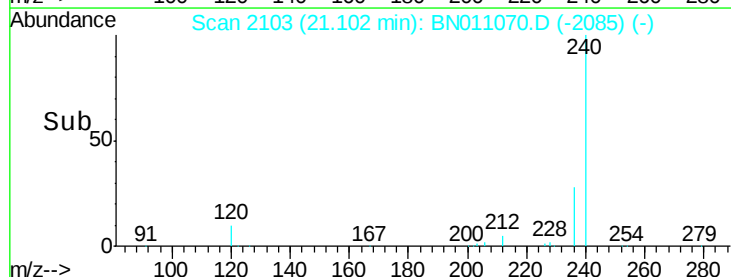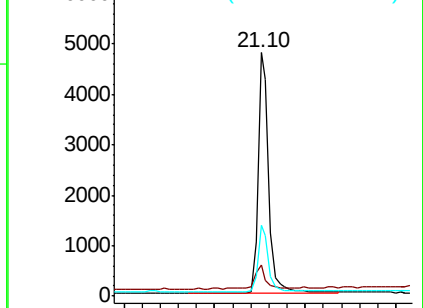

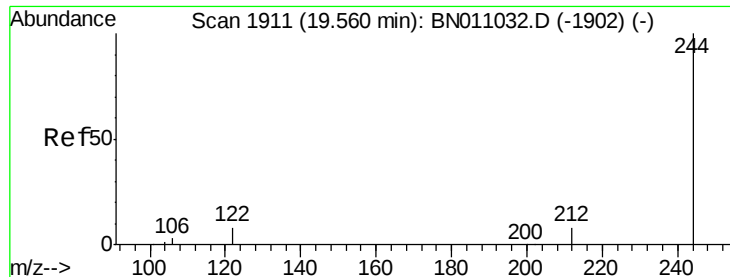

#31

Terphenyl-d14

Concen: 0.504 ng

RT: 19.55 min Scan# 1908

Delta R.T. -0.01 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56

Instrument :

BNA_N

ClientSampleId :

KY038PS037-200624


Tot Ion:244 Resp: 10659

Ion Ratio Lower Upper

244 100

212 8.4 6.9 10.3

122 8.7 7.4 11.0



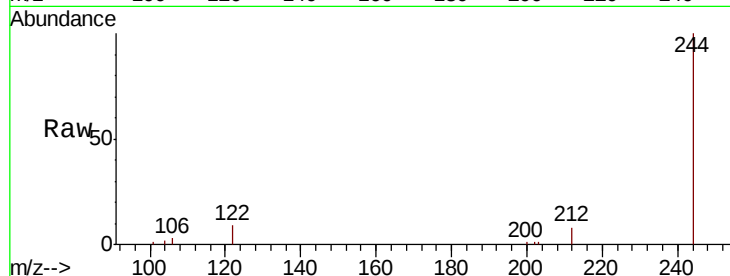


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

Time-->

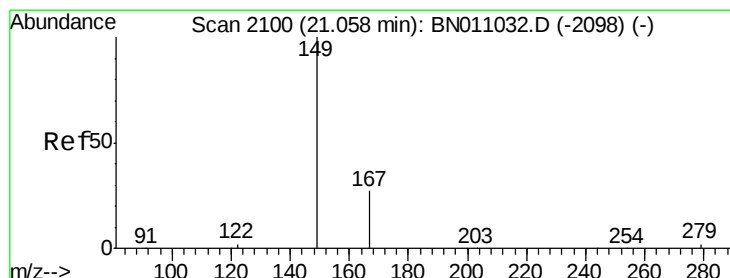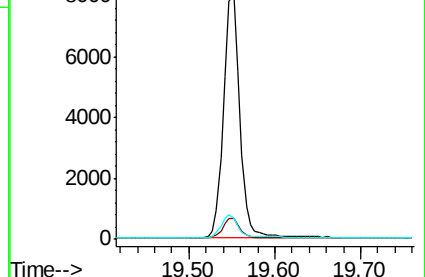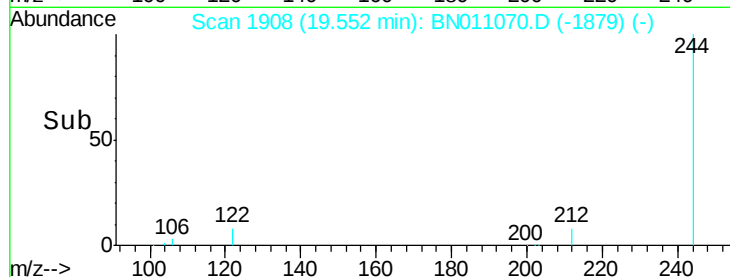

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.232 ng

RT: 21.05 min Scan# 2098

Delta R.T. -0.01 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56


Tgt Ion:149 Resp: 2546

Ion Ratio Lower Upper

149 100

167 29.1 22.2 33.2

279 5.1 3.9 5.9


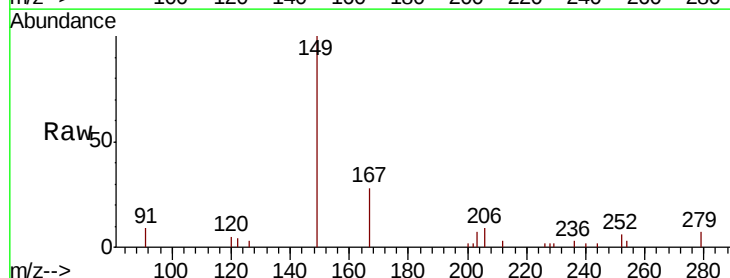





Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

Time-->

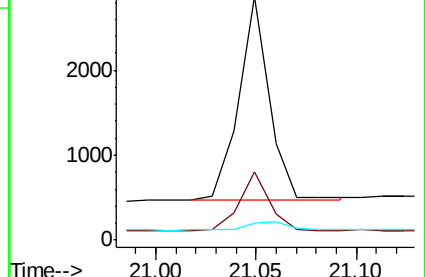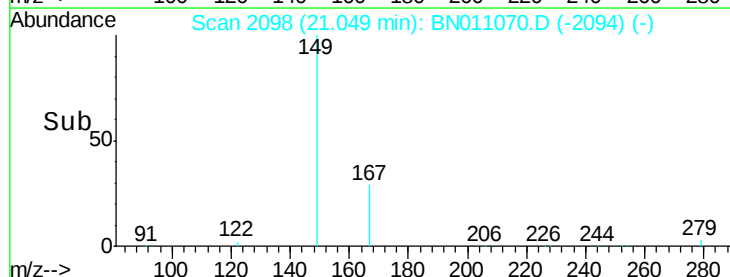

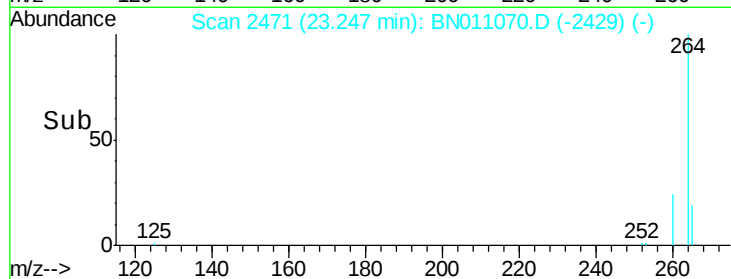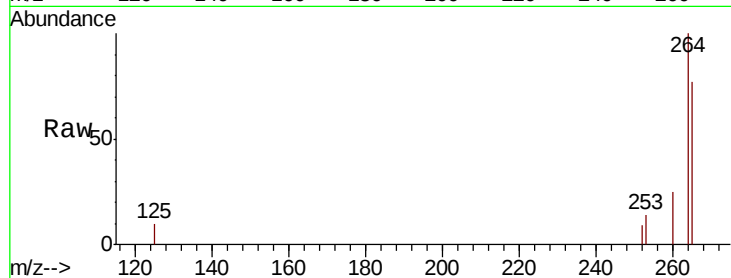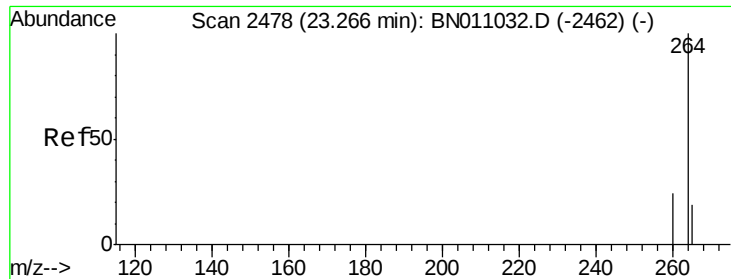

#36

Pervlene-d12

Concen: 0.400 ng

RT: 23.25 min Scan# 2471

Delta R.T. -0.01 min

Lab File: BN011070.D

Acq: 29 Jun 2020 16:56

Instrument :

BNA_N

ClientSampleId :

KY038PS037-200624

Tot Ion: 264 Resp: 7959

Ion Ratio Lower Upper

264 100

260 24.8 20.0 30.0

265 77.1 64.9 97.3

