


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062920\
 Data File : BN011064.D
 Acq On : 29 Jun 2020 08:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 26 11:59:47 2020

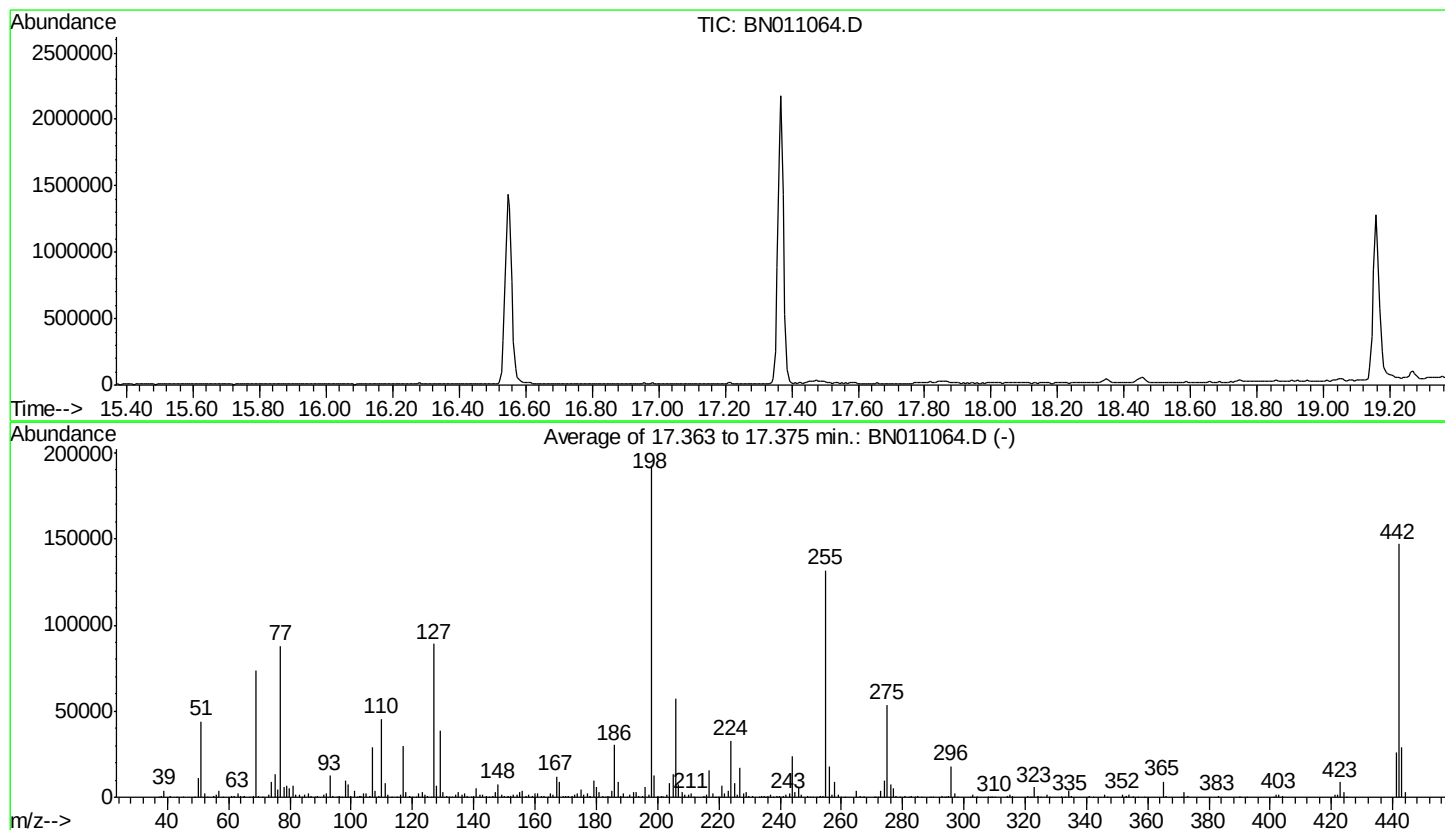

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	44066	PASS
68	69	0.00	2	1.5	1104	PASS
69	198	0.00	100	38.1	73284	PASS
70	69	0.00	2	0.7	532	PASS
127	198	10	80	46.3	89128	PASS
197	198	0.00	2	0.7	1272	PASS
198	198	100	100	100.0	192576	PASS
199	198	5	9	6.7	12930	PASS
275	198	10	60	27.9	53725	PASS
365	198	1	100	4.8	9258	PASS
441	198	0.01	100	13.5	26056	PASS
442	198	50	100	76.3	146914	PASS
443	442	15	24	19.8	29061	PASS