

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062923\
 Data File : BN026055.D
 Acq On : 28 Jun 2023 13:09
 Operator : MA/JU
 Sample : PB153626BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK626

Quant Time: Jun 28 23:14:27 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 22:47:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.972	152	6122	0.400	ng/ul	0.00
4) Naphthalene-d8	10.781	136	20180	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.607	164	12552	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.355	188	25301	0.400	ng/ul	0.00
17) Chrysene-d12	21.549	240	12703	0.400	ng/ul	0.00
23) Perylene-d12	23.999	264	15647	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	30275	4.391	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.376	152	7166	0.231	ng/ul	0.00
18) Fluoranthene-d10	19.382	212	14415	0.298	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.745	202	2549	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.841	252	4129	0.071	ng/ul#	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062923\
Data File : BN026055.D
Acq On : 28 Jun 2023 13:09
Operator : MA/JU
Sample : PB153626BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK626

Quant Time: Jun 28 23:14:27 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 22:47:20 2023
Response via : Initial Calibration




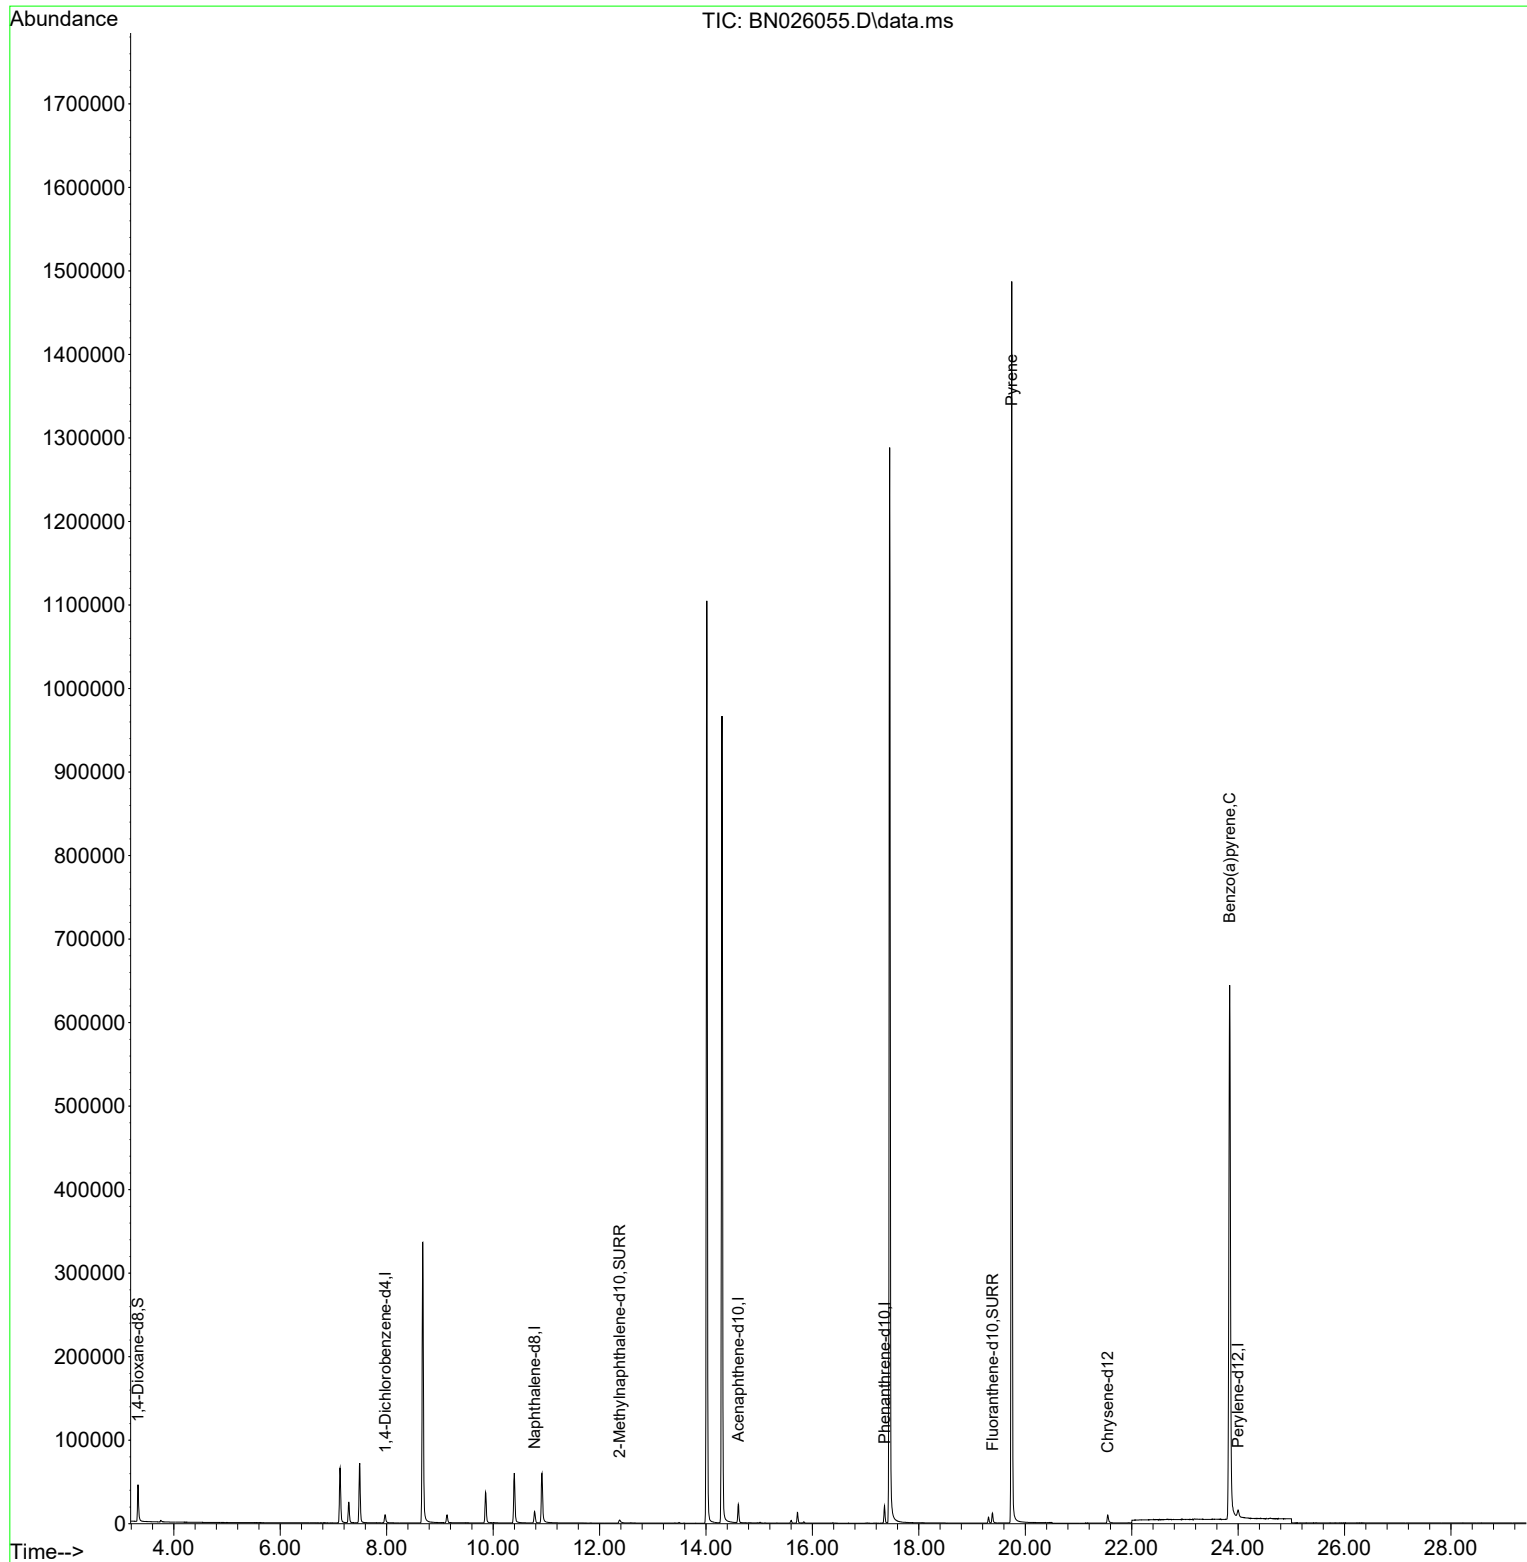


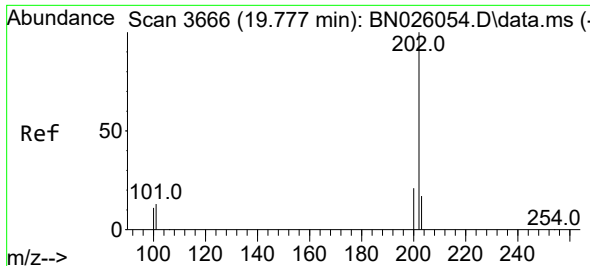

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.745 min Scan# 3659
Delta R.T. -0.032 min
Lab File: BN026055.D
Acq: 28 Jun 2023 13:09

Instrument :
BNA_N
ClientSampleId :
SBLK626

Tgt Ion:202 Resp: 2549
Ion Ratio Lower Upper
202 100
101 187.9 11.4 17.0#
100 1448.2 9.1 13.7#

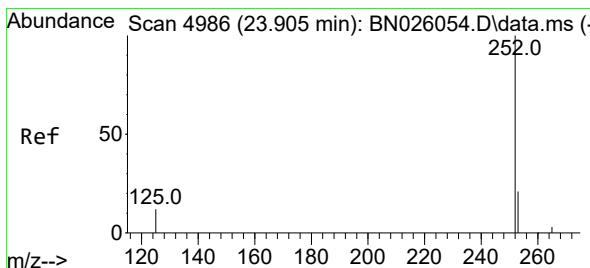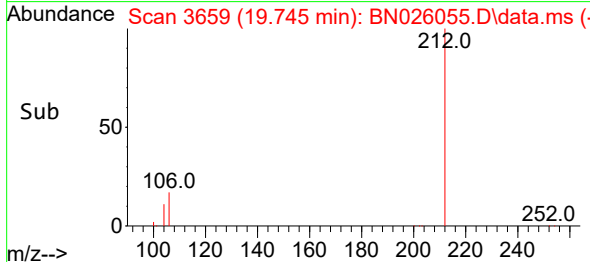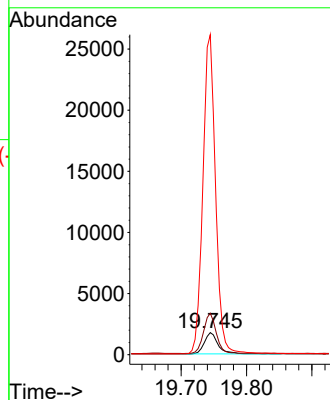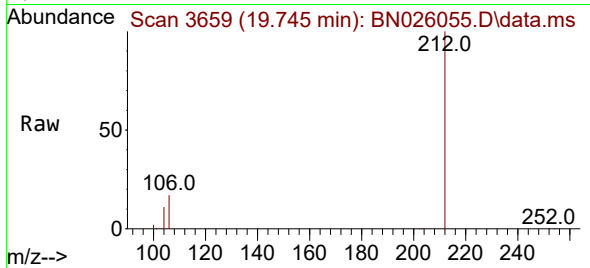

#26
Benzo(a)pyrene
Concen: 0.071 ng/ul
RT: 23.841 min Scan# 4964
Delta R.T. -0.064 min
Lab File: BN026055.D
Acq: 28 Jun 2023 13:09

Tgt Ion:252 Resp: 4129
Ion Ratio Lower Upper
252 100
253 62.0 26.0 39.0#
125 56.8 17.3 25.9#

