

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062923\
 Data File : BN026089.D
 Acq On : 29 Jun 2023 11:26
 Operator : MA/JU
 Sample : 03142-16DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCFT3DL

Quant Time: Jun 30 00:43:05 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 22:47:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	7401	0.400	ng/ul	0.00
4) Naphthalene-d8	10.776	136	25315	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.608	164	15278	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.352	188	31296	0.400	ng/ul	0.00
17) Chrysene-d12	21.547	240	17853	0.400	ng/ul	# 0.00
23) Perylene-d12	23.997	264	17248	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.326	96	6242	0.749	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.376	152	1949	0.050	ng/ul	0.00
18) Fluoranthene-d10	19.378	212	3990	0.059	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.394	178	18865	0.182	ng/ul	99
19) Fluoranthene	19.411	202	48781	0.512	ng/ul	99
20) Pyrene	19.773	202	43208	0.436	ng/ul	99
21) Benzo(a)anthracene	21.530	228	14296	0.194	ng/ul#	90
22) Chrysene	21.582	228	20730	0.271	ng/ul#	95
24) Benzo(b)fluoranthene	23.254	252	38955	0.529	ng/ul	89
26) Benzo(a)pyrene	23.889	252	17227	0.269	ng/ul#	91
27) Indeno(1,2,3-cd)pyrene	26.552	276	14655	0.210	ng/ul#	85
28) Dibenzo(a,h)anthracene	26.568	278	3291	0.062	ng/ul#	33
29) Benzo(g,h,i)perylene	27.350	276	15216	0.245	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062923\
Data File : BN026089.D
Acq On : 29 Jun 2023 11:26
Operator : MA/JU
Sample : 03142-16DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCFT3DL

Quant Time: Jun 30 00:43:05 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 22:47:20 2023
Response via : Initial Calibration




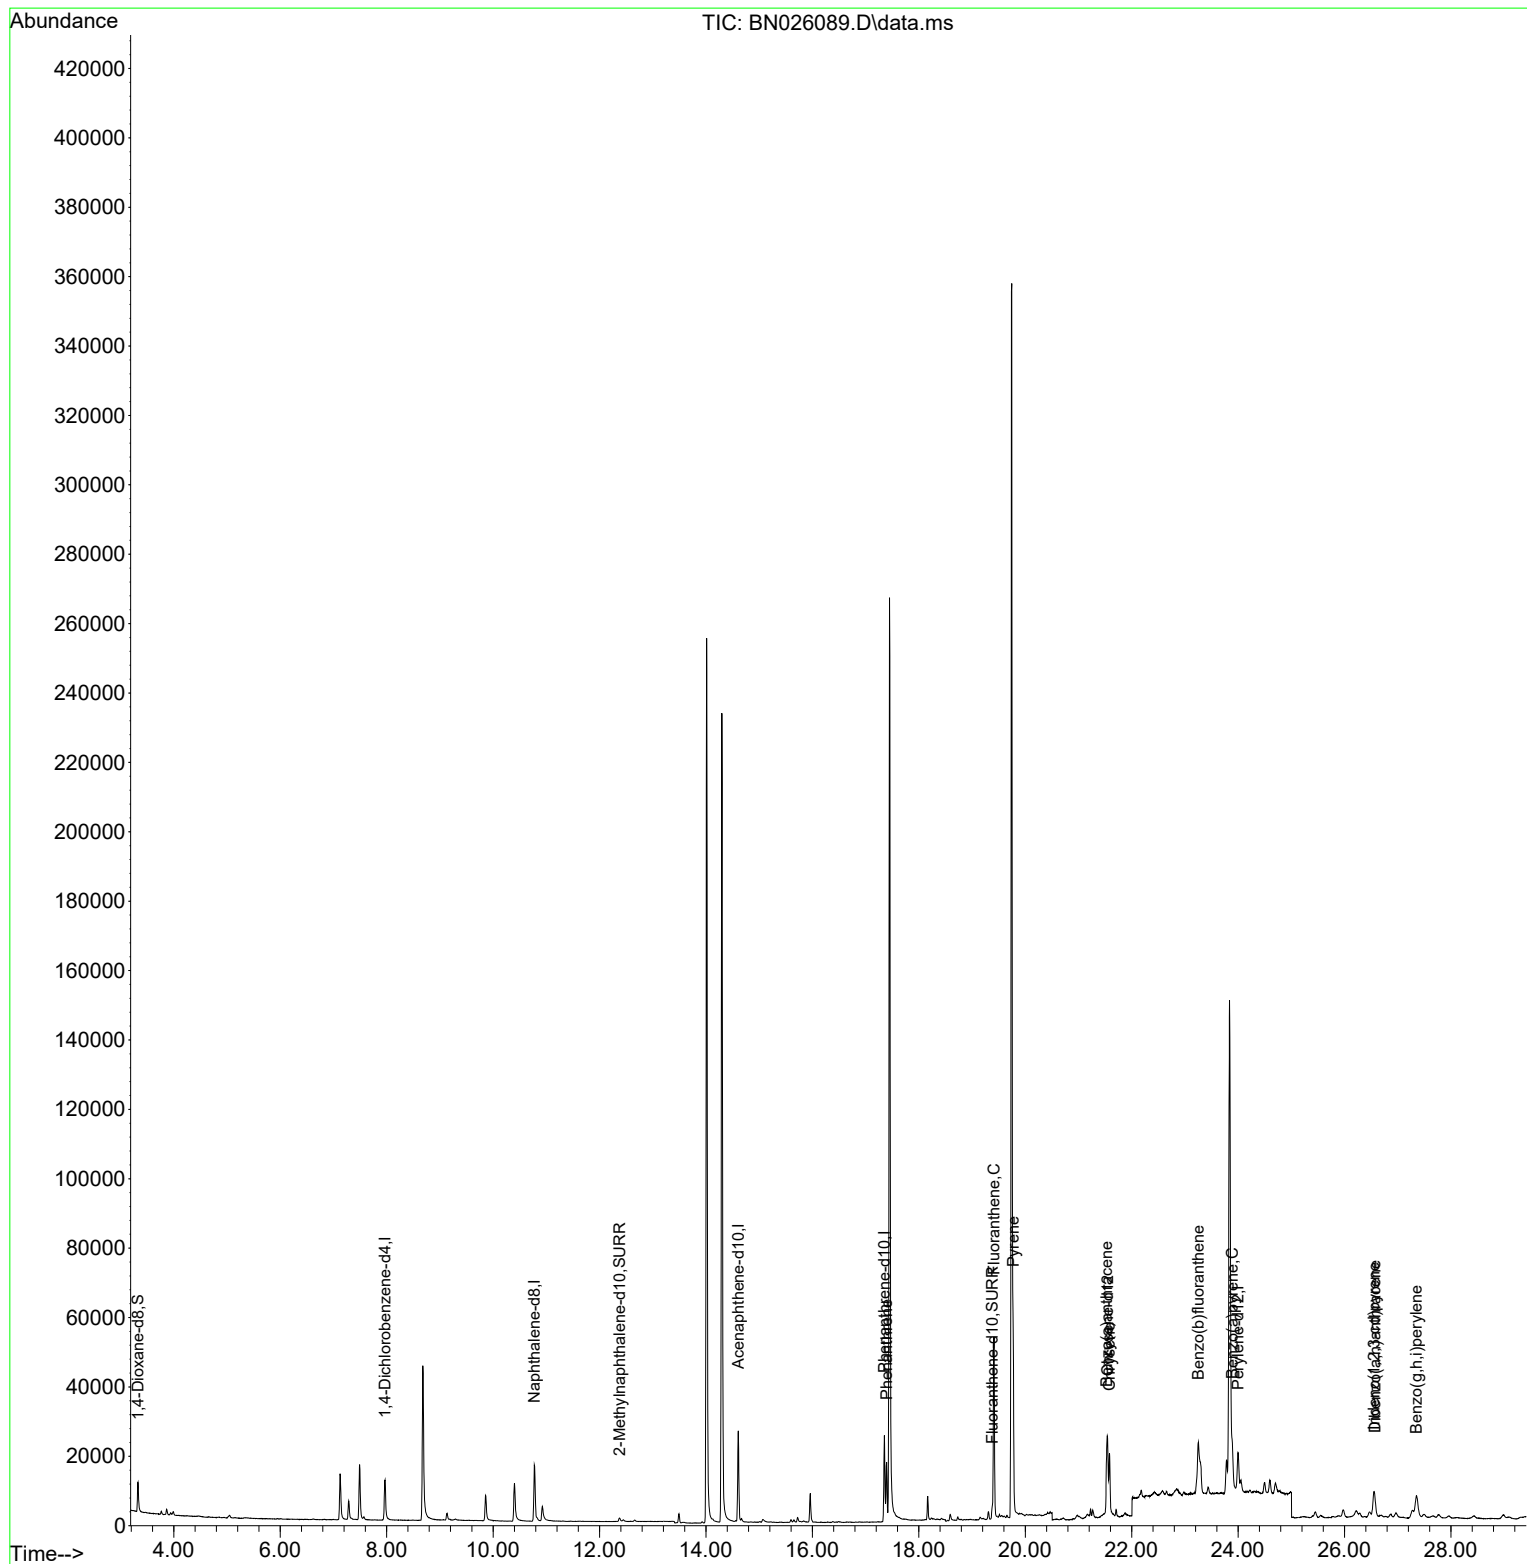


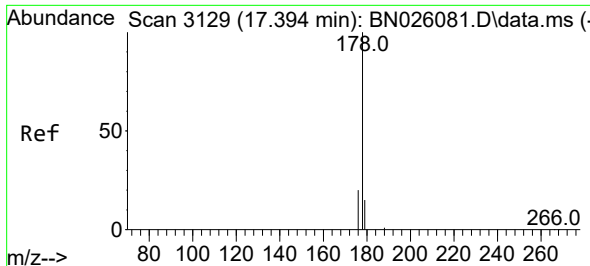

#15
Phenanthrene
Concen: 0.182 ng/ul
RT: 17.394 min Scan# 3129
Delta R.T. -0.008 min
Lab File: BN026089.D
Acq: 29 Jun 2023 11:26




Instrument :
BNA_N
ClientSampleId :
DCFT3DL


Tgt Ion:	178	Resp:	18865
Ion Ratio	Lower	Upper	
178	100		
179	16.6	12.6	19.0
176	20.1	15.8	23.6

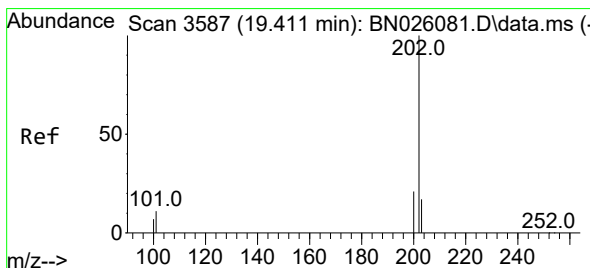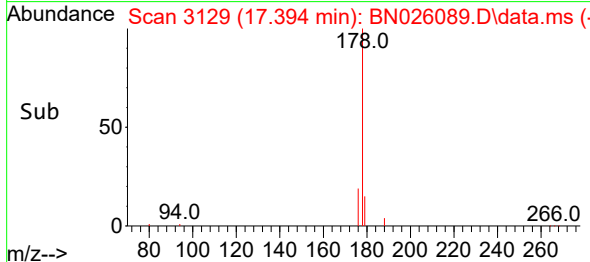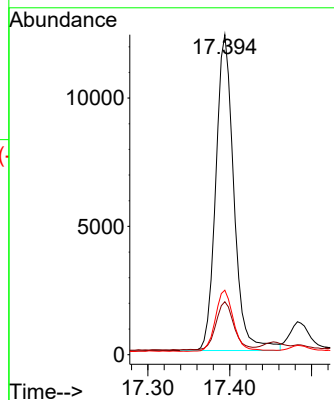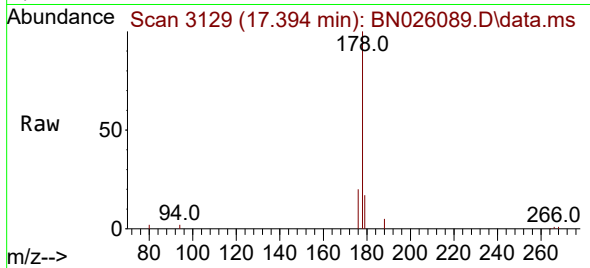

#19
Fluoranthene
Concen: 0.512 ng/ul
RT: 19.411 min Scan# 3587
Delta R.T. -0.004 min
Lab File: BN026089.D
Acq: 29 Jun 2023 11:26

Tgt Ion:	202	Resp:	48781
Ion Ratio	Lower	Upper	
202	100		
101	11.6	9.5	14.3
100	8.8	7.3	10.9


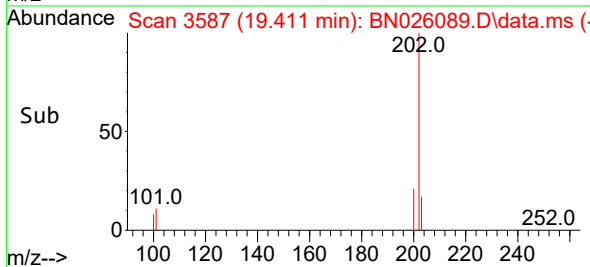
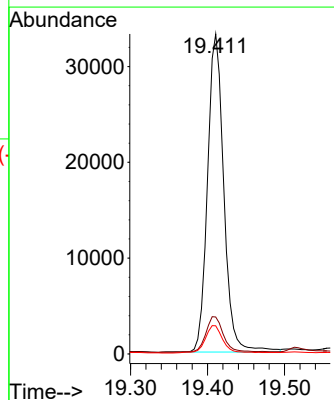
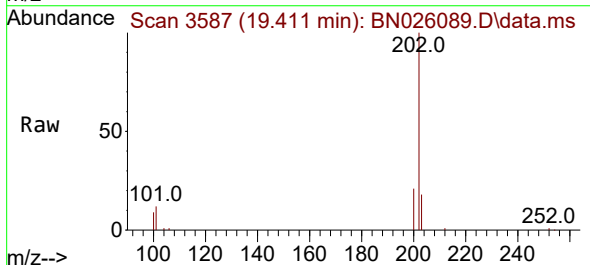


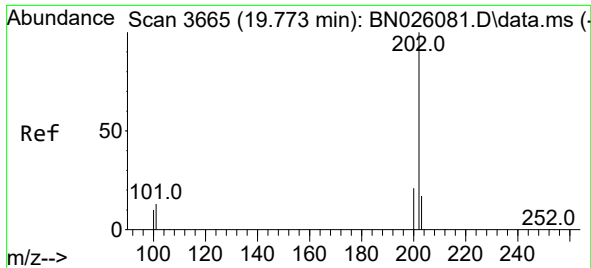

#20
Pyrene
Concen: 0.436 ng/ul
RT: 19.773 min Scan# 3665
Delta R.T. -0.004 min
Lab File: BN026089.D
Acq: 29 Jun 2023 11:26




Instrument :
BNA_N
ClientSampleId :
DCFT3DL


Tgt Ion:202 Resp: 43208
Ion Ratio Lower Upper
202 100
101 13.5 11.4 17.0
100 11.0 9.1 13.7

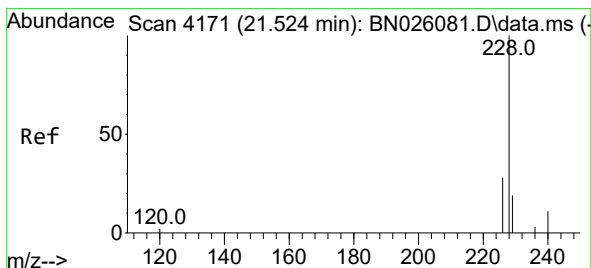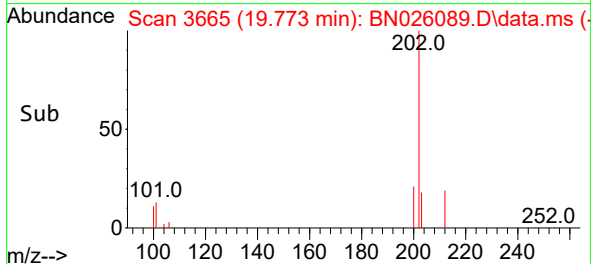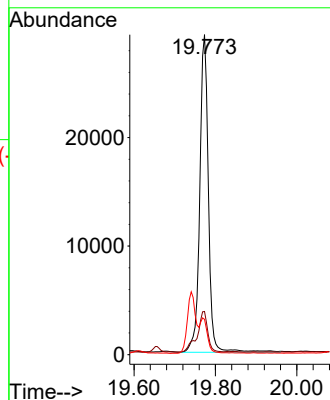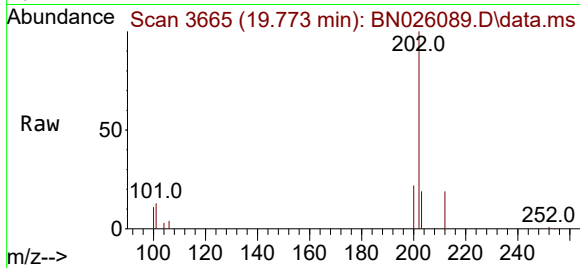

#21
Benzo(a)anthracene
Concen: 0.194 ng/ul
RT: 21.530 min Scan# 4173
Delta R.T. 0.001 min
Lab File: BN026089.D
Acq: 29 Jun 2023 11:26

Tgt Ion:228 Resp: 14296
Ion Ratio Lower Upper
228 100
229 28.3 15.8 23.6#
226 30.5 22.5 33.7


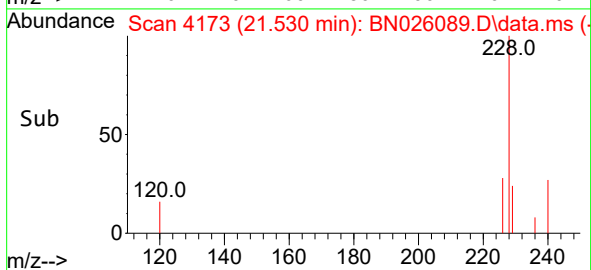
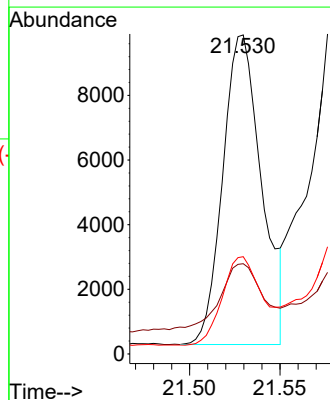
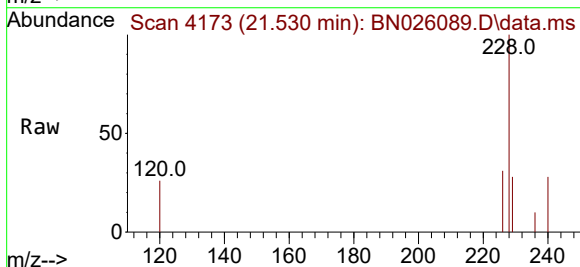


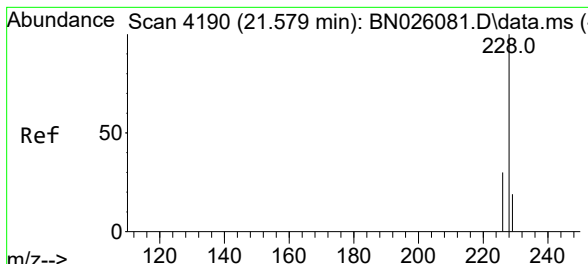

#22
 Chrysene
 Concen: 0.271 ng/ul
 RT: 21.582 min Scan# 4191
 Delta R.T. 0.004 min
 Lab File: BN026089.D
 Acq: 29 Jun 2023 11:26




Instrument :
 BNA_N
 ClientSampleId :
 DCFT3DL


Tgt Ion:	228	Resp:	20730
Ion Ratio	Lower	Upper	
228	100		
226	32.3	24.8	37.2
229	24.2	15.7	23.5

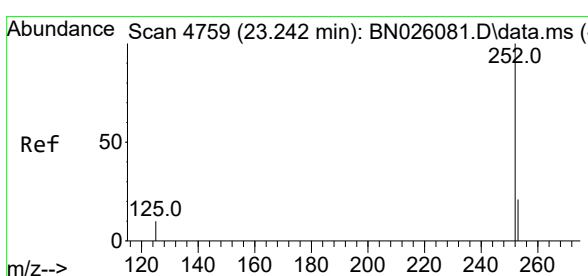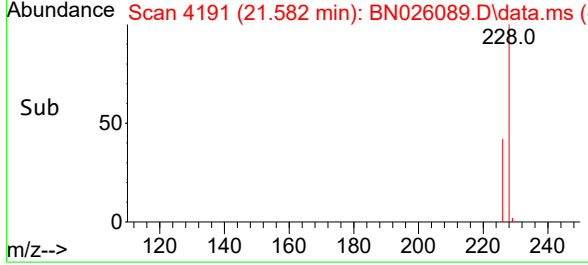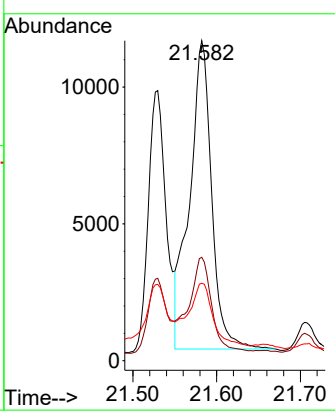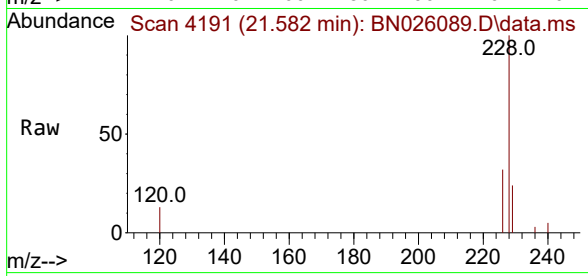

#24
 Benzo(b)fluoranthene
 Concen: 0.529 ng/ul
 RT: 23.254 min Scan# 4763
 Delta R.T. 0.001 min
 Lab File: BN026089.D
 Acq: 29 Jun 2023 11:26


Tgt Ion:	252	Resp:	38955
Ion Ratio	Lower	Upper	
252	100		
253	31.4	0.0	55.6
125	26.0	0.0	35.8

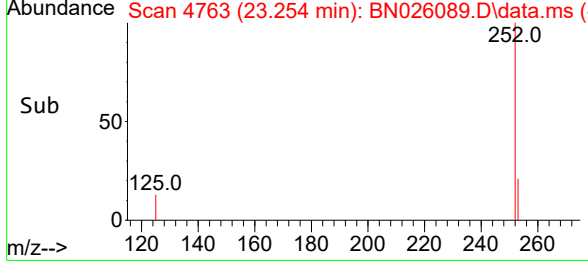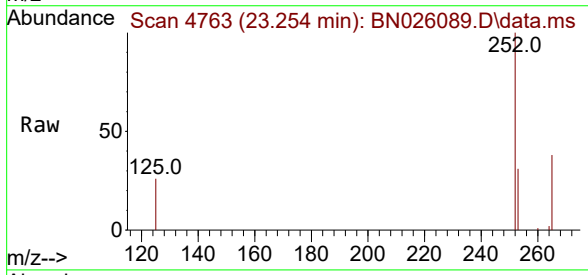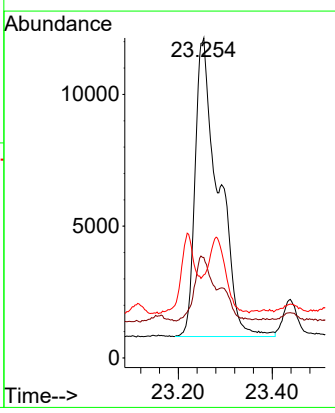



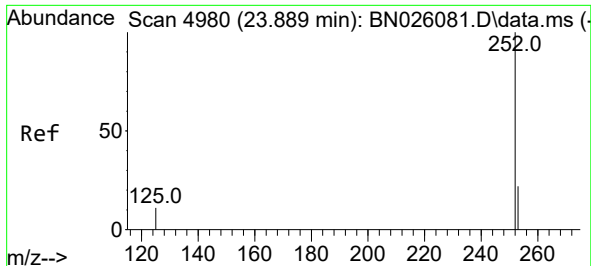


#26
Benzo(a)pyrene
Concen: 0.269 ng/ul
RT: 23.889 min Scan# 4980
Delta R.T. -0.017 min
Lab File: BN026089.D
Acq: 29 Jun 2023 11:26

Instrument :
BNA_N
ClientSampleId :
DCFT3DL



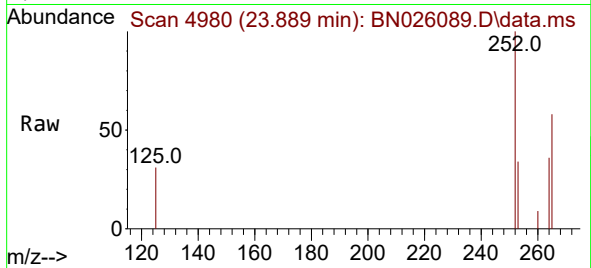



Tgt Ion:252 Resp: 17227
Ion Ratio Lower Upper
252 100
253 34.1 26.0 39.0
125 30.9 17.3 25.9#

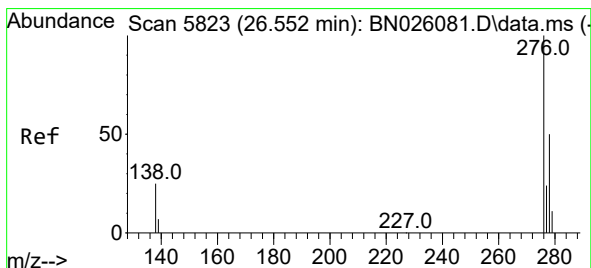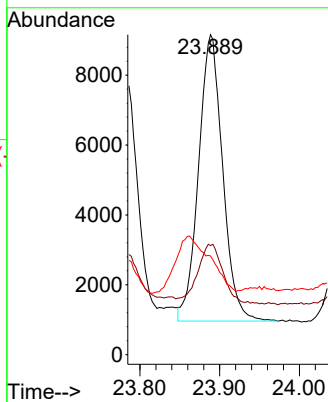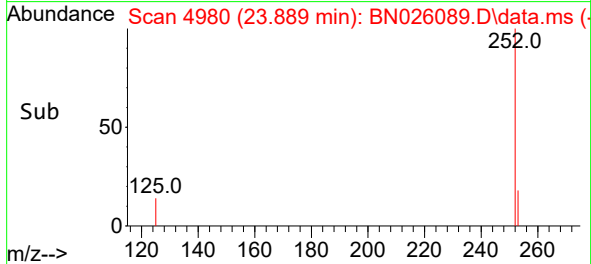

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.210 ng/ul
RT: 26.552 min Scan# 5823
Delta R.T. -0.043 min
Lab File: BN026089.D
Acq: 29 Jun 2023 11:26

Tgt Ion:276 Resp: 14655
Ion Ratio Lower Upper
276 100
138 22.6 24.5 36.7#
227 0.0 0.0 0.0


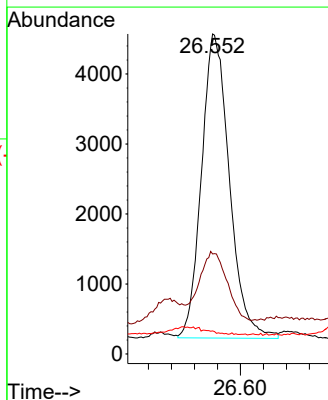
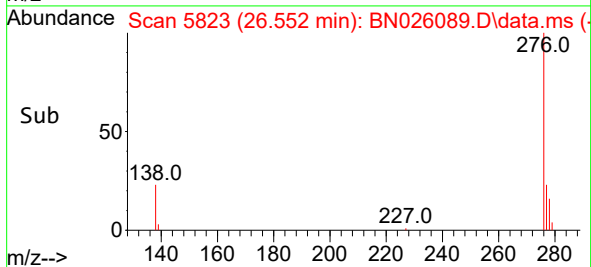
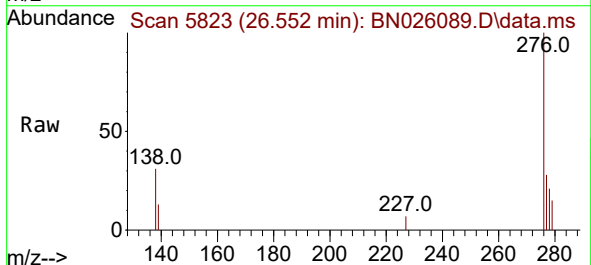


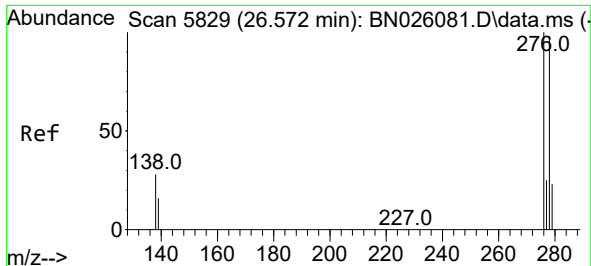

#28
Dibenzo(a,h)anthracene
Concen: 0.062 ng/ul
RT: 26.568 min Scan# 5828
Delta R.T. -0.046 min
Lab File: BN026089.D
Acq: 29 Jun 2023 11:26

Instrument :
BNA_N
ClientSampleId :
DCFT3DL

Tgt Ion:278 Resp: 3291
Ion Ratio Lower Upper
278 100
139 56.1 19.0 28.4#
279 71.9 26.7 40.1#

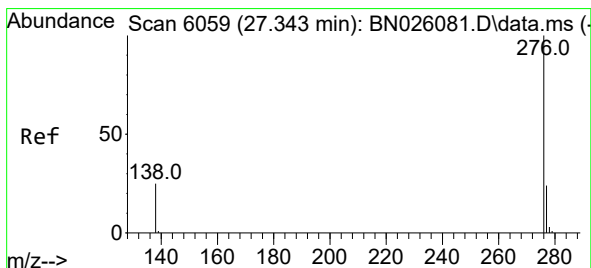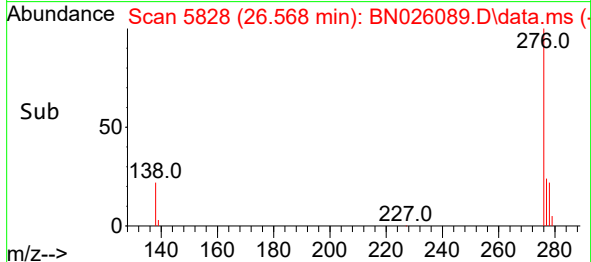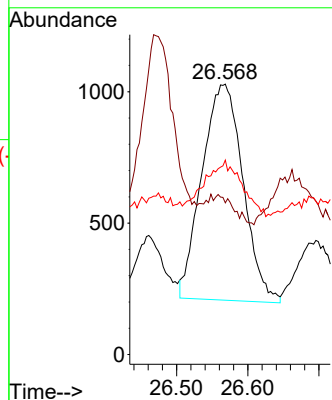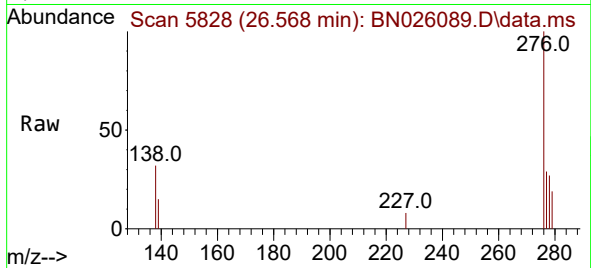

#29
Benzo(g,h,i)perylene
Concen: 0.245 ng/ul
RT: 27.350 min Scan# 6061
Delta R.T. -0.036 min
Lab File: BN026089.D
Acq: 29 Jun 2023 11:26

Tgt Ion:276 Resp: 15216
Ion Ratio Lower Upper
276 100
138 32.7 23.4 35.0
277 27.8 20.0 30.0

