

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062923\
 Data File : BN026098.D
 Acq On : 29 Jun 2023 17:16
 Operator : MA/JU
 Sample : PB153628BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK628

Quant Time: Jun 30 00:44:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 22:47:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.968	152	6948	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	23486	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.606	164	14401	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	28247	0.400	ng/ul	0.00
17) Chrysene-d12	21.548	240	14355	0.400	ng/ul	0.00
23) Perylene-d12	24.009	264	18375	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	38697	4.946	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.369	152	10120	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.381	212	18071	0.331	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.596	166	3705	0.059	ng/ul#	13
20) Pyrene	19.743	202	2725	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.854	252	4640	0.068	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062923\
Data File : BN026098.D
Acq On : 29 Jun 2023 17:16
Operator : MA/JU
Sample : PB153628BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK628

Quant Time: Jun 30 00:44:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 22:47:20 2023
Response via : Initial Calibration




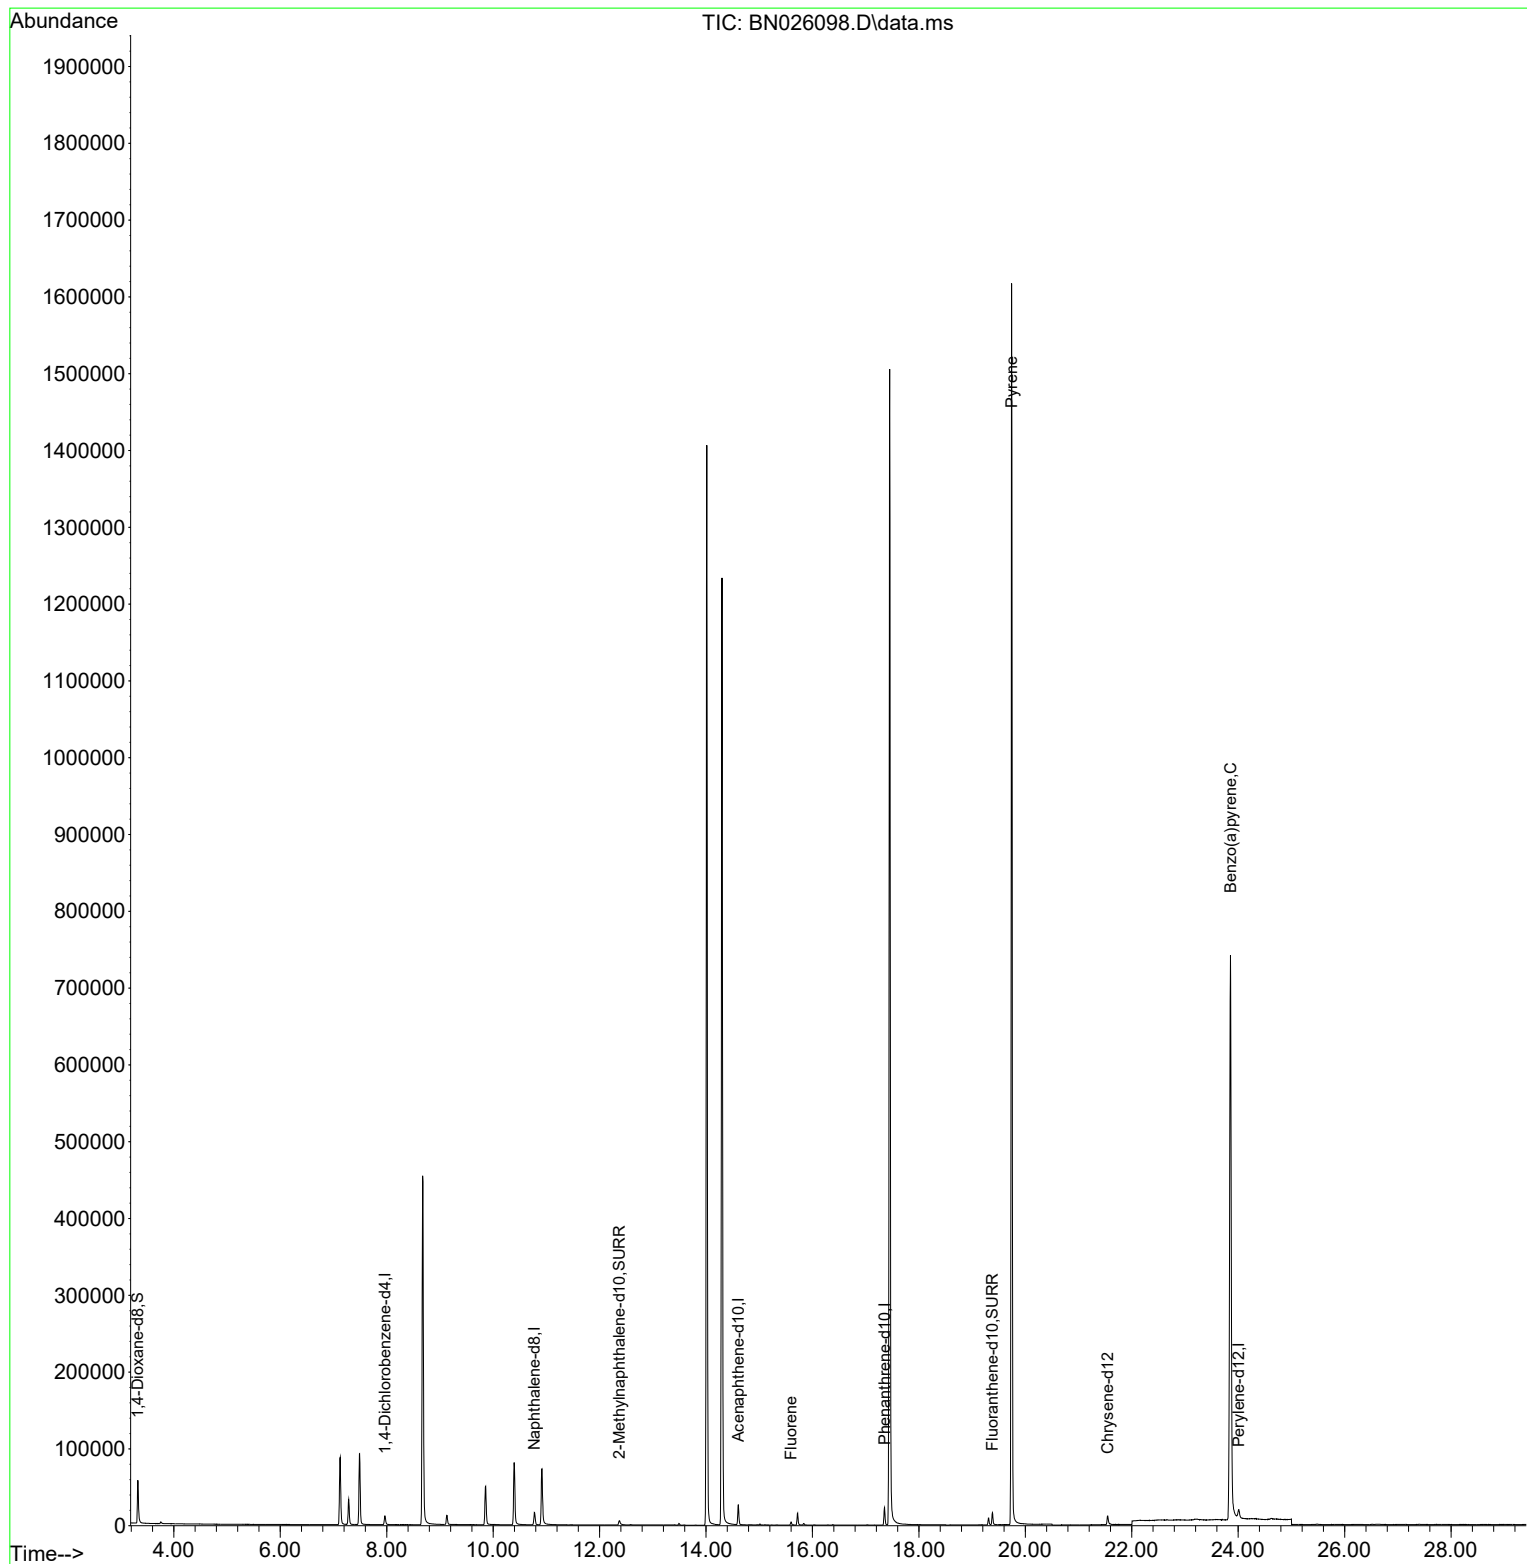


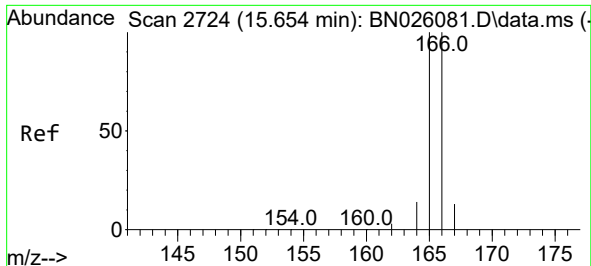

#12
Fluorene
Concen: 0.059 ng/ul
RT: 15.596 min Scan# 21
Delta R.T. -0.066 min
Lab File: BN026098.D
Acq: 29 Jun 2023 17:16




Instrument :
BNA_N
ClientSampleId :
SBLK628


Tgt Ion:166 Resp: 3705
Ion Ratio Lower Upper
166 100
165 7.3 79.9 119.9#
167 30.6 10.8 16.2#

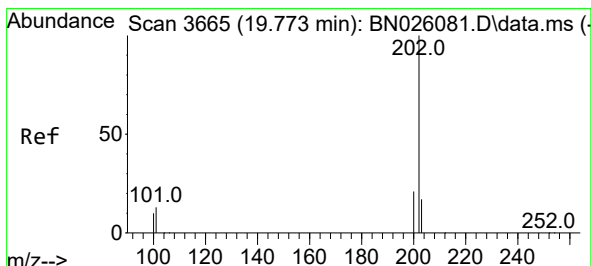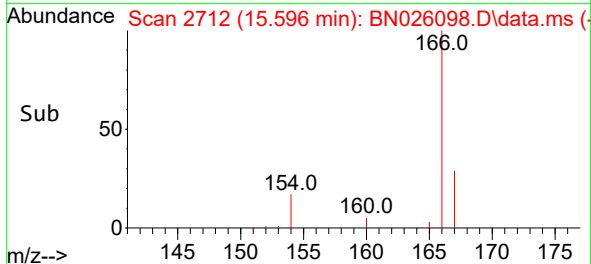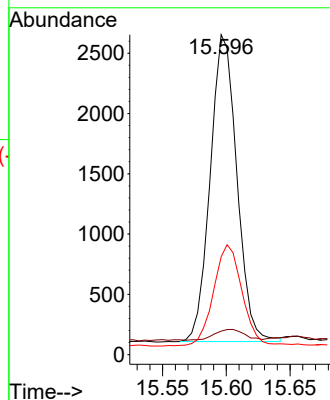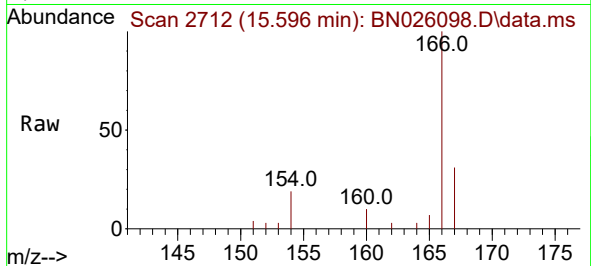

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.743 min Scan# 3659
Delta R.T. -0.034 min
Lab File: BN026098.D
Acq: 29 Jun 2023 17:16


Tgt Ion:202 Resp: 2725
Ion Ratio Lower Upper
202 100
101 173.4 11.4 17.0#
100 1315.1 9.1 13.7#

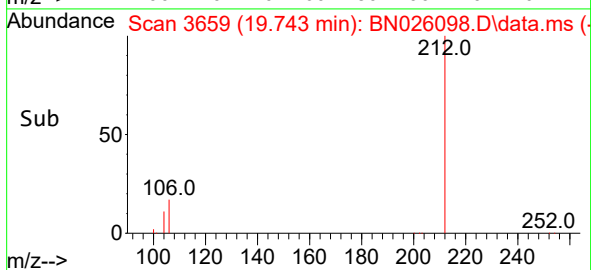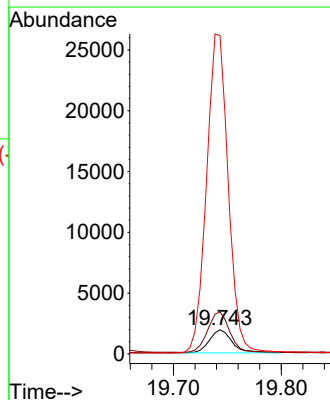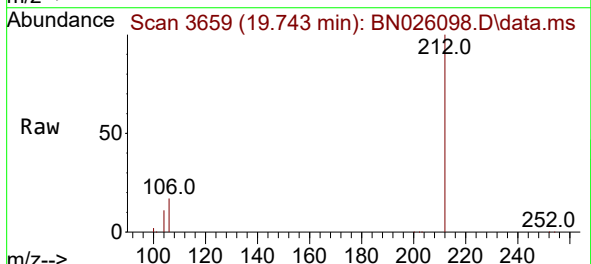

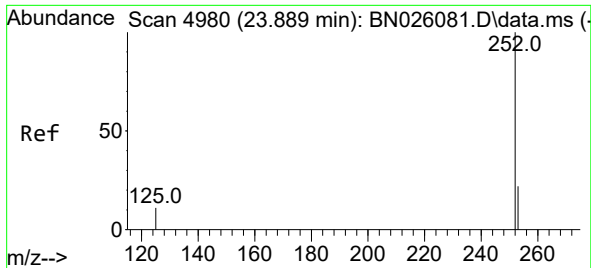

#26
Benzo(a)pyrene
Concen: 0.068 ng/ul
RT: 23.854 min Scan# 4969
Delta R.T. -0.051 min
Lab File: BN026098.D
Acq: 29 Jun 2023 17:16

Instrument :
BNA_N
ClientSampleId :
SBLK628

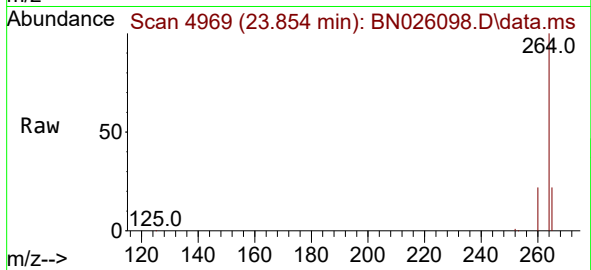

Tgt Ion:252 Resp: 4640
Ion Ratio Lower Upper
252 100
253 65.2 26.0 39.0#
125 66.5 17.3 25.9#

