

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062923\
 Data File : BN026064.D
 Acq On : 28 Jun 2023 18:39
 Operator : MA/JU
 Sample : 03142-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCFT4

Quant Time: Jun 28 23:15:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 22:47:20 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 06/29/2023
 Supervised By :mohammad ahmed 06/30/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	6652	0.400	ng/ul	0.00
4) Naphthalene-d8	10.781	136	22051	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.607	164	13625	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.355	188	28242	0.400	ng/ul	0.00
17) Chrysene-d12	21.541	240	15696	0.400	ng/ul	# 0.00
23) Perylene-d12	23.993	264	15621	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.327	96	21852	2.917	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.370	152	6850	0.202	ng/ul	0.00
18) Fluoranthene-d10	19.382	212	14900	0.249	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.831	128	3134	0.050	ng/ul#	89
7) 2-Methylnaphthalene	12.447	142	2186	0.054	ng/ul	99
8) 1-Methylnaphthalene	12.662	142	1784	0.043	ng/ul	99
10) Acenaphthylene	14.330	152	2117	0.033	ng/ul#	79
11) Acenaphthene	14.672	153	1404	0.027	ng/ul	96
15) Phenanthrene	17.393	178	33171	0.356	ng/ul	99
16) Anthracene	17.486	178	4464	0.054	ng/ul#	88
19) Fluoranthene	19.410	202	109496	1.306	ng/ul	99
20) Pyrene	19.772	202	87882m	1.008	ng/ul	
21) Benzo(a)anthracene	21.523	228	38979	0.602	ng/ul	97
22) Chrysene	21.579	228	56521	0.839	ng/ul	98
24) Benzo(b)fluoranthene	23.245	252	80558m	1.208	ng/ul	
25) Benzo(k)fluoranthene	23.288	252	27082m	0.405	ng/ul	
26) Benzo(a)pyrene	23.882	252	44582	0.770	ng/ul	94
27) Indeno(1,2,3-cd)pyrene	26.551	276	40987	0.648	ng/ul#	87
28) Dibenzo(a,h)anthracene	26.564	278	9106	0.190	ng/ul#	79
29) Benzo(g,h,i)perylene	27.346	276	39647	0.705	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062923\
Data File : BN026064.D
Acq On : 28 Jun 2023 18:39
Operator : MA/JU
Sample : 03142-17
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCFT4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/29/2023
Supervised By :mohammad ahmed 06/30/2023


Quant Time: Jun 28 23:15:50 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 22:47:20 2023
Response via : Initial Calibration

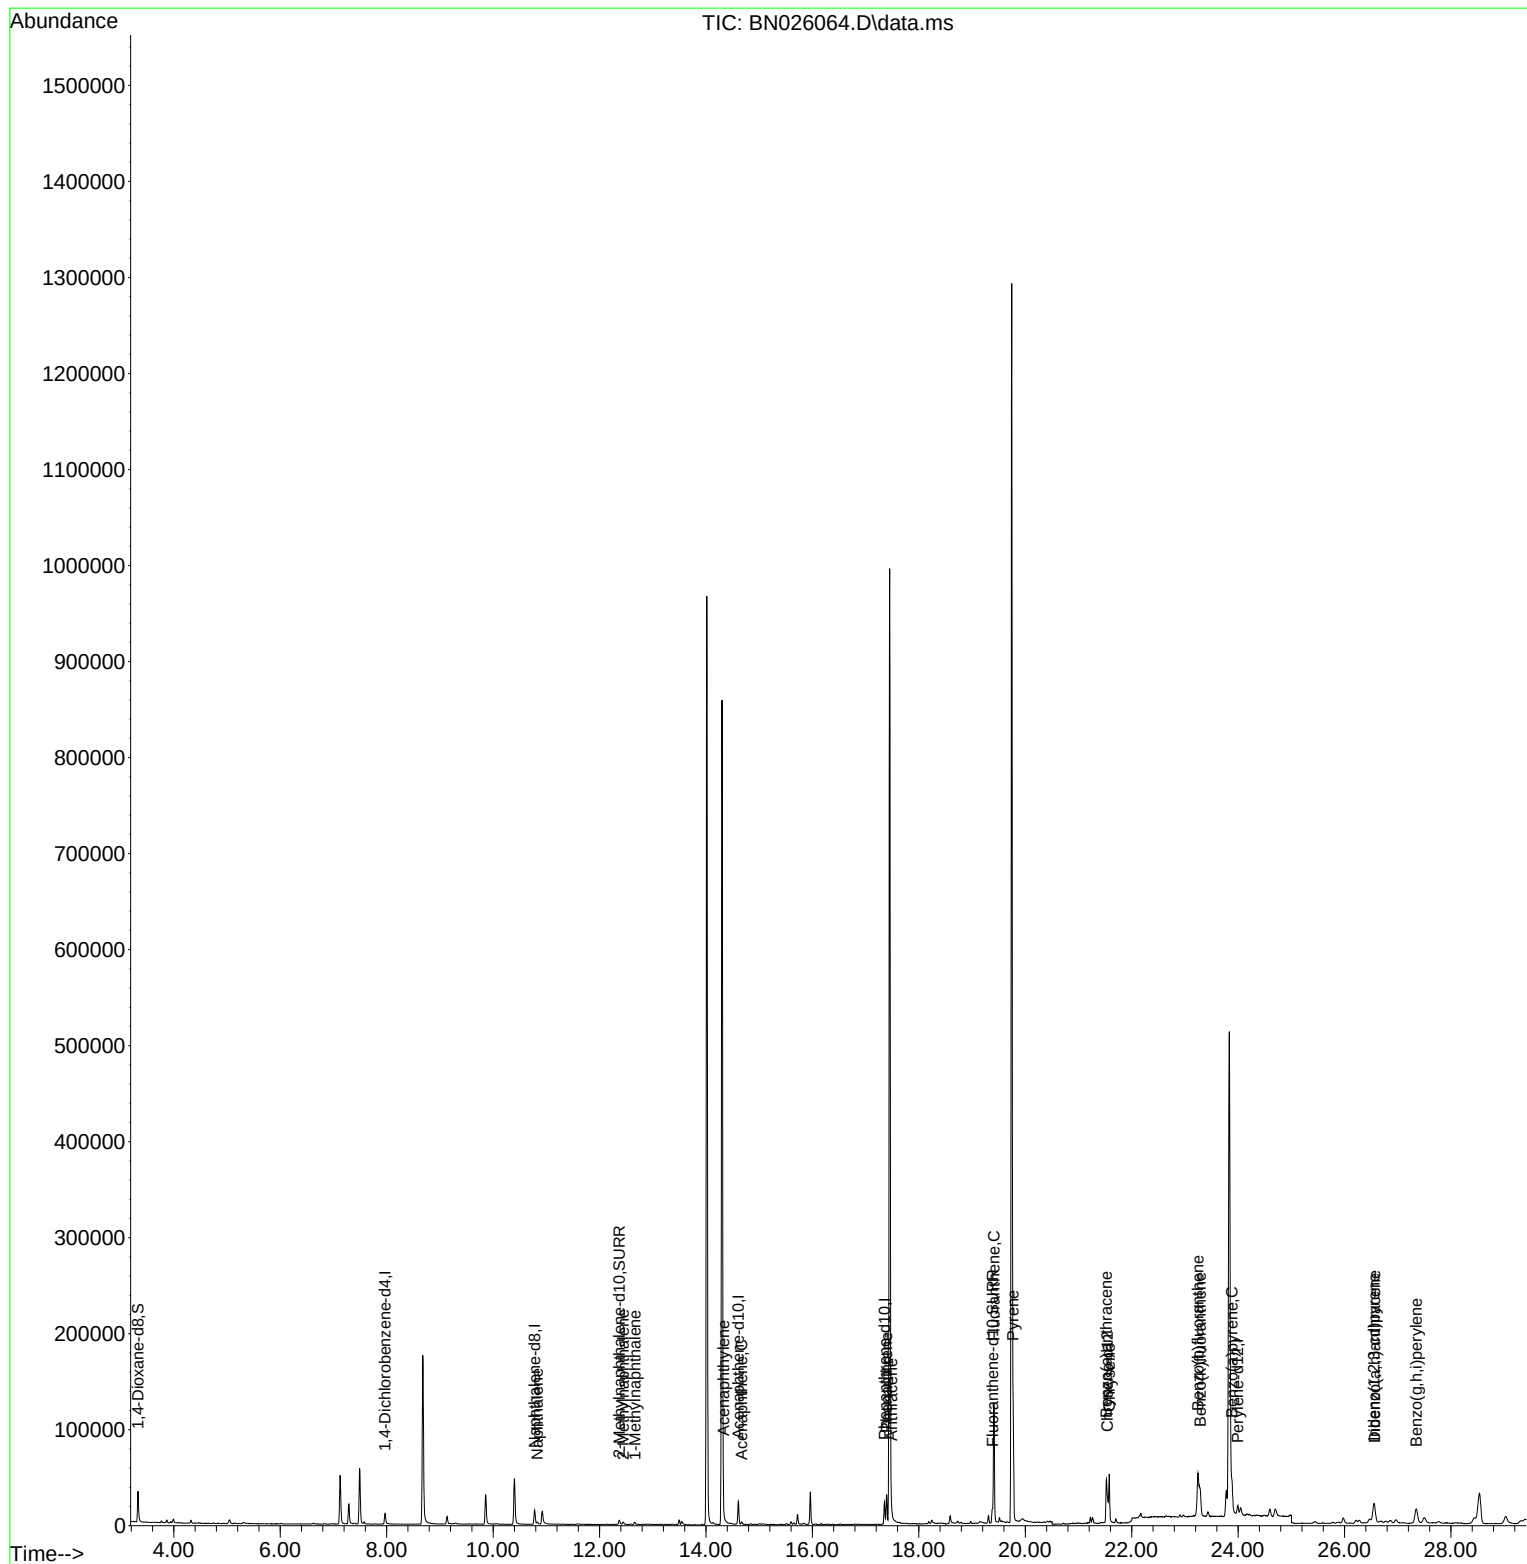

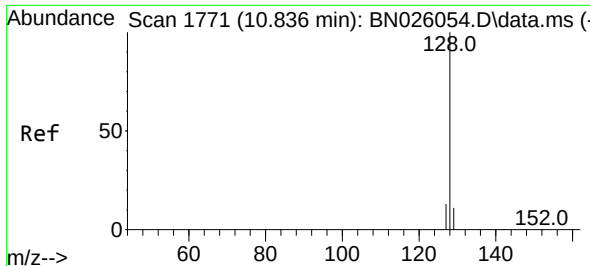

#5
Naphthalene
Concen: 0.050 ng/ul
RT: 10.831 min Scan# 1770
Delta R.T. -0.005 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39




Instrument :
BNA_N
ClientSampleId :
DCFT4



Tgt Ion:128 Resp: 3134
Ion Ratio Lower Upper
128 100
129 17.2 9.1 13.7
127 16.5 10.7 16.1




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/29/2023
Supervised By :mohammad ahmed 06/30/2023

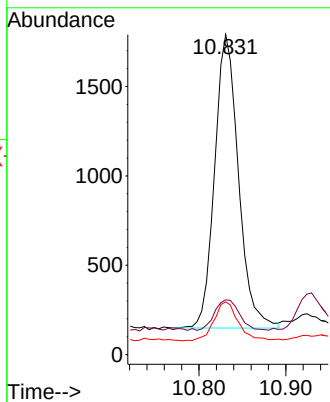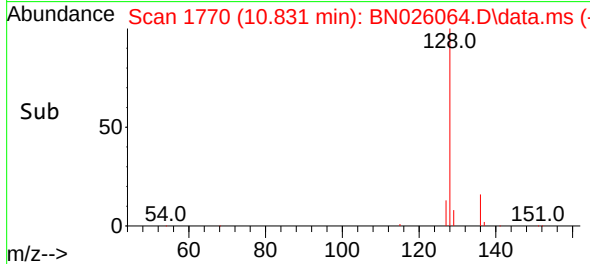

#7
2-Methylnaphthalene
Concen: 0.054 ng/ul
RT: 12.447 min Scan# 2064
Delta R.T. 0.000 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39


Tgt Ion:142 Resp: 2186
Ion Ratio Lower Upper
142 100
141 91.2 71.9 107.9

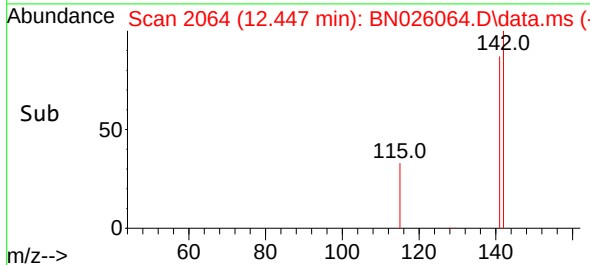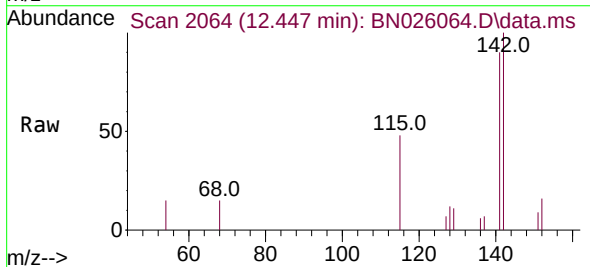



#8
1-Methylnaphthalene
Concen: 0.043 ng/ul
RT: 12.662 min Scan# 2103
Delta R.T. 0.000 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39




Instrument :
BNA_N
ClientSampleId :
DCFT4



Tgt Ion:142 Resp: 1784
Ion Ratio Lower Upper
142 100
141 92.3 74.2 111.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/29/2023
Supervised By :mohammad ahmed 06/30/2023

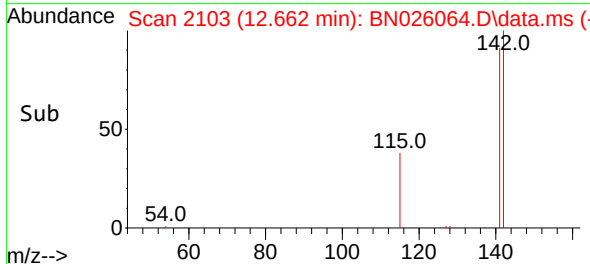

#10
Acenaphthylene
Concen: 0.033 ng/ul
RT: 14.330 min Scan# 2438
Delta R.T. 0.000 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39


Tgt Ion:152 Resp: 2117
Ion Ratio Lower Upper
152 100
151 27.0 16.2 24.4#
153 25.5 10.9 16.3#

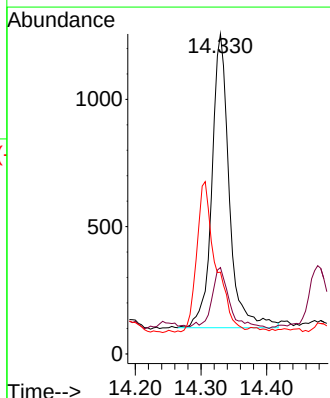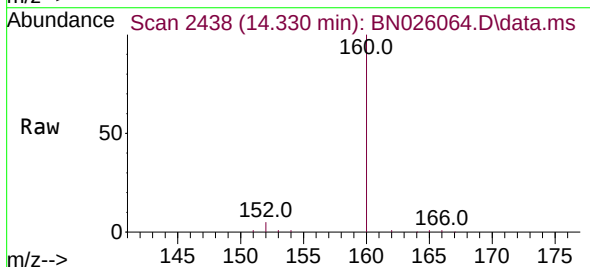

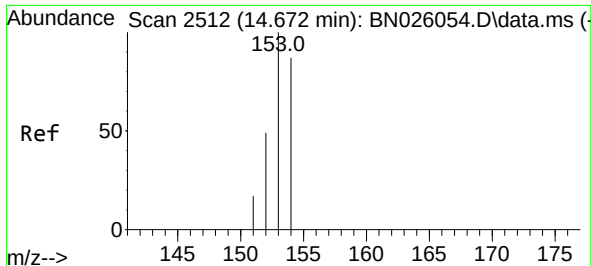

#11
Acenaphthene
Concen: 0.027 ng/u1
RT: 14.672 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39




Instrument :
BNA_N
ClientSampleId :
DCFT4

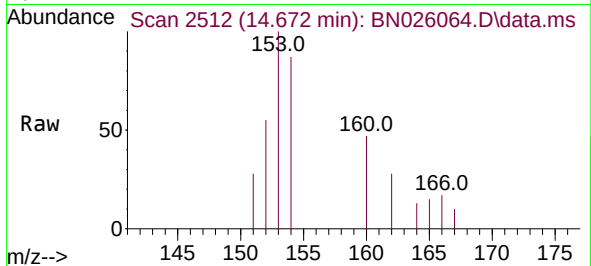

Tgt Ion:153 Resp: 1404
Ion Ratio Lower Upper
153 100
152 54.6 39.4 59.0
154 87.1 68.9 103.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/29/2023
Supervised By :mohammad ahmed 06/30/2023

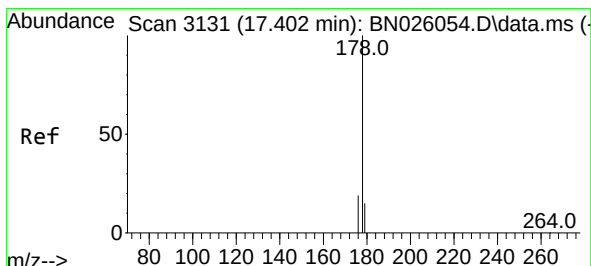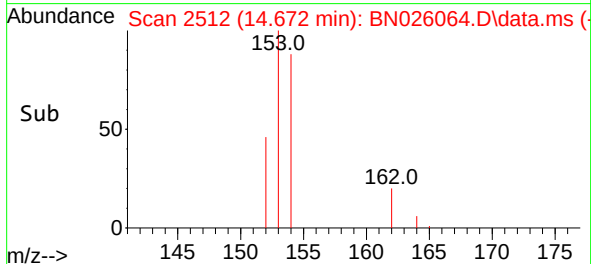

#15
Phenanthrene
Concen: 0.356 ng/u1
RT: 17.393 min Scan# 3129
Delta R.T. -0.008 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39

Tgt Ion:178 Resp: 33171
Ion Ratio Lower Upper
178 100
179 16.0 12.6 19.0
176 20.1 15.8 23.6

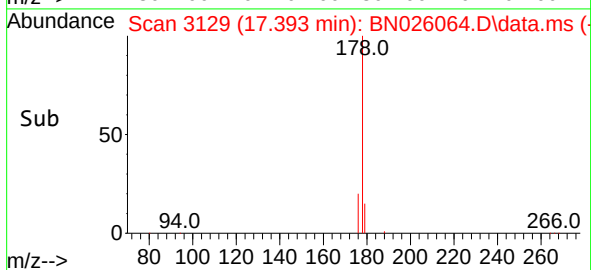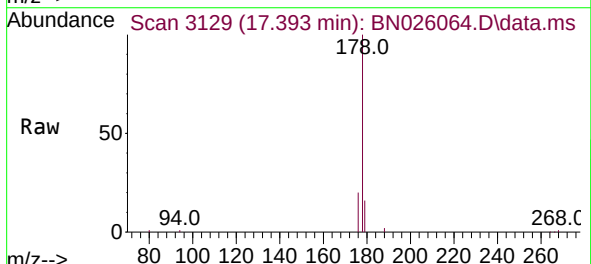

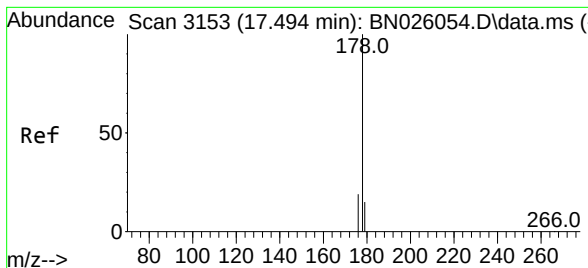

#16

Anthracene

Concen: 0.054 ng/ul

RT: 17.486 min Scan# 3151

Delta R.T. -0.008 min

Lab File: BN026064.D

Acq: 28 Jun 2023 18:39

Instrument :

BNA_N

ClientSampleId :

DCFT4





Tgt Ion:178	Resp:	4464
Ion Ratio	Lower	Upper
178	100	
179	21.3	12.6 18.8
176	23.5	15.1 22.7

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/29/2023

Supervised By :mohammad ahmed 06/30/2023

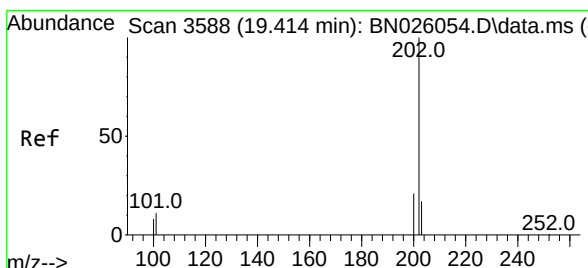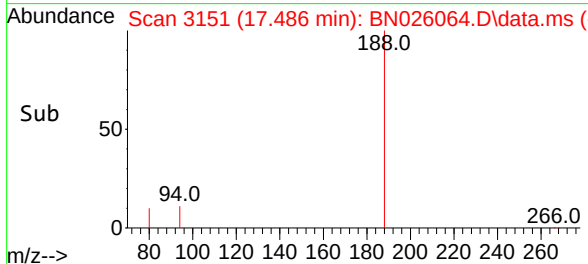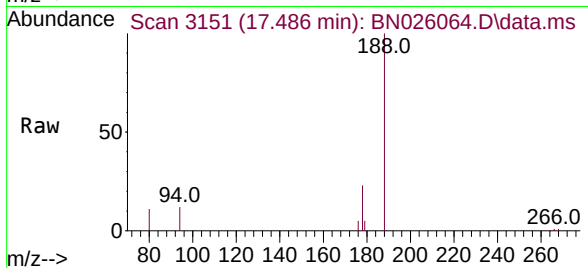

#19

Fluoranthene

Concen: 1.306 ng/ul




RT: 19.410 min Scan# 3587


Delta R.T. -0.005 min

Lab File: BN026064.D

Acq: 28 Jun 2023 18:39


Tgt Ion:202	Resp:	109496
Ion Ratio	Lower	Upper
202	100	
101	12.2	9.5 14.3
100	9.2	7.3 10.9

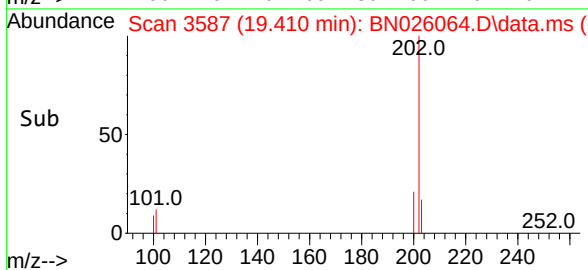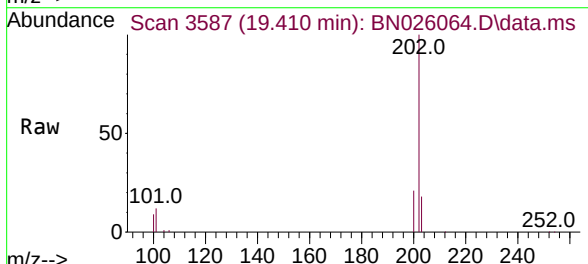

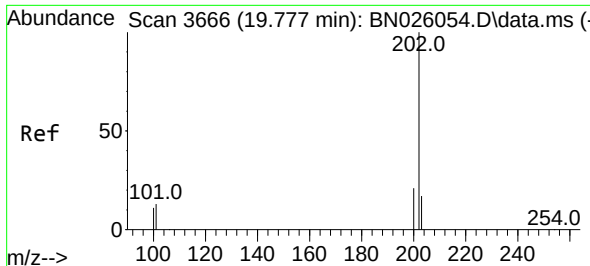

#20
Pyrene
Concen: 1.008 ng/ul m
RT: 19.772 min Scan# 3665
Delta R.T. -0.005 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39




Instrument :
BNA_N
ClientSampleId :
DCFT4




Tgt Ion:202 Resp: 8788
Ion Ratio Lower Upper
202 100
101 13.4 11.4 17.0
100 11.2 9.1 13.7

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/29/2023
Supervised By :mohammad ahmed 06/30/2023

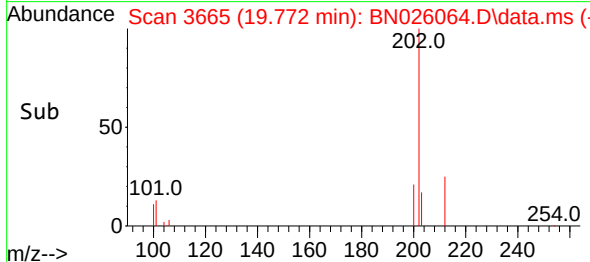


#21
Benzo(a)anthracene
Concen: 0.602 ng/ul
RT: 21.523 min Scan# 4171
Delta R.T. -0.006 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39

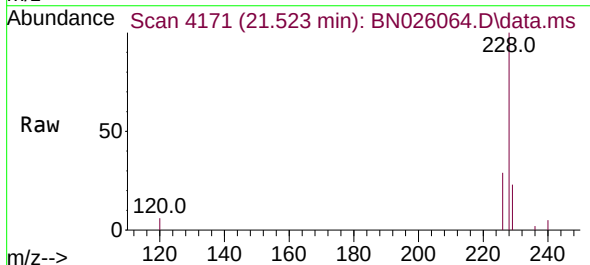


Tgt Ion:228 Resp: 38979
Ion Ratio Lower Upper
228 100
229 22.5 15.8 23.6
226 28.9 22.5 33.7

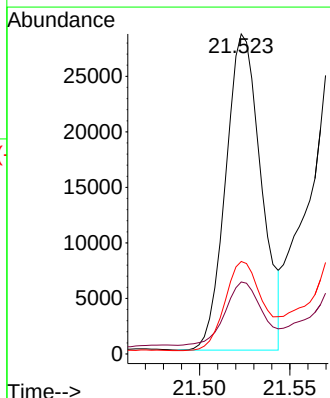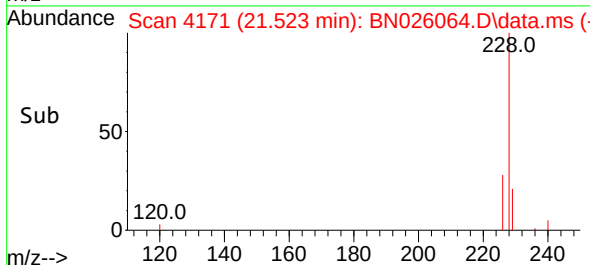

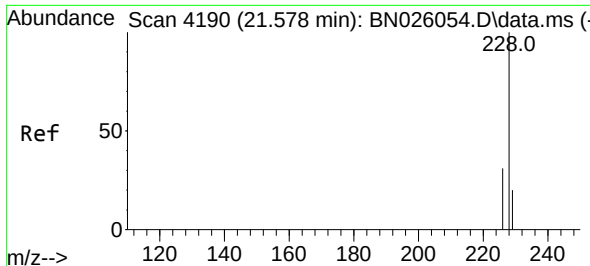

#22
Chrysene
Concen: 0.839 ng/ul
RT: 21.579 min Scan# 4190
Delta R.T. 0.000 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39




Instrument :
BNA_N
ClientSampleId :
DCFT4




Tgt Ion:228 Resp: 5652
Ion Ratio Lower Upper
228 100
226 31.3 24.8 37.2
229 21.8 15.7 23.5

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/29/2023
Supervised By :mohammad ahmed 06/30/2023

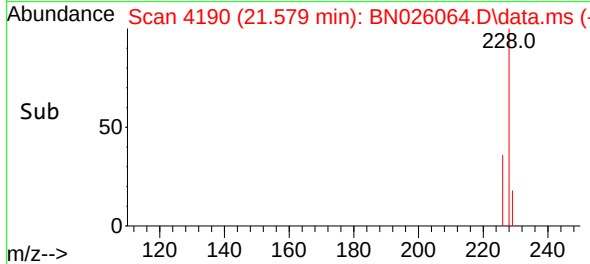


#24
Benzo(b)fluoranthene
Concen: 1.208 ng/ul m
RT: 23.245 min Scan# 4760
Delta R.T. -0.009 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39

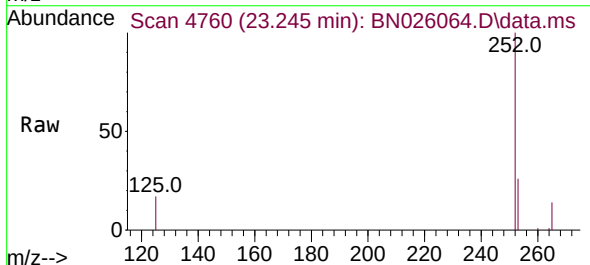


Tgt Ion:252 Resp: 80558
Ion Ratio Lower Upper
252 100
253 25.5 0.0 55.6
125 17.0 0.0 35.8

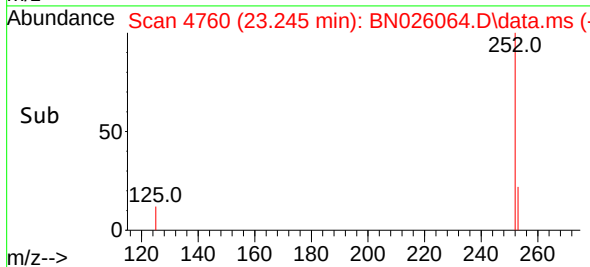



#25
Benzo(k)fluoranthene
Concen: 0.405 ng/ul m
RT: 23.288 min Scan# 4775
Delta R.T. -0.015 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39




Instrument :
BNA_N
ClientSampleId :
DCFT4

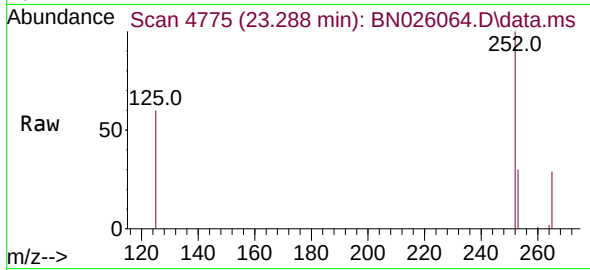

Tgt Ion:252 Resp: 27082
Ion Ratio Lower Upper
252 100
253 30.0 23.2 34.8
125 59.7 15.0 22.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/29/2023
Supervised By :mohammad ahmed 06/30/2023

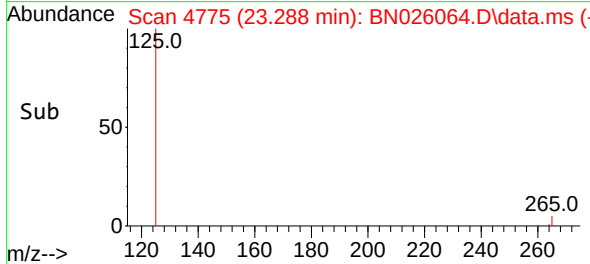

#26
Benzo(a)pyrene
Concen: 0.770 ng/ul
RT: 23.882 min Scan# 4978
Delta R.T. -0.023 min
Lab File: BN026064.D
Acq: 28 Jun 2023 18:39


Tgt Ion:252 Resp: 44582
Ion Ratio Lower Upper
252 100
253 28.2 26.0 39.0
125 19.8 17.3 25.9

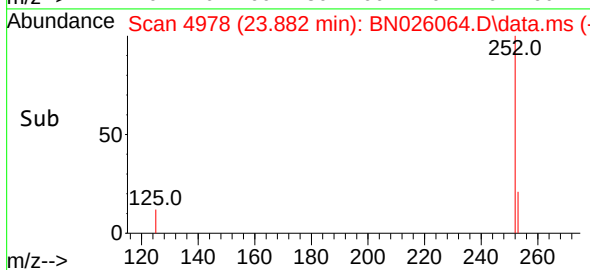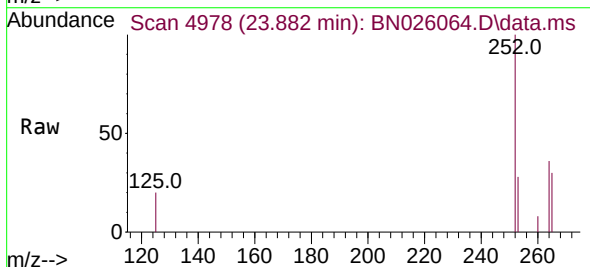

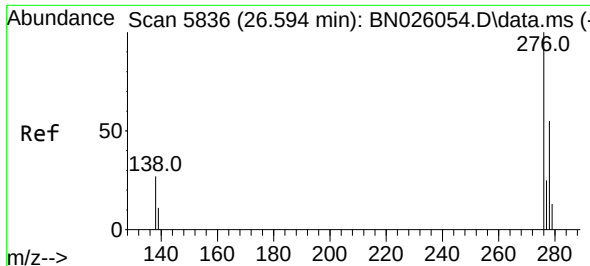

#27
 Indeno(1,2,3-cd)pyrene
 Concen: 0.648 ng/ul
 RT: 26.551 min Scan# 5823
 Delta R.T. -0.044 min
 Lab File: BN026064.D
 Acq: 28 Jun 2023 18:39




Instrument :
 BNA_N
 ClientSampleId :
 DCFT4




Tgt Ion:276 Resp: 4098
 Ion Ratio Lower Upper
 276 100
 138 23.4 24.5 36.7
 227 0.0 0.0 0.0

Manual Integrations
 APPROVED



Reviewed By :Yogesh Patel 06/29/2023
 Supervised By :mohammad ahmed 06/30/2023

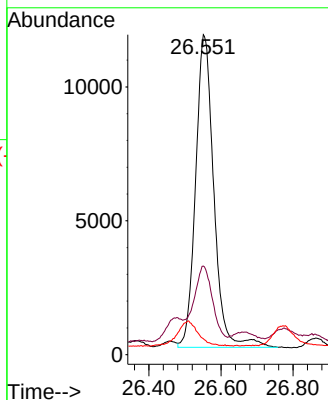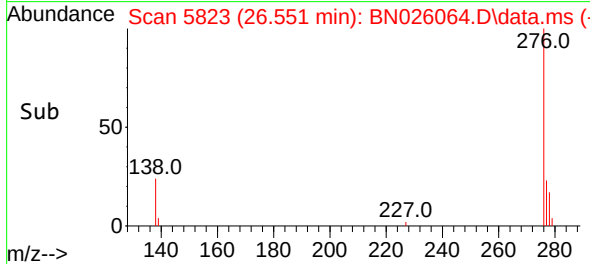


#28
 Dibenzo(a,h)anthracene
 Concen: 0.190 ng/ul
 RT: 26.564 min Scan# 5827
 Delta R.T. -0.050 min
 Lab File: BN026064.D
 Acq: 28 Jun 2023 18:39

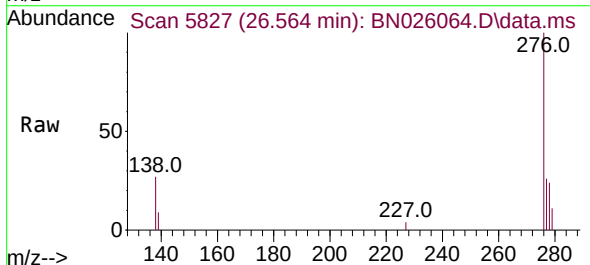


Tgt Ion:278 Resp: 9106
 Ion Ratio Lower Upper
 278 100
 139 36.0 19.0 28.4#
 279 43.3 26.7 40.1#

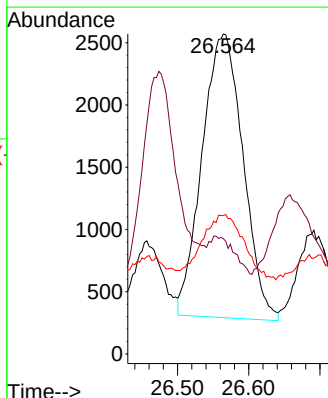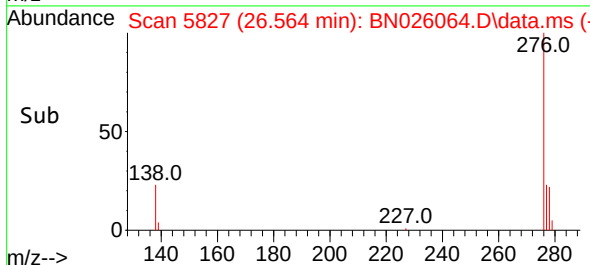

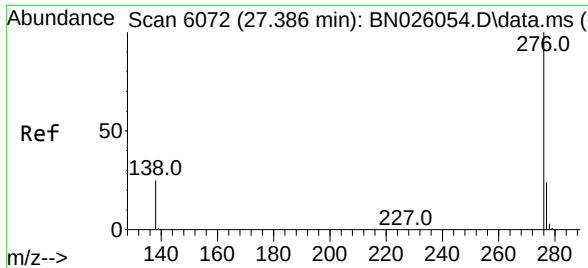

#29
 Benzo(g,h,i)perylene
 Concen: 0.705 ng/ul
 RT: 27.346 min Scan# 6072
 Delta R.T. -0.040 min
 Lab File: BN026064.D
 Acq: 28 Jun 2023 18:39

Instrument :
 BNA_N
 ClientSampleId :
 DCFT4

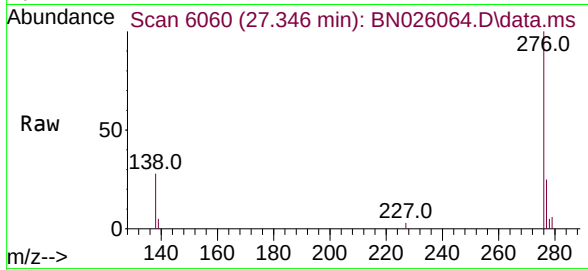

Tgt Ion: 276 Resp: 3964
 Ion Ratio Lower Upper
 276 100
 138 28.0 23.4 35.0
 277 25.1 20.0 30.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/29/2023
 Supervised By :mohammad ahmed 06/30/2023

