
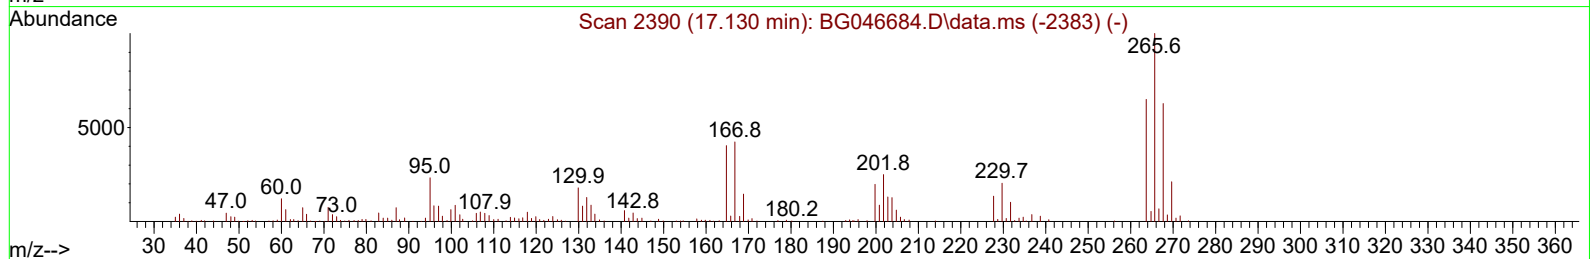
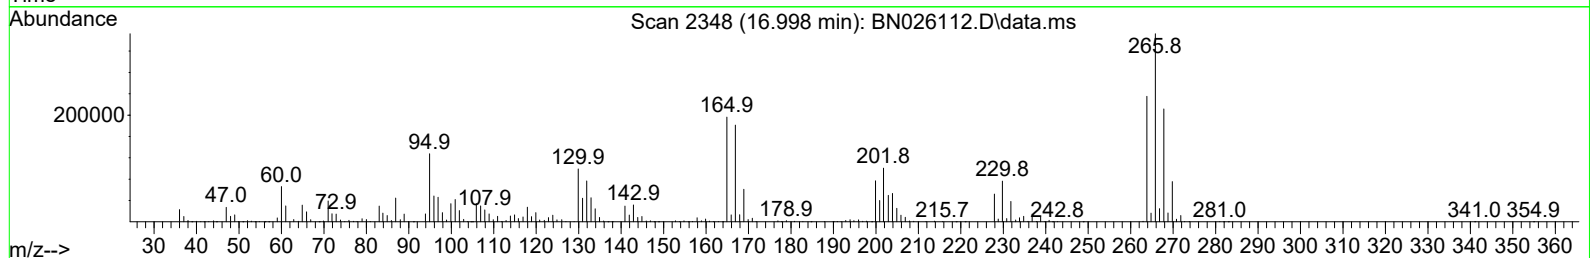


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063023\
Data File : BN026112.D
Acq On : 30 Jun 2023 03:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 08:14:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 08:14:10 2023
Response via : Initial Calibration

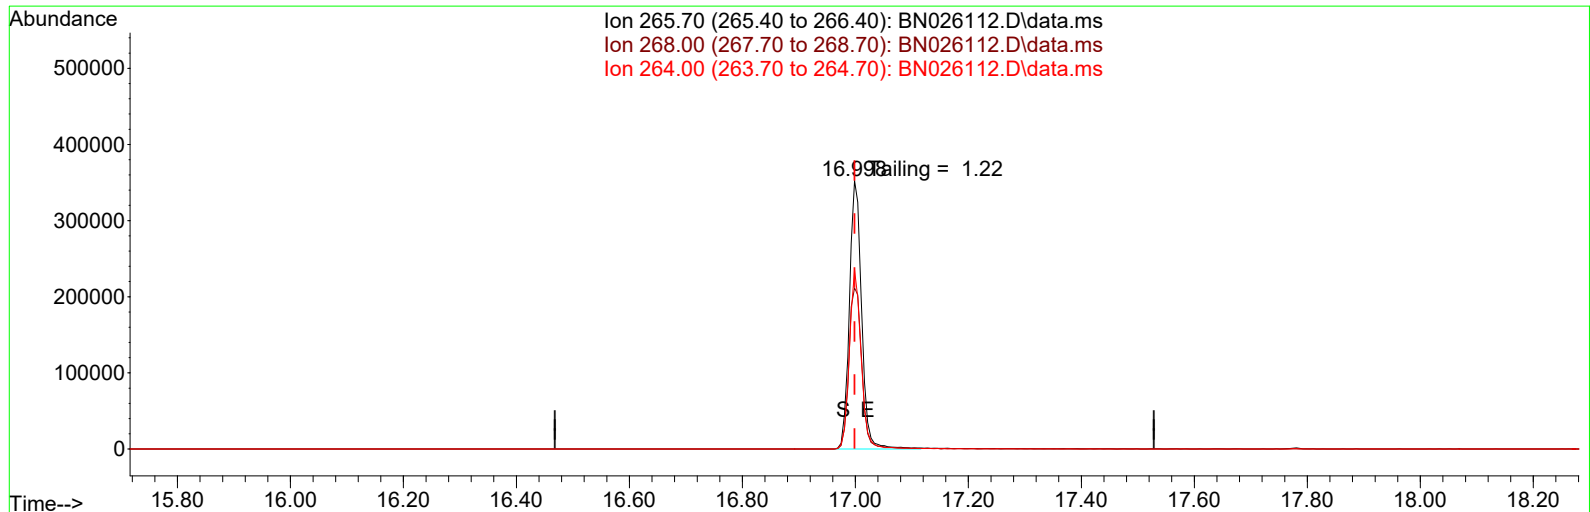

TIC: BN026112.D\data.ms

(70) Pentachlorophenol (C)




16.998min (0.000) 23154.49 ng

response 533684

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.06
264.00	61.60	66.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063023\
 Data File : BN026112.D
 Acq On : 30 Jun 2023 03:36
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 08:14:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 30 08:14:10 2023
 Response via : Initial Calibration

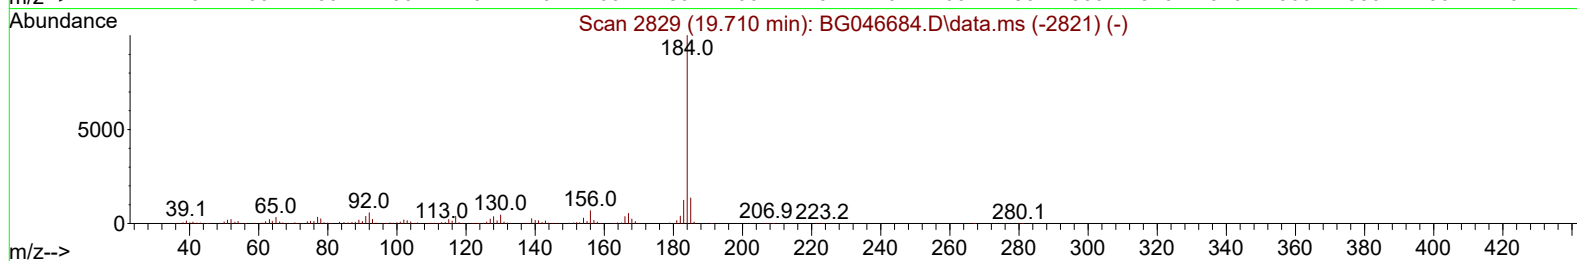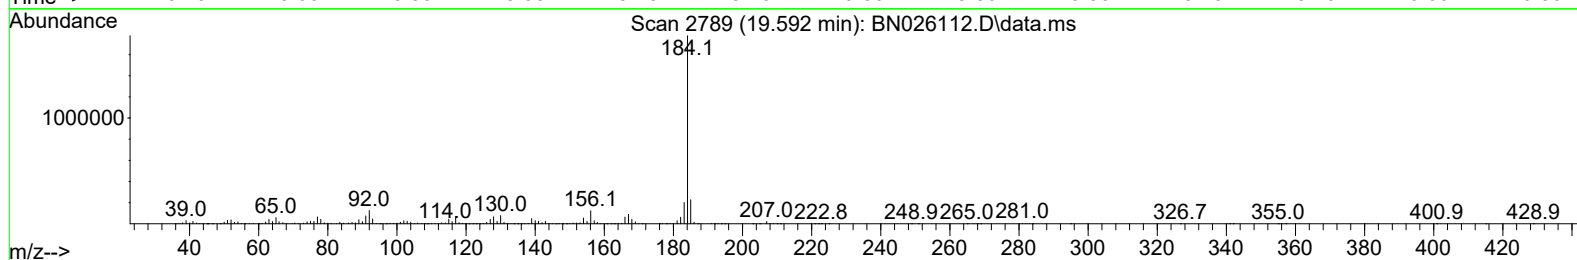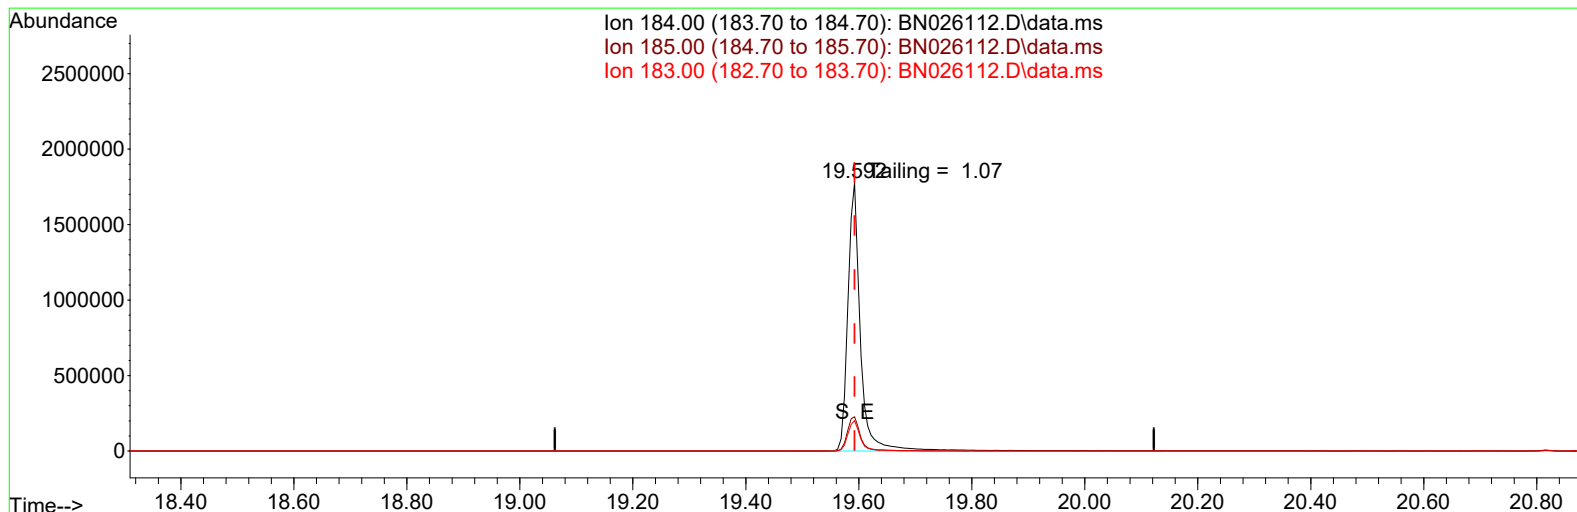

TIC: BN026112.D\data.ms

(77) Benzidine**19.592min (0.000) 1537378.33 ng****response 2748635**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.80
183.00	13.20	11.36
0.00	0.00	0.00