


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063023\
 Data File : BN026112.D
 Acq On : 30 Jun 2023 03:36
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 30 07:06:59 2023

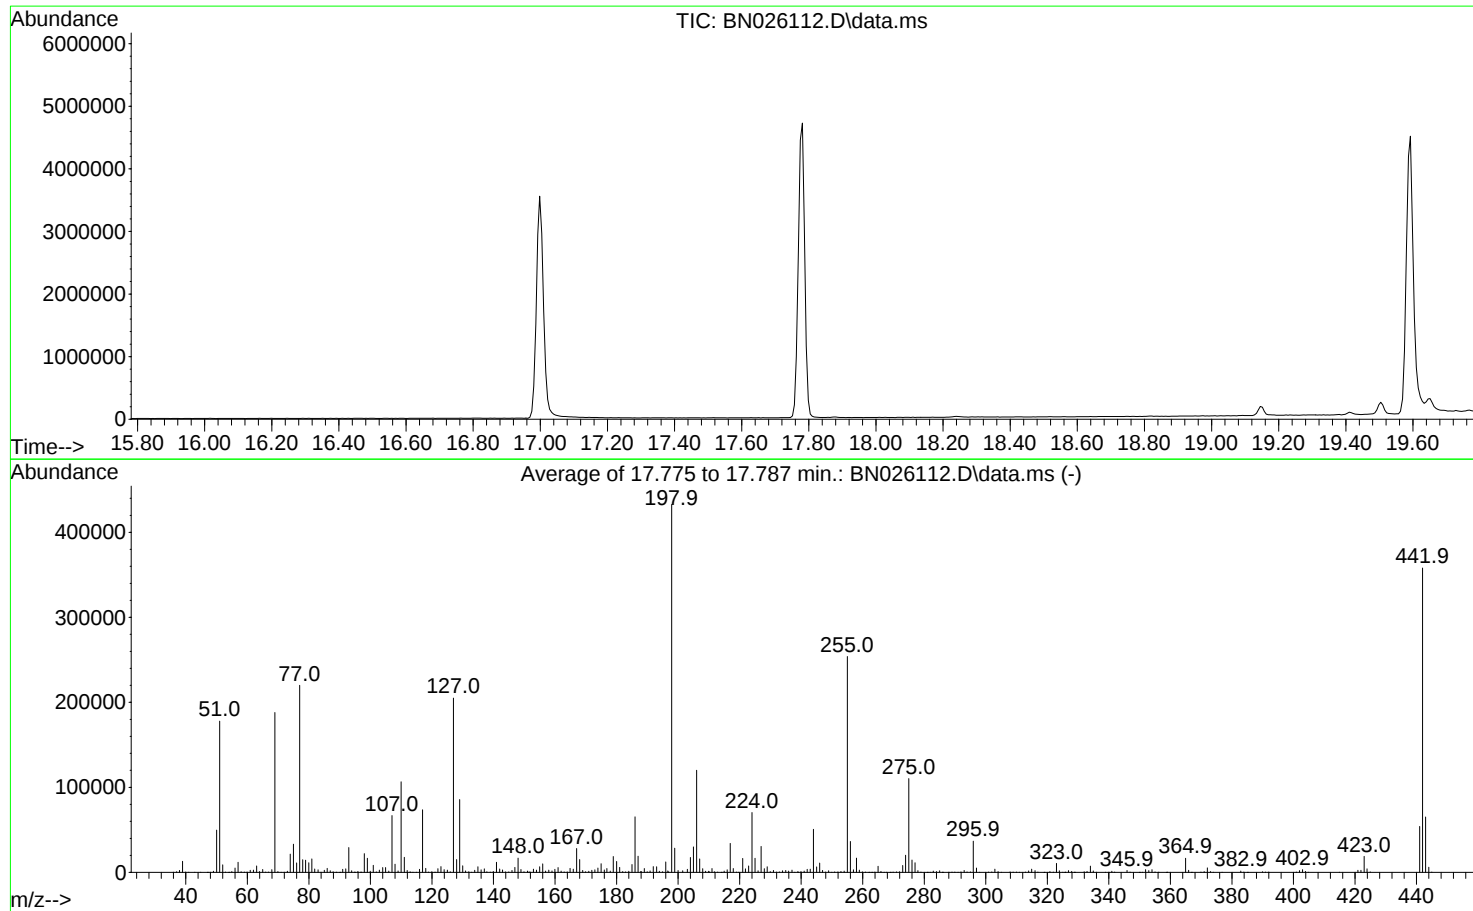

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	177887	PASS
68	69	0.00	2	1.7	3182	PASS
69	198	0.00	100	43.4	187952	PASS
70	69	0.00	2	0.5	995	PASS
127	198	10	80	47.4	204992	PASS
197	198	0.00	2	0.1	473	PASS
198	198	100	100	100.0	432725	PASS
199	198	5	9	6.6	28429	PASS
275	198	10	60	25.5	110288	PASS
365	198	1	100	3.8	16554	PASS
441	198	0.01	100	12.5	53947	PASS
442	442	50	100	100.0	357931	PASS
443	442	15	24	18.2	65115	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/30/2023	BNA_N	<u>BN026112.D</u>
Compound Name	Response	Retention Time
DDT	1265757	20.816
DDD	187899	20.38
DDE	2425	19.869
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
190324	1456081	13.07

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063023\
Data File : BN026112.D
Acq On : 30 Jun 2023 03:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 30 08:14:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 08:14:10 2023
Response via : Initial Calibration

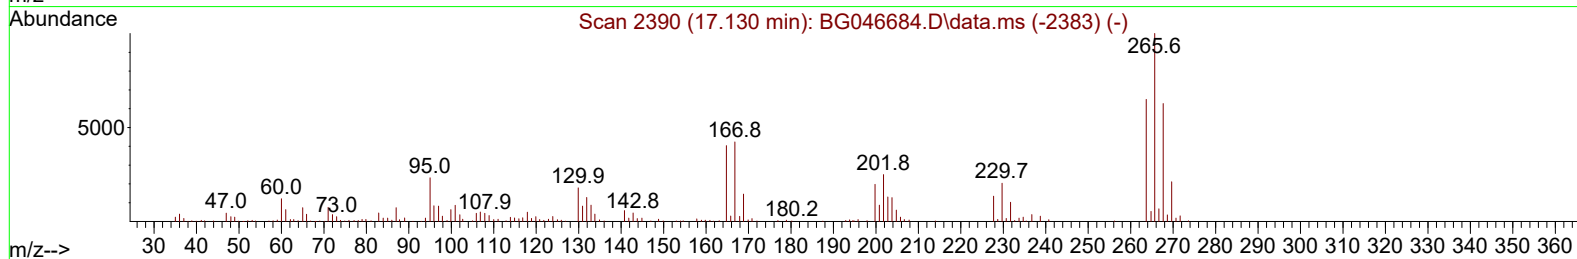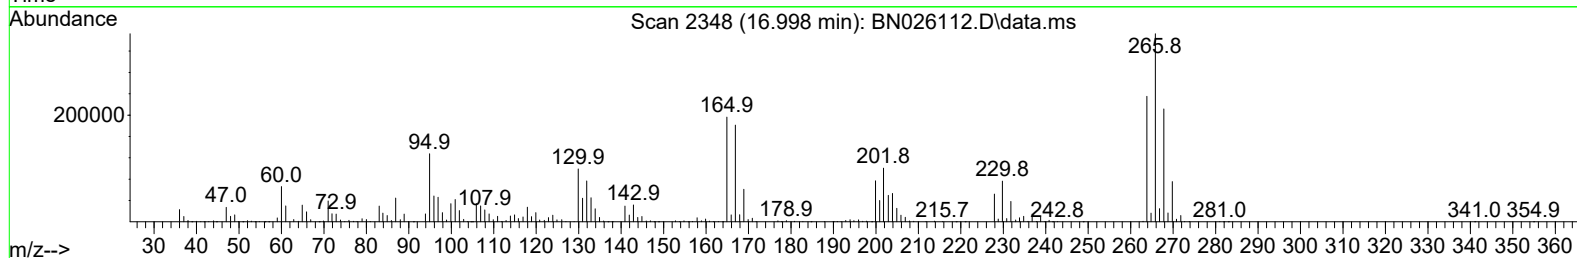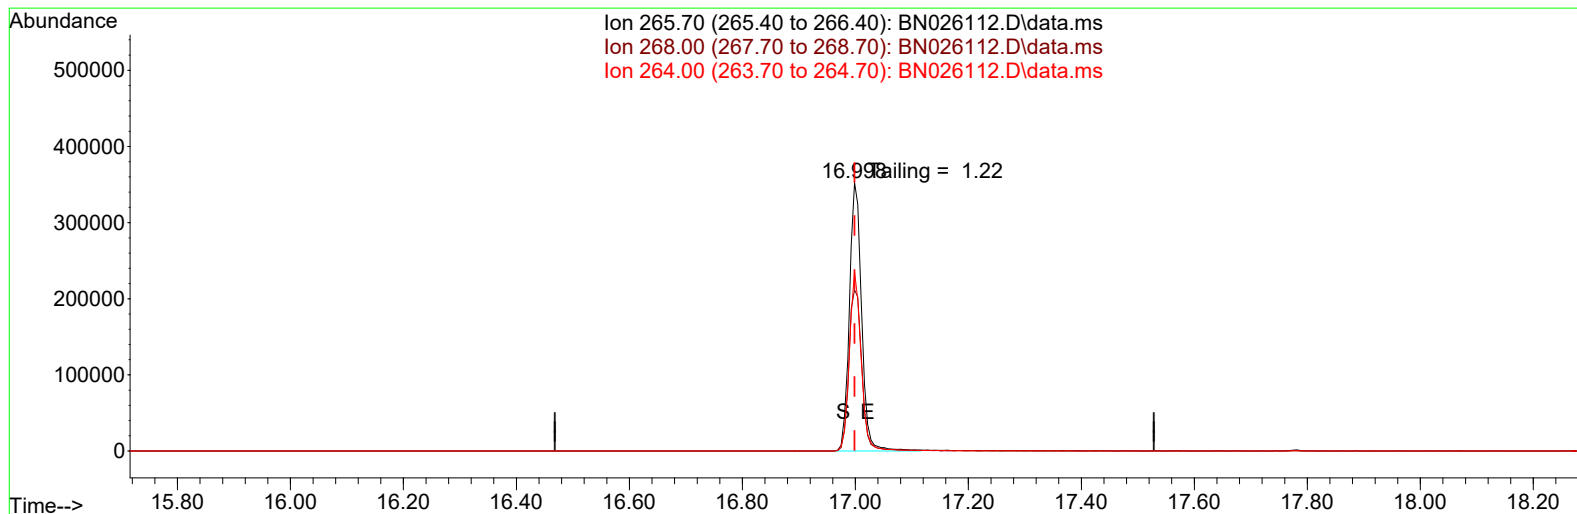

TIC: BN026112.D\data.ms

(70) Pentachlorophenol (C)

16.998min (0.000) 23154.49 ng




response 533684

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.06
264.00	61.60	66.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063023\
Data File : BN026112.D
Acq On : 30 Jun 2023 03:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 30 08:14:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 08:14:10 2023
Response via : Initial Calibration

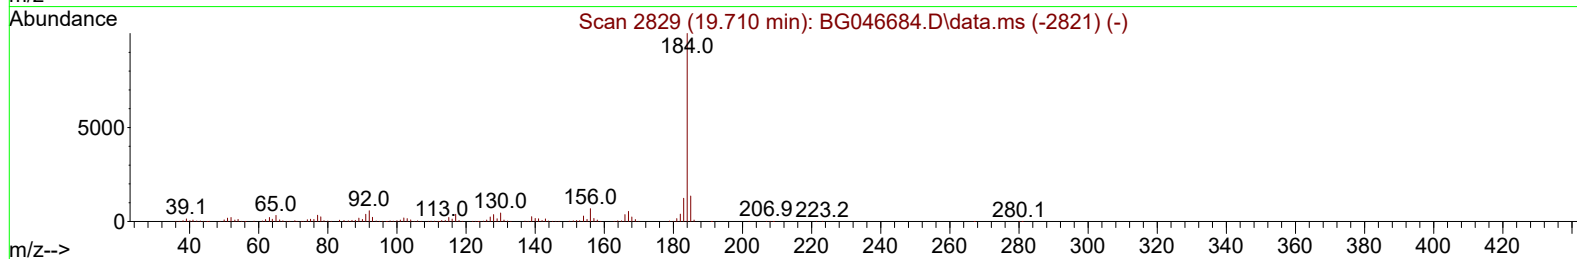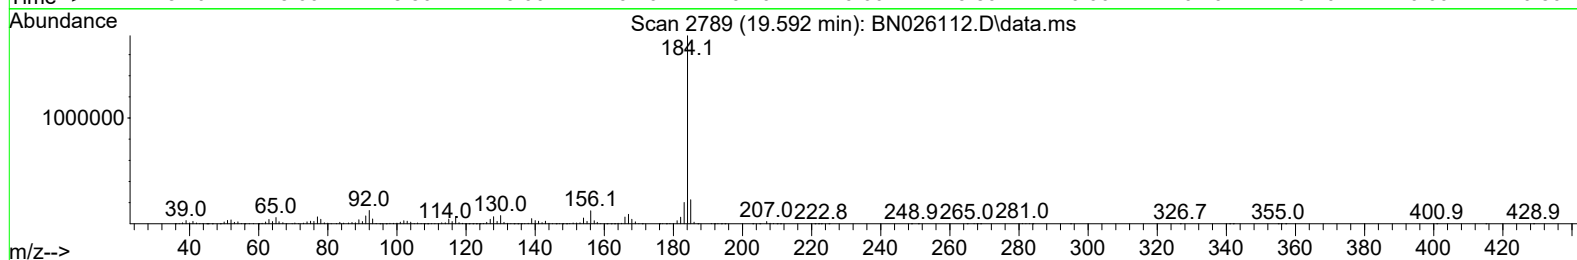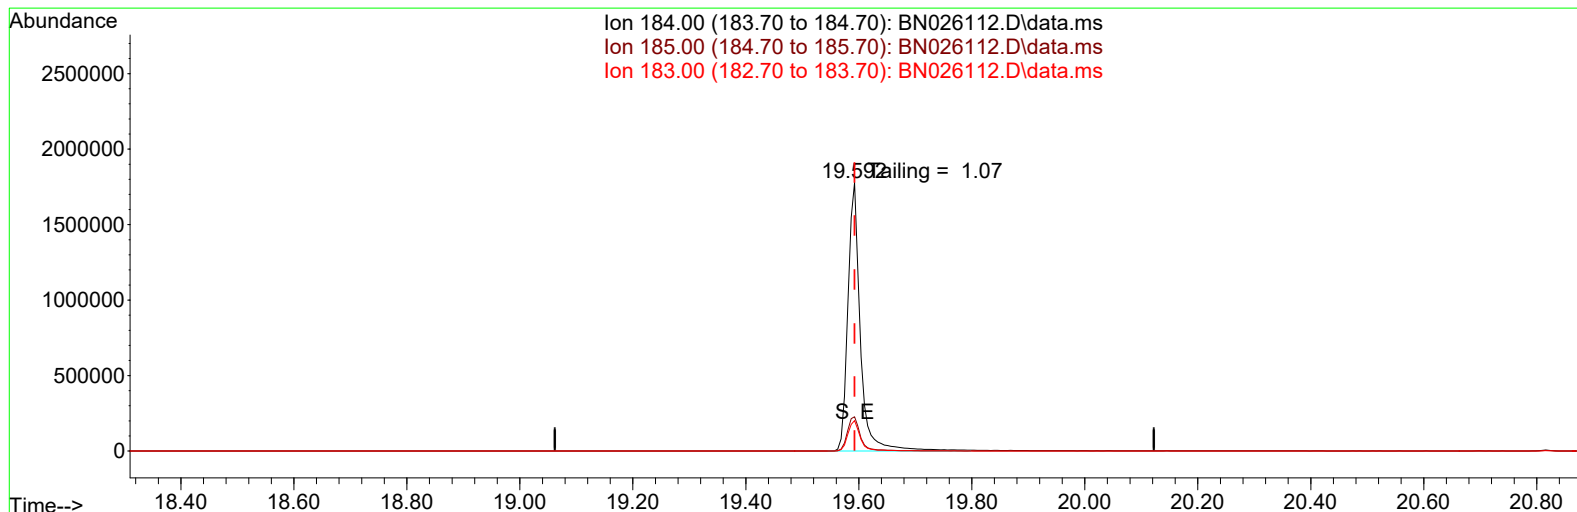

TIC: BN026112.D\data.ms

(77) Benzidine**19.592min (0.000) 1537378.33 ng****response 2748635**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.80
183.00	13.20	11.36
0.00	0.00	0.00