
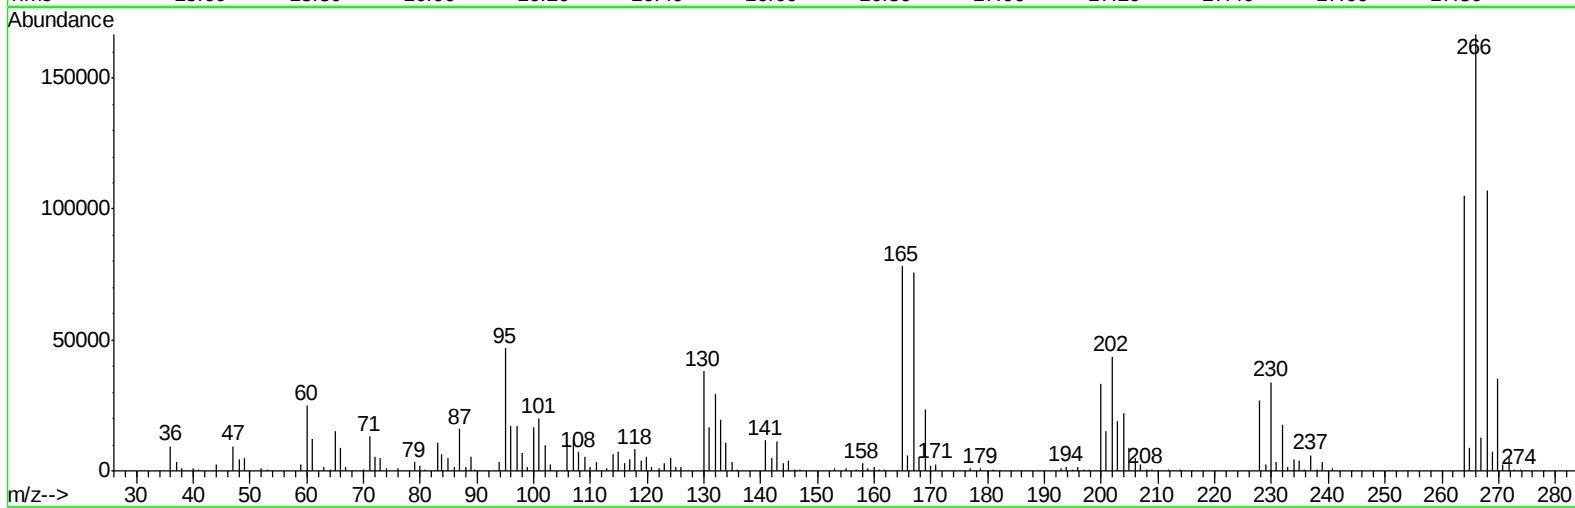


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070119\
Data File : BN006669.D
Acq On : 01 Jul 2019 20:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:44:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

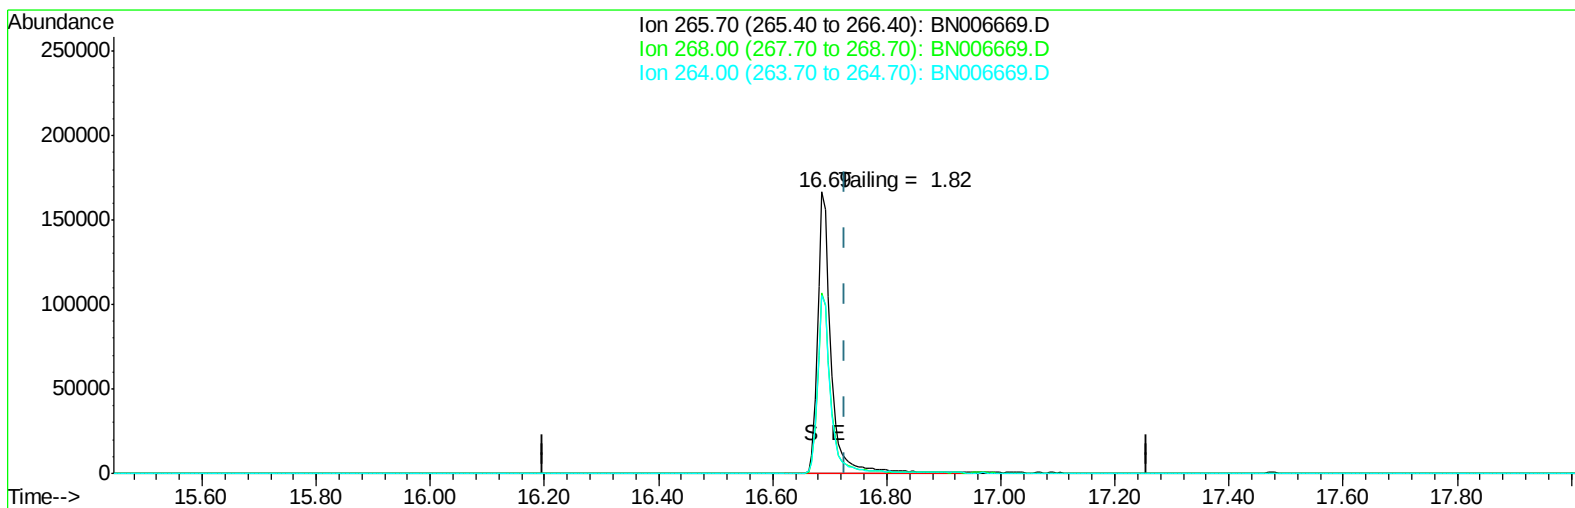

TIC: BN006669.D

(70) Pentachlorophenol (C)



16.686min (-0.041) 22995.77ng

response 271689

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	64.24
264.00	62.50	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070119\
Data File : BN006669.D
Acq On : 01 Jul 2019 20:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:44:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

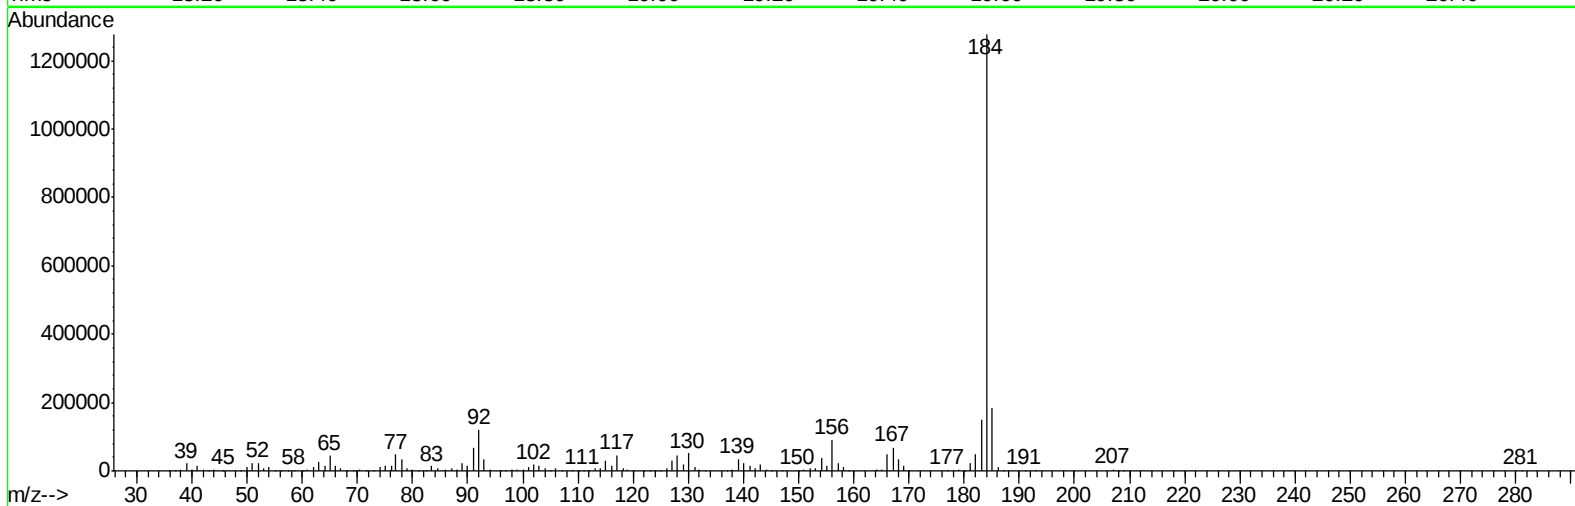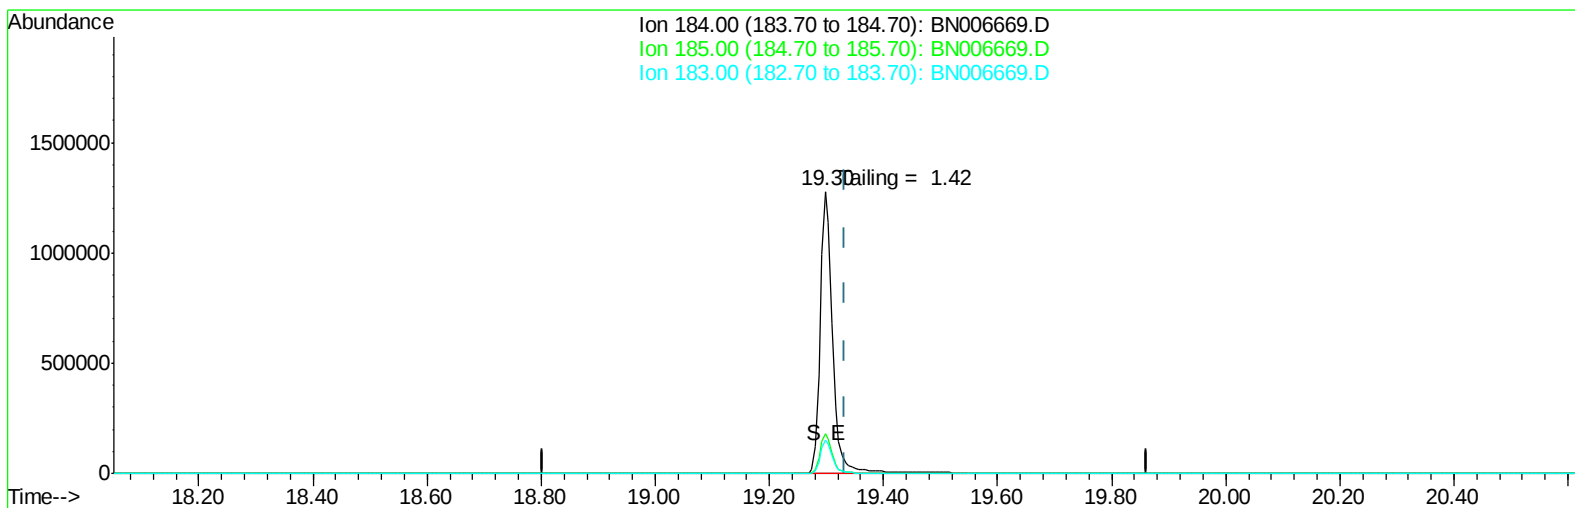

TIC: BN006669.D

(77) Benzidine

19.298min (-0.035) 0.00ng

response 1964546

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.32
183.00	12.40	11.76
0.00	0.00	0.00