


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070119\
Data File : BN006669.D
Acq On : 01 Jul 2019 20:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 28 13:47:56 2019

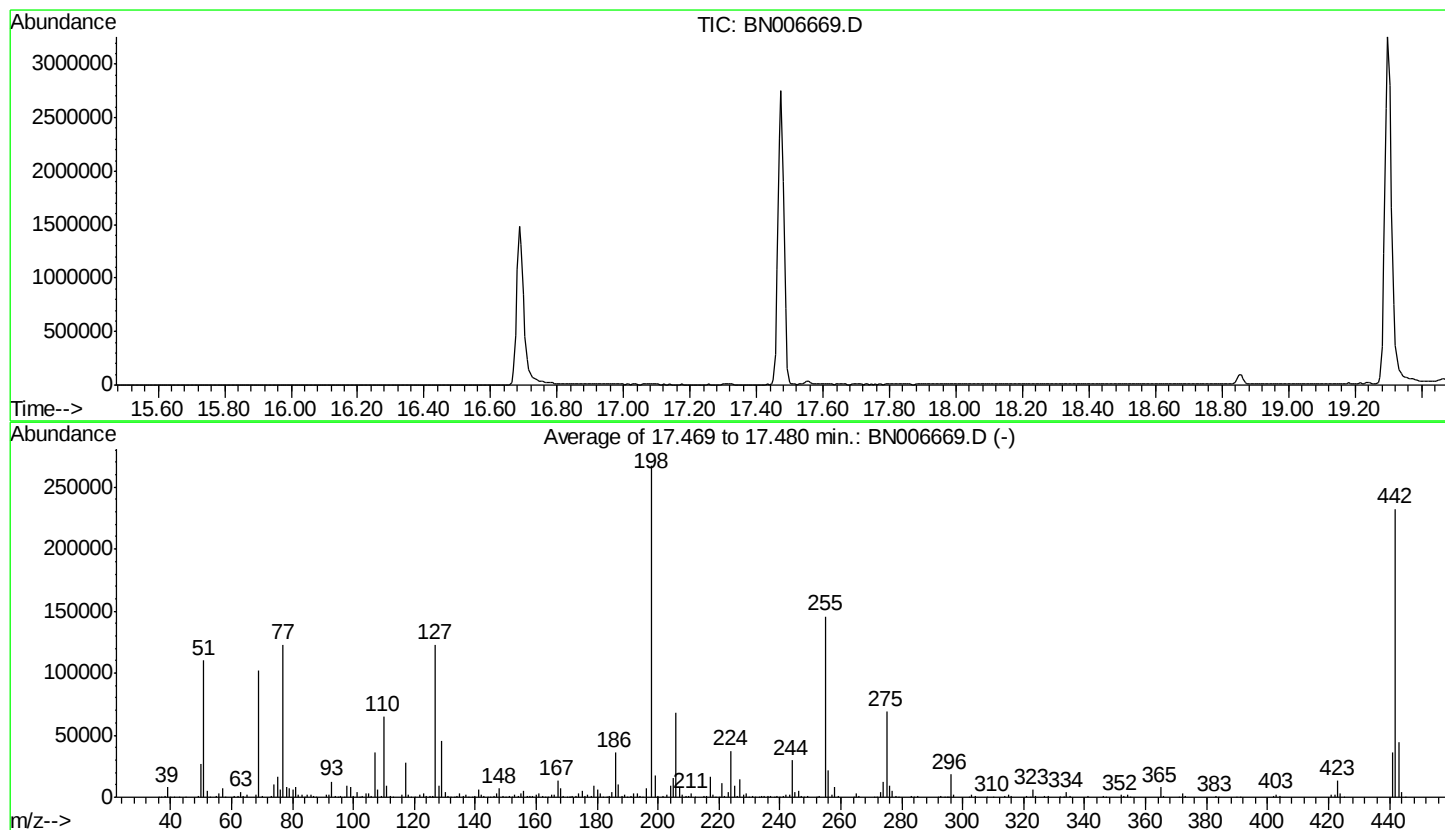

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	110232	PASS
68	69	0.00	2	1.8	1825	PASS
69	198	0.00	100	38.3	102418	PASS
70	69	0.00	2	0.6	570	PASS
127	198	10	80	46.1	123117	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	267200	PASS
199	198	5	9	6.8	18086	PASS
275	198	10	60	25.7	68661	PASS
365	198	1	100	3.1	8247	PASS
441	198	0.01	100	13.5	36136	PASS
442	198	50	100	87.0	232362	PASS
443	442	15	24	19.2	44512	PASS