

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070123\
 Data File : BN026121.D
 Acq On : 30 Jun 2023 09:05
 Operator : MA/JU
 Sample : PB153575BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK575

Quant Time: Jul 01 00:54:04 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 22:47:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.959	152	8949	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.770	136	30405	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.603	164	18316	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.347	188	35139	0.400	ng/ul	-0.01
17) Chrysene-d12	21.547	240	16972	0.400	ng/ul	0.00
23) Perylene-d12	23.993	264	21761	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	43666	4.333	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.365	152	11692	0.250	ng/ul	0.00
18) Fluoranthene-d10	19.377	212	19992	0.309	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.740	202	3215	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.832	252	5389	0.067	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070123\
Data File : BN026121.D
Acq On : 30 Jun 2023 09:05
Operator : MA/JU
Sample : PB153575BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK575

Quant Time: Jul 01 00:54:04 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 22:47:20 2023
Response via : Initial Calibration

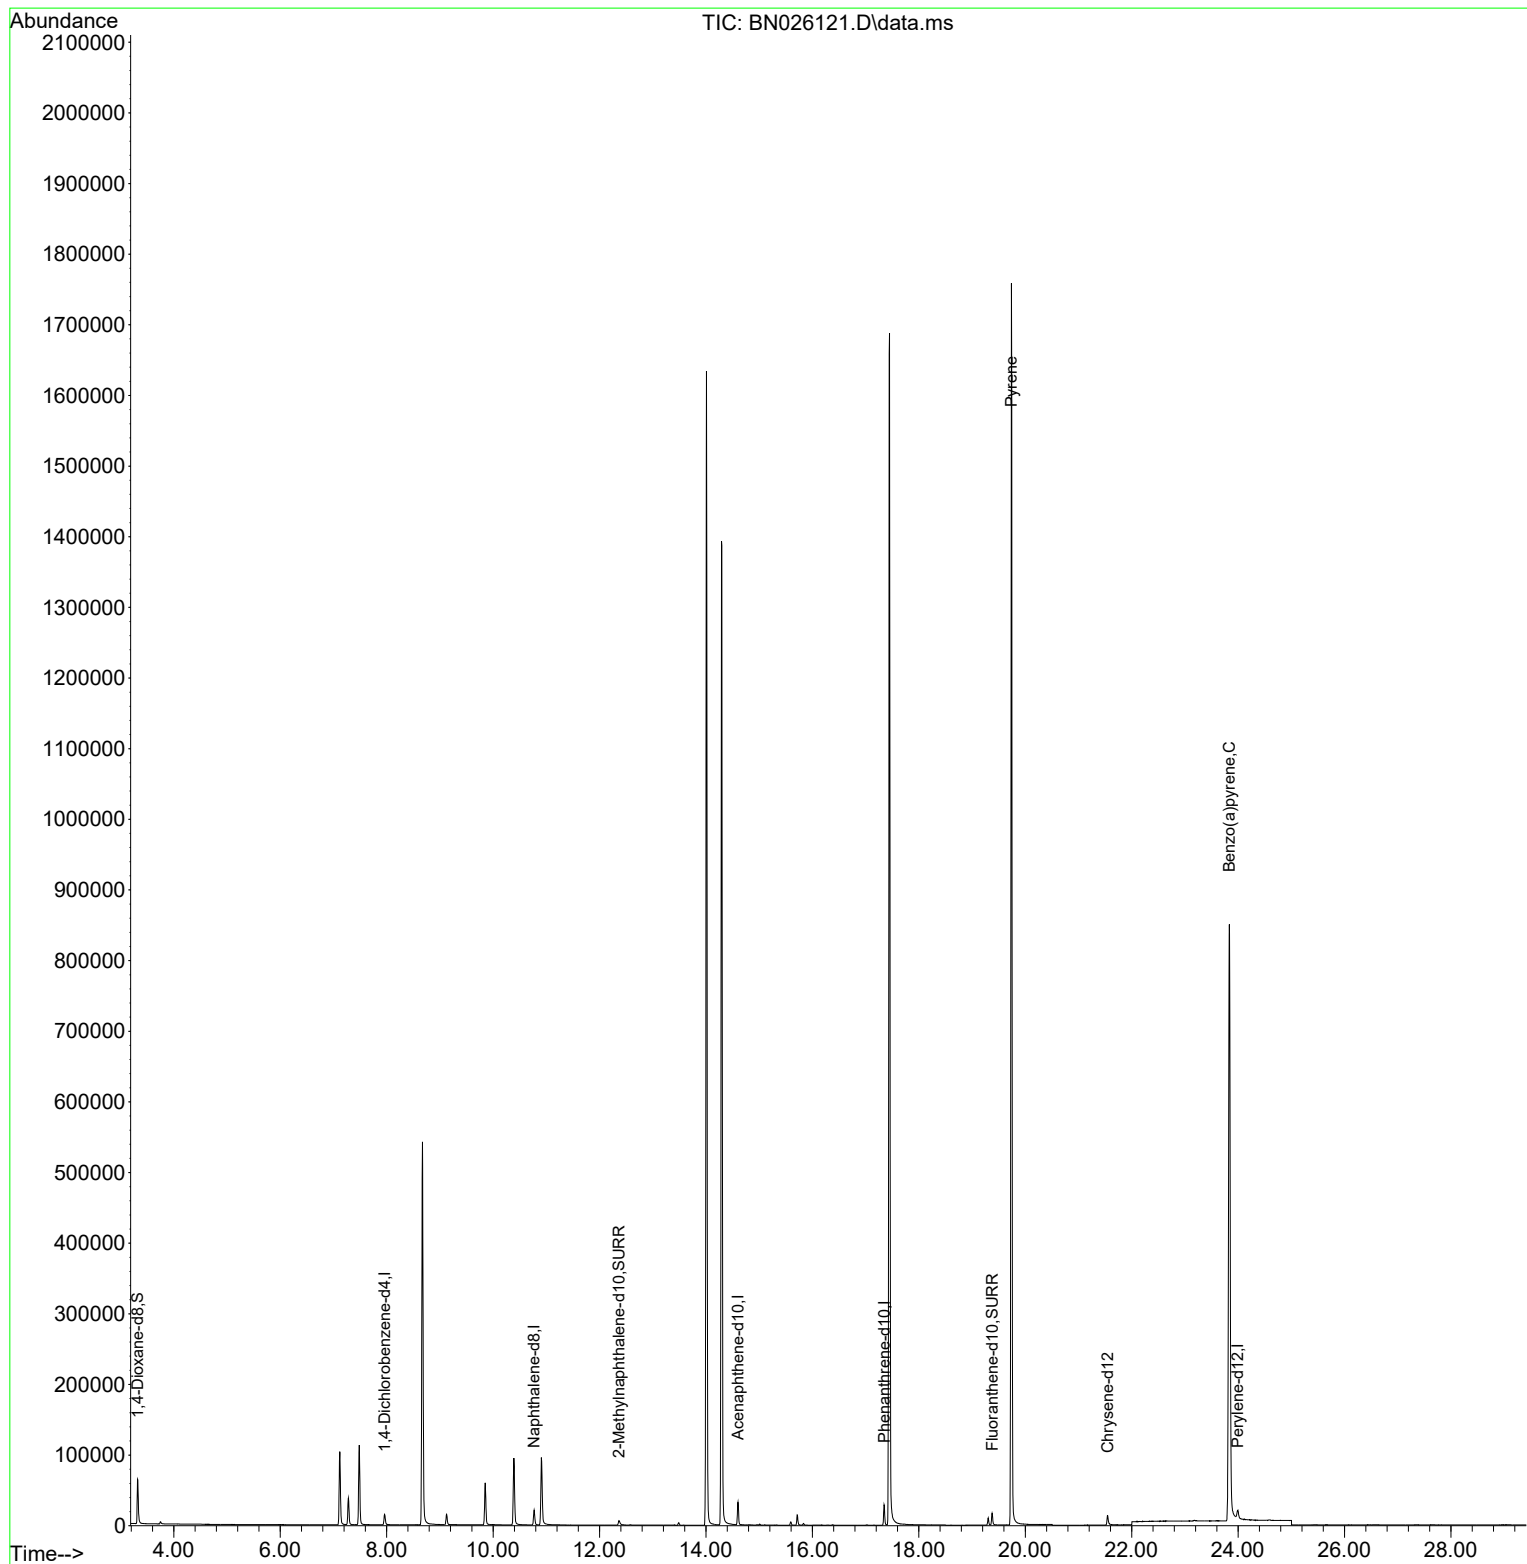

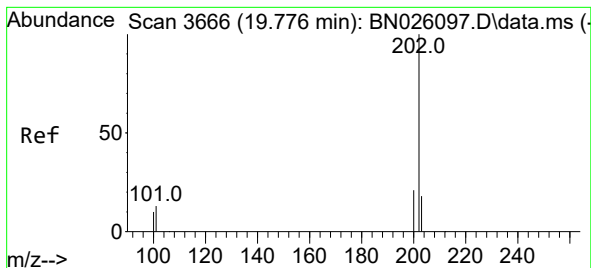

#20

Pyrene

Concen: 0.034 ng/ul

RT: 19.740 min Scan# 3

Delta R.T. -0.037 min

Lab File: BN026121.D

Acq: 30 Jun 2023 09:05

Instrument :

BNA_N

ClientSampleId :

SBLK575





Tgt Ion:202 Resp: 3215

Ion Ratio Lower Upper

202 100

101 182.3 11.4 17.0#

100 1416.8 9.1 13.7#

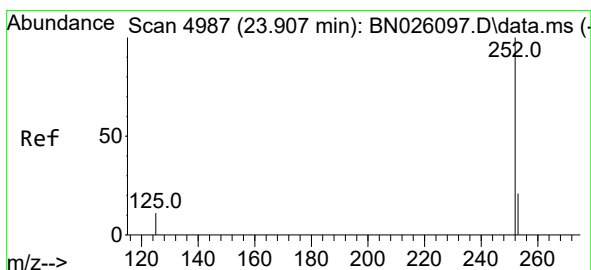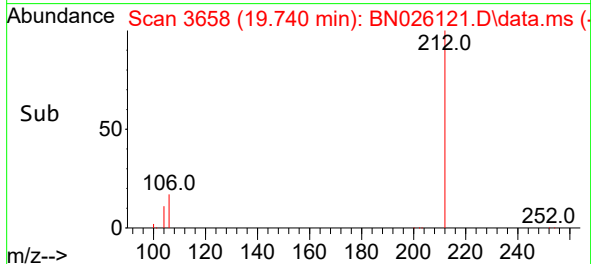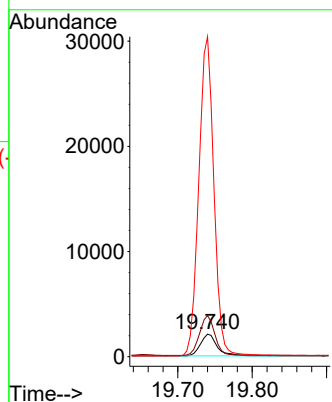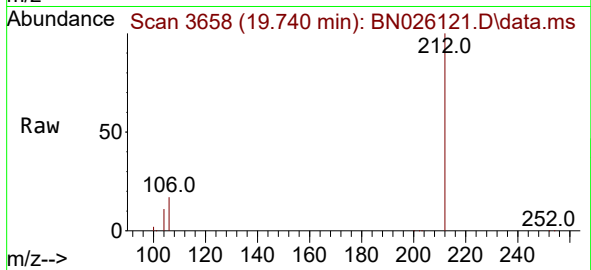

#26

Benzo(a)pyrene

Concen: 0.067 ng/ul

RT: 23.832 min Scan# 4961

Delta R.T. -0.073 min

Lab File: BN026121.D

Acq: 30 Jun 2023 09:05

Tgt Ion:252 Resp: 5389

Ion Ratio Lower Upper

252 100

253 56.4 26.0 39.0#

125 55.2 17.3 25.9#

