

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070123\
 Data File : BN026136.D
 Acq On : 30 Jun 2023 18:56
 Operator : MA/JU
 Sample : PB153636BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK636

Quant Time: Jul 01 01:47:43 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 01:46:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	9089	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	30454	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.602	164	17923	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.351	188	34422	0.400	ng/ul	0.00
17) Chrysene-d12	21.540	240	17638	0.400	ng/ul	0.00
23) Perylene-d12	24.004	264	20223	0.400	ng/ul	# 0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	40298	3.937	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.369	152	10590	0.226	ng/ul	0.00
18) Fluoranthene-d10	19.381	212	17599	0.262	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.597	166	3726	0.047	ng/ul#	13
20) Pyrene	19.744	202	2880	0.029	ng/ul#	1
26) Benzo(a)pyrene	23.852	252	4967	0.066	ng/ul#	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070123\
Data File : BN026136.D
Acq On : 30 Jun 2023 18:56
Operator : MA/JU
Sample : PB153636BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK636

Quant Time: Jul 01 01:47:43 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 01:46:24 2023
Response via : Initial Calibration




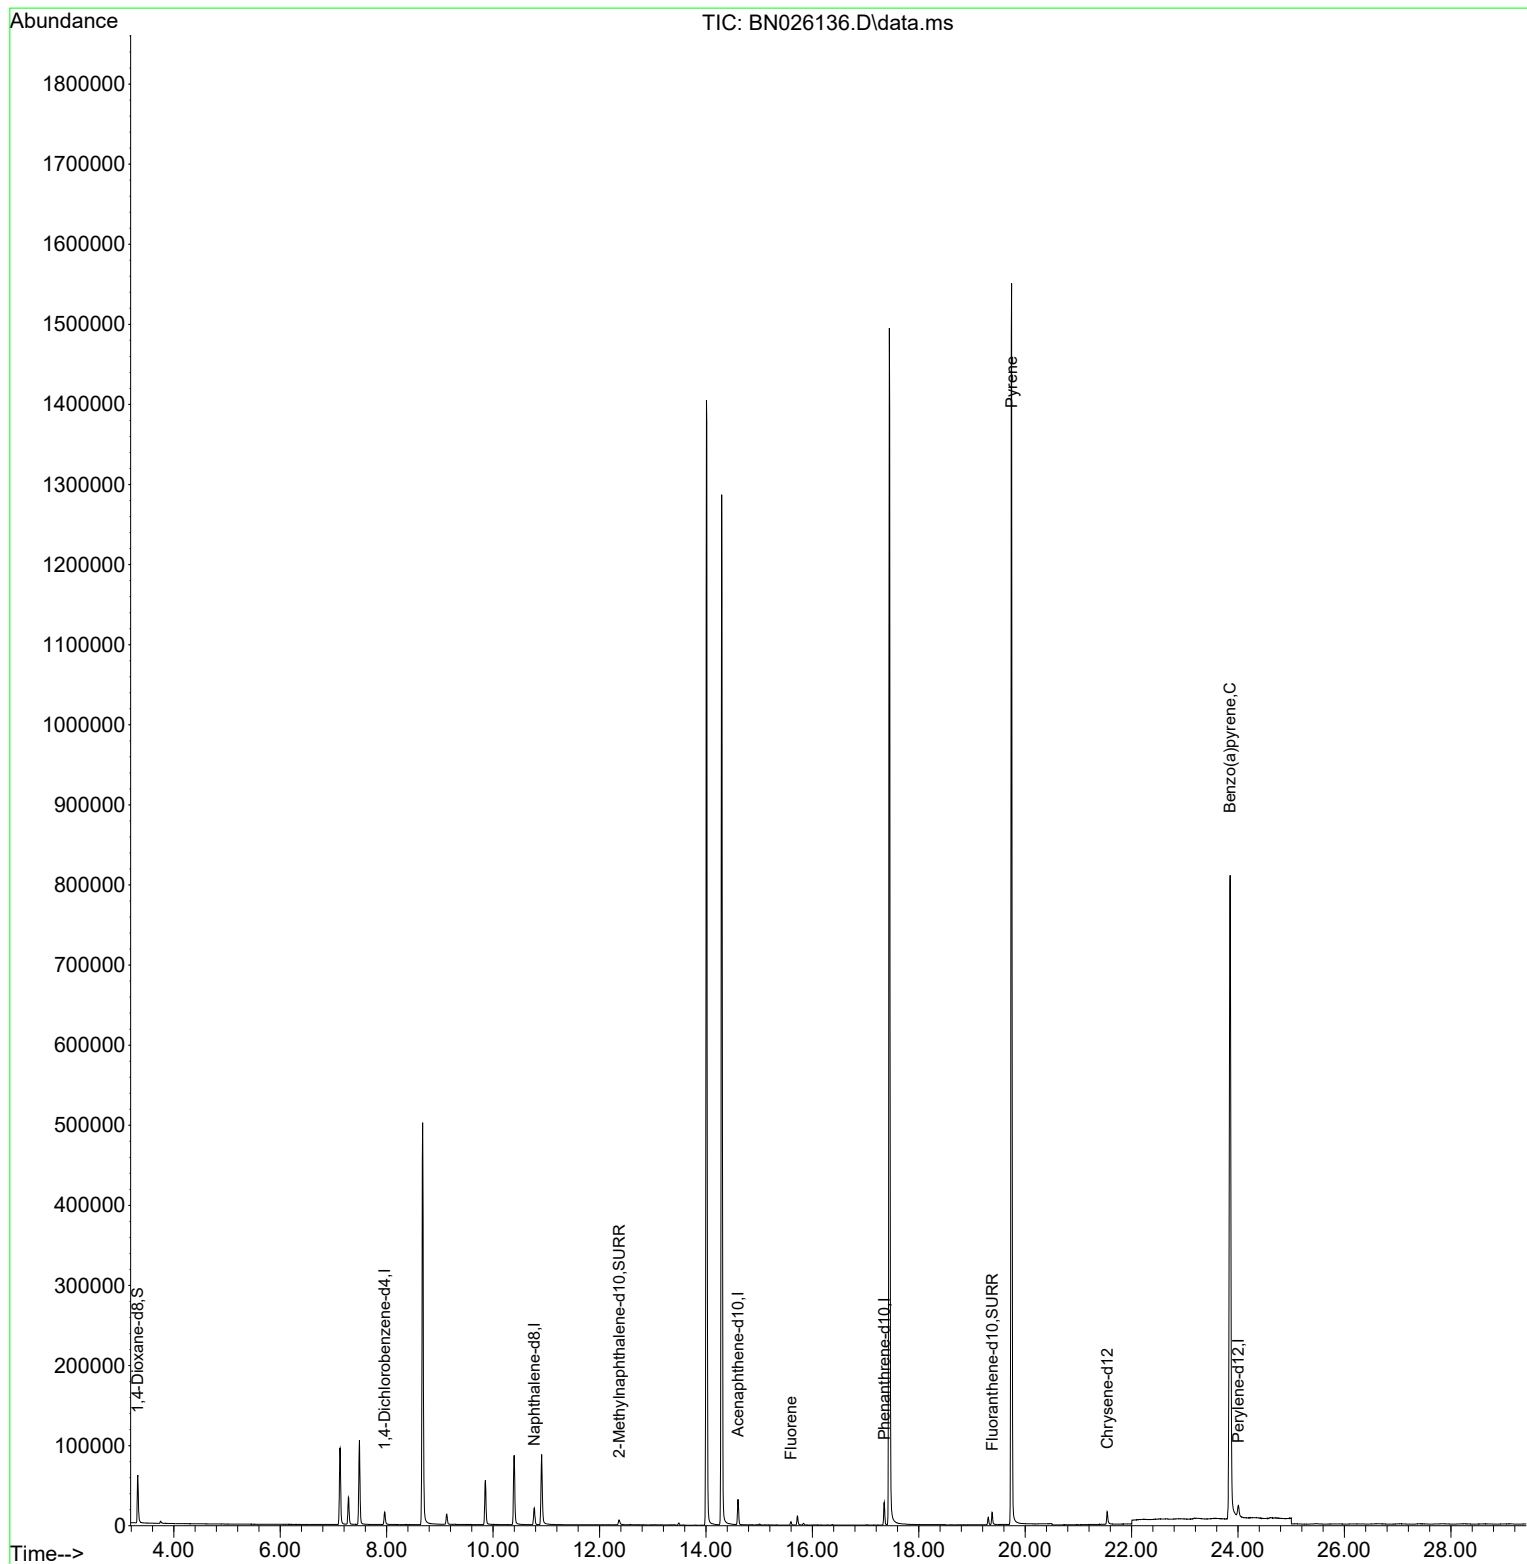


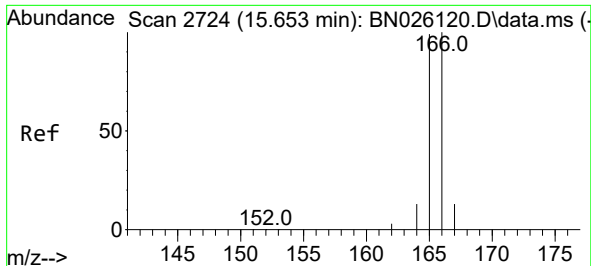

#12
Fluorene
Concen: 0.047 ng/ul
RT: 15.597 min Scan# 21
Delta R.T. -0.057 min
Lab File: BN026136.D
Acq: 30 Jun 2023 18:56




Instrument :
BNA_N
ClientSampleId :
SBLK636


Tgt Ion:166 Resp: 3726
Ion Ratio Lower Upper
166 100
165 8.7 79.9 119.9#
167 34.5 10.8 16.2#

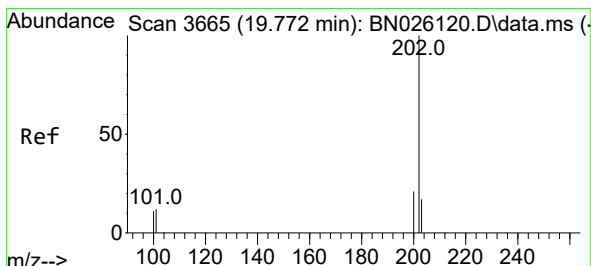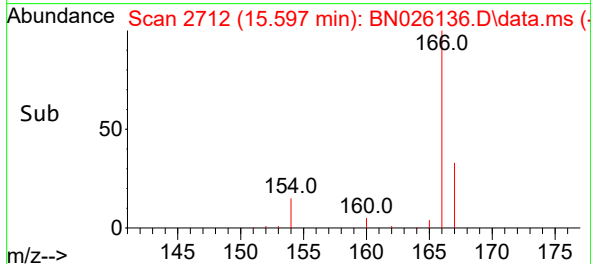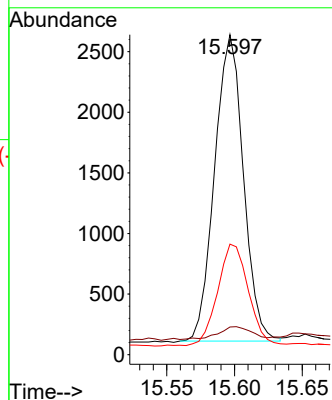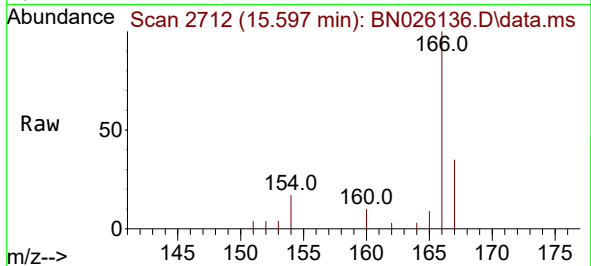

#20
Pyrene
Concen: 0.029 ng/ul
RT: 19.744 min Scan# 3659
Delta R.T. -0.030 min
Lab File: BN026136.D
Acq: 30 Jun 2023 18:56


Tgt Ion:202 Resp: 2880
Ion Ratio Lower Upper
202 100
101 170.6 11.4 17.0#
100 1255.9 9.1 13.7#

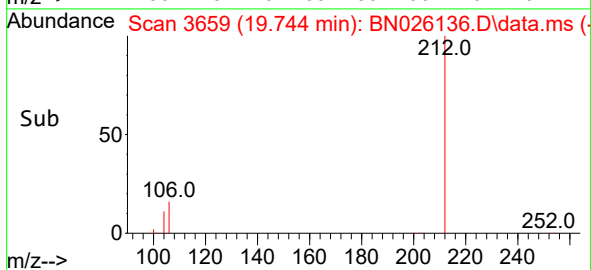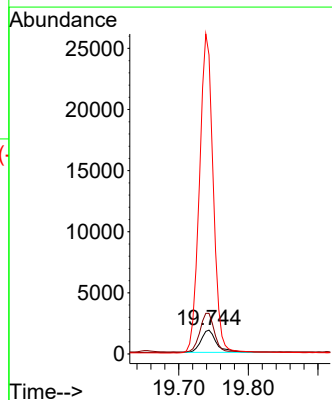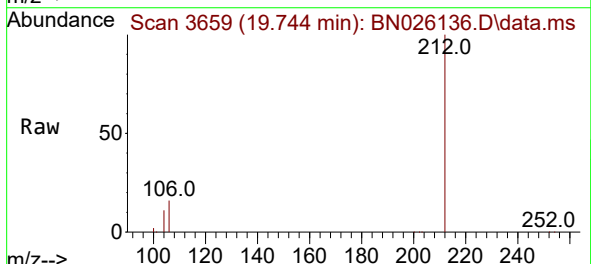

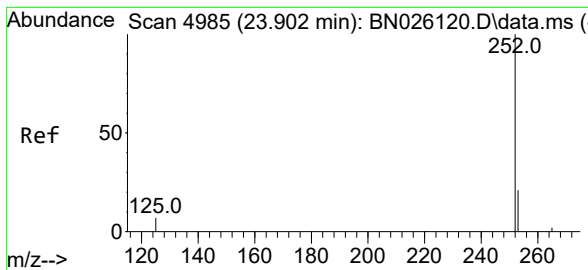

#26
Benzo(a)pyrene
Concen: 0.066 ng/ul
RT: 23.852 min Scan# 4968
Delta R.T. -0.034 min
Lab File: BN026136.D
Acq: 30 Jun 2023 18:56

Instrument :
BNA_N
ClientSampleId :
SBLK636

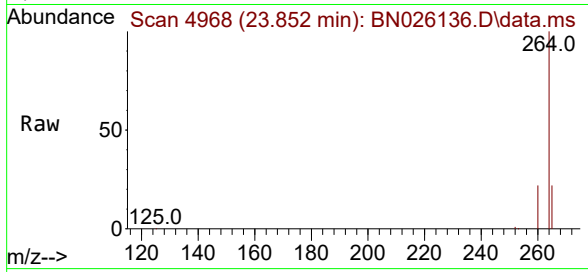

Tgt Ion:252	Resp:	4967
Ion	Ratio	Lower Upper
252	100	
253	66.8	26.0 39.0#
125	68.0	17.3 25.9#

