

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070123\
 Data File : BN026126.D
 Acq On : 30 Jun 2023 12:06
 Operator : MA/JU
 Sample : 03239-14
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCFZ2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/01/2023
 Supervised By :mohammad ahmed 07/01/2023

Quant Time: Jul 01 00:54:51 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 22:47:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.959	152	11235	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.770	136	35543	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.603	164	21013	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.347	188	41589	0.400	ng/ul	-0.01
17) Chrysene-d12	21.538	240	21498	0.400	ng/ul	0.00
23) Perylene-d12	23.996	264	28799	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	19955	1.577	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.360	152	6158	0.113	ng/ul	-0.01
18) Fluoranthene-d10	19.377	212	10688	0.131	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.820	128	71424	0.701	ng/ul	100
7) 2-Methylnaphthalene	12.431	142	23230	0.358	ng/ul	99
8) 1-Methylnaphthalene	12.651	142	18370	0.273	ng/ul	100
10) Acenaphthylene	14.325	152	134628	1.368	ng/ul	99
11) Acenaphthene	14.663	153	67601	0.840	ng/ul	100
12) Fluorene	15.648	166	63659	0.690	ng/ul	99
15) Phenanthrene	17.389	178	1512856	11.013	ng/ul	100
16) Anthracene	17.482	178	299517	2.453	ng/ul	100
19) Fluoranthene	19.410	202	3558564	30.991	ng/ul	97
20) Pyrene	19.772	202	2871988	24.047	ng/ul	95
21) Benzo(a)anthracene	21.523	228	1466173	16.532	ng/ul	98
22) Chrysene	21.576	228	1616510	17.517	ng/ul	97
24) Benzo(b)fluoranthene	23.253	252	2744501m	22.328	ng/ul	
25) Benzo(k)fluoranthene	23.294	252	1007354m	8.161	ng/ul	
26) Benzo(a)pyrene	23.891	252	1895581	17.756	ng/ul#	82
27) Indeno(1,2,3-cd)pyrene	26.568	276	1580804	13.556	ng/ul#	85
28) Dibenzo(a,h)anthracene	26.574	278	386134	4.375	ng/ul	91
29) Benzo(g,h,i)perylene	27.359	276	1551318	14.955	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070123\
Data File : BN026126.D
Acq On : 30 Jun 2023 12:06
Operator : MA/JU
Sample : 03239-14
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCFZ2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023


Quant Time: Jul 01 00:54:51 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 22:47:20 2023
Response via : Initial Calibration

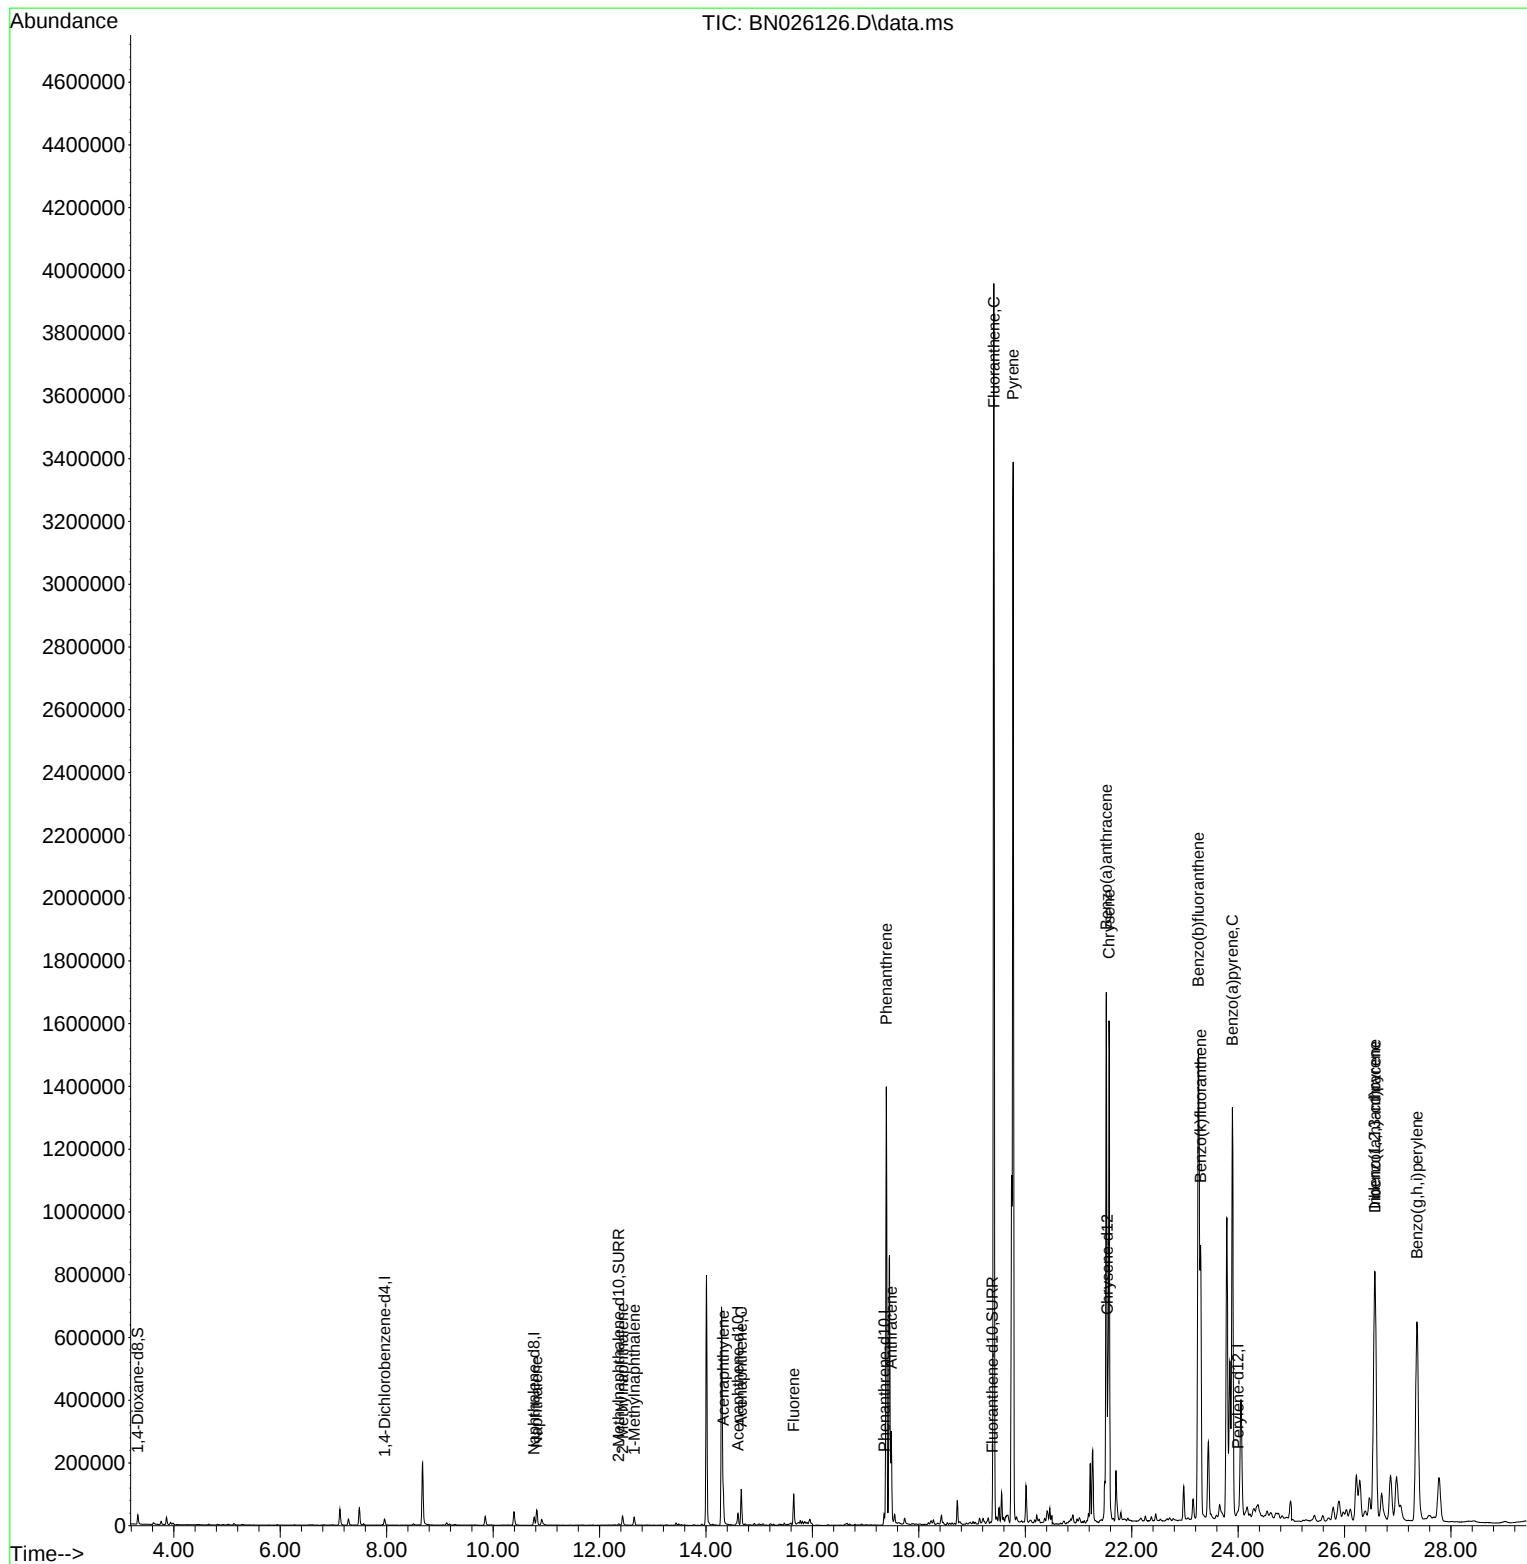



#5
Naphthalene
Concen: 0.701 ng/ul
RT: 10.820 min Scan# 1769
Delta R.T. -0.016 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06




Instrument :
BNA_N
ClientSampleId :
DCFZ2




Tgt Ion:128 Resp: 71424
Ion Ratio Lower Upper
128 100
129 11.6 9.1 13.7
127 13.3 10.7 16.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

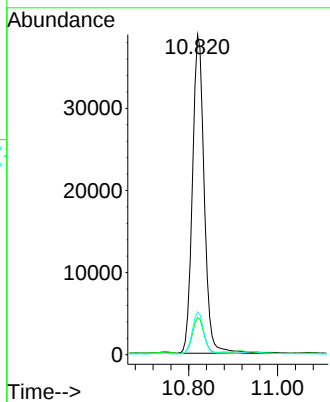


#7
2-Methylnaphthalene
Concen: 0.358 ng/ul
RT: 12.431 min Scan# 2061
Delta R.T. -0.016 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06

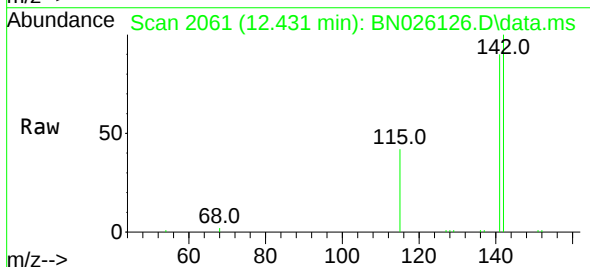

Tgt Ion:142 Resp: 23230
Ion Ratio Lower Upper
142 100
141 88.6 71.9 107.9

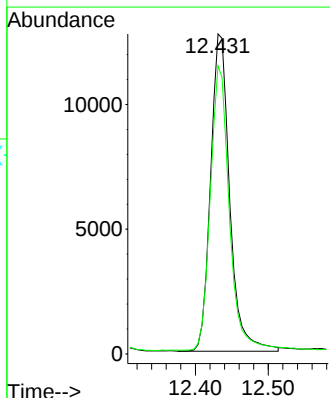

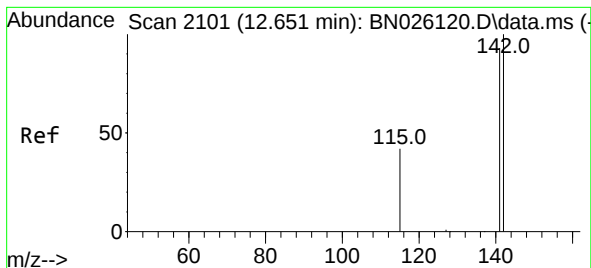

#8

1-Methylnaphthalene

Concen: 0.273 ng/ul

RT: 12.651 min Scan# 2101

Delta R.T. -0.011 min

Lab File: BN026126.D


Acq: 30 Jun 2023 12:06

Instrument :

BNA_N

ClientSampleId :

DCFZ2

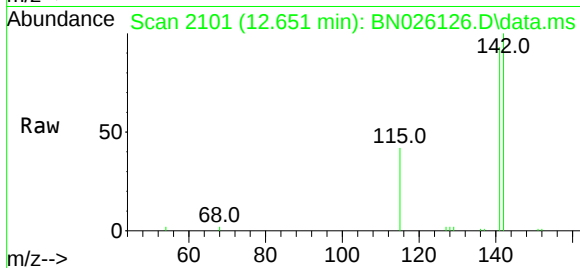

Tgt Ion:142 Resp: 18370

Ion Ratio Lower Upper

142 100



141 92.5 74.2 111.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/01/2023

Supervised By :mohammad ahmed 07/01/2023

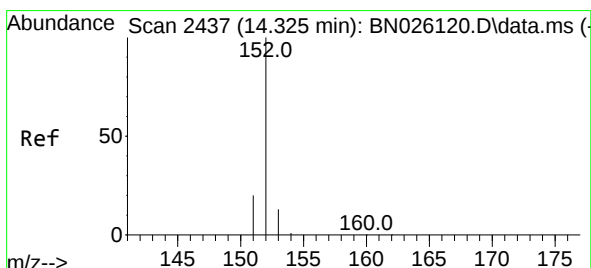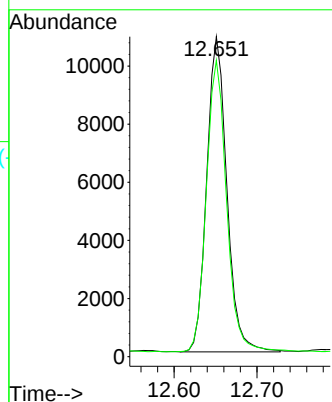

#10

Acenaphthylene

Concen: 1.368 ng/ul

RT: 14.325 min Scan# 2437

Delta R.T. -0.004 min

Lab File: BN026126.D

Acq: 30 Jun 2023 12:06




Tgt Ion:152 Resp: 134628


Ion Ratio Lower Upper

152 100

151 19.6 16.2 24.4


153 13.6 10.9 16.3

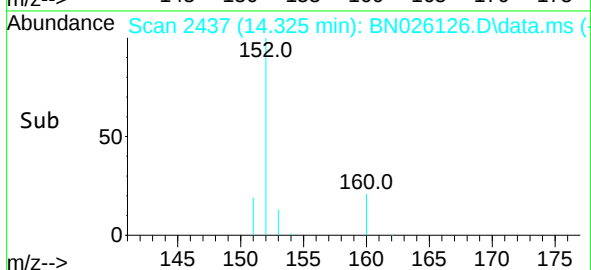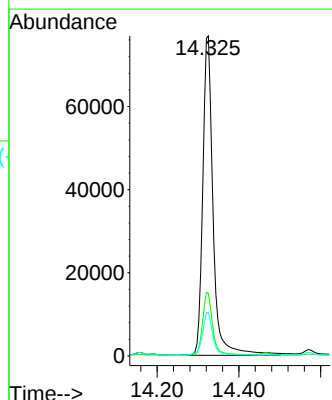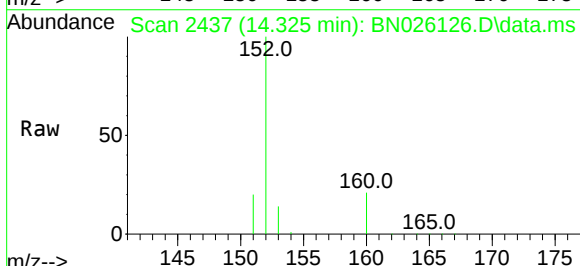



#11
Acenaphthene
Concen: 0.840 ng/u1
RT: 14.663 min Scan# 2510
Delta R.T. -0.009 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06




Instrument :
BNA_N
ClientSampleId :
DCFZ2




Tgt Ion:153 Resp: 6760
Ion Ratio Lower Upper
153 100
152 48.9 39.4 59.0
154 86.5 68.9 103.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

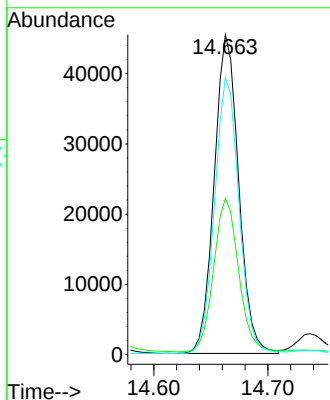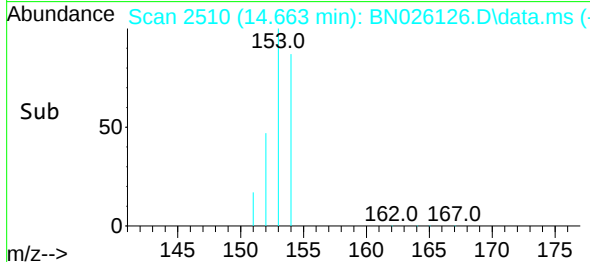


#12
Fluorene
Concen: 0.690 ng/u1
RT: 15.648 min Scan# 2723
Delta R.T. -0.014 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06

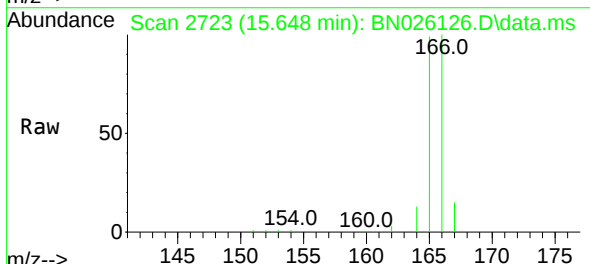


Tgt Ion:166 Resp: 63659
Ion Ratio Lower Upper
166 100
165 99.1 79.9 119.9
167 14.9 10.8 16.2

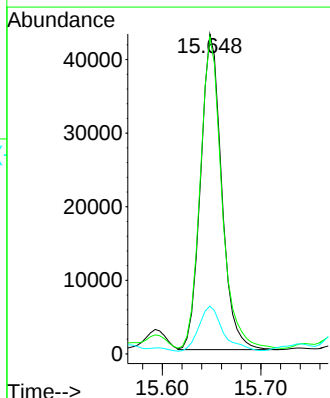



#15
Phenanthrene
Concen: 11.013 ng/u1
RT: 17.389 min Scan# 3128
Delta R.T. -0.013 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06




Instrument :
BNA_N
ClientSampleId :
DCFZ2



Tgt Ion:178 Resp: 1512850
Ion Ratio Lower Upper
178 100
179 15.6 12.6 19.0
176 19.6 15.8 23.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

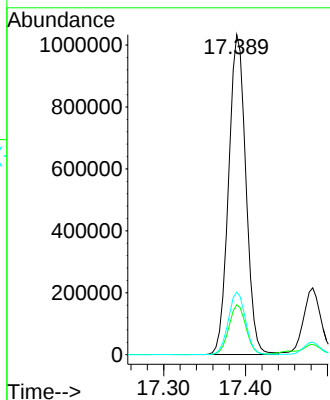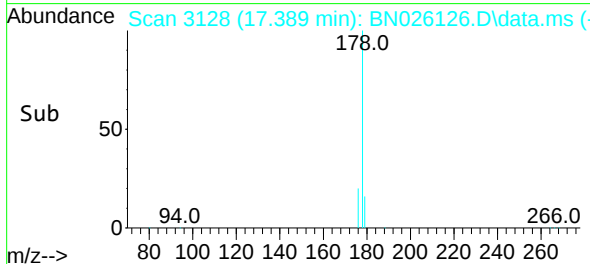

#16
Anthracene
Concen: 2.453 ng/u1
RT: 17.482 min Scan# 3150
Delta R.T. -0.013 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06


Tgt Ion:178 Resp: 299517
Ion Ratio Lower Upper
178 100
179 15.6 12.6 18.8
176 18.9 15.1 22.7

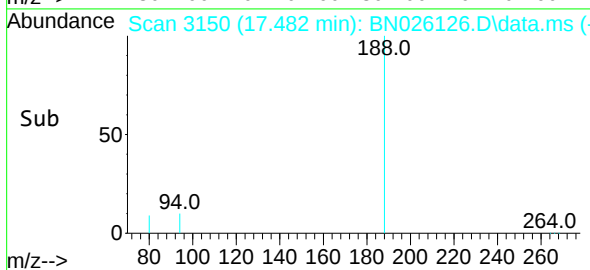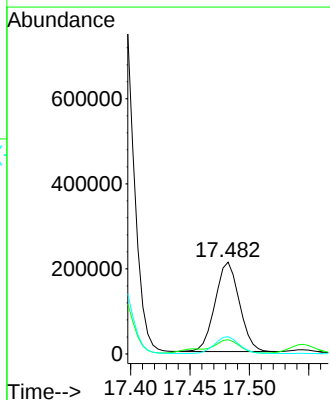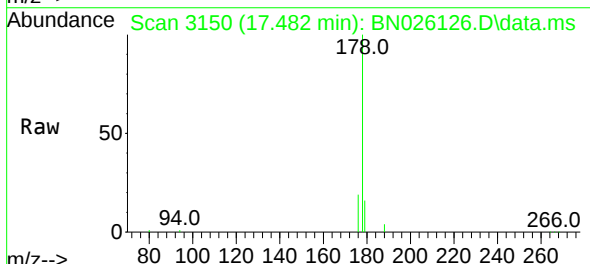



#19
Fluoranthene
Concen: 30.991 ng/u1
RT: 19.410 min Scan# 3587
Delta R.T. -0.005 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06




Instrument :
BNA_N
ClientSampleId :
DCFZ2



Tgt Ion:202 Resp: 3558564
Ion Ratio Lower Upper
202 100
101 10.5 9.5 14.3
100 8.0 7.3 10.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

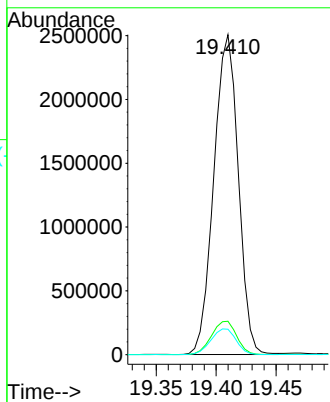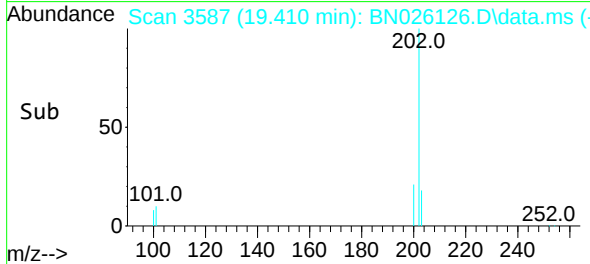

#20
Pyrene
Concen: 24.047 ng/u1
RT: 19.772 min Scan# 3665
Delta R.T. -0.005 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06


Tgt Ion:202 Resp: 2871988
Ion Ratio Lower Upper
202 100
101 12.1 11.4 17.0
100 9.8 9.1 13.7

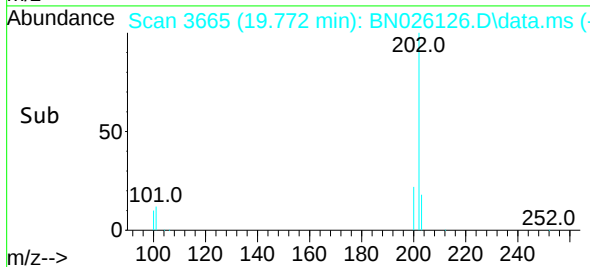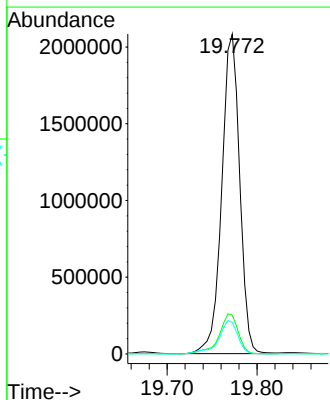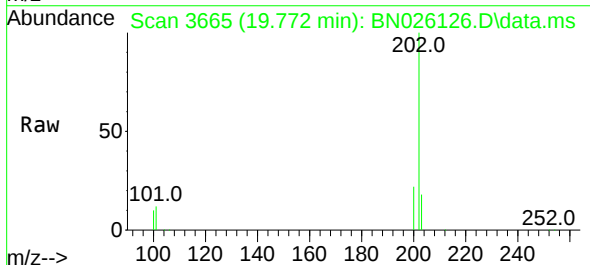



#21
Benzo(a)anthracene
Concen: 16.532 ng/u1
RT: 21.523 min Scan# 4171
Delta R.T. -0.006 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06




Instrument :
BNA_N
ClientSampleId :
DCFZ2



Tgt Ion:228 Resp: 146617
Ion Ratio Lower Upper
228 100
229 20.7 15.8 23.6
226 29.4 22.5 33.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

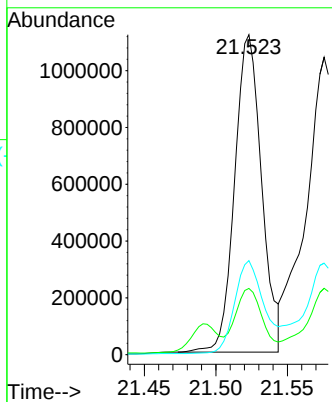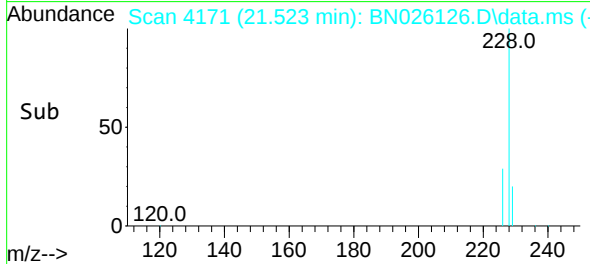

#22
Chrysene
Concen: 17.517 ng/u1
RT: 21.576 min Scan# 4189
Delta R.T. -0.003 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06


Tgt Ion:228 Resp: 1616510
Ion Ratio Lower Upper
228 100
226 30.8 24.8 37.2
229 22.3 15.7 23.5

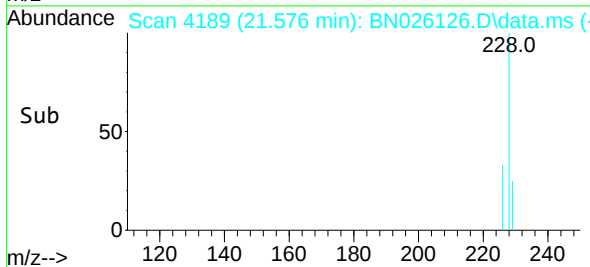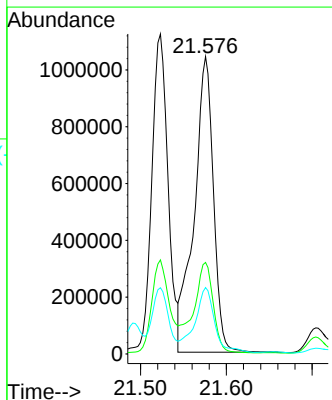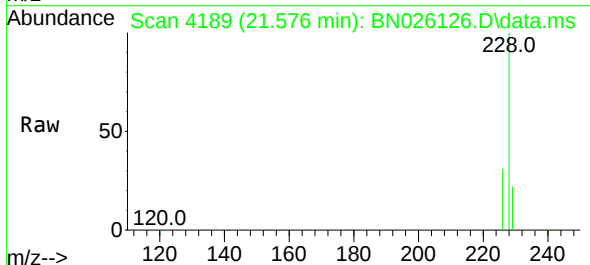



#24
Benzo(b)fluoranthene
Concen: 22.328 ng/ul m
RT: 23.253 min Scan# 4763
Delta R.T. 0.000 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06




Instrument :
BNA_N
ClientSampleId :
DCFZ2

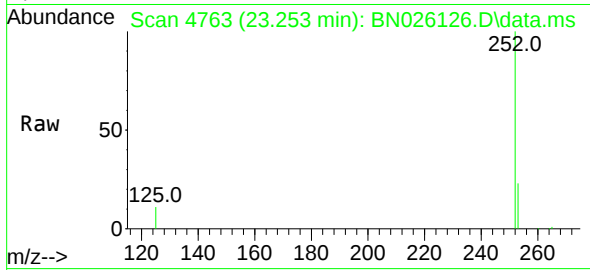

Tgt Ion:252 Resp: 274450
Ion Ratio Lower Upper
252 100
253 23.1 0.0 55.6
125 10.8 0.0 35.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

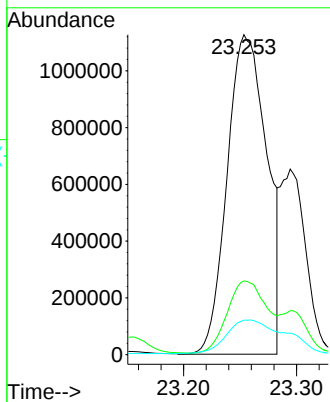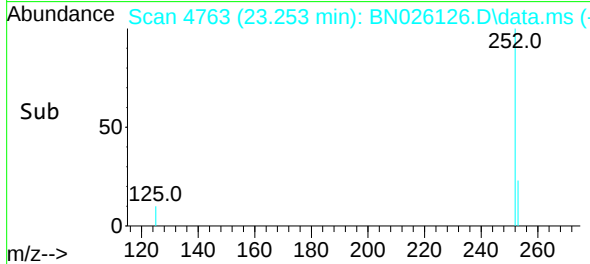

#25
Benzo(k)fluoranthene
Concen: 8.161 ng/ul m
RT: 23.294 min Scan# 4777
Delta R.T. -0.009 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06


Tgt Ion:252 Resp: 1007354
Ion Ratio Lower Upper
252 100
253 23.7 23.2 34.8
125 11.6 15.0 22.4#

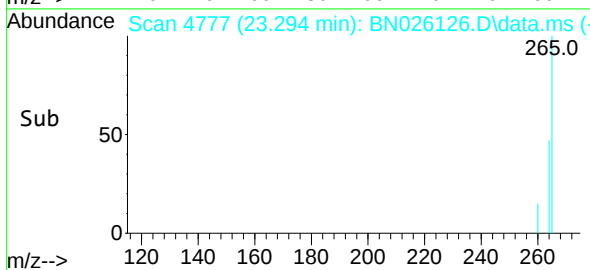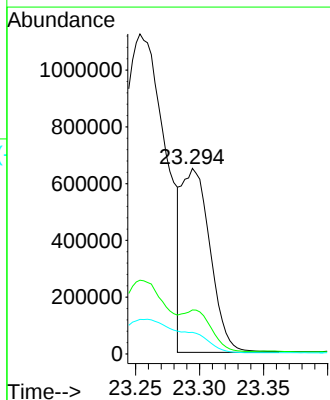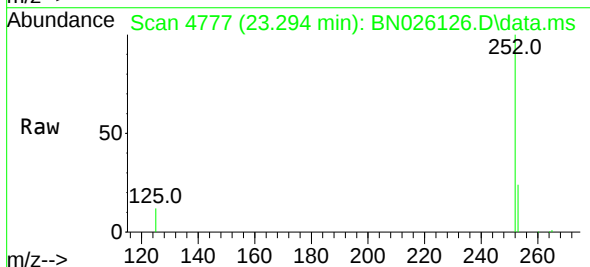

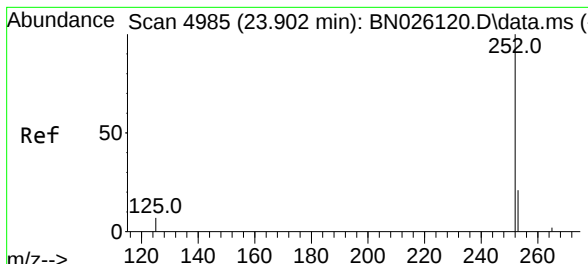

#26
Benzo(a)pyrene
Concen: 17.756 ng/ul
RT: 23.891 min Scan# 4985
Delta R.T. -0.014 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06




Instrument :
BNA_N
ClientSampleId :
DCFZ2

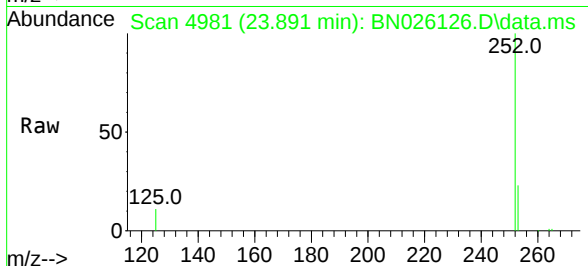

Tgt Ion:252 Resp: 189558
Ion Ratio Lower Upper
252 100
253 23.3 26.0 39.0
125 11.4 17.3 25.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

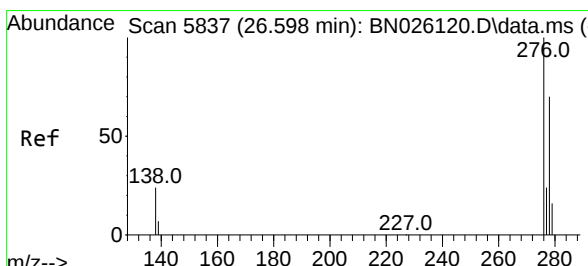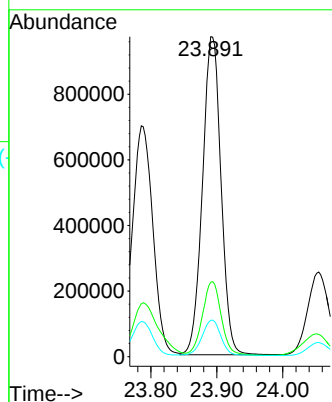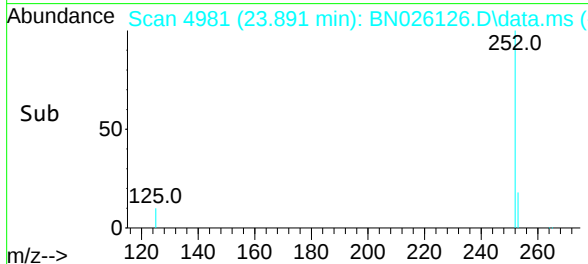

#27
Indeno(1,2,3-cd)pyrene
Concen: 13.556 ng/ul
RT: 26.568 min Scan# 5828
Delta R.T. -0.027 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06


Tgt Ion:276 Resp: 1580804
Ion Ratio Lower Upper
276 100
138 22.3 24.5 36.7
227 0.0 0.0 0.0

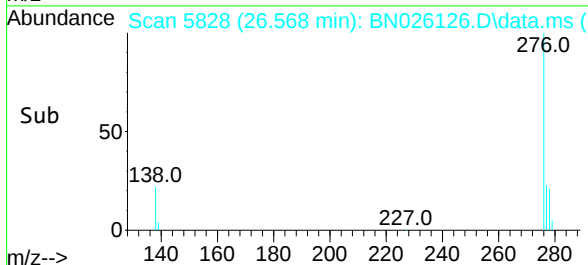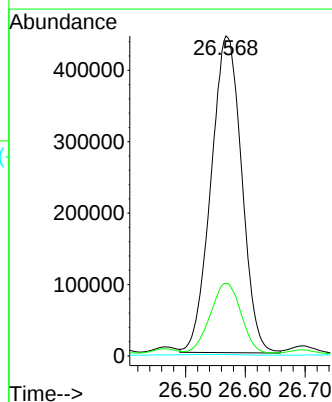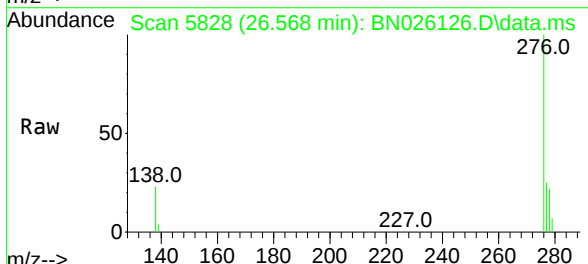



#28
Dibenzo(a,h)anthracene
Concen: 4.375 ng/ul
RT: 26.574 min Scan# 5830
Delta R.T. -0.040 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06




Instrument :
BNA_N
ClientSampleId :
DCFZ2




Tgt Ion:278 Resp: 386134
Ion Ratio Lower Upper
278 100
139 19.1 19.0 28.4
279 28.9 26.7 40.1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2023
Supervised By :mohammad ahmed 07/01/2023

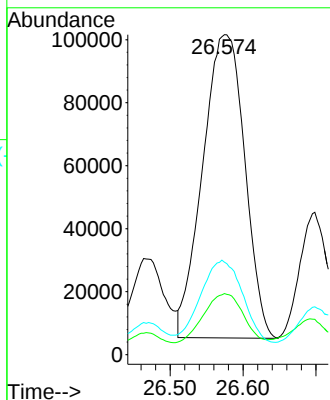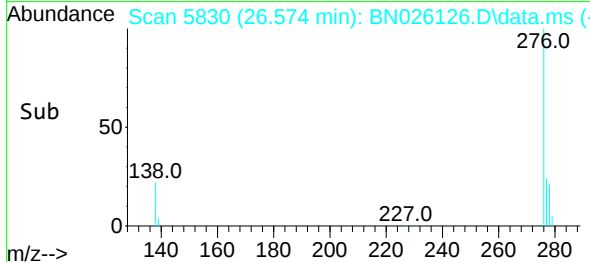

#29
Benzo(g,h,i)perylene
Concen: 14.955 ng/ul
RT: 27.359 min Scan# 6064
Delta R.T. -0.027 min
Lab File: BN026126.D
Acq: 30 Jun 2023 12:06

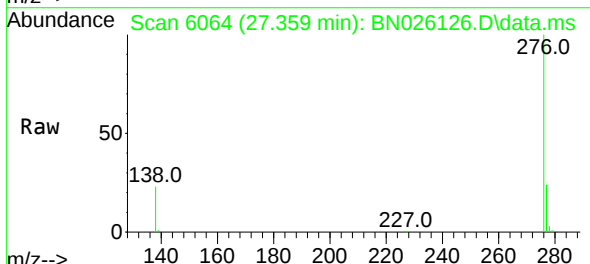

Tgt Ion:276 Resp: 1551318
Ion Ratio Lower Upper
276 100
138 23.0 23.4 35.0#
277 23.9 20.0 30.0

