

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
 Data File : BN020621.D
 Acq On : 02 Jul 2022 10:15
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Jul 04 02:38:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 02 03:10:12 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	4144	0.400	ng	0.00
7) Naphthalene-d8	10.626	136	12731	0.400	ng	0.00
13) Acenaphthene-d10	14.474	164	7432	0.400	ng	0.00
19) Phenanthrene-d10	17.225	188	15458	0.400	ng	0.00
29) Chrysene-d12	21.431	240	12167	0.400	ng	# 0.00
35) Perylene-d12	23.787	264	9676	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.413	112	3675	0.319	ng	0.00
5) Phenol-d6	7.024	99	4575	0.333	ng	0.00
8) Nitrobenzene-d5	8.982	82	3548	0.344	ng	-0.01
11) 2-Methylnaphthalene-d10	12.223	152	8242	0.378	ng	0.00
14) 2,4,6-Tribromophenol	15.974	330	832	0.297	ng	0.00
15) 2-Fluorobiphenyl	13.095	172	12143	0.396	ng	-0.01
27) Fluoranthene-d10	19.265	212	16609	0.362	ng	0.00
31) Terphenyl-d14	19.868	244	12262	0.422	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.261	88	1930	0.355	ng	98
3) n-Nitrosodimethylamine	3.600	42	1594	0.322	ng	99
6) bis(2-Chloroethyl)ether	7.255	93	4219	0.357	ng	97
9) Naphthalene	10.669	128	14614	0.384	ng	99
10) Hexachlorobutadiene	10.968	225	2645	0.382	ng	# 100
12) 2-Methylnaphthalene	12.295	142	9696	0.384	ng	99
16) Acenaphthylene	14.196	152	12875	0.360	ng	98
17) Acenaphthene	14.538	154	9241	0.380	ng	95
18) Fluorene	15.521	166	11969	0.377	ng	100
20) 4,6-Dinitro-2-methylph...	15.628	198	434	0.369	ng	# 65
21) 4-Bromophenyl-phenylether	16.415	248	3524	0.392	ng	96
22) Hexachlorobenzene	16.538	284	3997	0.402	ng	98
23) Atrazine	16.692	200	2231	0.315	ng	99
24) Pentachlorophenol	16.897	266	886	0.461	ng	96
25) Phenanthrene	17.266	178	19528	0.375	ng	100
26) Anthracene	17.359	178	15639	0.348	ng	100
28) Fluoranthene	19.295	202	21147	0.372	ng	100
30) Pyrene	19.662	202	21445	0.416	ng	100
32) Benzo(a)anthracene	21.413	228	15816	0.364	ng	98
33) Chrysene	21.467	228	18568	0.386	ng	98
34) Bis(2-ethylhexyl)phtha...	21.360	149	8320	0.340	ng	98
36) Indeno(1,2,3-cd)pyrene	26.223	276	15173	0.352	ng	98
37) Benzo(b)fluoranthene	23.071	252	14756	0.396	ng	97
38) Benzo(k)fluoranthene	23.121	252	16085	0.405	ng	98
39) Benzo(a)pyrene	23.688	252	11725	0.363	ng	# 89
40) Dibenzo(a,h)anthracene	26.237	278	12039	0.348	ng	97
41) Benzo(g,h,i)perylene	26.968	276	12600	0.334	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
Data File : BN020621.D
Acq On : 02 Jul 2022 10:15
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Jul 04 02:38:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 03:10:12 2022
Response via : Initial Calibration



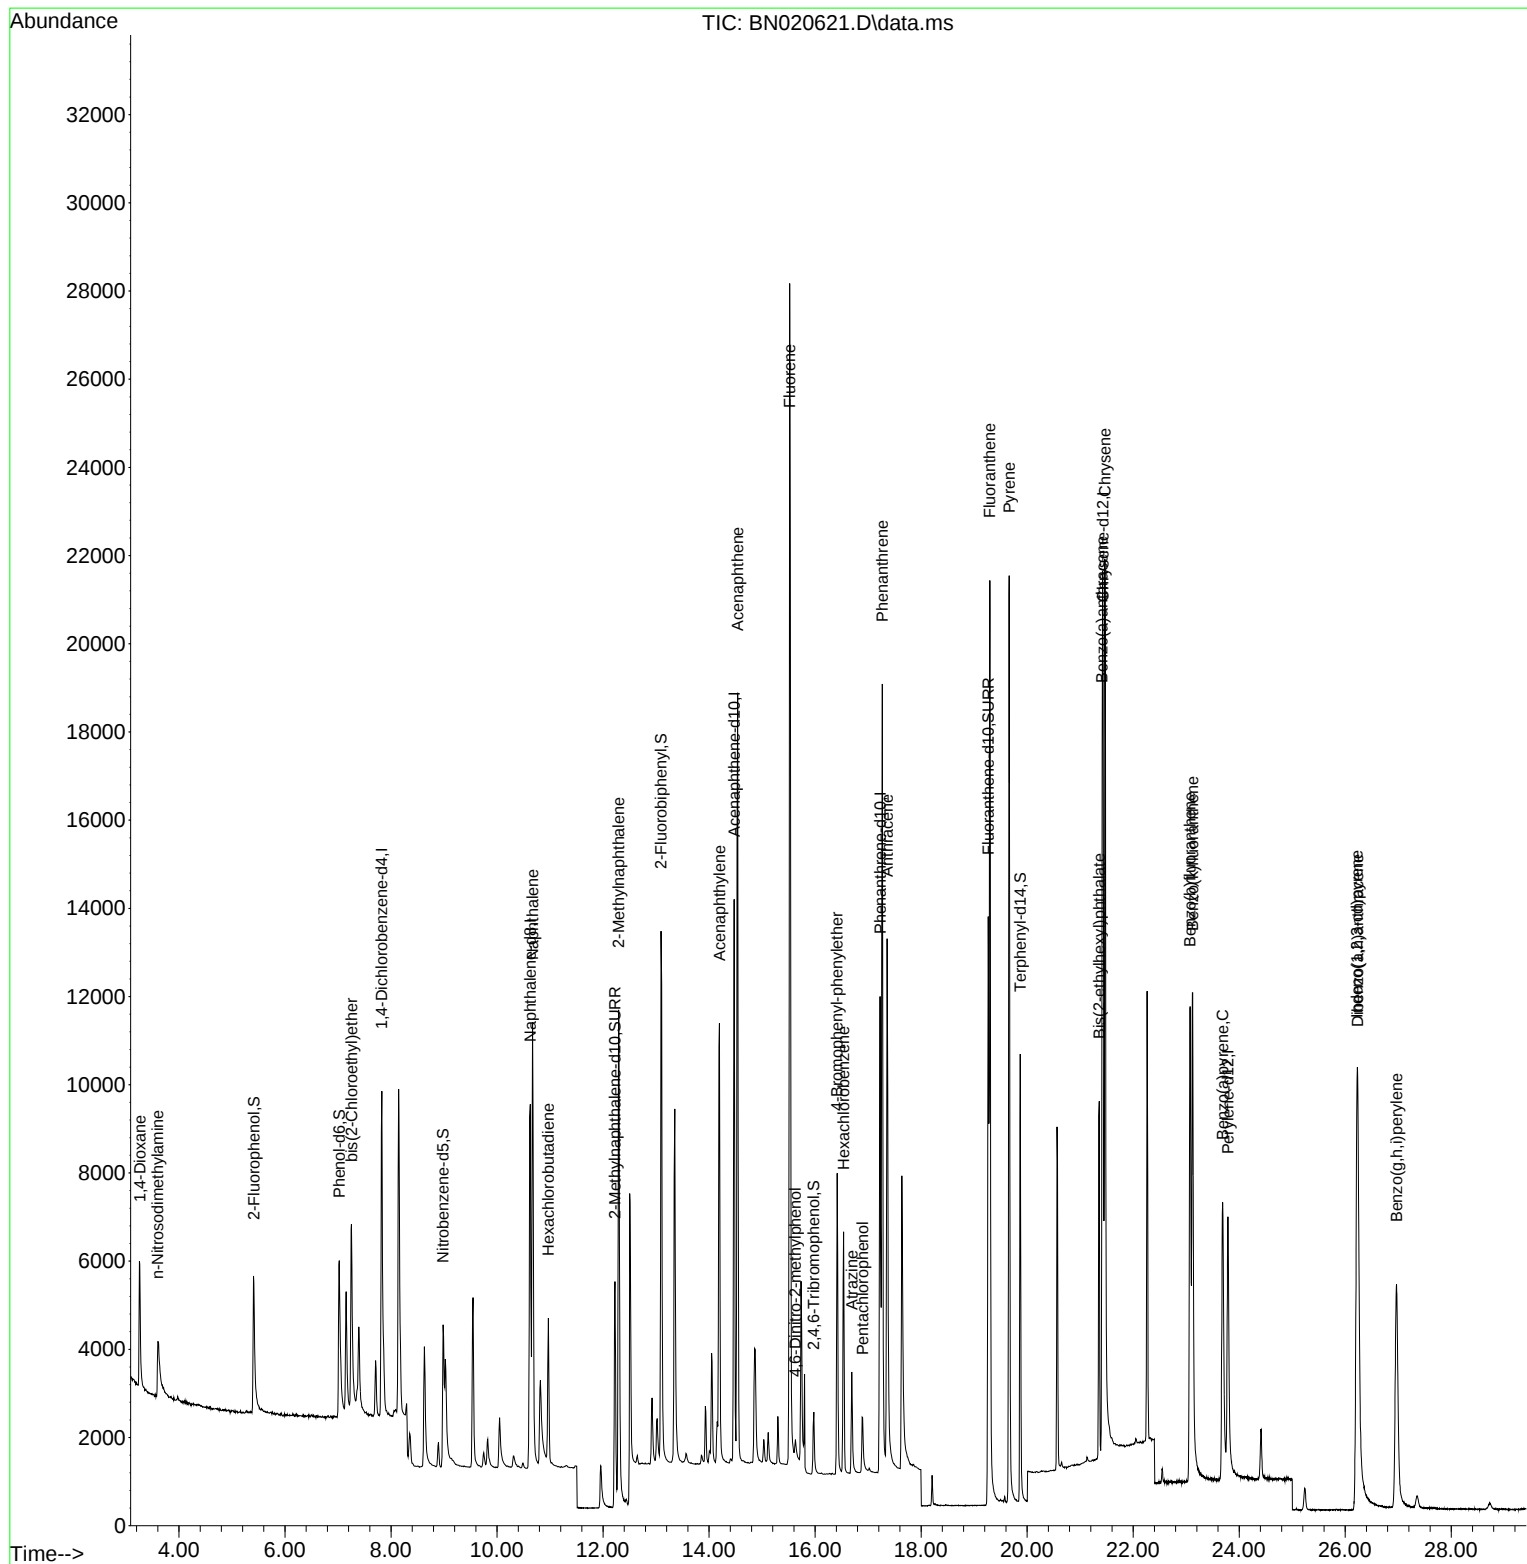




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.825 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN020621.D
 Acq: 02 Jul 2022 10:15




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:152 Resp: 4144
 Ion Ratio Lower Upper
 152 100
 150 155.1 127.9 191.9
 115 63.2 51.4 77.2

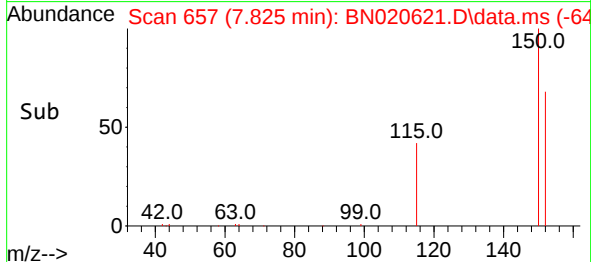

#2
 1,4-Dioxane
 Concen: 0.355 ng
 RT: 3.261 min Scan# 25
 Delta R.T. 0.000 min
 Lab File: BN020621.D
 Acq: 02 Jul 2022 10:15

Tgt Ion: 88 Resp: 1930
 Ion Ratio Lower Upper
 88 100
 43 35.9 30.2 45.2
 58 89.3 73.0 109.6

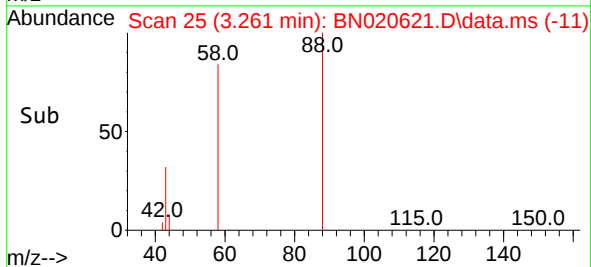

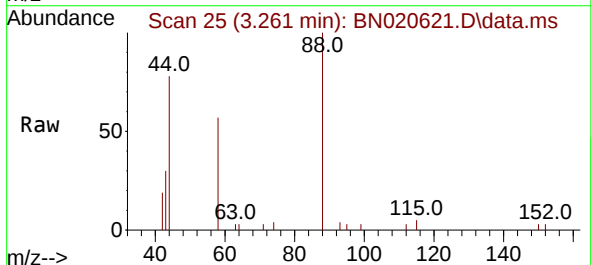




#3
n-Nitrosodimethylamine
Concen: 0.322 ng
RT: 3.600 min Scan# 71
Delta R.T. -0.007 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 1594
Ion Ratio Lower Upper
42 100
74 105.8 84.0 126.0
44 11.0 9.8 14.8

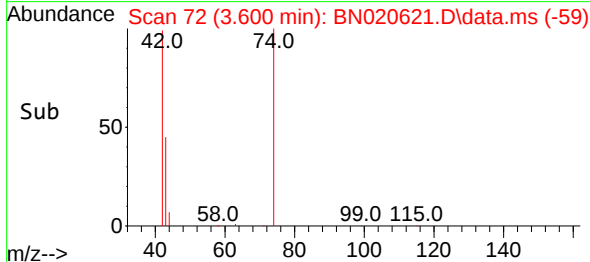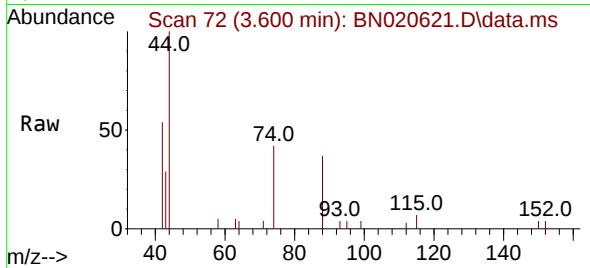

#4
2-Fluorophenol
Concen: 0.319 ng
RT: 5.413 min Scan# 323
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion: 112 Resp: 3675
Ion Ratio Lower Upper
112 100
64 62.9 49.1 73.7
63 33.7 26.3 39.5


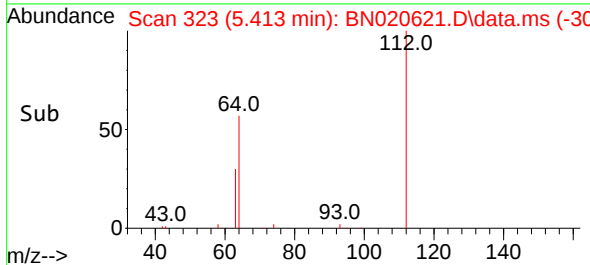

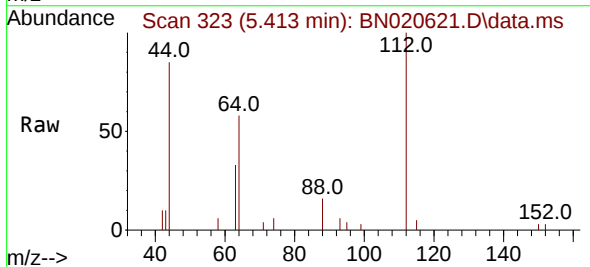


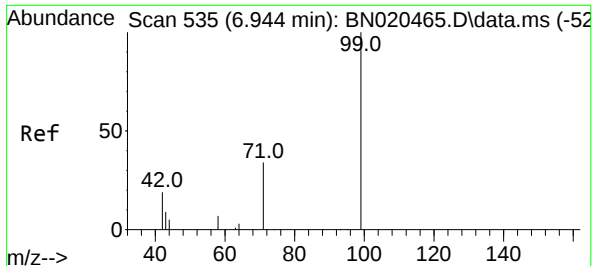

#5
Phenol-d6
Concen: 0.333 ng
RT: 7.024 min Scan# 54
Delta R.T. -0.007 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 99 Resp: 4575
Ion Ratio Lower Upper
99 100
42 22.3 19.3 28.9
71 35.3 27.5 41.3

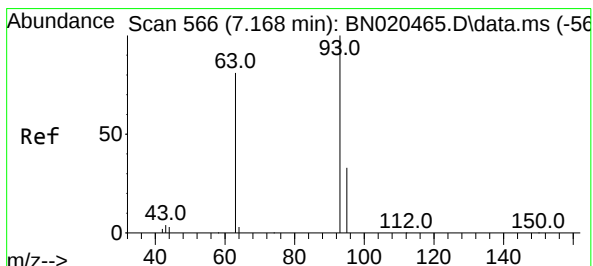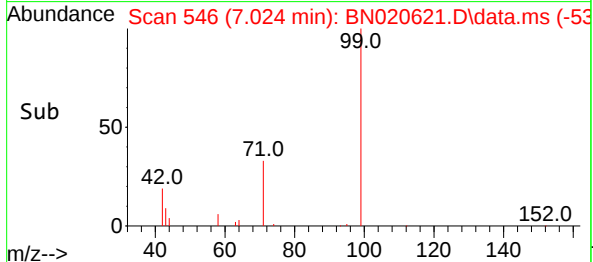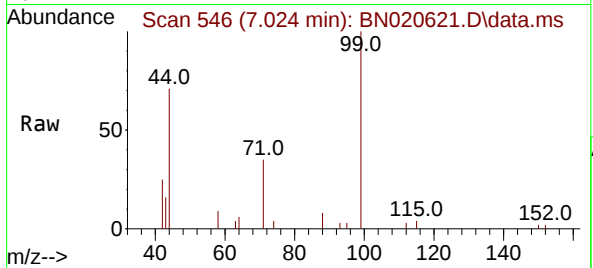

#6
bis(2-Chloroethyl)ether
Concen: 0.357 ng
RT: 7.255 min Scan# 578
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion: 93 Resp: 4219
Ion Ratio Lower Upper
93 100
63 87.5 67.4 101.0
95 33.7 26.5 39.7

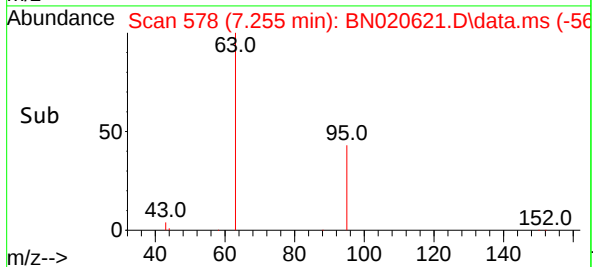

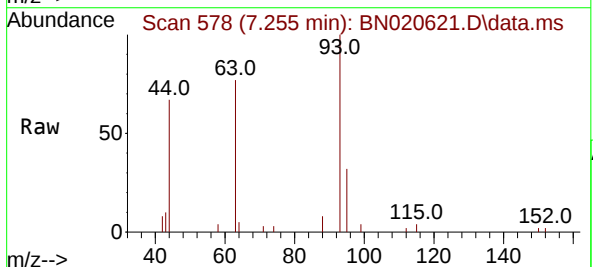




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.626 min Scan# 94
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:136	Resp:	12731
Ion Ratio	Lower	Upper
136	100	
137	11.6	9.0 13.6
54	8.4	6.2 9.2
68	5.6	4.4 6.6

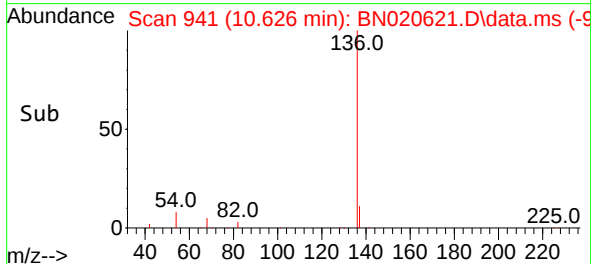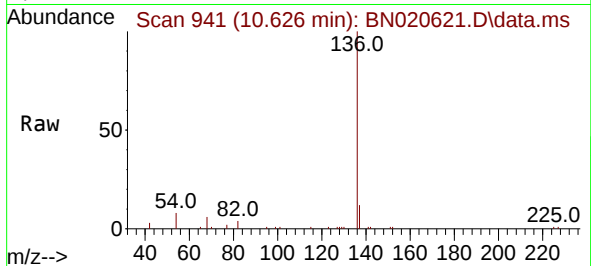

#8
Nitrobenzene-d5
Concen: 0.344 ng
RT: 8.982 min Scan# 787
Delta R.T. -0.011 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion: 82	Resp:	3548
Ion Ratio	Lower	Upper
82	100	
128	36.9	35.0 52.6
54	65.0	46.2 69.4


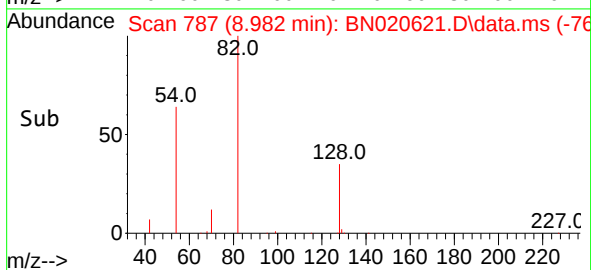

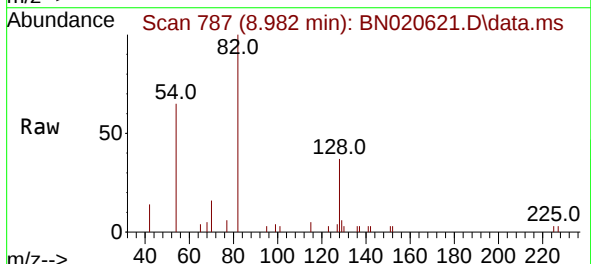




#9
Naphthalene
Concen: 0.384 ng
RT: 10.669 min Scan# 945
Delta R.T. -0.011 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:128 Resp: 14614
Ion Ratio Lower Upper
128 100
129 11.2 8.9 13.3
127 13.9 10.8 16.2

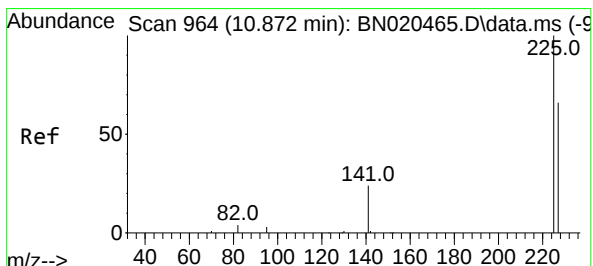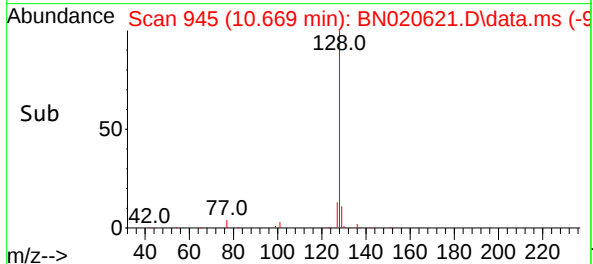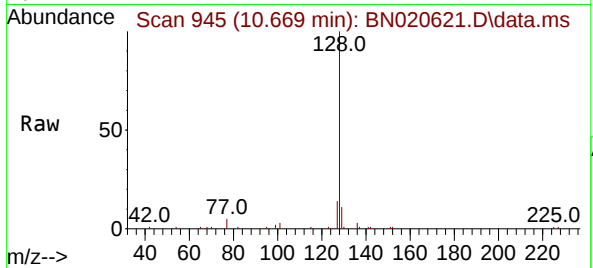

#10
Hexachlorobutadiene
Concen: 0.382 ng
RT: 10.968 min Scan# 973
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:225 Resp: 2645
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.8 50.9 76.3

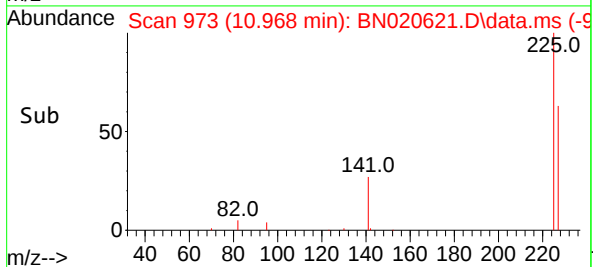

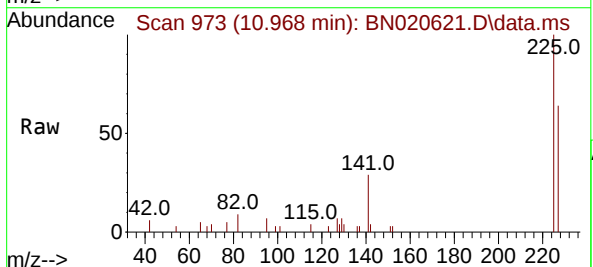




#11
2-Methylnaphthalene-d10
Concen: 0.378 ng
RT: 12.223 min Scan# 1185
Delta R.T. -0.004 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:152 Resp: 8242
Ion Ratio Lower Upper
152 100
151 20.0 16.2 24.4

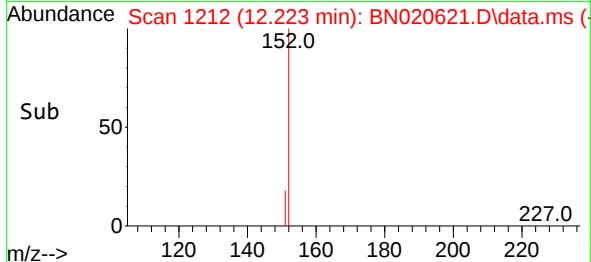

#12
2-Methylnaphthalene
Concen: 0.384 ng
RT: 12.295 min Scan# 1231
Delta R.T. -0.004 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:142 Resp: 9696
Ion Ratio Lower Upper
142 100
141 88.5 71.6 107.4
115 38.3 29.8 44.8

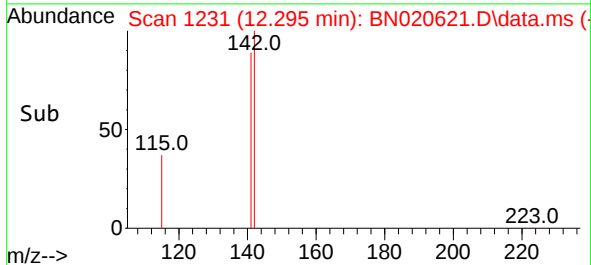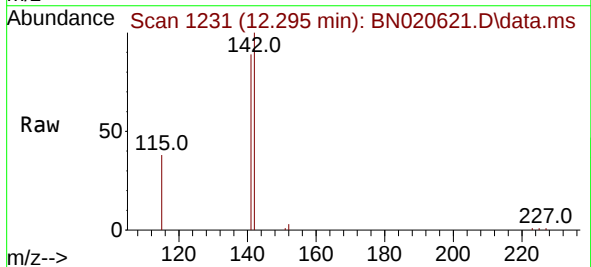



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.474 min Scan# 14

Delta R.T. 0.000 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:164 Resp: 7432

Ion Ratio Lower Upper

164 100

162 103.4 82.1 123.1

160 48.0 38.6 58.0

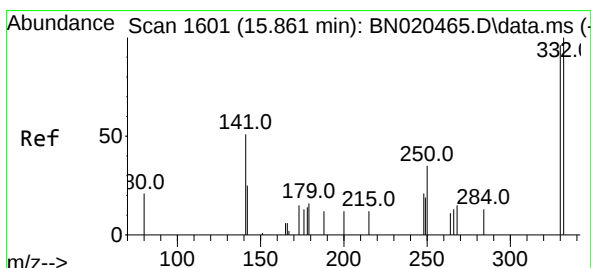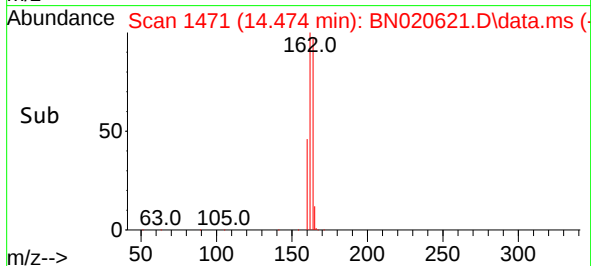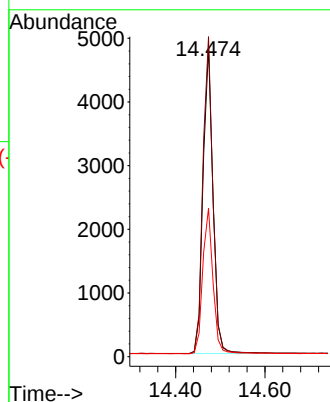

#14

2,4,6-Tribromophenol

Concen: 0.297 ng

RT: 15.974 min Scan# 1612

Delta R.T. 0.000 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15




Tgt Ion:330 Resp: 832

Ion Ratio Lower Upper

330 100

332 98.4 77.6 116.4

141 56.0 41.0 61.4

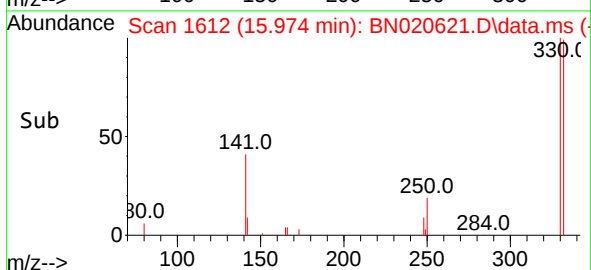

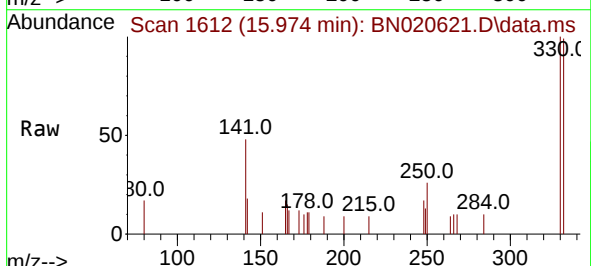




#15
2-Fluorobiphenyl
Concen: 0.396 ng
RT: 13.095 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:172 Resp: 12143
Ion Ratio Lower Upper
172 100
171 36.0 27.2 40.8
170 24.8 18.2 27.4

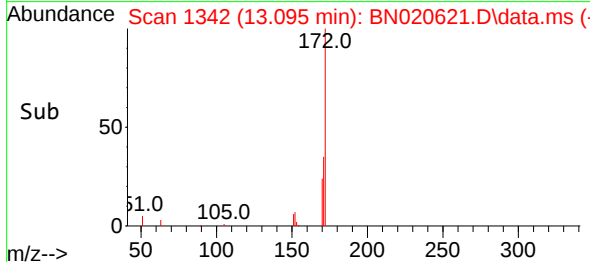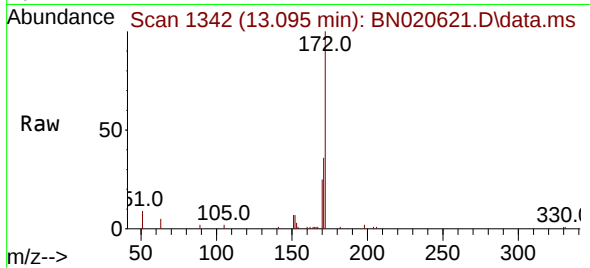

#16
Acenaphthylene
Concen: 0.360 ng
RT: 14.196 min Scan# 1445
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:152 Resp: 12875
Ion Ratio Lower Upper
152 100
151 19.5 16.2 24.4
153 12.7 10.7 16.1

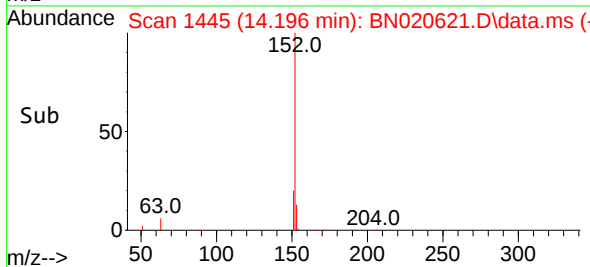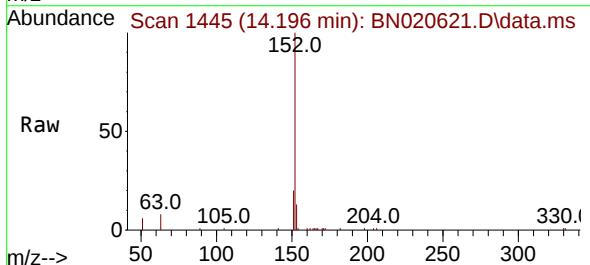

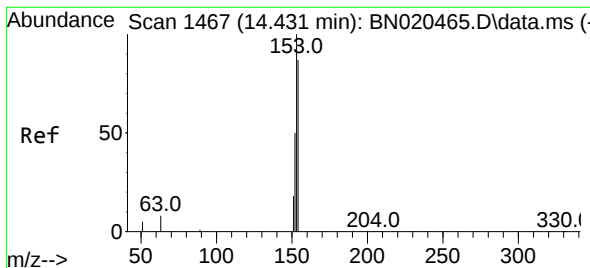

#17

Acenaphthene

Concen: 0.380 ng

RT: 14.538 min Scan# 1467

Delta R.T. 0.000 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:154 Resp: 9241

Ion Ratio Lower Upper

154 100

153 115.1 87.5 131.3

152 57.8 43.8 65.6

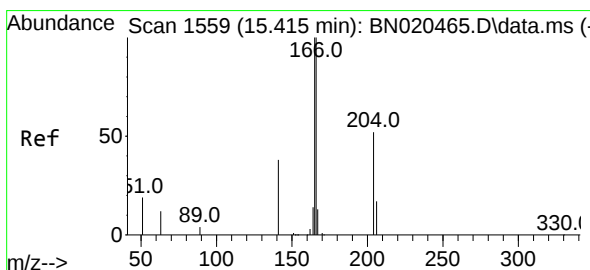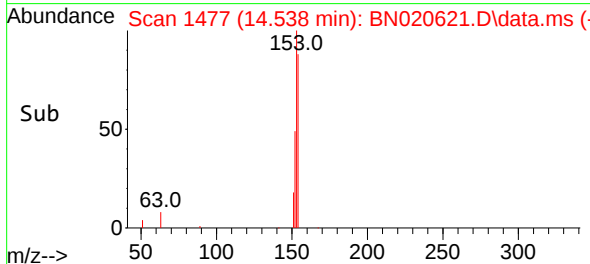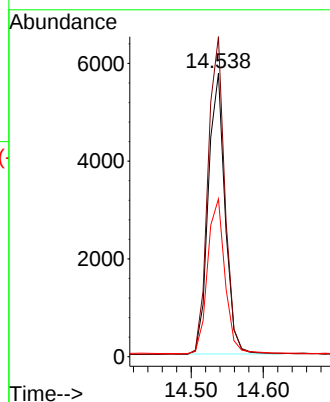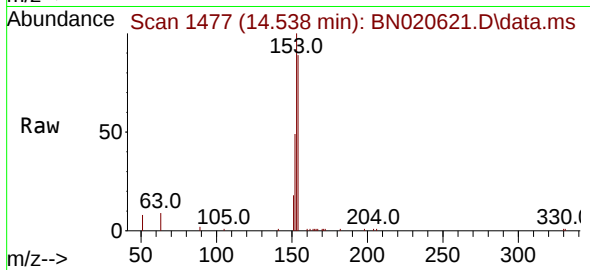

#18

Fluorene

Concen: 0.377 ng

RT: 15.521 min Scan# 1569

Delta R.T. -0.011 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15




Tgt Ion:166 Resp: 11969

Ion Ratio Lower Upper

166 100

165 98.7 78.6 118.0

167 13.3 10.8 16.2


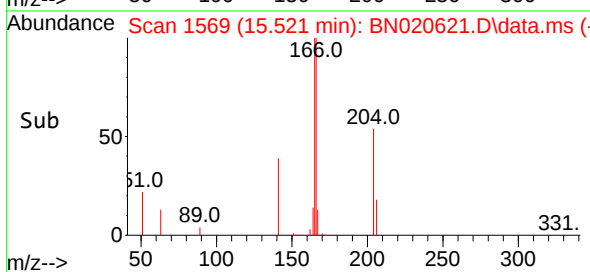
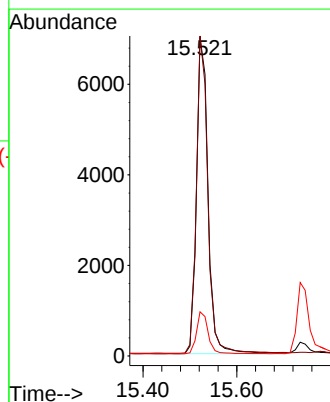
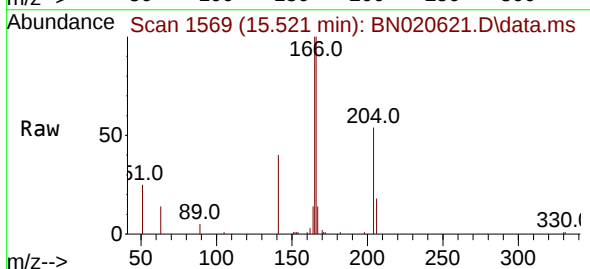




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.225 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:188 Resp: 15458
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.7 7.4 11.2

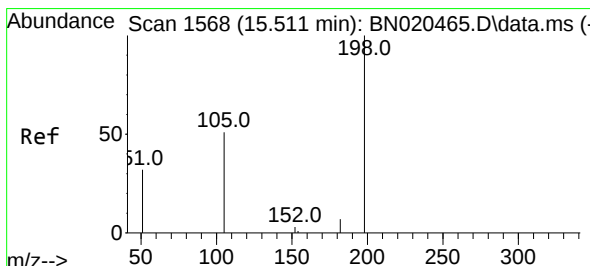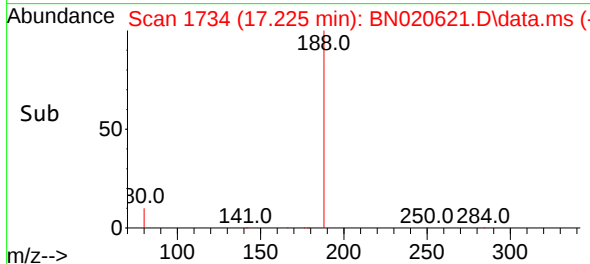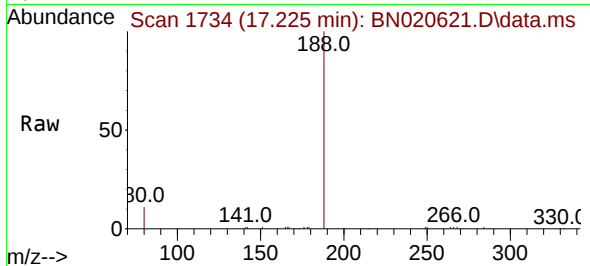

#20
4,6-Dinitro-2-methylphenol
Concen: 0.369 ng
RT: 15.628 min Scan# 1579
Delta R.T. -0.011 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:198 Resp: 434
Ion Ratio Lower Upper
198 100
182 29.8 12.1 18.1#
77 0.0 0.0 0.0


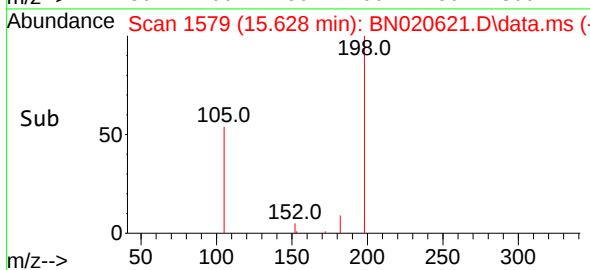

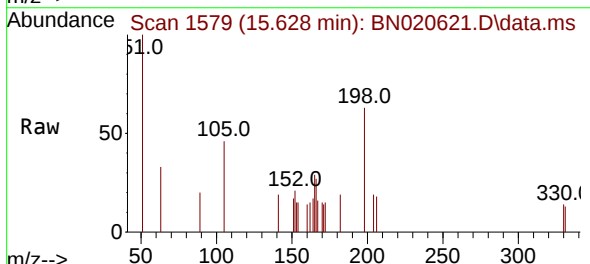




#21
4-Bromophenyl-phenylether
Concen: 0.392 ng
RT: 16.415 min Scan# 1665
Delta R.T. -0.010 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:248 Resp: 3524
Ion Ratio Lower Upper
248 100
250 93.6 75.3 112.9
141 91.5 67.3 100.9

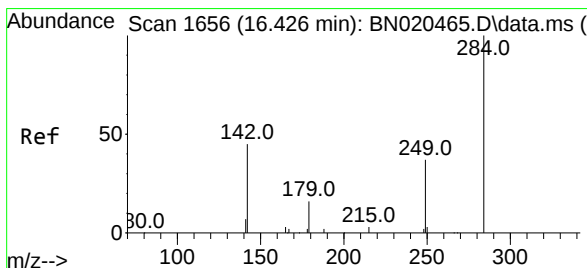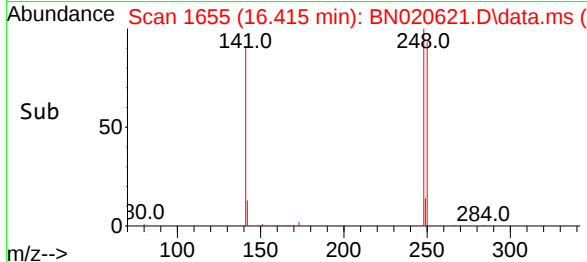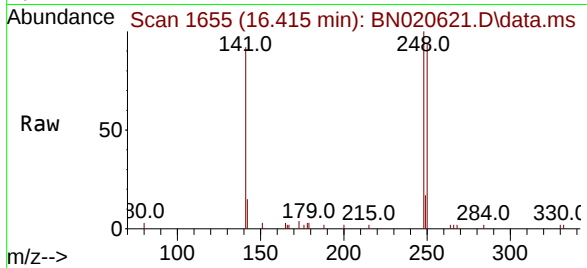

#22
Hexachlorobenzene
Concen: 0.402 ng
RT: 16.538 min Scan# 1667
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:284 Resp: 3997
Ion Ratio Lower Upper
284 100
142 45.5 35.2 52.8
249 32.8 26.6 40.0


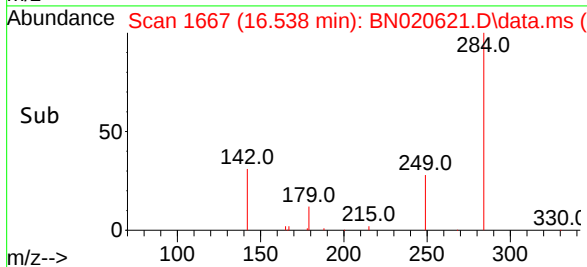

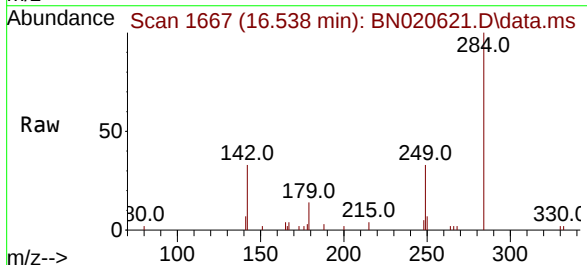




#23
Atrazine
Concen: 0.315 ng
RT: 16.692 min Scan# 1702
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:200 Resp: 2231
Ion Ratio Lower Upper
200 100
173 30.2 23.6 35.4
215 45.5 36.6 54.8

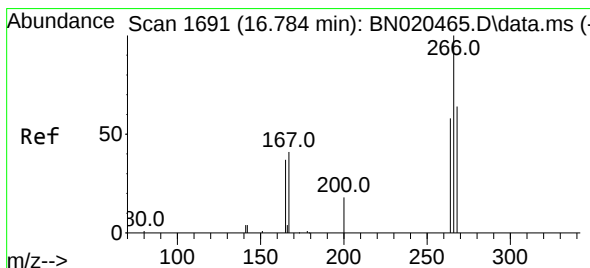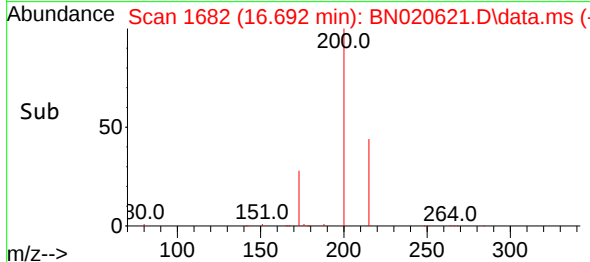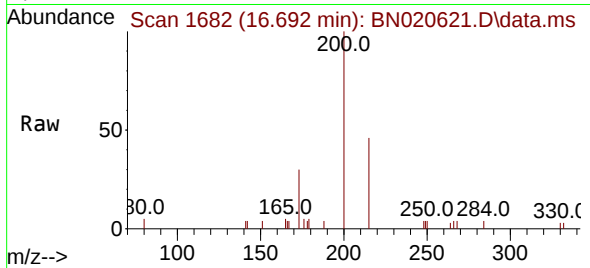

#24
Pentachlorophenol
Concen: 0.461 ng
RT: 16.897 min Scan# 1702
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:266 Resp: 886
Ion Ratio Lower Upper
266 100
264 59.7 51.3 76.9
268 63.8 52.6 79.0


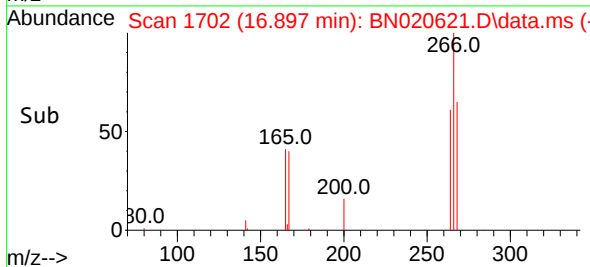

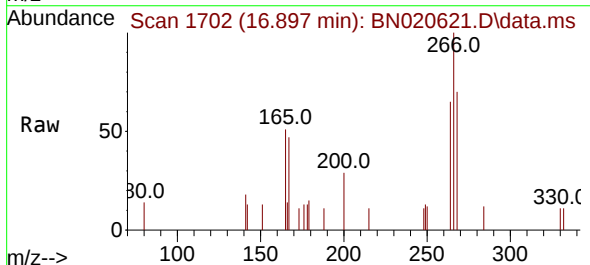




#25
Phenanthrene
Concen: 0.375 ng
RT: 17.266 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:178 Resp: 19528
Ion Ratio Lower Upper
178 100
176 19.3 15.3 22.9
179 15.2 12.2 18.4

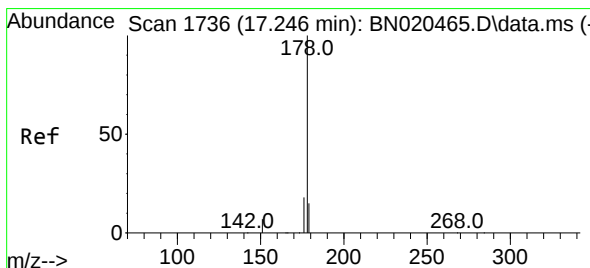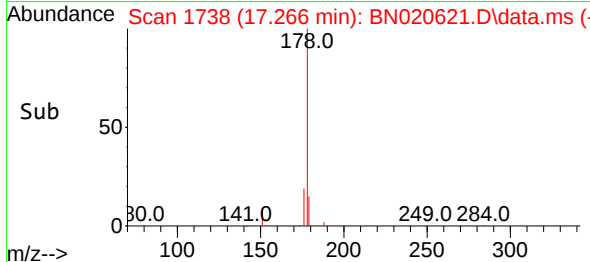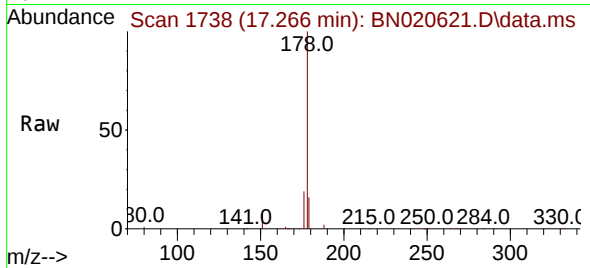

#26
Anthracene
Concen: 0.348 ng
RT: 17.359 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:178 Resp: 15639
Ion Ratio Lower Upper
178 100
176 18.5 14.9 22.3
179 15.6 12.2 18.4

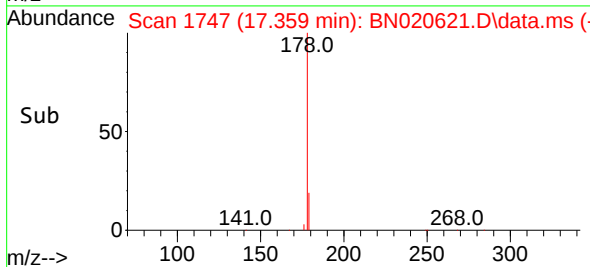

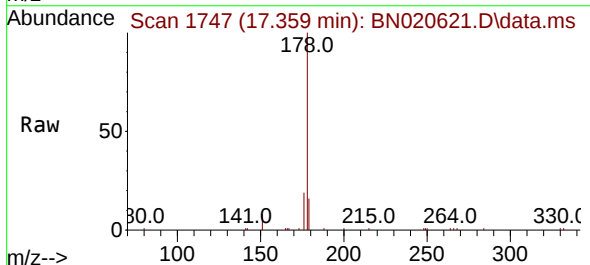




#27
Fluoranthene-d10
Concen: 0.362 ng
RT: 19.265 min Scan# 2109
Delta R.T. -0.004 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 16609
Ion Ratio Lower Upper
212 100
106 15.4 12.6 19.0
104 8.9 7.2 10.8

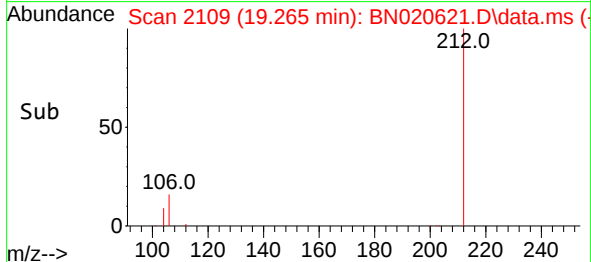

#28
Fluoranthene
Concen: 0.372 ng
RT: 19.295 min Scan# 2116
Delta R.T. -0.004 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:202 Resp: 21147
Ion Ratio Lower Upper
202 100
101 11.9 9.6 14.4
203 16.8 13.5 20.3

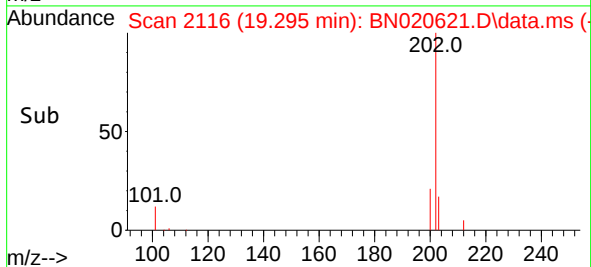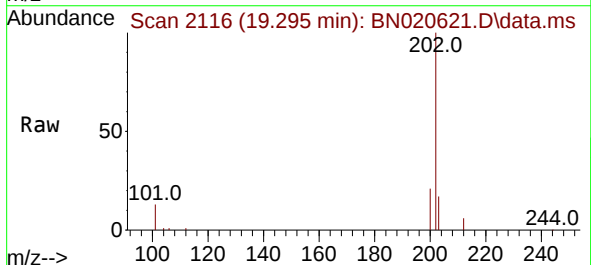



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.431 min Scan# 2444

Delta R.T. 0.000 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:240 Resp: 12167

Ion Ratio Lower Upper

240 100

120 14.4 14.6 21.8#

236 27.7 22.6 33.8

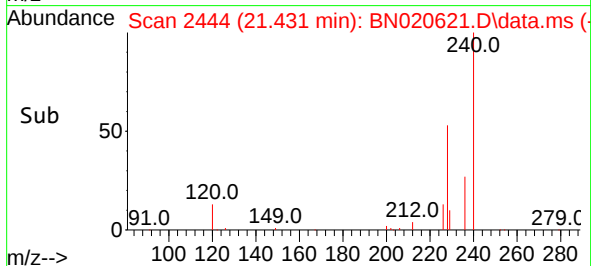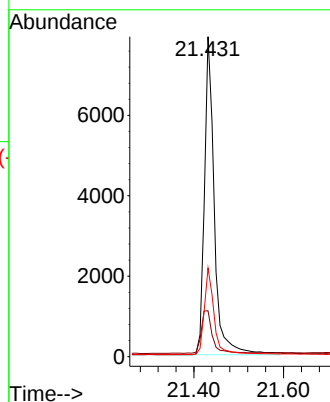

#30

Pyrene

Concen: 0.416 ng

RT: 19.662 min Scan# 2203

Delta R.T. 0.000 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15




Tgt Ion:202 Resp: 21445

Ion Ratio Lower Upper

202 100

200 20.8 16.6 25.0

203 17.6 14.2 21.2

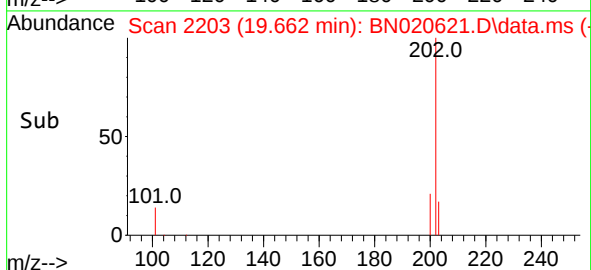

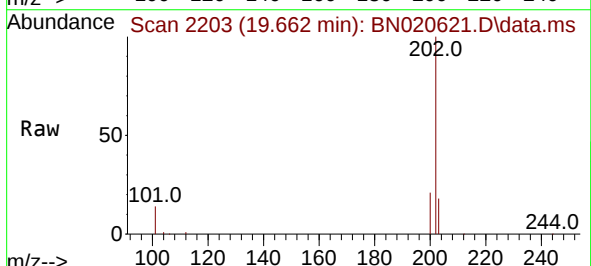




#31
 Terphenyl-d14
 Concen: 0.422 ng
 RT: 19.868 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN020621.D
 Acq: 02 Jul 2022 10:15




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:244 Resp: 12262
 Ion Ratio Lower Upper
 244 100
 212 8.9 7.1 10.7
 122 0.0 0.0 0.0

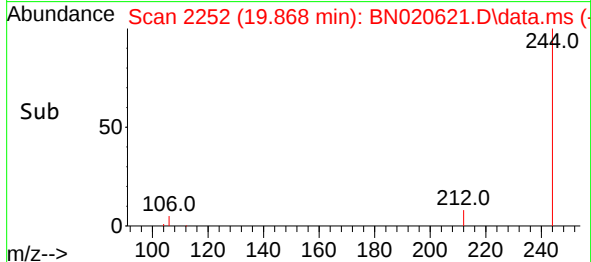

#32
 Benzo(a)anthracene
 Concen: 0.364 ng
 RT: 21.413 min Scan# 2442
 Delta R.T. -0.009 min
 Lab File: BN020621.D
 Acq: 02 Jul 2022 10:15

Tgt Ion:228 Resp: 15816
 Ion Ratio Lower Upper
 228 100
 226 28.2 21.2 31.8
 229 19.4 15.6 23.4

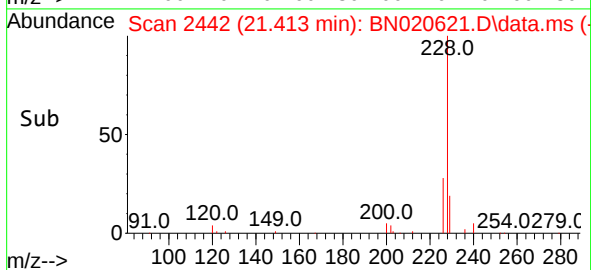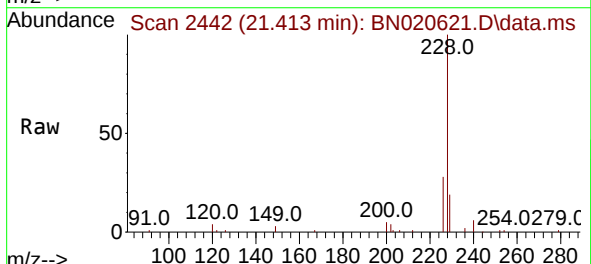



#33

Chrysene

Concen: 0.386 ng

RT: 21.467 min Scan# 2448

Delta R.T. 0.000 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4




Tgt Ion:228 Resp: 18568

Ion Ratio Lower Upper

228 100

226 30.7 23.4 35.0

229 19.7 15.7 23.5

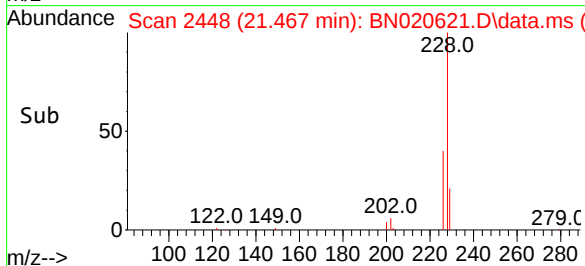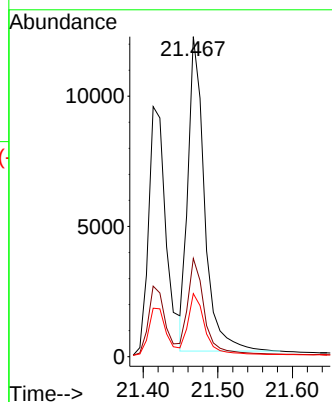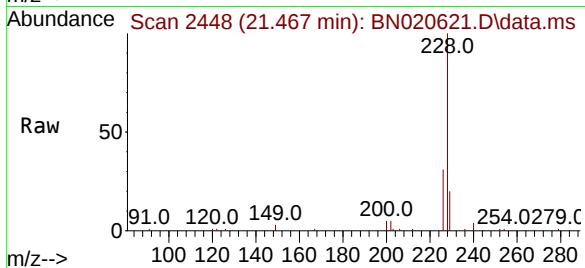

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.340 ng

RT: 21.360 min Scan# 2436

Delta R.T. 0.009 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15




Tgt Ion:149 Resp: 8320

Ion Ratio Lower Upper

149 100

167 26.1 21.7 32.5

279 3.1 2.2 3.2

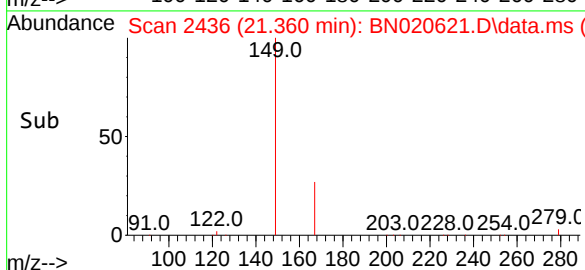

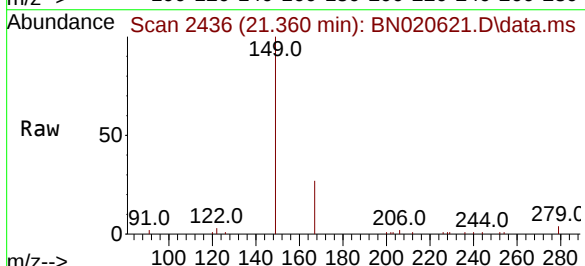




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.787 min Scan# 30
Delta R.T. -0.003 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:264 Resp: 9676
Ion Ratio Lower Upper
264 100
260 26.7 20.9 31.3
265 32.7 28.0 42.0

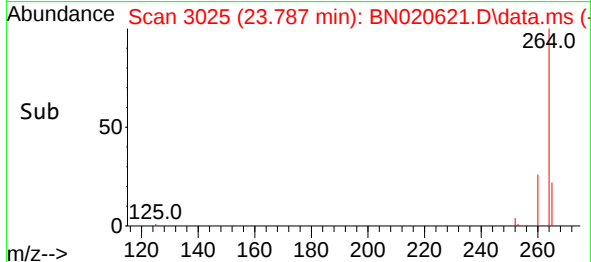

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.352 ng
RT: 26.223 min Scan# 3858
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:276 Resp: 15173
Ion Ratio Lower Upper
276 100
138 33.8 25.9 38.9
277 24.6 19.8 29.8

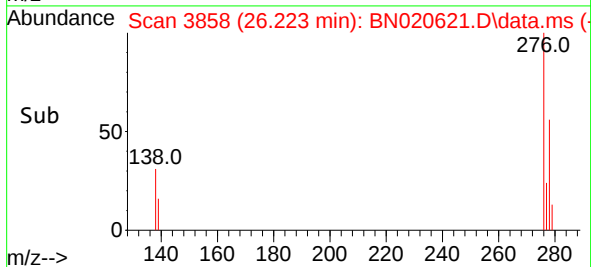

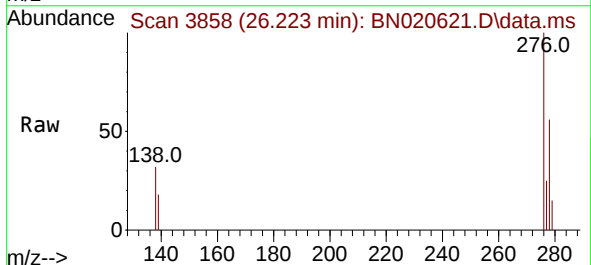




#37
Benzo(b)fluoranthene
Concen: 0.396 ng
RT: 23.071 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 14756
Ion Ratio Lower Upper
252 100
253 24.2 18.5 27.7
125 15.6 11.4 17.0

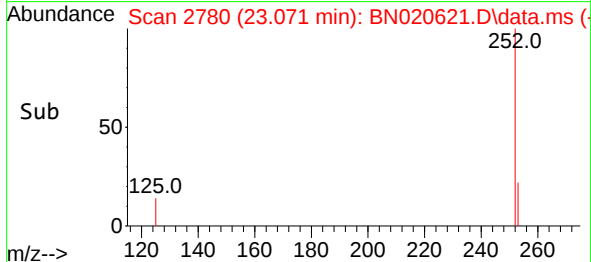

#38
Benzo(k)fluoranthene
Concen: 0.405 ng
RT: 23.121 min Scan# 2797
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Tgt Ion:252 Resp: 16085
Ion Ratio Lower Upper
252 100
253 23.9 18.0 27.0
125 13.6 11.0 16.4

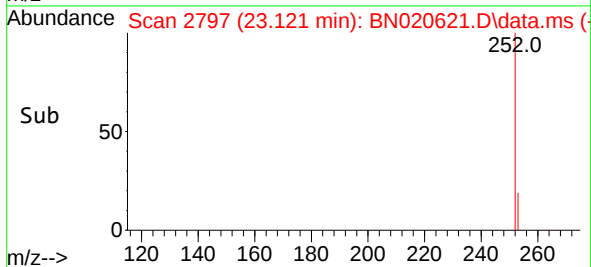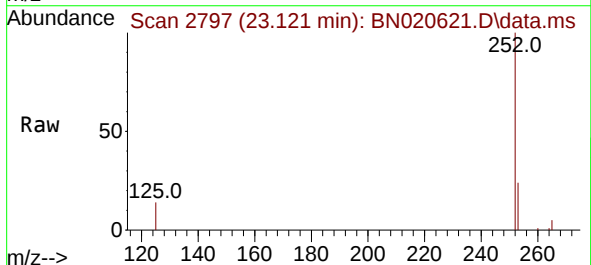



#39

Benzo(a)pyrene

Concen: 0.363 ng

RT: 23.688 min Scan# 2926

Delta R.T. 0.003 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4




Tgt Ion:252 Resp: 11725

Ion Ratio Lower Upper

252 100

253 26.6 19.0 28.4

125 24.7 13.8 20.8#

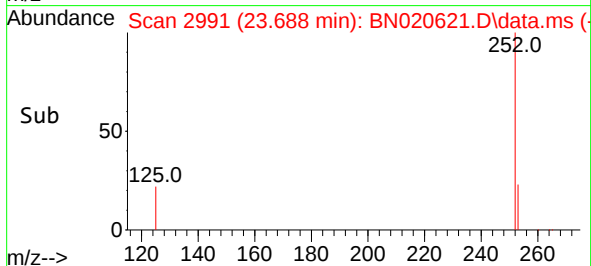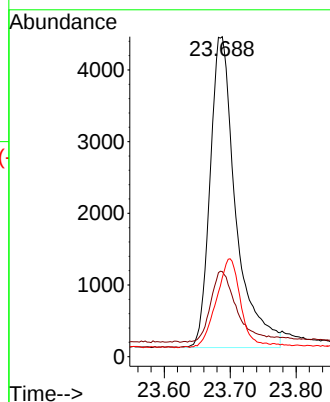

#40

Dibenzo(a,h)anthracene

Concen: 0.348 ng

RT: 26.237 min Scan# 3863

Delta R.T. -0.009 min

Lab File: BN020621.D

Acq: 02 Jul 2022 10:15




Tgt Ion:278 Resp: 12039

Ion Ratio Lower Upper

278 100

139 24.9 18.6 28.0


279 25.7 19.7 29.5

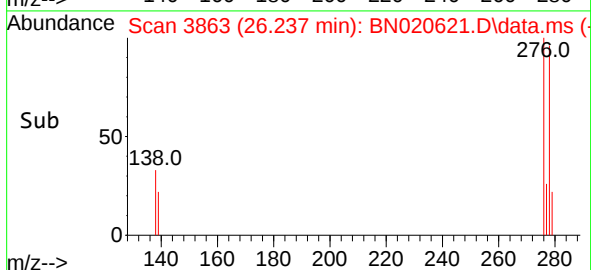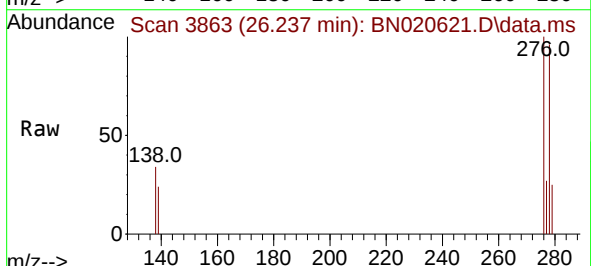



#41
Benzo(g,h,i)perylene
Concen: 0.334 ng
RT: 26.968 min Scan# 41
Delta R.T. 0.000 min
Lab File: BN020621.D
Acq: 02 Jul 2022 10:15

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

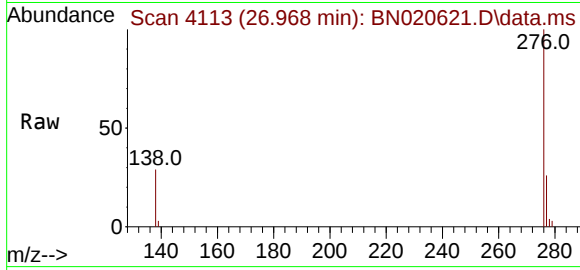

Tgt Ion:276 Resp: 12600
Ion Ratio Lower Upper
276 100
277 25.7 19.5 29.3
138 28.8 22.6 34.0

