

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
 Data File : BN020638.D
 Acq On : 02 Jul 2022 20:36
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Jul 04 02:39:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 02 03:10:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	4876	0.400	ng	0.00
7) Naphthalene-d8	10.626	136	14808	0.400	ng	0.00
13) Acenaphthene-d10	14.474	164	8104	0.400	ng	0.00
19) Phenanthrene-d10	17.225	188	16607	0.400	ng	0.00
29) Chrysene-d12	21.431	240	13320	0.400	ng	# 0.00
35) Perylene-d12	23.787	264	10820	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.413	112	4279	0.316	ng	0.00
5) Phenol-d6	7.024	99	5515	0.341	ng	0.00
8) Nitrobenzene-d5	8.982	82	4244	0.354	ng	-0.01
11) 2-Methylnaphthalene-d10	12.223	152	9319	0.367	ng	0.00
14) 2,4,6-Tribromophenol	15.974	330	952	0.312	ng	0.00
15) 2-Fluorobiphenyl	13.095	172	13404	0.401	ng	-0.01
27) Fluoranthene-d10	19.265	212	18011	0.365	ng	0.00
31) Terphenyl-d14	19.868	244	12835	0.403	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.261	88	2250	0.352	ng	99
3) n-Nitrosodimethylamine	3.600	42	1922	0.330	ng	# 98
6) bis(2-Chloroethyl)ether	7.255	93	5048	0.363	ng	99
9) Naphthalene	10.669	128	16905	0.382	ng	99
10) Hexachlorobutadiene	10.968	225	3023	0.375	ng	# 98
12) 2-Methylnaphthalene	12.295	142	11008	0.374	ng	99
16) Acenaphthylene	14.196	152	14180	0.364	ng	98
17) Acenaphthene	14.538	154	10094	0.381	ng	96
18) Fluorene	15.521	166	12790	0.370	ng	100
20) 4,6-Dinitro-2-methylph...	15.628	198	614	0.414	ng	# 79
21) 4-Bromophenyl-phenylether	16.415	248	3803	0.394	ng	97
22) Hexachlorobenzene	16.538	284	4232	0.396	ng	98
23) Atrazine	16.692	200	2415	0.317	ng	99
24) Pentachlorophenol	16.897	266	887	0.443	ng	100
25) Phenanthrene	17.266	178	20930	0.374	ng	100
26) Anthracene	17.359	178	16816	0.348	ng	100
28) Fluoranthene	19.295	202	22766	0.373	ng	100
30) Pyrene	19.657	202	23103	0.410	ng	100
32) Benzo(a)anthracene	21.413	228	16637	0.350	ng	99
33) Chrysene	21.467	228	20965	0.398	ng	99
34) Bis(2-ethylhexyl)phtha...	21.351	149	9336	0.348	ng	98
36) Indeno(1,2,3-cd)pyrene	26.217	276	16786	0.348	ng	99
37) Benzo(b)fluoranthene	23.071	252	16899	0.405	ng	98
38) Benzo(k)fluoranthene	23.115	252	17987	0.405	ng	98
39) Benzo(a)pyrene	23.682	252	13924	0.385	ng	# 94
40) Dibenzo(a,h)anthracene	26.237	278	13213	0.342	ng	98
41) Benzo(g,h,i)perylene	26.962	276	14043	0.333	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
Data File : BN020638.D
Acq On : 02 Jul 2022 20:36
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Quant Time: Jul 04 02:39:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 03:10:12 2022
Response via : Initial Calibration

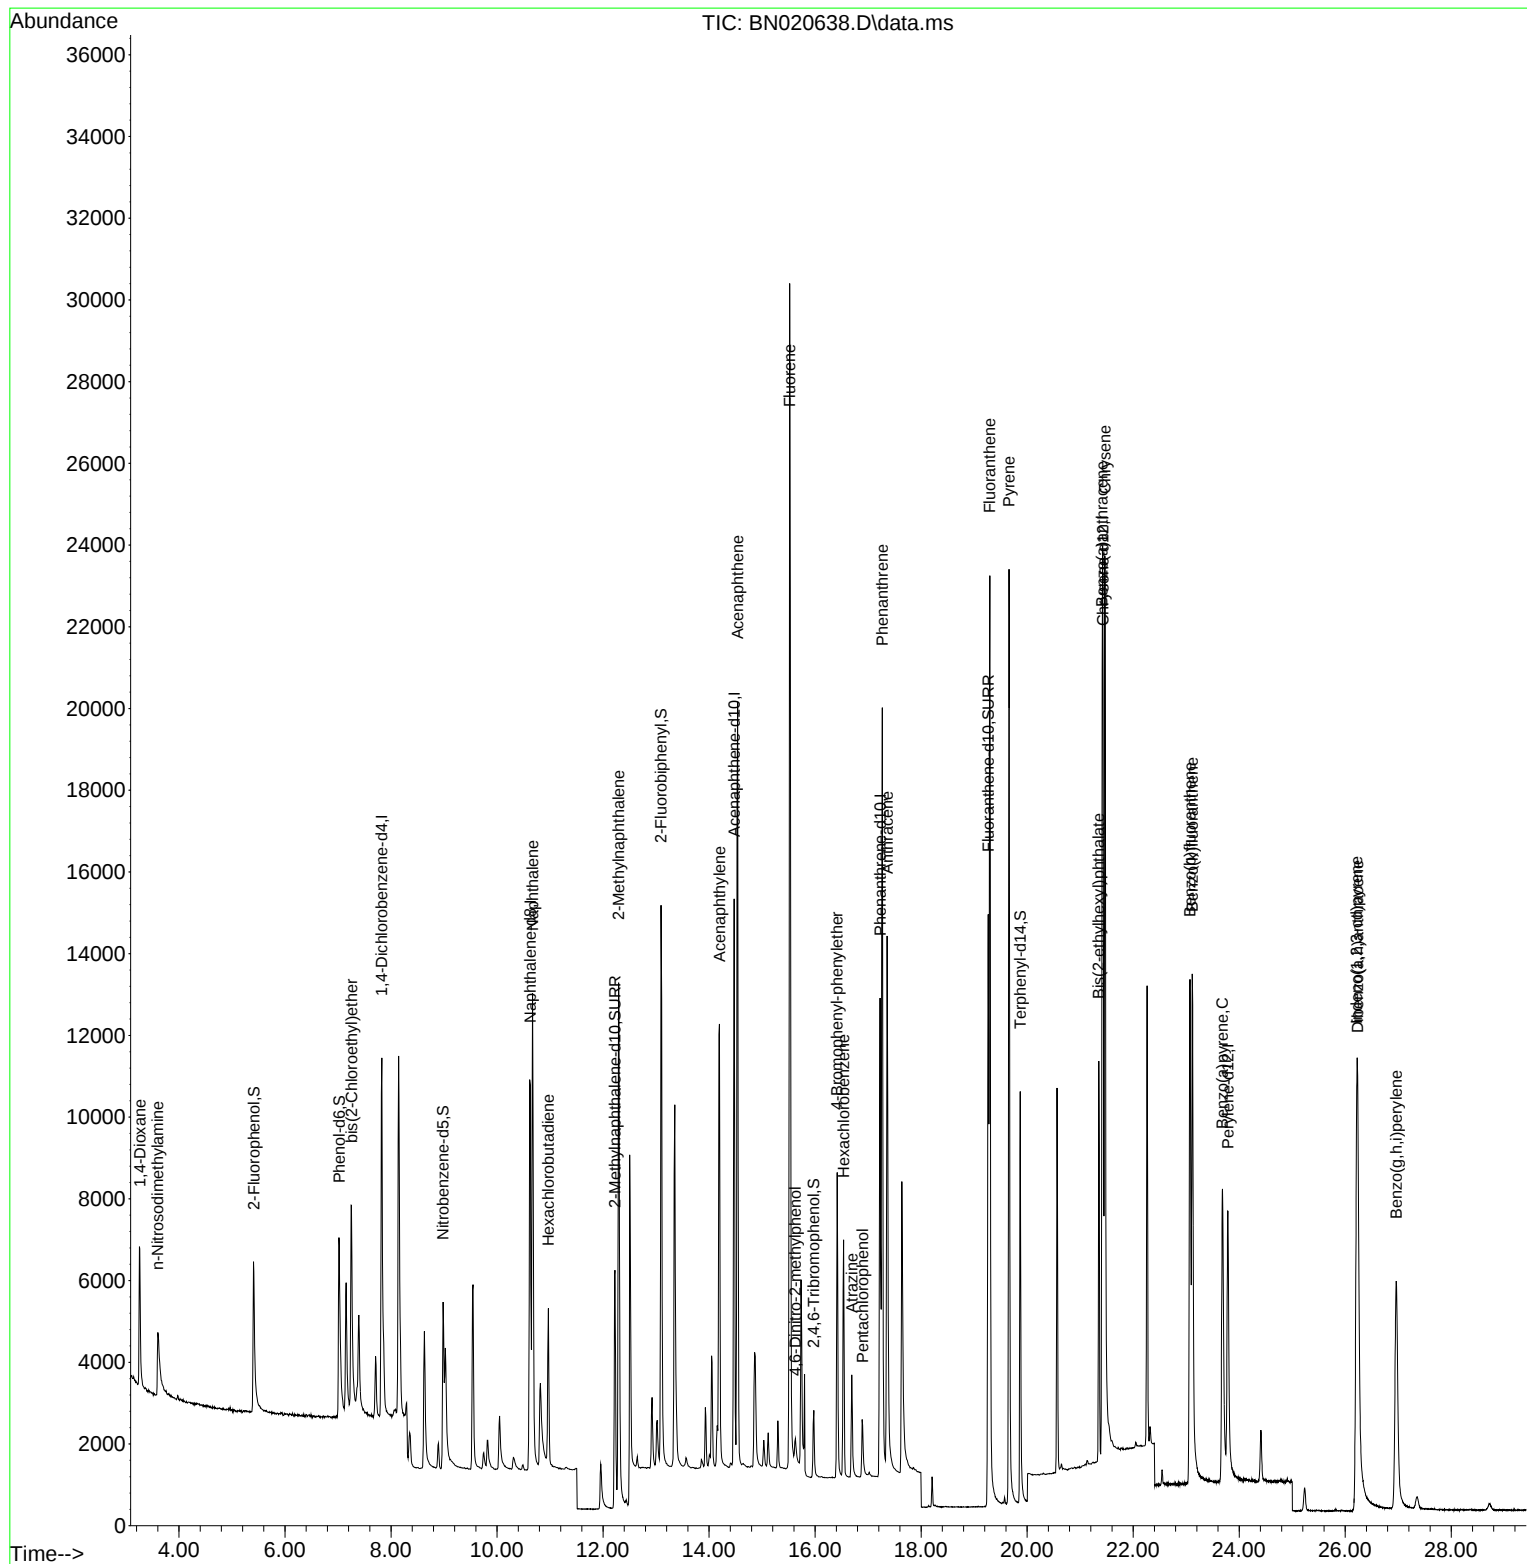





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.825 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN020638.D
 Acq: 02 Jul 2022 20:36

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC






Tgt Ion: 152 Resp: 4876
 Ion Ratio Lower Upper
 152 100
 150 155.6 127.9 191.9
 115 62.5 51.4 77.2

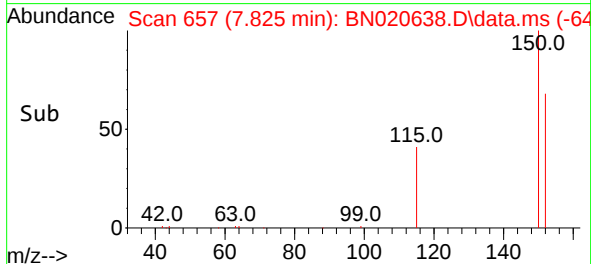

#2
 1,4-Dioxane
 Concen: 0.352 ng
 RT: 3.261 min Scan# 25
 Delta R.T. 0.000 min
 Lab File: BN020638.D
 Acq: 02 Jul 2022 20:36

Tgt Ion: 88 Resp: 2250
 Ion Ratio Lower Upper
 88 100
 43 36.8 30.2 45.2
 58 90.3 73.0 109.6



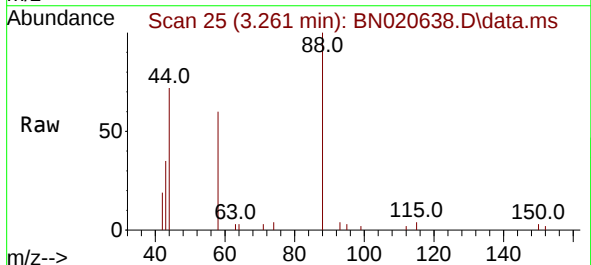




#3
n-Nitrosodimethylamine
Concen: 0.330 ng
RT: 3.600 min Scan# 71
Delta R.T. -0.007 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 1922
Ion Ratio Lower Upper
42 100
74 106.6 84.0 126.0
44 8.8 9.8 14.8#

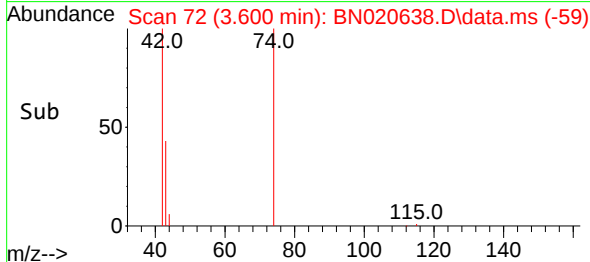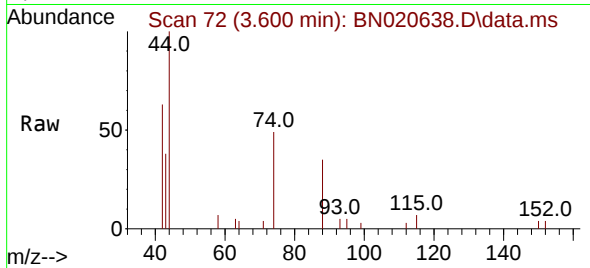

#4
2-Fluorophenol
Concen: 0.316 ng
RT: 5.413 min Scan# 323
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion: 112 Resp: 4279
Ion Ratio Lower Upper
112 100
64 63.5 49.1 73.7
63 34.2 26.3 39.5


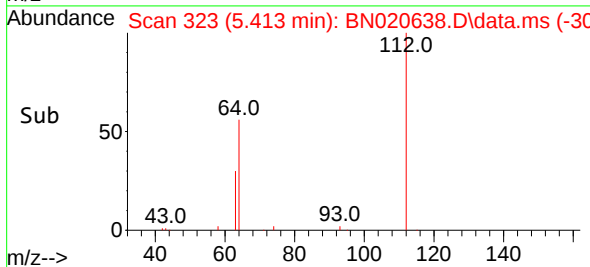

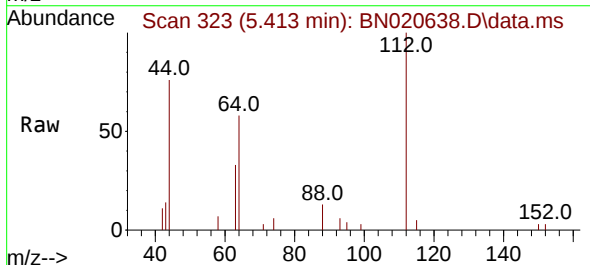


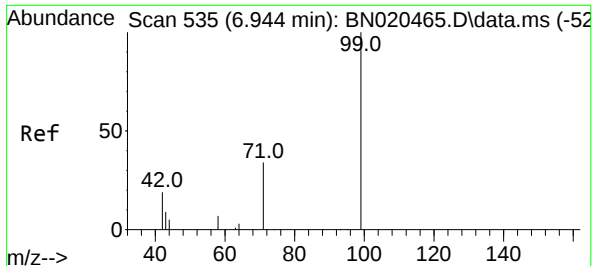

#5
Phenol-d6
Concen: 0.341 ng
RT: 7.024 min Scan# 54
Delta R.T. -0.007 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 99 Resp: 5515
Ion Ratio Lower Upper
99 100
42 23.0 19.3 28.9
71 35.0 27.5 41.3

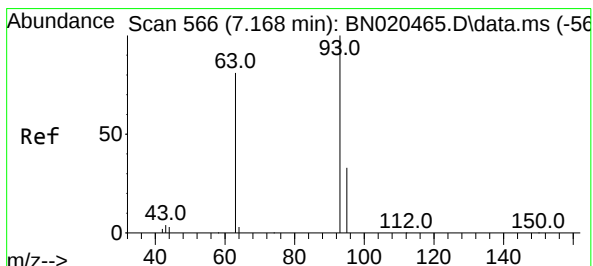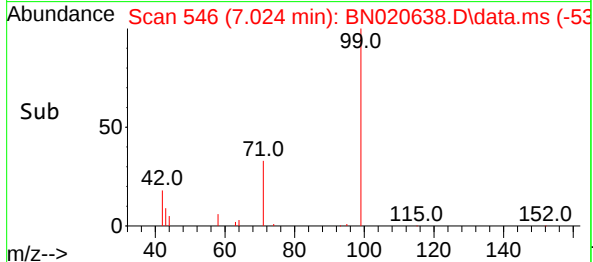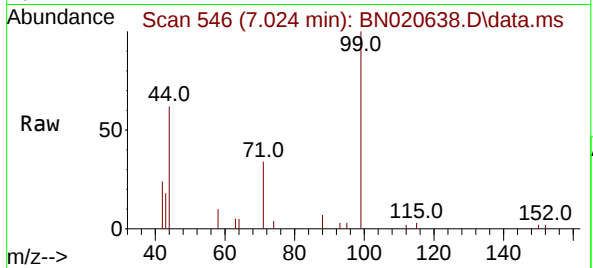

#6
bis(2-Chloroethyl)ether
Concen: 0.363 ng
RT: 7.255 min Scan# 578
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion: 93 Resp: 5048
Ion Ratio Lower Upper
93 100
63 85.0 67.4 101.0
95 34.0 26.5 39.7

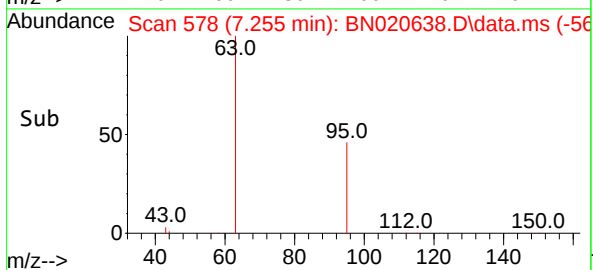

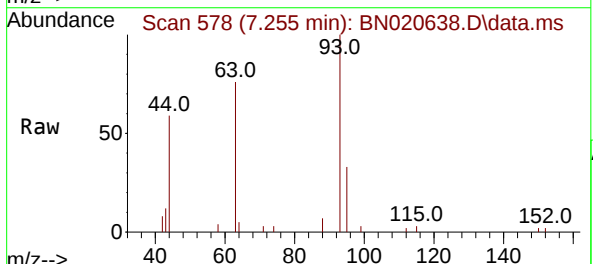




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.626 min Scan# 941
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:136	Resp:	14808
Ion Ratio	Lower	Upper
136	100	
137	11.1	9.0 13.6
54	7.9	6.2 9.2
68	5.3	4.4 6.6

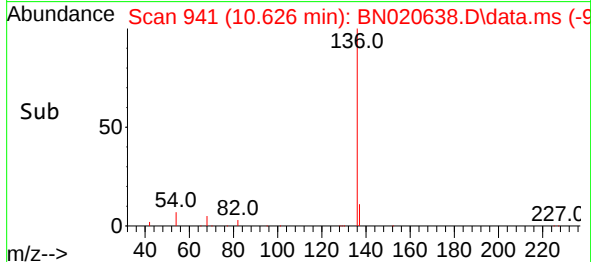

#8
Nitrobenzene-d5
Concen: 0.354 ng
RT: 8.982 min Scan# 787
Delta R.T. -0.011 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion: 82	Resp:	4244
Ion Ratio	Lower	Upper
82	100	
128	38.0	35.0 52.6
54	62.9	46.2 69.4

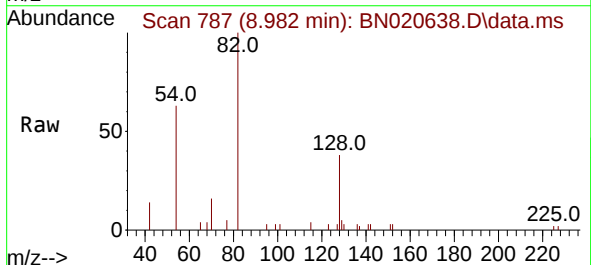

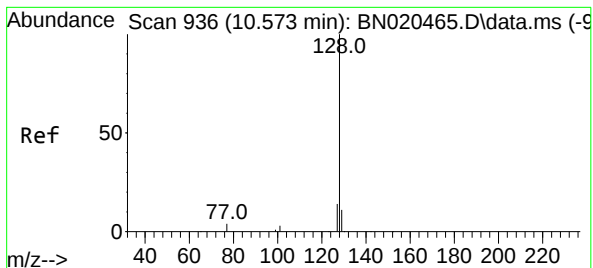

#9

Naphthalene

Concen: 0.382 ng

RT: 10.669 min Scan# 945

Delta R.T. -0.011 min

Lab File: BN020638.D

Acq: 02 Jul 2022 20:36

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:128 Resp: 16905

Ion Ratio Lower Upper

128 100

129 11.5 8.9 13.3

127 13.8 10.8 16.2

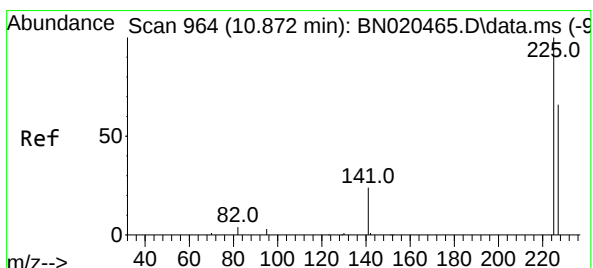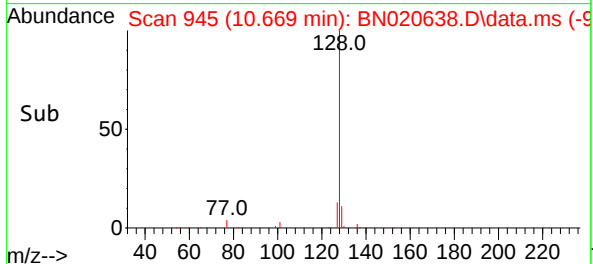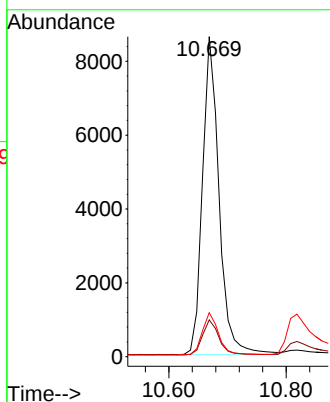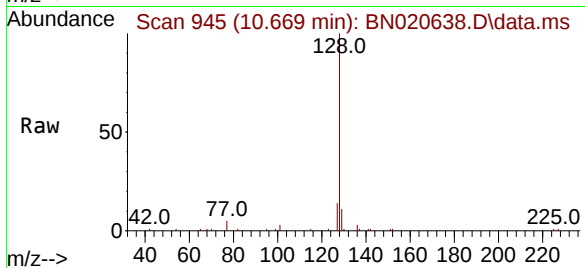

#10

Hexachlorobutadiene

Concen: 0.375 ng

RT: 10.968 min Scan# 973

Delta R.T. 0.000 min

Lab File: BN020638.D

Acq: 02 Jul 2022 20:36




Tgt Ion:225 Resp: 3023

Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 65.0 50.9 76.3


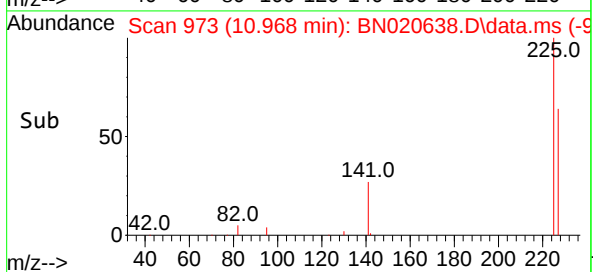
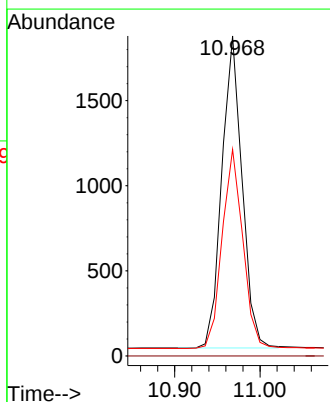
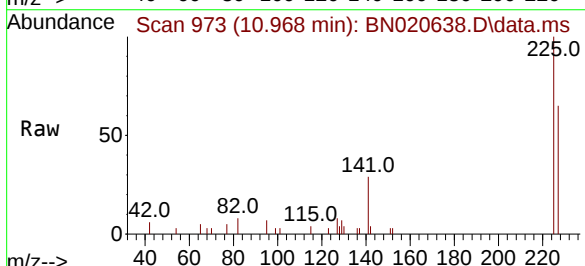




#11
2-Methylnaphthalene-d10
Concen: 0.367 ng
RT: 12.223 min Scan# 1185
Delta R.T. -0.004 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:152 Resp: 9319
Ion Ratio Lower Upper
152 100
151 20.7 16.2 24.4

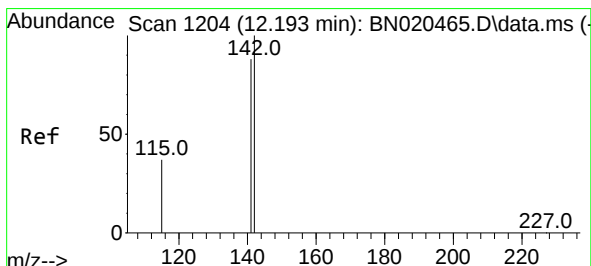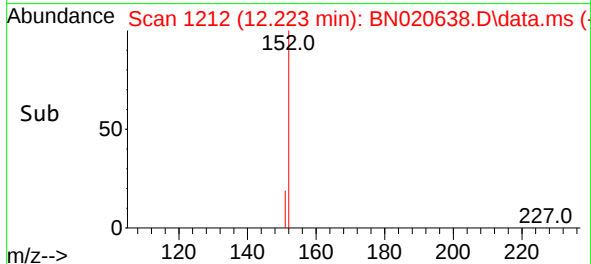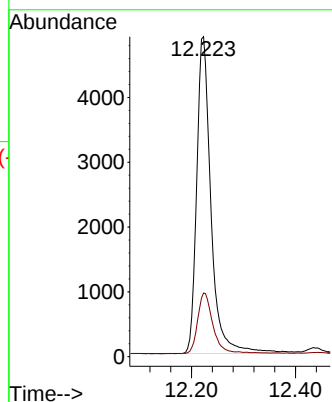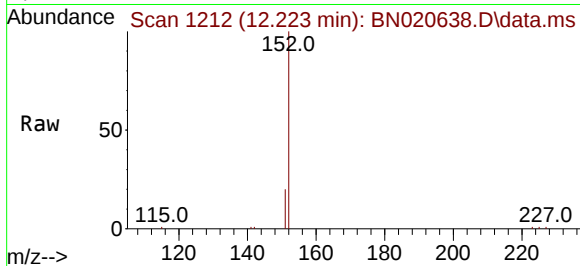

#12
2-Methylnaphthalene
Concen: 0.374 ng
RT: 12.295 min Scan# 1231
Delta R.T. -0.004 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:142 Resp: 11008
Ion Ratio Lower Upper
142 100
141 89.7 71.6 107.4
115 38.4 29.8 44.8



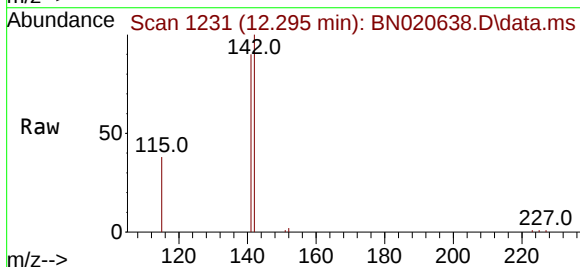




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.474 min Scan# 14
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:164 Resp: 8104
Ion Ratio Lower Upper
164 100
162 102.0 82.1 123.1
160 47.7 38.6 58.0

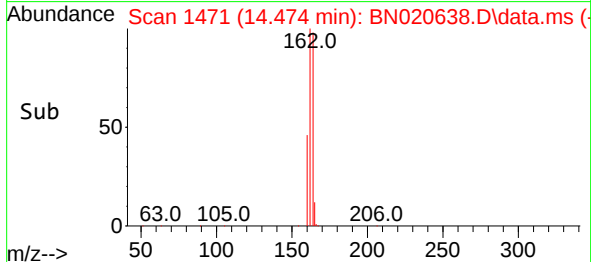

#14
2,4,6-Tribromophenol
Concen: 0.312 ng
RT: 15.974 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:330 Resp: 952
Ion Ratio Lower Upper
330 100
332 95.9 77.6 116.4
141 55.4 41.0 61.4



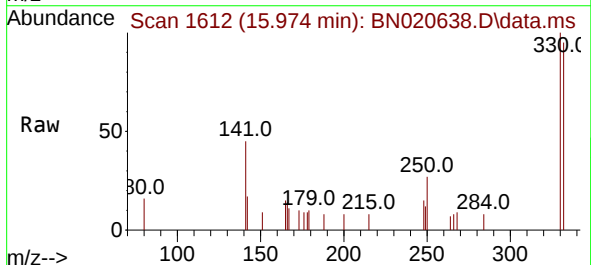




#15
2-Fluorobiphenyl
Concen: 0.401 ng
RT: 13.095 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172 Resp: 13404
Ion Ratio Lower Upper
172 100
171 36.3 27.2 40.8
170 24.5 18.2 27.4

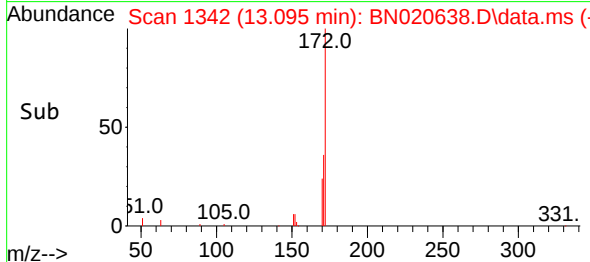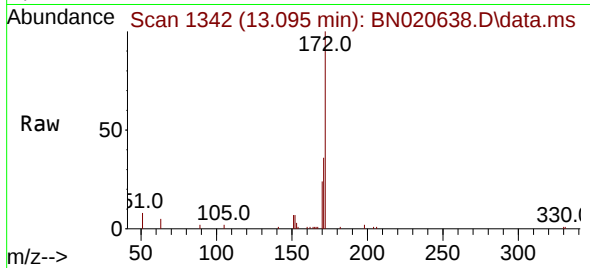

#16
Acenaphthylene
Concen: 0.364 ng
RT: 14.196 min Scan# 1445
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:152 Resp: 14180
Ion Ratio Lower Upper
152 100
151 19.4 16.2 24.4
153 13.0 10.7 16.1

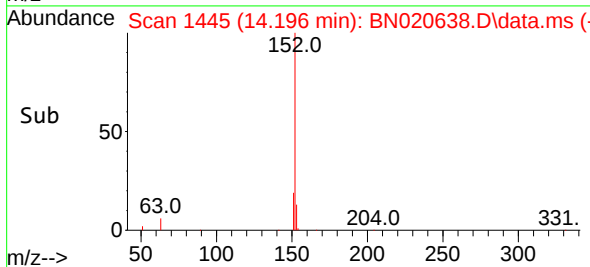

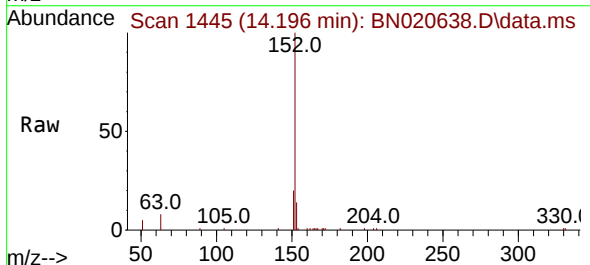


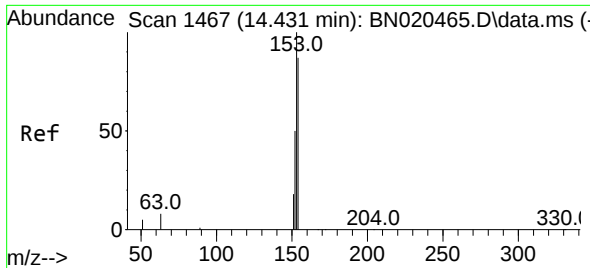

#17
Acenaphthene
Concen: 0.381 ng
RT: 14.538 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:154 Resp: 10094
Ion Ratio Lower Upper
154 100
153 114.4 87.5 131.3
152 56.9 43.8 65.6

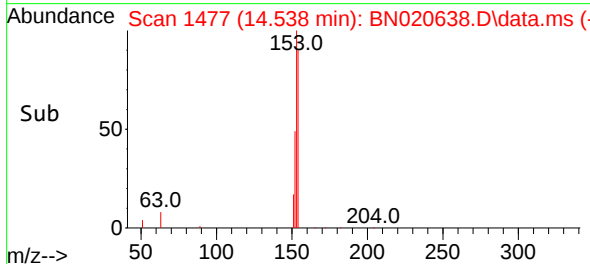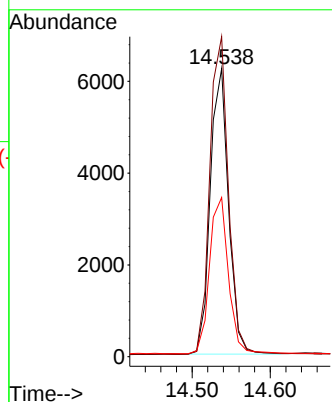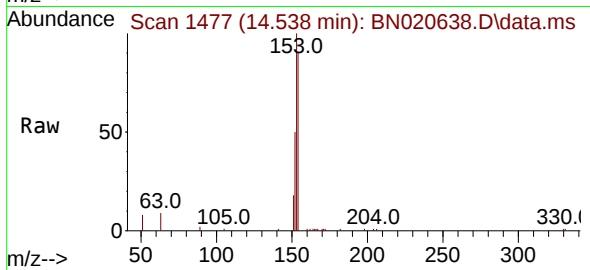

#18
Fluorene
Concen: 0.370 ng
RT: 15.521 min Scan# 1569
Delta R.T. -0.011 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:166 Resp: 12790
Ion Ratio Lower Upper
166 100
165 98.1 78.6 118.0
167 13.4 10.8 16.2


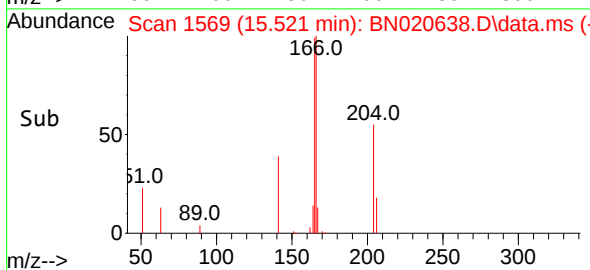
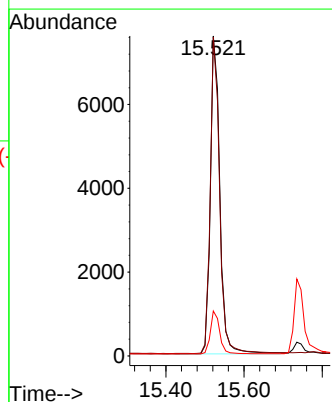
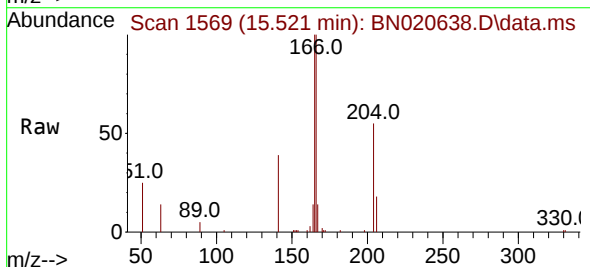




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.225 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:188 Resp: 16607
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.5 7.4 11.2

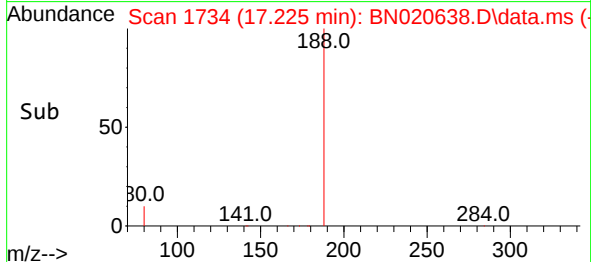

#20
4,6-Dinitro-2-methylphenol
Concen: 0.414 ng
RT: 15.628 min Scan# 1579
Delta R.T. -0.011 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:198 Resp: 614
Ion Ratio Lower Upper
198 100
182 23.7 12.1 18.1#
77 0.0 0.0 0.0




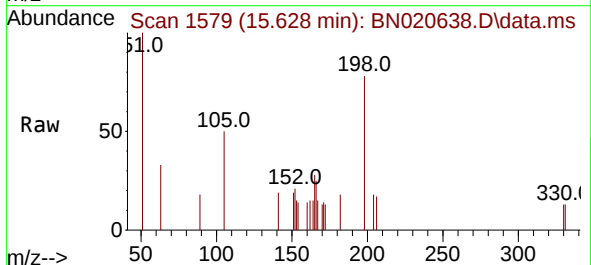




#21
4-Bromophenyl-phenylether
Concen: 0.394 ng
RT: 16.415 min Scan# 1665
Delta R.T. -0.010 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 3803
Ion Ratio Lower Upper
248 100
250 92.3 75.3 112.9
141 88.1 67.3 100.9

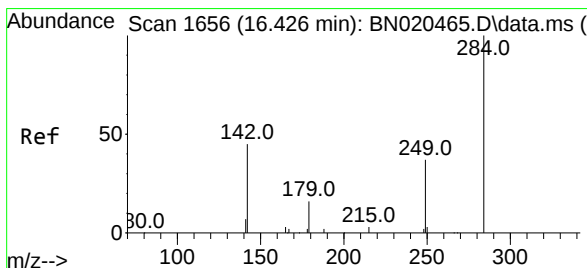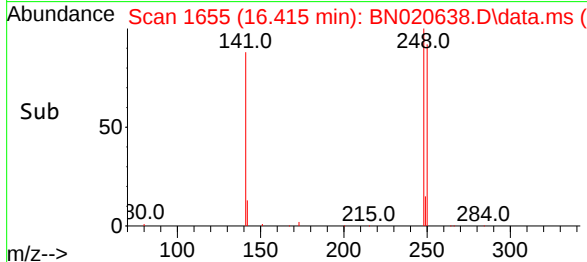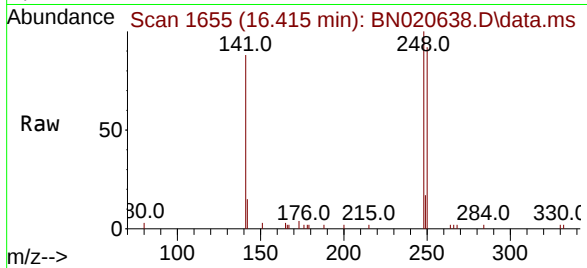

#22
Hexachlorobenzene
Concen: 0.396 ng
RT: 16.538 min Scan# 1667
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:284 Resp: 4232
Ion Ratio Lower Upper
284 100
142 45.5 35.2 52.8
249 33.7 26.6 40.0


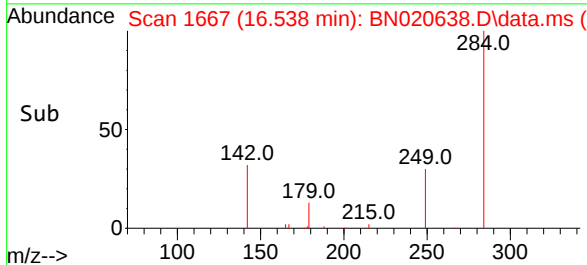

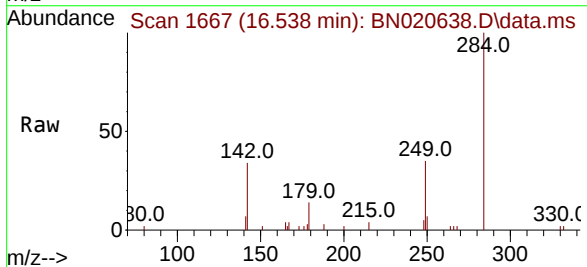


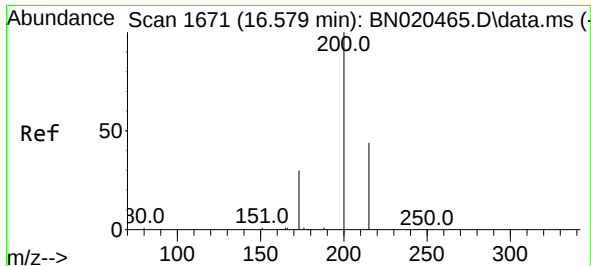

#23
 Atrazine
 Concen: 0.317 ng
 RT: 16.692 min Scan# 1702
 Delta R.T. 0.000 min
 Lab File: BN020638.D
 Acq: 02 Jul 2022 20:36




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:200 Resp: 2415
 Ion Ratio Lower Upper
 200 100
 173 30.9 23.6 35.4
 215 46.0 36.6 54.8

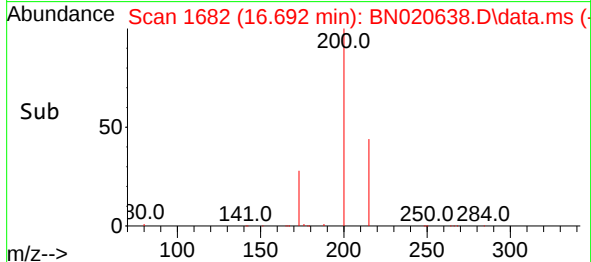

#24
 Pentachlorophenol
 Concen: 0.443 ng
 RT: 16.897 min Scan# 1702
 Delta R.T. 0.000 min
 Lab File: BN020638.D
 Acq: 02 Jul 2022 20:36

Tgt Ion:266 Resp: 887
 Ion Ratio Lower Upper
 266 100
 264 63.6 51.3 76.9
 268 66.1 52.6 79.0


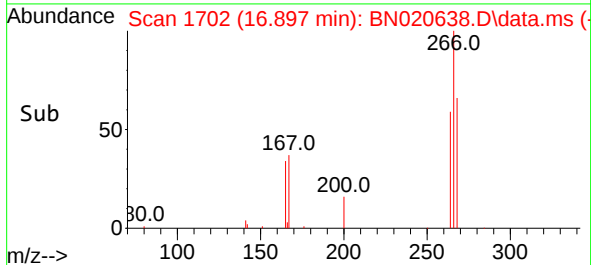






#25
Phenanthrene
Concen: 0.374 ng
RT: 17.266 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:178 Resp: 20930
Ion Ratio Lower Upper
178 100
176 19.4 15.3 22.9
179 15.3 12.2 18.4

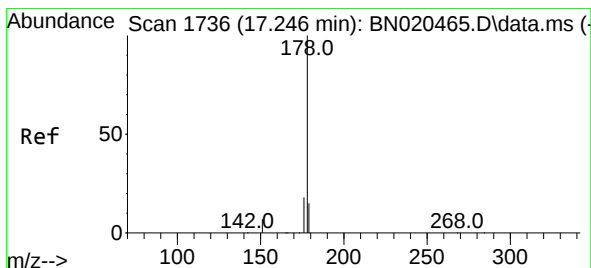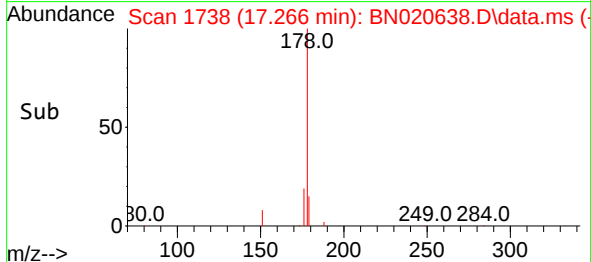

#26
Anthracene
Concen: 0.348 ng
RT: 17.359 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:178 Resp: 16816
Ion Ratio Lower Upper
178 100
176 18.5 14.9 22.3
179 15.2 12.2 18.4



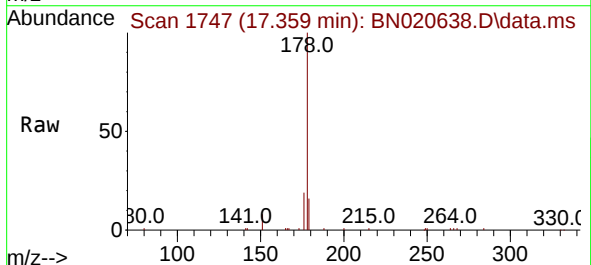




#27
Fluoranthene-d10
Concen: 0.365 ng
RT: 19.265 min Scan# 2109
Delta R.T. -0.004 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 18011
Ion Ratio Lower Upper
212 100
106 15.8 12.6 19.0
104 8.7 7.2 10.8

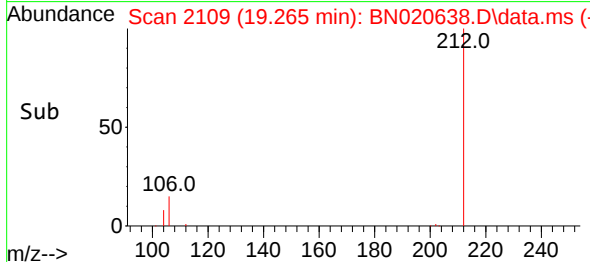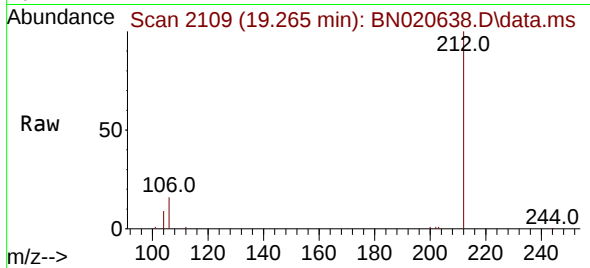

#28
Fluoranthene
Concen: 0.373 ng
RT: 19.295 min Scan# 2116
Delta R.T. -0.004 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:202 Resp: 22766
Ion Ratio Lower Upper
202 100
101 12.3 9.6 14.4
203 16.9 13.5 20.3


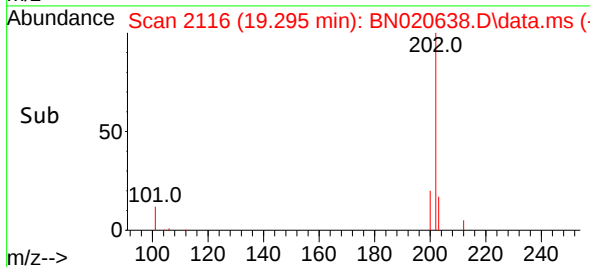

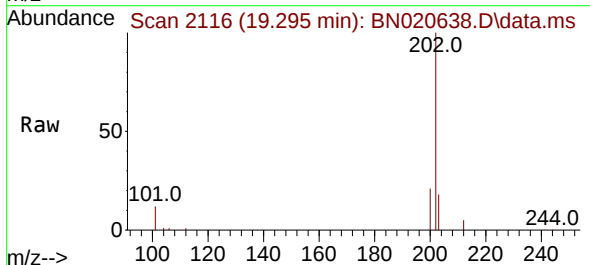


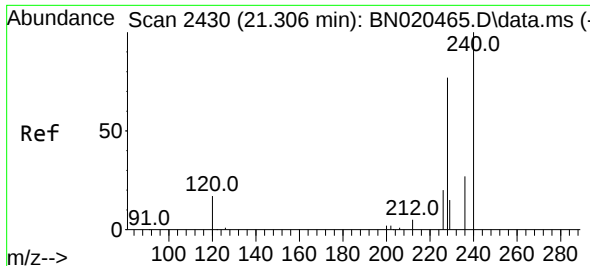

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.431 min Scan# 2444
Delta R.T. 0.000 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:240 Resp: 13320
Ion Ratio Lower Upper
240 100
120 12.7 14.6 21.8#
236 27.1 22.6 33.8

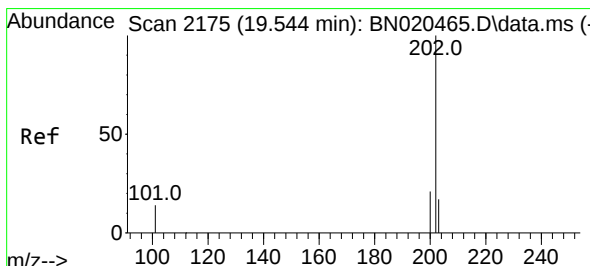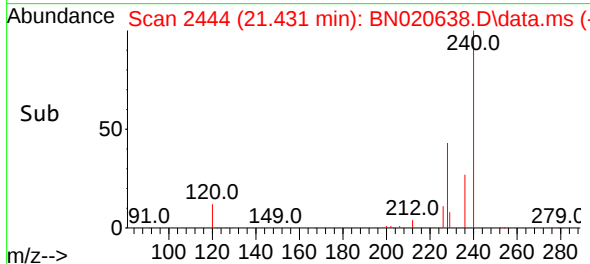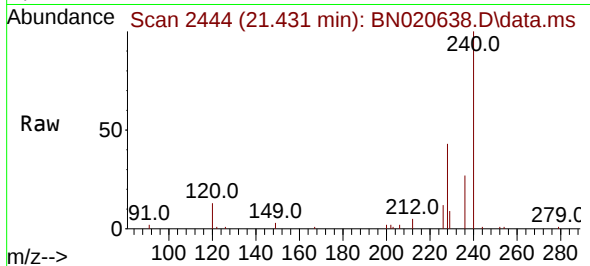

#30
Pyrene
Concen: 0.410 ng
RT: 19.657 min Scan# 2202
Delta R.T. -0.004 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:202 Resp: 23103
Ion Ratio Lower Upper
202 100
200 20.9 16.6 25.0
203 17.6 14.2 21.2

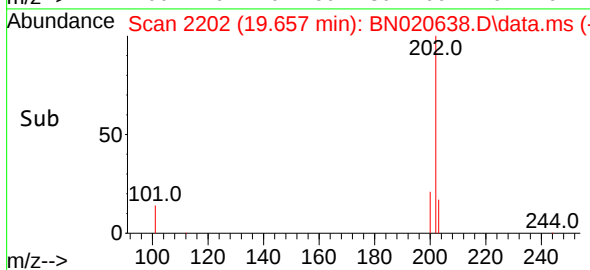

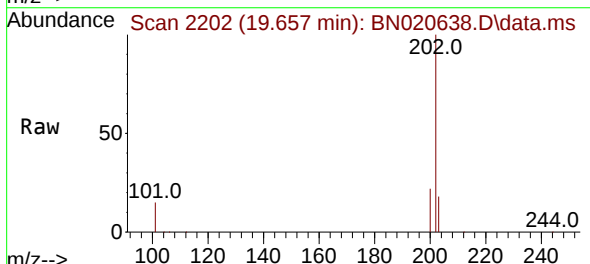




#31
 Terphenyl-d14
 Concen: 0.403 ng
 RT: 19.868 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN020638.D
 Acq: 02 Jul 2022 20:36




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:244 Resp: 12835
 Ion Ratio Lower Upper
 244 100
 212 9.2 7.1 10.7
 122 0.0 0.0 0.0

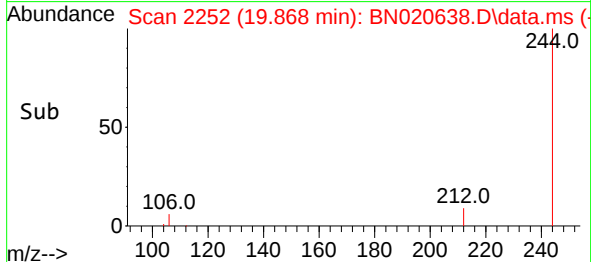

#32
 Benzo(a)anthracene
 Concen: 0.350 ng
 RT: 21.413 min Scan# 2442
 Delta R.T. -0.009 min
 Lab File: BN020638.D
 Acq: 02 Jul 2022 20:36

Tgt Ion:228 Resp: 16637
 Ion Ratio Lower Upper
 228 100
 226 27.4 21.2 31.8
 229 19.6 15.6 23.4

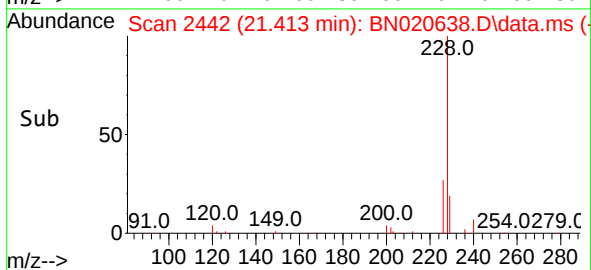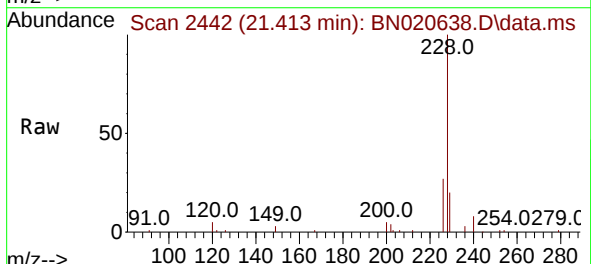



#33

Chrysene

Concen: 0.398 ng

RT: 21.467 min Scan# 2448

Delta R.T. 0.000 min

Lab File: BN020638.D

Acq: 02 Jul 2022 20:36

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC




Tgt Ion:228 Resp: 20965

Ion Ratio Lower Upper

228 100

226 30.3 23.4 35.0

229 19.9 15.7 23.5

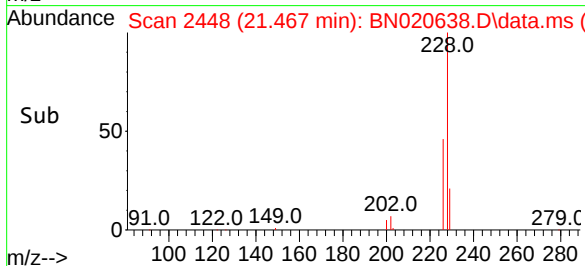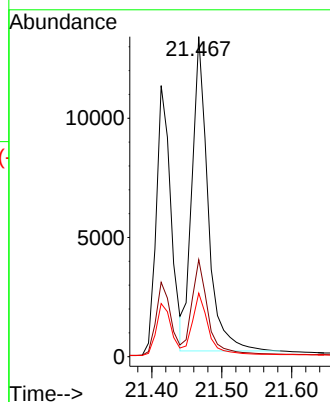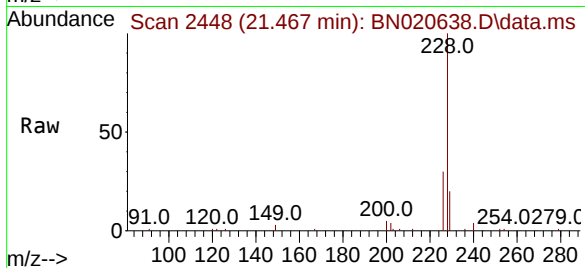

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.348 ng

RT: 21.351 min Scan# 2435

Delta R.T. 0.000 min

Lab File: BN020638.D

Acq: 02 Jul 2022 20:36




Tgt Ion:149 Resp: 9336

Ion Ratio Lower Upper

149 100

167 26.1 21.7 32.5

279 2.9 2.2 3.2

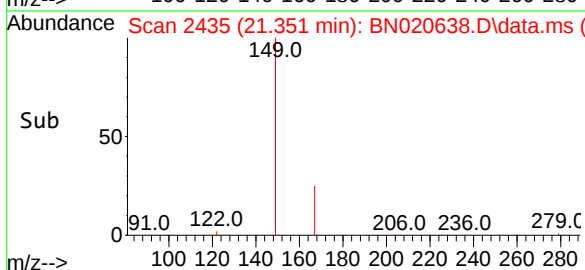

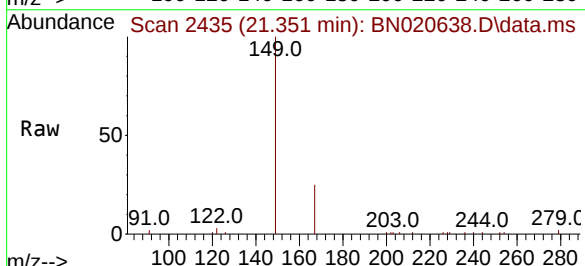




#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.787 min Scan# 30
 Delta R.T. -0.003 min
 Lab File: BN020638.D
 Acq: 02 Jul 2022 20:36




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:264 Resp: 10820
 Ion Ratio Lower Upper
 264 100
 260 26.2 20.9 31.3
 265 31.3 28.0 42.0

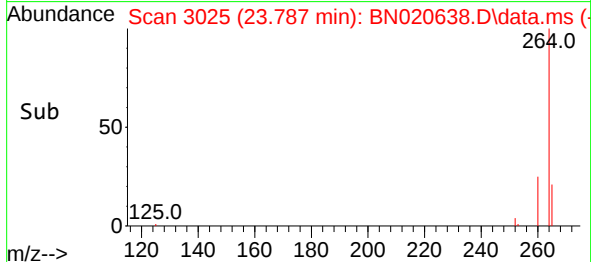

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.348 ng
 RT: 26.217 min Scan# 3856
 Delta R.T. -0.006 min
 Lab File: BN020638.D
 Acq: 02 Jul 2022 20:36

Tgt Ion:276 Resp: 16786
 Ion Ratio Lower Upper
 276 100
 138 33.6 25.9 38.9
 277 24.8 19.8 29.8



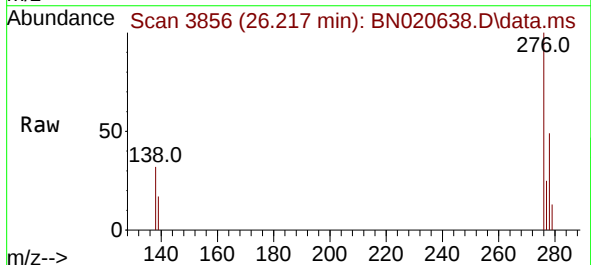




#37
Benzo(b)fluoranthene
Concen: 0.405 ng
RT: 23.071 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:252 Resp: 16899
Ion Ratio Lower Upper
252 100
253 24.1 18.5 27.7
125 15.1 11.4 17.0

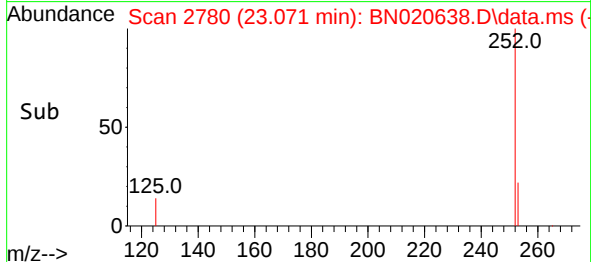

#38
Benzo(k)fluoranthene
Concen: 0.405 ng
RT: 23.115 min Scan# 2795
Delta R.T. -0.006 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36

Tgt Ion:252 Resp: 17987
Ion Ratio Lower Upper
252 100
253 23.6 18.0 27.0
125 13.8 11.0 16.4

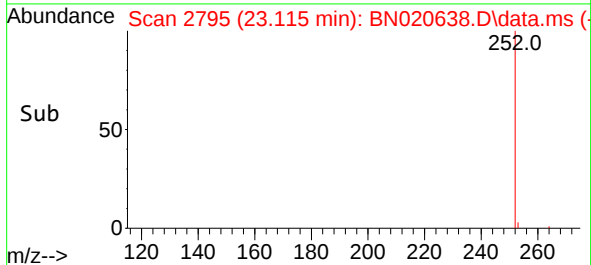






#39
Benzo(a)pyrene
Concen: 0.385 ng
RT: 23.682 min Scan# 2926
Delta R.T. -0.003 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:252 Resp: 13924
Ion Ratio Lower Upper
252 100
253 25.3 19.0 28.4
125 21.9 13.8 20.8#

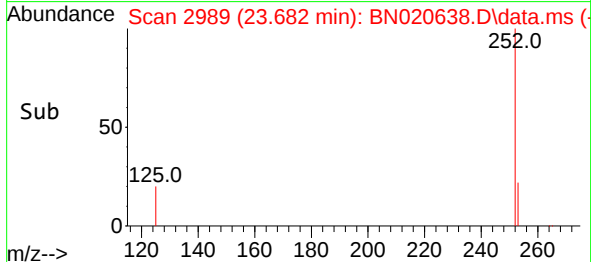

#40
Dibenzo(a,h)anthracene
Concen: 0.342 ng
RT: 26.237 min Scan# 3863
Delta R.T. -0.009 min
Lab File: BN020638.D
Acq: 02 Jul 2022 20:36


Tgt Ion:278 Resp: 13213
Ion Ratio Lower Upper
278 100
139 24.1 18.6 28.0
279 25.7 19.7 29.5

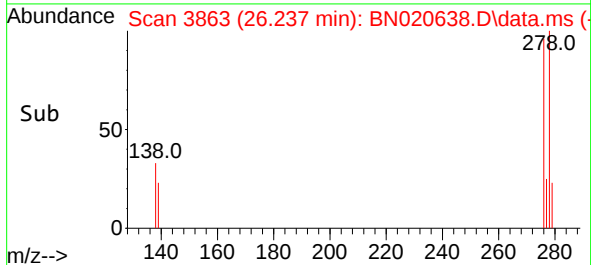



#41
 Benzo(g,h,i)perylene
 Concen: 0.333 ng
 RT: 26.962 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: BN020638.D
 Acq: 02 Jul 2022 20:36

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

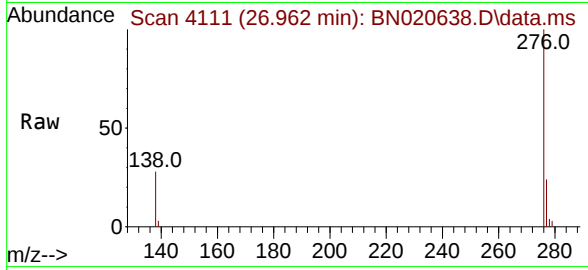

Tgt Ion:	276	Resp:	14043
Ion Ratio	Lower	Upper	
276	100		
277	24.4	19.5	29.3
138	28.5	22.6	34.0

