
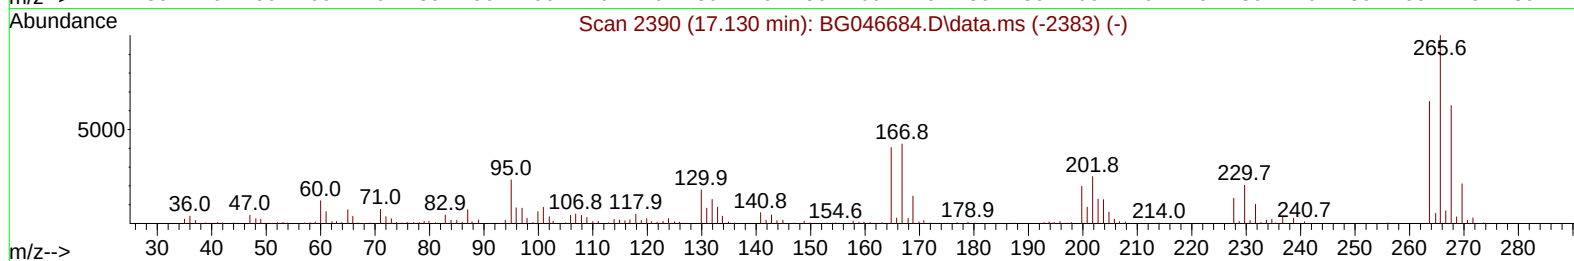
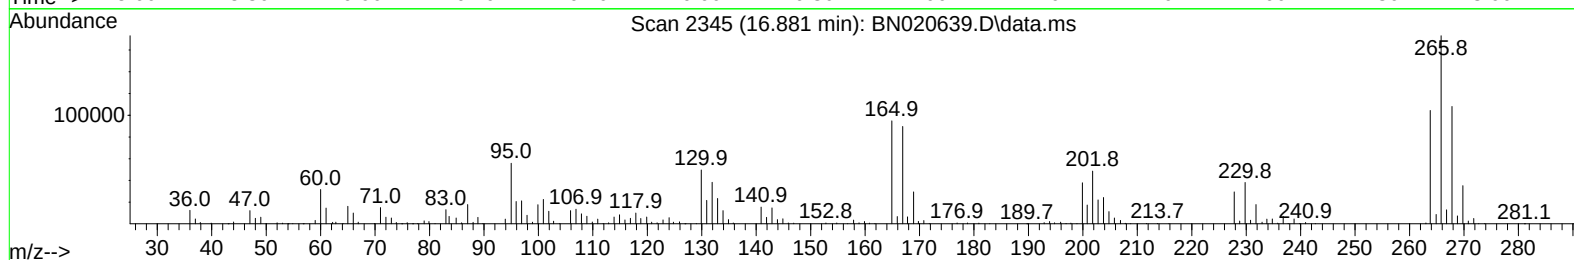


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070222\  
 Data File : BN020639.D  
 Acq On : 02 Jul 2022 21:49  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 39 Sample Multiplier: 1

Quant Time: Jul 04 05:04:18 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jul 04 05:02:31 2022  
 Response via : Initial Calibration

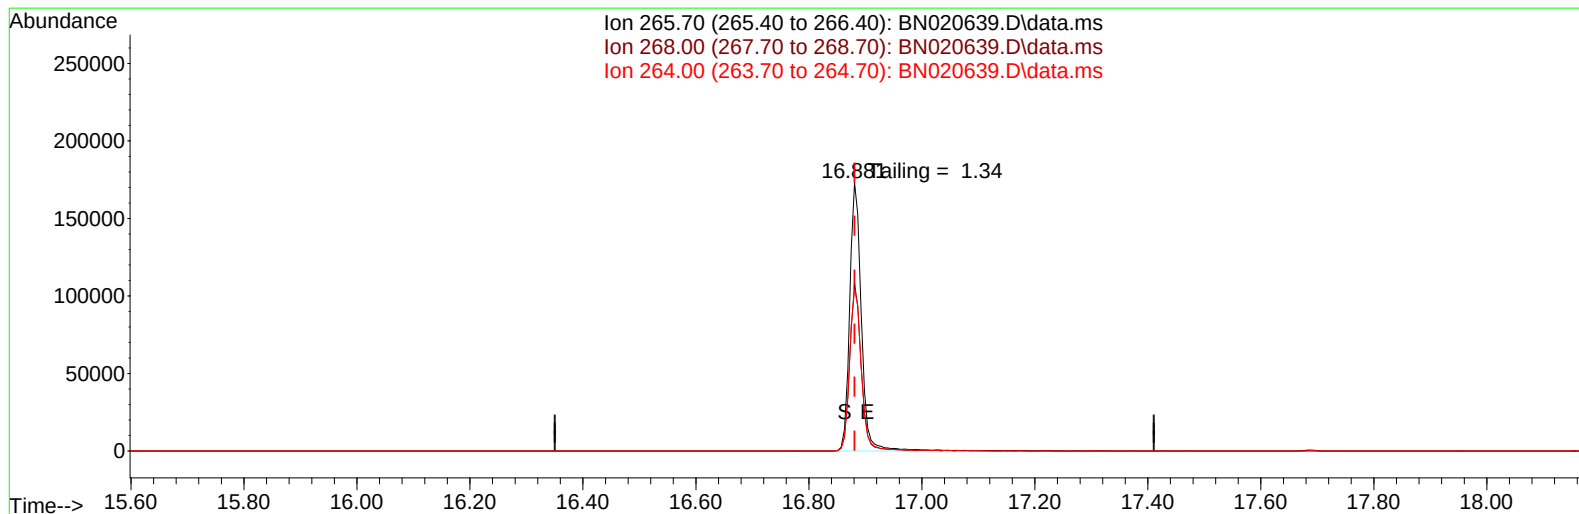

TIC: BN020639.D\data.ms

**(70) Pentachlorophenol (C)**




16.881min (-0.000) 16118.46 ng

response 248560

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 62.41  |
| 264.00 | 61.60  | 60.31  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070222\  
Data File : BN020639.D  
Acq On : 02 Jul 2022 21:49  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 39 Sample Multiplier: 1

Quant Time: Jul 04 05:04:18 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Jul 04 05:02:31 2022  
Response via : Initial Calibration

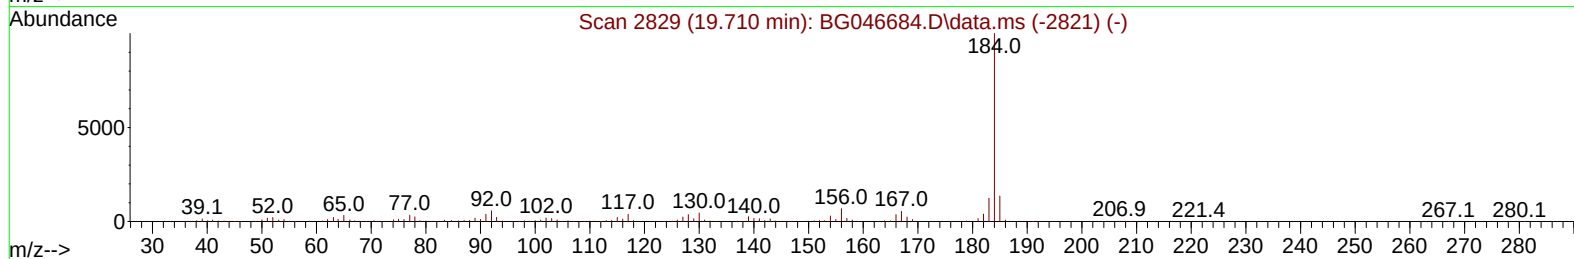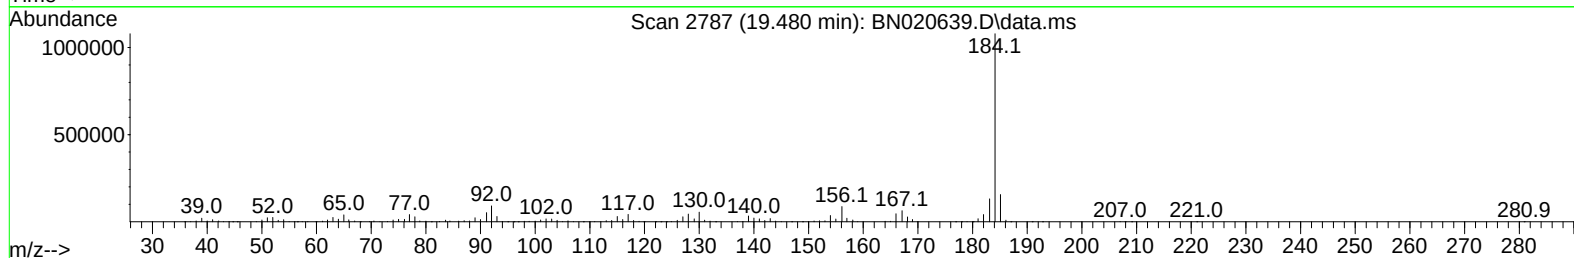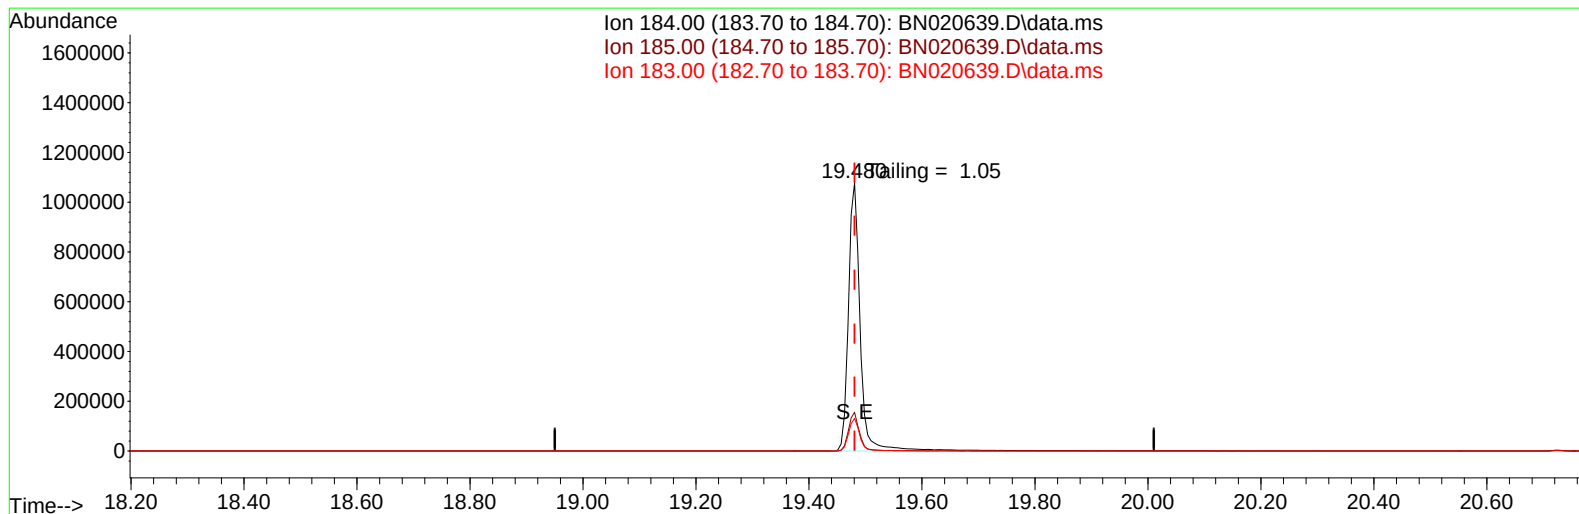

TIC: BN020639.D\data.ms

**(77) Benzidine**

19.480min (-0.000) 0.00 ng

response 1555270

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.45  |
| 183.00 | 13.20  | 12.17  |
| 0.00   | 0.00   | 0.00   |