Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
Data File : BN020605.D
Acq On : 01 Jul 2022 22:40
Operator : CG/JU
Sample : N3458-08MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

Quant Time: Jul 02 03:13:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 03:10:12 2022
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units		Dev(Min)
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.826	152	4170	0.400	ng		0.00
7) Naphthalene-d8	10.626	136	12368	0.400	ng	#	0.00
13) Acenaphthene-d10	14.474	164	6487	0.400	ng		0.00
19) Phenanthrene-d10	17.226	188	12588	0.400	ng	#	0.00
29) Chrysene-d12	21.431	240	10102	0.400	ng	#	0.00
35) Perylene-d12	23.782	264	7744	0.400	ng		0.00
System Monitoring Compounds							
4) 2-Fluorophenol	5.435	112	276	0.024	ng		0.02
5) Phenol-d6	7.060	99	71	0.005	ng		0.03
8) Nitrobenzene-d5	8.993	82	2386	0.238	ng		0.00
11) 2-Methylnaphthalene-d10	12.227	152	6585	0.311	ng		0.00
14) 2,4,6-Tribromophenol	15.985	330	230	0.094	ng		0.01
15) 2-Fluorobiphenyl	13.105	172	7387	0.276	ng		0.00
27) Fluoranthene-d10	19.265	212	10996	0.294	ng		0.00
31) Terphenyl-d14	19.868	244	8149	0.338	ng		0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.254	88	12913	2.363	ng		95
3) n-Nitrosodimethylamine	3.615	42	503	0.101	ng	#	69
6) bis(2-Chloroethyl)ether	7.255	93	4191	0.352	ng		97
9) Naphthalene	10.680	128	12855	0.348	ng		99
10) Hexachlorobutadiene	10.968	225	2138	0.318	ng	#	100
12) 2-Methylnaphthalene	12.299	142	8166	0.333	ng		99
16) Acenaphthylene	14.196	152	10364	0.332	ng		99
17) Acenaphthene	14.538	154	7299	0.344	ng		96
18) Fluorene	15.532	166	9008	0.325	ng		99
20) 4,6-Dinitro-2-methylph...	15.693	198	34m	0.239	ng		
21) 4-Bromophenyl-phenylether	16.426	248	2709	0.370	ng	#	83
22) Hexachlorobenzene	16.538	284	3094	0.382	ng		97
23) Atrazine	16.692	200	1993	0.345	ng		97
24) Pentachlorophenol	16.897	266	295	0.297	ng		89
25) Phenanthrene	17.267	178	16040	0.378	ng		100
26) Anthracene	17.359	178	13396	0.366	ng		100
28) Fluoranthene	19.295	202	18054	0.390	ng		100
30) Pyrene	19.662	202	18222	0.426	ng		100
32) Benzo(a)anthracene	21.413	228	13634	0.378	ng		98
33) Chrysene	21.467	228	16098	0.403	ng		99
34) Bis(2-ethylhexyl)phtha...	21.351	149	7718	0.380	ng		98
36) Indeno(1,2,3-cd)pyrene	26.223	276	11141	0.323	ng		99
37) Benzo(b)fluoranthene	23.068	252	13391	0.449	ng		99
38) Benzo(k)fluoranthene	23.115	252	13572	0.427	ng		97
39) Benzo(a)pyrene	23.679	252	11186	0.432	ng		97
40) Dibenzo(a,h)anthracene	26.241	278	9797	0.354	ng		97
41) Benzo(g,h,i)perylene	26.969	276	10498	0.347	ng		99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
Data File : BN020605.D
Acq On : 01 Jul 2022 22:40
Operator : CG/JU
Sample : N3458-08MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jul 02 03:13:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 03:10:12 2022
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

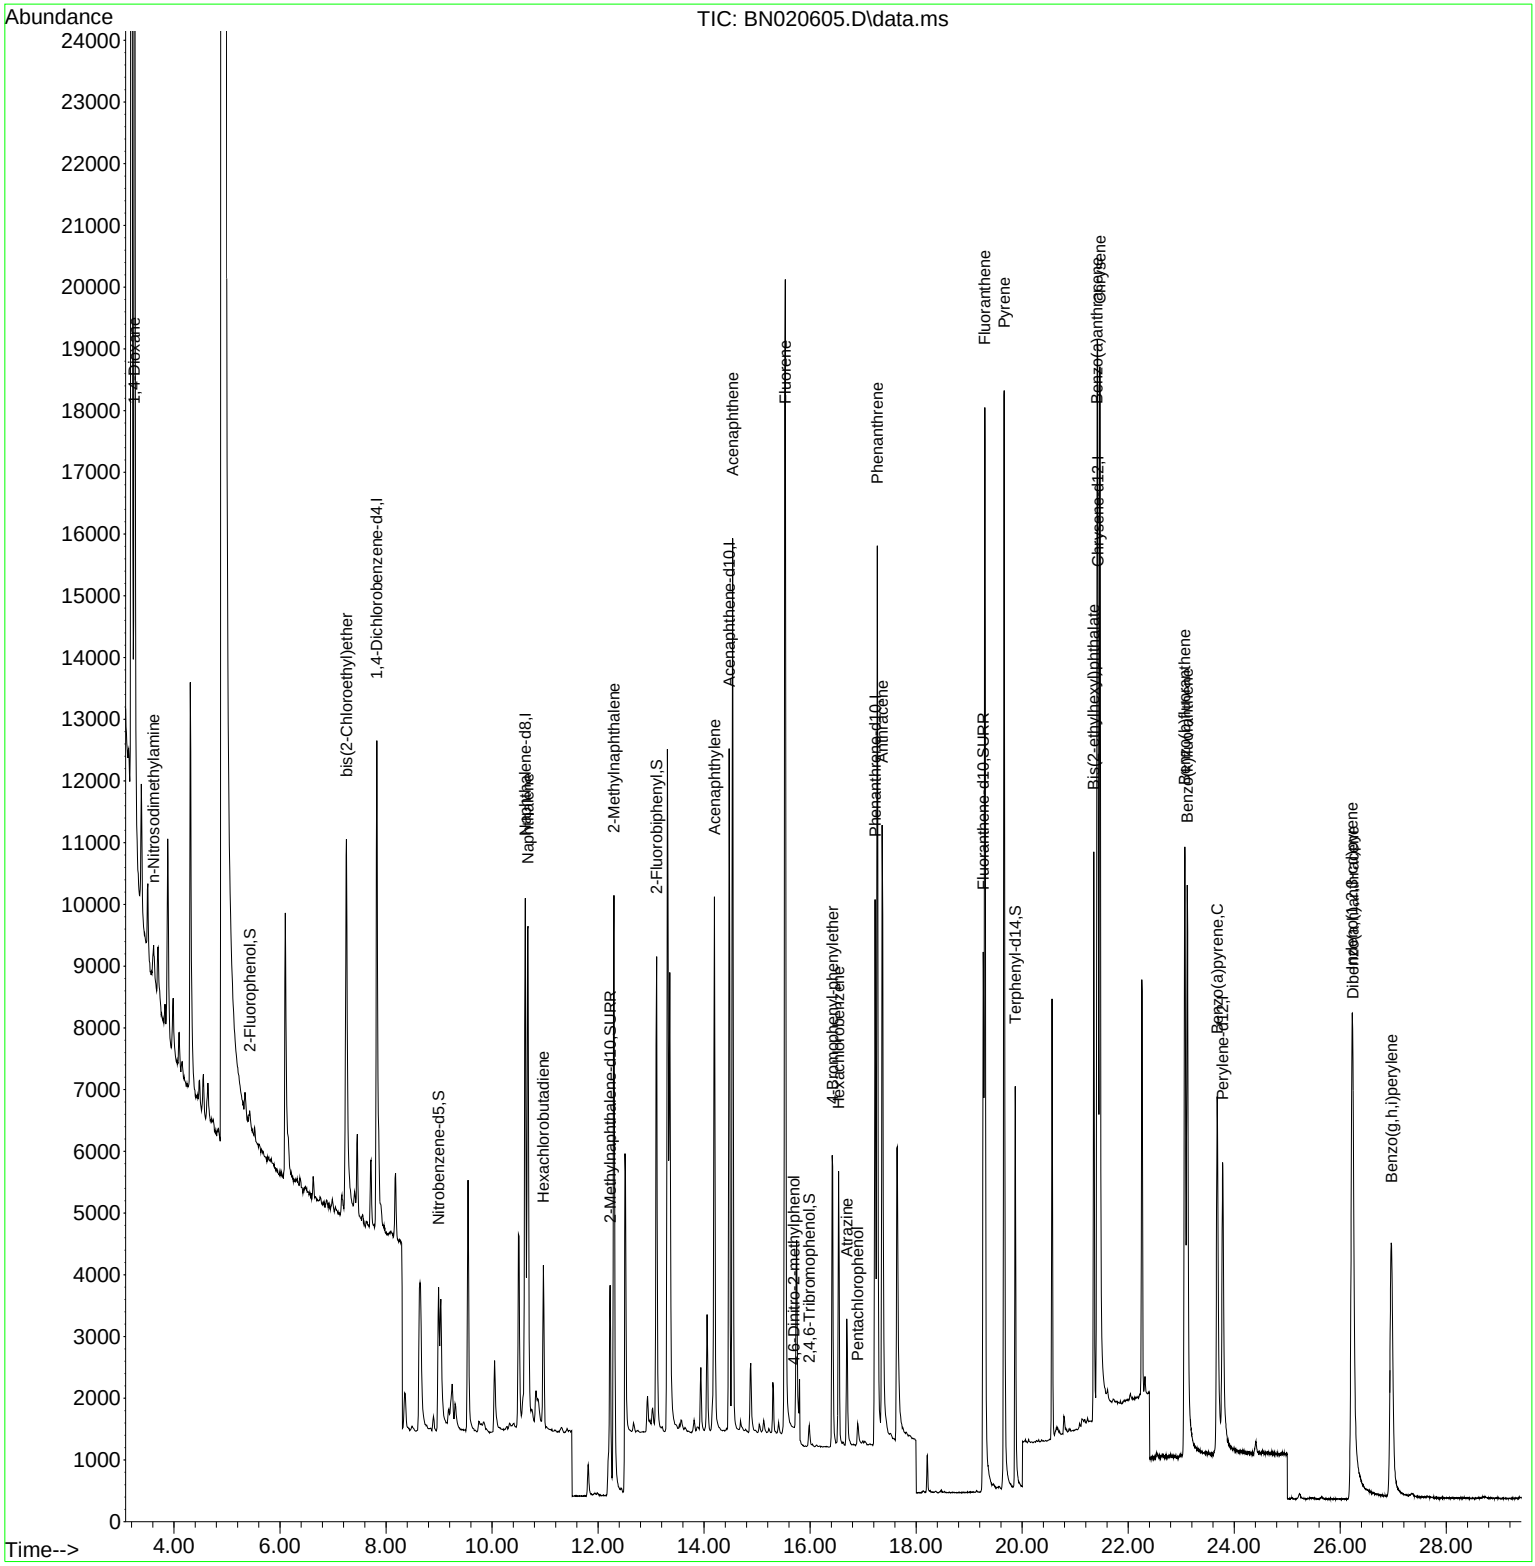

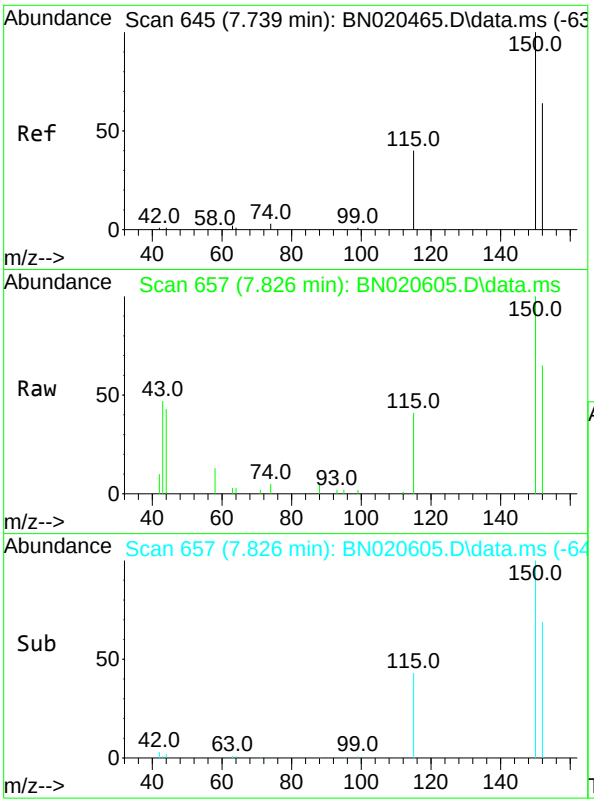

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.826 min Scan# 6
Delta R.T. 0.001 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:152 Resp: 417

Ion	Ratio	Lower	Upper
152	100		
150	154.9	127.9	191.9
115	63.9	51.4	77.2



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

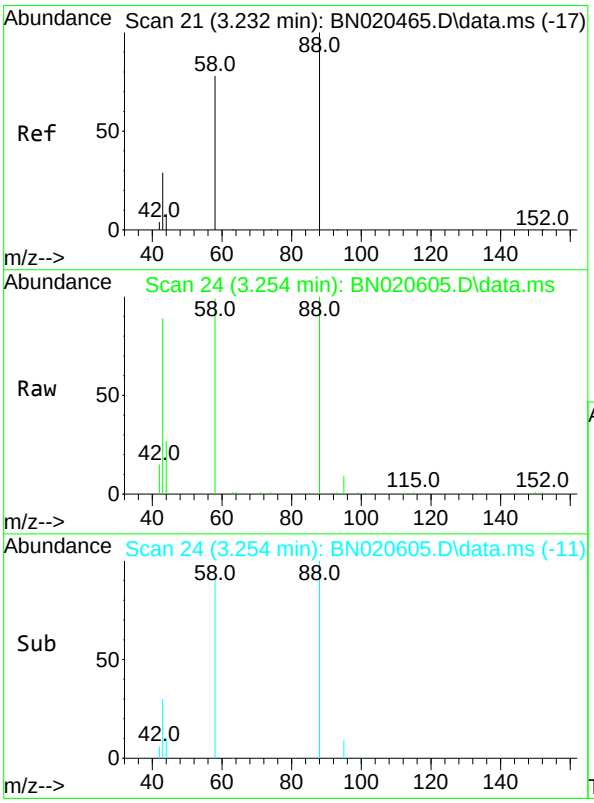

#2
1,4-Dioxane
Concen: 2.363 ng
RT: 3.254 min Scan# 24
Delta R.T. -0.007 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion: 88 Resp: 12913

Ion	Ratio	Lower	Upper
88	100		
43	38.0	30.2	45.2
58	85.3	73.0	109.6



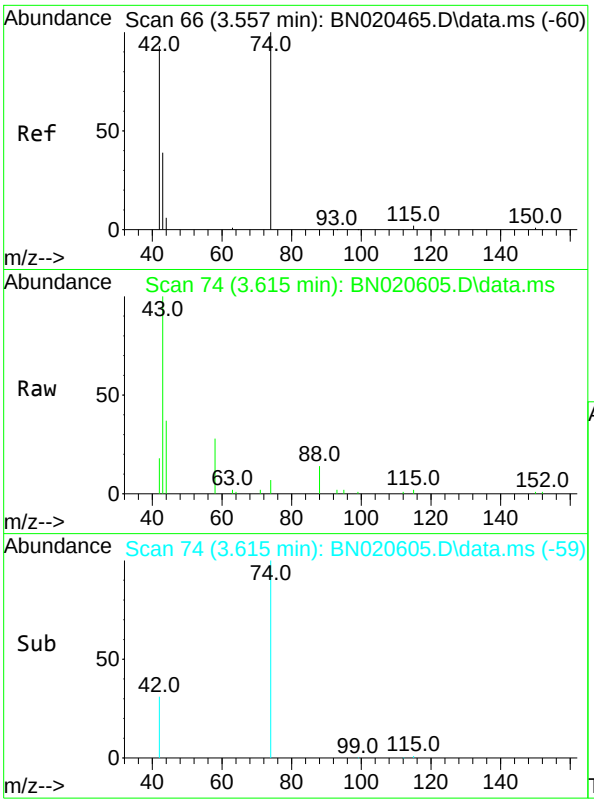

#3
n-Nitrosodimethylamine
Concen: 0.101 ng
RT: 3.615 min Scan# 7
Delta R.T. 0.007 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion: 42 Resp: 50

Ion	Ratio	Lower	Upper
42	100		
74	136.4	84.0	126.0#
44	0.0	9.8	14.8#



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

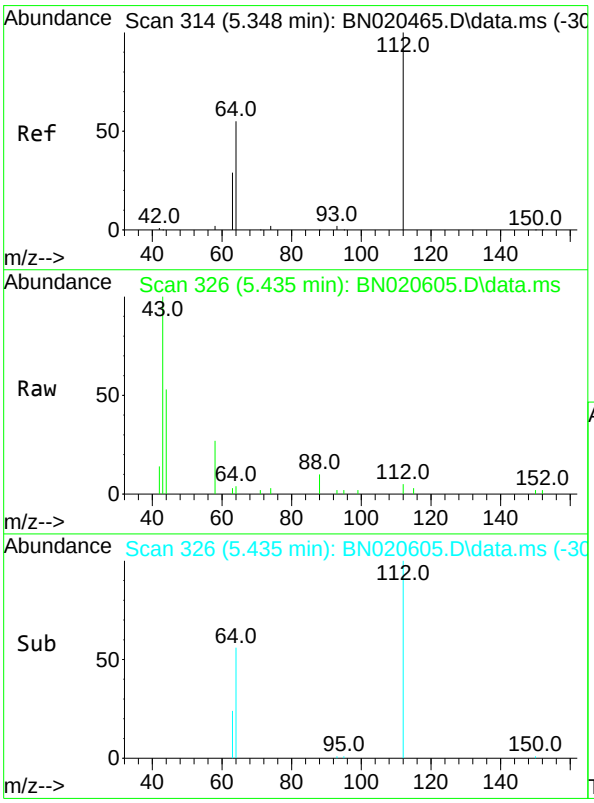

#4
2-Fluorophenol
Concen: 0.024 ng
RT: 5.435 min Scan# 326
Delta R.T. 0.022 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:112 Resp: 276

Ion	Ratio	Lower	Upper
112	100		
64	68.8	49.1	73.7
63	33.7	26.3	39.5



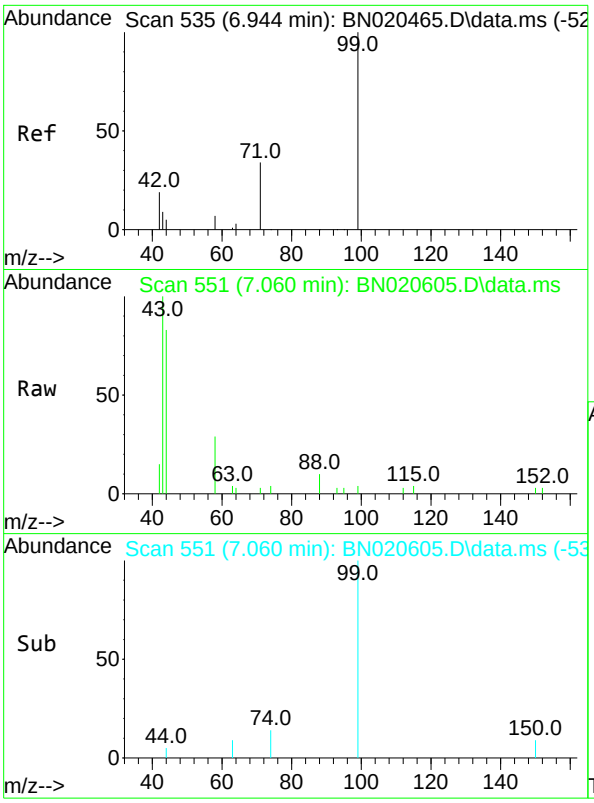

#5
Phenol-d6
Concen: 0.005 ng
RT: 7.060 min Scan# 5
Delta R.T. 0.029 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion: 99 Resp: 7

Ion	Ratio	Lower	Upper
99	100		
42	40.8	19.3	28.9#
71	25.4	27.5	41.3#



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

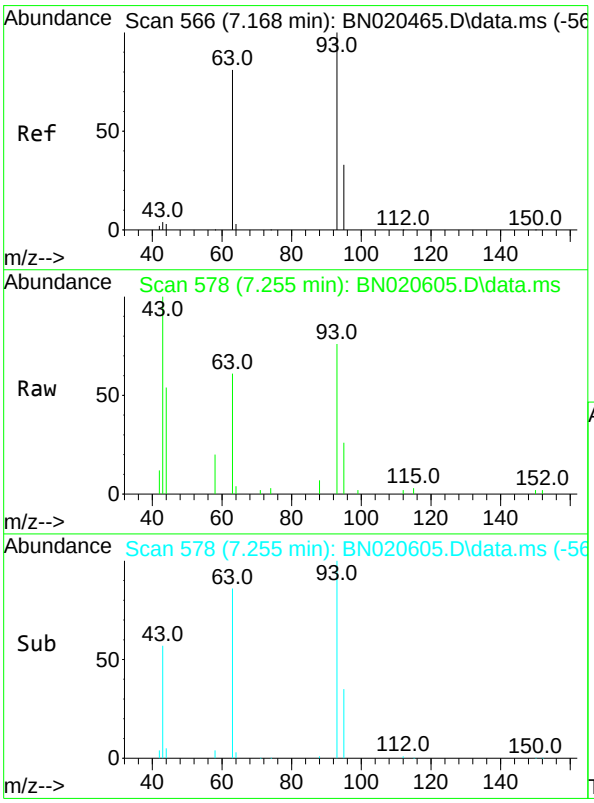

#6
bis(2-Chloroethyl)ether
Concen: 0.352 ng
RT: 7.255 min Scan# 578
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion: 93 Resp: 4191

Ion	Ratio	Lower	Upper
93	100		
63	87.1	67.4	101.0
95	34.4	26.5	39.7



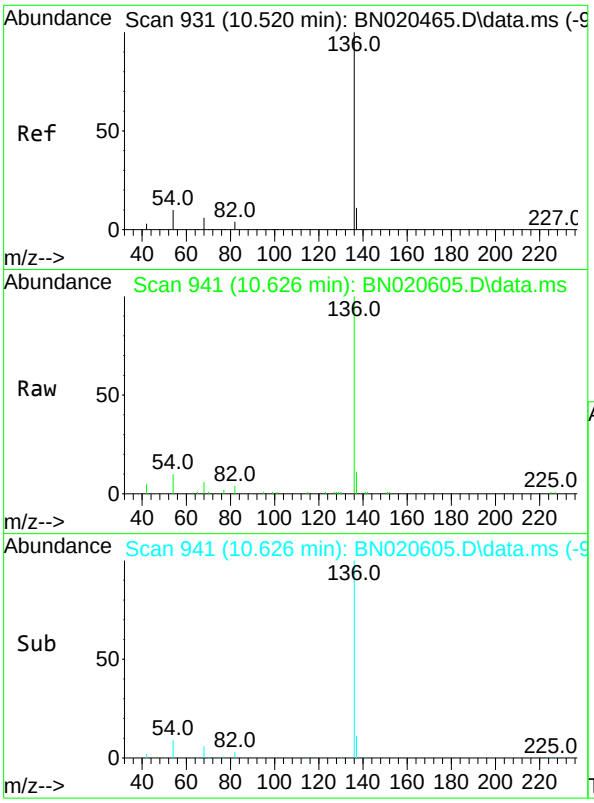

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.626 min Scan# 94
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:136 Resp: 1236

Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.0	13.6
54	9.8	6.2	9.2
68	6.5	4.4	6.6



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

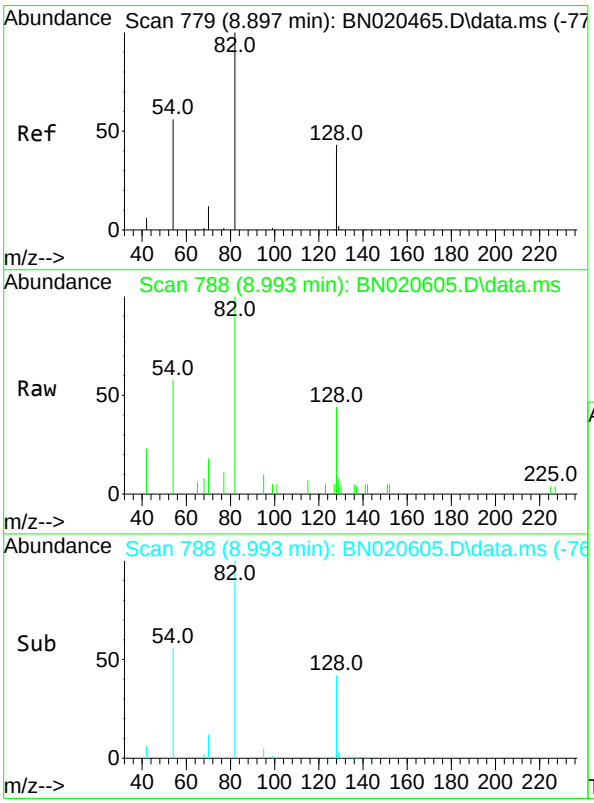

#8
Nitrobenzene-d5
Concen: 0.238 ng
RT: 8.993 min Scan# 788
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion: 82 Resp: 2386

Ion	Ratio	Lower	Upper
82	100		
128	44.4	35.0	52.6
54	58.4	46.2	69.4



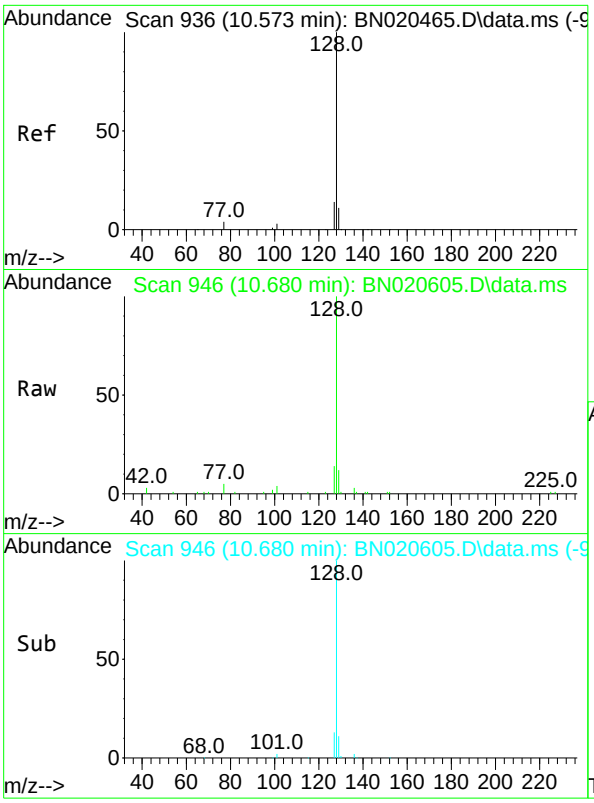

#9
Naphthalene
Concen: 0.348 ng
RT: 10.680 min Scan# 94
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:128 Resp: 1285

Ion	Ratio	Lower	Upper
128	100		
129	11.6	8.9	13.3
127	13.6	10.8	16.2

Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022



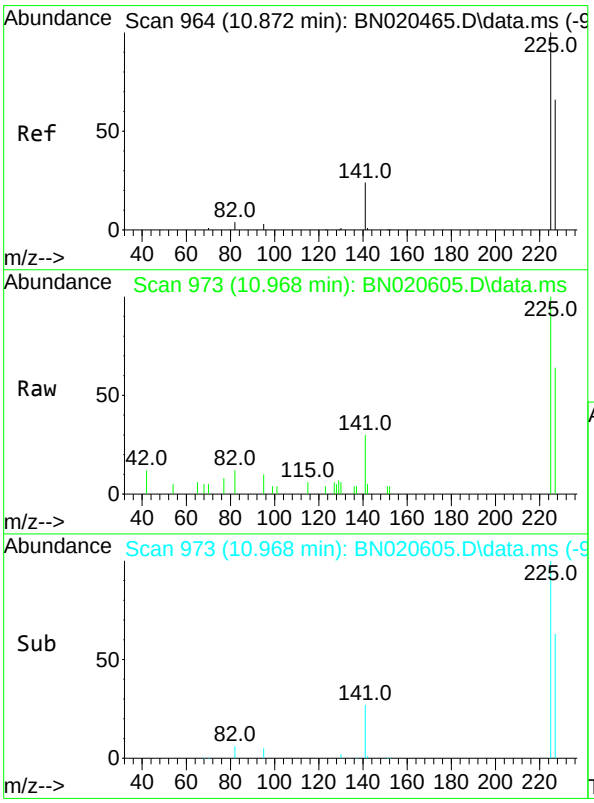

#10
Hexachlorobutadiene
Concen: 0.318 ng
RT: 10.968 min Scan# 973
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:225 Resp: 2138

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.8	50.9	76.3



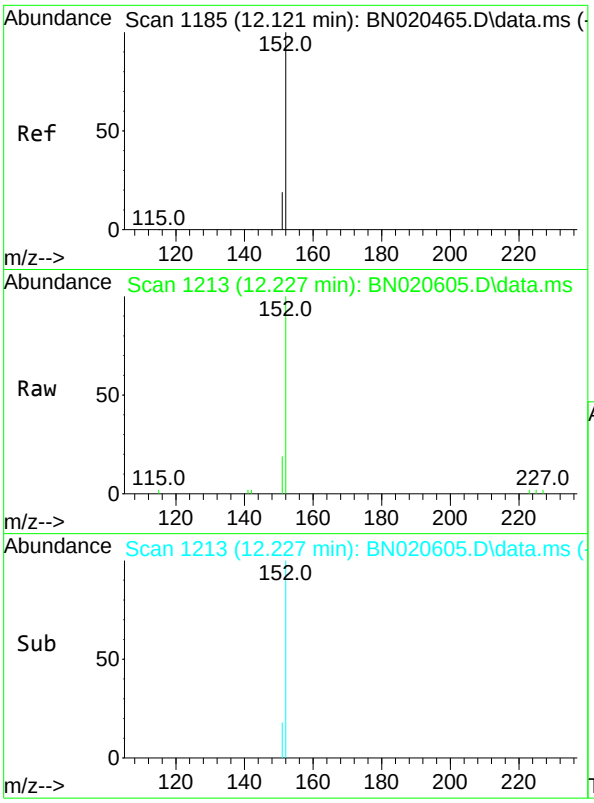

#11
2-Methylnaphthalene-d10
Concen: 0.311 ng
RT: 12.227 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:152 Resp: 658

Ion	Ratio	Lower	Upper
152	100		
151	16.7	16.2	24.4



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

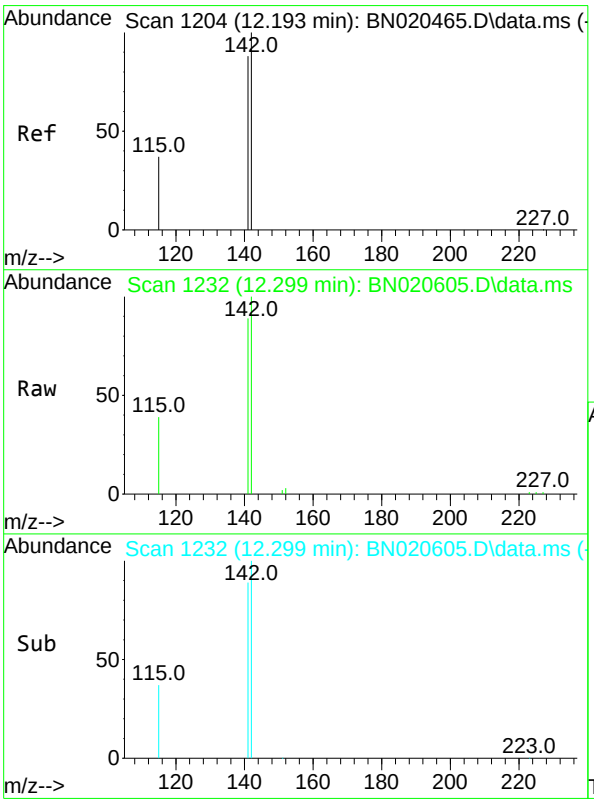

#12
2-Methylnaphthalene
Concen: 0.333 ng
RT: 12.299 min Scan# 1232
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:142 Resp: 8166

Ion	Ratio	Lower	Upper
142	100		
141	89.2	71.6	107.4
115	38.8	29.8	44.8



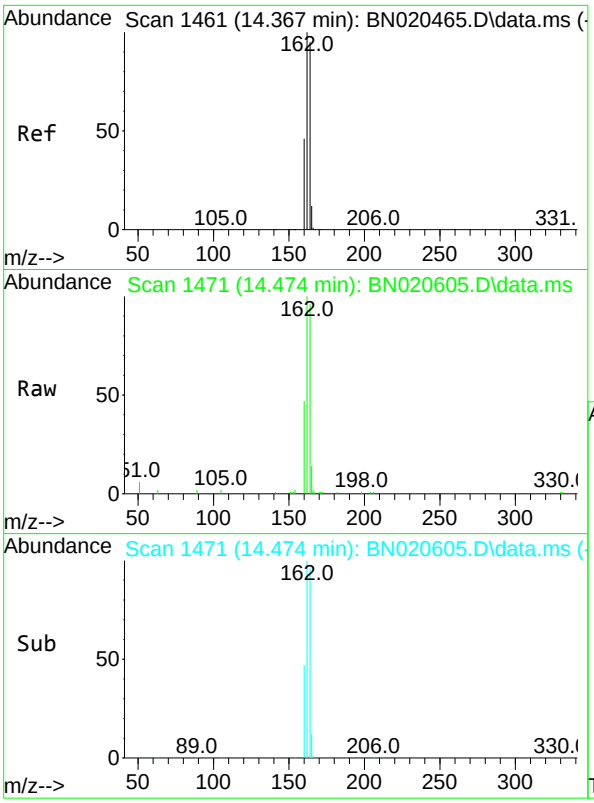

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.474 min Scan# 14
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:164 Resp: 648

Ion	Ratio	Lower	Upper
164	100		
162	104.2	82.1	123.1
160	49.0	38.6	58.0



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

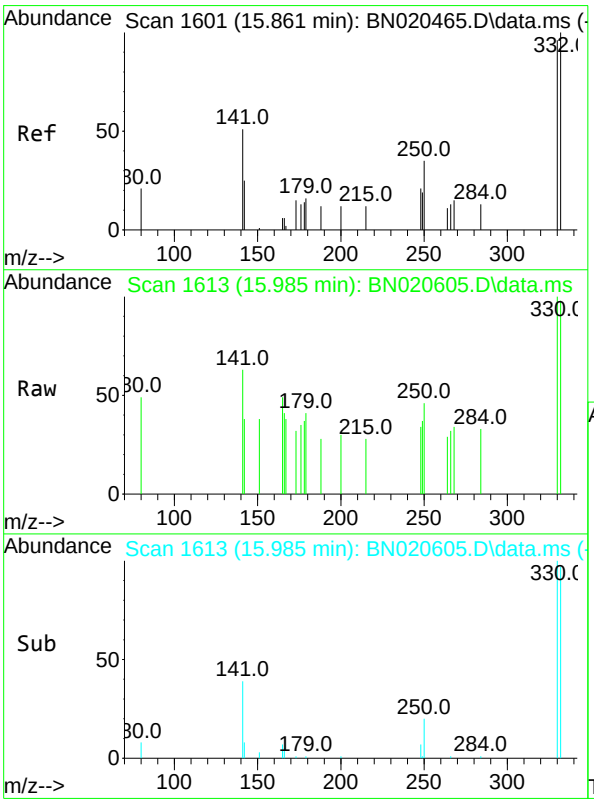

#14
2,4,6-Tribromophenol
Concen: 0.094 ng
RT: 15.985 min Scan# 1613
Delta R.T. 0.011 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:330 Resp: 230

Ion	Ratio	Lower	Upper
330	100		
332	95.7	77.6	116.4
141	57.4	41.0	61.4



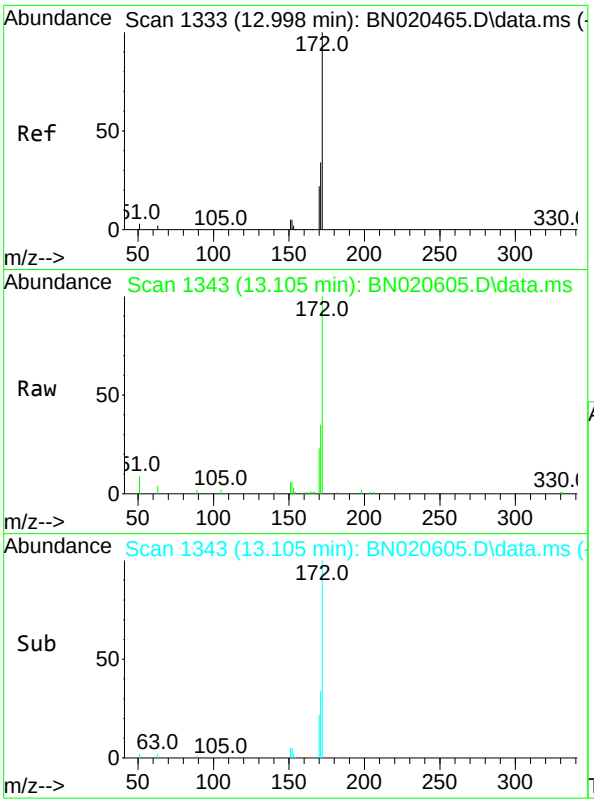

#15
2-Fluorobiphenyl
Concen: 0.276 ng
RT: 13.105 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:172 Resp: 738

Ion	Ratio	Lower	Upper
172	100		
171	35.0	27.2	40.8
170	23.2	18.2	27.4



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

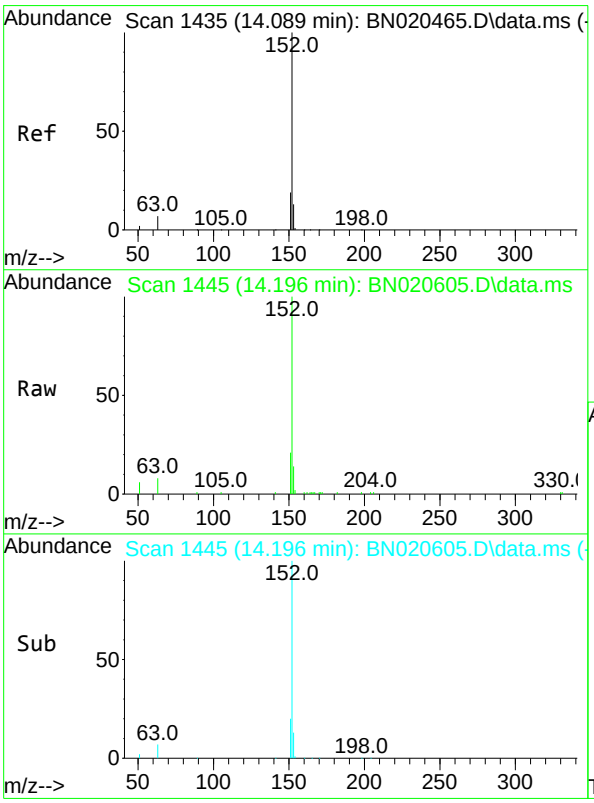

#16
Acenaphthylene
Concen: 0.332 ng
RT: 14.196 min Scan# 1445
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:152 Resp: 10364

Ion	Ratio	Lower	Upper
152	100		
151	19.7	16.2	24.4
153	12.9	10.7	16.1



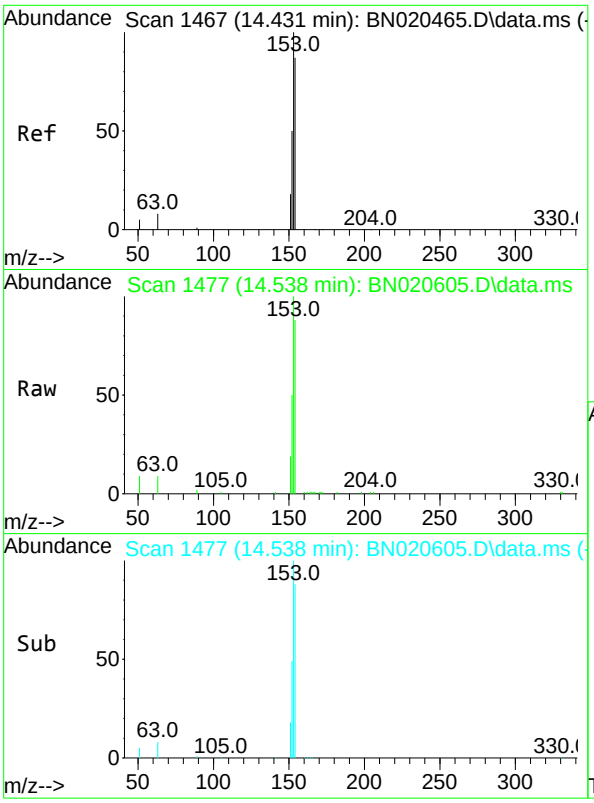

#17
Acenaphthene
Concen: 0.344 ng
RT: 14.538 min Scan# 14
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:154 Resp: 729

Ion	Ratio	Lower	Upper
154	100		
153	114.3	87.5	131.3
152	57.1	43.8	65.6



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

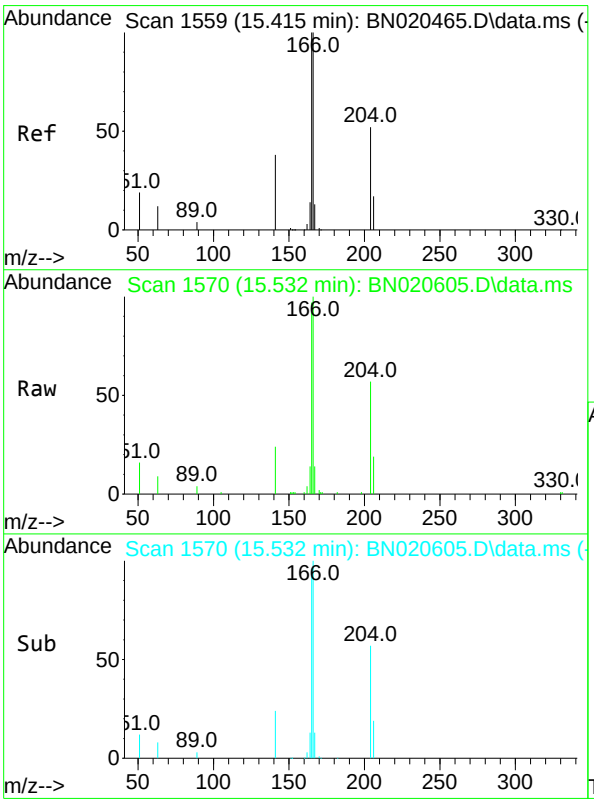

#18
Fluorene
Concen: 0.325 ng
RT: 15.532 min Scan# 1570
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:166 Resp: 9008

Ion	Ratio	Lower	Upper
166	100		
165	98.8	78.6	118.0
167	13.3	10.8	16.2



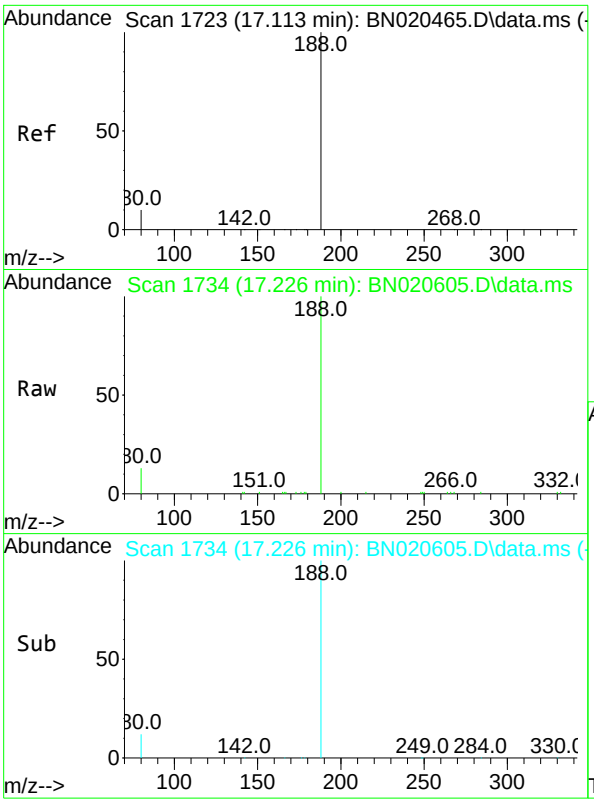

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.226 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:188 Resp: 1258

Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.7	7.4	11.2#



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

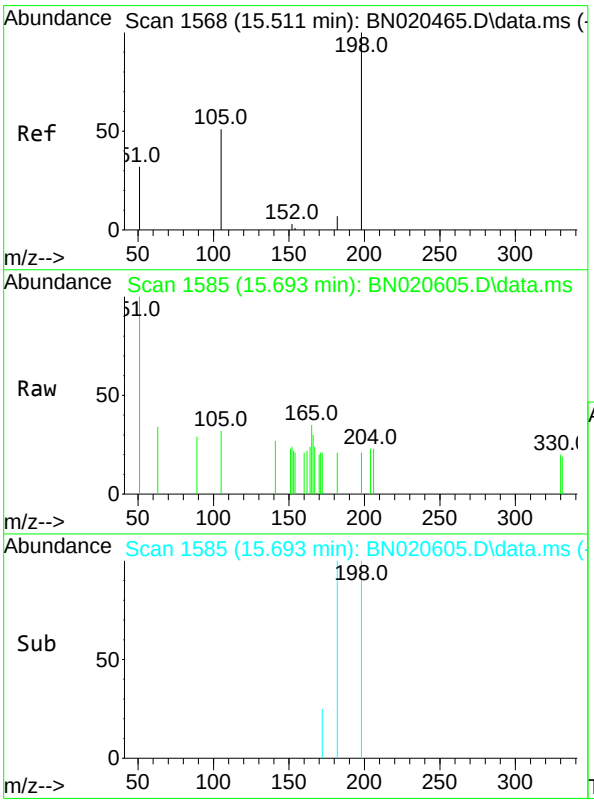

#20
4,6-Dinitro-2-methylphenol
Concen: 0.239 ng m
RT: 15.693 min Scan# 1585
Delta R.T. 0.054 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:198 Resp: 34

Ion	Ratio	Lower	Upper
198	100		
182	100.0	12.1	18.1#
77	0.0	0.0	0.0



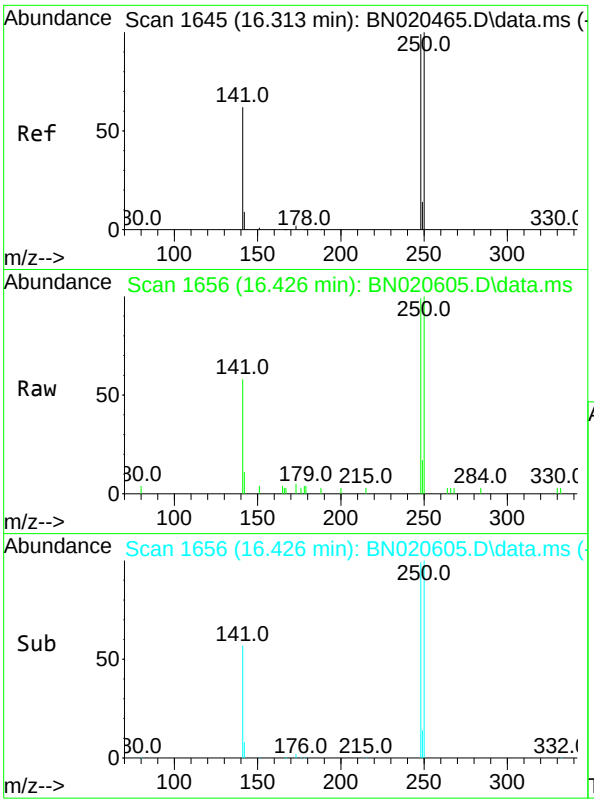

#21
4-Bromophenyl-phenylether
Concen: 0.370 ng
RT: 16.426 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:248 Resp: 270

Ion	Ratio	Lower	Upper
248	100		
250	101.2	75.3	112.9
141	59.0	67.3	100.9#

Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022



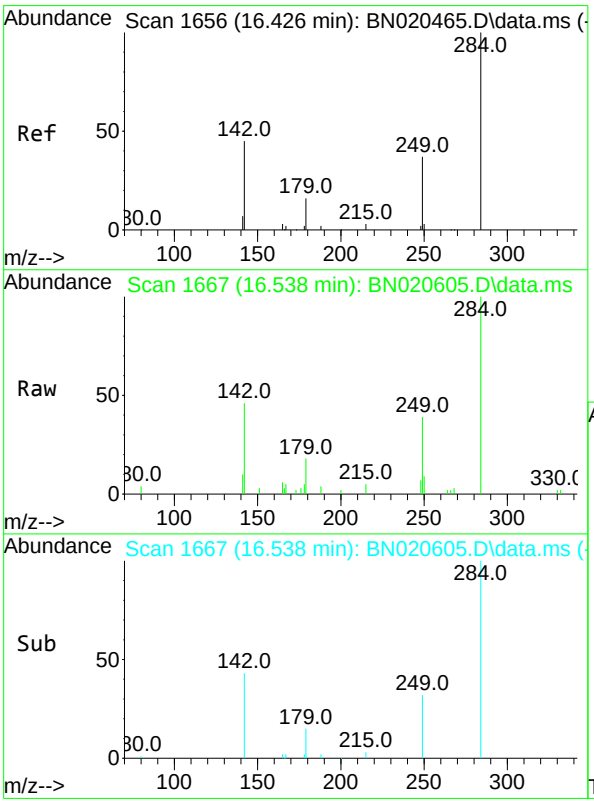

#22
Hexachlorobenzene
Concen: 0.382 ng
RT: 16.538 min Scan# 1667
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:284 Resp: 3094

Ion	Ratio	Lower	Upper
284	100		
142	46.5	35.2	52.8
249	34.1	26.6	40.0



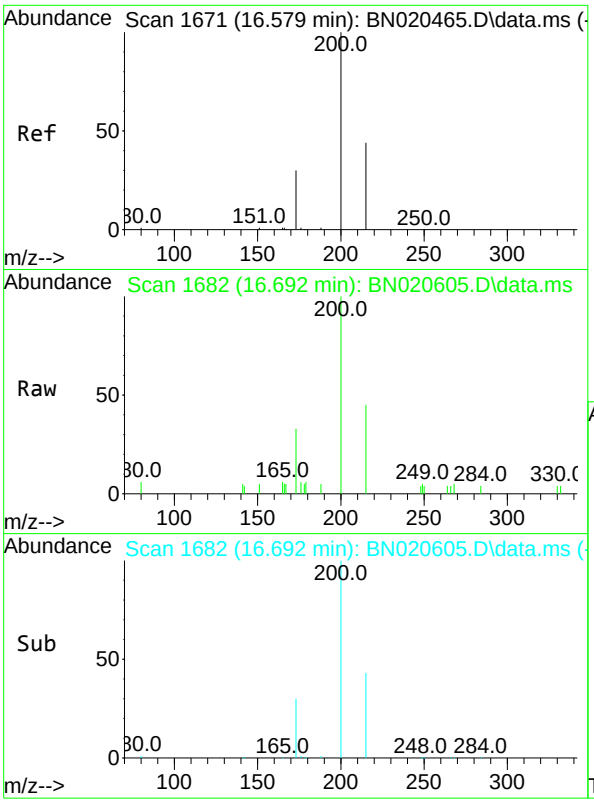

#23
Atrazine
Concen: 0.345 ng
RT: 16.692 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:200 Resp: 199

Ion	Ratio	Lower	Upper
200	100		
173	33.1	23.6	35.4
215	45.3	36.6	54.8

Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022



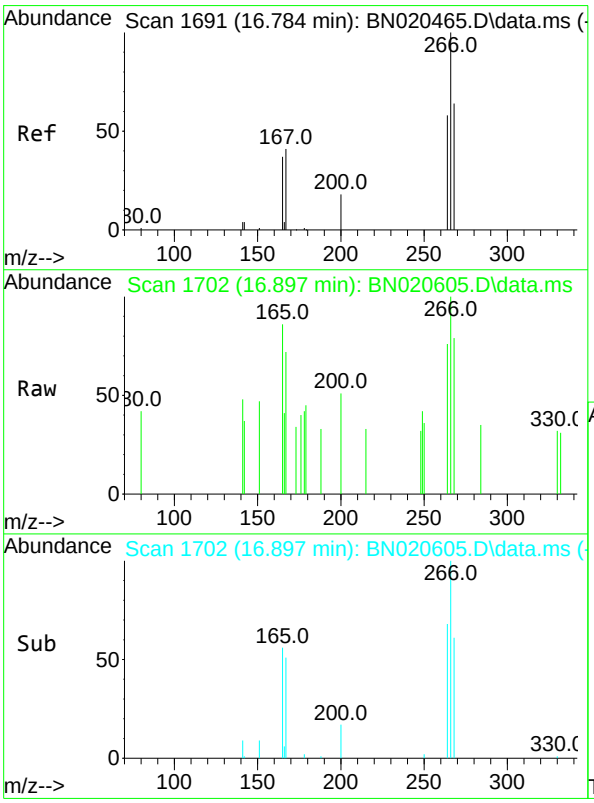

#24
Pentachlorophenol
Concen: 0.297 ng
RT: 16.897 min Scan# 1702
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:266 Resp: 295

Ion	Ratio	Lower	Upper
266	100		
264	56.6	51.3	76.9
268	56.3	52.6	79.0



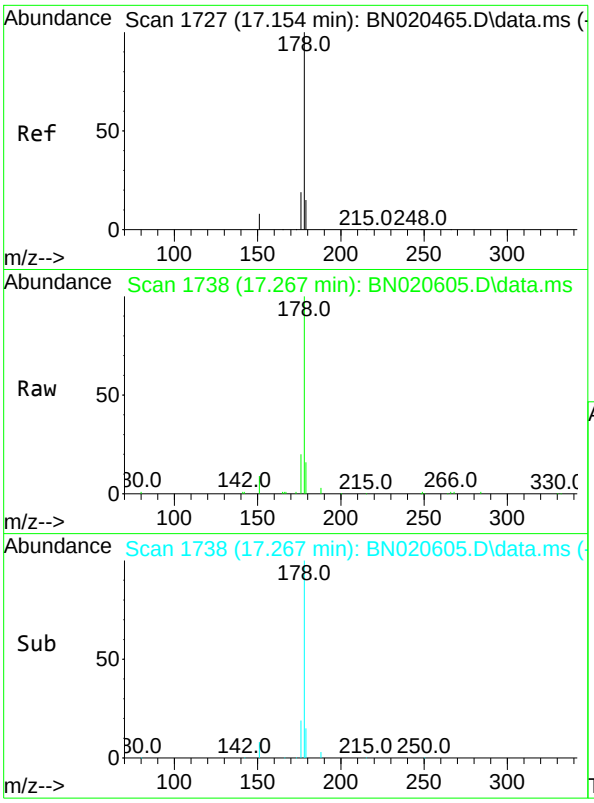

#25
Phenanthrene
Concen: 0.378 ng
RT: 17.267 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:178 Resp: 1604

Ion	Ratio	Lower	Upper
178	100		
176	19.2	15.3	22.9
179	15.5	12.2	18.4



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

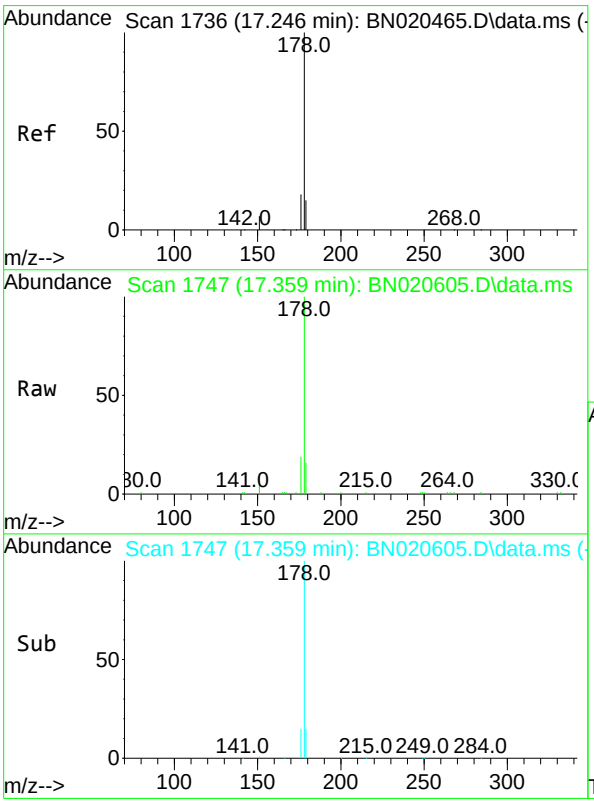

#26
Anthracene
Concen: 0.366 ng
RT: 17.359 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:178 Resp: 13396

Ion	Ratio	Lower	Upper
178	100		
176	18.5	14.9	22.3
179	15.0	12.2	18.4



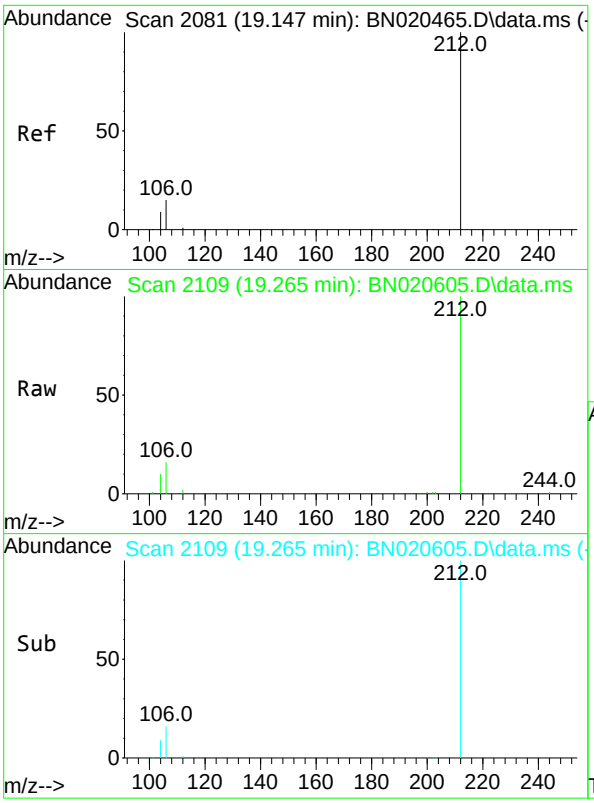

#27
Fluoranthene-d10
Concen: 0.294 ng
RT: 19.265 min Scan# 21
Delta R.T. -0.004 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:212 Resp: 1099

Ion	Ratio	Lower	Upper
212	100		
106	15.4	12.6	19.0
104	8.9	7.2	10.8

Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022



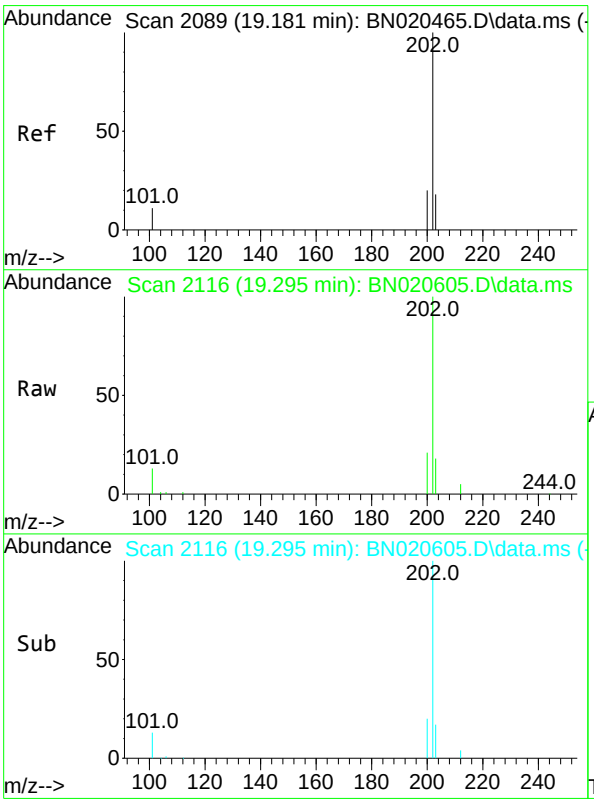

#28
Fluoranthene
Concen: 0.390 ng
RT: 19.295 min Scan# 2116
Delta R.T. -0.004 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:202 Resp: 18054

Ion	Ratio	Lower	Upper
202	100		
101	11.9	9.6	14.4
203	17.0	13.5	20.3



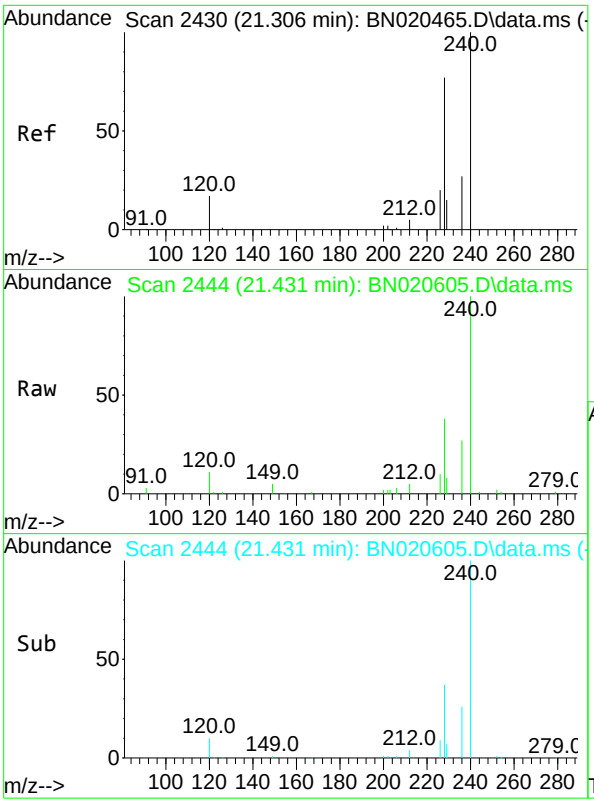

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.431 min Scan# 24
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:240 Resp: 1010

Ion	Ratio	Lower	Upper
240	100		
120	11.4	14.6	21.8
236	26.8	22.6	33.8



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

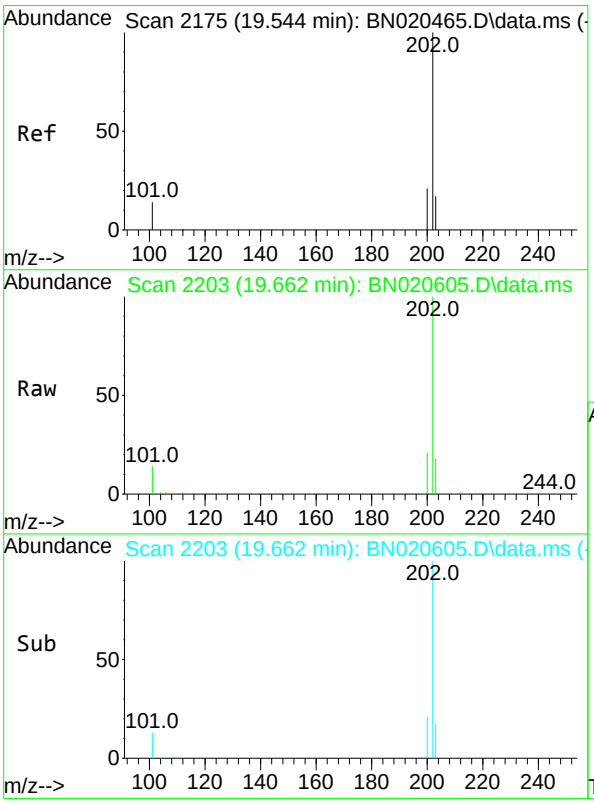

#30
Pyrene
Concen: 0.426 ng
RT: 19.662 min Scan# 2203
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:202 Resp: 18222

Ion	Ratio	Lower	Upper
202	100		
200	20.9	16.6	25.0
203	17.6	14.2	21.2



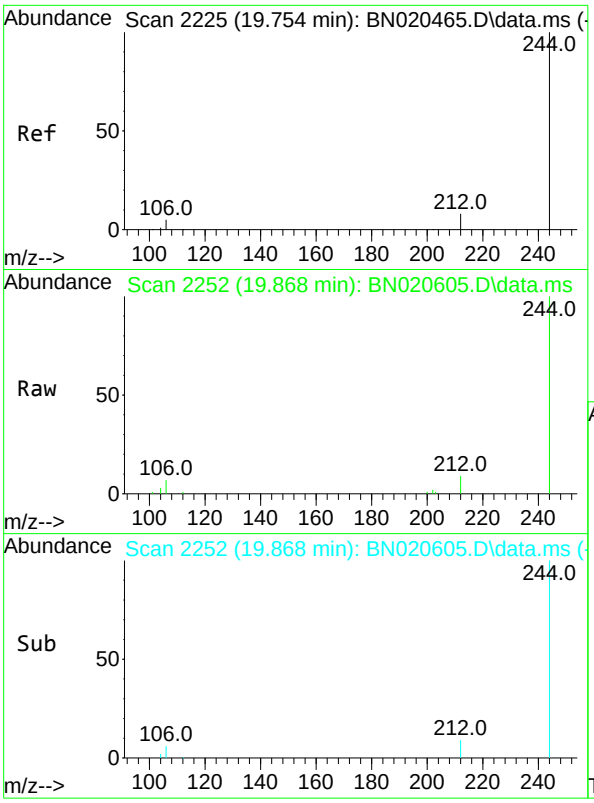

#31
Terphenyl-d14
Concen: 0.338 ng
RT: 19.868 min Scan# 2
Delta R.T. -0.004 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:244 Resp: 814

Ion	Ratio	Lower	Upper
244	100		
212	9.5	7.1	10.7
122	0.0	0.0	0.0

Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022



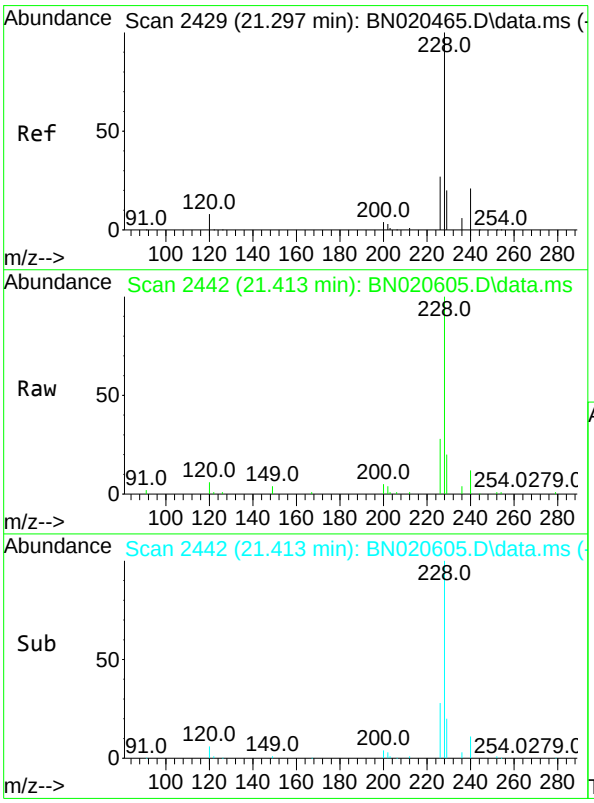

#32
Benzo(a)anthracene
Concen: 0.378 ng
RT: 21.413 min Scan# 2442
Delta R.T. -0.009 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:228 Resp: 13634

Ion	Ratio	Lower	Upper
228	100		
226	28.0	21.2	31.8
229	20.1	15.6	23.4



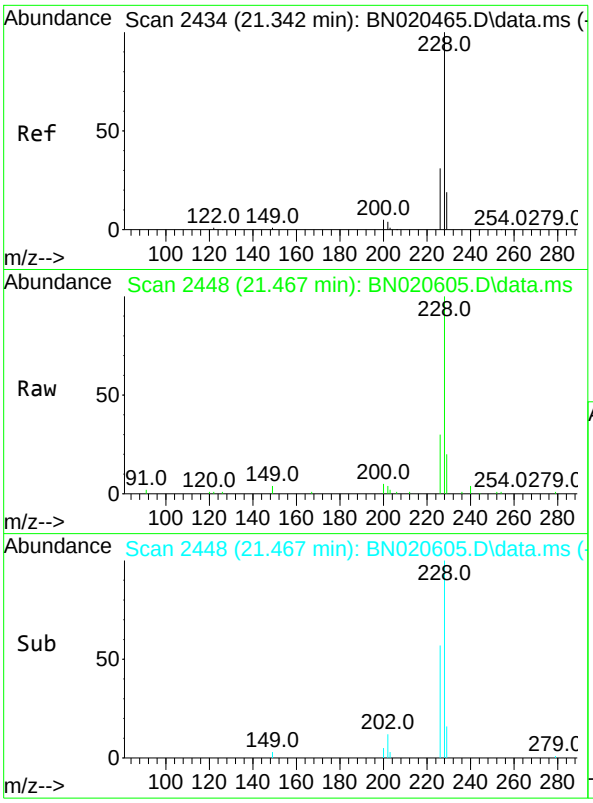

#33
Chrysene
Concen: 0.403 ng
RT: 21.467 min Scan# 24
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:228 Resp: 1609

Ion	Ratio	Lower	Upper
228	100		
226	29.7	23.4	35.0
229	19.8	15.7	23.5



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

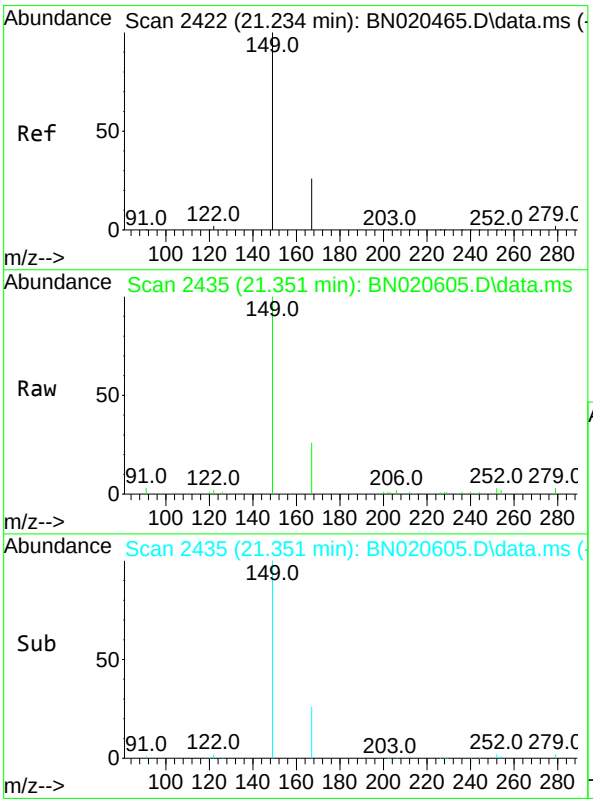

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.380 ng
RT: 21.351 min Scan# 2435
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:149 Resp: 7718

Ion	Ratio	Lower	Upper
149	100		
167	26.0	21.7	32.5
279	2.8	2.2	3.2



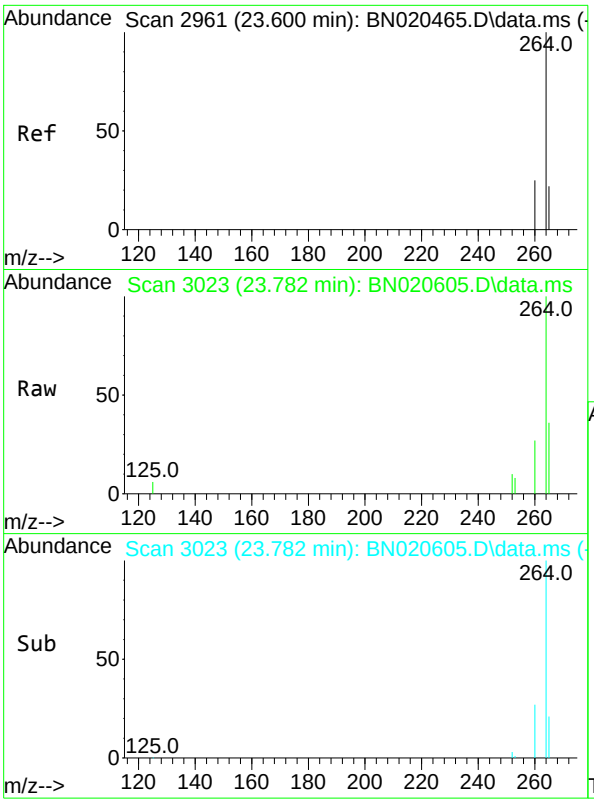

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.782 min Scan# 3
Delta R.T. -0.009 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:264 Resp: 7744

Ion	Ratio	Lower	Upper
264	100		
260	27.5	20.9	31.3
265	36.4	28.0	42.0

Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022



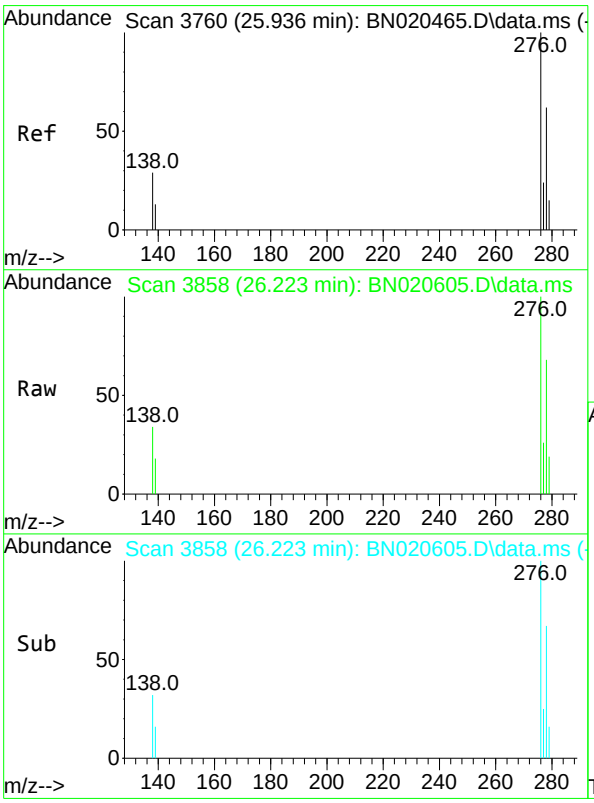

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.323 ng
RT: 26.223 min Scan# 3858
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:276 Resp: 11141

Ion	Ratio	Lower	Upper
276	100		
138	32.9	25.9	38.9
277	25.2	19.8	29.8



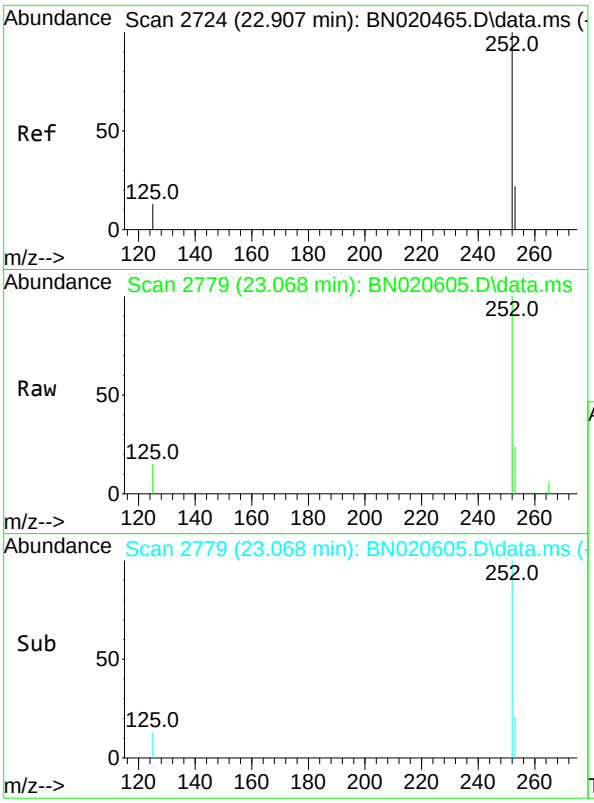

#37
Benzo(b)fluoranthene
Concen: 0.449 ng
RT: 23.068 min Scan# 2
Delta R.T. -0.006 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:252 Resp: 1339

Ion	Ratio	Lower	Upper
252	100		
253	23.7	18.5	27.7
125	14.9	11.4	17.0

Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022



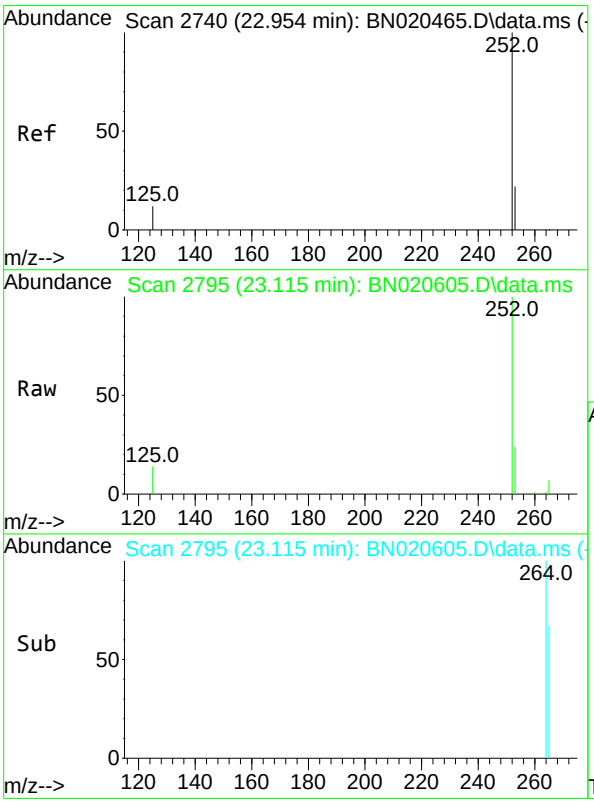

#38
Benzo(k)fluoranthene
Concen: 0.427 ng
RT: 23.115 min Scan# 2795
Delta R.T. -0.006 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:252 Resp: 13572

Ion	Ratio	Lower	Upper
252	100		
253	24.4	18.0	27.0
125	14.4	11.0	16.4



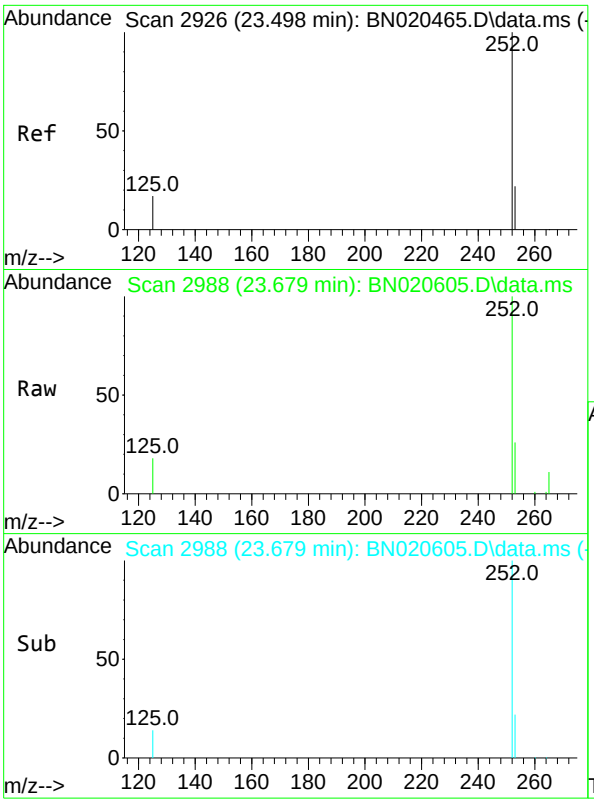

#39
Benzo(a)pyrene
Concen: 0.432 ng
RT: 23.679 min Scan# 2
Delta R.T. -0.006 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:252 Resp: 1118

Ion	Ratio	Lower	Upper
252	100		
253	26.2	19.0	28.4
125	17.6	13.8	20.8



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022

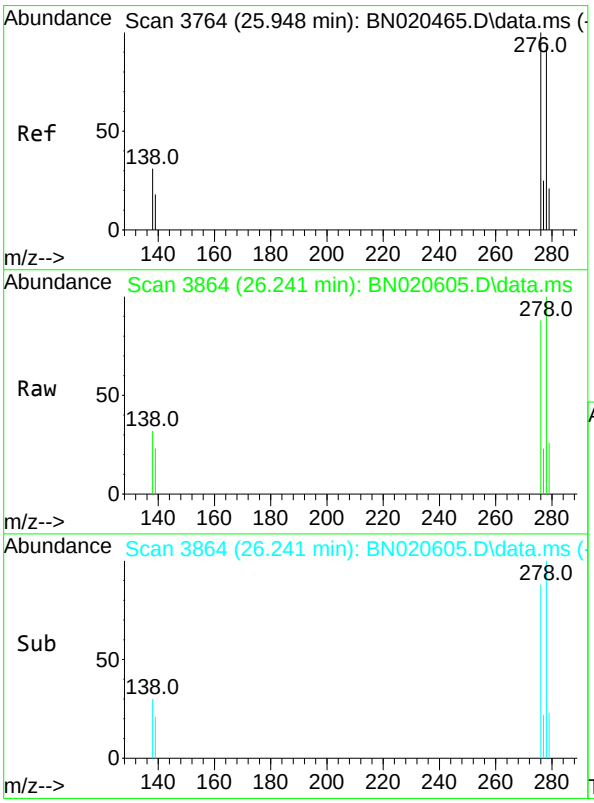

#40
Dibenzo(a,h)anthracene
Concen: 0.354 ng
RT: 26.241 min Scan# 3864
Delta R.T. -0.006 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:278 Resp: 9797

Ion	Ratio	Lower	Upper
278	100		
139	22.5	18.6	28.0
279	26.3	19.7	29.5



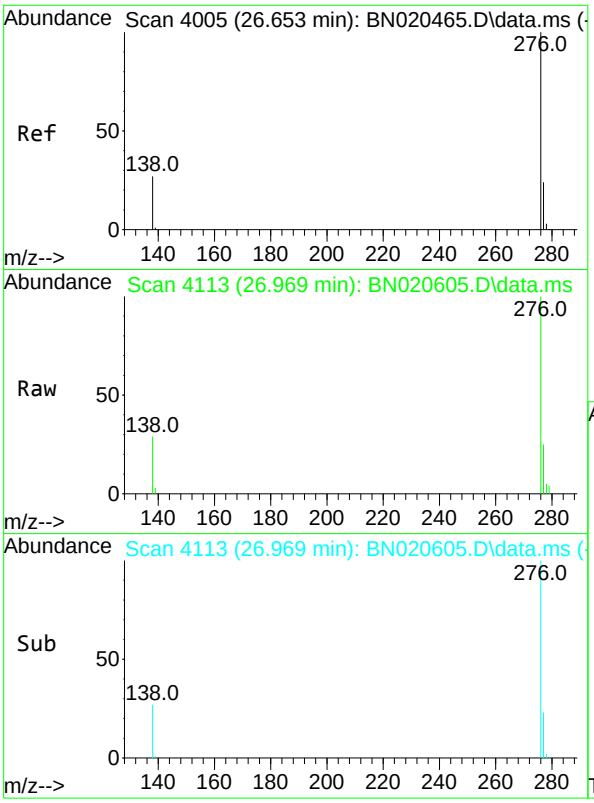

#41
Benzo(g,h,i)perylene
Concen: 0.347 ng
RT: 26.969 min Scan# 4
Delta R.T. 0.000 min
Lab File: BN020605.D
Acq: 01 Jul 2022 22:40

Tgt Ion:276 Resp: 1049

Ion	Ratio	Lower	Upper
276	100		
277	25.1	19.5	29.3
138	29.1	22.6	34.0



Instrument :
BNA_N
ClientSampleId :
RE114D2-20220622MS

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 07/05/2022
Supervised By :Jagrut Upadhyay 07/05/2022