

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
 Data File : BN020640.D
 Acq On : 02 Jul 2022 23:38
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Jul 04 02:39:57 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 02 03:10:12 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	4116	0.400	ng	0.00
7) Naphthalene-d8	10.626	136	12696	0.400	ng	0.00
13) Acenaphthene-d10	14.474	164	7303	0.400	ng	0.00
19) Phenanthrene-d10	17.225	188	14904	0.400	ng	0.00
29) Chrysene-d12	21.431	240	11792	0.400	ng	# 0.00
35) Perylene-d12	23.784	264	9289	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.413	112	3584	0.314	ng	0.00
5) Phenol-d6	7.024	99	4521	0.331	ng	0.00
8) Nitrobenzene-d5	8.982	82	3534	0.343	ng	-0.01
11) 2-Methylnaphthalene-d10	12.223	152	8050	0.370	ng	0.00
14) 2,4,6-Tribromophenol	15.974	330	825	0.300	ng	0.00
15) 2-Fluorobiphenyl	13.095	172	11932	0.396	ng	-0.01
27) Fluoranthene-d10	19.265	212	16252	0.367	ng	0.00
31) Terphenyl-d14	19.868	244	11772	0.418	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.261	88	1968	0.365	ng	96
3) n-Nitrosodimethylamine	3.608	42	1554	0.316	ng	# 97
6) bis(2-Chloroethyl)ether	7.255	93	4044	0.344	ng	95
9) Naphthalene	10.669	128	14471	0.382	ng	99
10) Hexachlorobutadiene	10.968	225	2647	0.383	ng	# 100
12) 2-Methylnaphthalene	12.295	142	9467	0.376	ng	99
16) Acenaphthylene	14.196	152	12646	0.360	ng	98
17) Acenaphthene	14.538	154	9012	0.377	ng	94
18) Fluorene	15.521	166	11501	0.369	ng	99
20) 4,6-Dinitro-2-methylph...	15.628	198	477	0.389	ng	# 66
21) 4-Bromophenyl-phenylether	16.415	248	3431	0.396	ng	96
22) Hexachlorobenzene	16.538	284	3874	0.404	ng	98
23) Atrazine	16.692	200	2198	0.322	ng	99
24) Pentachlorophenol	16.887	266	899	0.476	ng	96
25) Phenanthrene	17.266	178	19071	0.379	ng	100
26) Anthracene	17.359	178	15313	0.353	ng	99
28) Fluoranthene	19.295	202	20605	0.376	ng	100
30) Pyrene	19.657	202	20897	0.419	ng	100
32) Benzo(a)anthracene	21.413	228	14515	0.345	ng	99
33) Chrysene	21.467	228	18595	0.399	ng	98
34) Bis(2-ethylhexyl)phtha...	21.351	149	8222	0.346	ng	99
36) Indeno(1,2,3-cd)pyrene	26.217	276	14707	0.355	ng	99
37) Benzo(b)fluoranthene	23.068	252	14662	0.410	ng	97
38) Benzo(k)fluoranthene	23.115	252	15768	0.414	ng	98
39) Benzo(a)pyrene	23.682	252	11937	0.385	ng	# 89
40) Dibenzo(a,h)anthracene	26.232	278	11730	0.353	ng	97
41) Benzo(g,h,i)perylene	26.957	276	12299	0.339	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
Data File : BN020640.D
Acq On : 02 Jul 2022 23:38
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Jul 04 02:39:57 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 03:10:12 2022
Response via : Initial Calibration



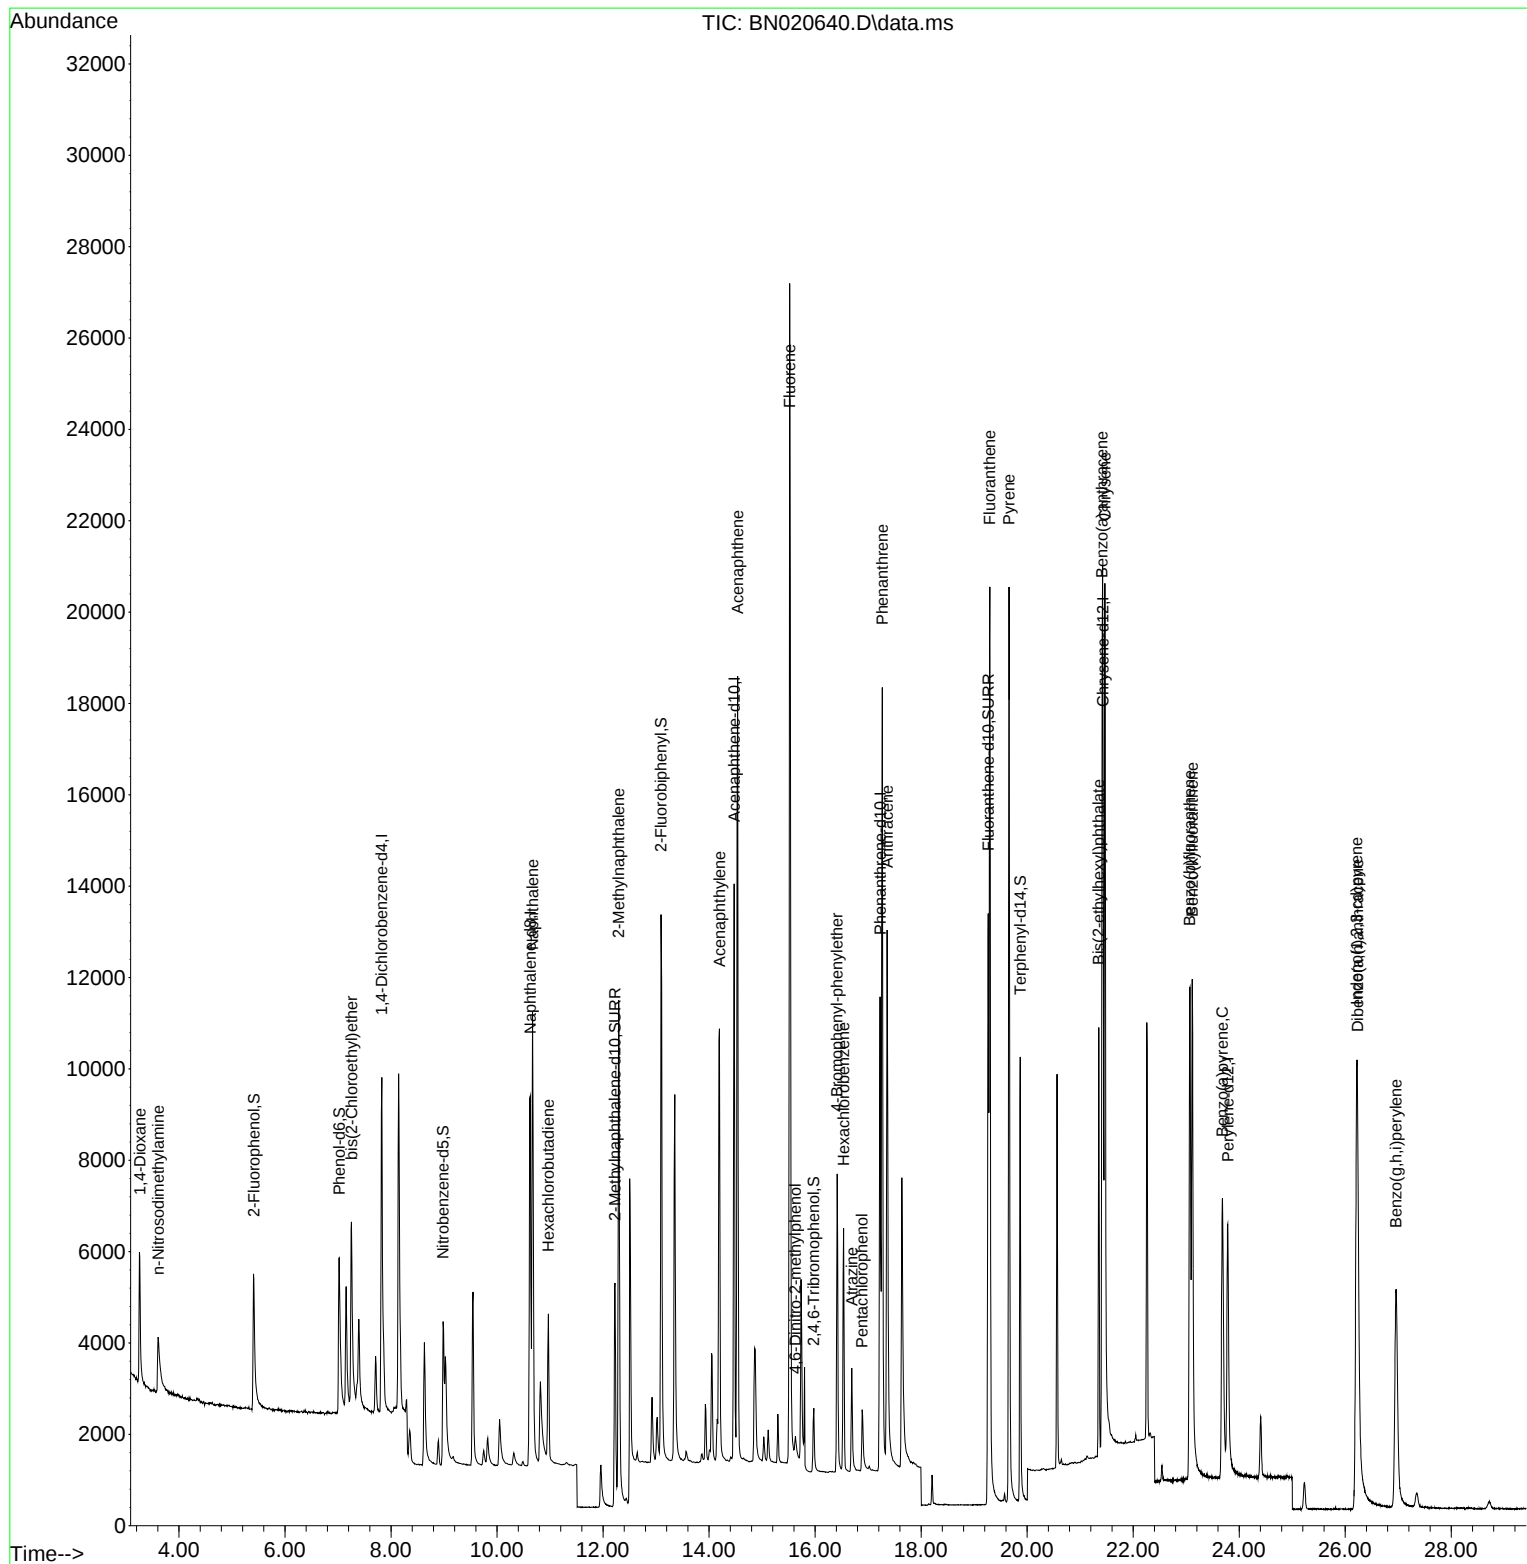




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.825 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN020640.D
 Acq: 02 Jul 2022 23:38




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:152 Resp: 4116
 Ion Ratio Lower Upper
 152 100
 150 154.1 127.9 191.9
 115 63.1 51.4 77.2

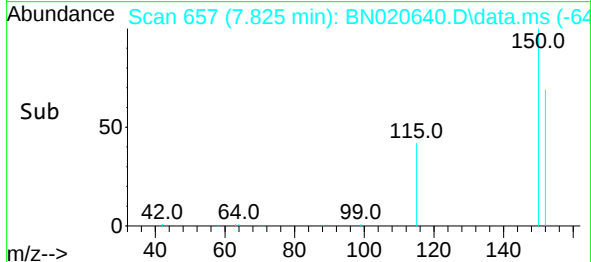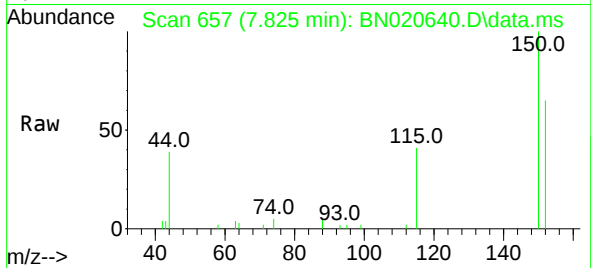

#2
 1,4-Dioxane
 Concen: 0.365 ng
 RT: 3.261 min Scan# 25
 Delta R.T. 0.000 min
 Lab File: BN020640.D
 Acq: 02 Jul 2022 23:38

Tgt Ion: 88 Resp: 1968
 Ion Ratio Lower Upper
 88 100
 43 35.3 30.2 45.2
 58 86.9 73.0 109.6

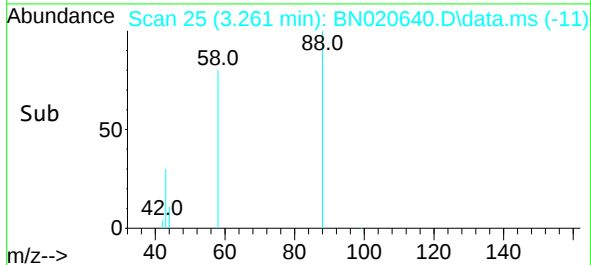

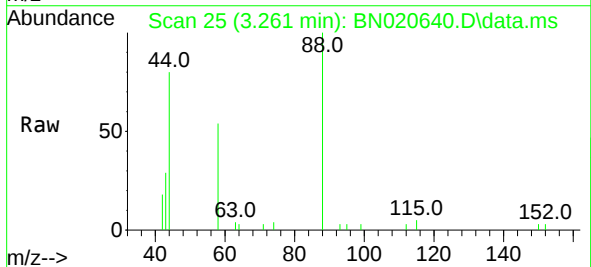




#3
n-Nitrosodimethylamine
Concen: 0.316 ng
RT: 3.608 min Scan# 71
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 42 Resp: 1554
Ion Ratio Lower Upper
42 100
74 102.5 84.0 126.0
44 7.5 9.8 14.8#

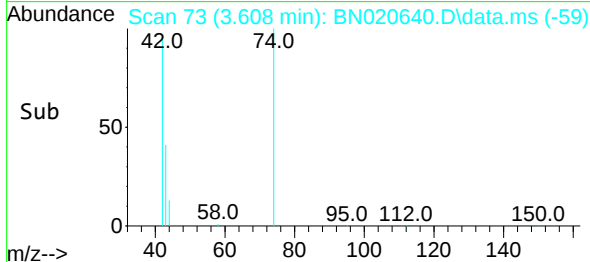

#4
2-Fluorophenol
Concen: 0.314 ng
RT: 5.413 min Scan# 323
Delta R.T. -0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion: 112 Resp: 3584
Ion Ratio Lower Upper
112 100
64 63.0 49.1 73.7
63 34.3 26.3 39.5

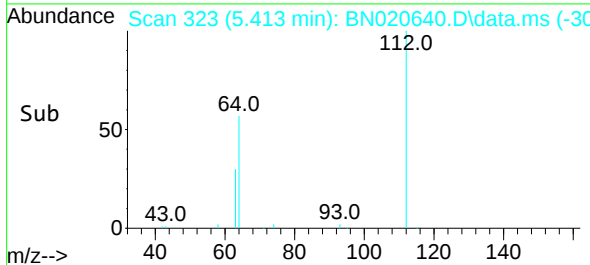

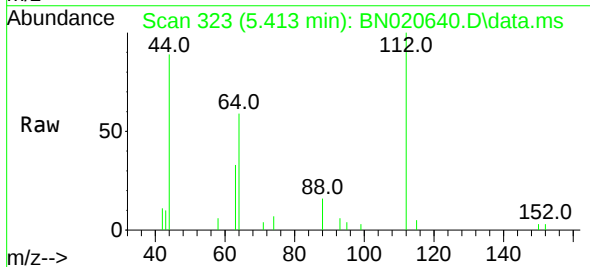




#5
Phenol-d6
Concen: 0.331 ng
RT: 7.024 min Scan# 54
Delta R.T. -0.007 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 99	Resp: 4521
Ion Ratio	Lower Upper
99 100	
42 22.8	19.3 28.9
71 35.4	27.5 41.3

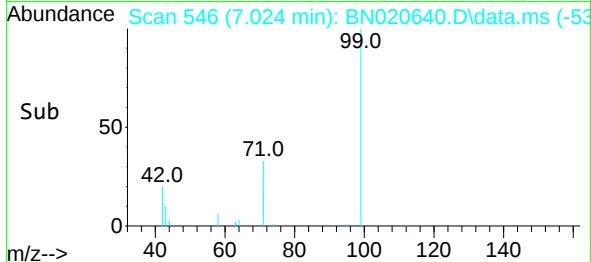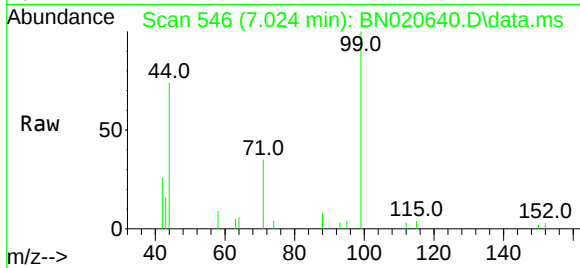

#6
bis(2-Chloroethyl)ether
Concen: 0.344 ng
RT: 7.255 min Scan# 578
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion: 93	Resp: 4044
Ion Ratio	Lower Upper
93 100	
63 89.3	67.4 101.0
95 35.0	26.5 39.7

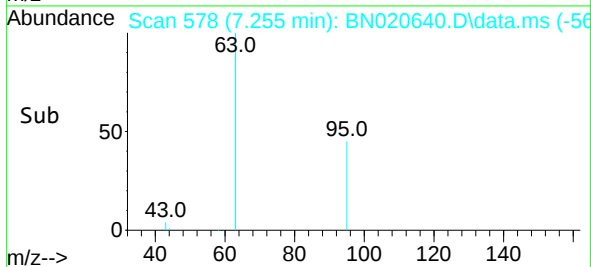

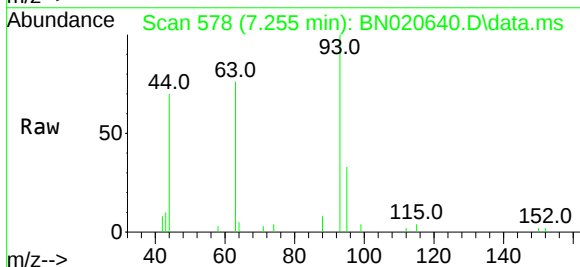




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.626 min Scan# 94
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	136	Resp:	12696
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.0	13.6
54	8.1	6.2	9.2
68	5.4	4.4	6.6

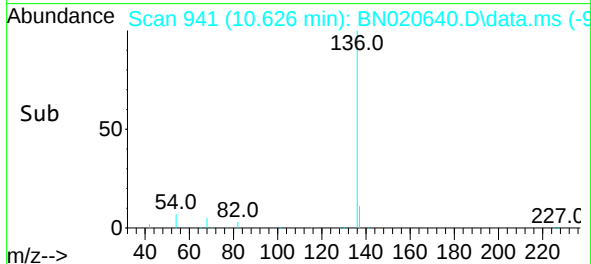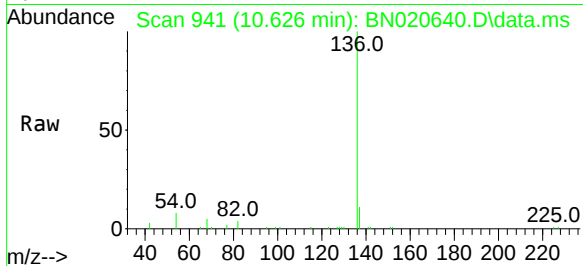

#8
Nitrobenzene-d5
Concen: 0.343 ng
RT: 8.982 min Scan# 787
Delta R.T. -0.011 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:	82	Resp:	3534
Ion	Ratio	Lower	Upper
82	100		
128	36.8	35.0	52.6
54	63.5	46.2	69.4


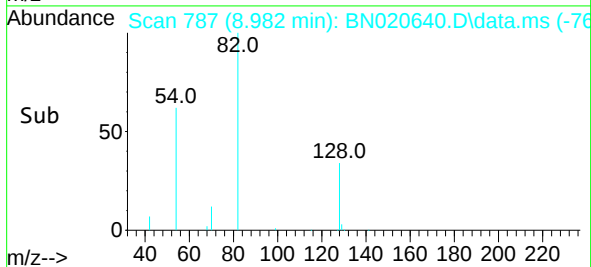

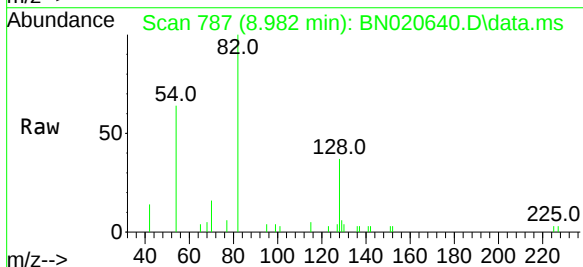




#9
Naphthalene
Concen: 0.382 ng
RT: 10.669 min Scan# 945
Delta R.T. -0.011 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:128	Resp:	14471
Ion Ratio	Lower	Upper
128	100	
129	11.4	8.9 13.3
127	13.8	10.8 16.2

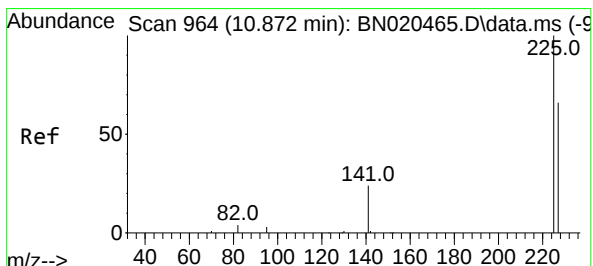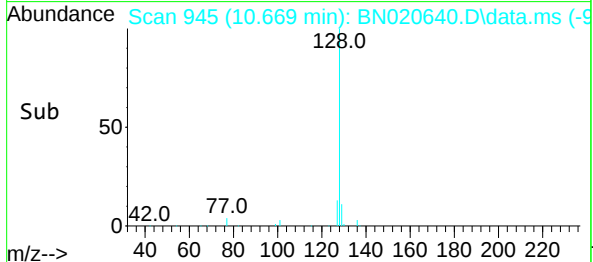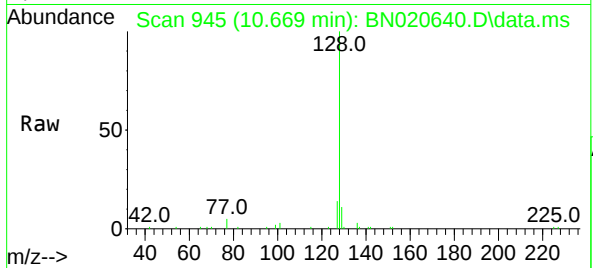

#10
Hexachlorobutadiene
Concen: 0.383 ng
RT: 10.968 min Scan# 973
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:225	Resp:	2647
Ion Ratio	Lower	Upper
225	100	
223	0.0	0.0 0.0
227	64.0	50.9 76.3

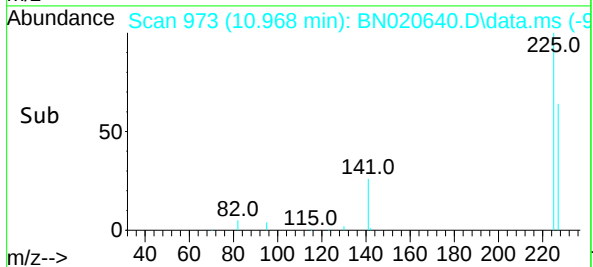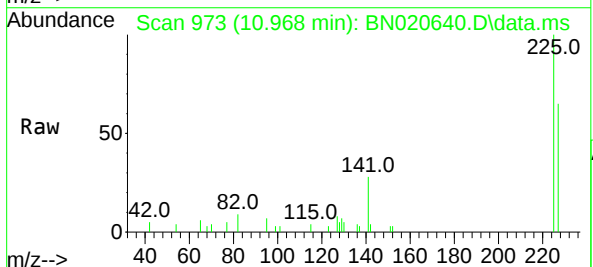



#11

2-Methylnaphthalene-d10

Concen: 0.370 ng

RT: 12.223 min Scan# 1185

Delta R.T. -0.004 min

Lab File: BN020640.D

Acq: 02 Jul 2022 23:38

Instrument :

BNA_N

ClientSampleId :





SSTDCCC0.4

Tgt Ion:152 Resp: 8050

Ion Ratio Lower Upper

152 100

151 20.0 16.2 24.4

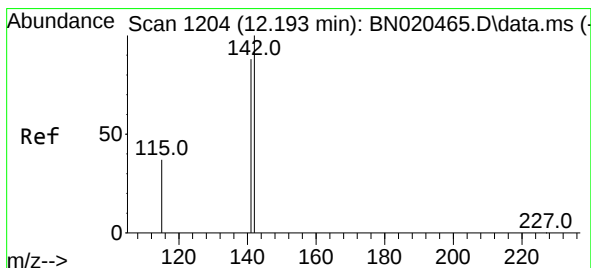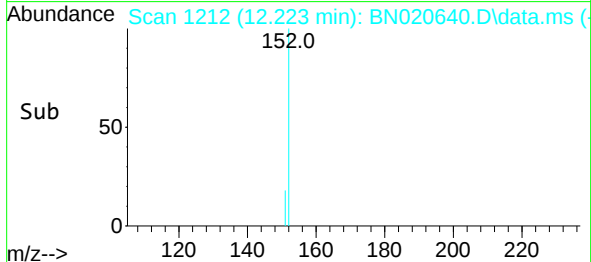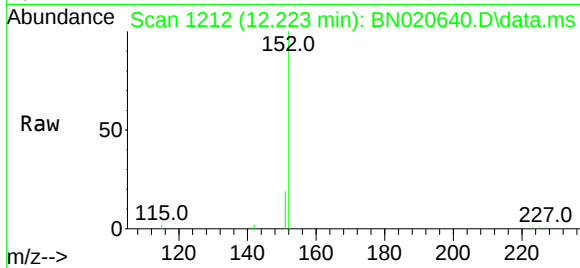

#12

2-Methylnaphthalene

Concen: 0.376 ng

RT: 12.295 min Scan# 1231

Delta R.T. -0.004 min

Lab File: BN020640.D

Acq: 02 Jul 2022 23:38




Tgt Ion:142 Resp: 9467

Ion Ratio Lower Upper

142 100

141 90.1 71.6 107.4

115 39.1 29.8 44.8

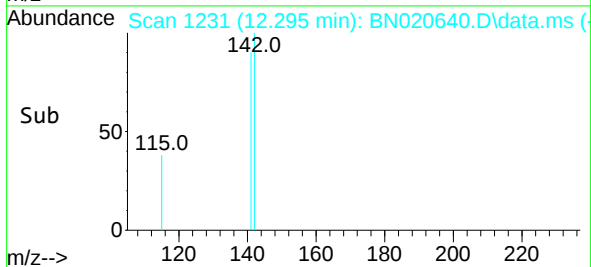

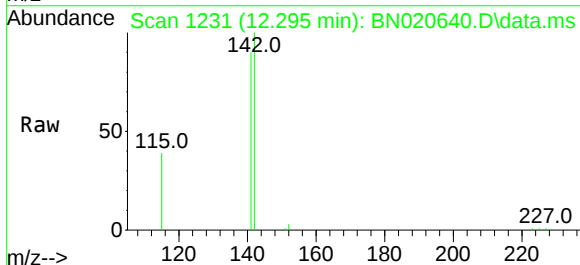




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.474 min Scan# 14
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:164 Resp: 7303
Ion Ratio Lower Upper
164 100
162 101.8 82.1 123.1
160 47.2 38.6 58.0

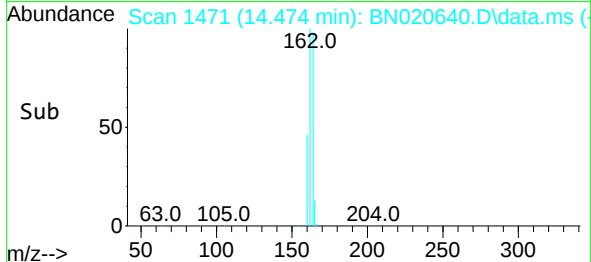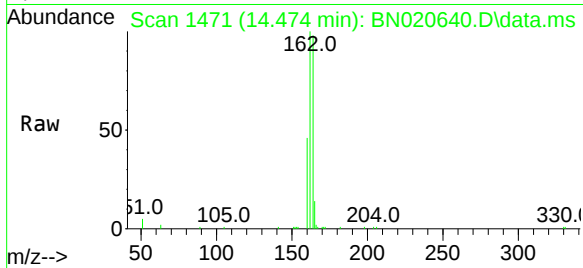

#14
2,4,6-Tribromophenol
Concen: 0.300 ng
RT: 15.974 min Scan# 1612
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:330 Resp: 825
Ion Ratio Lower Upper
330 100
332 98.4 77.6 116.4
141 56.1 41.0 61.4

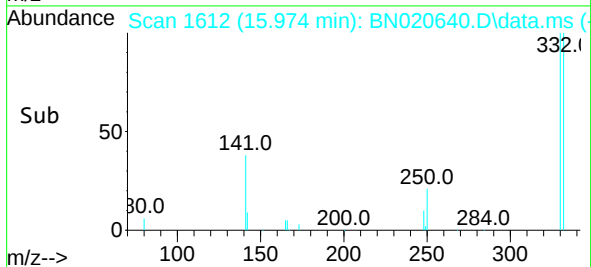

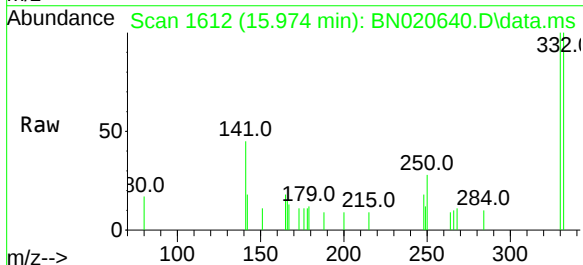




#15
2-Fluorobiphenyl
Concen: 0.396 ng
RT: 13.095 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	172	Resp:	11932
Ion Ratio	Lower	Upper	
172	100		
171	36.1	27.2	40.8
170	24.9	18.2	27.4

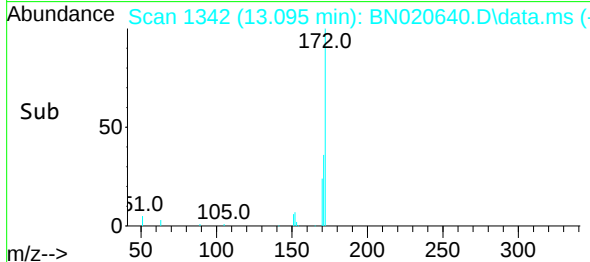

#16
Acenaphthylene
Concen: 0.360 ng
RT: 14.196 min Scan# 1445
Delta R.T. -0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:	152	Resp:	12646
Ion Ratio	Lower	Upper	
152	100		
151	19.5	16.2	24.4
153	12.7	10.7	16.1

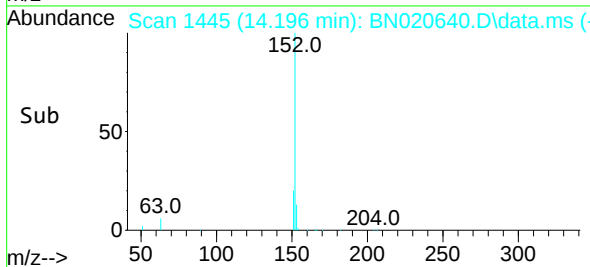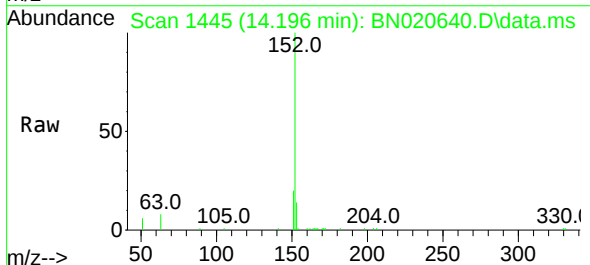

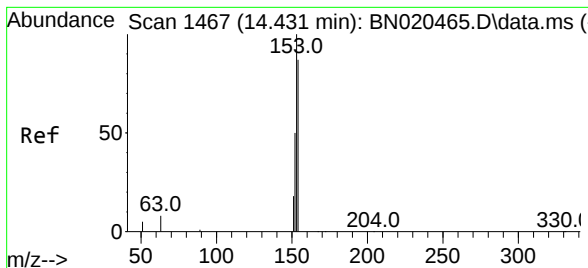

#17

Acenaphthene

Concen: 0.377 ng

RT: 14.538 min Scan# 1467

Delta R.T. 0.000 min

Lab File: BN020640.D

Acq: 02 Jul 2022 23:38

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:154 Resp: 9012

Ion Ratio Lower Upper

154 100

153 116.1 87.5 131.3

152 57.4 43.8 65.6

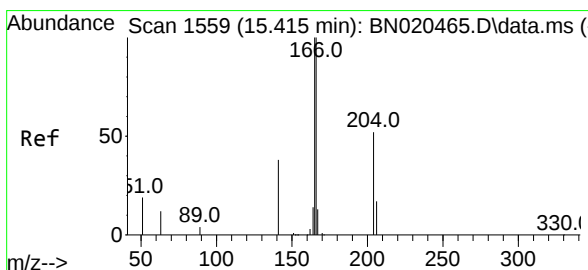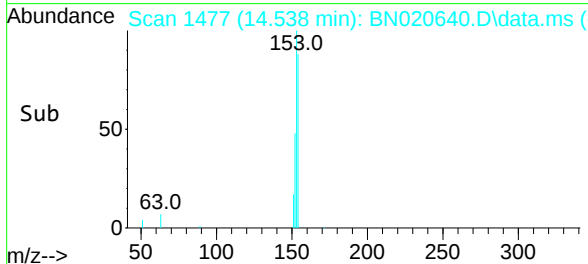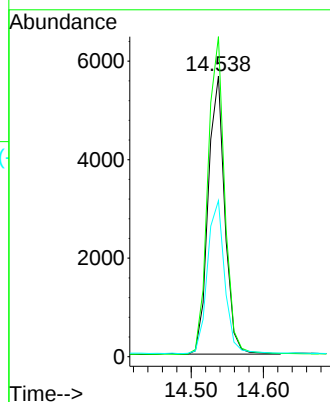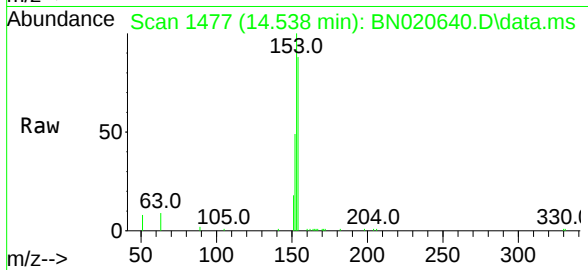

#18

Fluorene

Concen: 0.369 ng

RT: 15.521 min Scan# 1569

Delta R.T. -0.011 min

Lab File: BN020640.D

Acq: 02 Jul 2022 23:38




Tgt Ion:166 Resp: 11501

Ion Ratio Lower Upper

166 100

165 99.5 78.6 118.0

167 13.5 10.8 16.2


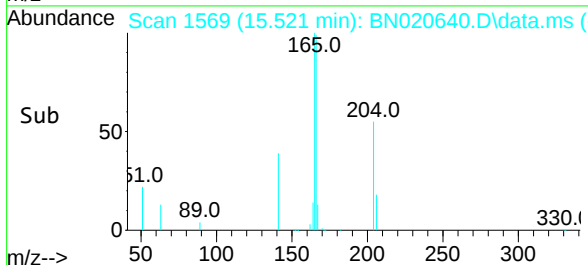

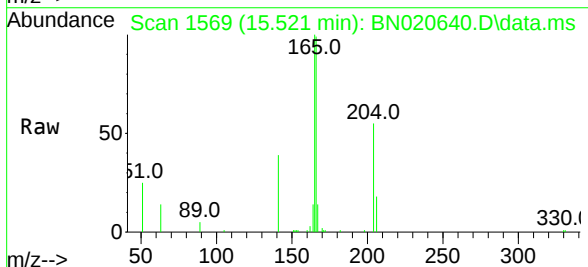




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.225 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 14904
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.7 7.4 11.2

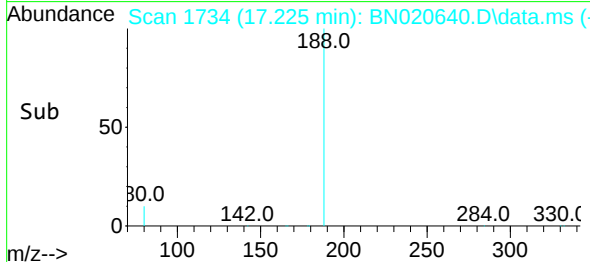

#20
4,6-Dinitro-2-methylphenol
Concen: 0.389 ng
RT: 15.628 min Scan# 1579
Delta R.T. -0.011 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:198 Resp: 477
Ion Ratio Lower Upper
198 100
182 29.3 12.1 18.1#
77 0.0 0.0 0.0


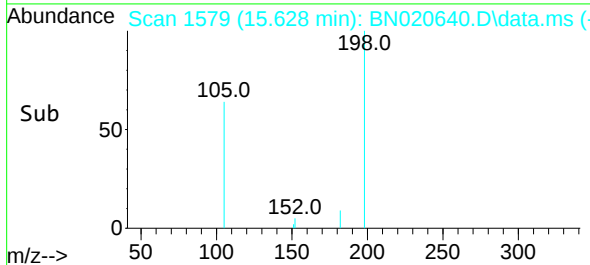

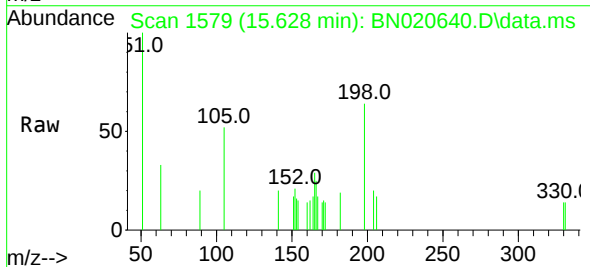


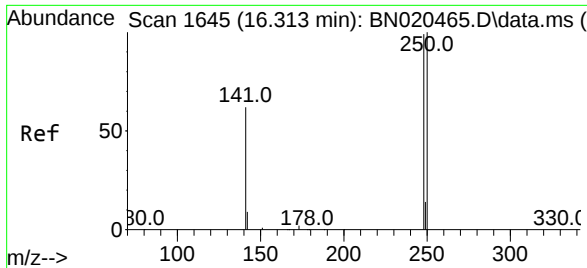

#21
4-Bromophenyl-phenylether
Concen: 0.396 ng
RT: 16.415 min Scan# 1665
Delta R.T. -0.010 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248	Resp:	3431
Ion Ratio	Lower	Upper
248	100	
250	93.7	75.3 112.9
141	91.5	67.3 100.9

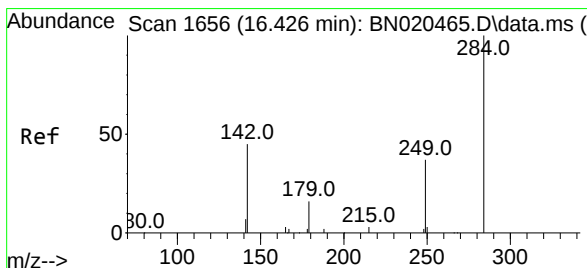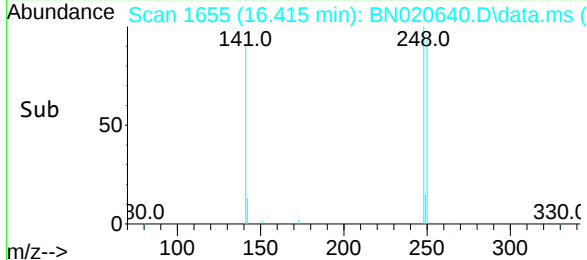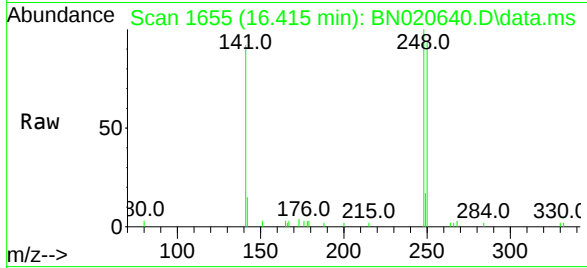

#22
Hexachlorobenzene
Concen: 0.404 ng
RT: 16.538 min Scan# 1667
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:284	Resp:	3874
Ion Ratio	Lower	Upper
284	100	
142	46.2	35.2 52.8
249	33.3	26.6 40.0


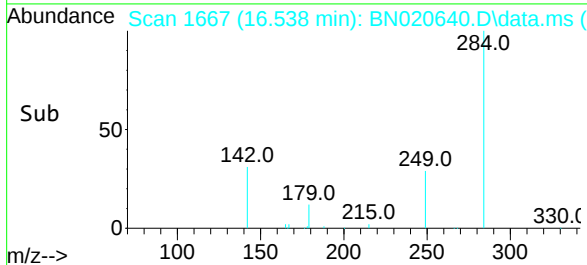

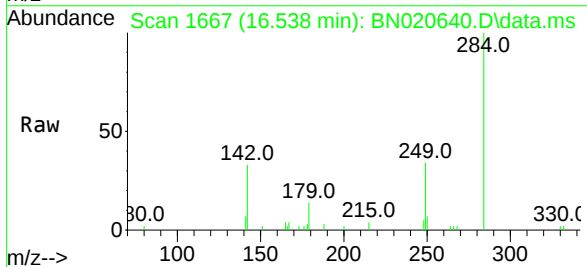




#23
 Atrazine
 Concen: 0.322 ng
 RT: 16.692 min Scan# 1701
 Delta R.T. -0.000 min
 Lab File: BN020640.D
 Acq: 02 Jul 2022 23:38




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:200 Resp: 2198
 Ion Ratio Lower Upper
 200 100
 173 29.8 23.6 35.4
 215 46.2 36.6 54.8

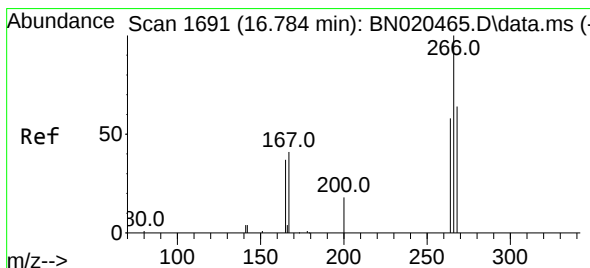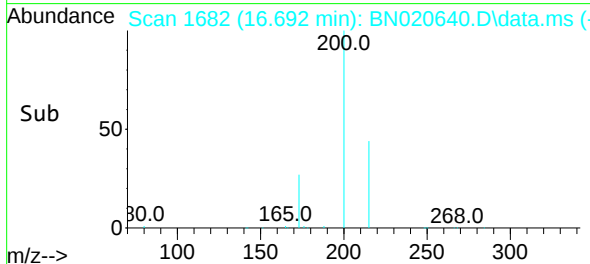

#24
 Pentachlorophenol
 Concen: 0.476 ng
 RT: 16.887 min Scan# 1701
 Delta R.T. -0.010 min
 Lab File: BN020640.D
 Acq: 02 Jul 2022 23:38

Tgt Ion:266 Resp: 899
 Ion Ratio Lower Upper
 266 100
 264 63.1 51.3 76.9
 268 60.6 52.6 79.0


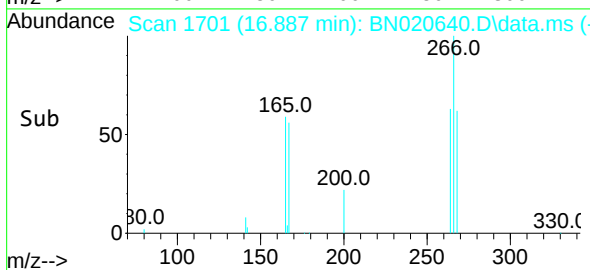

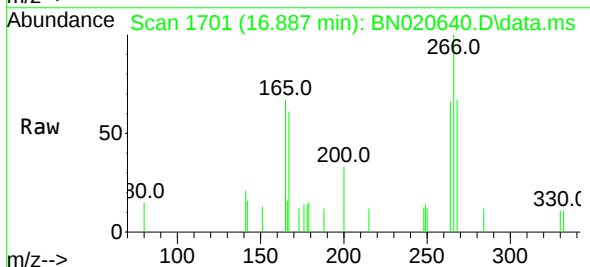




#25
Phenanthrene
Concen: 0.379 ng
RT: 17.266 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:178 Resp: 19071
Ion Ratio Lower Upper
178 100
176 19.3 15.3 22.9
179 15.3 12.2 18.4

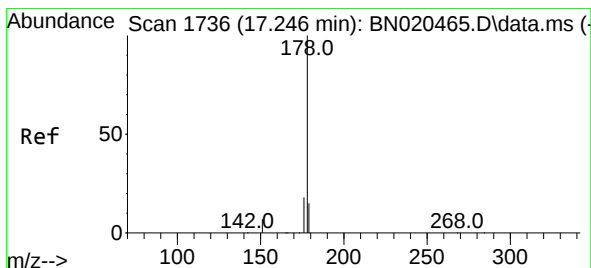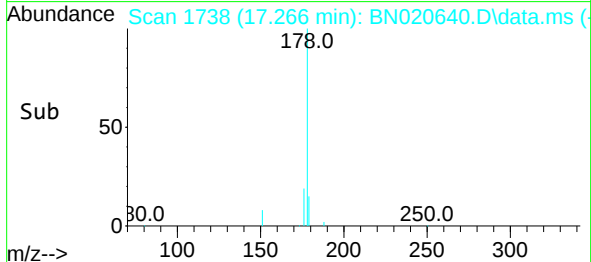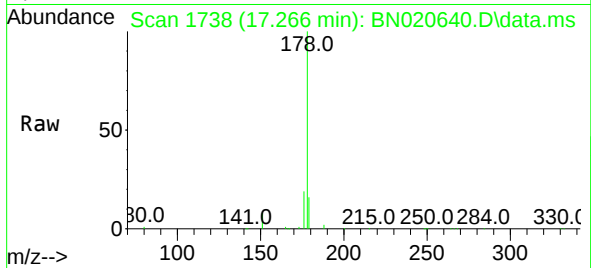

#26
Anthracene
Concen: 0.353 ng
RT: 17.359 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:178 Resp: 15313
Ion Ratio Lower Upper
178 100
176 18.8 14.9 22.3
179 15.0 12.2 18.4

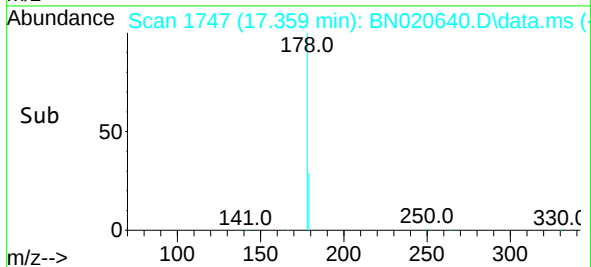

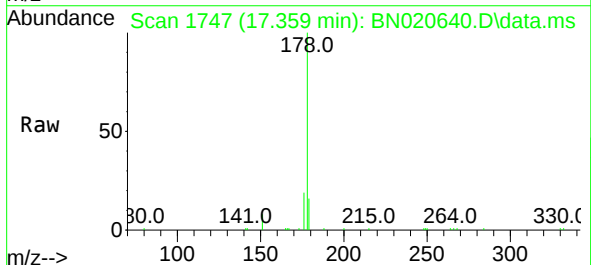




#27
Fluoranthene-d10
Concen: 0.367 ng
RT: 19.265 min Scan# 2110
Delta R.T. -0.004 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:212 Resp: 16252
Ion Ratio Lower Upper
212 100
106 15.3 12.6 19.0
104 8.7 7.2 10.8

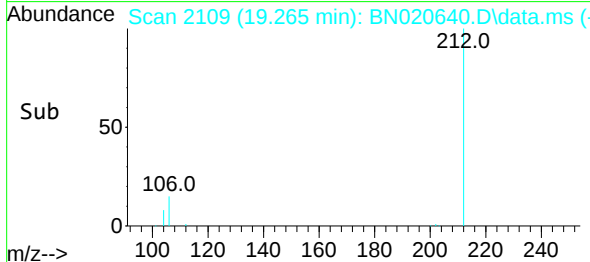

#28
Fluoranthene
Concen: 0.376 ng
RT: 19.295 min Scan# 2116
Delta R.T. -0.004 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:202 Resp: 20605
Ion Ratio Lower Upper
202 100
101 12.0 9.6 14.4
203 16.9 13.5 20.3


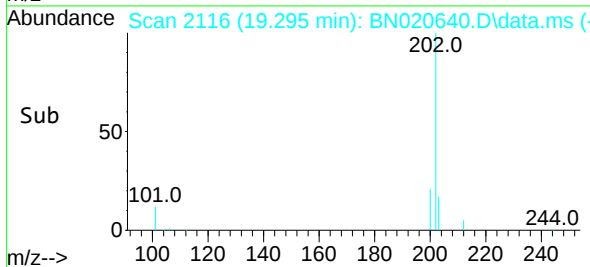

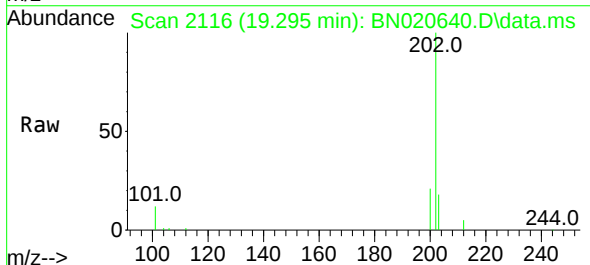




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.431 min Scan# 2444
Delta R.T. -0.000 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:240 Resp: 11792
Ion Ratio Lower Upper
240 100
120 11.4 14.6 21.8#
236 27.9 22.6 33.8

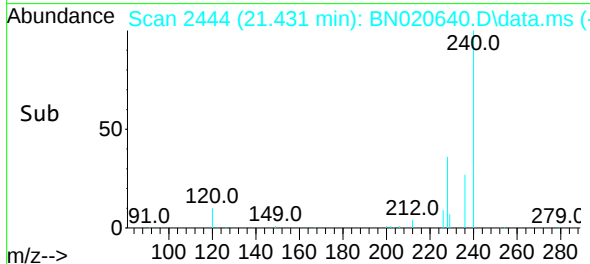

#30
Pyrene
Concen: 0.419 ng
RT: 19.657 min Scan# 2202
Delta R.T. -0.004 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:202 Resp: 20897
Ion Ratio Lower Upper
202 100
200 20.7 16.6 25.0
203 17.6 14.2 21.2

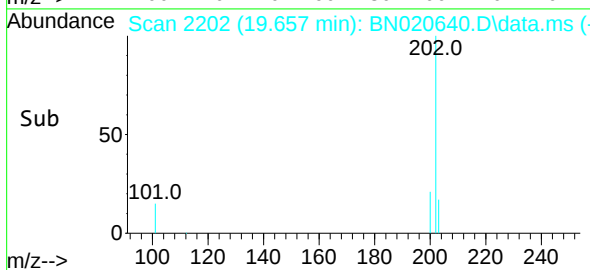

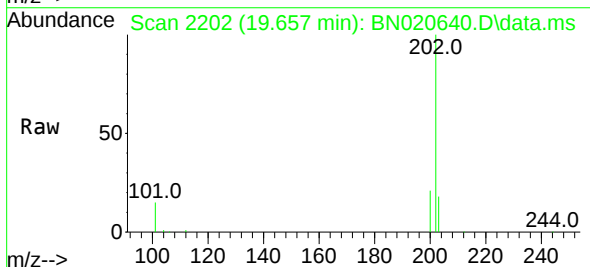




#31
 Terphenyl-d14
 Concen: 0.418 ng
 RT: 19.868 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN020640.D
 Acq: 02 Jul 2022 23:38




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:244 Resp: 11772
 Ion Ratio Lower Upper
 244 100
 212 8.9 7.1 10.7
 122 0.0 0.0 0.0

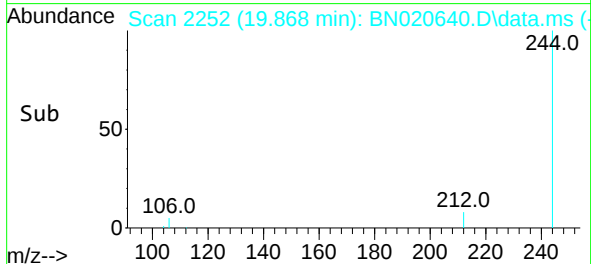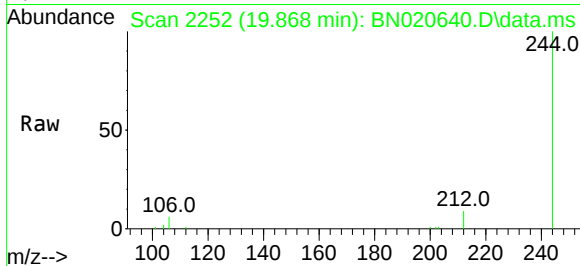

#32
 Benzo(a)anthracene
 Concen: 0.345 ng
 RT: 21.413 min Scan# 2442
 Delta R.T. -0.009 min
 Lab File: BN020640.D
 Acq: 02 Jul 2022 23:38

Tgt Ion:228 Resp: 14515
 Ion Ratio Lower Upper
 228 100
 226 27.3 21.2 31.8
 229 19.7 15.6 23.4

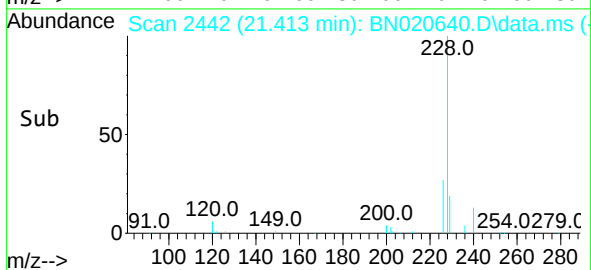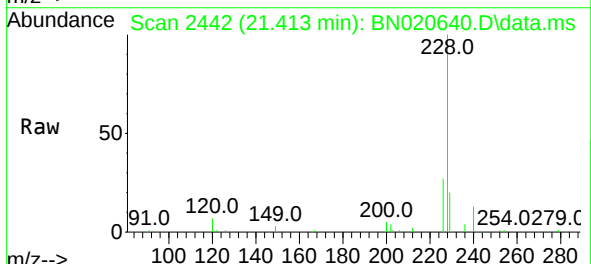



#33

Chrysene

Concen: 0.399 ng

RT: 21.467 min Scan# 2448

Delta R.T. 0.000 min

Lab File: BN020640.D

Acq: 02 Jul 2022 23:38

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:228 Resp: 18595

Ion Ratio Lower Upper

228 100

226 30.5 23.4 35.0

229 19.8 15.7 23.5

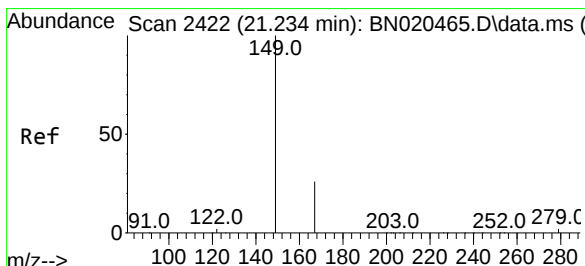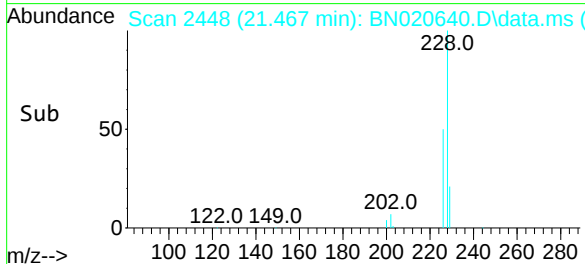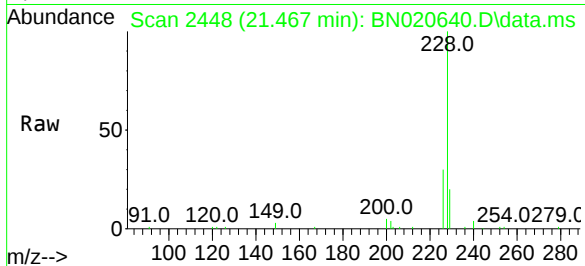

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.346 ng

RT: 21.351 min Scan# 2435

Delta R.T. 0.000 min

Lab File: BN020640.D

Acq: 02 Jul 2022 23:38




Tgt Ion:149 Resp: 8222

Ion Ratio Lower Upper

149 100

167 26.3 21.7 32.5

279 2.7 2.2 3.2

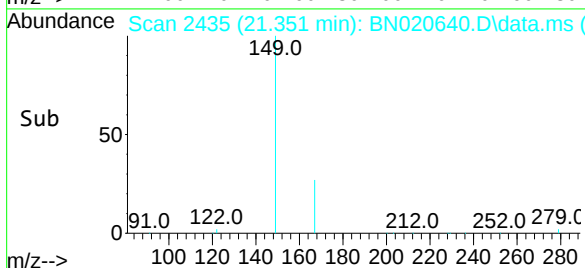
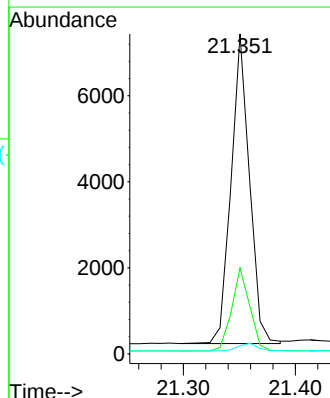
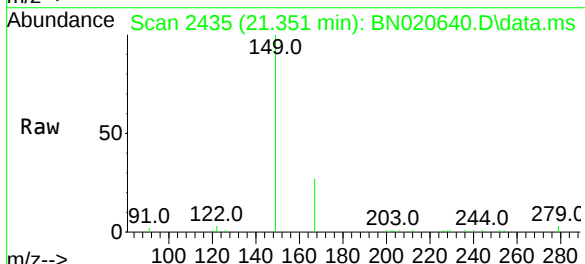




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.784 min Scan# 30
Delta R.T. -0.006 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:264	Resp:	9289
Ion Ratio	Lower	Upper
264	100	
260	26.6	20.9 31.3
265	33.3	28.0 42.0

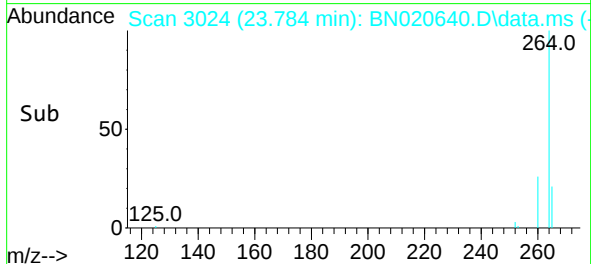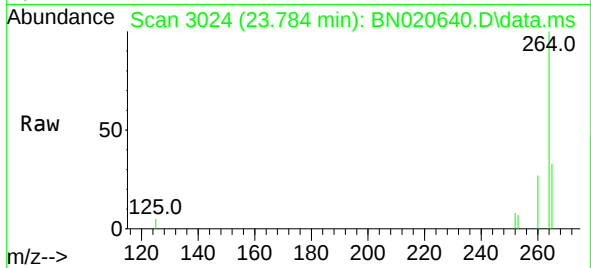

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.355 ng
RT: 26.217 min Scan# 3856
Delta R.T. -0.006 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Tgt Ion:276	Resp:	14707
Ion Ratio	Lower	Upper
276	100	
138	32.9	25.9 38.9
277	24.5	19.8 29.8

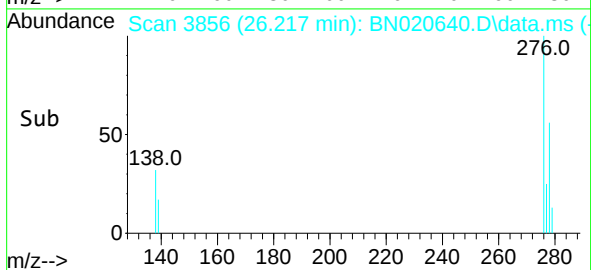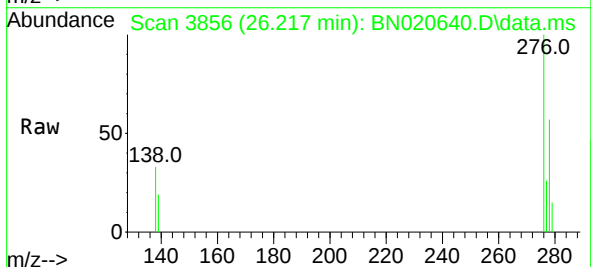



#37

Benzo(b)fluoranthene

Concen: 0.410 ng

RT: 23.068 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN020640.D

Acq: 02 Jul 2022 23:38

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4





Tgt Ion:252 Resp: 14662

Ion Ratio Lower Upper

252 100

253 23.7 18.5 27.7

125 16.4 11.4 17.0

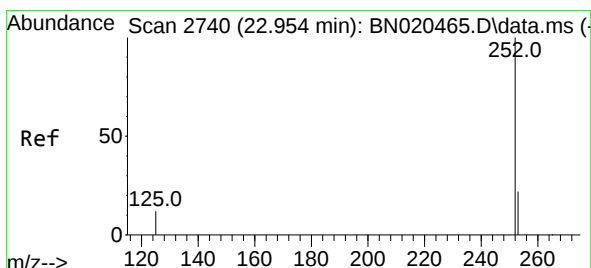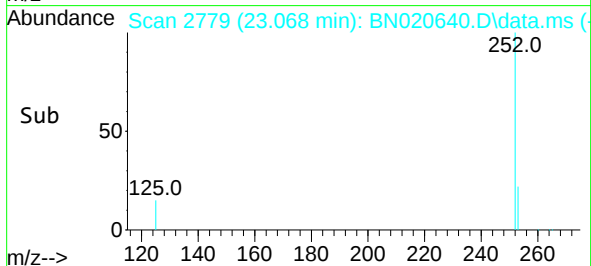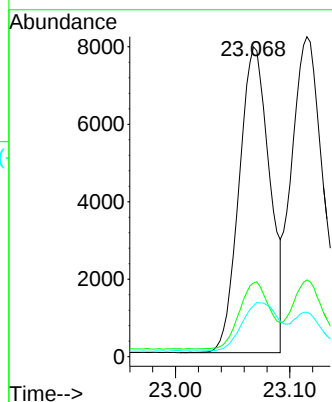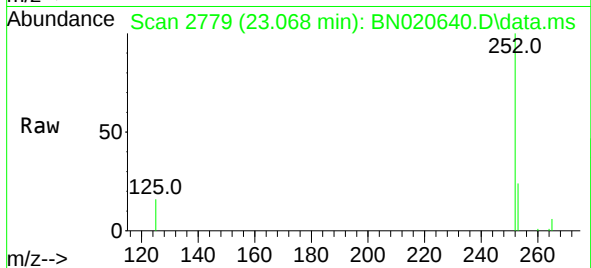

#38

Benzo(k)fluoranthene

Concen: 0.414 ng

RT: 23.115 min Scan# 2795

Delta R.T. -0.006 min

Lab File: BN020640.D

Acq: 02 Jul 2022 23:38




Tgt Ion:252 Resp: 15768

Ion Ratio Lower Upper

252 100

253 24.0 18.0 27.0

125 13.9 11.0 16.4

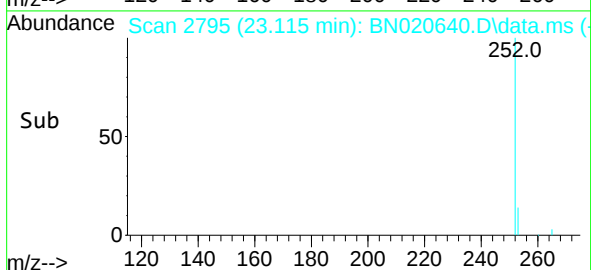

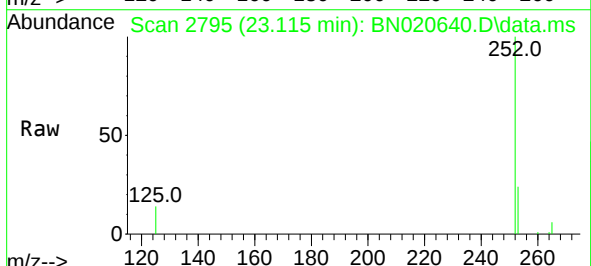




#39
Benzo(a)pyrene
Concen: 0.385 ng
RT: 23.682 min Scan# 2926
Delta R.T. -0.003 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 11937
Ion Ratio Lower Upper
252 100
253 26.8 19.0 28.4
125 25.4 13.8 20.8#

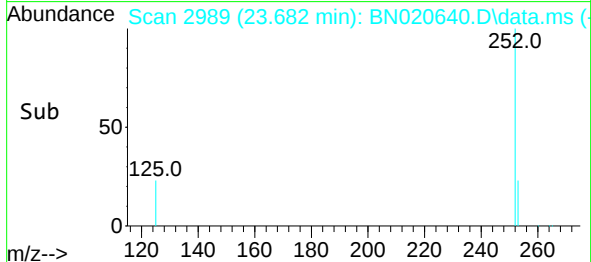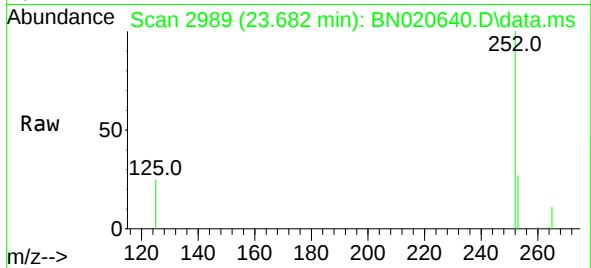

#40
Dibenzo(a,h)anthracene
Concen: 0.353 ng
RT: 26.232 min Scan# 3861
Delta R.T. -0.015 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38


Tgt Ion:278 Resp: 11730
Ion Ratio Lower Upper
278 100
139 24.8 18.6 28.0
279 26.4 19.7 29.5

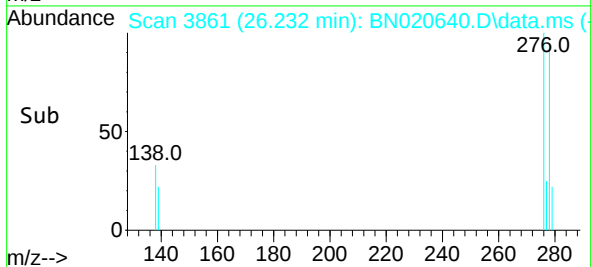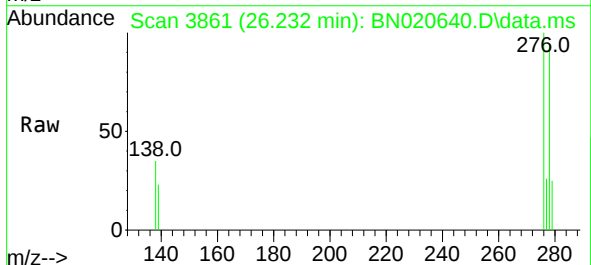



#41
Benzo(g,h,i)perylene
Concen: 0.339 ng
RT: 26.957 min Scan# 41
Delta R.T. -0.012 min
Lab File: BN020640.D
Acq: 02 Jul 2022 23:38

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

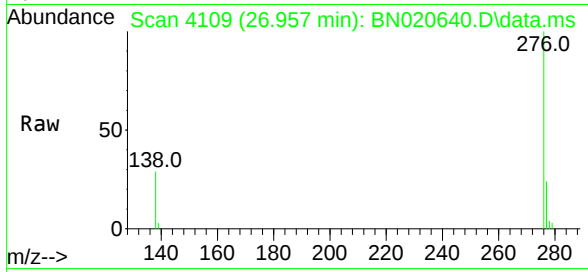

Tgt Ion:276 Resp: 12299
Ion Ratio Lower Upper
276 100
277 24.4 19.5 29.3
138 29.4 22.6 34.0

