
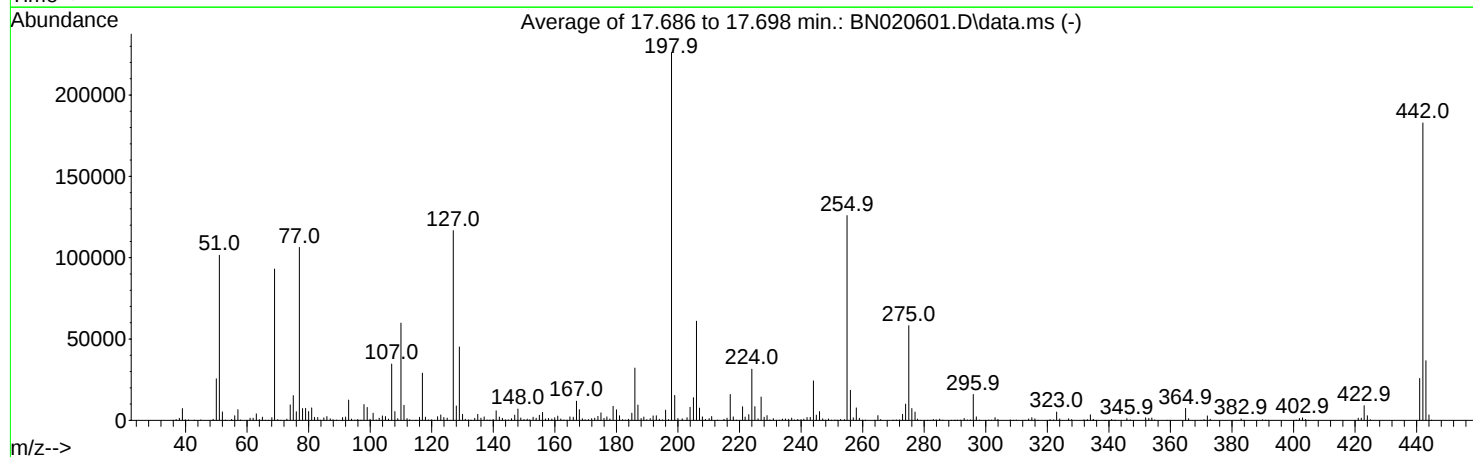


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
 Data File : BN020601.D
 Acq On : 01 Jul 2022 20:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 02 03:10:12 2022

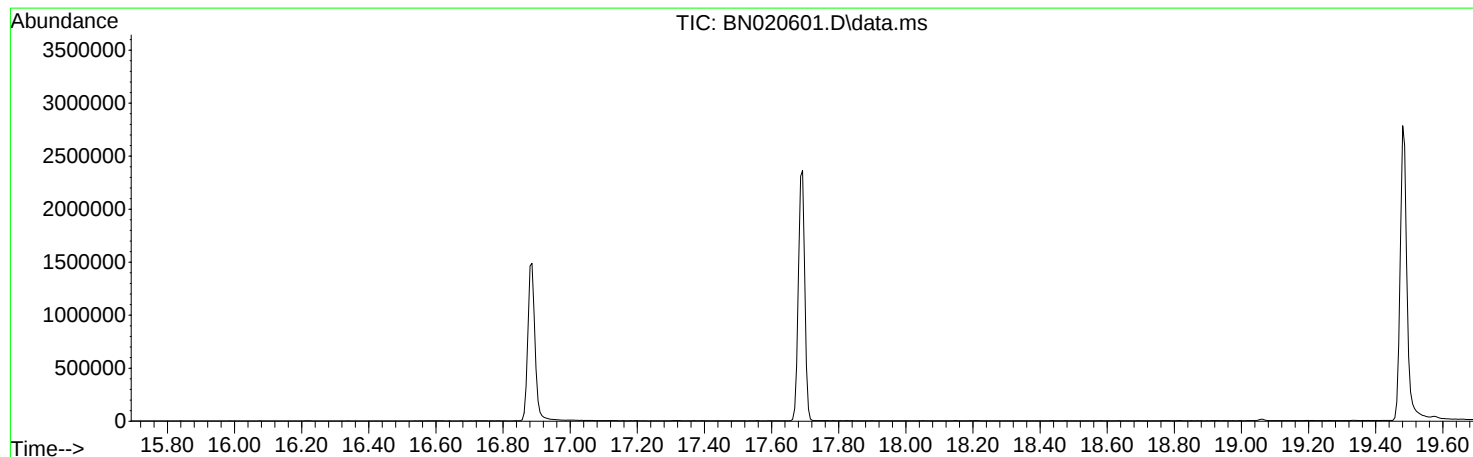




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	101547	PASS
68	69	0.00	2	1.9	1722	PASS
69	198	0.00	100	41.1	93051	PASS
70	69	0.00	2	0.5	497	PASS
127	198	10	80	51.6	116632	PASS
197	198	0.00	2	0.2	544	PASS
198	198	100	100	100.0	226155	PASS
199	198	5	9	6.8	15396	PASS
275	198	10	60	25.7	58197	PASS
365	198	1	100	3.3	7367	PASS
441	198	0.01	100	11.4	25813	PASS
442	442	50	100	100.0	182912	PASS
443	442	15	24	20.1	36731	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
Data File : BN020601.D
Acq On : 01 Jul 2022 20:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 02 04:34:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 02 04:34:03 2022
Response via : Initial Calibration

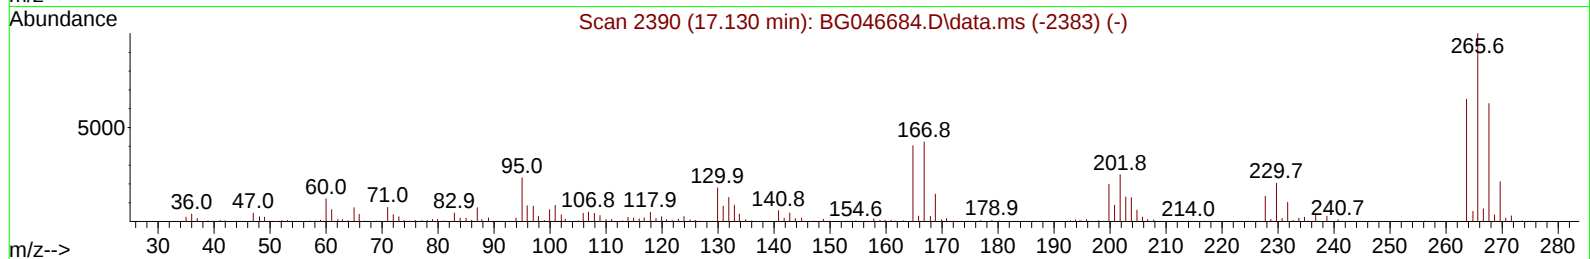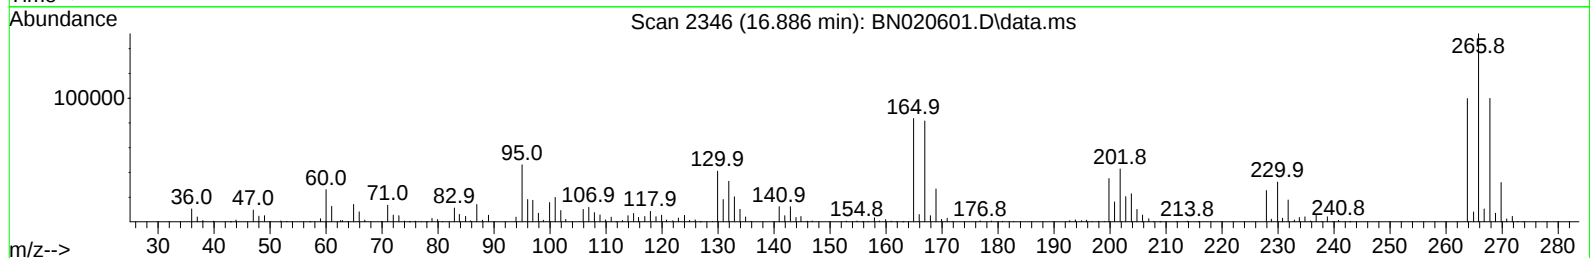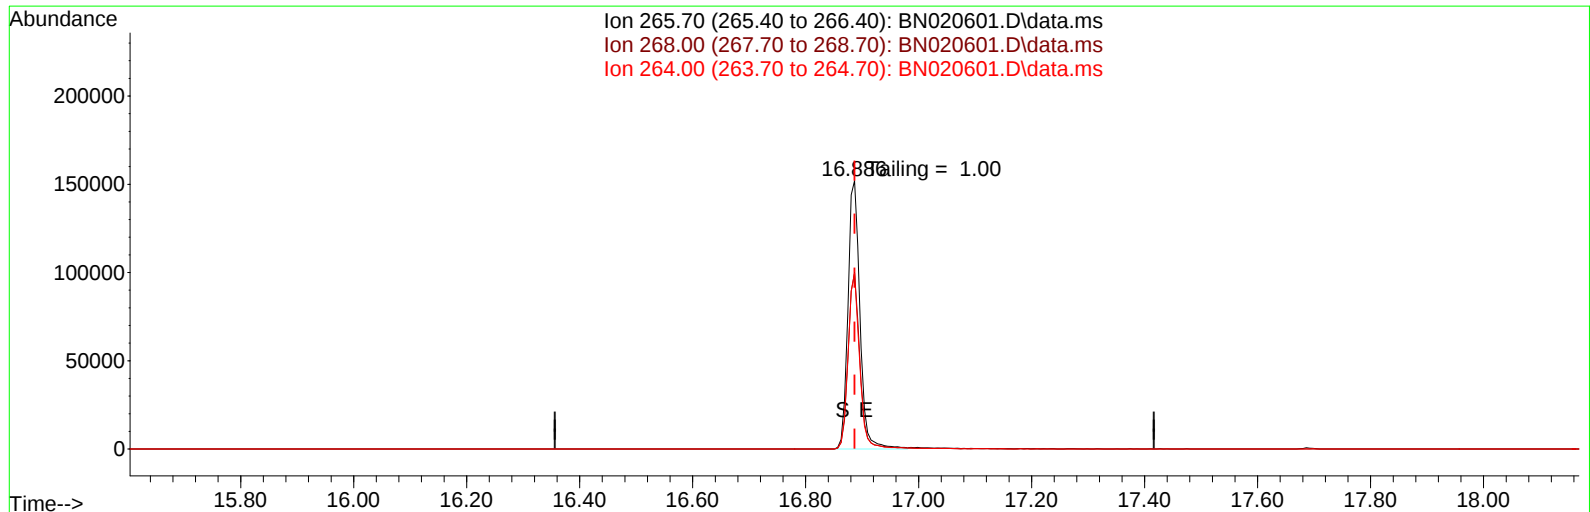

TIC: BN020601.D\data.ms

(70) Pentachlorophenol (C)

16.886min (0.000) 15636.11 ng




response 226274

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.67
264.00	61.60	65.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
 Data File : BN020601.D
 Acq On : 01 Jul 2022 20:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 02 04:34:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 02 04:34:03 2022
 Response via : Initial Calibration

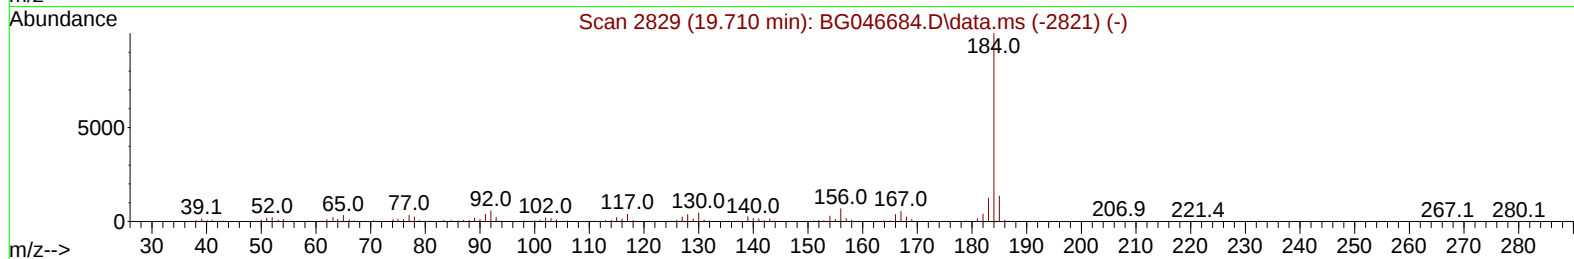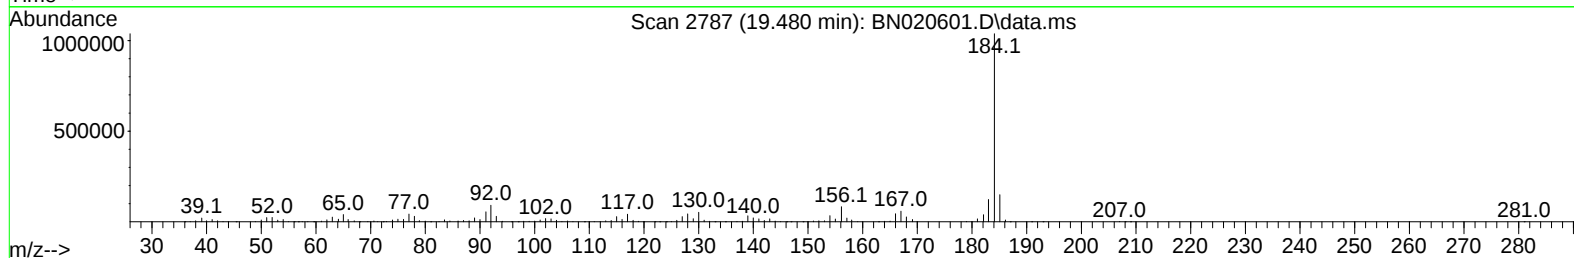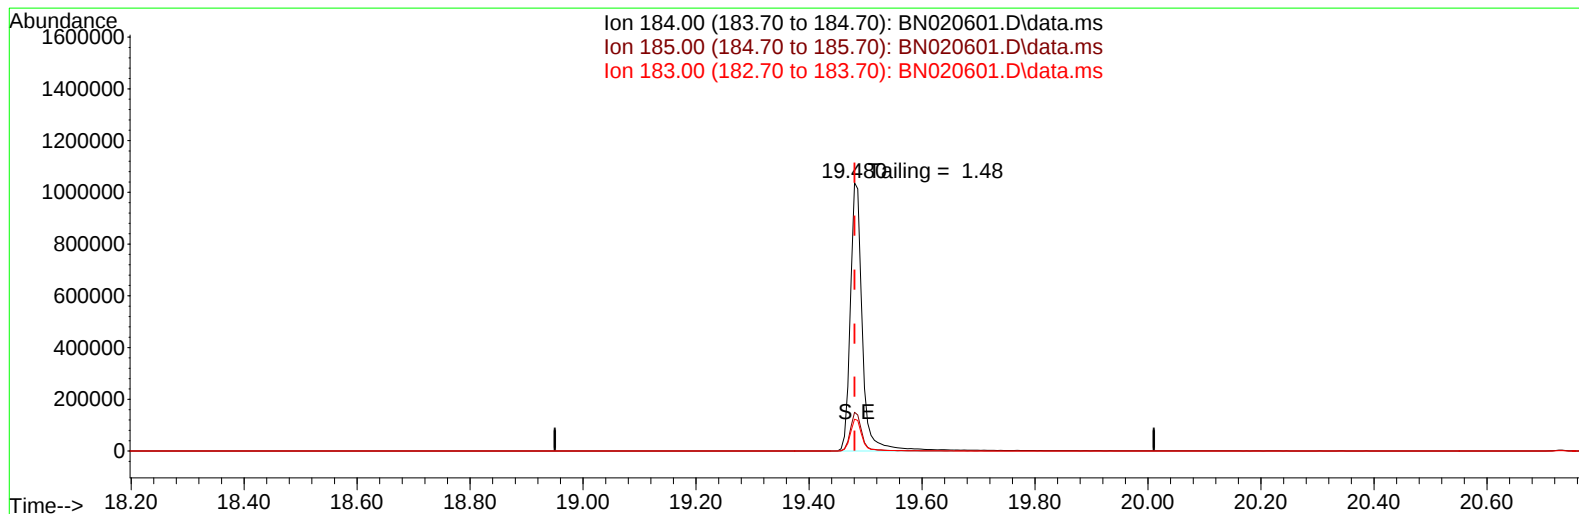

TIC: BN020601.D\data.ms

(77) Benzidine

19.480min (0.000) 0.00 ng

response 1556957

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/1/2022	BNA_N	<u>BN020601.D</u>
Compound Name	Response	Retention Time
DDT	764628	20.727
DDD	23649	20.286
DDE	1183	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24832	789460	3.15

Instrument :
BNA_N
ClientSampleId :
DFTPP