
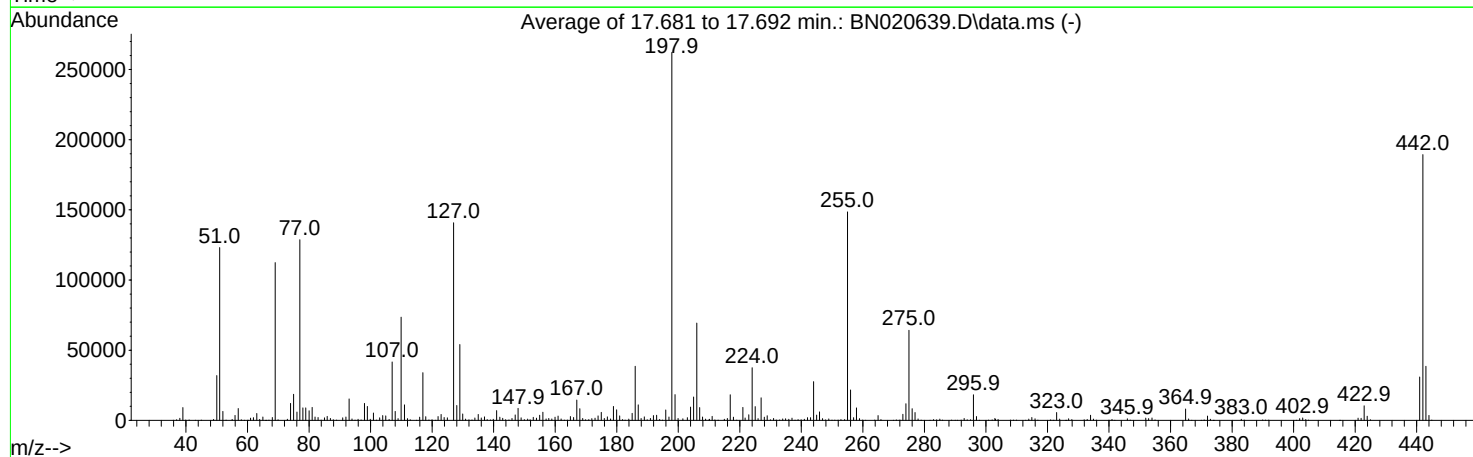


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
 Data File : BN020639.D
 Acq On : 02 Jul 2022 21:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 02 03:10:12 2022

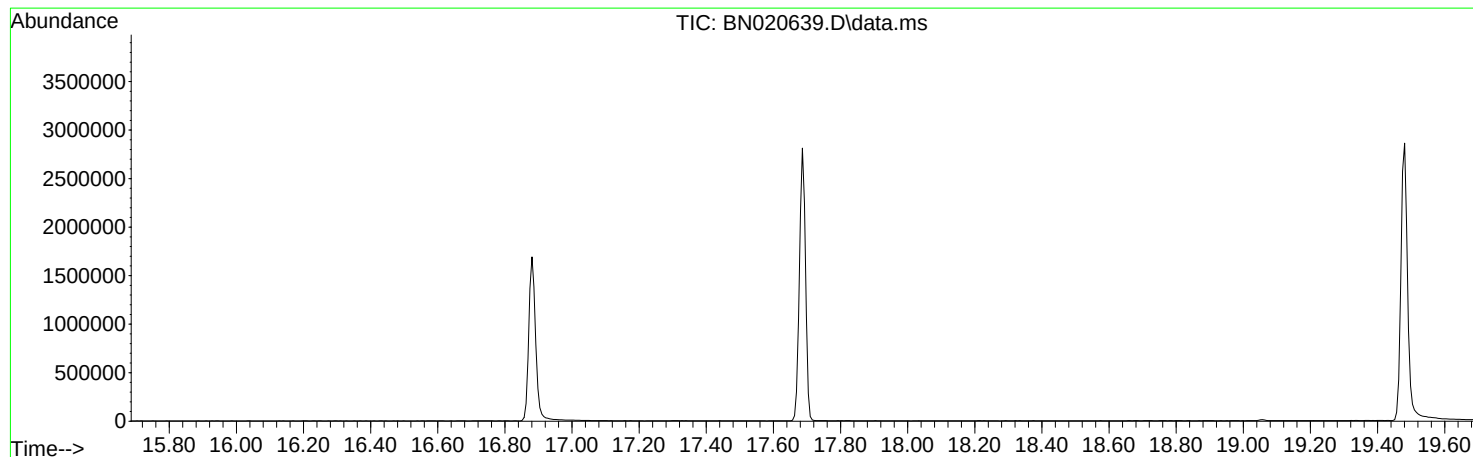




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	123169	PASS
68	69	0.00	2	1.8	2033	PASS
69	198	0.00	100	42.9	112483	PASS
70	69	0.00	2	0.5	523	PASS
127	198	10	80	53.7	140848	PASS
197	198	0.00	2	0.9	2397	PASS
198	198	100	100	100.0	262144	PASS
199	198	5	9	7.0	18405	PASS
275	198	10	60	24.5	64160	PASS
365	198	1	100	3.1	8067	PASS
441	198	0.01	100	11.8	30960	PASS
442	442	50	100	100.0	189376	PASS
443	442	15	24	20.4	38541	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
 Data File : BN020639.D
 Acq On : 02 Jul 2022 21:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 04 05:04:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 04 05:02:31 2022
 Response via : Initial Calibration

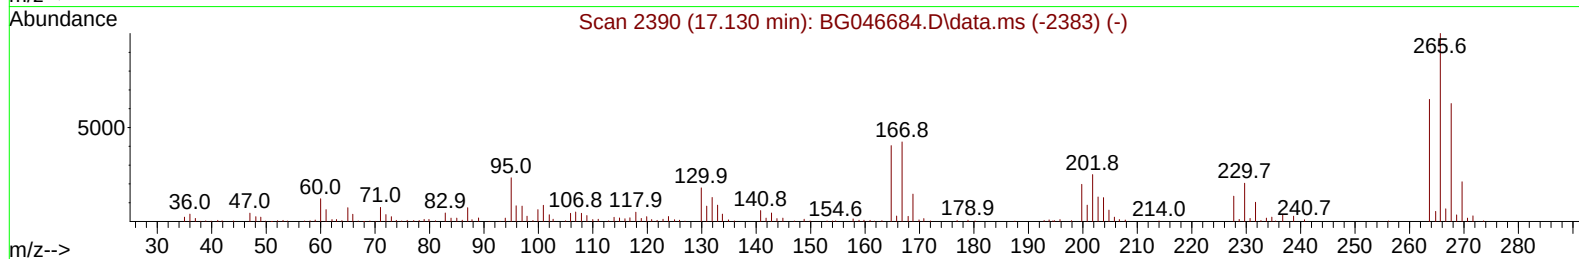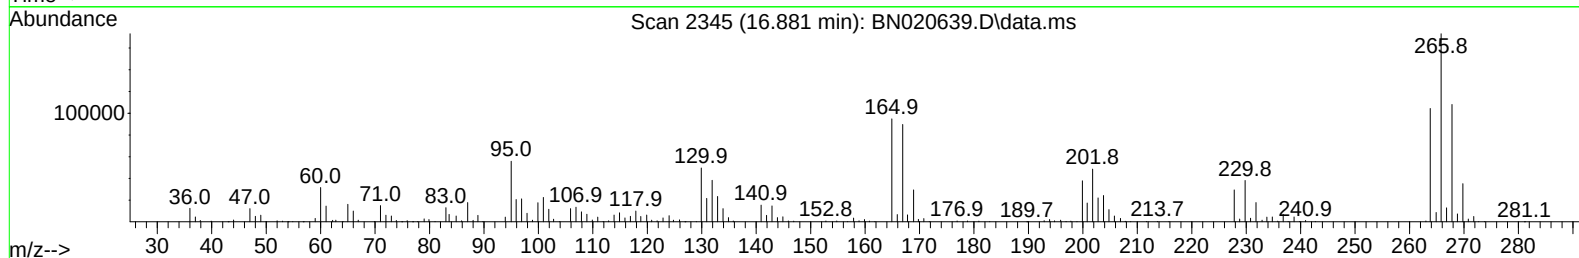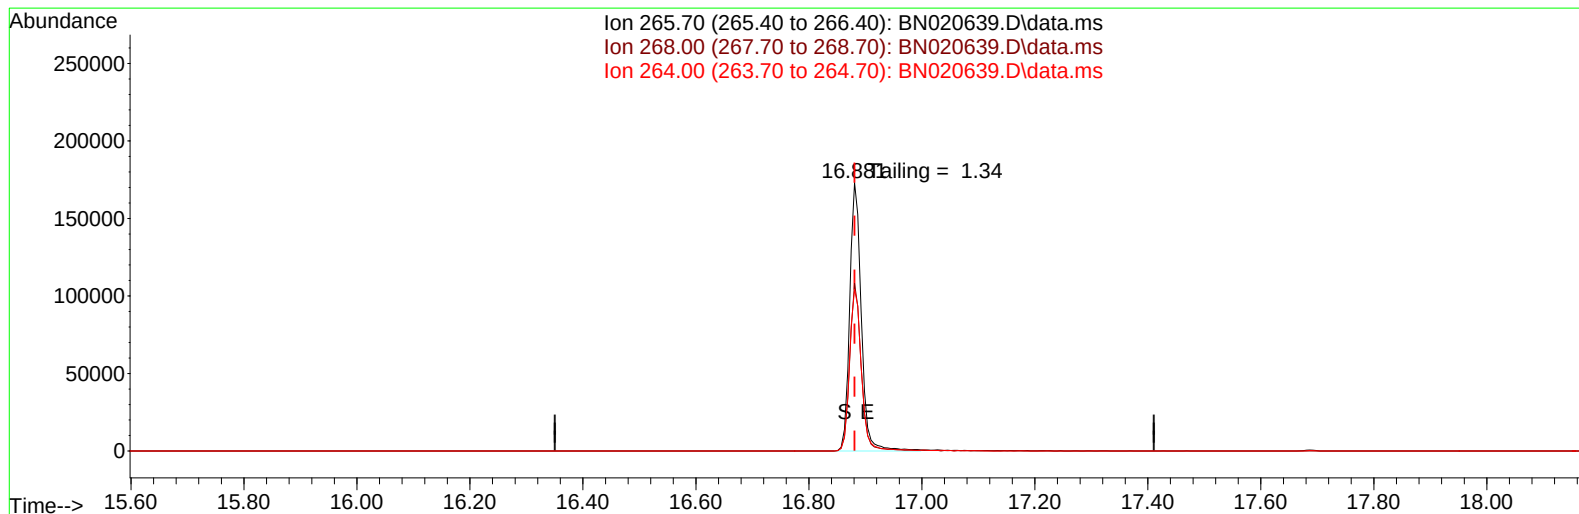

TIC: BN020639.D\data.ms

(70) Pentachlorophenol (C)

16.881min (-0.000) 16118.46 ng




response 248560

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.41
264.00	61.60	60.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070222\
Data File : BN020639.D
Acq On : 02 Jul 2022 21:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 04 05:04:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 04 05:02:31 2022
Response via : Initial Calibration

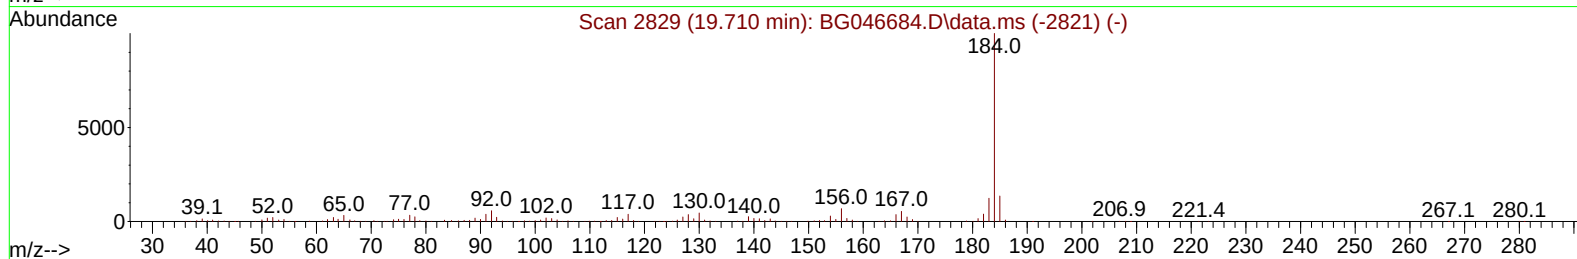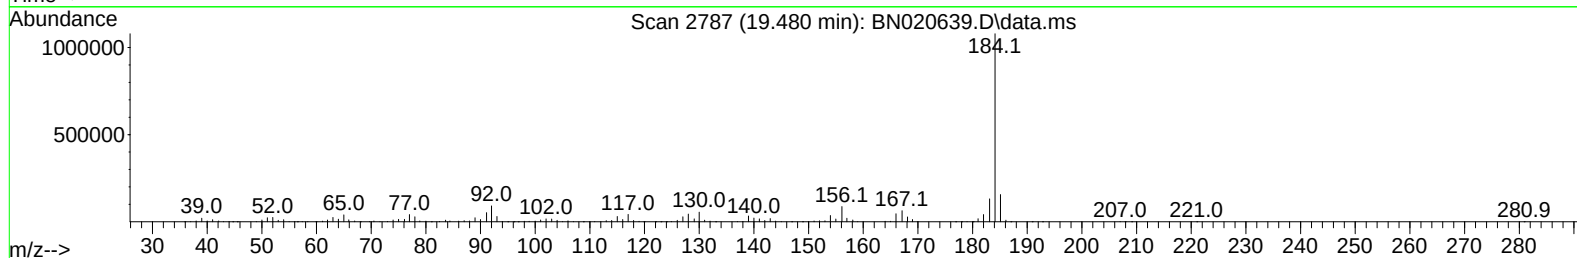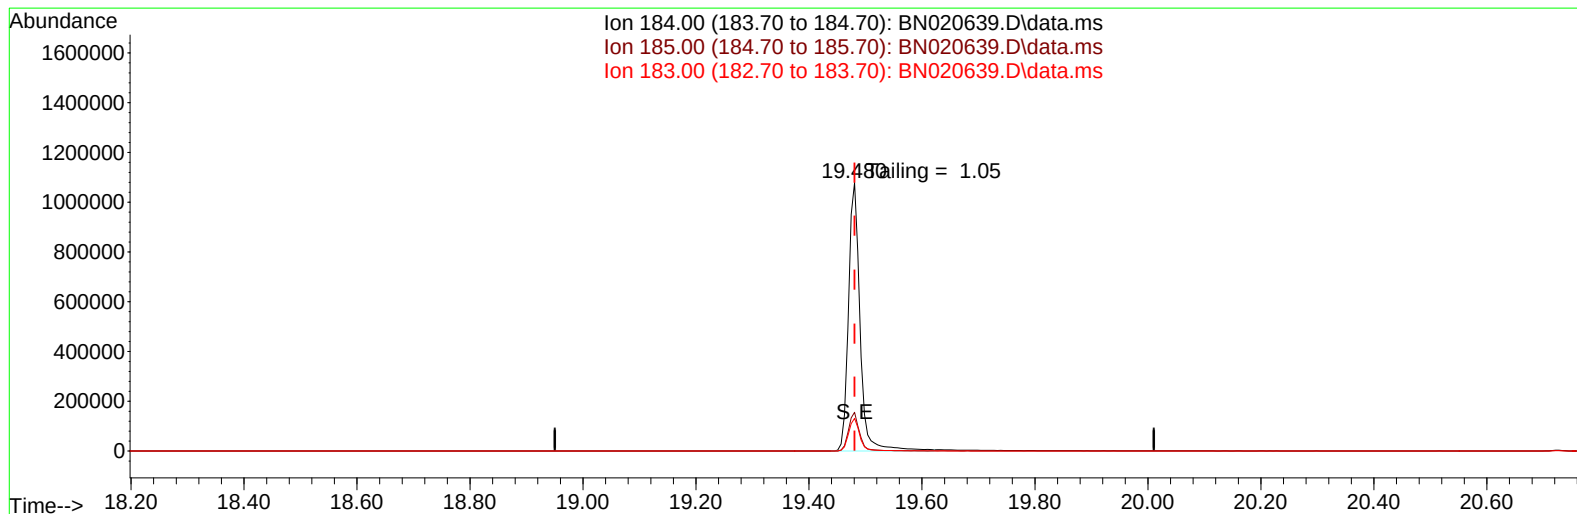

TIC: BN020639.D\data.ms

(77) Benzidine

19.480min (-0.000) 0.00 ng

response 1555270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	12.17
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/2/2022	BNA_N	<u>BN020639.D</u>
Compound Name	Response	Retention Time
DDT	856757	20.727
DDD	20066	20.28
DDE	1031	19.775
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21097	877854	2.40

Instrument :
BNA_N
ClientSampleId :
DFTPP