

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
 Data File : BN026146.D
 Acq On : 01 Jul 2023 11:47
 Operator : MA/JU
 Sample : PB153575BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK575

Quant Time: Jul 01 22:34:20 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 01:46:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.959	152	7494	0.400	ng/ul	0.00
4) Naphthalene-d8	10.770	136	24446	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.598	164	13903	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.347	188	24072	0.400	ng/ul	0.00
17) Chrysene-d12	21.544	240	12420	0.400	ng/ul	0.00
23) Perylene-d12	24.002	264	15642	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.318	96	40762	4.830	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.365	152	10568	0.281	ng/ul	0.00
18) Fluoranthene-d10	19.377	212	15425	0.326	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.593	166	3508	0.057	ng/ul#	13
20) Pyrene	19.740	202	2489	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	4614	0.080	ng/ul#	30


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
Data File : BN026146.D
Acq On : 01 Jul 2023 11:47
Operator : MA/JU
Sample : PB153575BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK575

Quant Time: Jul 01 22:34:20 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 01:46:24 2023
Response via : Initial Calibration




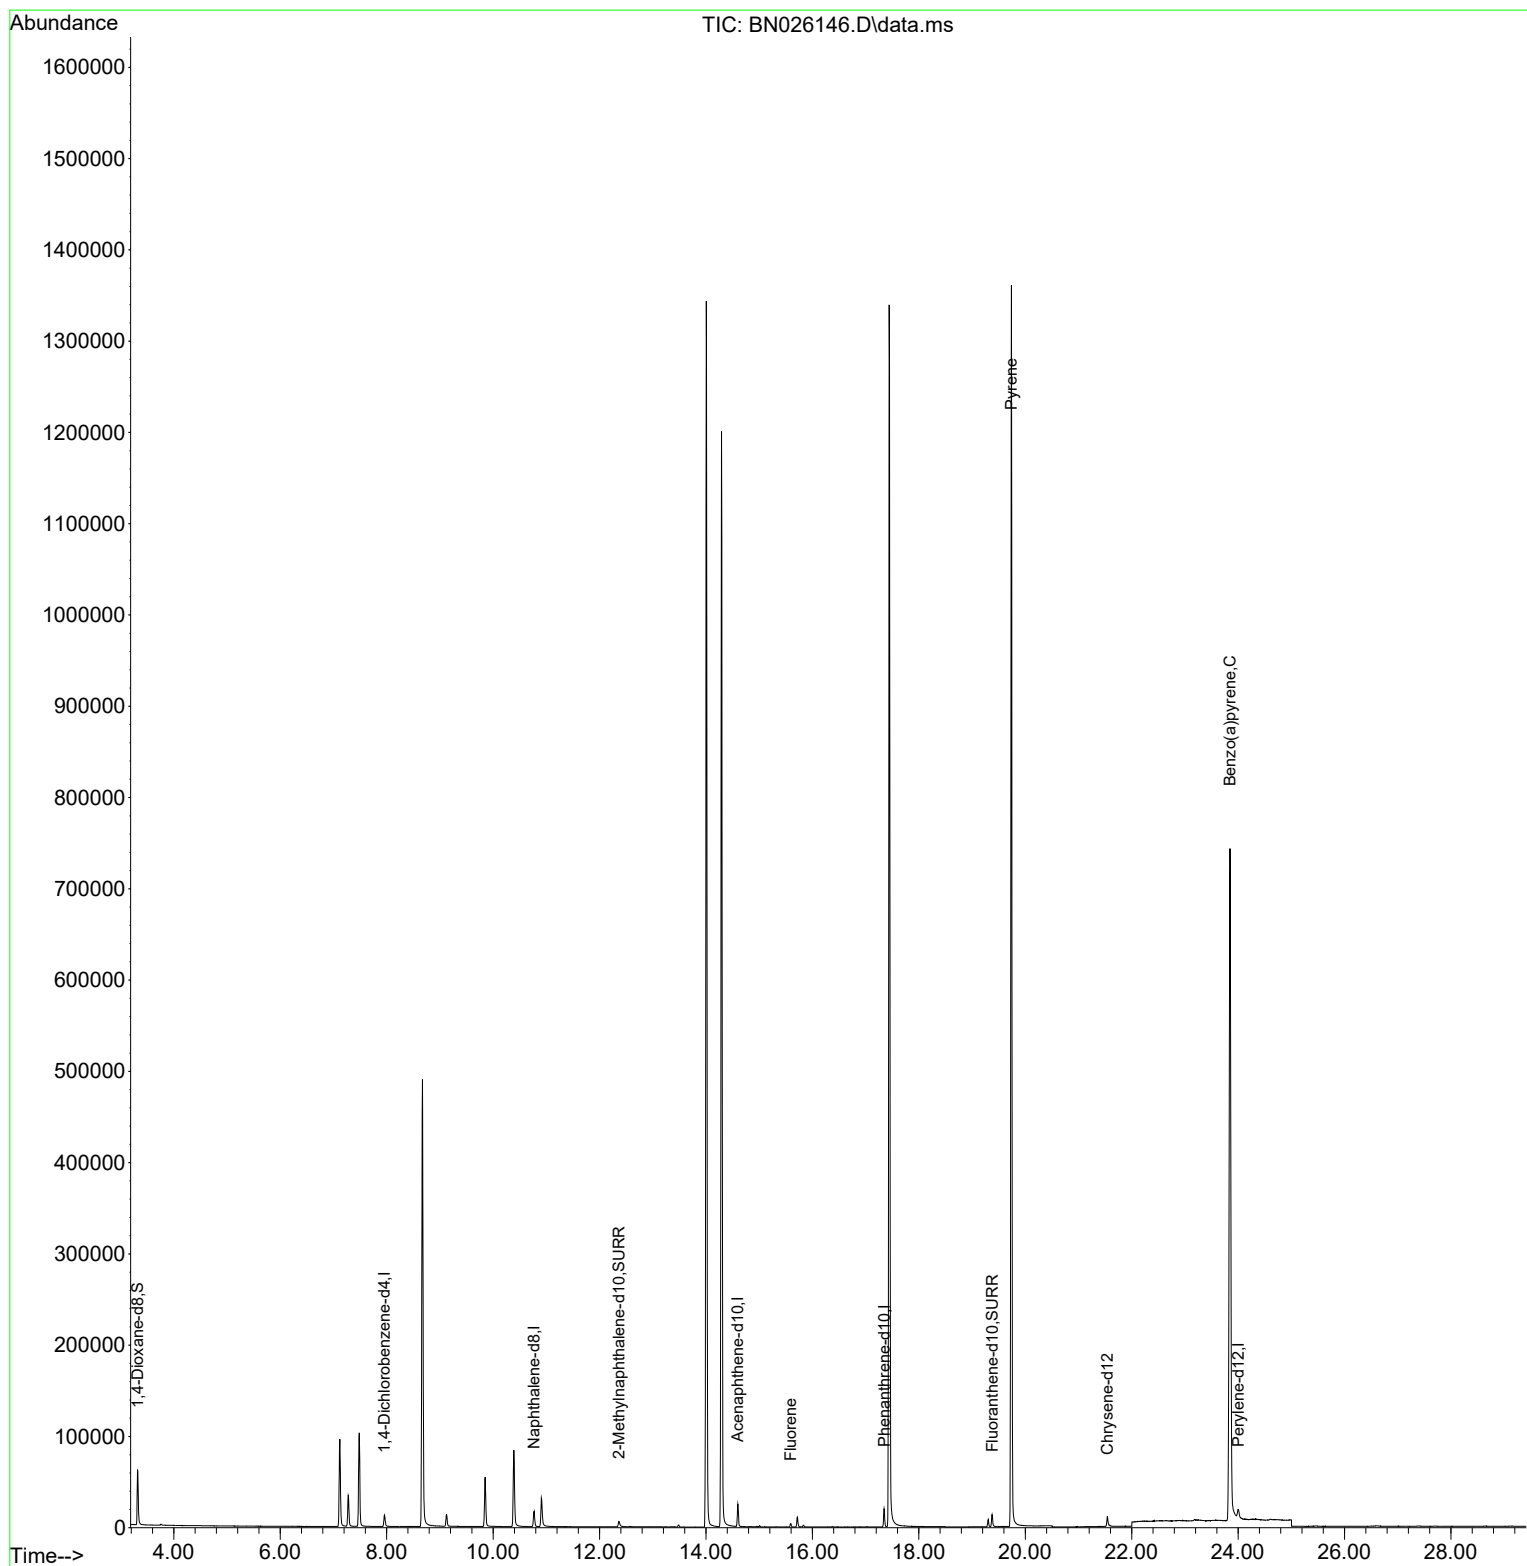


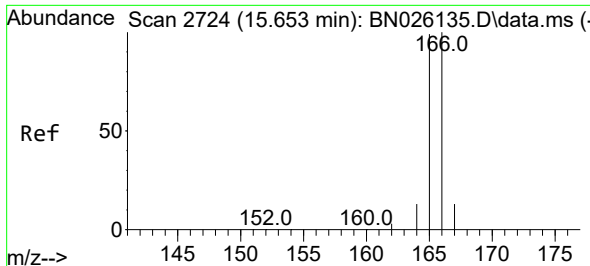

#12
Fluorene
Concen: 0.057 ng/ul
RT: 15.593 min Scan# 21
Delta R.T. -0.061 min
Lab File: BN026146.D
Acq: 01 Jul 2023 11:47




Instrument :
BNA_N
ClientSampleId :
SBLK575


Tgt Ion:166 Resp: 3508
Ion Ratio Lower Upper
166 100
165 7.9 79.9 119.9#
167 34.7 10.8 16.2#

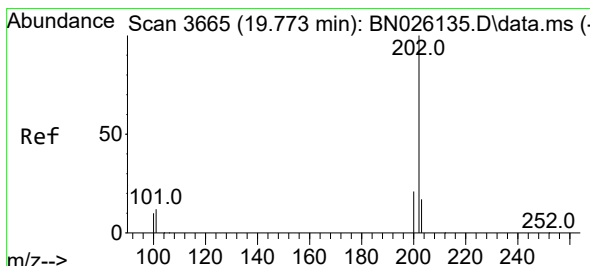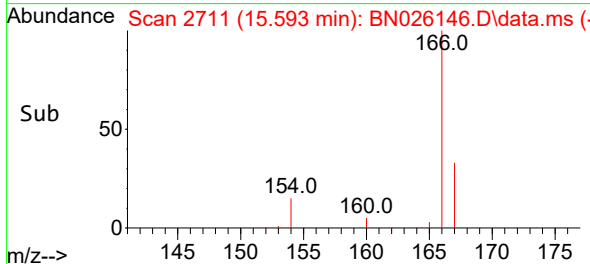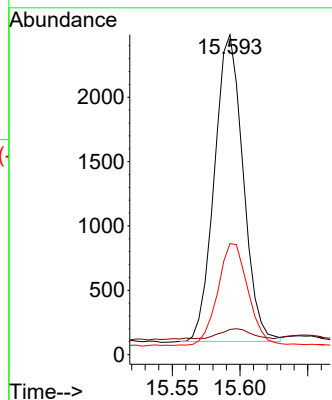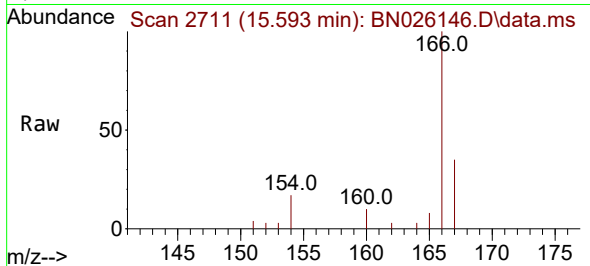

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.740 min Scan# 3658
Delta R.T. -0.033 min
Lab File: BN026146.D
Acq: 01 Jul 2023 11:47


Tgt Ion:202 Resp: 2489
Ion Ratio Lower Upper
202 100
101 170.5 11.4 17.0#
100 1250.8 9.1 13.7#

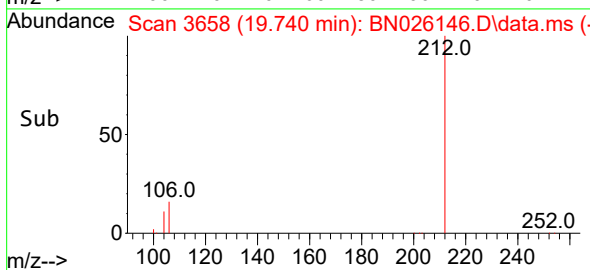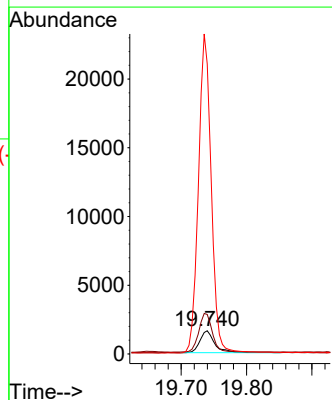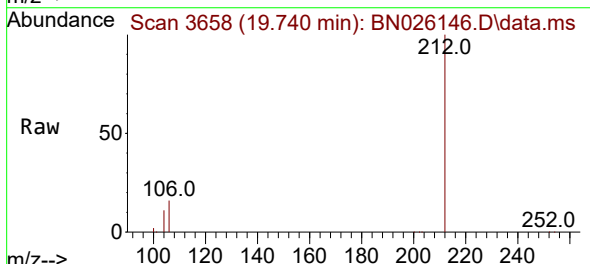

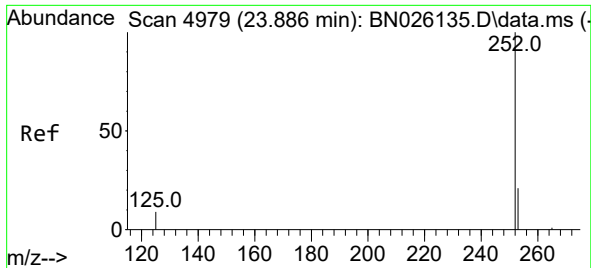

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.847 min Scan# 4966
Delta R.T. -0.039 min
Lab File: BN026146.D
Acq: 01 Jul 2023 11:47

Instrument :
BNA_N
ClientSampleId :
SBLK575

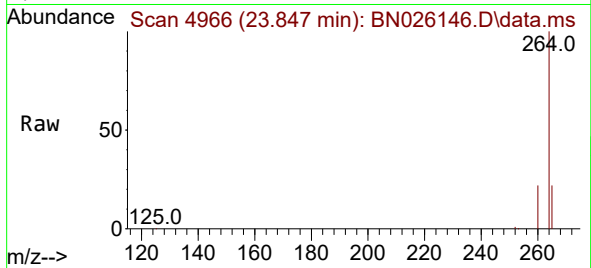

Tgt Ion:252 Resp: 4614
Ion Ratio Lower Upper
252 100
253 64.4 26.0 39.0#
125 64.0 17.3 25.9#

