

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
 Data File : BN026231.D
 Acq On : 03 Jul 2023 18:43
 Operator : MA/JU
 Sample : PB153769BL
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK769

Quant Time: Jul 04 00:40:27 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 04 00:40:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	8432	0.400	ng/ul	0.00
4) Naphthalene-d8	10.765	136	27198	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.598	164	15841	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.347	188	29749	0.400	ng/ul	0.00
17) Chrysene-d12	21.538	240	15566	0.400	ng/ul	0.00
23) Perylene-d12	24.008	264	19519	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	42685	4.495	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.360	152	11822	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.377	212	19407	0.328	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.740	202	3466	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.841	252	6156	0.085	ng/ul#	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
Data File : BN026231.D
Acq On : 03 Jul 2023 18:43
Operator : MA/JU
Sample : PB153769BL
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK769

Quant Time: Jul 04 00:40:27 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 04 00:40:07 2023
Response via : Initial Calibration




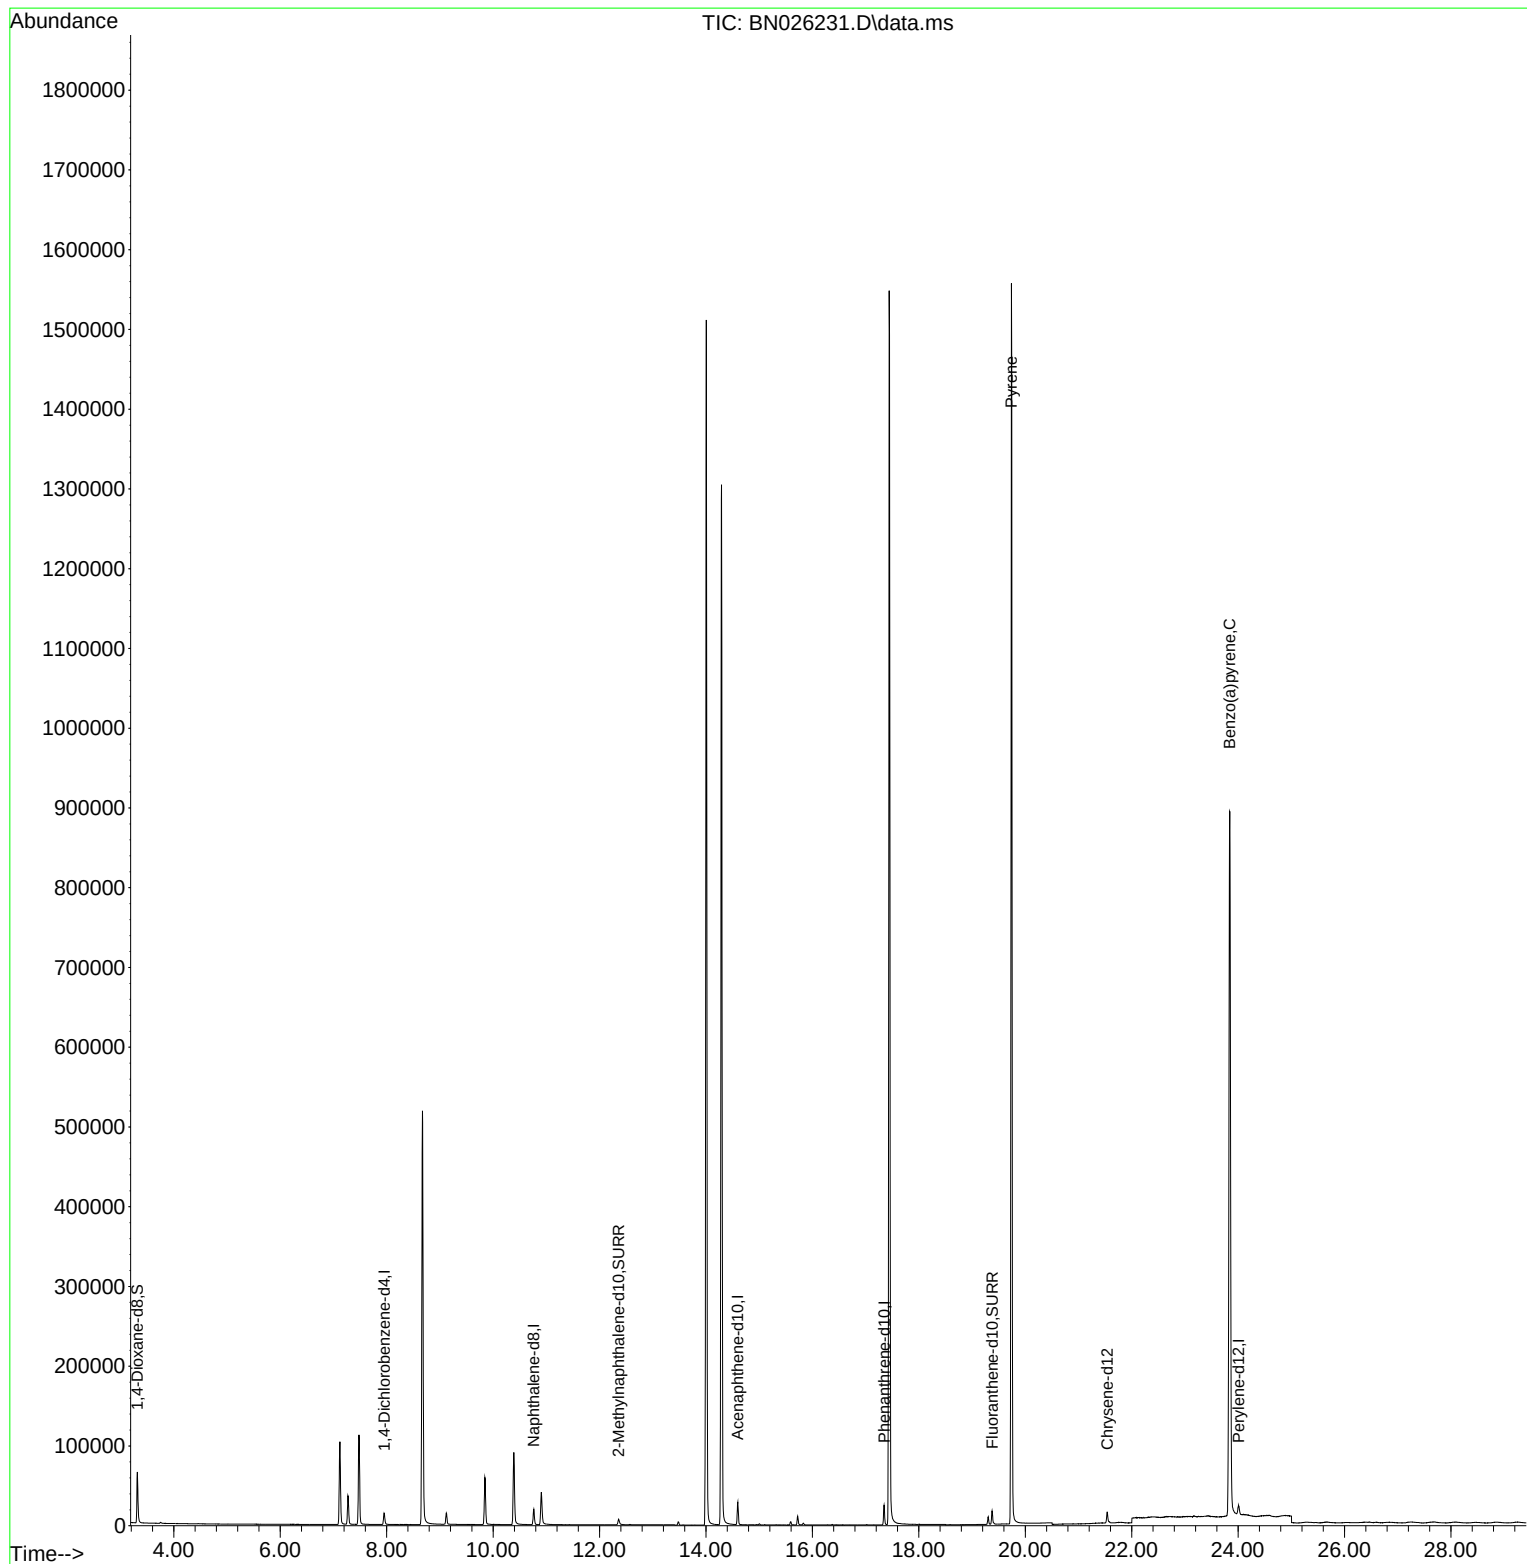


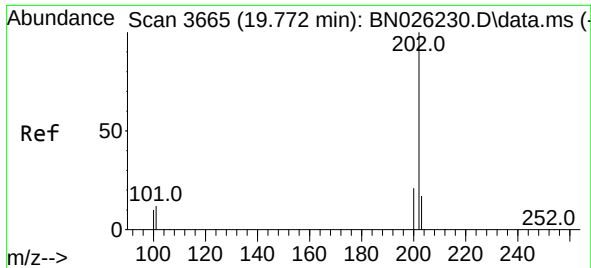

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.740 min Scan# 3658
Delta R.T. -0.032 min
Lab File: BN026231.D
Acq: 03 Jul 2023 18:43

Instrument :
BNA_N
ClientSampleId :
SBLK769

Tgt Ion:202 Resp: 3466
Ion Ratio Lower Upper
202 100
101 177.6 11.4 17.0#
100 1332.9 9.1 13.7#

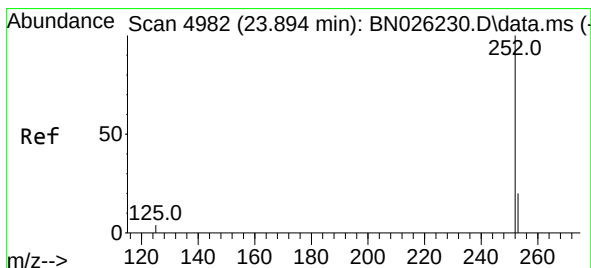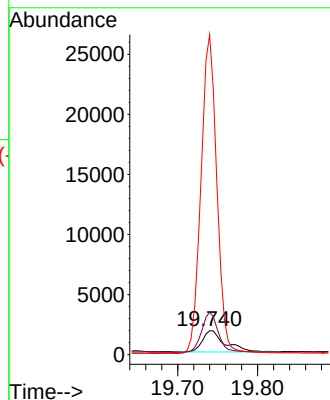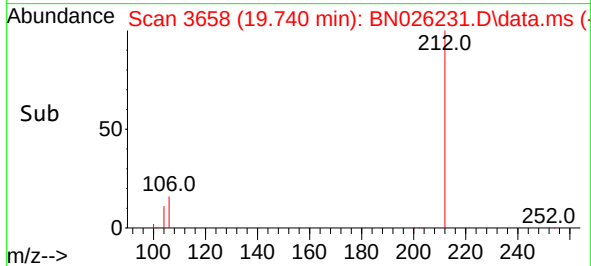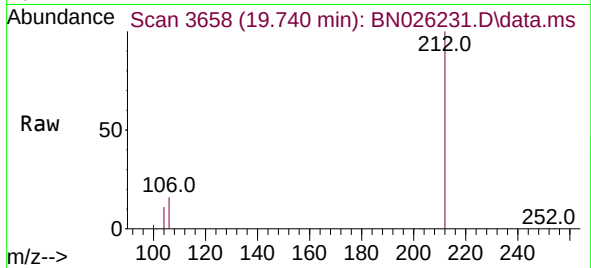

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.841 min Scan# 4964
Delta R.T. -0.053 min
Lab File: BN026231.D
Acq: 03 Jul 2023 18:43

Tgt Ion:252 Resp: 6156
Ion Ratio Lower Upper
252 100
253 72.5 26.0 39.0#
125 83.3 17.3 25.9#

