

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
 Data File : BN026184.D
 Acq On : 02 Jul 2023 12:05
 Operator : MA/JU
 Sample : 03247-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGL2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :Sohil Jodhani 07/04/2023

Quant Time: Jul 03 05:39:31 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 01:46:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	8803	0.400	ng/ul	0.00
4) Naphthalene-d8	10.765	136	28467	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.598	164	16694	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.343	188	32467	0.400	ng/ul	0.00
17) Chrysene-d12	21.529	240	16860	0.400	ng/ul	#-0.01
23) Perylene-d12	23.990	264	17820	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.318	96	30536	3.080	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	9527	0.218	ng/ul	-0.01
18) Fluoranthene-d10	19.373	212	17210	0.268	ng/ul	0.00
Target Compounds					Qvalue	
5) Naphthalene	10.814	128	7702	0.094	ng/ul#	96
7) 2-Methylnaphthalene	12.425	142	5662	0.109	ng/ul	99
8) 1-Methylnaphthalene	12.645	142	4266	0.079	ng/ul	98
10) Acenaphthylene	14.316	152	7414	0.095	ng/ul#	91
11) Acenaphthene	14.658	153	3273	0.051	ng/ul	98
12) Fluorene	15.644	166	2560	0.035	ng/ul#	96
15) Phenanthrene	17.385	178	83165	0.775	ng/ul	100
16) Anthracene	17.478	178	12308	0.129	ng/ul	95
19) Fluoranthene	19.401	202	232174	2.578	ng/ul	99
20) Pyrene	19.763	202	188692	2.015	ng/ul	98
21) Benzo(a)anthracene	21.511	228	82583	1.187	ng/ul	97
22) Chrysene	21.564	228	104916	1.450	ng/ul	96
24) Benzo(b)fluoranthene	23.239	252	153249m	2.015	ng/ul	
25) Benzo(k)fluoranthene	23.277	252	51594m	0.676	ng/ul	
26) Benzo(a)pyrene	23.885	252	93710	1.419	ng/ul#	89
27) Indeno(1,2,3-cd)pyrene	26.568	276	78086	1.082	ng/ul#	84
28) Dibenzo(a,h)anthracene	26.578	278	17791	0.326	ng/ul#	88
29) Benzo(g,h,i)perylene	27.373	276	72018	1.122	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
Data File : BN026184.D
Acq On : 02 Jul 2023 12:05
Operator : MA/JU
Sample : 03247-06
Misc :
ALS Vial : 41 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCGL2

Quant Time: Jul 03 05:39:31 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 01:46:24 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

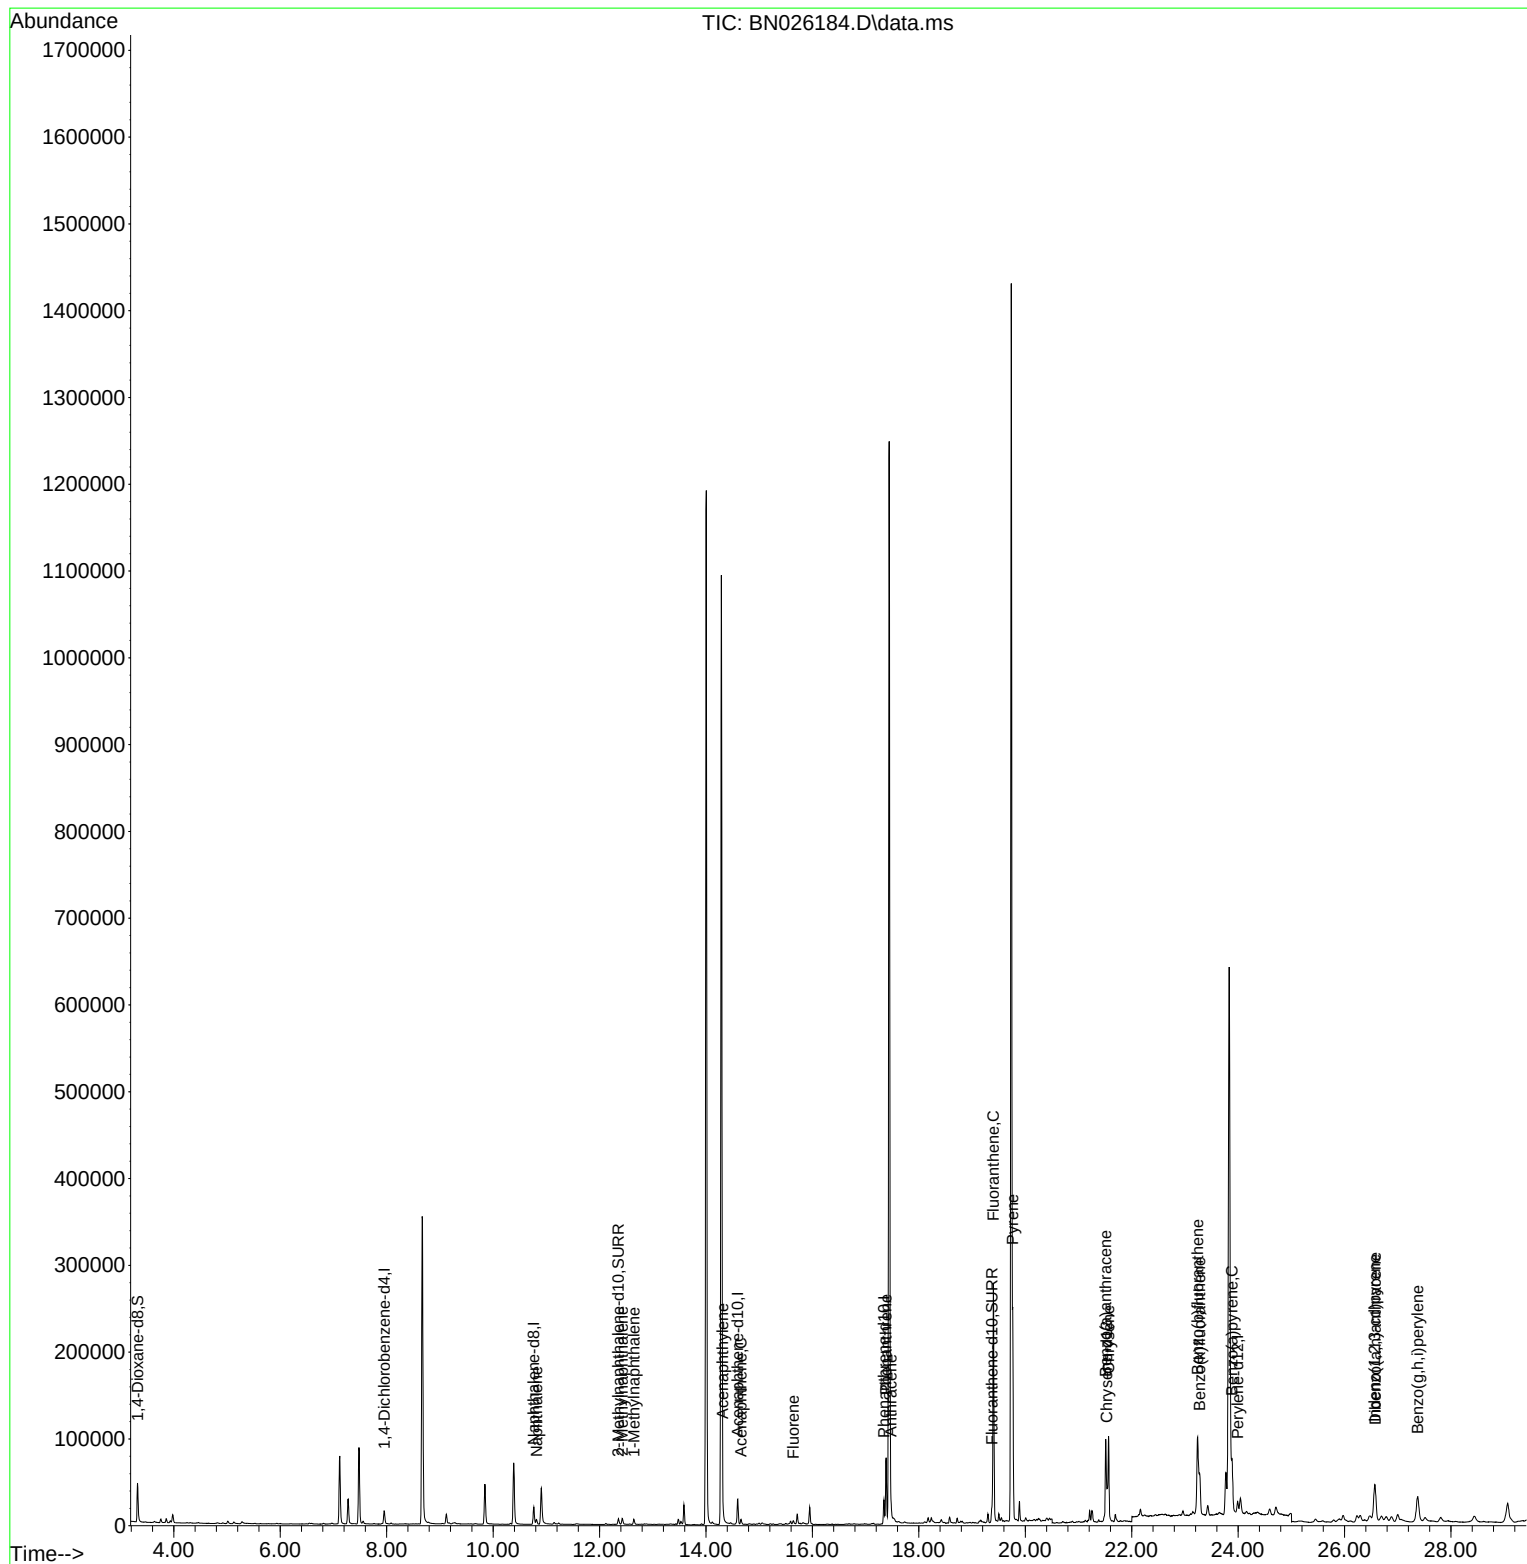

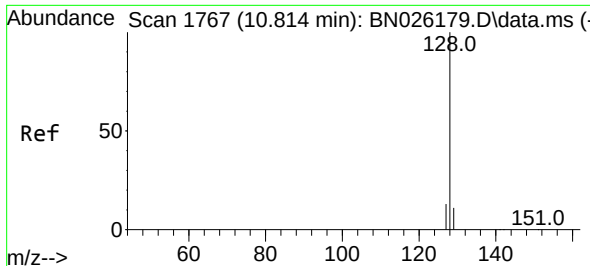

#5
Naphthalene
Concen: 0.094 ng/ul
RT: 10.814 min Scan# 1767
Delta R.T. -0.011 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05




Instrument :
BNA_N
ClientSampleId :
DCGL2

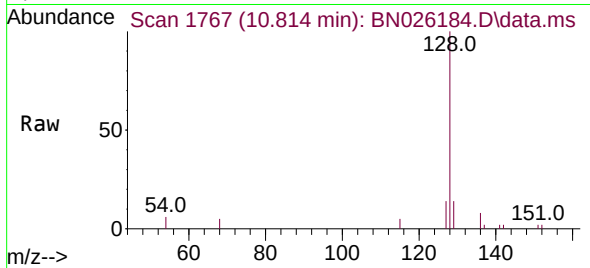


Tgt Ion:128 Resp: 7702
Ion Ratio Lower Upper
128 100
129 13.9 9.1 13.7
127 14.4 10.7 16.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

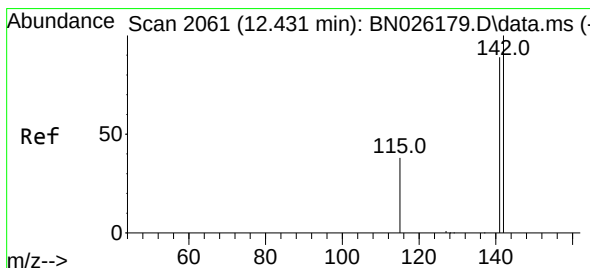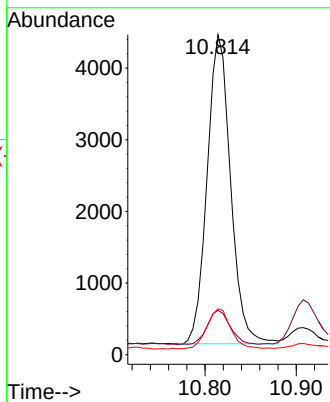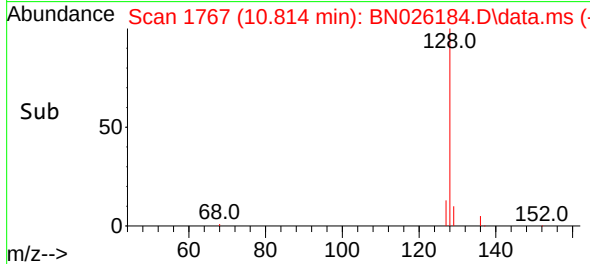


#7
2-Methylnaphthalene
Concen: 0.109 ng/ul
RT: 12.425 min Scan# 2060
Delta R.T. -0.011 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05

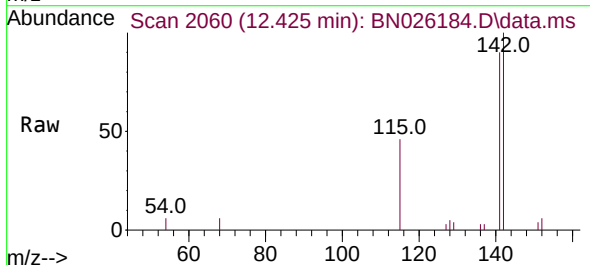

Tgt Ion:142 Resp: 5662
Ion Ratio Lower Upper
142 100
141 88.9 71.9 107.9

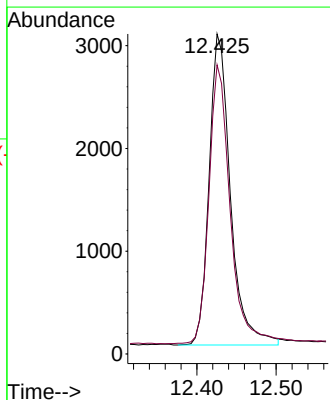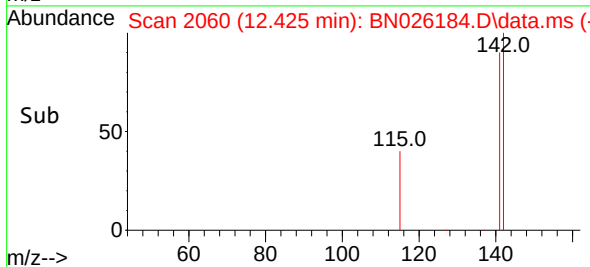



#8

1-Methylnaphthalene

Concen: 0.079 ng/ul

RT: 12.645 min Scan# 2100

Delta R.T. -0.005 min

Lab File: BN026184.D


Acq: 02 Jul 2023 12:05

Instrument :

BNA_N

ClientSampleId :

DCGL2



Tgt Ion:142 Resp: 4260

Ion Ratio Lower Upper

142 100




141 94.3 74.2 111.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/03/2023

Supervised By :Sohil Jodhani 07/04/2023

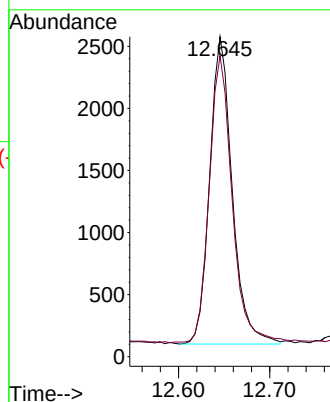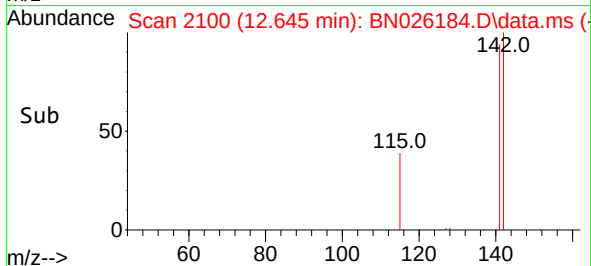

#10

Acenaphthylene

Concen: 0.095 ng/ul

RT: 14.316 min Scan# 2435

Delta R.T. -0.010 min

Lab File: BN026184.D

Acq: 02 Jul 2023 12:05




Tgt Ion:152 Resp: 7414


Ion Ratio Lower Upper

152 100

151 23.3 16.2 24.4


153 18.8 10.9 16.3#

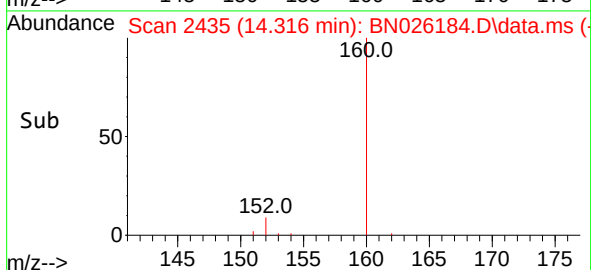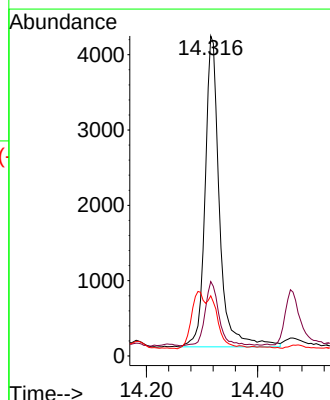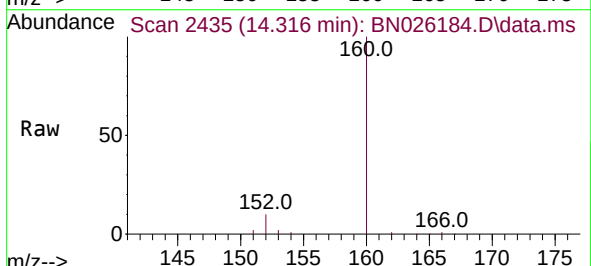

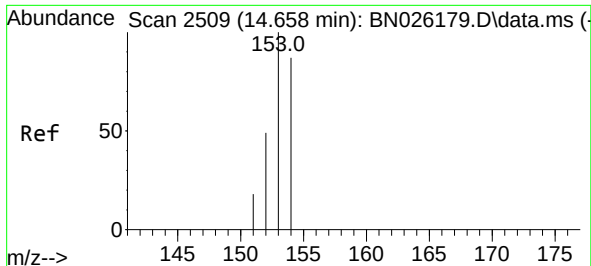

#11
Acenaphthene
Concen: 0.051 ng/ul
RT: 14.658 min Scan# 2509
Delta R.T. -0.010 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05




Instrument :
BNA_N
ClientSampleId :
DCGL2




Tgt Ion:153 Resp: 327
Ion Ratio Lower Upper
153 100
152 53.0 39.4 59.0
154 85.9 68.9 103.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

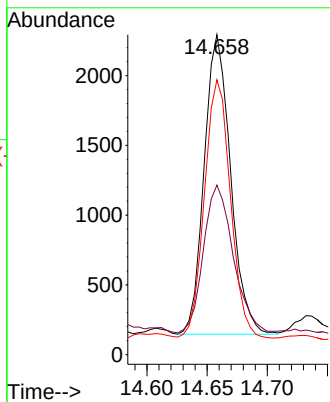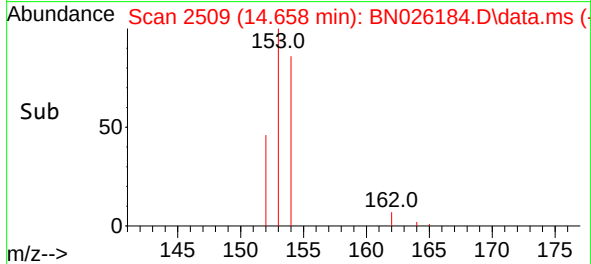


#12
Fluorene
Concen: 0.035 ng/ul
RT: 15.644 min Scan# 2722
Delta R.T. -0.010 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05

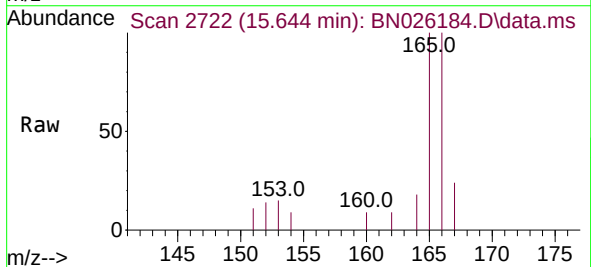


Tgt Ion:166 Resp: 2560
Ion Ratio Lower Upper
166 100
165 100.5 79.9 119.9
167 24.5 10.8 16.2#

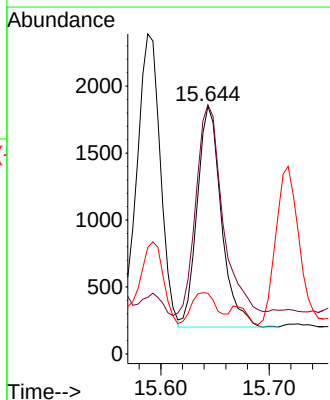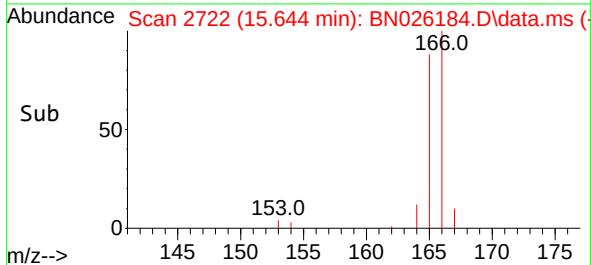

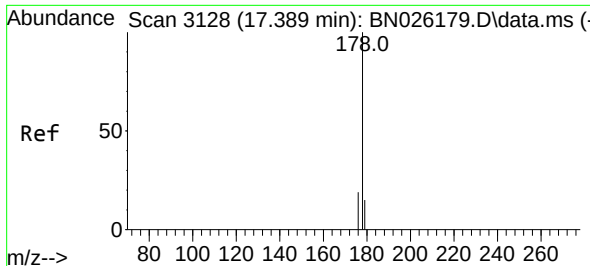

#15
Phenanthrene
Concen: 0.775 ng/ul
RT: 17.385 min Scan# 3127
Delta R.T. -0.009 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05




Instrument :
BNA_N
ClientSampleId :
DCGL2

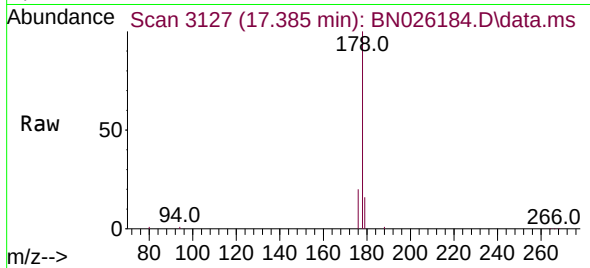

Tgt Ion:178 Resp: 8316
Ion Ratio Lower Upper
178 100
179 15.8 12.6 19.0
176 19.8 15.8 23.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

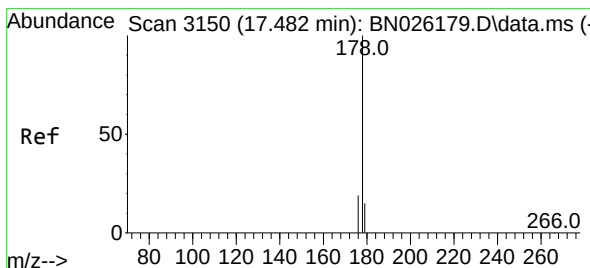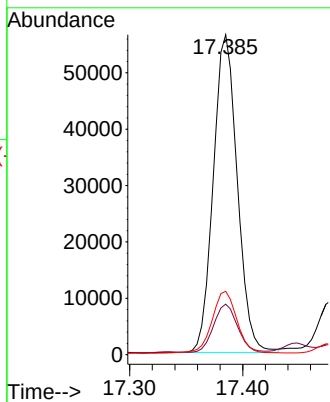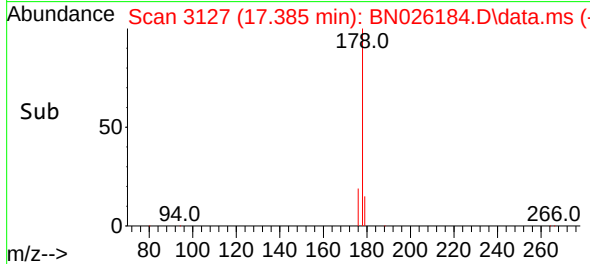

#16
Anthracene
Concen: 0.129 ng/ul
RT: 17.478 min Scan# 3149
Delta R.T. -0.009 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05


Tgt Ion:178 Resp: 12308
Ion Ratio Lower Upper
178 100
179 18.6 12.6 18.8
176 20.7 15.1 22.7

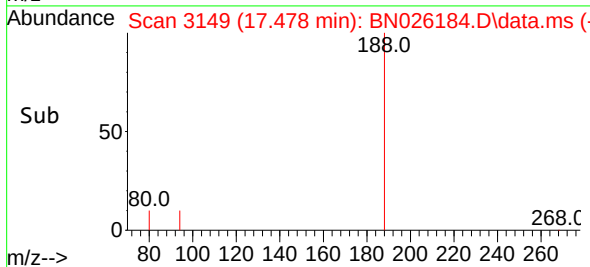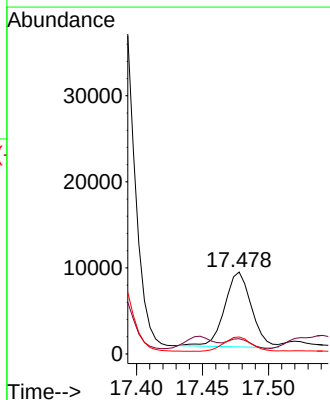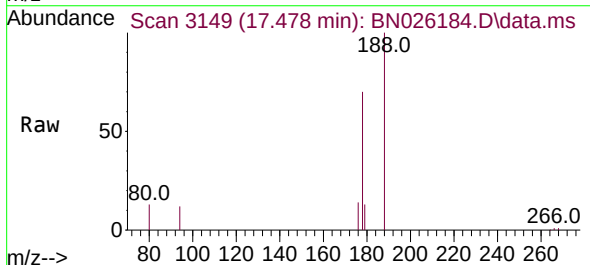

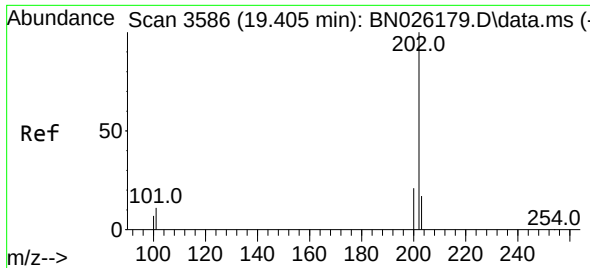

#19
Fluoranthene
Concen: 2.578 ng/ul
RT: 19.401 min Scan# 3585
Delta R.T. -0.010 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05




Instrument :
BNA_N
ClientSampleId :
DCGL2

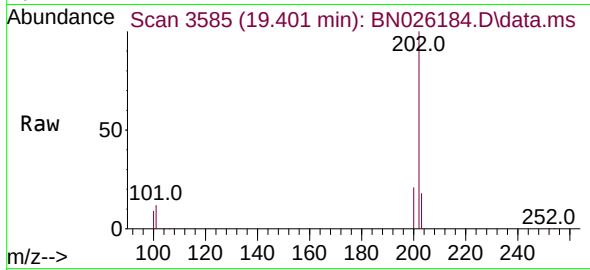


Tgt Ion:202 Resp: 232174
Ion Ratio Lower Upper
202 100
101 11.8 9.5 14.3
100 8.7 7.3 10.9

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

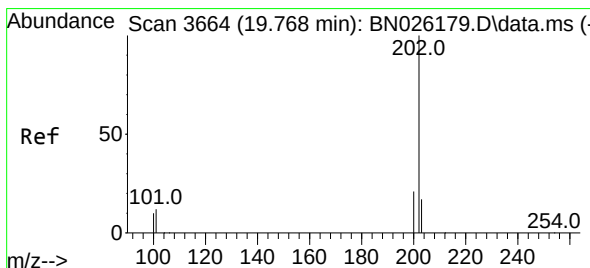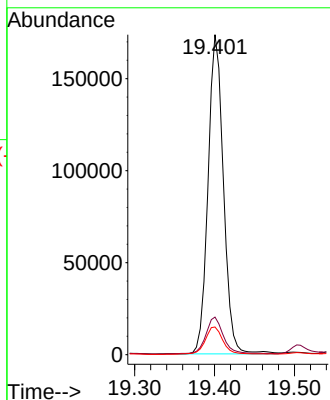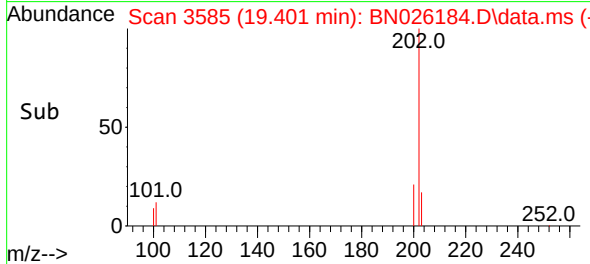


#20
Pyrene
Concen: 2.015 ng/ul
RT: 19.763 min Scan# 3663
Delta R.T. -0.010 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05

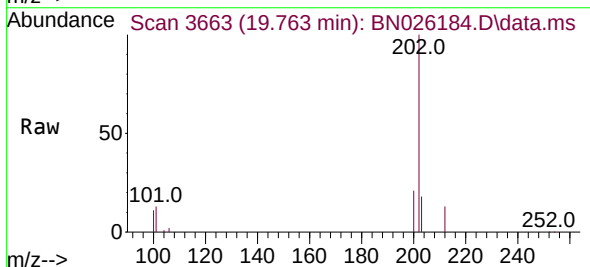

Tgt Ion:202 Resp: 188692
Ion Ratio Lower Upper
202 100
101 13.1 11.4 17.0
100 11.0 9.1 13.7

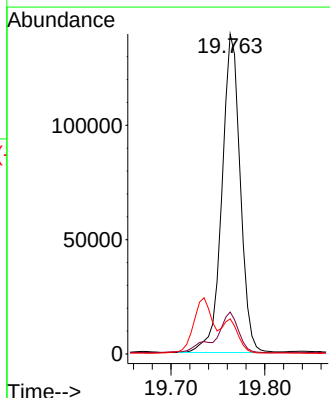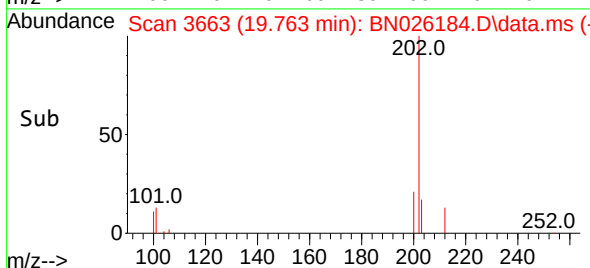



#21

Benzo(a)anthracene

Concen: 1.187 ng/ul

RT: 21.511 min Scan# 4167

Delta R.T. -0.015 min

Lab File: BN026184.D

Acq: 02 Jul 2023 12:05

Instrument :

BNA_N

ClientSampleId :





DCGL2

Tgt Ion:228 Resp: 82583
 Ion Ratio Lower Upper
 228 100
 229 22.1 15.8 23.6
 226 29.2 22.5 33.7

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :Sohil Jodhani 07/04/2023

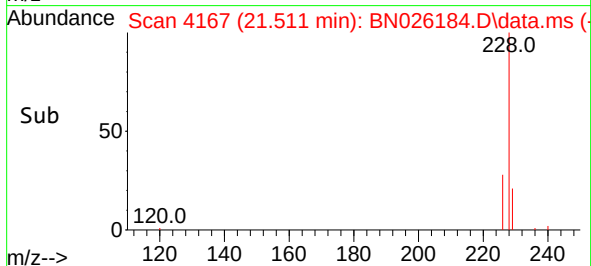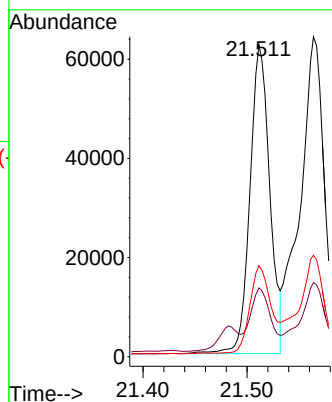

#22

Chrysene

Concen: 1.450 ng/ul




RT: 21.564 min Scan# 4185


Delta R.T. -0.015 min

Lab File: BN026184.D

Acq: 02 Jul 2023 12:05


Tgt Ion:228 Resp: 104916
 Ion Ratio Lower Upper
 228 100
 226 31.7 24.8 37.2
 229 23.2 15.7 23.5

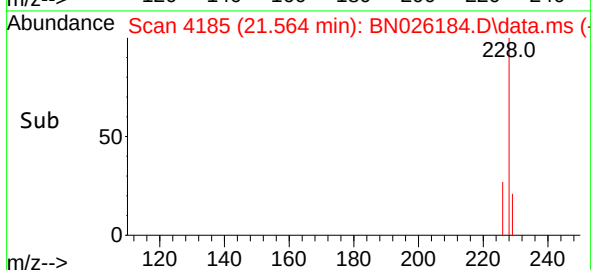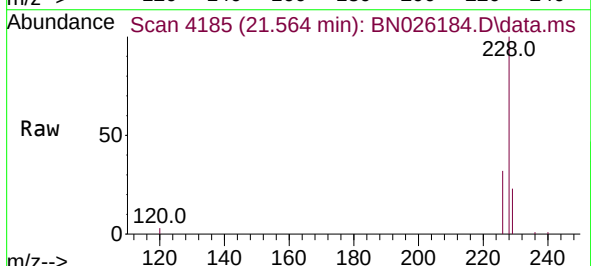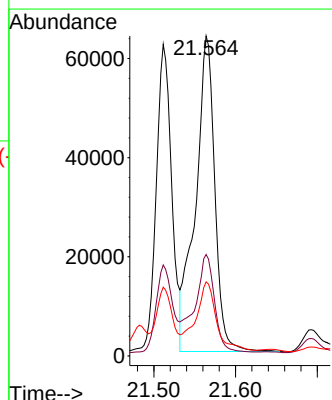

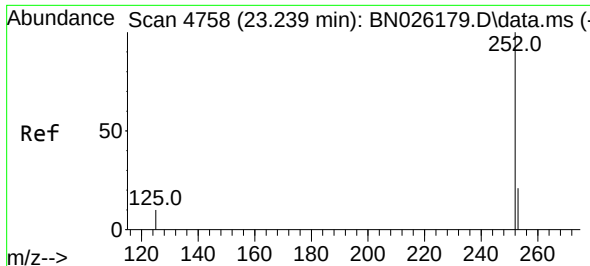

#24
Benzo(b)fluoranthene
Concen: 2.015 ng/ul m
RT: 23.239 min Scan# 4758
Delta R.T. -0.004 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05




Instrument :
BNA_N
ClientSampleId :
DCGL2

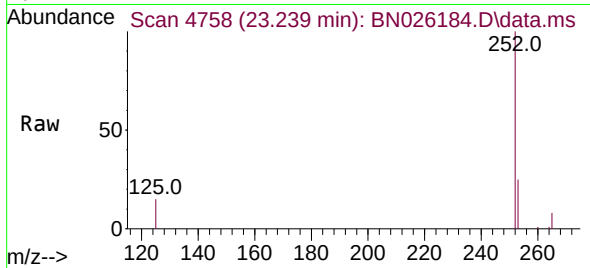


Tgt Ion:252 Resp: 153249
Ion Ratio Lower Upper
252 100
253 24.8 0.0 55.6
125 14.7 0.0 35.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

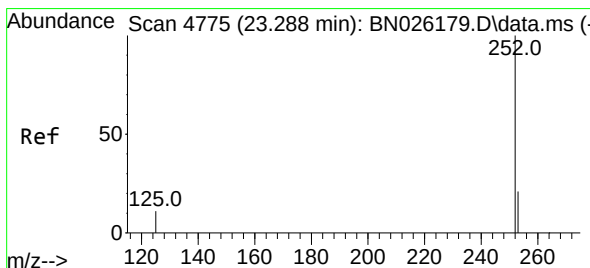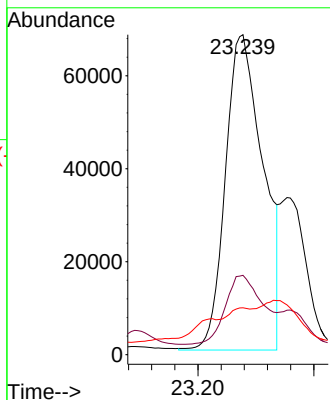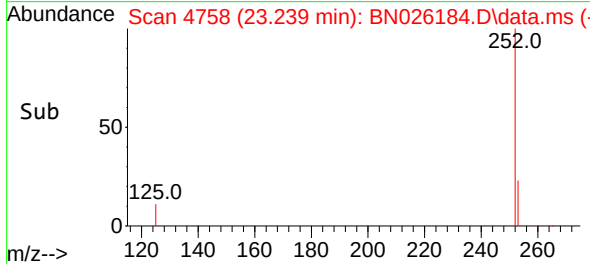


#25
Benzo(k)fluoranthene
Concen: 0.676 ng/ul m
RT: 23.277 min Scan# 4771
Delta R.T. -0.015 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05

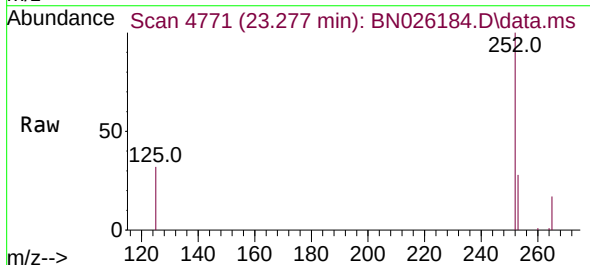


Tgt Ion:252 Resp: 51594
Ion Ratio Lower Upper
252 100
253 28.3 23.2 34.8
125 31.7 15.0 22.4#

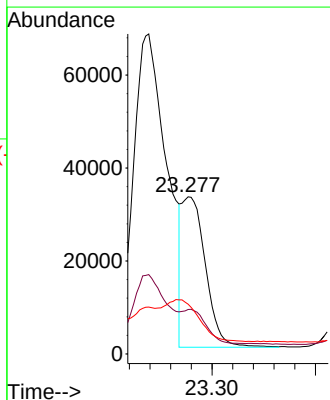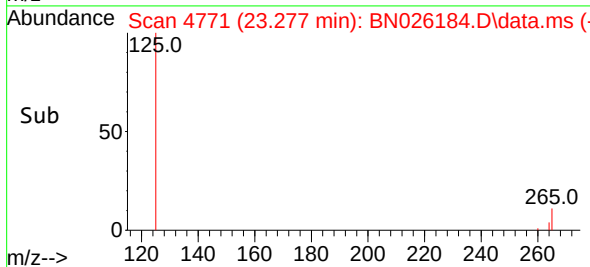

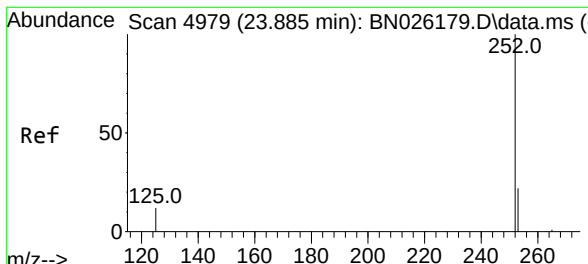

#26
Benzo(a)pyrene
Concen: 1.419 ng/ul
RT: 23.885 min Scan# 4979
Delta R.T. -0.001 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05




Instrument :
BNA_N
ClientSampleId :
DCGL2

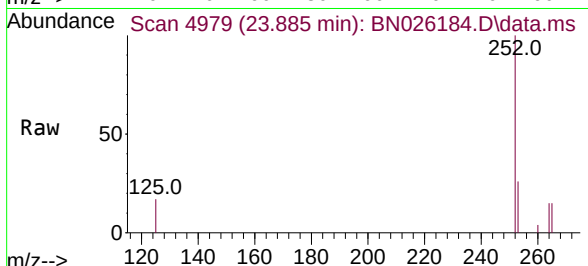


Tgt Ion:252 Resp: 93710
Ion Ratio Lower Upper
252 100
253 26.1 26.0 39.0
125 16.6 17.3 25.9

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

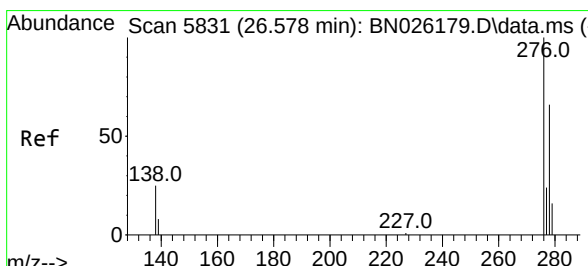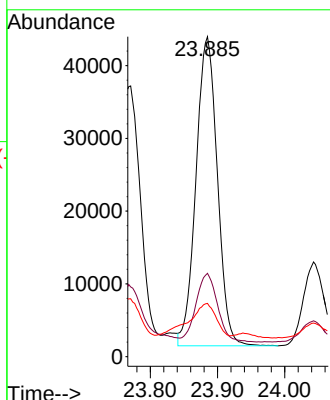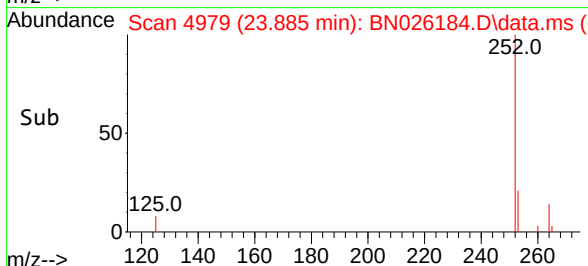


#27
Indeno(1,2,3-cd)pyrene
Concen: 1.082 ng/ul
RT: 26.568 min Scan# 5828
Delta R.T. 0.009 min
Lab File: BN026184.D
Acq: 02 Jul 2023 12:05

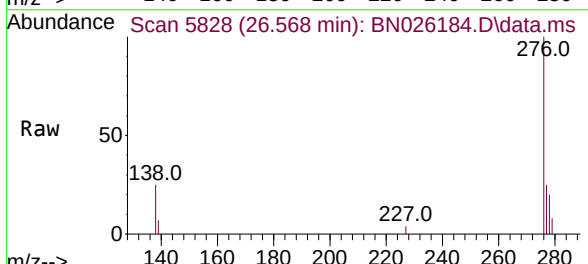

Tgt Ion:276 Resp: 78086
Ion Ratio Lower Upper
276 100
138 21.7 24.5 36.7#
227 0.0 0.0 0.0

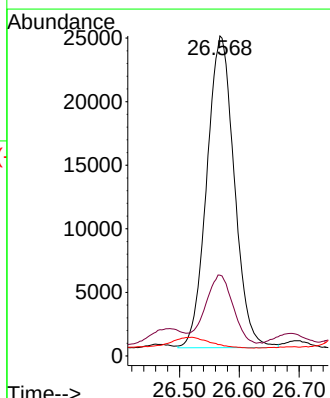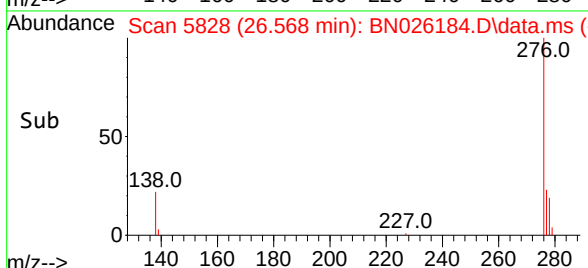

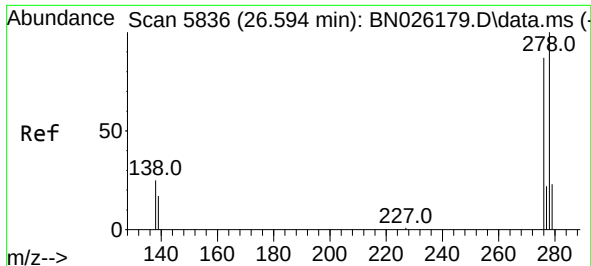

#28

Dibenzo(a,h)anthracene

Concen: 0.326 ng/ul

RT: 26.578 min Scan# 5831

Delta R.T. -0.001 min

Lab File: BN026184.D

Acq: 02 Jul 2023 12:05

Instrument :

BNA_N

ClientSampleId :

DCGL2

Tgt Ion:278 Resp: 1779

Ion Ratio Lower Upper

278 100

139 32.0 19.0 28.4





279 38.5 26.7 40.1

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/03/2023

Supervised By :Sohil Jodhani 07/04/2023

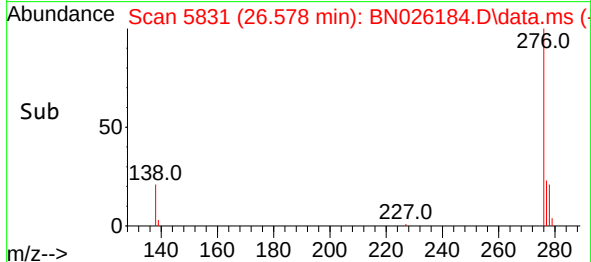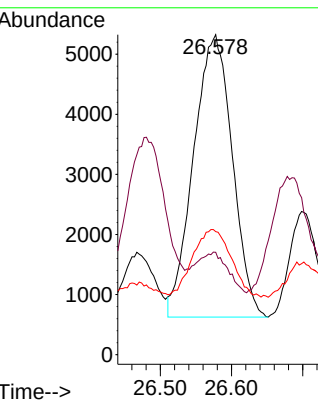

#29

Benzo(g,h,i)perylene

Concen: 1.122 ng/ul

RT: 27.373 min Scan# 6068

Delta R.T. 0.026 min

Lab File: BN026184.D

Acq: 02 Jul 2023 12:05

Tgt Ion:276 Resp: 72018

Ion Ratio Lower Upper

276 100

138 27.3 23.4 35.0

277 25.4 20.0 30.0

