

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
 Data File : BN026191.D
 Acq On : 02 Jul 2023 16:22
 Operator : MA/JU
 Sample : 03247-13
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGL9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :Sohil Jodhani 07/04/2023

Quant Time: Jul 03 05:40:45 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 01:46:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	9030	0.400	ng/ul	0.00
4) Naphthalene-d8	10.765	136	27938	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.598	164	15990	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.347	188	30697	0.400	ng/ul	0.00
17) Chrysene-d12	21.535	240	15549	0.400	ng/ul	# 0.00
23) Perylene-d12	24.005	264	17808	0.400	ng/ul	# 0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.318	96	19401	1.908	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.360	152	6353	0.148	ng/ul	0.00
18) Fluoranthene-d10	19.377	212	11095	0.187	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.814	128	8579	0.107	ng/ul#	95
7) 2-Methylnaphthalene	12.431	142	5093	0.100	ng/ul	99
8) 1-Methylnaphthalene	12.651	142	4114	0.078	ng/ul	99
10) Acenaphthylene	14.320	152	13824	0.185	ng/ul	96
11) Acenaphthene	14.663	153	11015	0.180	ng/ul	98
12) Fluorene	15.648	166	8929	0.127	ng/ul#	97
14) Pentachlorophenol	17.005	266	568	0.052	ng/ul	97
15) Phenanthrene	17.389	178	271606	2.679	ng/ul	100
16) Anthracene	17.478	178	34831	0.386	ng/ul	97
19) Fluoranthene	19.405	202	905668	10.905	ng/ul	97
20) Pyrene	19.768	202	700779	8.113	ng/ul	97
21) Benzo(a)anthracene	21.520	228	348061	5.426	ng/ul	98
22) Chrysene	21.573	228	402342	6.028	ng/ul	98
24) Benzo(b)fluoranthene	23.251	252	629211m	8.278	ng/ul	
25) Benzo(k)fluoranthene	23.294	252	219489m	2.876	ng/ul	
26) Benzo(a)pyrene	23.900	252	380463	5.763	ng/ul#	84
27) Indeno(1,2,3-cd)pyrene	26.591	276	320339	4.443	ng/ul#	83
28) Dibenzo(a,h)anthracene	26.601	278	77302	1.417	ng/ul	99
29) Benzo(g,h,i)perylene	27.393	276	295937	4.614	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
Data File : BN026191.D
Acq On : 02 Jul 2023 16:22
Operator : MA/JU
Sample : 03247-13
Misc :
ALS Vial : 48 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCGL9

Quant Time: Jul 03 05:40:45 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 01:46:24 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

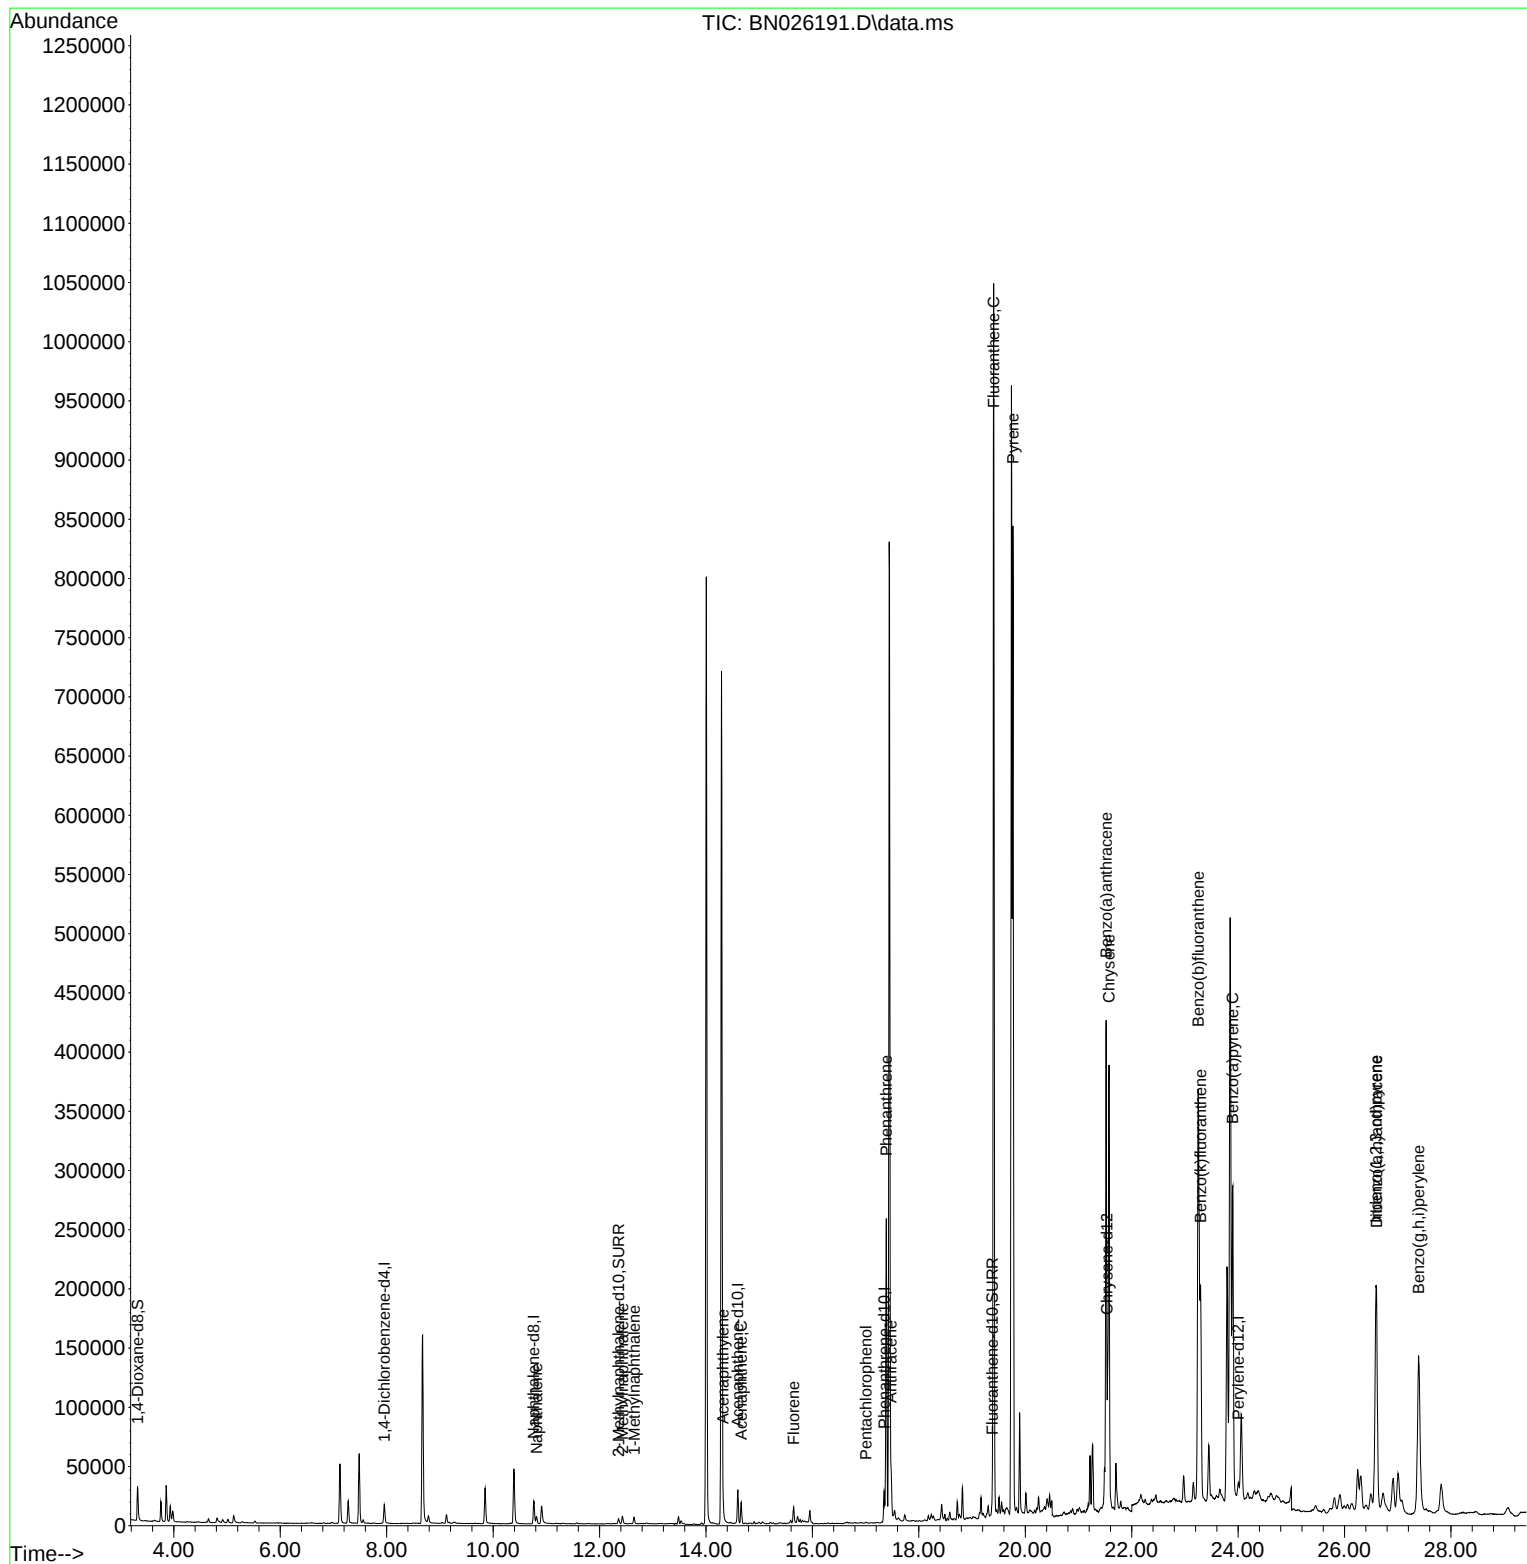

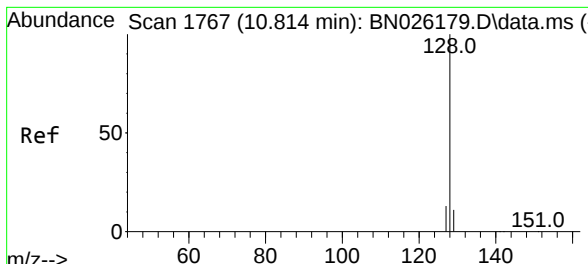

#5
Naphthalene
Concen: 0.107 ng/ul
RT: 10.814 min Scan# 1767
Delta R.T. -0.011 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22




Instrument :
BNA_N
ClientSampleId :
DCGL9

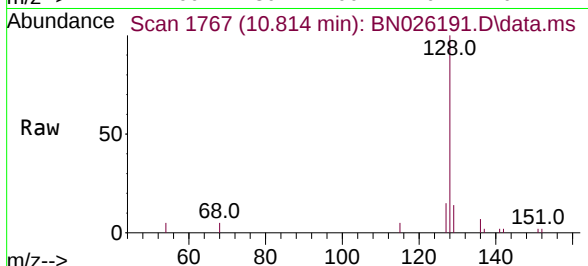

Tgt Ion:128 Resp: 8579
Ion Ratio Lower Upper
128 100
129 13.9 9.1 13.7
127 14.7 10.7 16.1




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

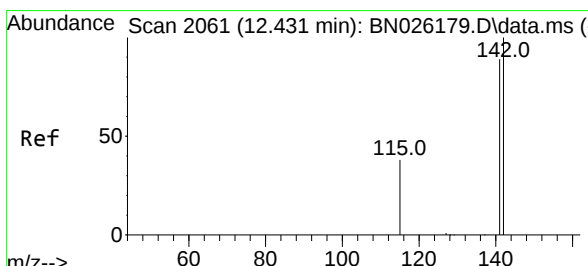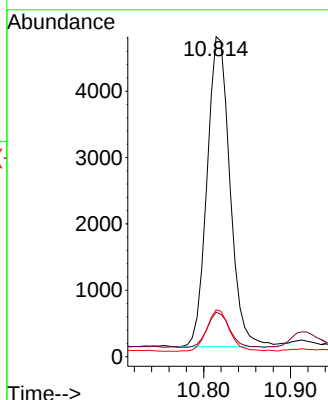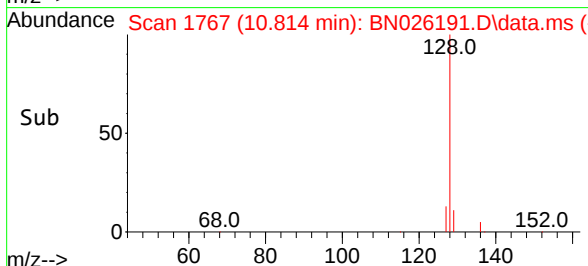

#7
2-Methylnaphthalene
Concen: 0.100 ng/ul
RT: 12.431 min Scan# 2061
Delta R.T. -0.005 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22


Tgt Ion:142 Resp: 5093
Ion Ratio Lower Upper
142 100
141 90.6 71.9 107.9

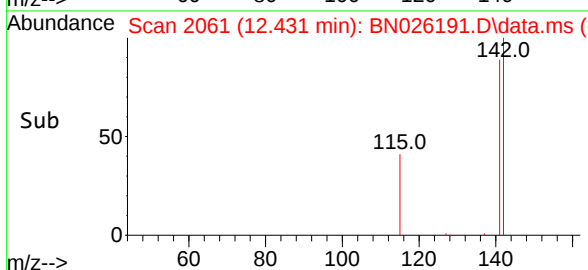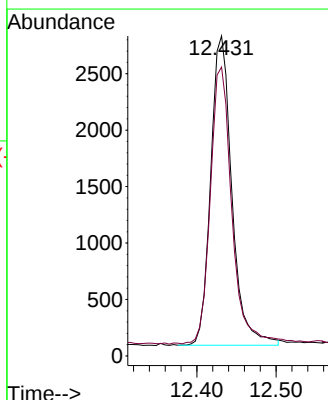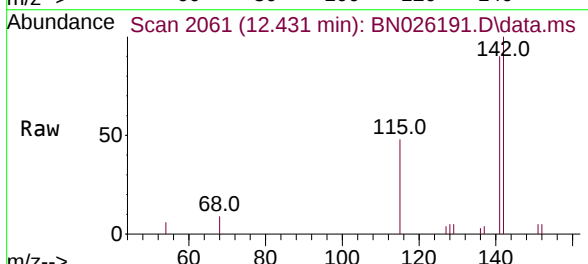

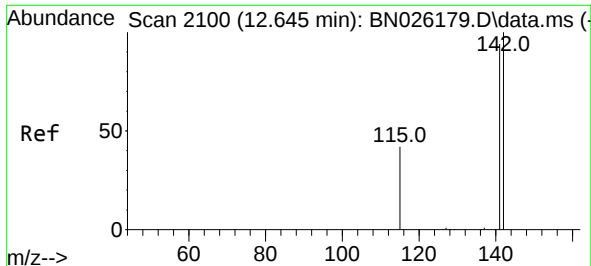

#8
1-Methylnaphthalene
Concen: 0.078 ng/ul
RT: 12.651 min Scan# 2101
Delta R.T. 0.000 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22




Instrument :
BNA_N
ClientSampleId :
DCGL9

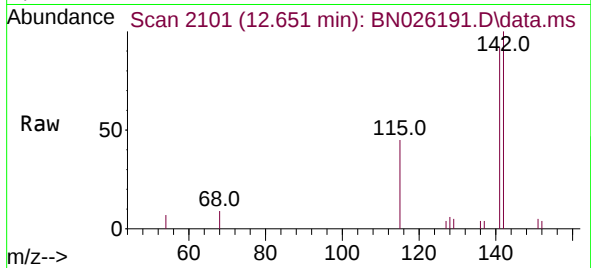

Tgt Ion:142 Resp: 4114
Ion Ratio Lower Upper
142 100
141 93.4 74.2 111.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

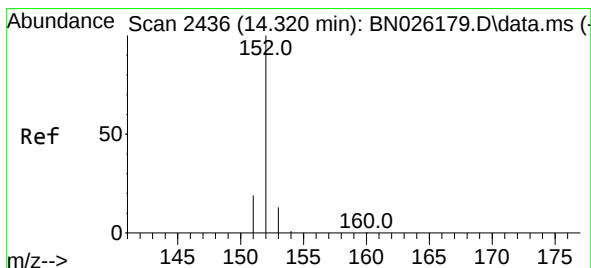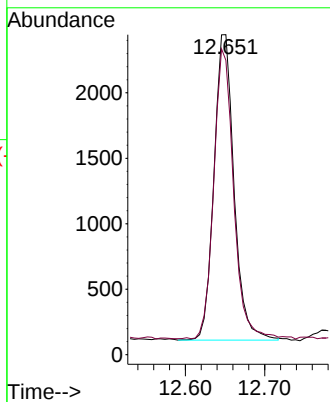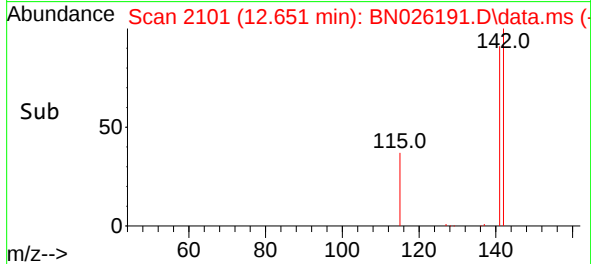

#10
Acenaphthylene
Concen: 0.185 ng/ul
RT: 14.320 min Scan# 2436
Delta R.T. -0.005 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22


Tgt Ion:152 Resp: 13824
Ion Ratio Lower Upper
152 100
151 21.7 16.2 24.4
153 15.8 10.9 16.3

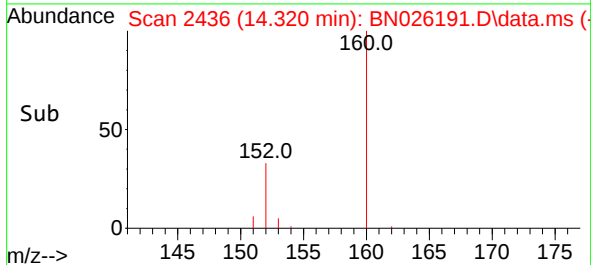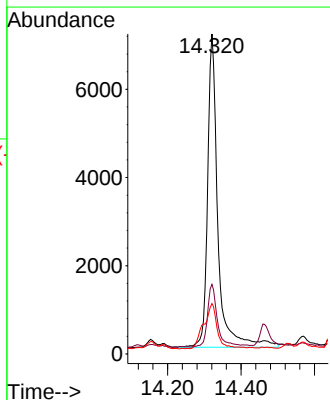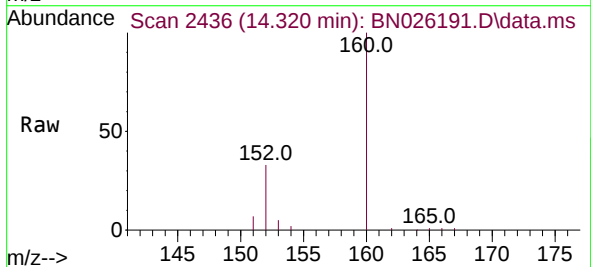

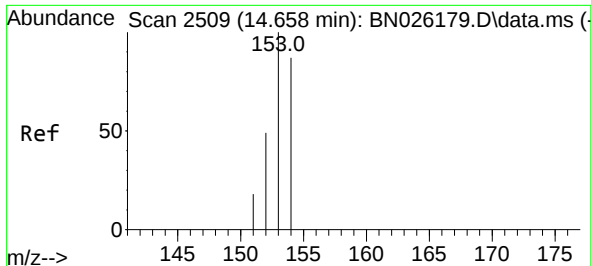

#11
Acenaphthene
Concen: 0.180 ng/ul
RT: 14.663 min Scan# 2510
Delta R.T. -0.005 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22




Instrument :
BNA_N
ClientSampleId :
DCGL9

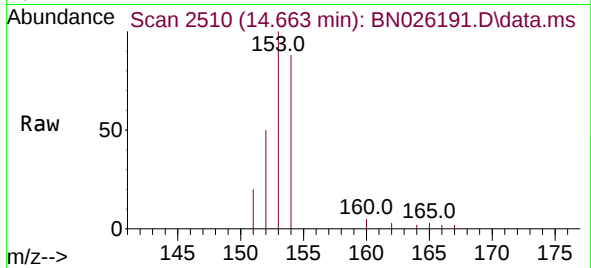

Tgt Ion:153 Resp: 11015
Ion Ratio Lower Upper
153 100
152 50.1 39.4 59.0
154 87.9 68.9 103.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

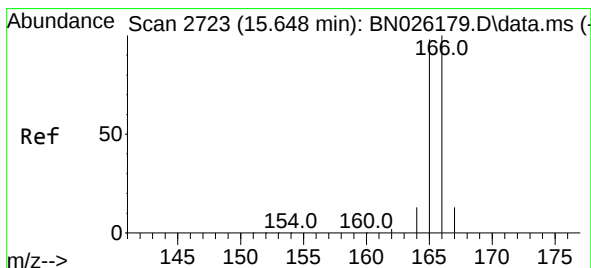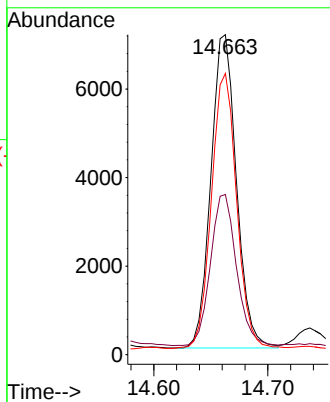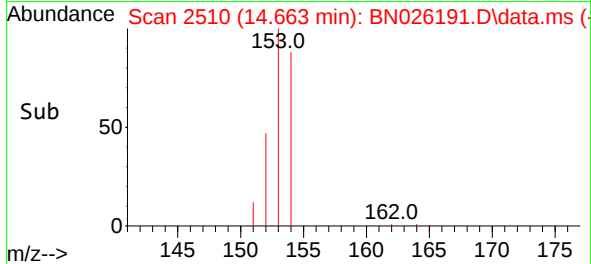

#12
Fluorene
Concen: 0.127 ng/ul
RT: 15.648 min Scan# 2723
Delta R.T. -0.005 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22

Tgt Ion:166 Resp: 8929
Ion Ratio Lower Upper
166 100
165 98.2 79.9 119.9
167 17.7 10.8 16.2#

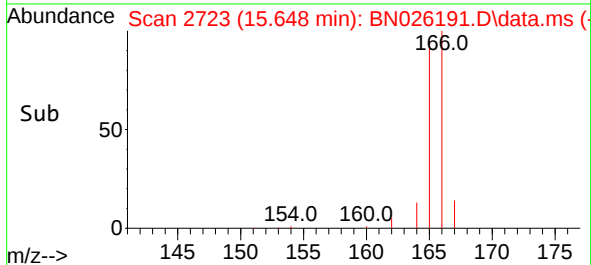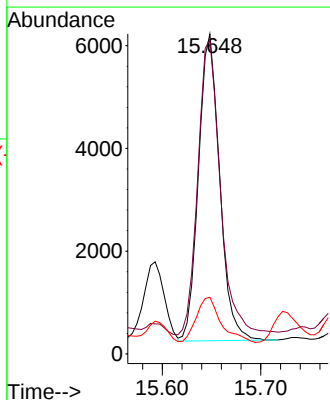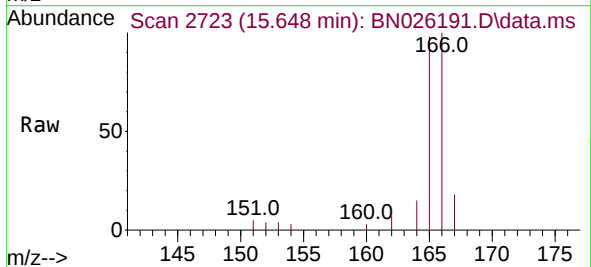

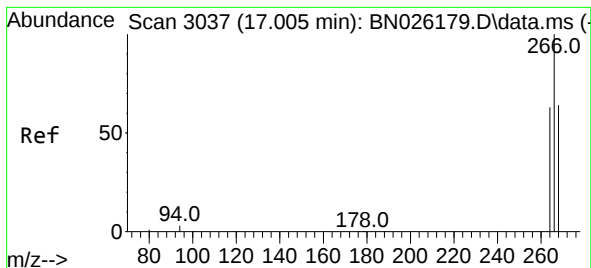

#14

Pentachlorophenol

Concen: 0.052 ng/uI

RT: 17.005 min Scan# 3037

Delta R.T. -0.005 min

Lab File: BN026191.D

Acq: 02 Jul 2023 16:22

Instrument :

BNA_N

ClientSampleId :





DCGL9

Tgt Ion:266	Resp:	568
Ion Ratio	Lower	Upper
266	100	
264	60.0	50.5 75.7
268	63.4	51.6 77.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

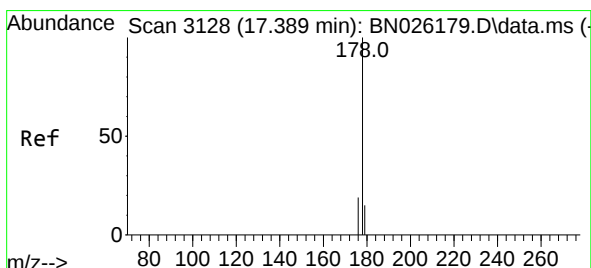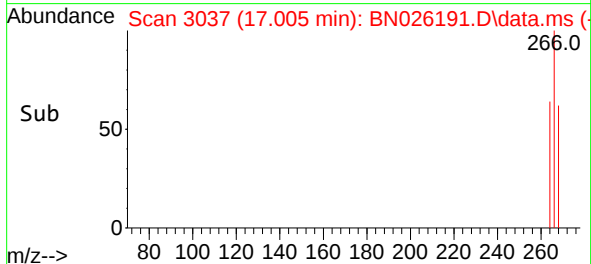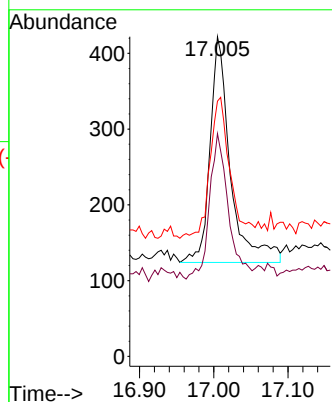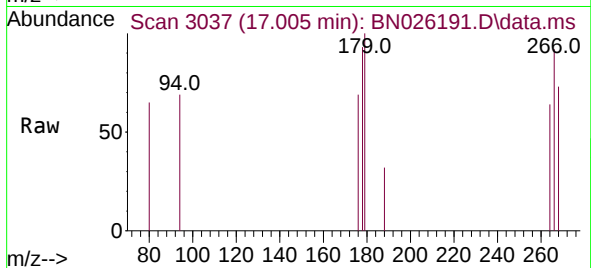

#15

Phenanthrene

Concen: 2.679 ng/uI




RT: 17.389 min Scan# 3128


Delta R.T. -0.005 min

Lab File: BN026191.D

Acq: 02 Jul 2023 16:22


Tgt Ion:178	Resp:	271606
Ion Ratio	Lower	Upper
178	100	
179	15.5	12.6 19.0
176	19.6	15.8 23.6

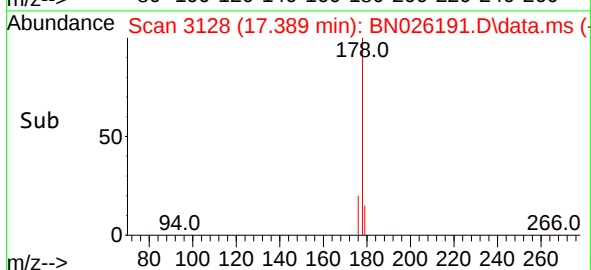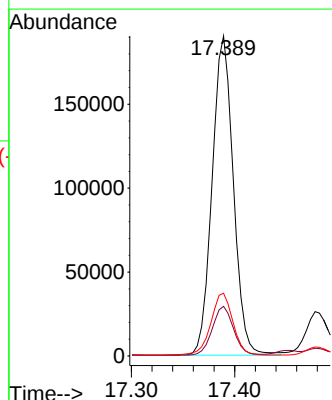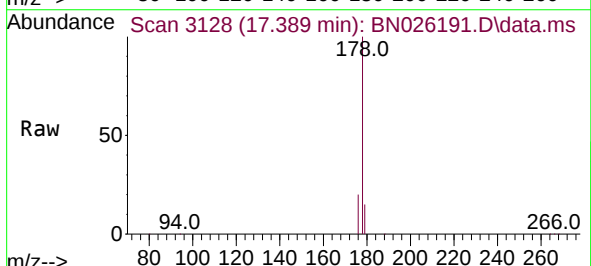

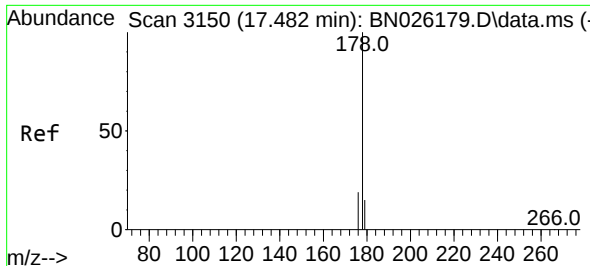

#16
 Anthracene
 Concen: 0.386 ng/ul
 RT: 17.478 min Scan# 3150
 Delta R.T. -0.009 min
 Lab File: BN026191.D
 Acq: 02 Jul 2023 16:22




Instrument :
 BNA_N
 ClientSampleId :
 DCGL9

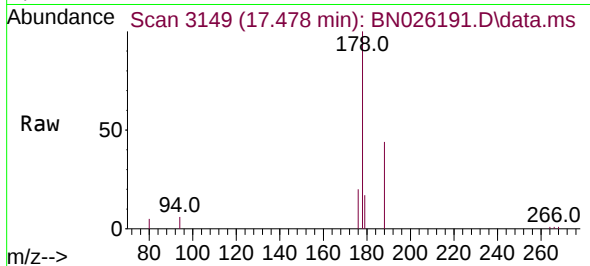

Tgt Ion:178 Resp: 3483
 Ion Ratio Lower Upper
 178 100
 179 17.2 12.6 18.8
 176 20.1 15.1 22.7




Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :Sohil Jodhani 07/04/2023

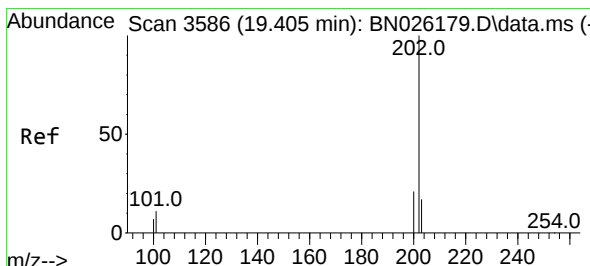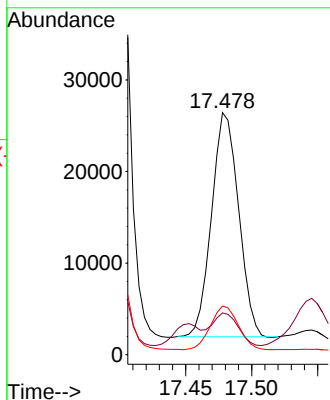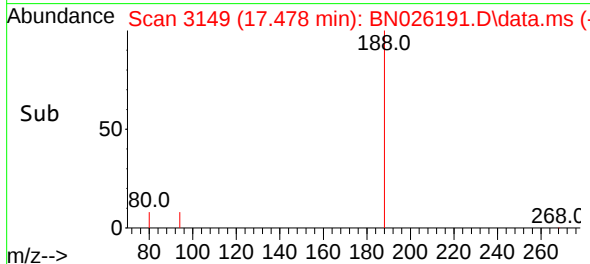

#19
 Fluoranthene
 Concen: 10.905 ng/ul
 RT: 19.405 min Scan# 3586
 Delta R.T. -0.005 min
 Lab File: BN026191.D
 Acq: 02 Jul 2023 16:22


Tgt Ion:202 Resp: 905668
 Ion Ratio Lower Upper
 202 100
 101 10.7 9.5 14.3
 100 8.2 7.3 10.9

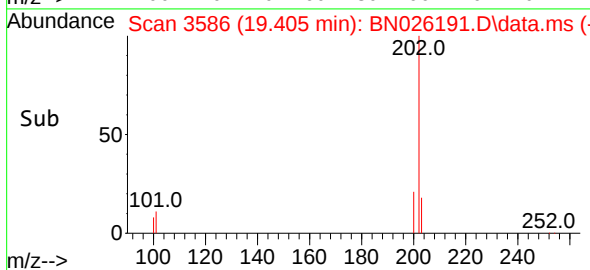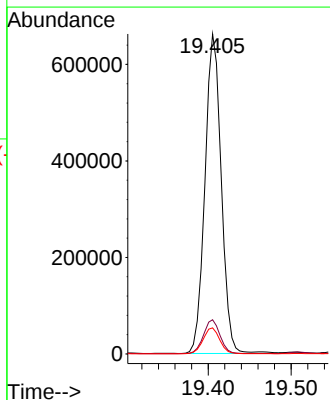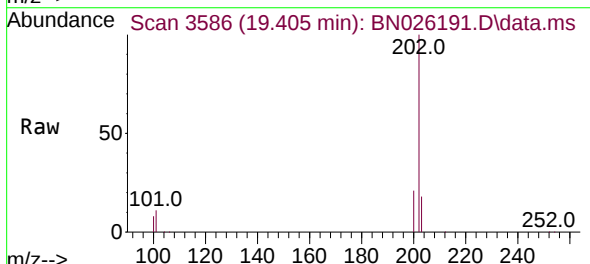



#20
Pyrene
Concen: 8.113 ng/ul
RT: 19.768 min Scan# 30
Delta R.T. -0.005 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22




Instrument :
BNA_N
ClientSampleId :
DCGL9




Tgt Ion:202 Resp: 700779
Ion Ratio Lower Upper
202 100
101 12.6 11.4 17.0
100 10.3 9.1 13.7

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

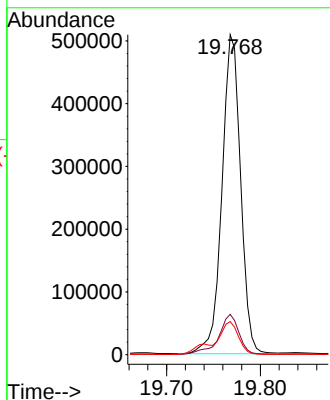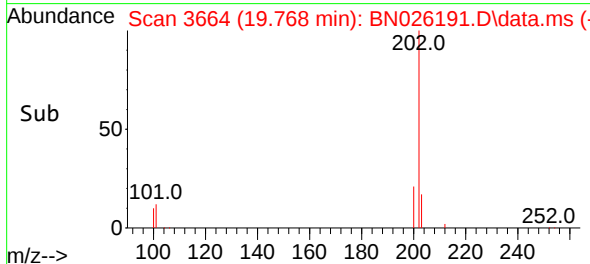


#21
Benzo(a)anthracene
Concen: 5.426 ng/ul
RT: 21.520 min Scan# 4170
Delta R.T. -0.006 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22

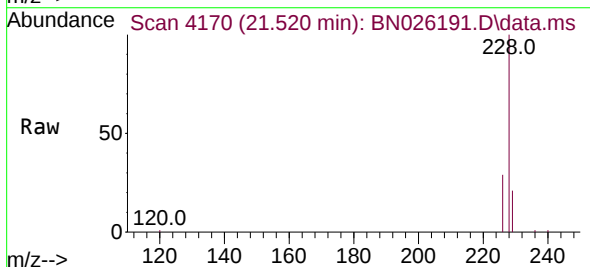


Tgt Ion:228 Resp: 348061
Ion Ratio Lower Upper
228 100
229 21.2 15.8 23.6
226 28.8 22.5 33.7

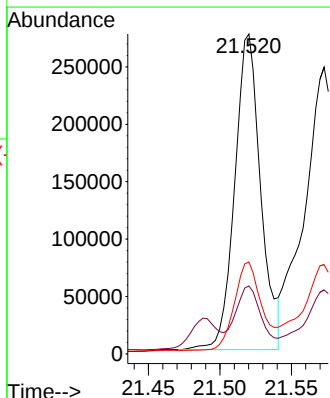

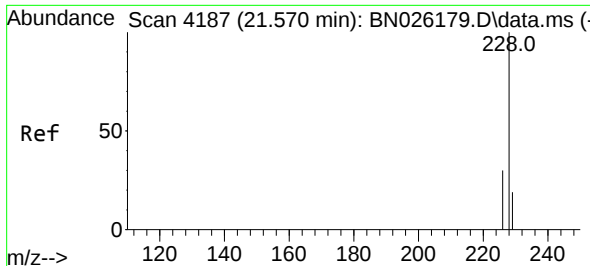

#22
Chrysene
Concen: 6.028 ng/ul
RT: 21.573 min Scan# 4187
Delta R.T. -0.006 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22




Instrument :
BNA_N
ClientSampleId :
DCGL9




Tgt Ion:228 Resp: 40234
Ion Ratio Lower Upper
228 100
226 31.1 24.8 37.2
229 22.3 15.7 23.5

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

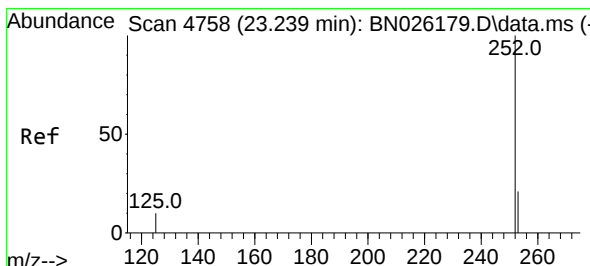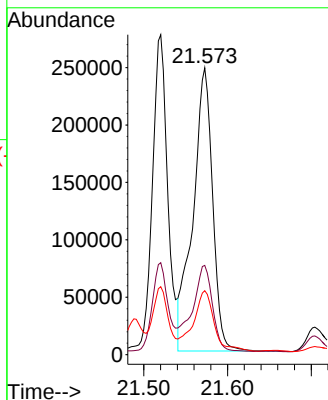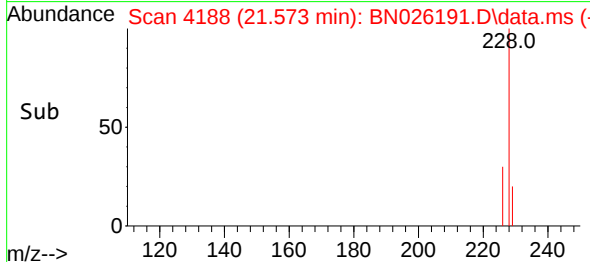


#24
Benzo(b)fluoranthene
Concen: 8.278 ng/ul m
RT: 23.251 min Scan# 4762
Delta R.T. 0.008 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22

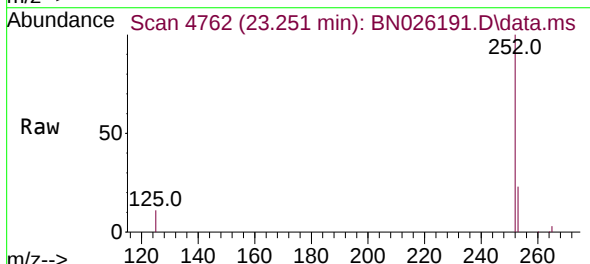


Tgt Ion:252 Resp: 629211
Ion Ratio Lower Upper
252 100
253 23.5 0.0 55.6
125 11.5 0.0 35.8

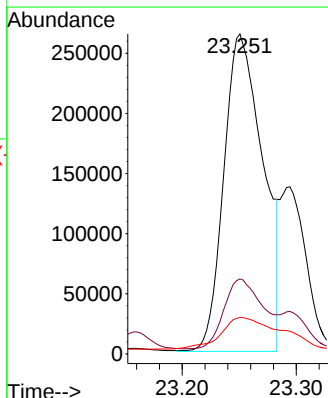

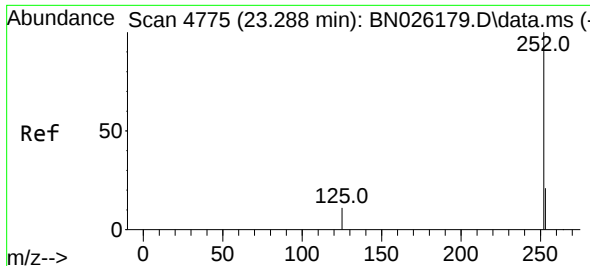

#25
Benzo(k)fluoranthene
Concen: 2.876 ng/ul m
RT: 23.294 min Scan# 4775
Delta R.T. 0.002 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22




Instrument :
BNA_N
ClientSampleId :
DCGL9



Tgt Ion:252 Resp: 219489
Ion Ratio Lower Upper
252 100
253 25.4 23.2 34.8
125 13.6 15.0 22.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

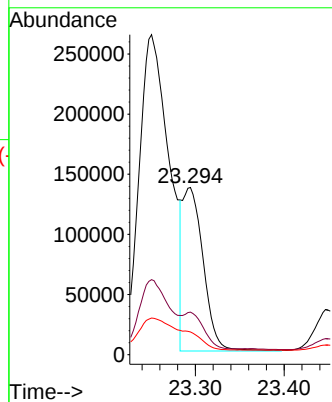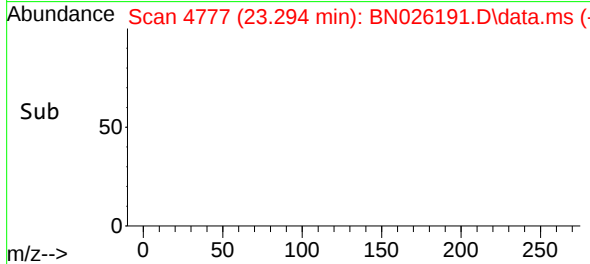

#26
Benzo(a)pyrene
Concen: 5.763 ng/ul
RT: 23.900 min Scan# 4984
Delta R.T. 0.014 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22


Tgt Ion:252 Resp: 380463
Ion Ratio Lower Upper
252 100
253 24.6 26.0 39.0#
125 12.6 17.3 25.9#

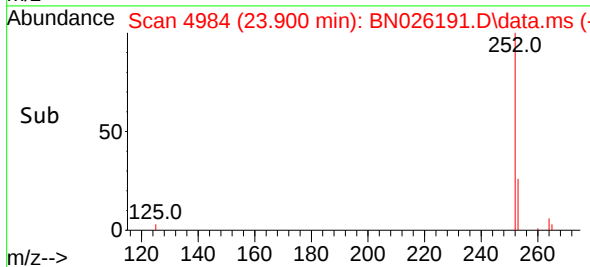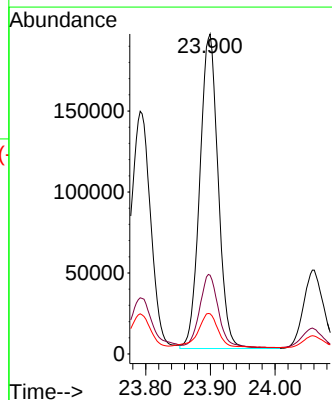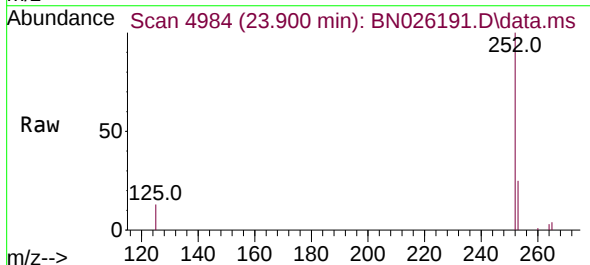

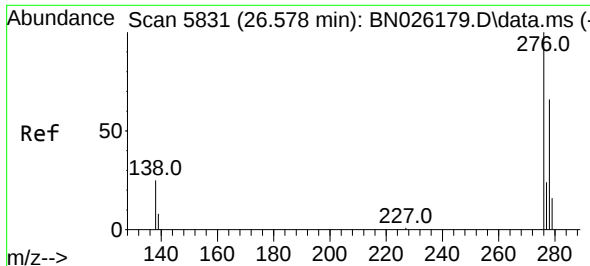

#27
Indeno(1,2,3-cd)pyrene
Concen: 4.443 ng/ul
RT: 26.591 min Scan# 5835
Delta R.T. 0.033 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22




Instrument :
BNA_N
ClientSampleId :
DCGL9




Tgt Ion:276 Resp: 320339
Ion Ratio Lower Upper
276 100
138 21.4 24.5 36.7
227 0.0 0.0 0.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

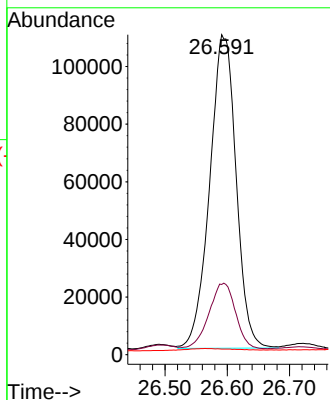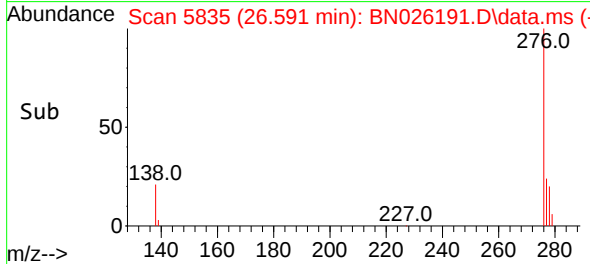


#28
Dibenzo(a,h)anthracene
Concen: 1.417 ng/ul
RT: 26.601 min Scan# 5838
Delta R.T. 0.023 min
Lab File: BN026191.D
Acq: 02 Jul 2023 16:22

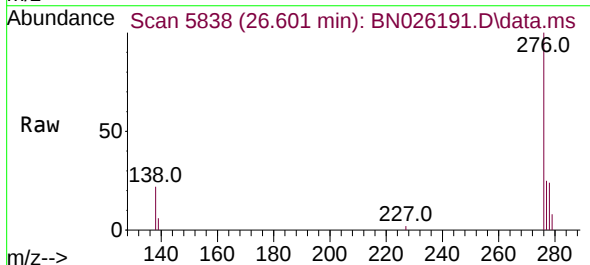


Tgt Ion:278 Resp: 77302
Ion Ratio Lower Upper
278 100
139 23.6 19.0 28.4
279 34.0 26.7 40.1

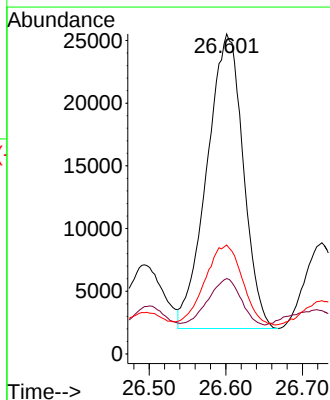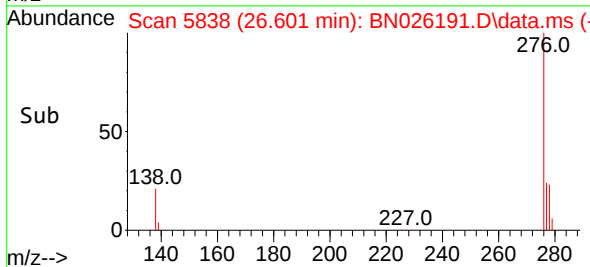

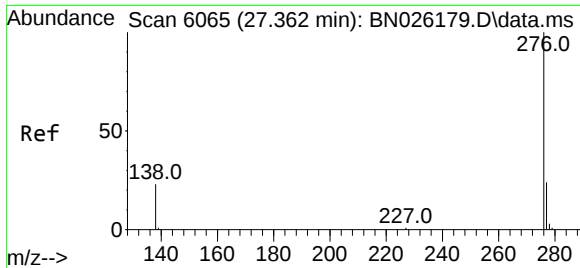

#29
 Benzo(g,h,i)perylene
 Concen: 4.614 ng/ul
 RT: 27.393 min Scan# 6065
 Delta R.T. 0.046 min
 Lab File: BN026191.D
 Acq: 02 Jul 2023 16:22

Instrument :
 BNA_N
 ClientSampleId :
 DCGL9

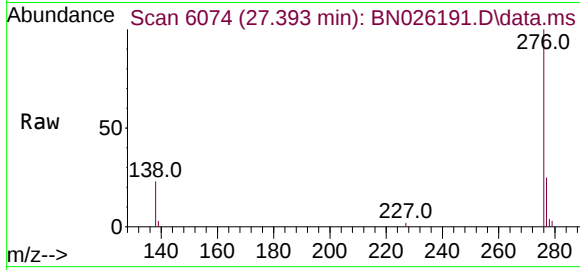

Tgt Ion: 276 Resp: 29593

Ion	Ratio	Lower	Upper
276	100		
138	23.2	23.4	35.0
277	25.4	20.0	30.0

Manual Integrations
 APPROVED

Reviewed By : Yogesh Patel 07/03/2023
 Supervised By : Sohil Jodhani 07/04/2023

