

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
 Data File : BN026209.D
 Acq On : 03 Jul 2023 03:58
 Operator : MA/JU
 Sample : 03244-15
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGF4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :Sohil Jodhani 07/04/2023

Quant Time: Jul 03 06:29:32 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 01:46:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	7182	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.765	136	22561	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.598	164	13159	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.347	188	25883	0.400	ng/ul	0.00
17) Chrysene-d12	21.538	240	13638	0.400	ng/ul	# 0.00
23) Perylene-d12	24.008	264	15145	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.318	96	51170	6.327	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	14367	0.414	ng/ul	-0.01
18) Fluoranthene-d10	19.373	212	24505	0.472	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.814	128	3627	0.056	ng/ul#	89
7) 2-Methylnaphthalene	12.425	142	2866	0.070	ng/ul	98
8) 1-Methylnaphthalene	12.645	142	2148	0.050	ng/ul	99
10) Acenaphthylene	14.316	152	3666	0.059	ng/ul#	83
11) Acenaphthene	14.658	153	1114	0.022	ng/ul	95
15) Phenanthrene	17.385	178	22912	0.268	ng/ul	98
16) Anthracene	17.478	178	3566	0.047	ng/ul#	82
19) Fluoranthene	19.405	202	52392	0.719	ng/ul#	93
20) Pyrene	19.768	202	42601m	0.562	ng/ul	
21) Benzo(a)anthracene	21.520	228	21267	0.378	ng/ul#	89
22) Chrysene	21.573	228	28391	0.485	ng/ul#	89
24) Benzo(b)fluoranthene	23.250	252	48056m	0.743	ng/ul	
25) Benzo(k)fluoranthene	23.294	252	14014m	0.216	ng/ul	
26) Benzo(a)pyrene	23.902	252	29450	0.525	ng/ul#	94
27) Indeno(1,2,3-cd)pyrene	26.598	276	27636	0.451	ng/ul#	86
28) Dibenzo(a,h)anthracene	26.601	278	6518	0.140	ng/ul#	43
29) Benzo(g,h,i)perylene	27.396	276	28190	0.517	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
Data File : BN026209.D
Acq On : 03 Jul 2023 03:58
Operator : MA/JU
Sample : 03244-15
Misc :
ALS Vial : 66 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCGF4

Quant Time: Jul 03 06:29:32 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 01:46:24 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

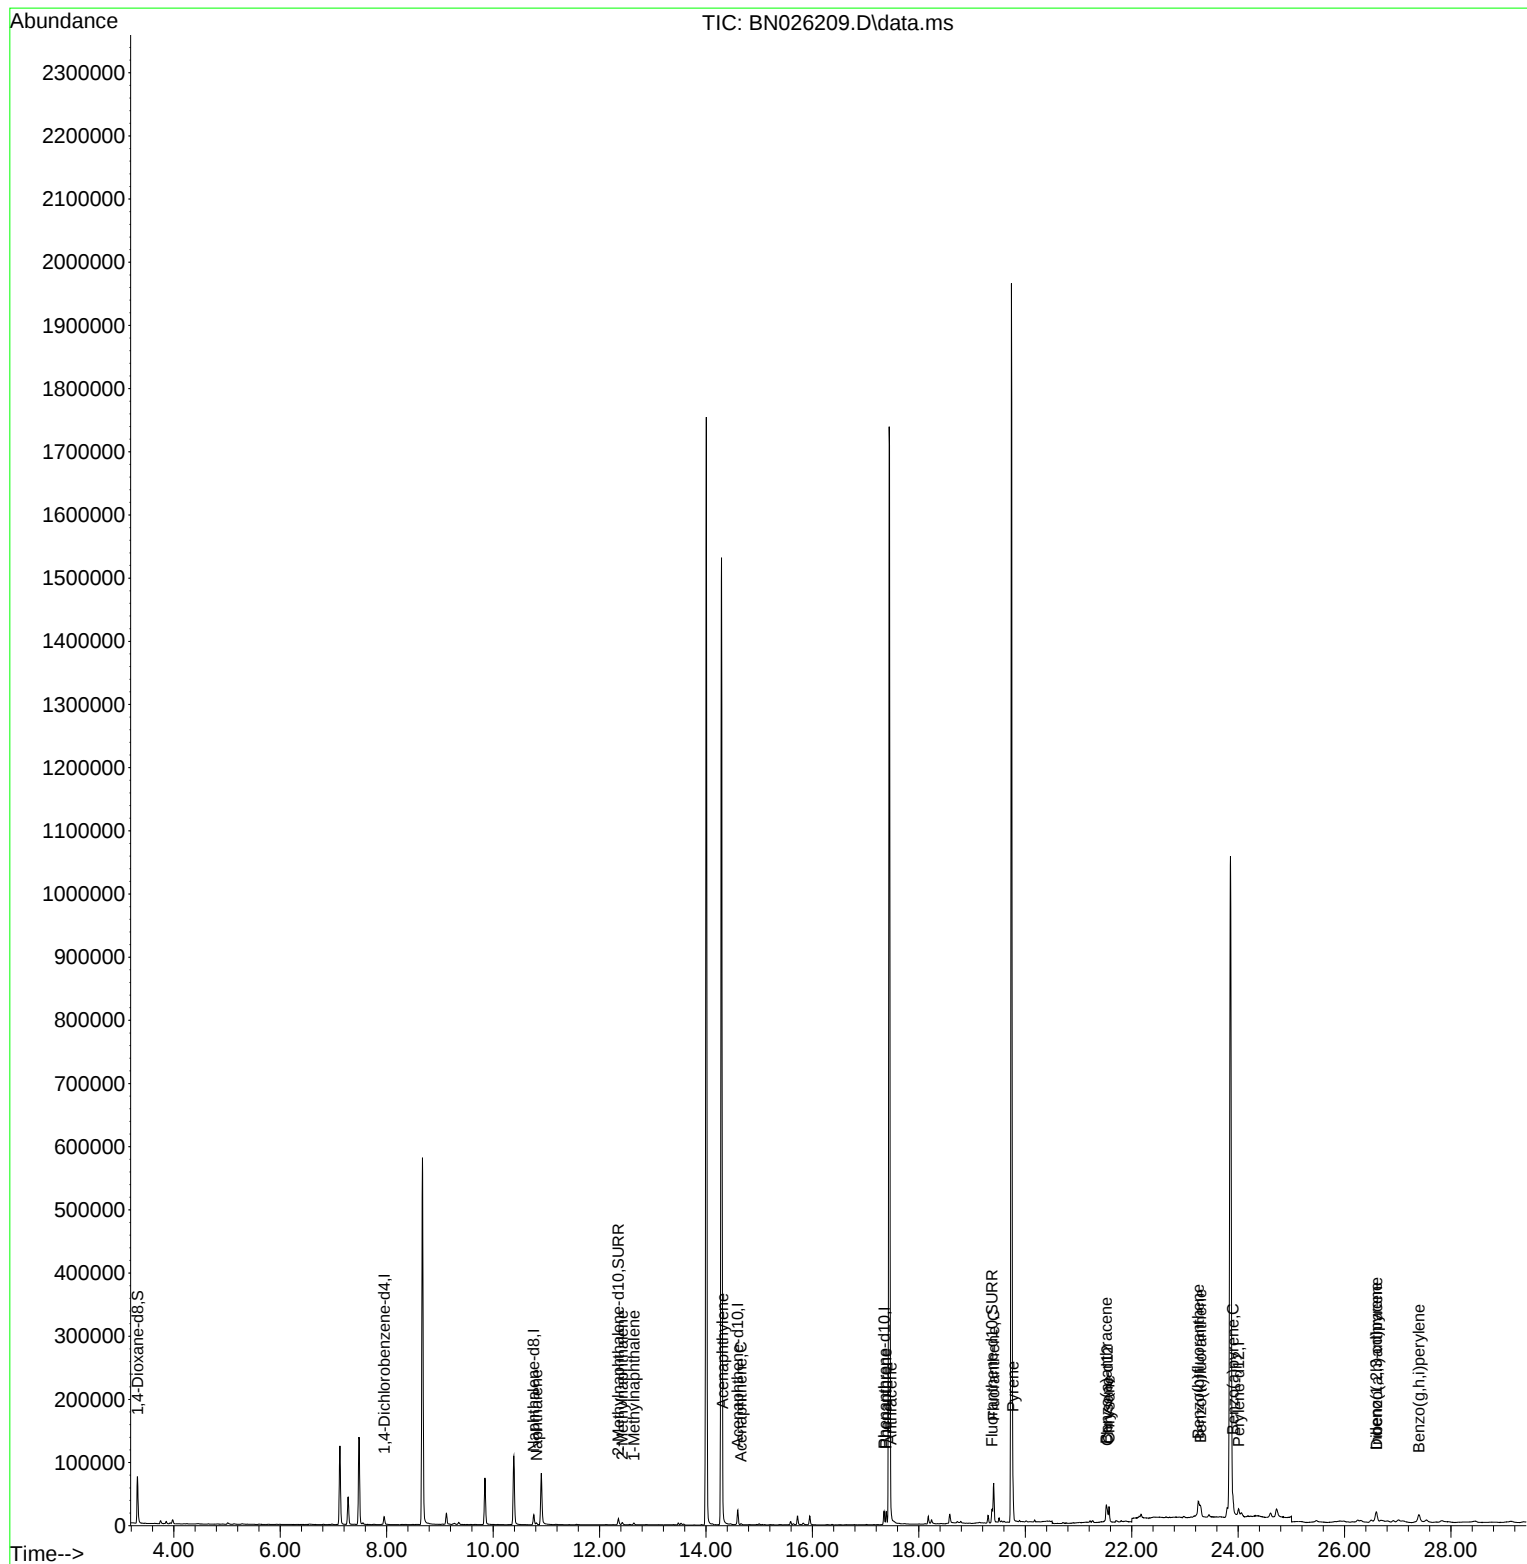



#5
Naphthalene
Concen: 0.056 ng/ul
RT: 10.814 min Scan# 1767
Delta R.T. -0.011 min
Lab File: BN026209.D
Acq: 03 Jul 2023 03:58




Instrument :
BNA_N
ClientSampleId :
DCGF4



Tgt Ion:128 Resp: 3627
Ion Ratio Lower Upper
128 100
129 17.0 9.1 13.7
127 16.5 10.7 16.1




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

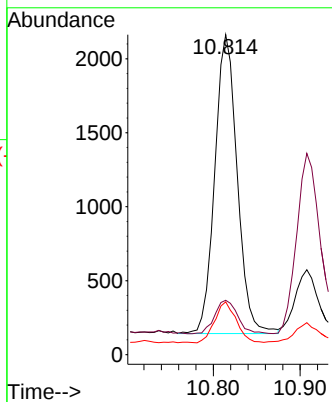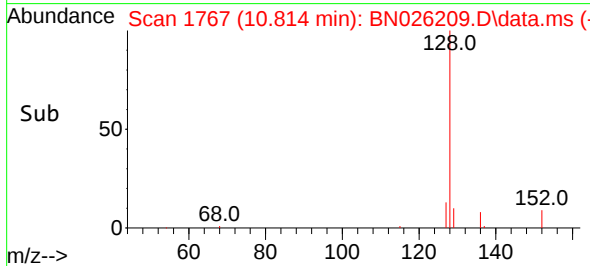

#7
2-Methylnaphthalene
Concen: 0.070 ng/ul
RT: 12.425 min Scan# 2060
Delta R.T. -0.011 min
Lab File: BN026209.D
Acq: 03 Jul 2023 03:58


Tgt Ion:142 Resp: 2866
Ion Ratio Lower Upper
142 100
141 88.3 71.9 107.9

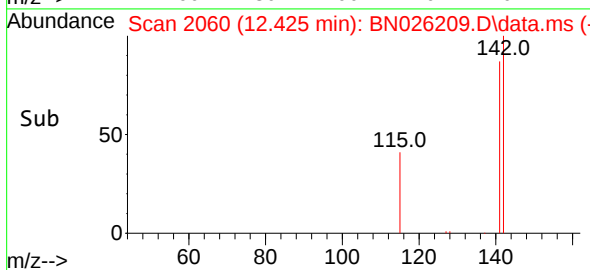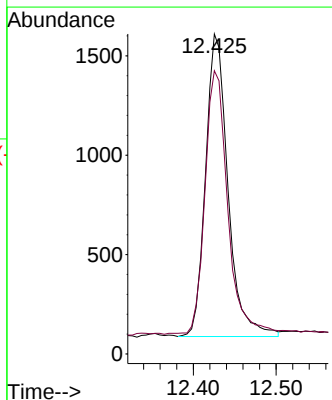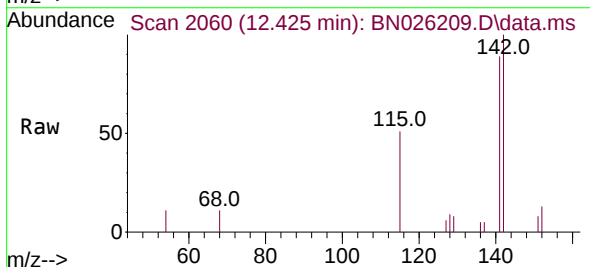

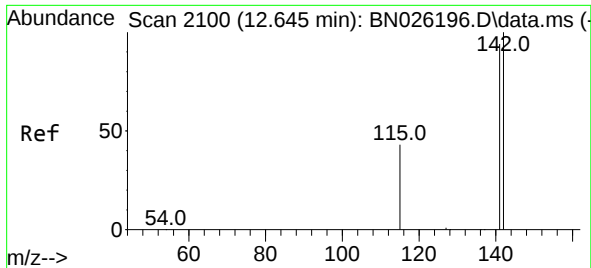

#8
1-Methylnaphthalene
Concen: 0.050 ng/ul
RT: 12.645 min Scan# 2100
Delta R.T. -0.005 min
Lab File: BN026209.D
Acq: 03 Jul 2023 03:58




Instrument :
BNA_N
ClientSampleId :
DCGF4

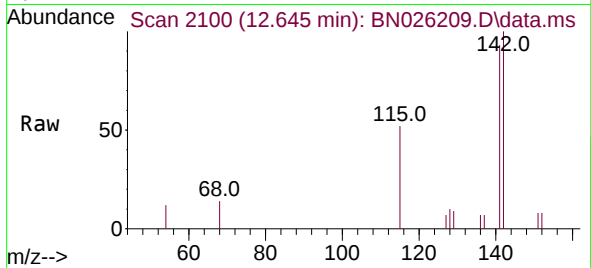

Tgt Ion:142 Resp: 2148
Ion Ratio Lower Upper
142 100
141 93.9 74.2 111.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

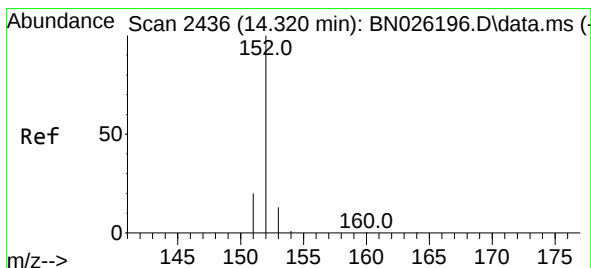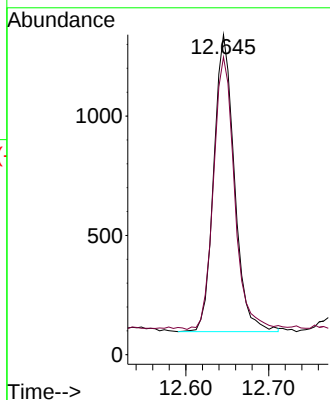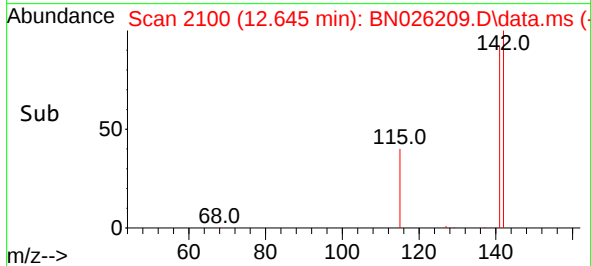

#10
Acenaphthylene
Concen: 0.059 ng/ul
RT: 14.316 min Scan# 2435
Delta R.T. -0.010 min
Lab File: BN026209.D
Acq: 03 Jul 2023 03:58

Tgt Ion:152 Resp: 3666
Ion Ratio Lower Upper
152 100
151 25.1 16.2 24.4#
153 24.8 10.9 16.3#

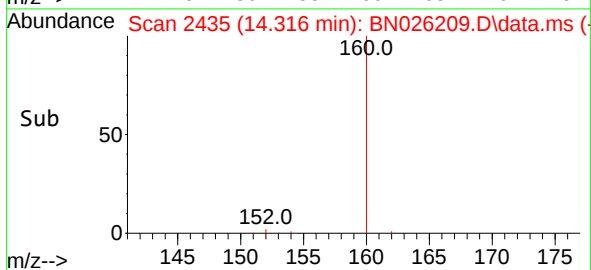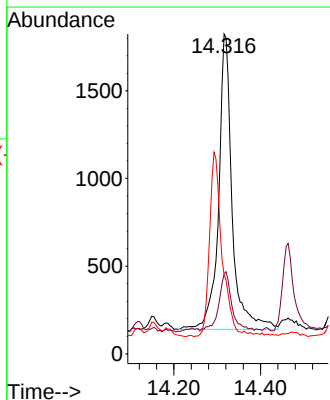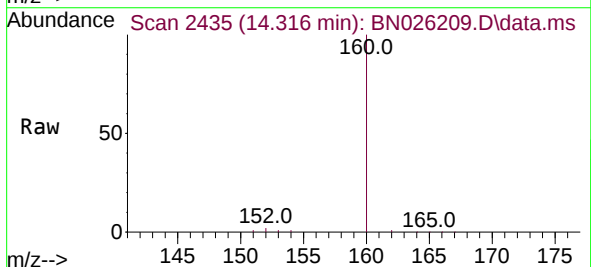



#11

Acenaphthene

Concen: 0.022 ng/u1

RT: 14.658 min Scan# 2510

Delta R.T. -0.010 min

Lab File: BN026209.D

Acq: 03 Jul 2023 03:58

Instrument :

BNA_N

ClientSampleId :

DCGF4





Tgt Ion:153	Resp:	1114
Ion Ratio	Lower	Upper
153	100	
152	57.3	39.4 59.0
154	84.6	68.9 103.3

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/03/2023

Supervised By :Sohil Jodhani 07/04/2023

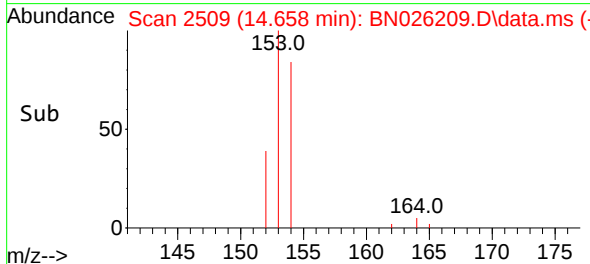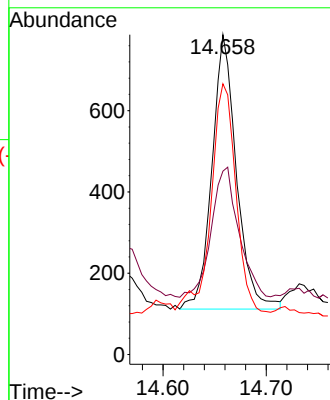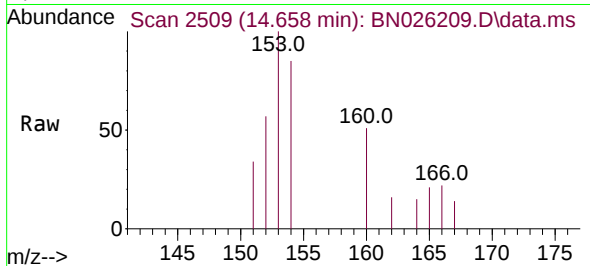

#15

Phenanthrene

Concen: 0.268 ng/u1




RT: 17.385 min Scan# 3127


Delta R.T. -0.009 min

Lab File: BN026209.D

Acq: 03 Jul 2023 03:58

Tgt Ion:178	Resp:	22912
Ion Ratio	Lower	Upper
178	100	
179	16.8	12.6 19.0
176	20.4	15.8 23.6

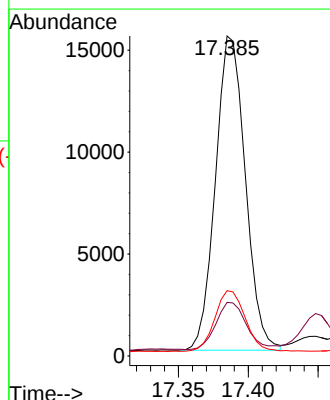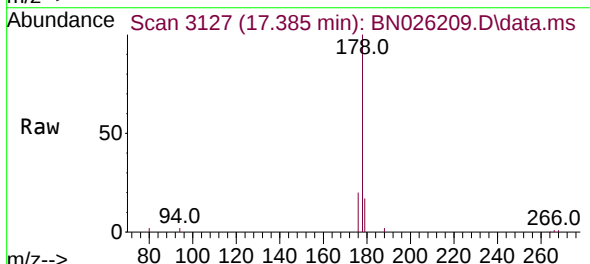

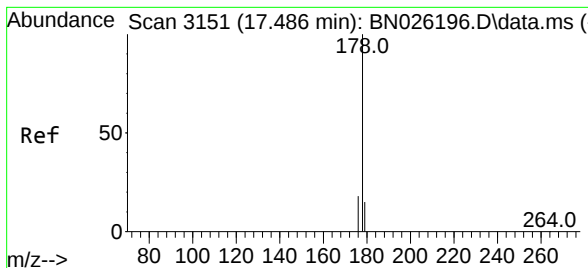

#16

Anthracene

Concen: 0.047 ng/ul

RT: 17.478 min Scan# 3149

Delta R.T. -0.009 min

Lab File: BN026209.D

Acq: 03 Jul 2023 03:58

Instrument :

BNA_N

ClientSampleId :

DCGF4





Tgt Ion:178	Resp:	3560
Ion Ratio	Lower	Upper
178	100	
179	25.5	12.6 18.8#
176	25.2	15.1 22.7#

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/03/2023

Supervised By :Sohil Jodhani 07/04/2023

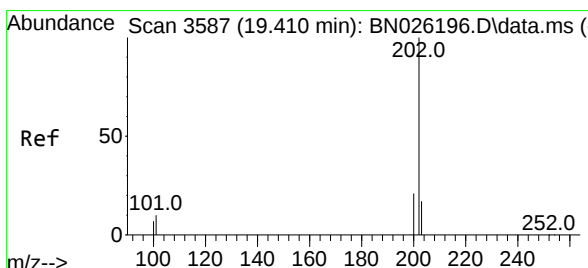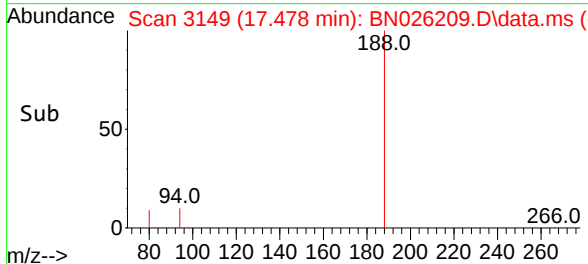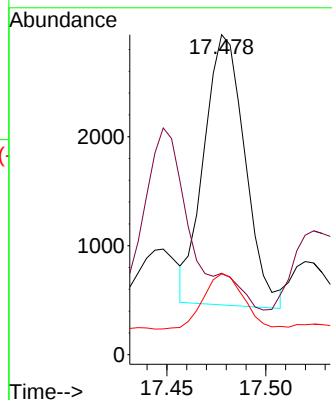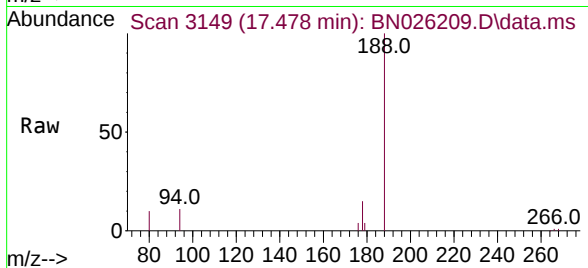

#19

Fluoranthene

Concen: 0.719 ng/ul




RT: 19.405 min Scan# 3586


Delta R.T. -0.005 min

Lab File: BN026209.D

Acq: 03 Jul 2023 03:58


Tgt Ion:202	Resp:	52392
Ion Ratio	Lower	Upper
202	100	
101	15.2	9.5 14.3#
100	11.0	7.3 10.9#

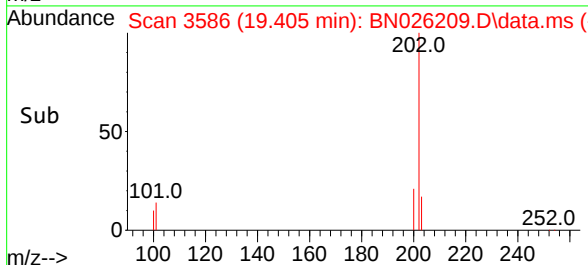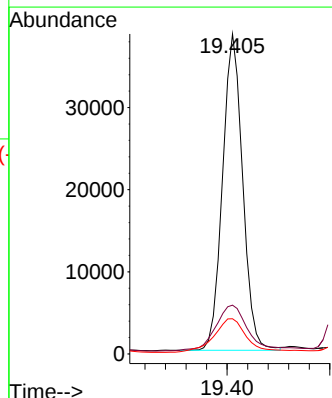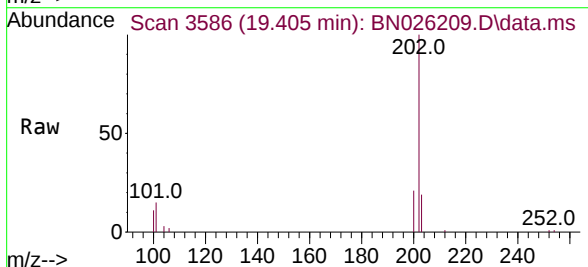



#20
Pyrene
Concen: 0.562 ng/ul m
RT: 19.768 min Scan# 3664
Delta R.T. -0.005 min
Lab File: BN026209.D
Acq: 03 Jul 2023 03:58




Instrument :
BNA_N
ClientSampleId :
DCGF4




Tgt Ion:202 Resp: 4260
Ion Ratio Lower Upper
202 100
101 13.6 11.4 17.0
100 11.6 9.1 13.7

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

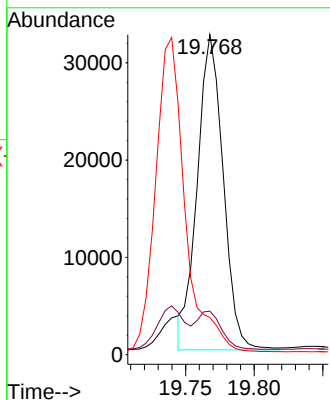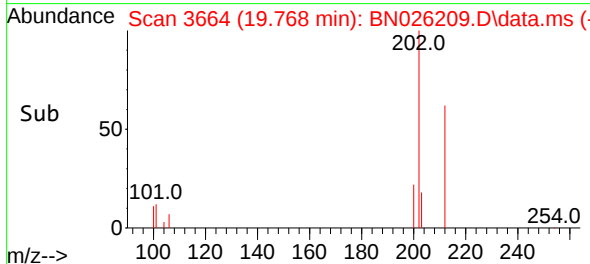


#21
Benzo(a)anthracene
Concen: 0.378 ng/ul
RT: 21.520 min Scan# 4170
Delta R.T. -0.007 min
Lab File: BN026209.D
Acq: 03 Jul 2023 03:58

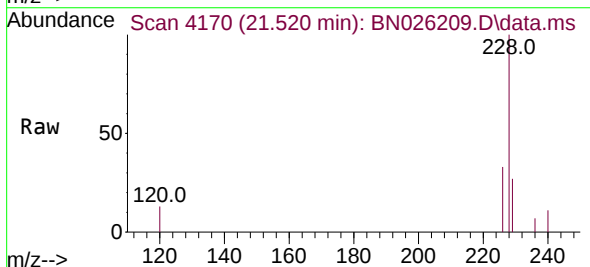


Tgt Ion:228 Resp: 21267
Ion Ratio Lower Upper
228 100
229 26.7 15.8 23.6#
226 32.7 22.5 33.7

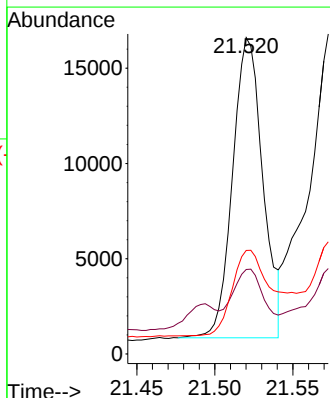

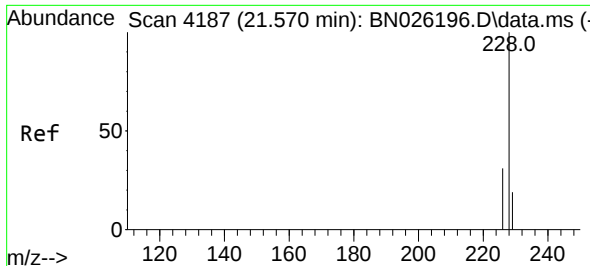

#22
Chrysene
Concen: 0.485 ng/ul
RT: 21.573 min Scan# 4187
Delta R.T. -0.007 min
Lab File: BN026209.D
Acq: 03 Jul 2023 03:58




Instrument :
BNA_N
ClientSampleId :
DCGF4




Tgt Ion:228 Resp: 2839
Ion Ratio Lower Upper
228 100
226 35.1 24.8 37.2
229 26.7 15.7 23.5

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

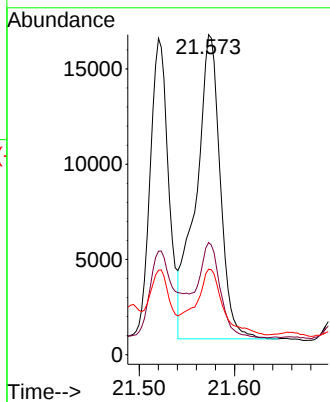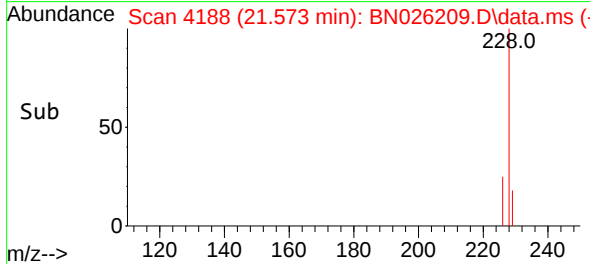


#24
Benzo(b)fluoranthene
Concen: 0.743 ng/ul m
RT: 23.250 min Scan# 4762
Delta R.T. 0.008 min
Lab File: BN026209.D
Acq: 03 Jul 2023 03:58

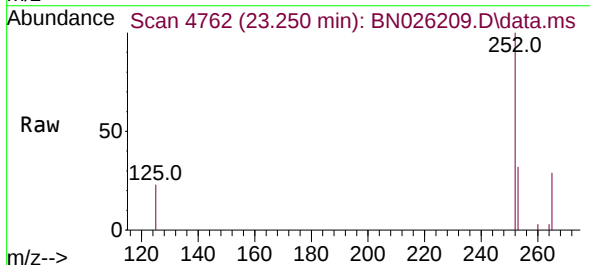

Tgt Ion:252 Resp: 48056
Ion Ratio Lower Upper
252 100
253 32.0 0.0 55.6
125 23.3 0.0 35.8

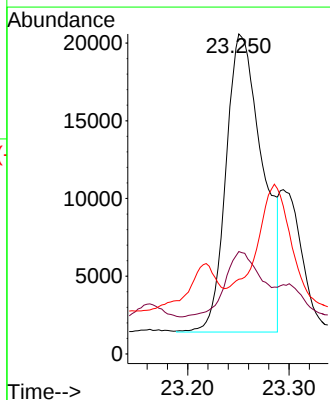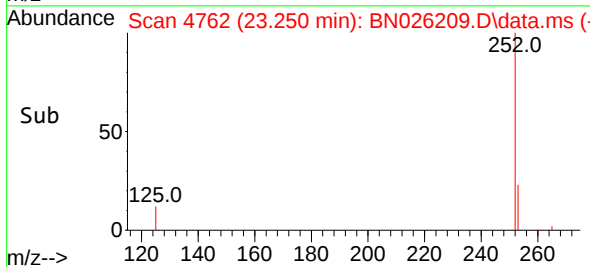

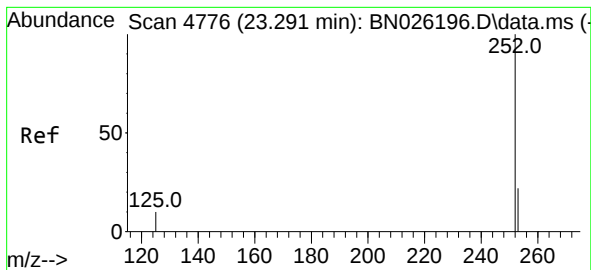

#25

Benzo(k)fluoranthene

Concen: 0.216 ng/ul m

RT: 23.294 min Scan# 4776

Delta R.T. 0.002 min

Lab File: BN026209.D

Acq: 03 Jul 2023 03:58

Instrument :

BN026196.D

ClientSampleId :





DCGF4

Tgt Ion:252	Resp:	14014
Ion Ratio	Lower	Upper
252	100	
253	42.2	23.2 34.8
125	89.9	15.0 22.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/03/2023
Supervised By :Sohil Jodhani 07/04/2023

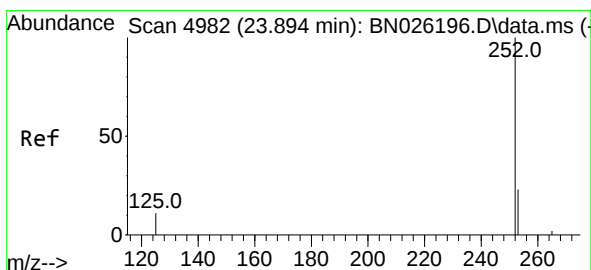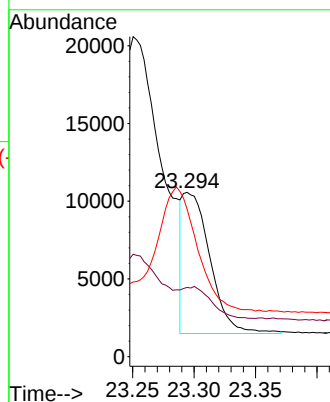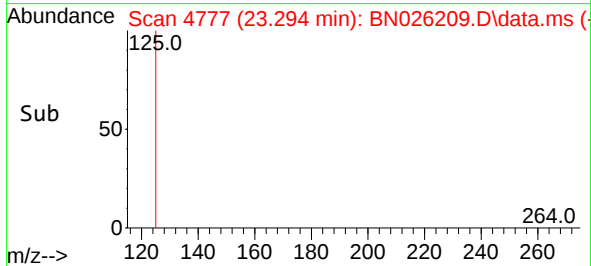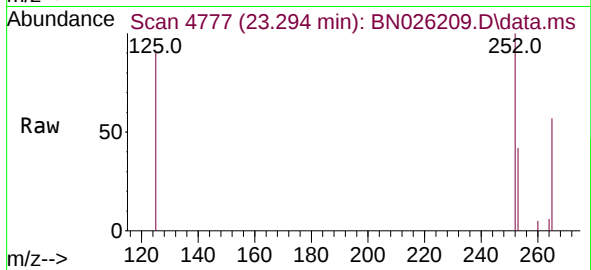

#26

Benzo(a)pyrene

Concen: 0.525 ng/ul




RT: 23.902 min Scan# 4985


Delta R.T. 0.017 min

Lab File: BN026209.D

Acq: 03 Jul 2023 03:58

Tgt Ion:252	Resp:	29450
Ion Ratio	Lower	Upper
252	100	
253	34.4	26.0 39.0
125	26.8	17.3 25.9

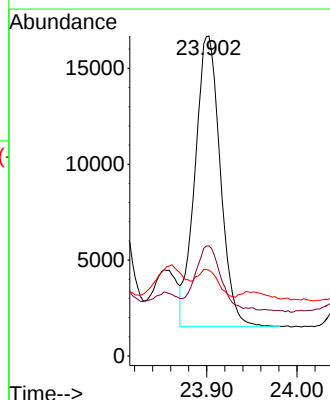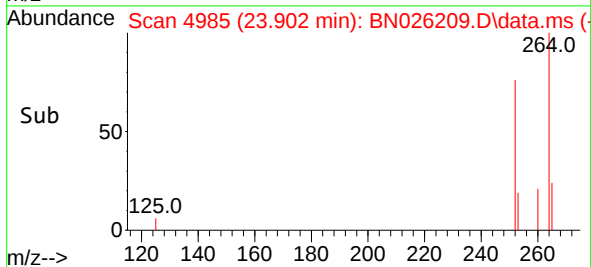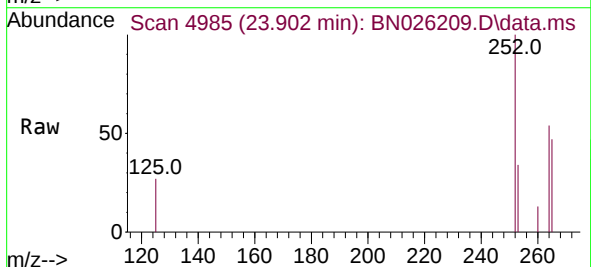

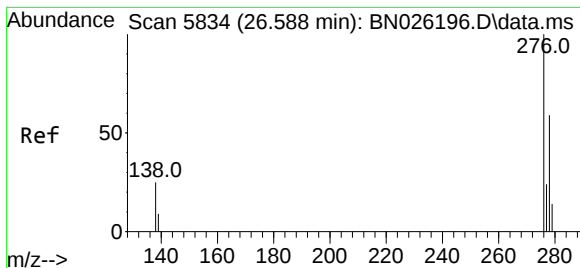

#27

Indeno(1,2,3-cd)pyrene

Concen: 0.451 ng/ul

RT: 26.598 min Scan# 5837

Delta R.T. 0.040 min

Lab File: BN026209.D


Acq: 03 Jul 2023 03:58

Instrument :

BNA_N

ClientSampleId :

DCGF4

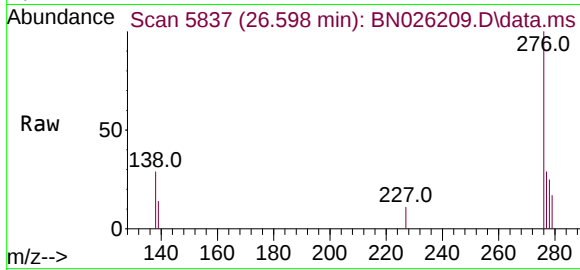

Tgt Ion:276 Resp: 27630

Ion Ratio Lower Upper

276 100

138 22.8 24.5 36.7




227 0.0 0.0 0.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/03/2023

Supervised By :Sohil Jodhani 07/04/2023

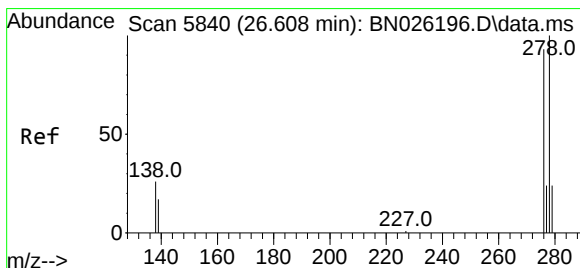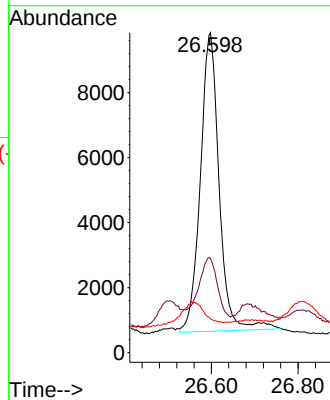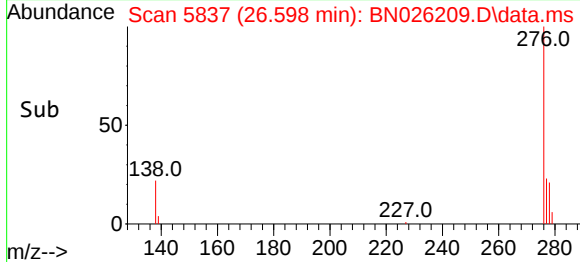

#28

Dibenzo(a,h)anthracene

Concen: 0.140 ng/ul

RT: 26.601 min Scan# 5838

Delta R.T. 0.023 min

Lab File: BN026209.D

Acq: 03 Jul 2023 03:58




Tgt Ion:278 Resp: 6518


Ion Ratio Lower Upper

278 100

139 56.2 19.0 28.4#


279 62.6 26.7 40.1#

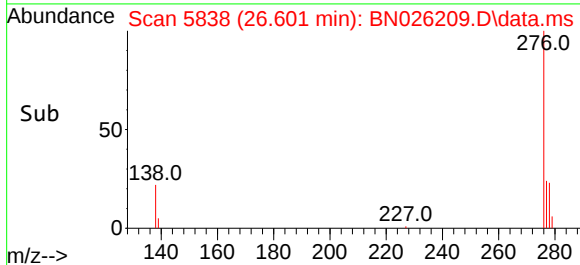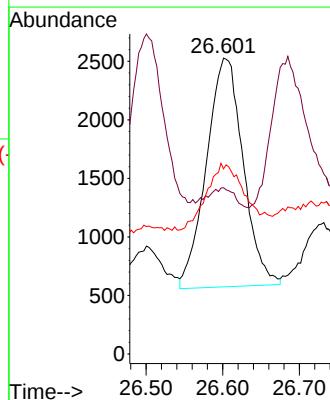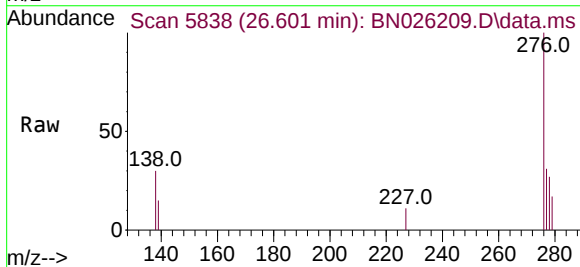

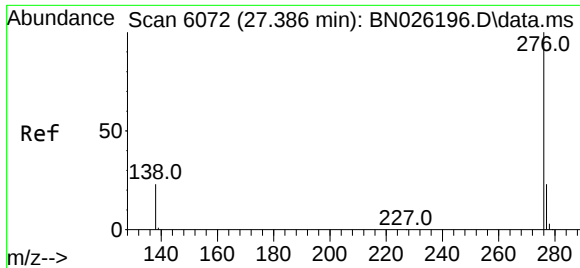

#29
 Benzo(g,h,i)perylene
 Concen: 0.517 ng/ul
 RT: 27.396 min Scan# 6075
 Delta R.T. 0.050 min
 Lab File: BN026209.D
 Acq: 03 Jul 2023 03:58

Instrument :
 BNA_N
 ClientSampleId :
 DCGF4

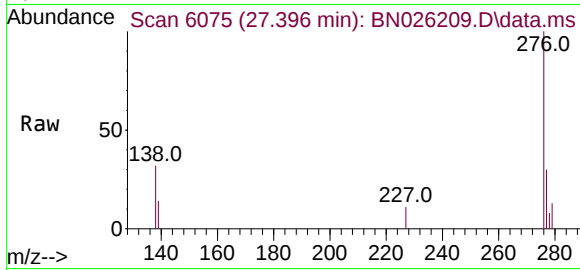

Tgt Ion:276 Resp: 28190
 Ion Ratio Lower Upper
 276 100
 138 31.6 23.4 35.0
 277 29.6 20.0 30.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2023
 Supervised By :Sohil Jodhani 07/04/2023

