

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
 Data File : BN026227.D
 Acq On : 03 Jul 2023 15:36
 Operator : MA/JU
 Sample : 03246-10
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGJ7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/04/2023
 Supervised By :Sohil Jodhani 07/04/2023

Quant Time: Jul 03 23:22:30 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 01 01:46:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	11898	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.765	136	36462	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.598	164	22693	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.347	188	48666	0.400	ng/ul	0.00
17) Chrysene-d12	21.541	240	25520	0.400	ng/ul	# 0.00
23) Perylene-d12	24.011	264	26871	0.400	ng/ul	# 0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	41540	3.100	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.354	152	12515	0.223	ng/ul	-0.01
18) Fluoranthene-d10	19.373	212	25996	0.268	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.814	128	36838	0.353	ng/ul	99
7) 2-Methylnaphthalene	12.426	142	12809	0.192	ng/ul	99
8) 1-Methylnaphthalene	12.645	142	8452	0.123	ng/ul	100
10) Acenaphthylene	14.320	152	46706	0.440	ng/ul	99
11) Acenaphthene	14.658	153	10653	0.123	ng/ul	99
12) Fluorene	15.644	166	18010	0.181	ng/ul#	98
15) Phenanthrene	17.389	178	282980	1.760	ng/ul	99
16) Anthracene	17.478	178	75198	0.526	ng/ul	99
19) Fluoranthene	19.405	202	514601	3.775	ng/ul	97
20) Pyrene	19.772	202	429441	3.029	ng/ul	94
21) Benzo(a)anthracene	21.523	228	219284	2.083	ng/ul	95
22) Chrysene	21.576	228	258921	2.364	ng/ul#	95
24) Benzo(b)fluoranthene	23.259	252	423197m	3.690	ng/ul	
25) Benzo(k)fluoranthene	23.300	252	115234m	1.001	ng/ul	
26) Benzo(a)pyrene	23.908	252	232253	2.332	ng/ul#	88
27) Indeno(1,2,3-cd)pyrene	26.605	276	186203	1.711	ng/ul#	81
28) Dibenzo(a,h)anthracene	26.618	278	45008	0.547	ng/ul#	75
29) Benzo(g,h,i)perylene	27.416	276	183057	1.891	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
Data File : BN026227.D
Acq On : 03 Jul 2023 15:36
Operator : MA/JU
Sample : 03246-10
Misc :
ALS Vial : 84 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCGJ7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/04/2023
Supervised By :Sohil Jodhani 07/04/2023


Quant Time: Jul 03 23:22:30 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 01 01:46:24 2023
Response via : Initial Calibration

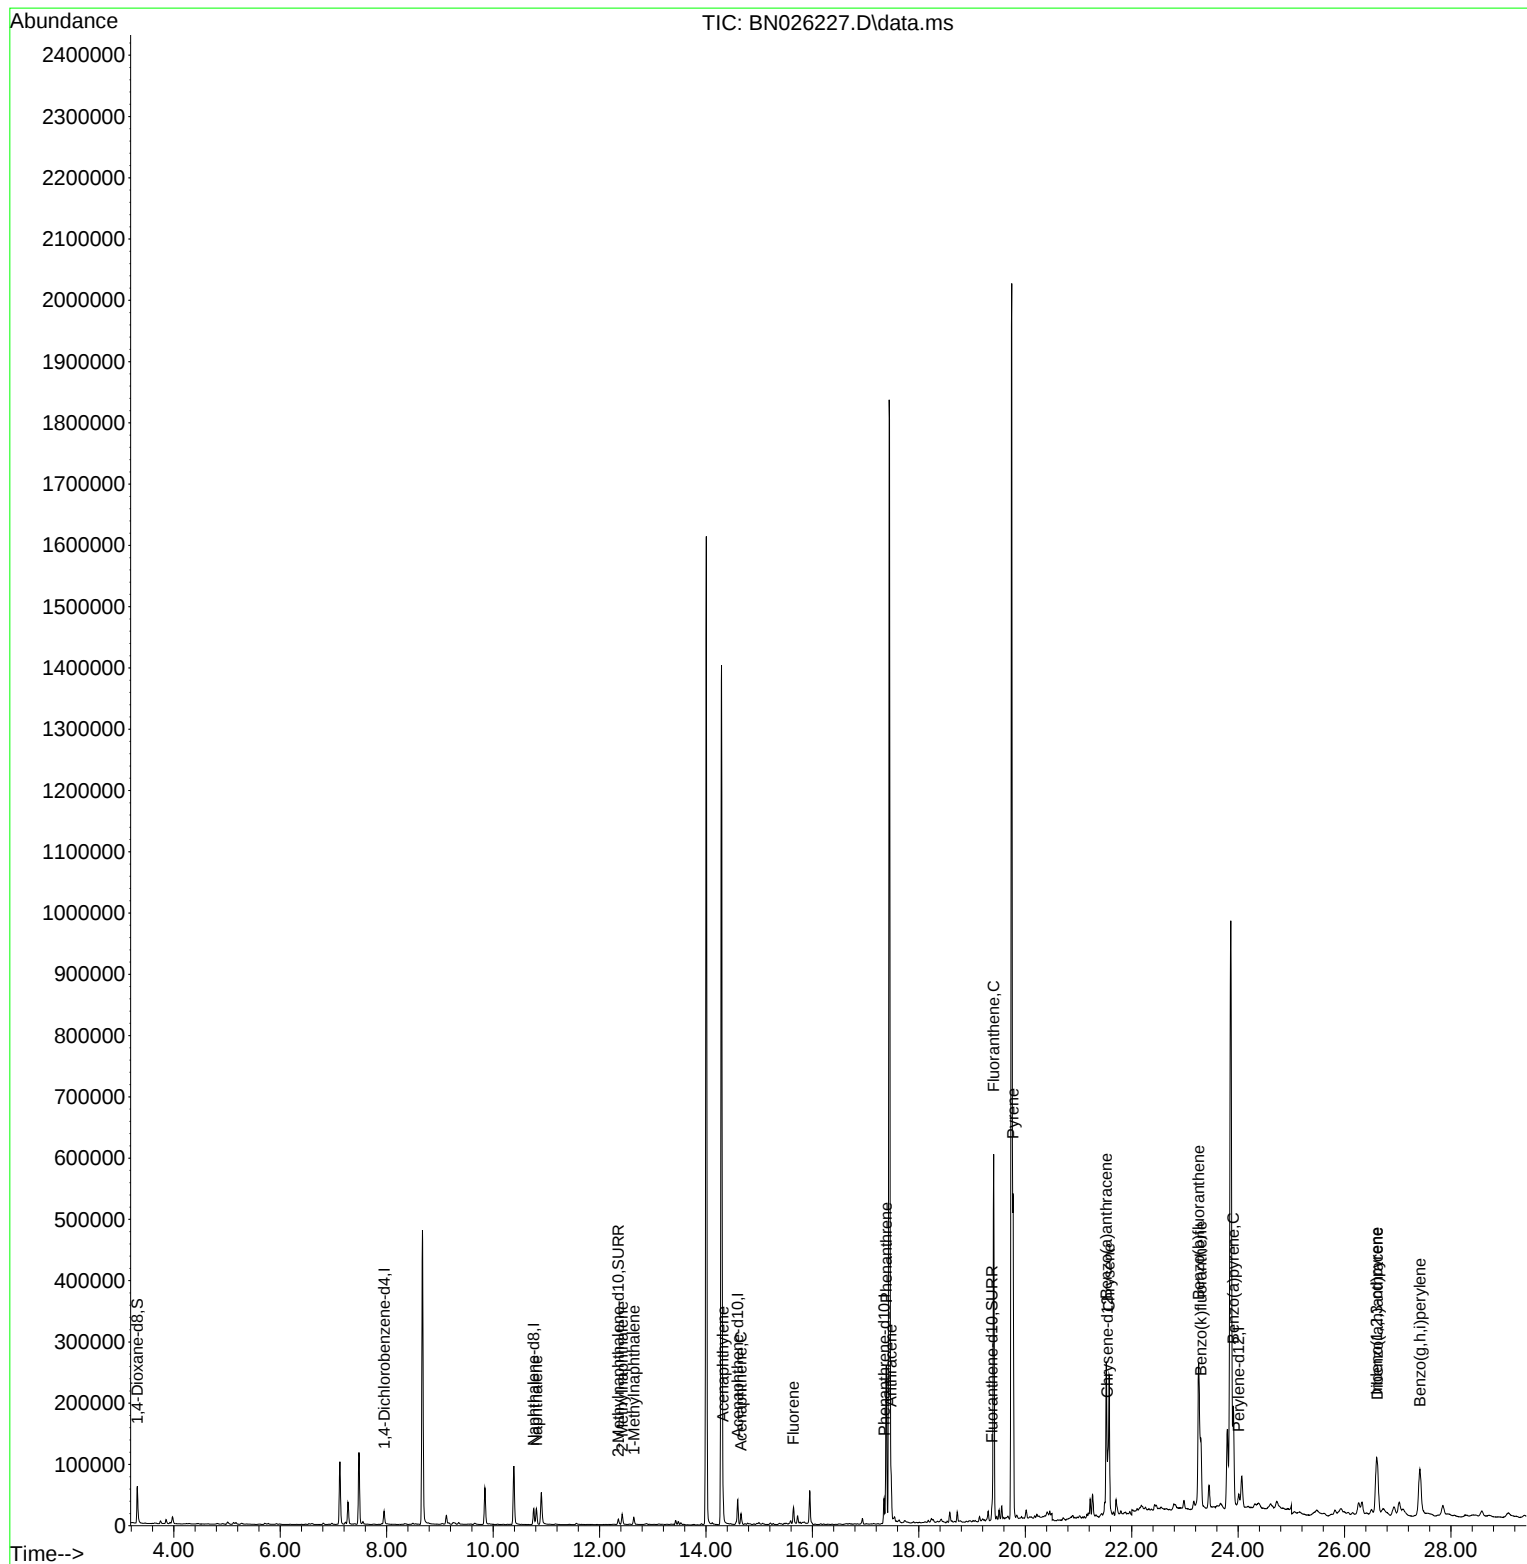

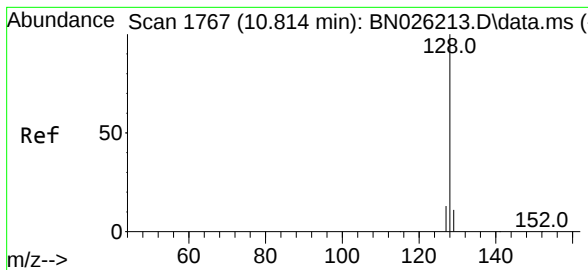

#5
Naphthalene
Concen: 0.353 ng/ul
RT: 10.814 min Scan# 1767
Delta R.T. -0.011 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36




Instrument :
BNA_N
ClientSampleId :
DCGJ7

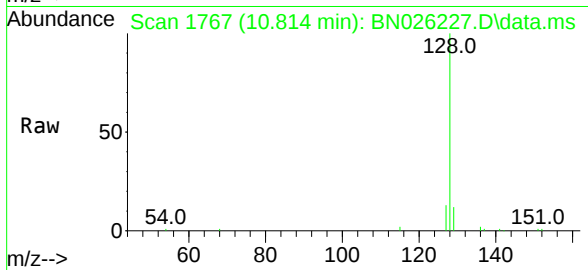


Tgt Ion:128 Resp: 36838
Ion Ratio Lower Upper
128 100
129 11.8 9.1 13.7
127 13.4 10.7 16.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/04/2023
Supervised By :Sohil Jodhani 07/04/2023

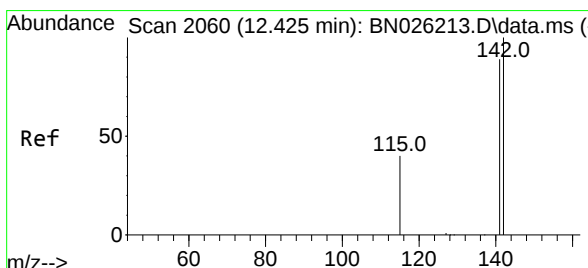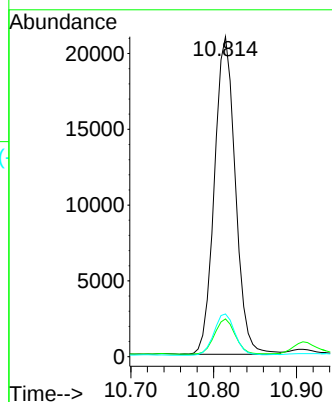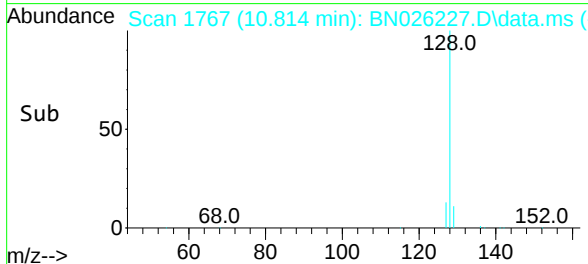


#7
2-Methylnaphthalene
Concen: 0.192 ng/ul
RT: 12.426 min Scan# 2060
Delta R.T. -0.011 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36

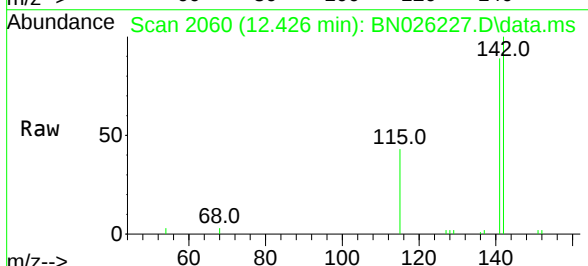

Tgt Ion:142 Resp: 12809
Ion Ratio Lower Upper
142 100
141 89.1 71.9 107.9

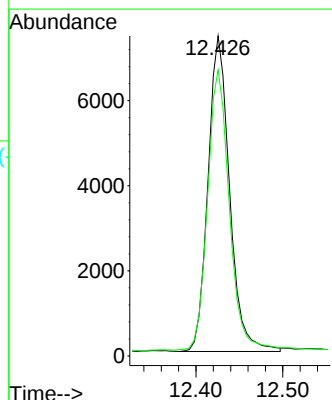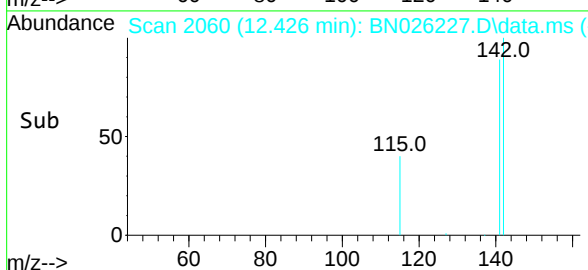

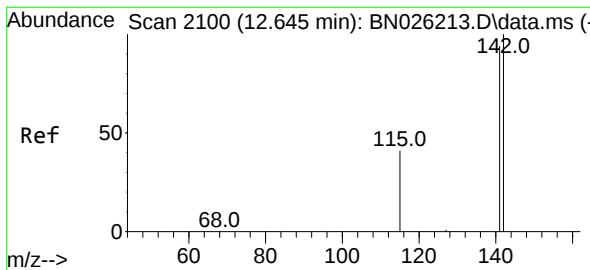

#8

1-Methylnaphthalene

Concen: 0.123 ng/ul

RT: 12.645 min Scan# 2100

Delta R.T. -0.005 min

Lab File: BN026227.D


Acq: 03 Jul 2023 15:36

Instrument :

BNA_N

ClientSampleId :

DCGJ7



Tgt Ion:142 Resp: 845

Ion Ratio Lower Upper

142 100




141 92.8 74.2 111.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/04/2023

Supervised By :Sohil Jodhani 07/04/2023

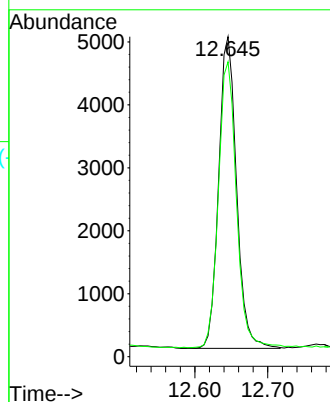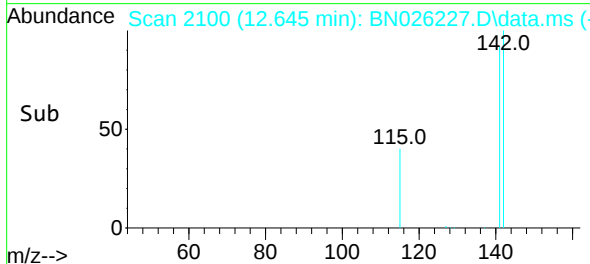

#10

Acenaphthylene

Concen: 0.440 ng/ul

RT: 14.320 min Scan# 2436

Delta R.T. -0.005 min

Lab File: BN026227.D

Acq: 03 Jul 2023 15:36




Tgt Ion:152 Resp: 46706


Ion Ratio Lower Upper

152 100

151 20.4 16.2 24.4


153 14.1 10.9 16.3

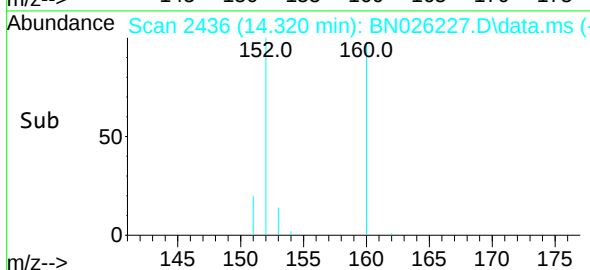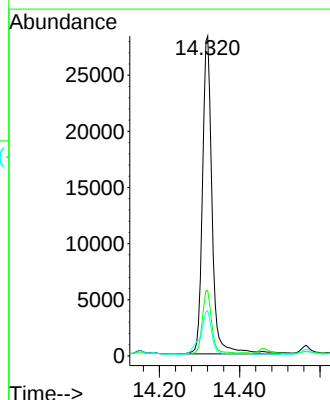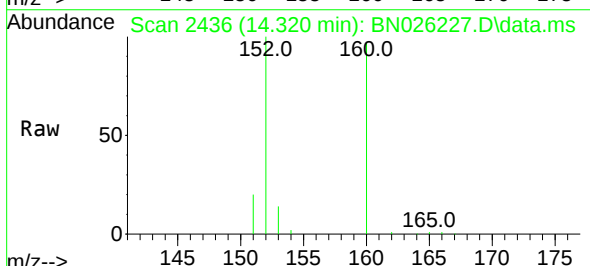

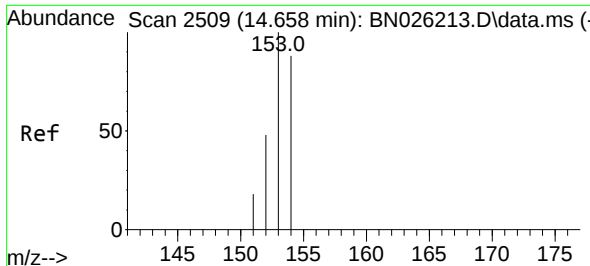

#11
Acenaphthene
Concen: 0.123 ng/ul
RT: 14.658 min Scan# 21
Delta R.T. -0.010 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36




Instrument :
BNA_N
ClientSampleId :
DCGJ7



Tgt Ion:153 Resp: 1065
Ion Ratio Lower Upper
153 100
152 51.3 39.4 59.0
154 86.6 68.9 103.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/04/2023
Supervised By :Sohil Jodhani 07/04/2023

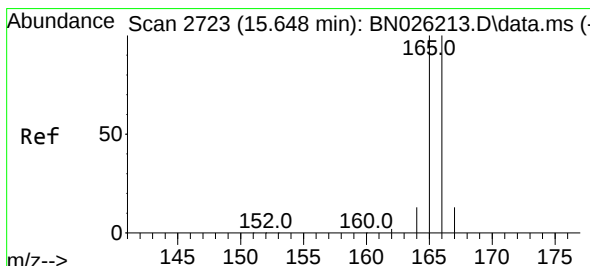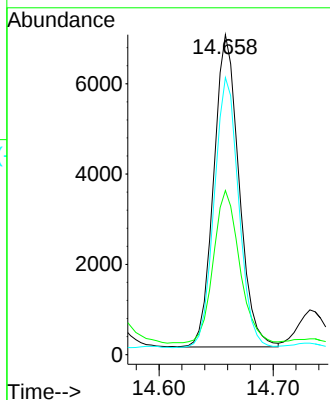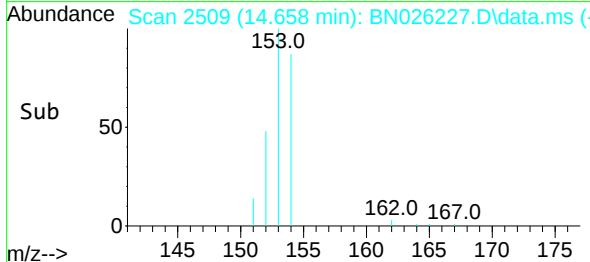

#12
Fluorene
Concen: 0.181 ng/ul
RT: 15.644 min Scan# 2722
Delta R.T. -0.010 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36

Tgt Ion:166 Resp: 18010
Ion Ratio Lower Upper
166 100
165 100.6 79.9 119.9
167 17.0 10.8 16.2#

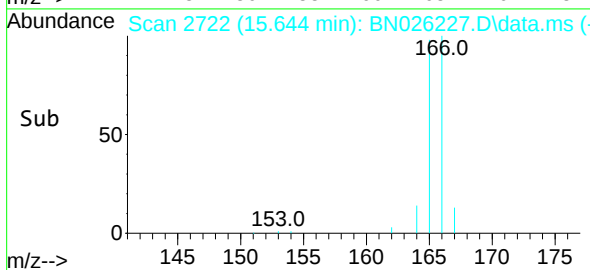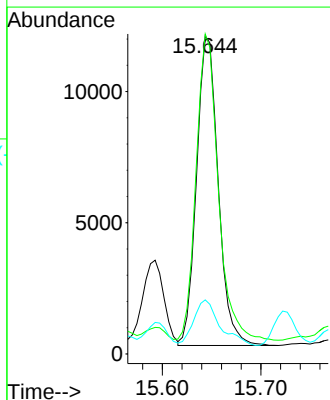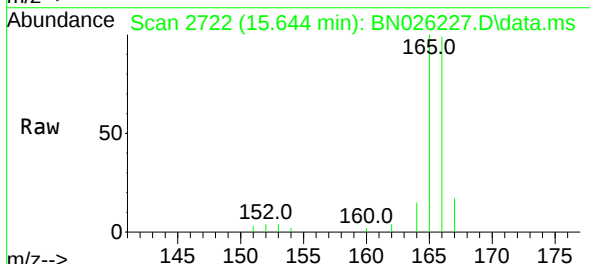

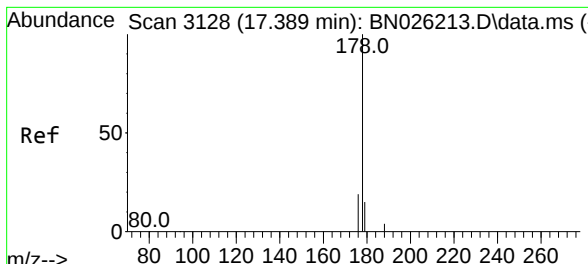





#15
 Phenanthrene
 Concen: 1.760 ng/ul
 RT: 17.389 min Scan# 3128
 Delta R.T. -0.005 min
 Lab File: BN026227.D
 Acq: 03 Jul 2023 15:36

Instrument : BNA_N
 ClientSampleId : DCGJ7

Tgt Ion:178 Resp: 282980

Ion	Ratio	Lower	Upper
178	100		
179	15.4	12.6	19.0
176	19.6	15.8	23.6




Manual Integrations
APPROVED
 Reviewed By :Yogesh Patel 07/04/2023
 Supervised By :Sohil Jodhani 07/04/2023

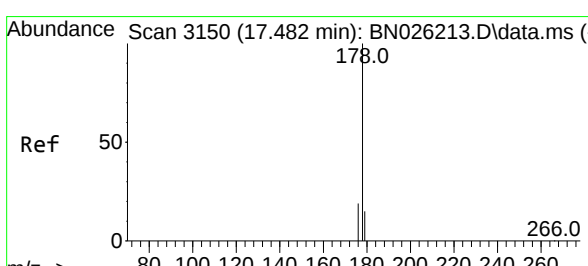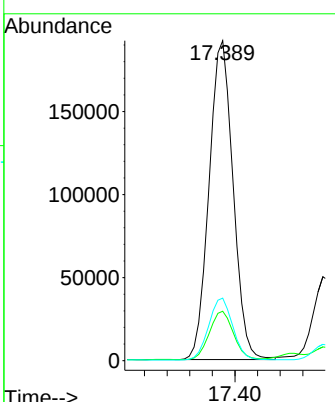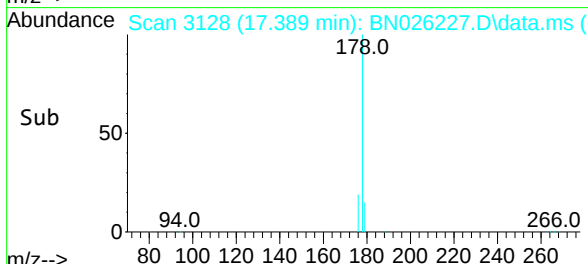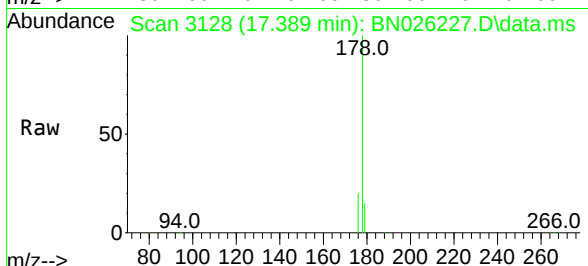


#16
 Anthracene
 Concen: 0.526 ng/ul
 RT: 17.478 min Scan# 3149
 Delta R.T. -0.009 min
 Lab File: BN026227.D
 Acq: 03 Jul 2023 15:36

Tgt Ion:178 Resp: 75198


Ion	Ratio	Lower	Upper
178	100		
179	16.4	12.6	18.8
176	19.4	15.1	22.7

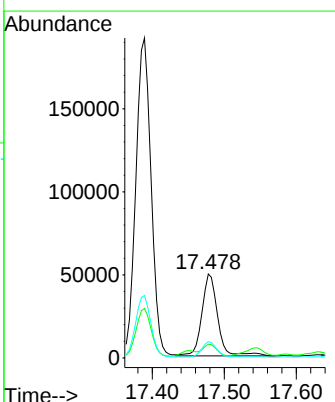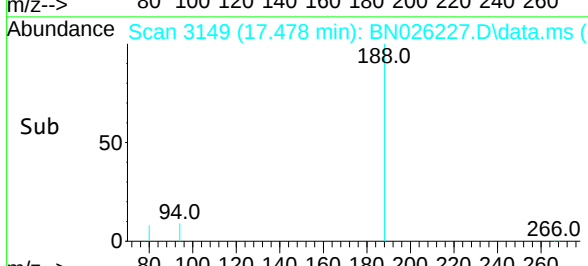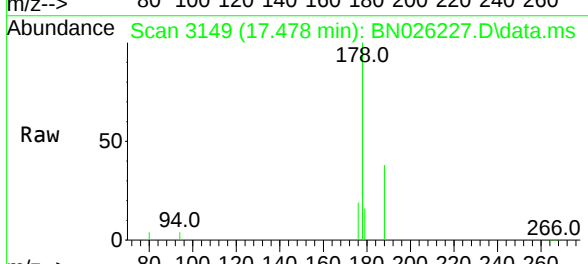

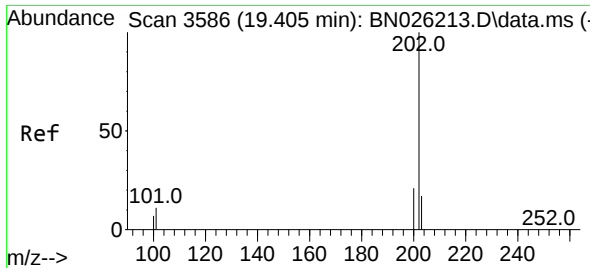

#19
Fluoranthene
Concen: 3.775 ng/u1
RT: 19.405 min Scan# 3586
Delta R.T. -0.005 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36




Instrument :
BNA_N
ClientSampleId :
DCGJ7




Tgt Ion:202 Resp: 51460
Ion Ratio Lower Upper
202 100
101 10.7 9.5 14.3
100 8.1 7.3 10.9

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/04/2023
Supervised By :Sohil Jodhani 07/04/2023

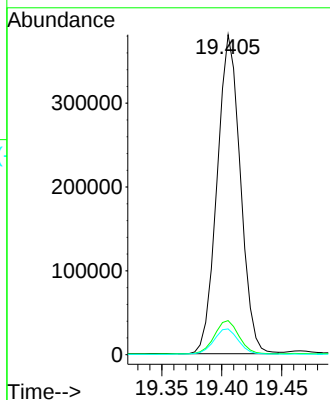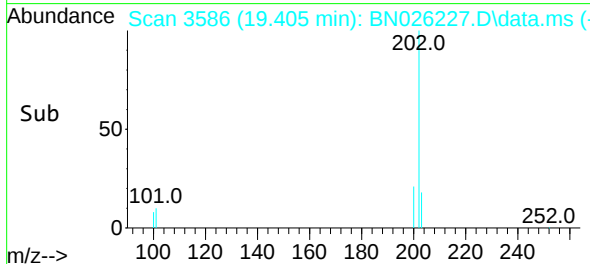


#20
Pyrene
Concen: 3.029 ng/u1
RT: 19.772 min Scan# 3665
Delta R.T. -0.001 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36

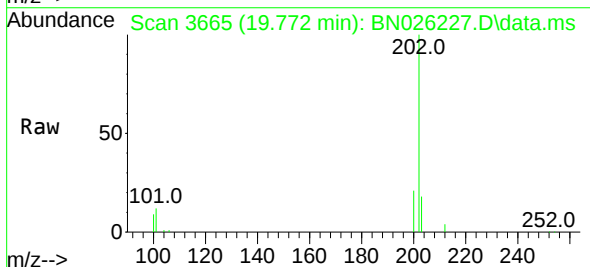


Tgt Ion:202 Resp: 429441
Ion Ratio Lower Upper
202 100
101 11.6 11.4 17.0
100 9.5 9.1 13.7

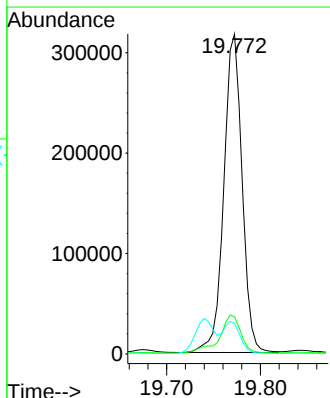

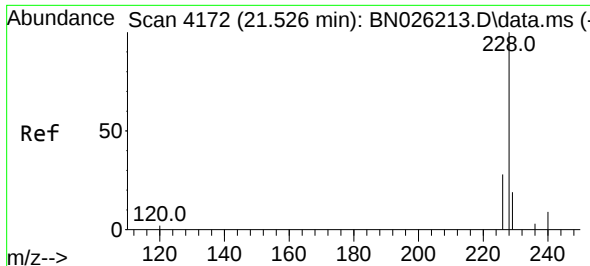

#21
Benzo(a)anthracene
Concen: 2.083 ng/u1
RT: 21.523 min Scan# 4172
Delta R.T. -0.004 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36




Instrument :
BNA_N
ClientSampleId :
DCGJ7



Tgt Ion:228 Resp: 219284
Ion Ratio Lower Upper
228 100
229 23.4 15.8 23.6
226 29.9 22.5 33.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/04/2023
Supervised By :Sohil Jodhani 07/04/2023

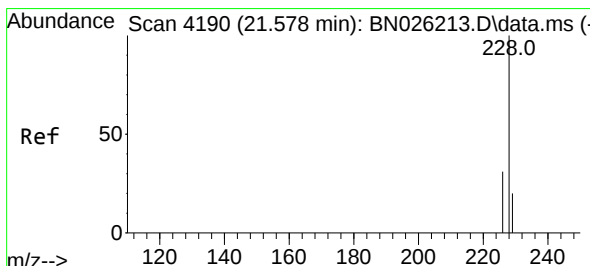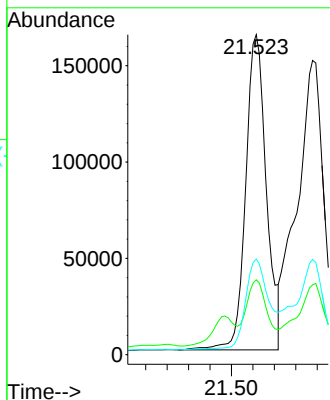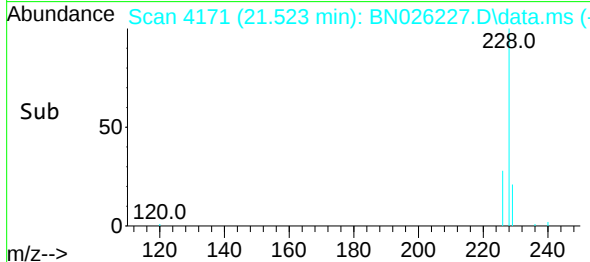

#22
Chrysene
Concen: 2.364 ng/u1
RT: 21.576 min Scan# 4189
Delta R.T. -0.004 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36


Tgt Ion:228 Resp: 258921
Ion Ratio Lower Upper
228 100
226 32.3 24.8 37.2
229 23.7 15.7 23.5#

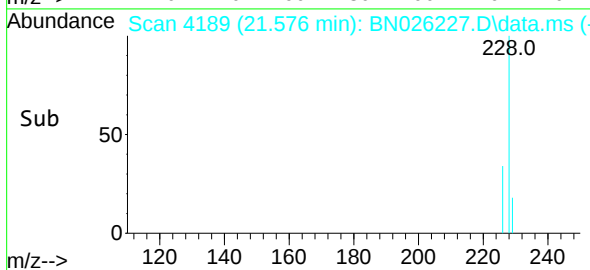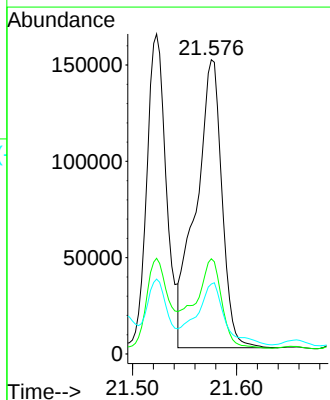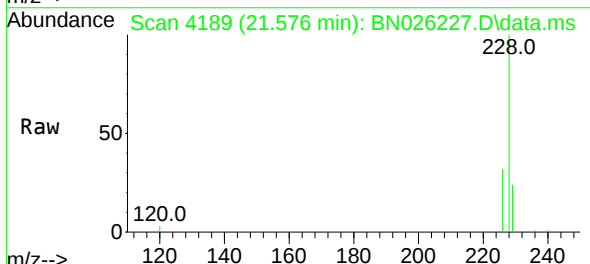

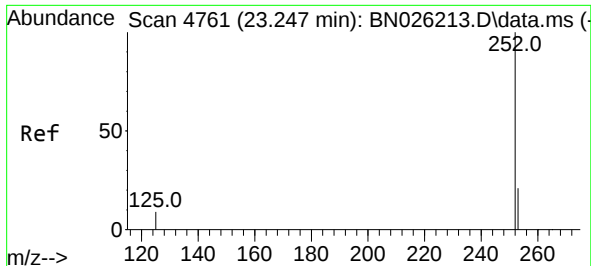

#24
Benzo(b)fluoranthene
Concen: 3.690 ng/ul m
RT: 23.259 min Scan# 4765
Delta R.T. 0.017 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36




Instrument :
BNA_N
ClientSampleId :
DCGJ7

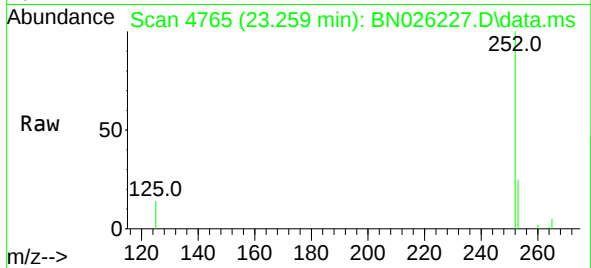


Tgt Ion:252 Resp: 423197
Ion Ratio Lower Upper
252 100
253 25.2 0.0 55.6
125 13.6 0.0 35.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/04/2023
Supervised By :Sohil Jodhani 07/04/2023

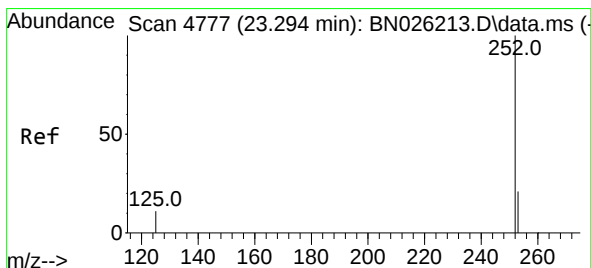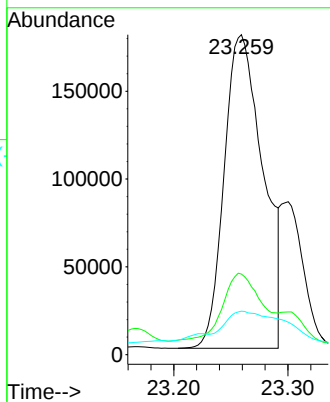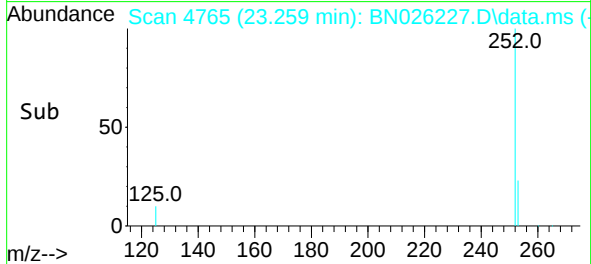


#25
Benzo(k)fluoranthene
Concen: 1.001 ng/ul m
RT: 23.300 min Scan# 4779
Delta R.T. 0.008 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36

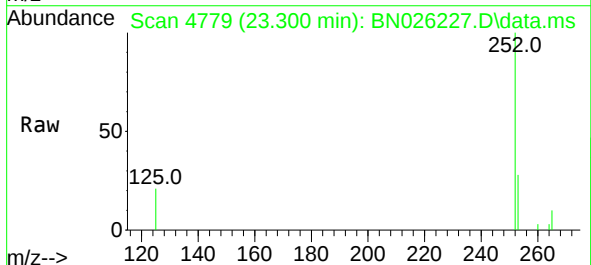


Tgt Ion:252 Resp: 115234
Ion Ratio Lower Upper
252 100
253 27.9 23.2 34.8
125 21.2 15.0 22.4

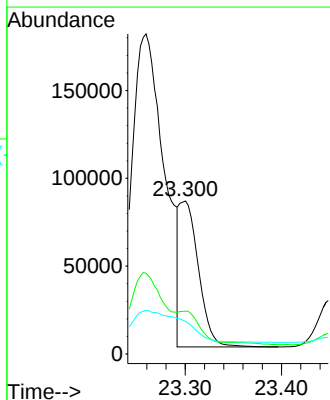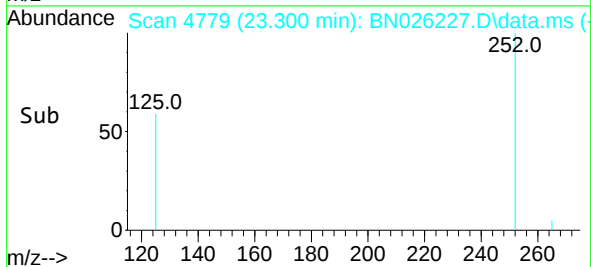

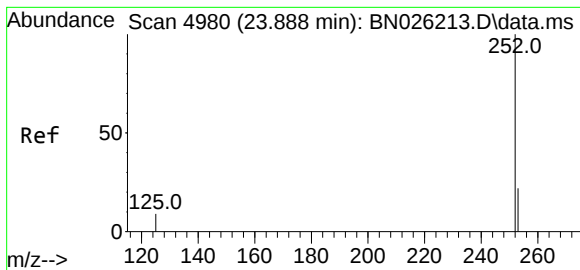

#26
Benzo(a)pyrene
Concen: 2.332 ng/ul
RT: 23.908 min Scan# 4980
Delta R.T. 0.023 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36




Instrument :
BNA_N
ClientSampleId :
DCGJ7

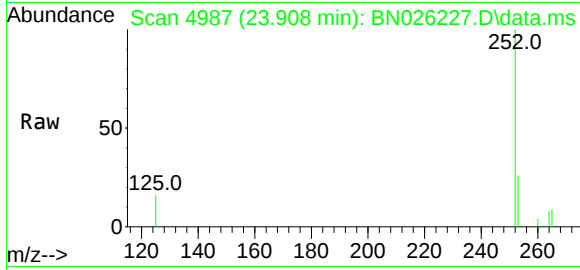


Tgt Ion:252 Resp: 23225
Ion Ratio Lower Upper
252 100
253 26.0 26.0 39.0
125 15.9 17.3 25.9

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/04/2023
Supervised By :Sohil Jodhani 07/04/2023

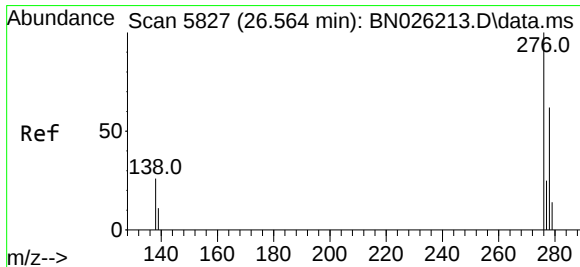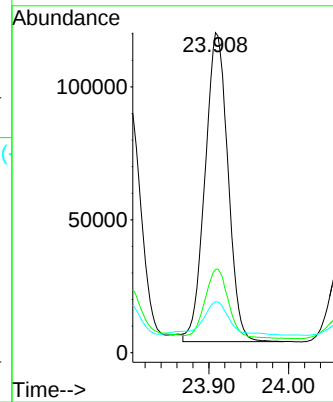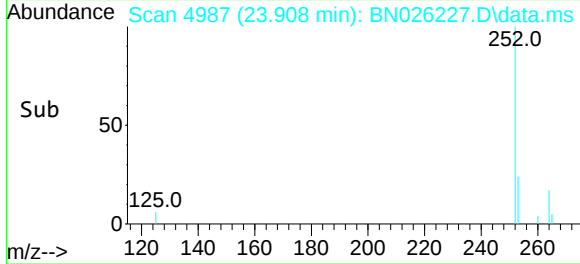


#27
Indeno(1,2,3-cd)pyrene
Concen: 1.711 ng/ul
RT: 26.605 min Scan# 5839
Delta R.T. 0.046 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36

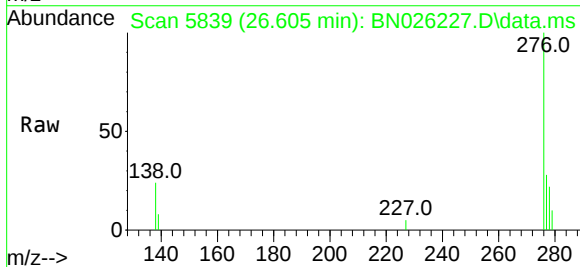


Tgt Ion:276 Resp: 186203
Ion Ratio Lower Upper
276 100
138 20.3 24.5 36.7#
227 1.3 0.0 0.0#

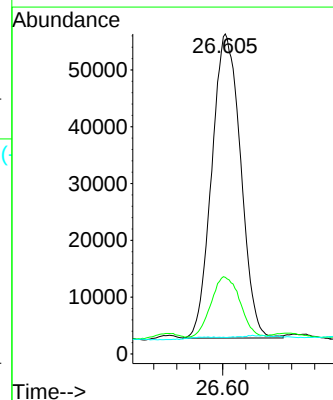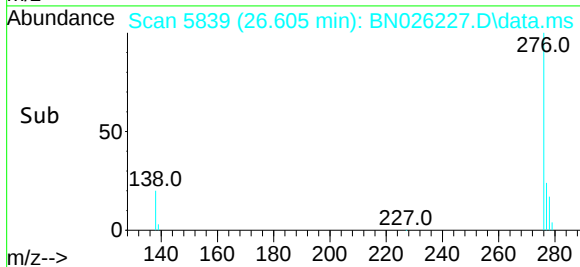



#28
Dibenzo(a,h)anthracene
Concen: 0.547 ng/ul
RT: 26.618 min Scan# 5843
Delta R.T. 0.040 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36




Instrument :
BNA_N
ClientSampleId :
DCGJ7




Tgt Ion:278 Resp: 45000
Ion Ratio Lower Upper
278 100
139 36.8 19.0 28.4
279 46.6 26.7 40.1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/04/2023
Supervised By :Sohil Jodhani 07/04/2023

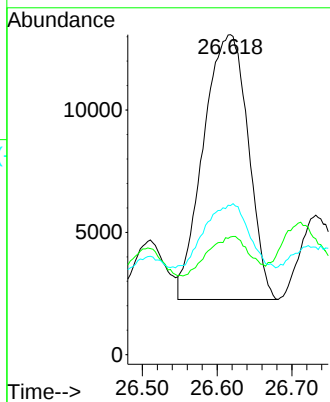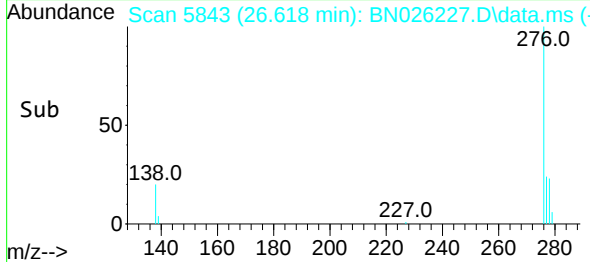

#29
Benzo(g,h,i)perylene
Concen: 1.891 ng/ul
RT: 27.416 min Scan# 6081
Delta R.T. 0.070 min
Lab File: BN026227.D
Acq: 03 Jul 2023 15:36

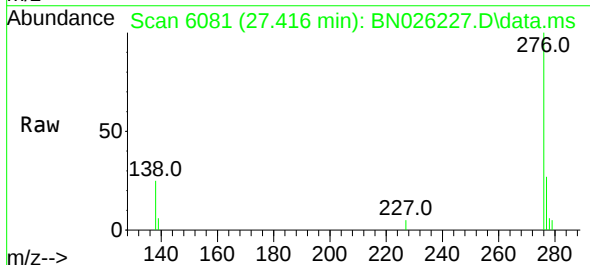

Tgt Ion:276 Resp: 183057
Ion Ratio Lower Upper
276 100
138 25.4 23.4 35.0
277 26.9 20.0 30.0

