

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
 Data File : BN026262.D
 Acq On : 04 Jul 2023 14:22
 Operator : MA/JU
 Sample : 03247-07DL 5X
 Misc :
 ALS Vial : 119 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGL3DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :mohammad ahmed 07/05/2023

Quant Time: Jul 04 23:30:27 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 04 00:40:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	8707	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	27484	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.589	164	14675	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.343	188	25505	0.400	ng/ul	0.00
17) Chrysene-d12	21.535	240	15716	0.400	ng/ul	# 0.00
23) Perylene-d12	23.999	264	17816	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.318	96	3476	0.354	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	940	0.022	ng/ul	0.00
18) Fluoranthene-d10	19.368	212	1568	0.026	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.381	178	5551	0.066	ng/ul#	93
19) Fluoranthene	19.401	202	14363	0.171	ng/ul#	95
20) Pyrene	19.763	202	12812	0.147	ng/ul	99
21) Benzo(a)anthracene	21.517	228	7659	0.118	ng/ul#	79
22) Chrysene	21.573	228	7200	0.107	ng/ul#	83
24) Benzo(b)fluoranthene	23.247	252	13787m	0.181	ng/ul	
25) Benzo(k)fluoranthene	23.288	252	4326m	0.057	ng/ul	
26) Benzo(a)pyrene	23.891	252	8141	0.123	ng/ul#	60
27) Indeno(1,2,3-cd)pyrene	26.588	276	7504	0.104	ng/ul#	92
28) Dibenzo(a,h)anthracene	26.598	278	1883	0.034	ng/ul#	1
29) Benzo(g,h,i)perylene	27.383	276	7340	0.114	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070223\
Data File : BN026262.D
Acq On : 04 Jul 2023 14:22
Operator : MA/JU
Sample : 03247-07DL 5X
Misc :
ALS Vial : 119 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCGL3DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2023
Supervised By :mohammad ahmed 07/05/2023


Quant Time: Jul 04 23:30:27 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 04 00:40:07 2023
Response via : Initial Calibration

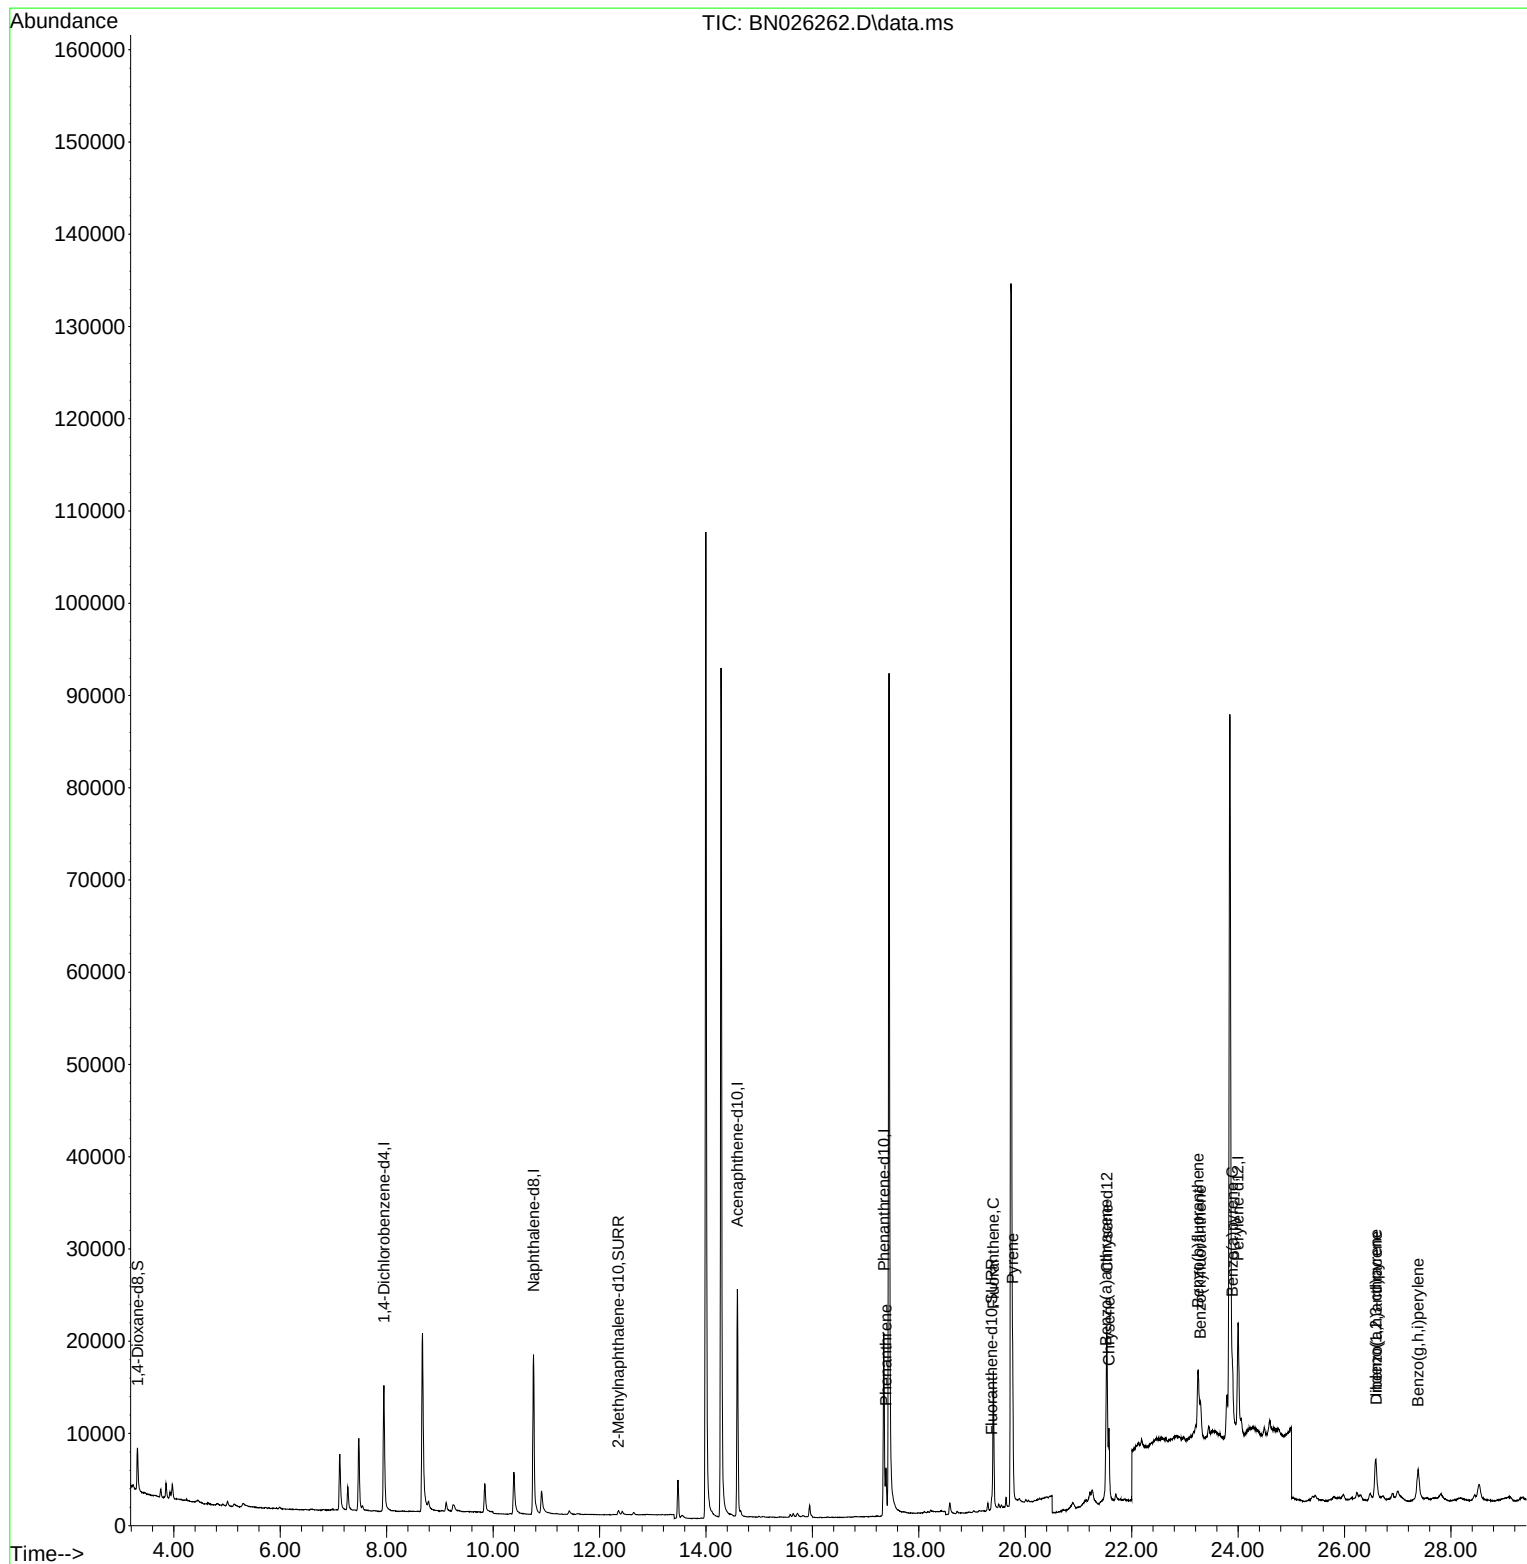

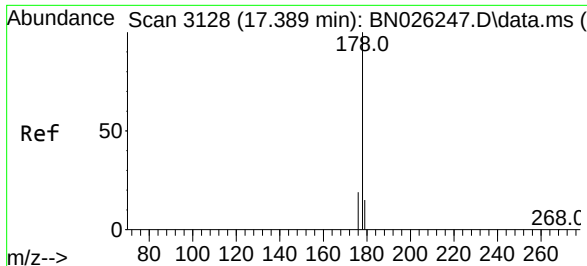

#15
Phenanthrene
Concen: 0.066 ng/ul
RT: 17.381 min Scan# 3126
Delta R.T. -0.008 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22




Instrument :
BNA_N
ClientSampleId :
DCGL3DL

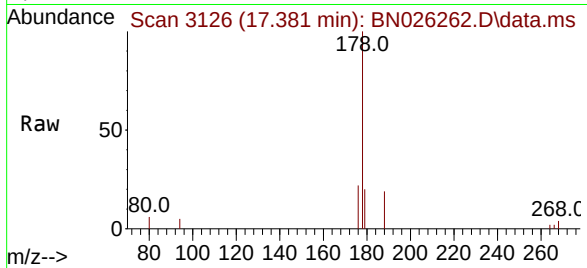

Tgt Ion:178 Resp: 555
Ion Ratio Lower Upper
178 100
179 19.8 12.6 19.0
176 22.3 15.8 23.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/05/2023
Supervised By :mohammad ahmed 07/05/2023

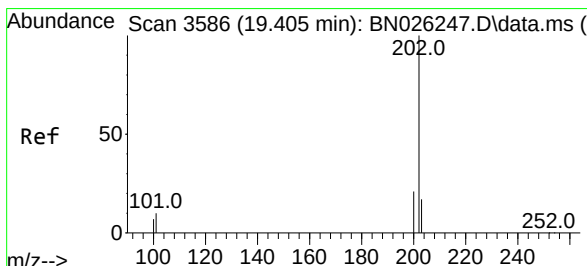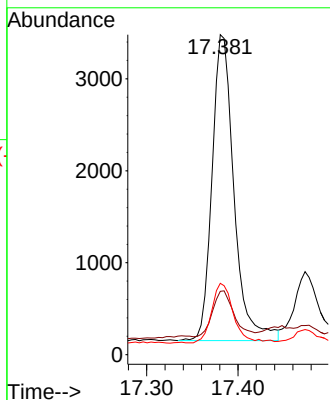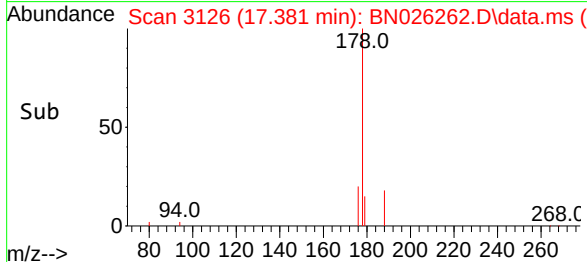

#19
Fluoranthene
Concen: 0.171 ng/ul
RT: 19.401 min Scan# 3585
Delta R.T. -0.005 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22


Tgt Ion:202 Resp: 14363
Ion Ratio Lower Upper
202 100
101 14.5 9.5 14.3
100 10.1 7.3 10.9

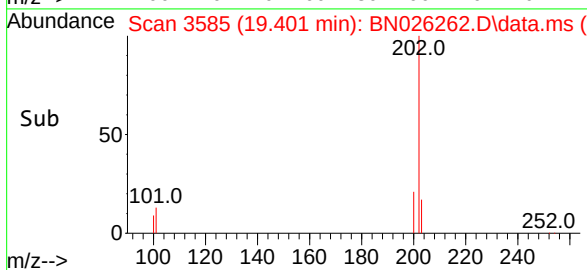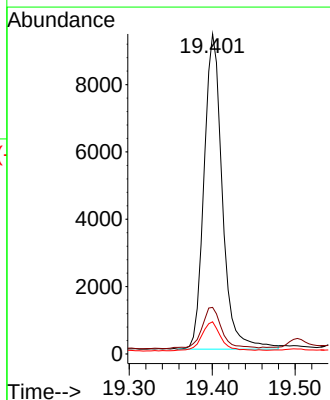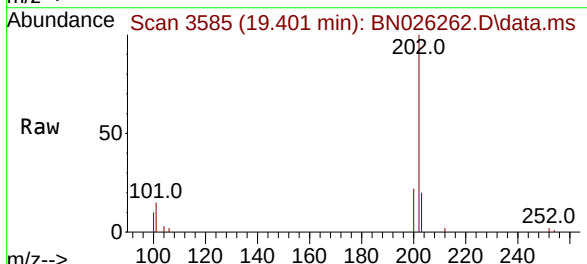



#20
Pyrene
Concen: 0.147 ng/ul
RT: 19.763 min Scan# 3663
Delta R.T. -0.009 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22




Instrument :
BNA_N
ClientSampleId :
DCGL3DL




Tgt Ion:202 Resp: 1281
Ion Ratio Lower Upper
202 100
101 14.3 11.4 17.0
100 11.9 9.1 13.7

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :mohammad ahmed 07/05/2023

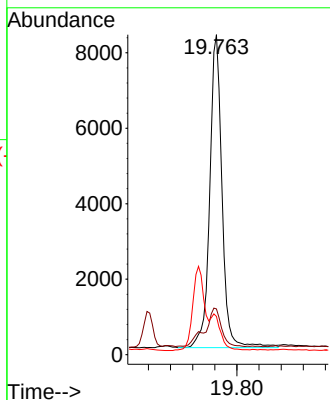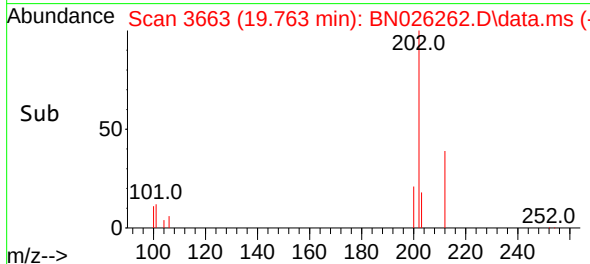


#21
Benzo(a)anthracene
Concen: 0.118 ng/ul
RT: 21.517 min Scan# 4169
Delta R.T. -0.006 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22

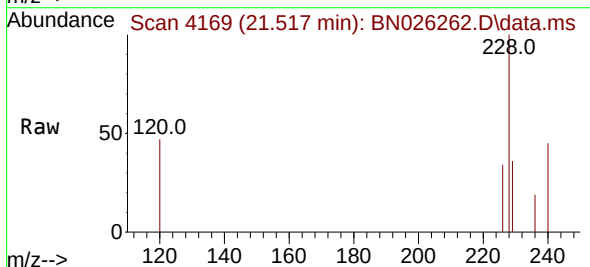


Tgt Ion:228 Resp: 7659
Ion Ratio Lower Upper
228 100
229 36.1 15.8 23.6#
226 33.8 22.5 33.7#

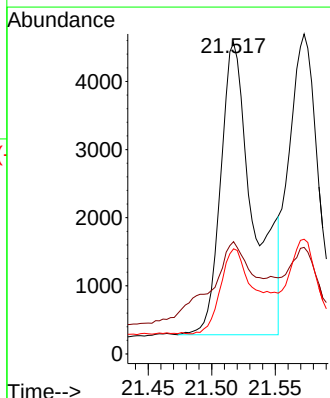

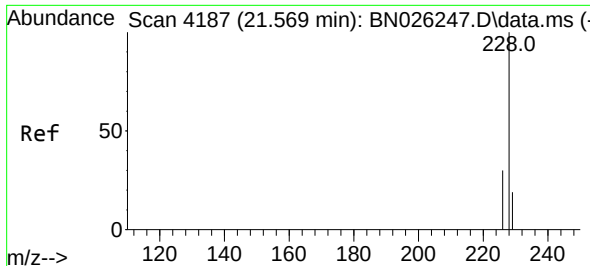

#22
Chrysene
Concen: 0.107 ng/ul
RT: 21.573 min Scan# 4187
Delta R.T. -0.006 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22




Instrument :
BNA_N
ClientSampleId :
DCGL3DL




Tgt Ion:228 Resp: 7200
Ion Ratio Lower Upper
228 100
226 35.8 24.8 37.2
229 33.3 15.7 23.5

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/05/2023
Supervised By :mohammad ahmed 07/05/2023

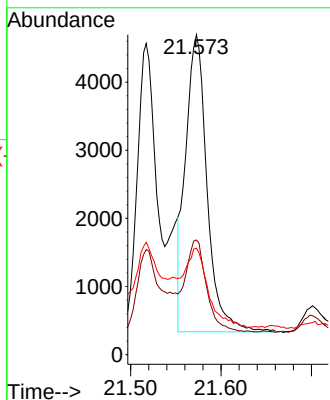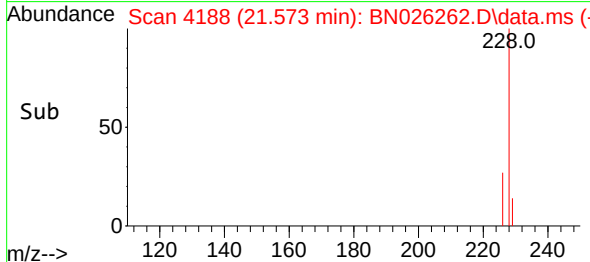


#24
Benzo(b)fluoranthene
Concen: 0.181 ng/ul m
RT: 23.247 min Scan# 4761
Delta R.T. -0.006 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22

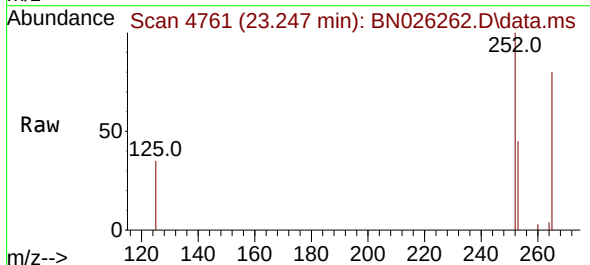


Tgt Ion:252 Resp: 13787
Ion Ratio Lower Upper
252 100
253 45.0 0.0 55.6
125 35.3 0.0 35.8

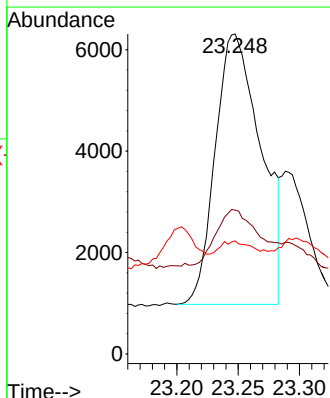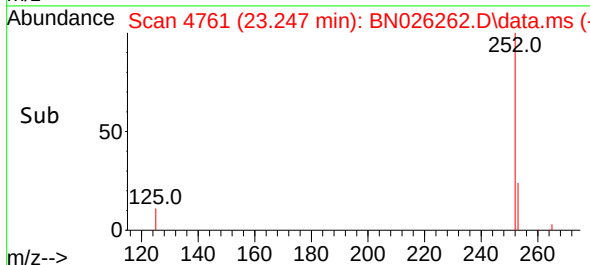



#25
Benzo(k)fluoranthene
Concen: 0.057 ng/ul m
RT: 23.288 min Scan# 4775
Delta R.T. -0.015 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22




Instrument :
BNA_N
ClientSampleId :
DCGL3DL



Tgt Ion:252 Resp: 4320
Ion Ratio Lower Upper
252 100
253 61.2 23.2 34.8#
125 61.3 15.0 22.4#




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/05/2023
Supervised By :mohammad ahmed 07/05/2023

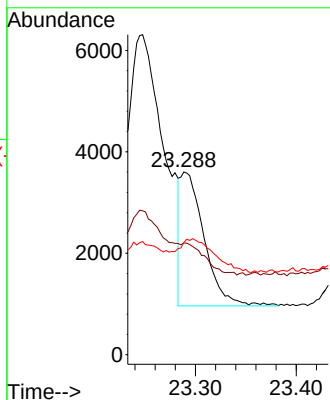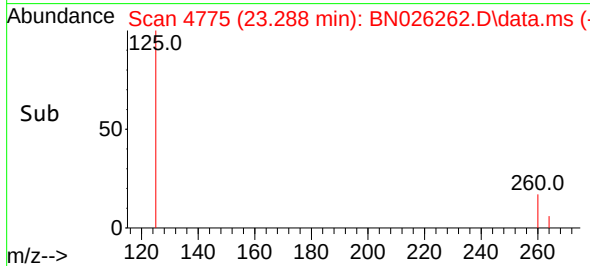

#26
Benzo(a)pyrene
Concen: 0.123 ng/ul
RT: 23.891 min Scan# 4981
Delta R.T. -0.003 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22

Tgt Ion:252 Resp: 8141
Ion Ratio Lower Upper
252 100
253 52.5 26.0 39.0#
125 44.2 17.3 25.9#

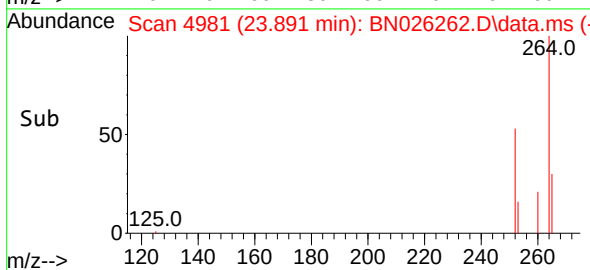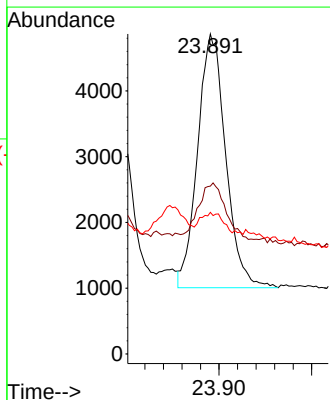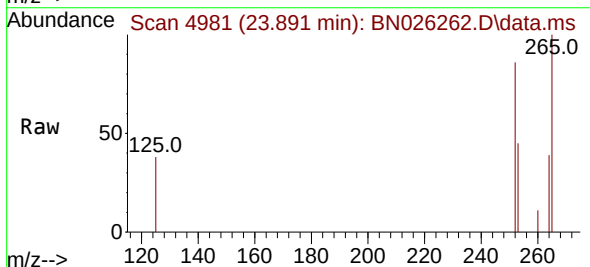

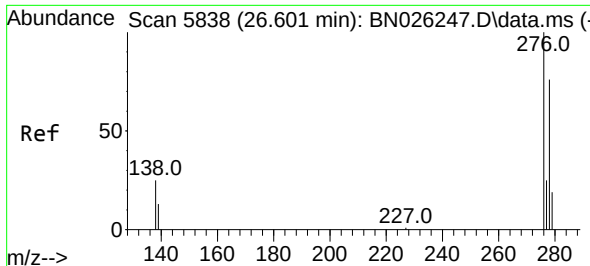


#27
Indeno(1,2,3-cd)pyrene
Concen: 0.104 ng/ul
RT: 26.588 min Scan# 5834
Delta R.T. -0.000 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22

Instrument :

BNA_N

ClientSampleId :

DCGL3DL






Tgt Ion:276 Resp: 7504
Ion Ratio Lower Upper
276 100
138 26.2 24.5 36.7
227 6.1 0.0 0.0

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/05/2023



Supervised By :mohammad ahmed 07/05/2023

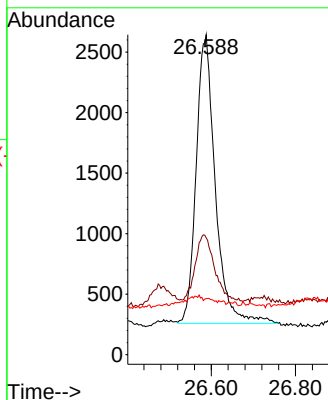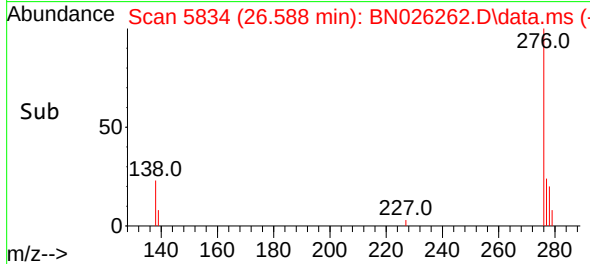


#28
Dibenzo(a,h)anthracene
Concen: 0.034 ng/ul
RT: 26.598 min Scan# 5837
Delta R.T. -0.010 min
Lab File: BN026262.D
Acq: 04 Jul 2023 14:22

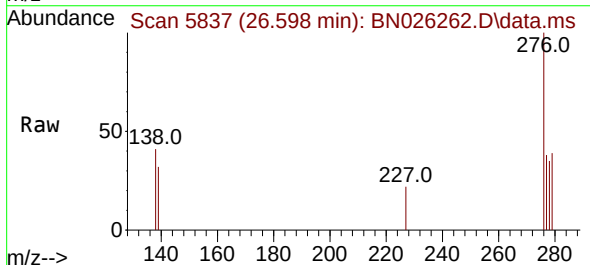


Tgt Ion:278 Resp: 1883
Ion Ratio Lower Upper
278 100
139 92.8 19.0 28.4#
279 113.6 26.7 40.1#

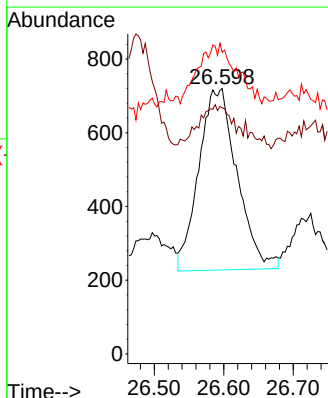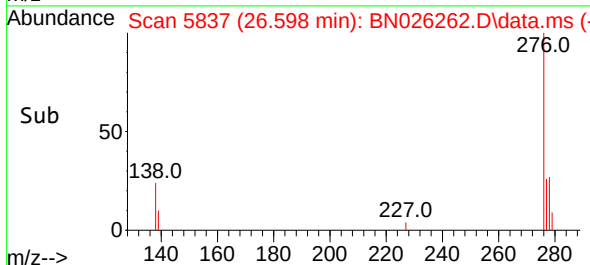

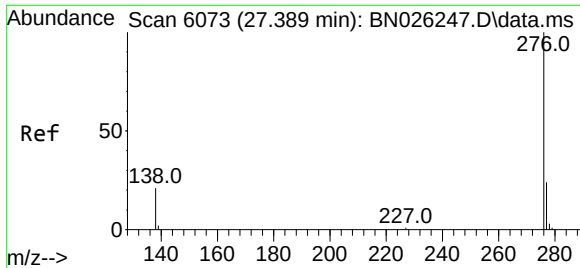

#29
 Benzo(g,h,i)perylene
 Concen: 0.114 ng/ul
 RT: 27.383 min Scan# 6071
 Delta R.T. -0.003 min
 Lab File: BN026262.D
 Acq: 04 Jul 2023 14:22

Instrument :
 BNA_N
 ClientSampleId :
 DCGL3DL

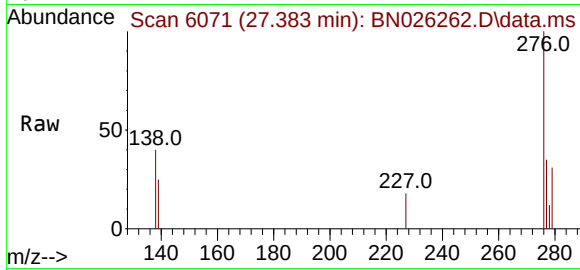

Tgt Ion:276 Resp: 7340
 Ion Ratio Lower Upper
 276 100
 138 39.7 23.4 35.0
 277 35.3 20.0 30.0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/05/2023
 Supervised By :mohammad ahmed 07/05/2023

