

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
 Data File : BN032475.D
 Acq On : 04 Jul 2024 15:45
 Operator : MA/JU
 Sample : PB161807BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK807

Quant Time: Jul 04 23:06:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.595	152	9044	0.400	ng/ul	0.00
4) Naphthalene-d8	10.371	136	27398	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.244	164	14767	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.096	188	1497538	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.21
23) Perylene-d12	23.427	264	28867	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	49669	4.941	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.977	152	10500	0.256	ng/ul	0.00
18) Fluoranthene-d10	19.041	212	17443	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.177	88	383	0.033	ng/ul#	31
26) Benzo(a)pyrene	23.287	252	6124	0.070	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032475.D
Acq On : 04 Jul 2024 15:45
Operator : MA/JU
Sample : PB161807BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK807

Quant Time: Jul 04 23:06:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

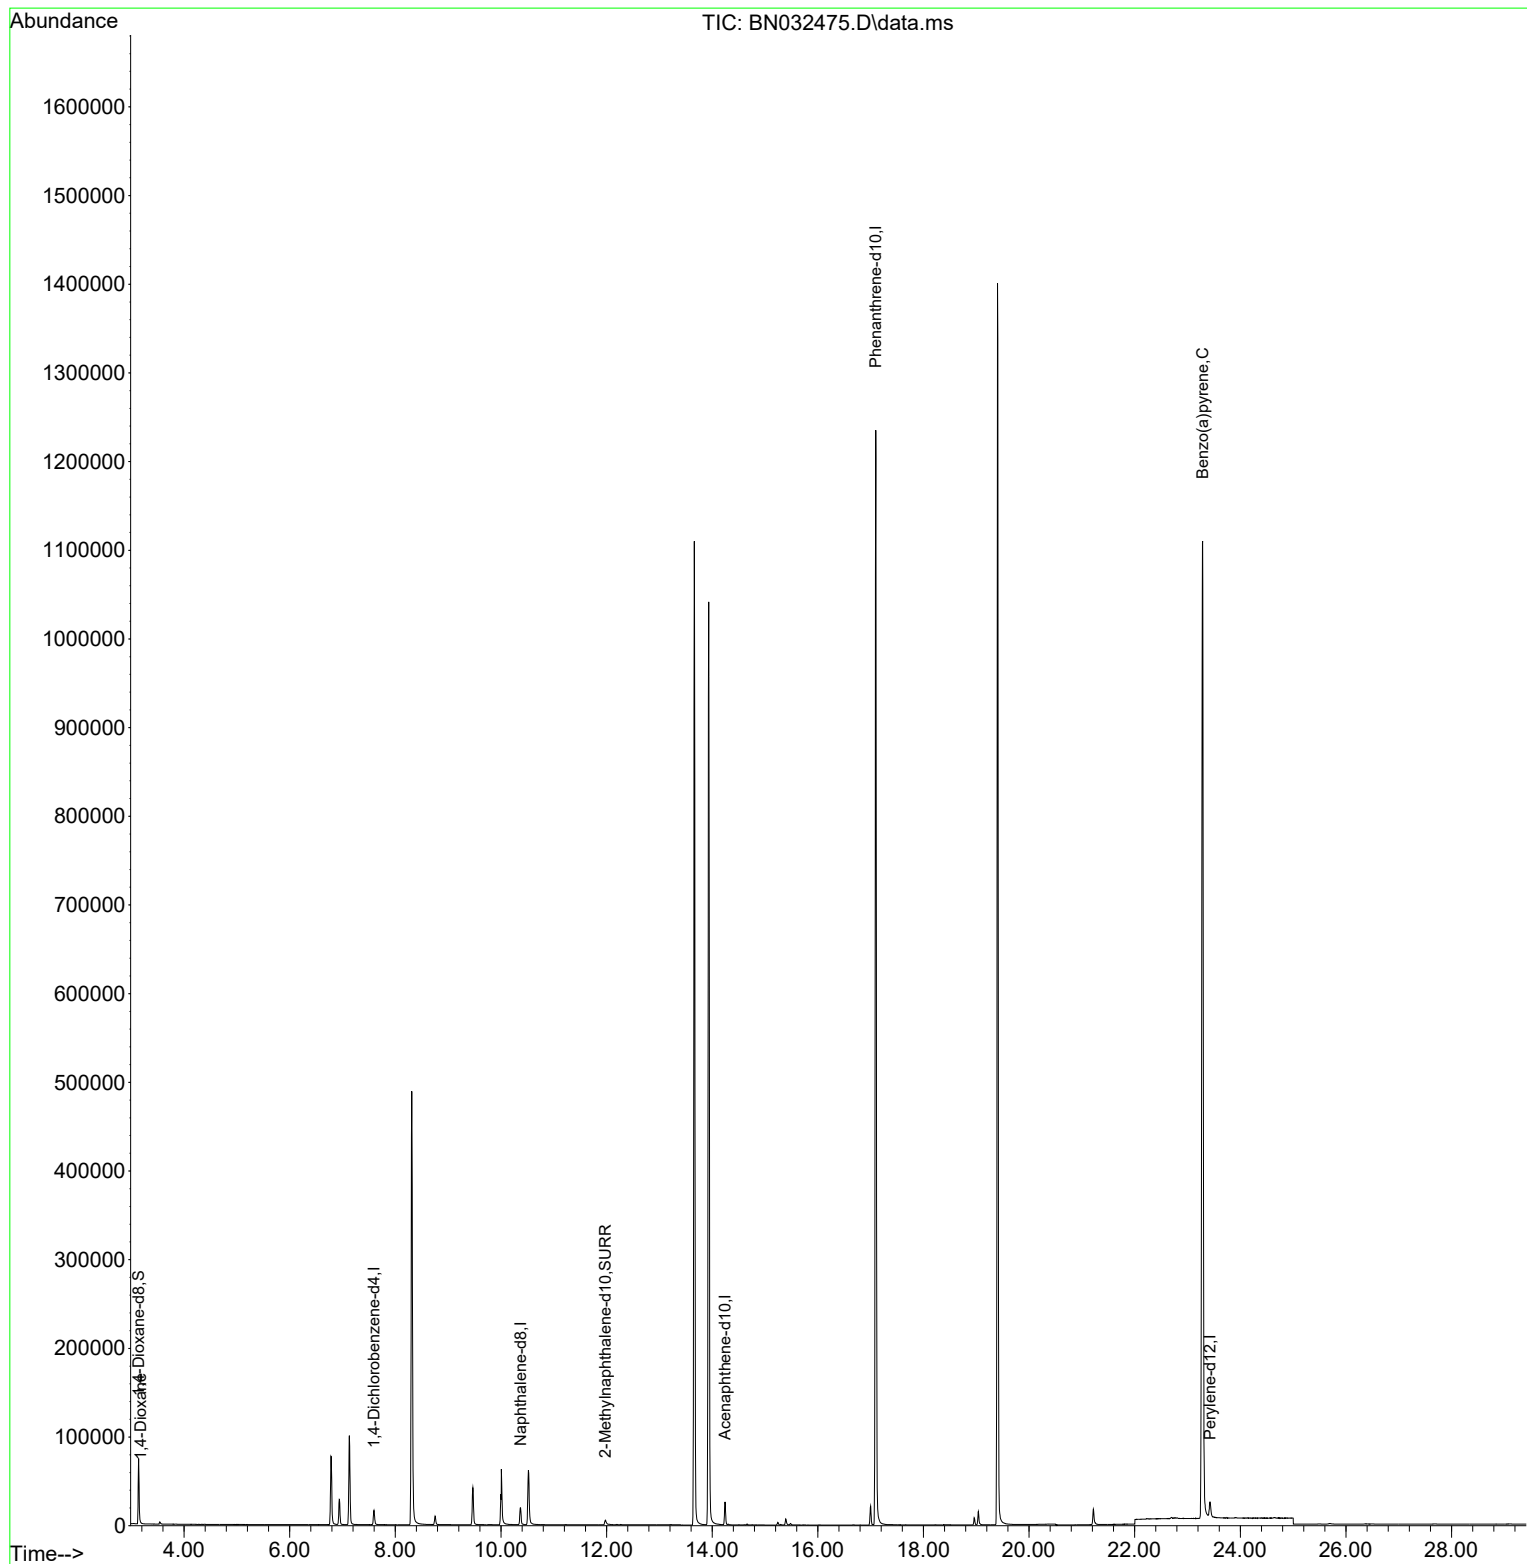

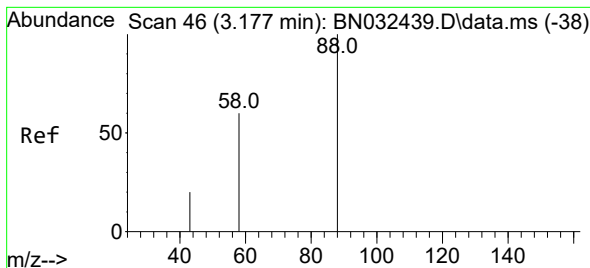

#2

1,4-Dioxane

Concen: 0.033 ng/ul

RT: 3.177 min Scan# 4

Delta R.T. -0.004 min

Lab File: BN032475.D

Acq: 04 Jul 2024 15:45

Instrument :

BNA_N

ClientSampleId :

SBLK807





Tgt Ion: 88 Resp: 383

Ion Ratio Lower Upper

88 100

43 121.1 28.4 42.6#

58 41.6 43.3 64.9#

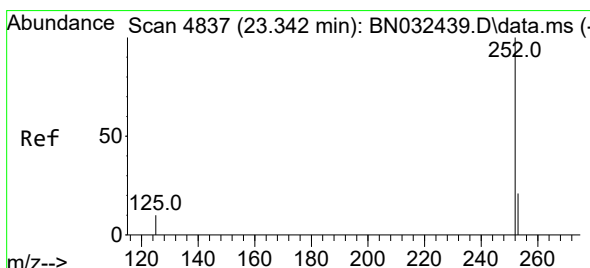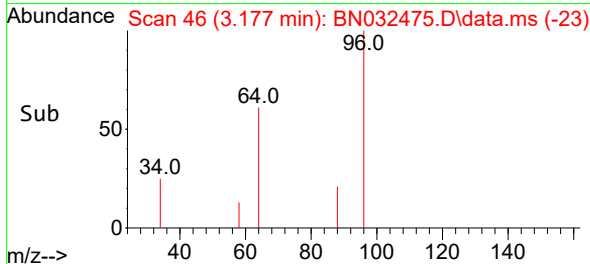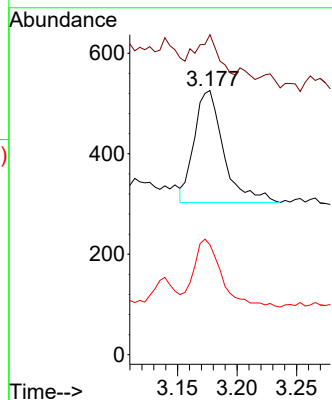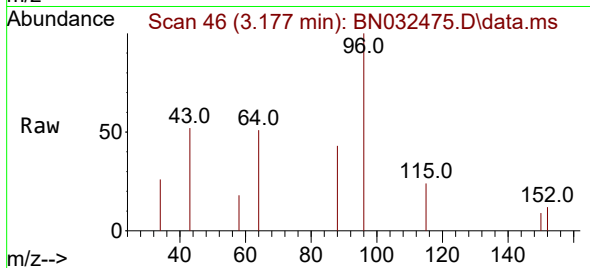

#26

Benzo(a)pyrene

Concen: 0.070 ng/ul

RT: 23.287 min Scan# 4818

Delta R.T. -0.041 min

Lab File: BN032475.D

Acq: 04 Jul 2024 15:45

Tgt Ion: 252 Resp: 6124

Ion Ratio Lower Upper

252 100

253 52.7 22.2 33.2#

125 62.4 16.4 24.6#

