

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
 Data File : BN032486.D
 Acq On : 04 Jul 2024 22:22
 Operator : MA/JU
 Sample : P3065-06
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4CD2

Quant Time: Jul 04 23:08:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.595	152	7417	0.400	ng/ul	0.00
4) Naphthalene-d8	10.371	136	21331	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.244	164	12257	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.101	188	1466278	0.400	ng/ul	0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.21
23) Perylene-d12	23.421	264	29638	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.144	96	27066	3.283	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.971	152	7108	0.222	ng/ul	0.00
18) Fluoranthene-d10	19.041	212	18752	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
10) Acenaphthylene	13.966	152	1279	0.025	ng/ul#	72
24) Benzo(b)fluoranthene	22.760	252	2578	0.020	ng/ul#	1
26) Benzo(a)pyrene	23.281	252	6573	0.073	ng/ul#	11


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032486.D
Acq On : 04 Jul 2024 22:22
Operator : MA/JU
Sample : P3065-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CD2

Quant Time: Jul 04 23:08:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration




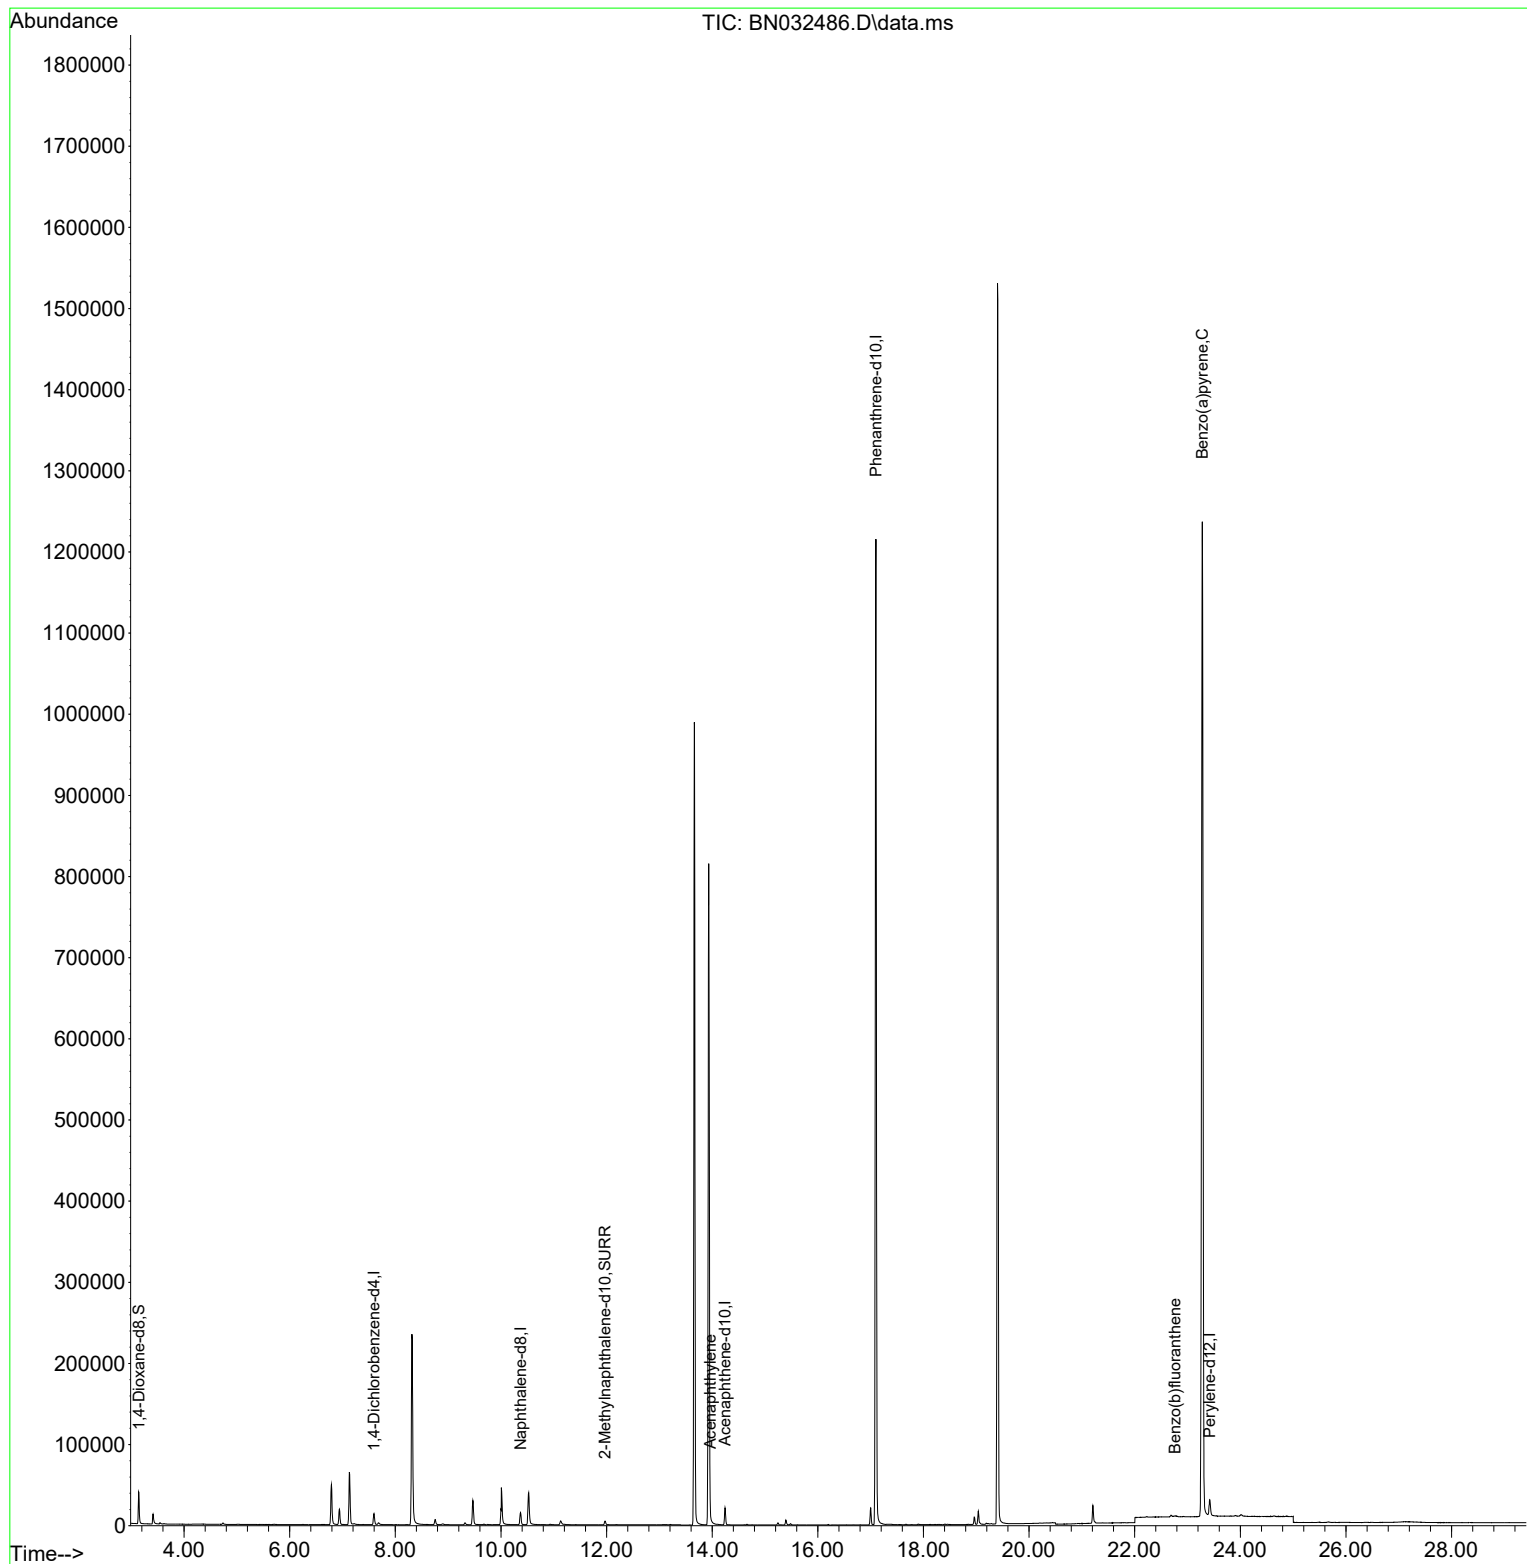


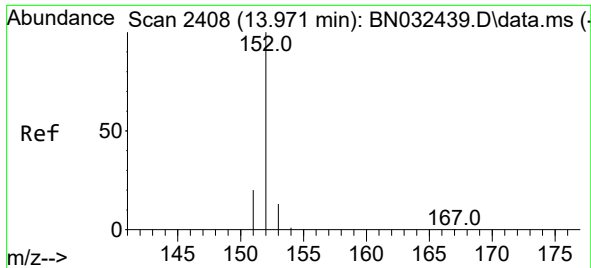

#10
Acenaphthylene
Concen: 0.025 ng/ul
RT: 13.966 min Scan# 2407
Delta R.T. -0.004 min
Lab File: BN032486.D
Acq: 04 Jul 2024 22:22




Instrument :
BNA_N
ClientSampleId :
A4CD2


Tgt Ion:152 Resp: 1279
Ion Ratio Lower Upper
152 100
151 30.8 15.7 23.5#
153 27.1 10.9 16.3#

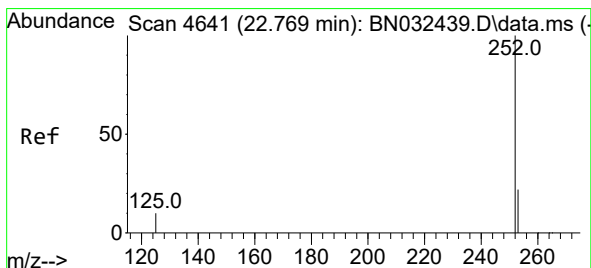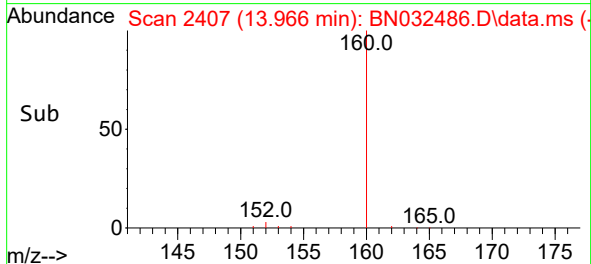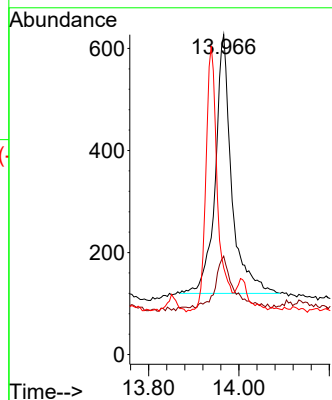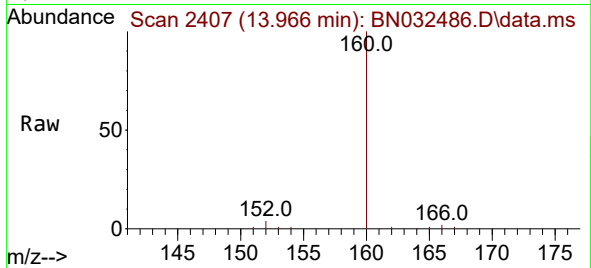

#24
Benzo(b)fluoranthene
Concen: 0.020 ng/ul
RT: 22.760 min Scan# 4638
Delta R.T. 0.003 min
Lab File: BN032486.D
Acq: 04 Jul 2024 22:22


Tgt Ion:252 Resp: 2578
Ion Ratio Lower Upper
252 100
253 95.4 0.0 50.2#
125 150.7 0.0 32.0#

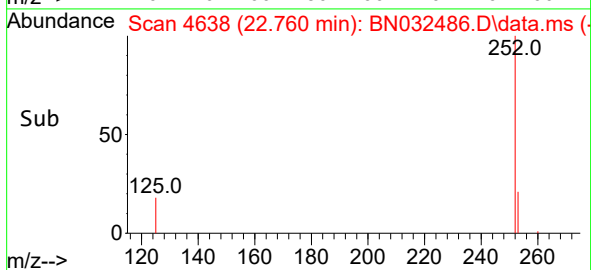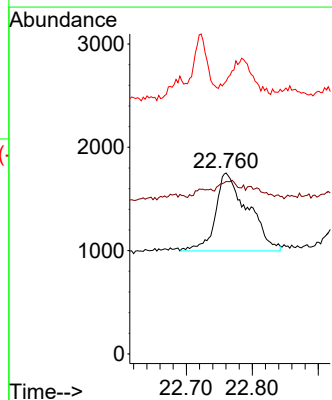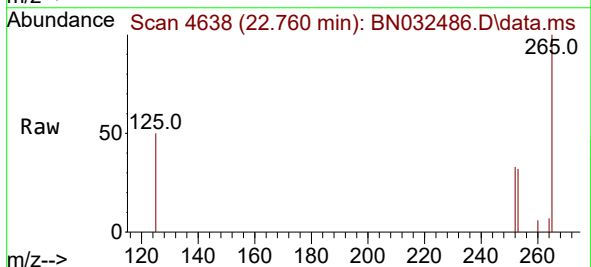

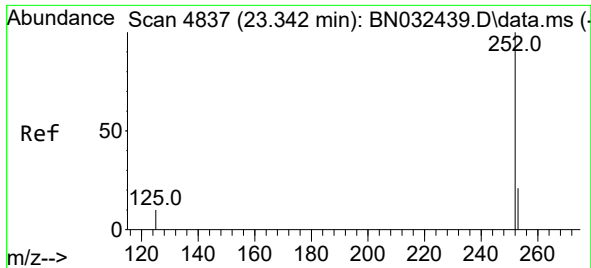

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.281 min Scan# 4816
Delta R.T. -0.047 min
Lab File: BN032486.D
Acq: 04 Jul 2024 22:22

Instrument :
BNA_N
ClientSampleId :
A4CD2

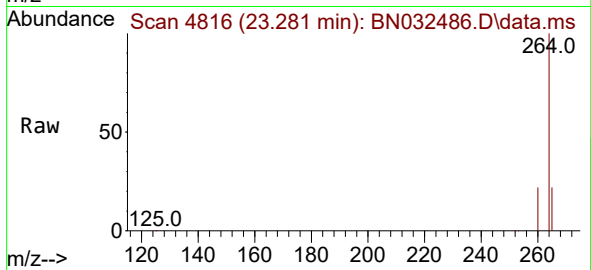

Tgt Ion:252 Resp: 6573
Ion Ratio Lower Upper
252 100
253 58.0 22.2 33.2#
125 81.4 16.4 24.6#

