




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032432.D
Acq On : 03 Jul 2024 11:20
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 03 11:57:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

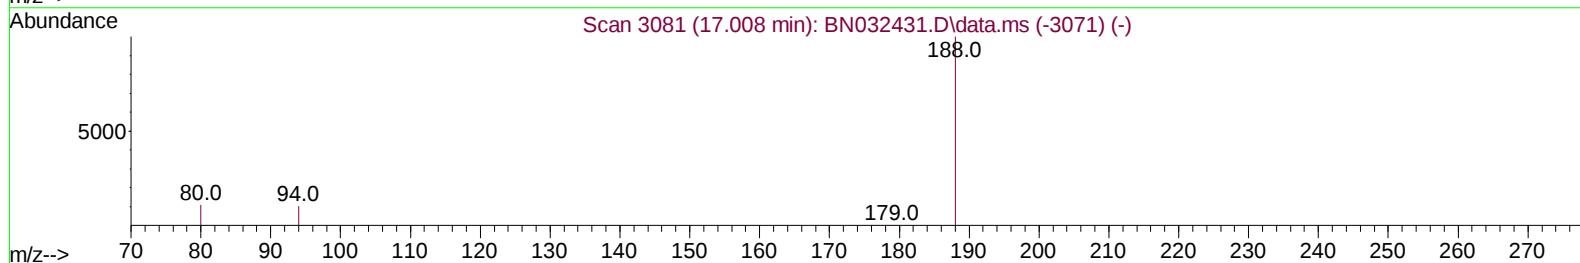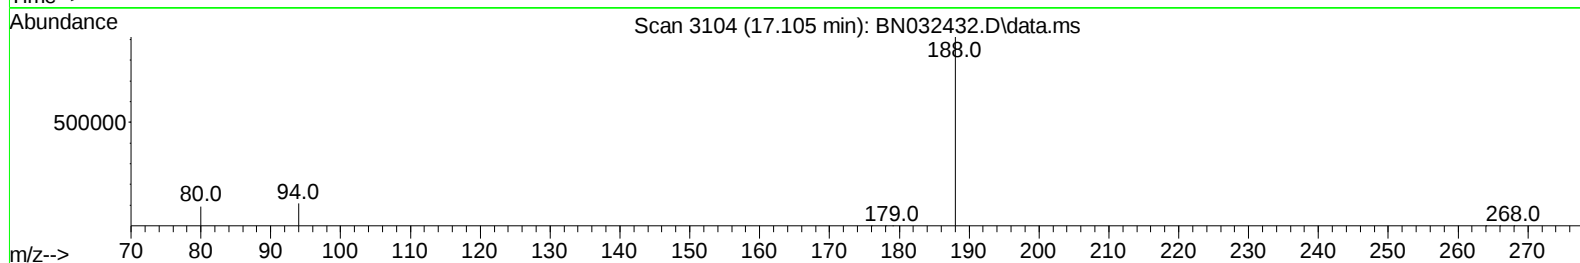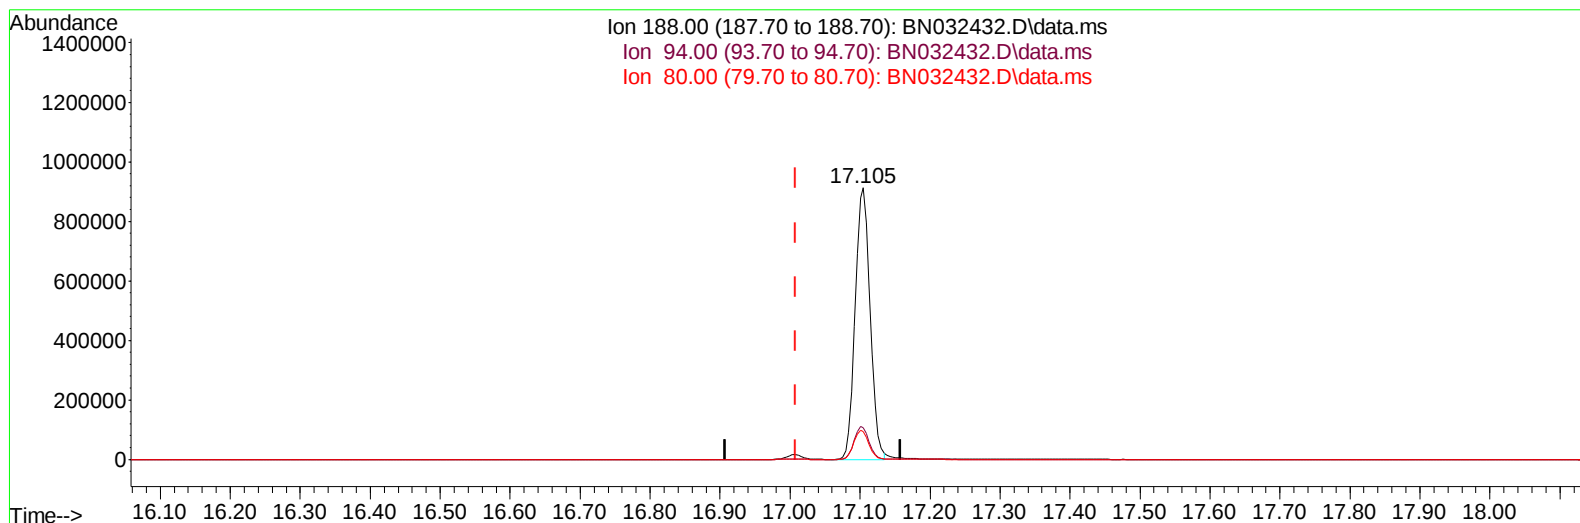

TIC: BN032432.D\data.ms

(13) Phenanthrene-d10 (I)

17.105min (+ 0.097) 0.40 ng/u1

response 1352683

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	11.74
80.00	10.50	10.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032432.D
Acq On : 03 Jul 2024 11:20
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Quant Time: Jul 03 11:57:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

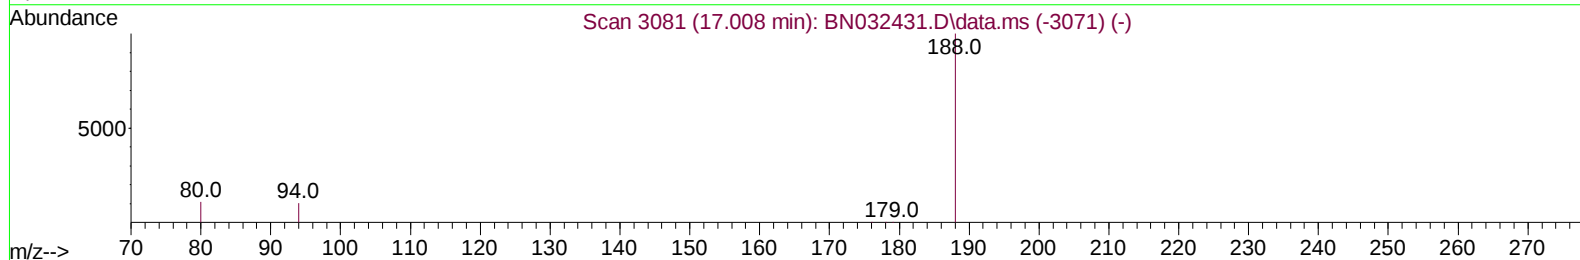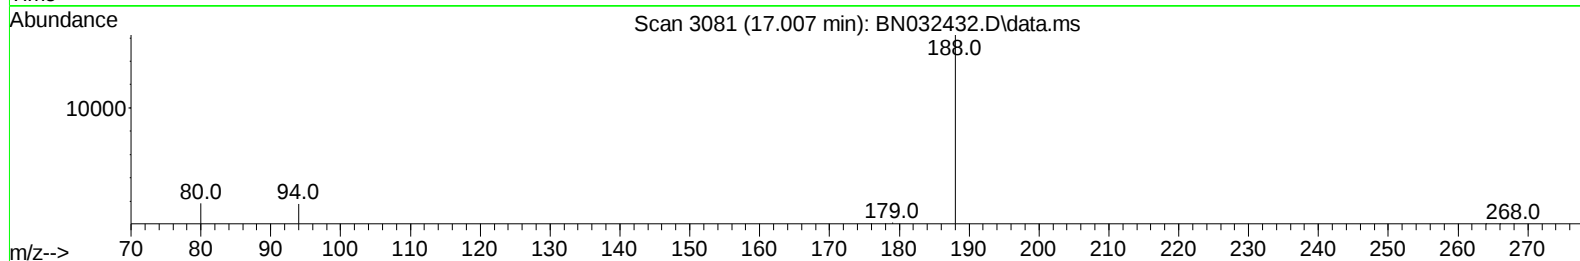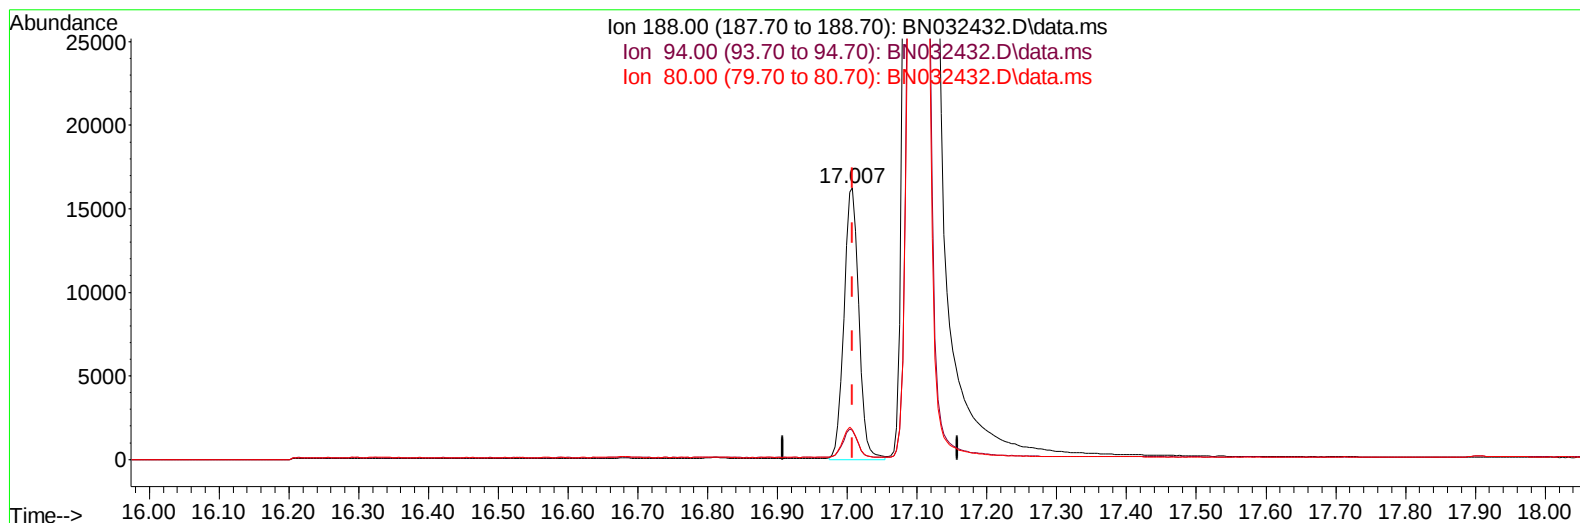

TIC: BN032432.D\data.ms

(13) Phenanthrene-d10 (I)

17.007min (-0.000) 0.40 ng/ul m

response 24048

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	10.73
80.00	10.50	11.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032432.D
Acq On : 03 Jul 2024 11:20
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Quant Time: Jul 03 11:57:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

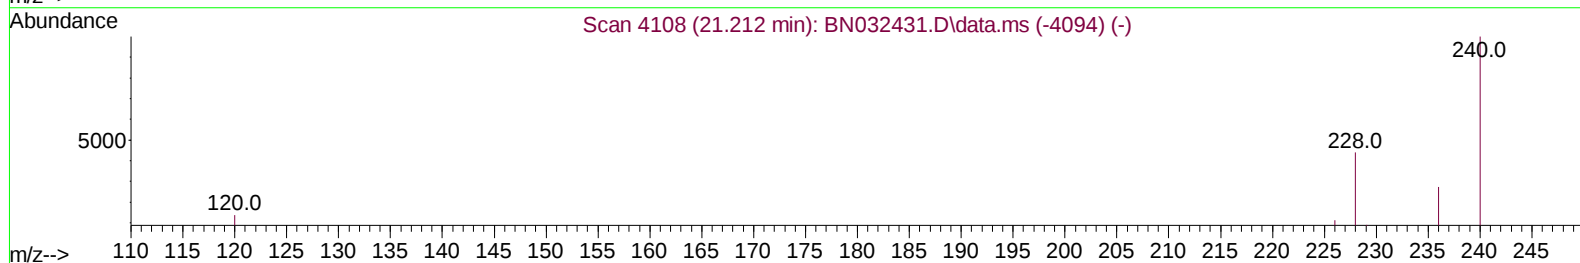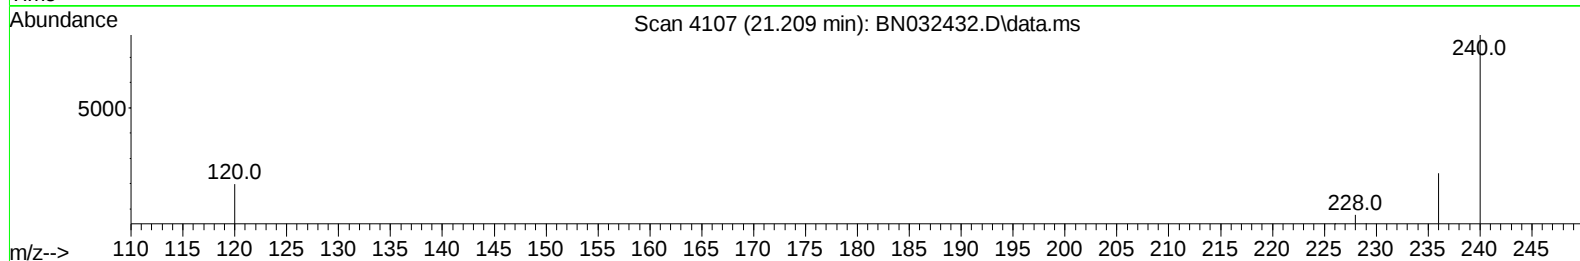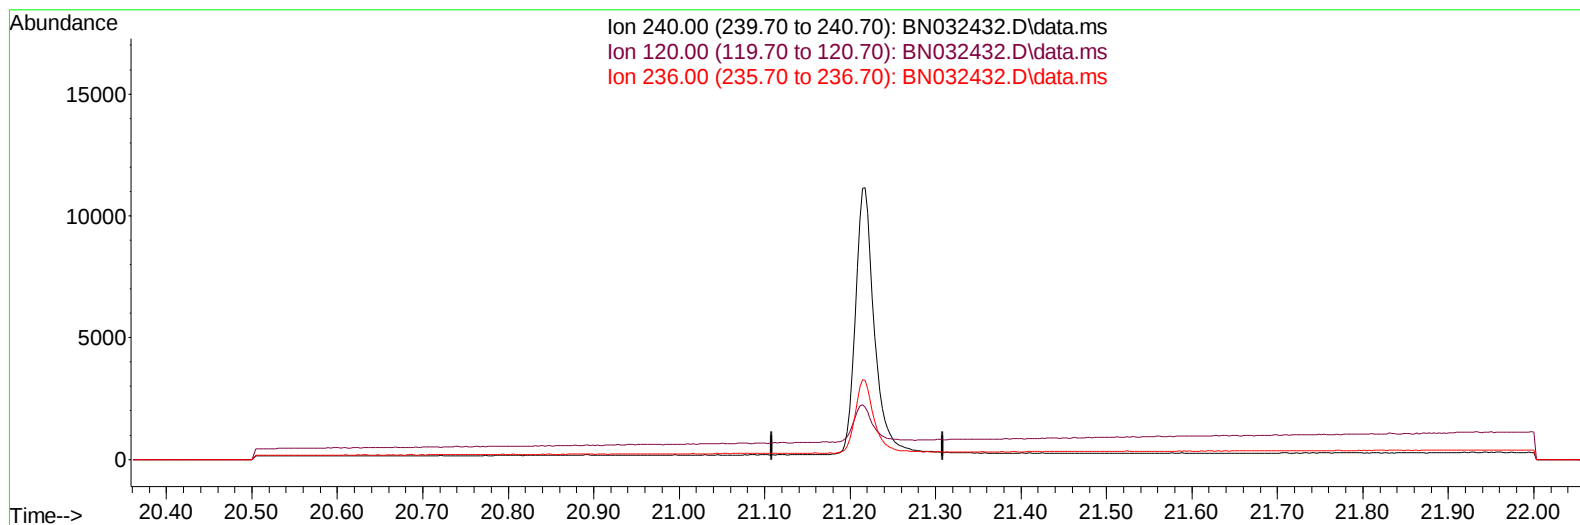

TIC: BN032432.D\data.ms

(17) Chrysene-d12

21.209min (-21.209) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.80	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032432.D
Acq On : 03 Jul 2024 11:20
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 03 11:57:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

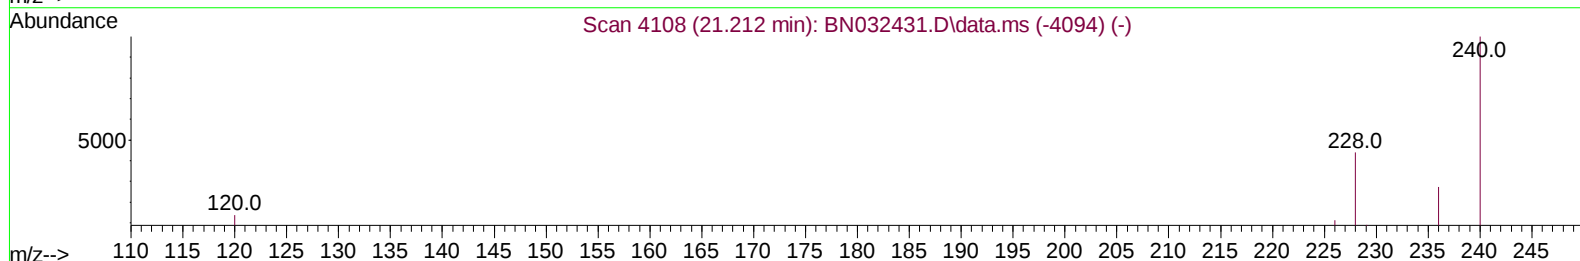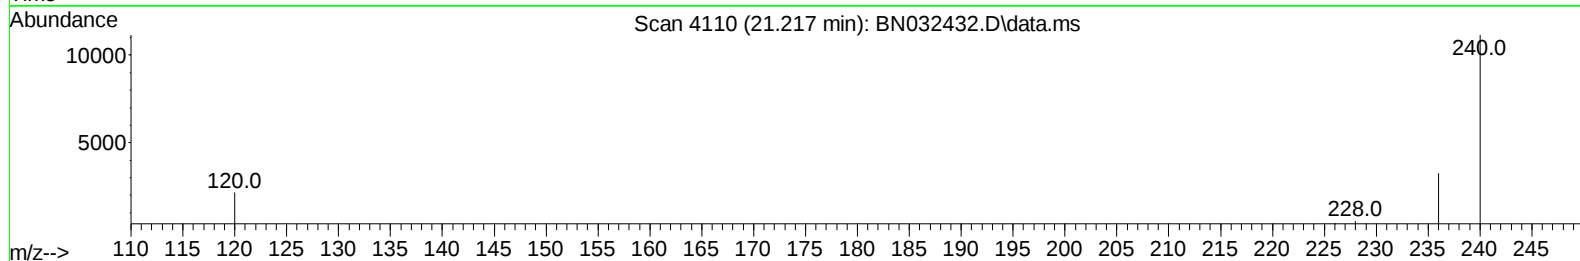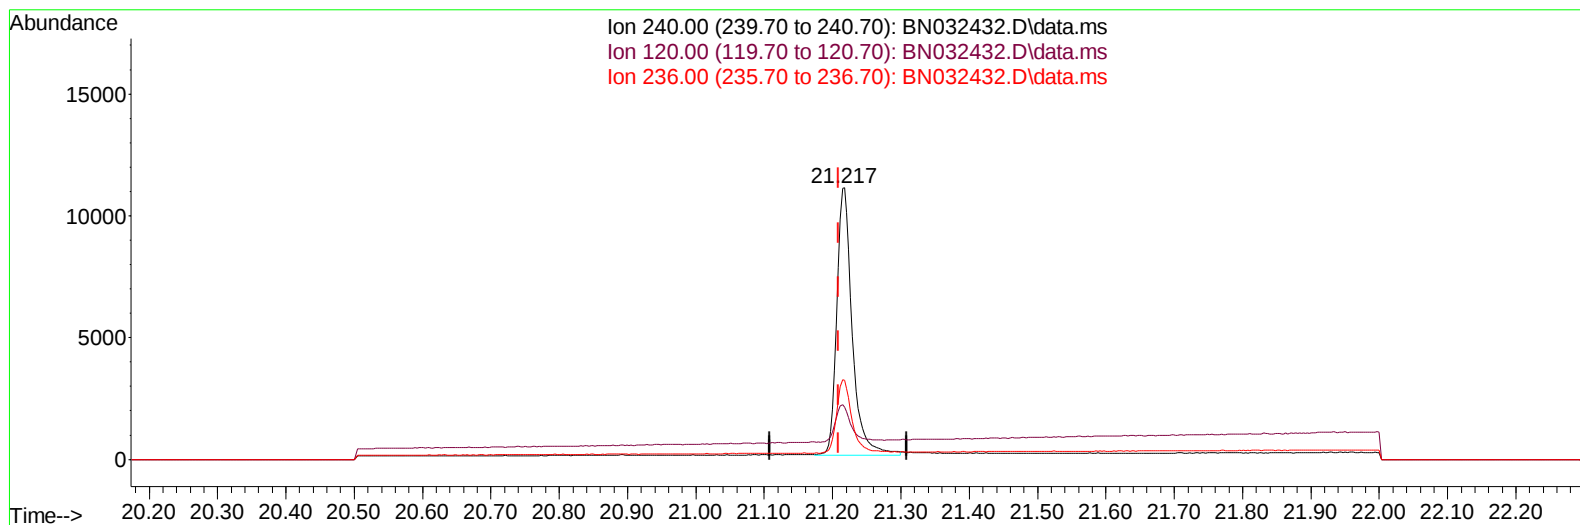

TIC: BN032432.D\data.ms

(17) Chrysene-d12

21.217min (+ 0.009) 0.40 ng/ul m

response 17198

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	19.34
236.00	28.40	29.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032432.D
Acq On : 03 Jul 2024 11:20
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Quant Time: Jul 03 11:57:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

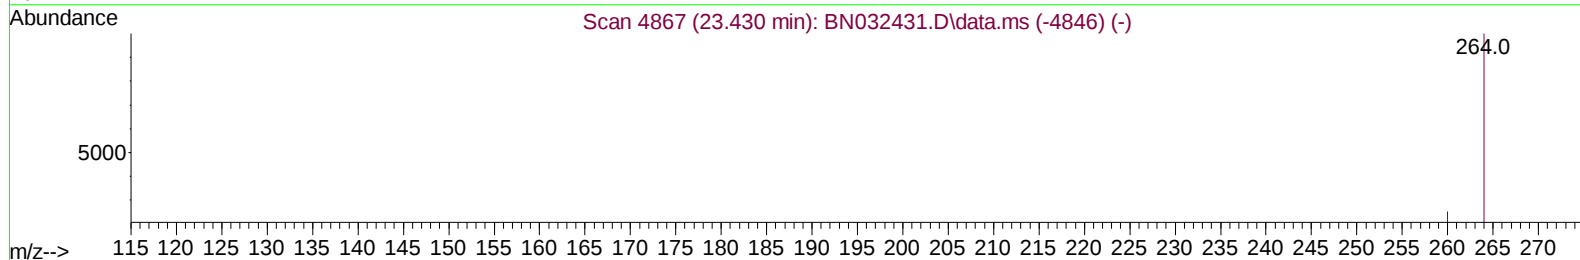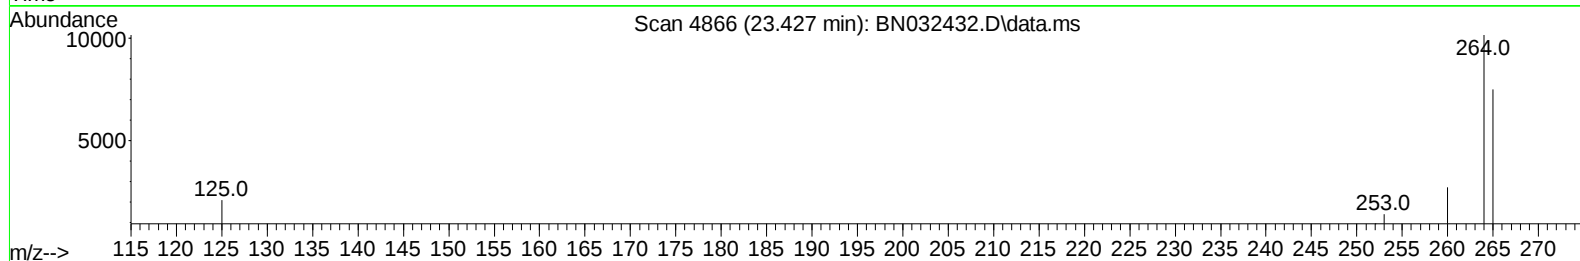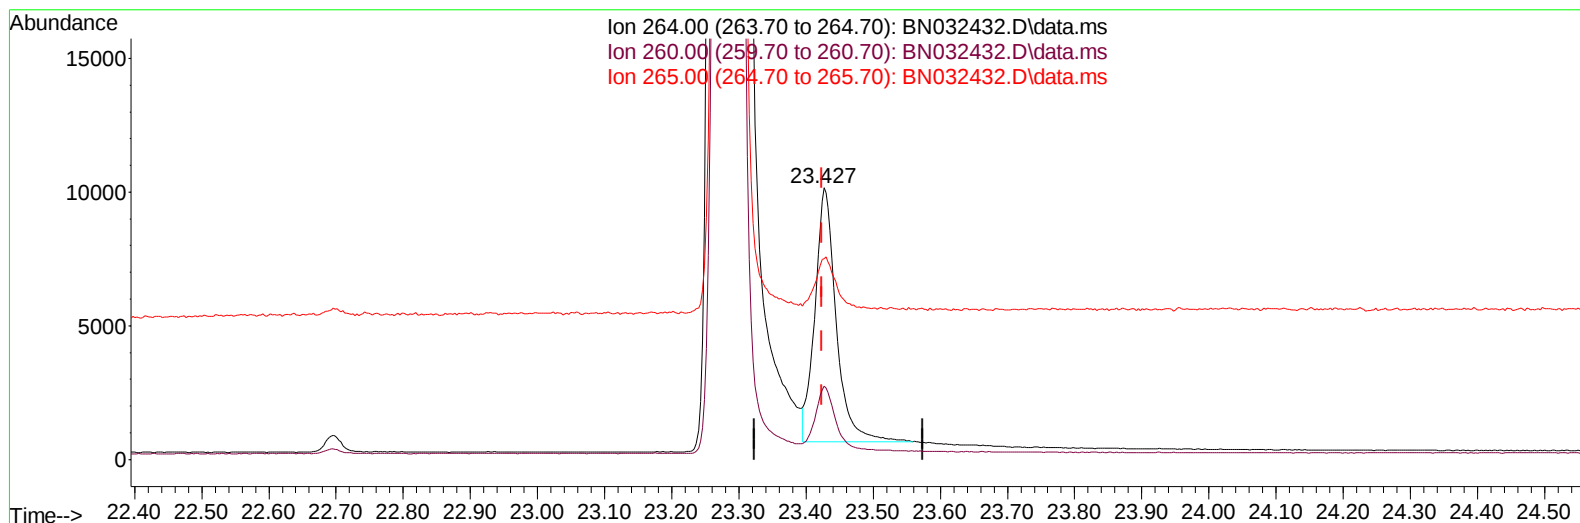

TIC: BN032432.D\data.ms

(23) Perylene-d12 (I)

23.427min (+ 0.003) 0.40 ng/u1

response 20933

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	27.00
265.00	67.20	73.87
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032432.D
Acq On : 03 Jul 2024 11:20
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 03 11:57:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

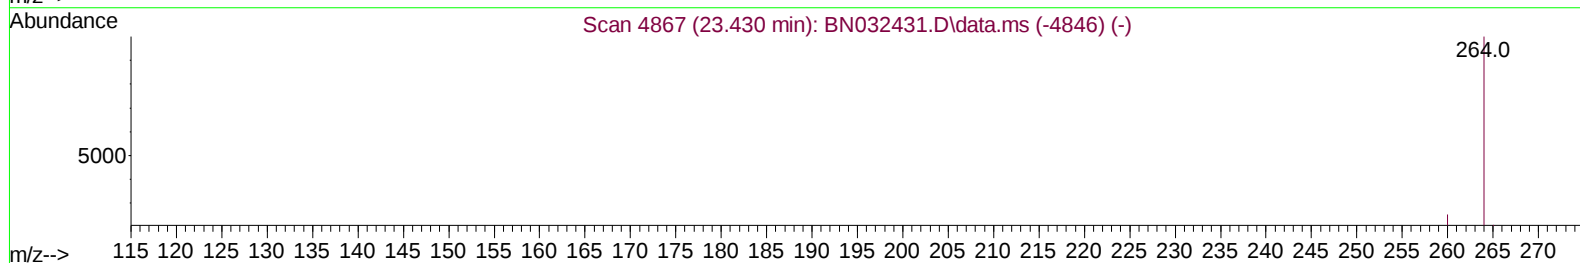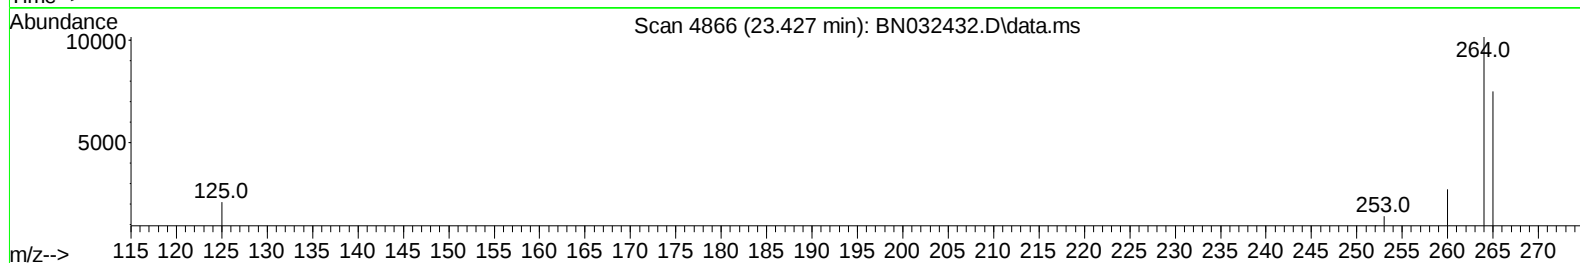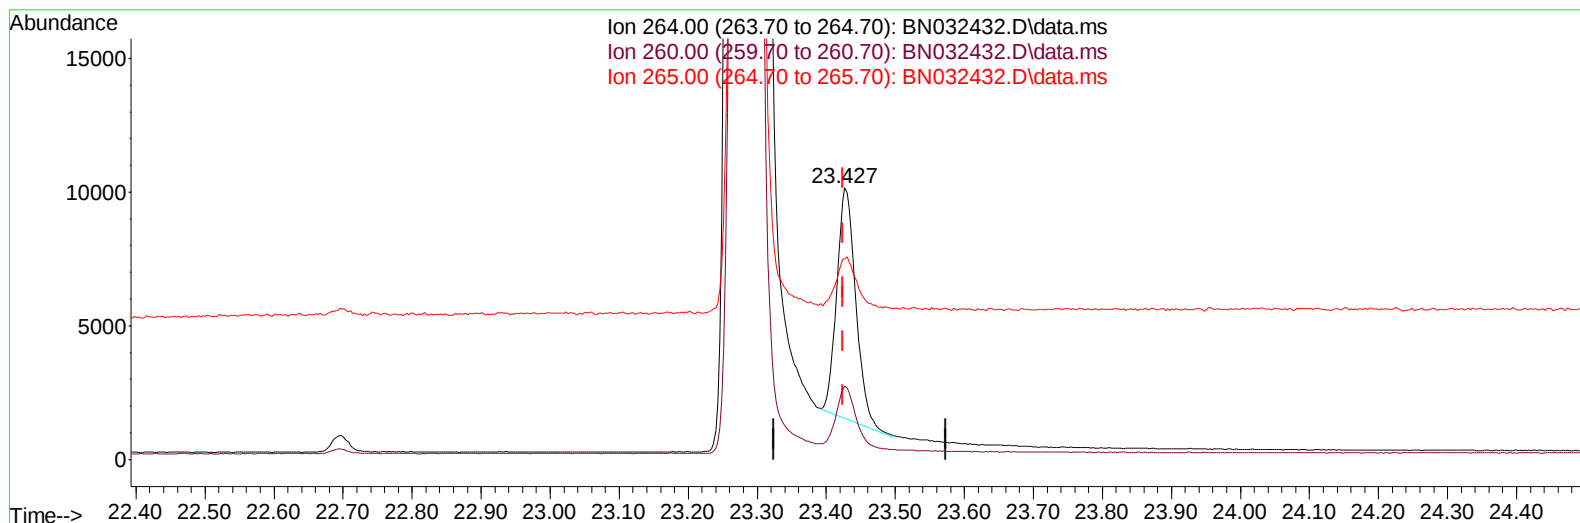

TIC: BN032432.D\data.ms

(23) Perylene-d12 (I)

23.427min (+ 0.003) 0.40 ng/ul m

response 16481

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	27.00
265.00	67.20	73.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
 Data File : BN032432.D
 Acq On : 03 Jul 2024 11:20
 Operator : MA/JU
 Sample : PB161653BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK653

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
 Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 03 11:57:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.603	152	5755	0.400	ng/ul	0.00
4) Naphthalene-d8	10.376	136	18261	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.248	164	11646	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.007	188	24048m	0.400	ng/ul	0.00
17) Chrysene-d12	21.217	240	17198m	0.400	ng/ul	0.00
23) Perylene-d12	23.427	264	16481m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	32821	5.131	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.982	152	7484	0.273	ng/ul	0.00
18) Fluoranthene-d10	19.045	212	16662	0.322	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032432.D
Acq On : 03 Jul 2024 11:20
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Quant Time: Jul 03 11:57:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

