




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032440.D
Acq On : 03 Jul 2024 17:34
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Quant Time: Jul 03 18:01:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

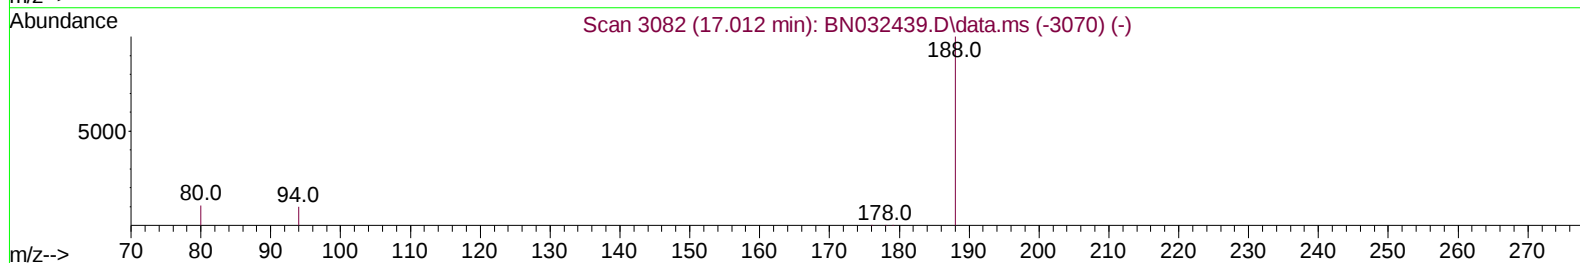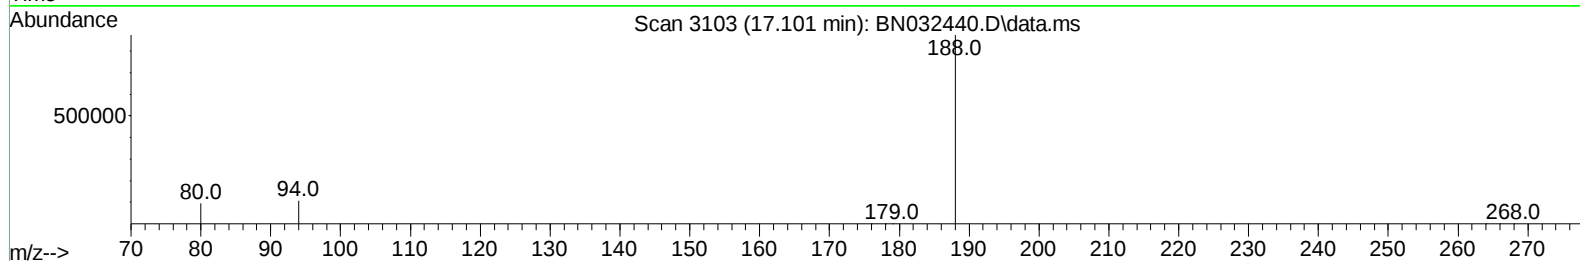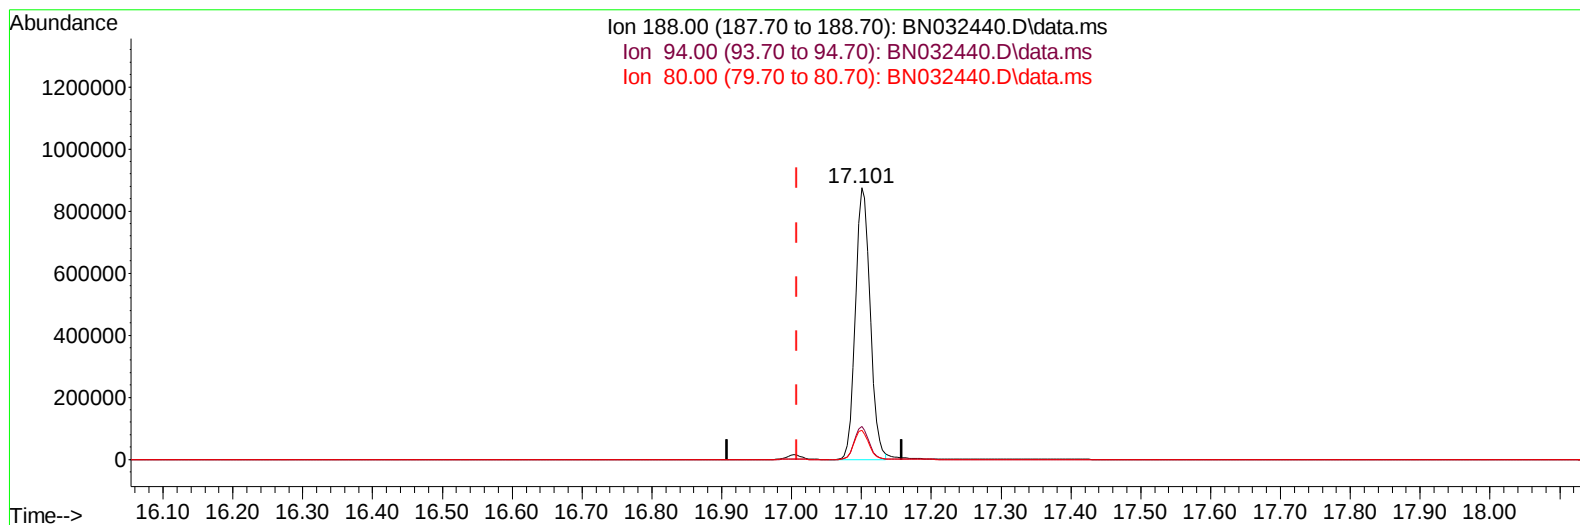

TIC: BN032440.D\data.ms

(13) Phenanthrene-d10 (I)

17.101min (+ 0.093) 0.40 ng/u1

response 1286718

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	12.16
80.00	10.50	10.77
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032440.D
Acq On : 03 Jul 2024 17:34
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Quant Time: Jul 03 18:01:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

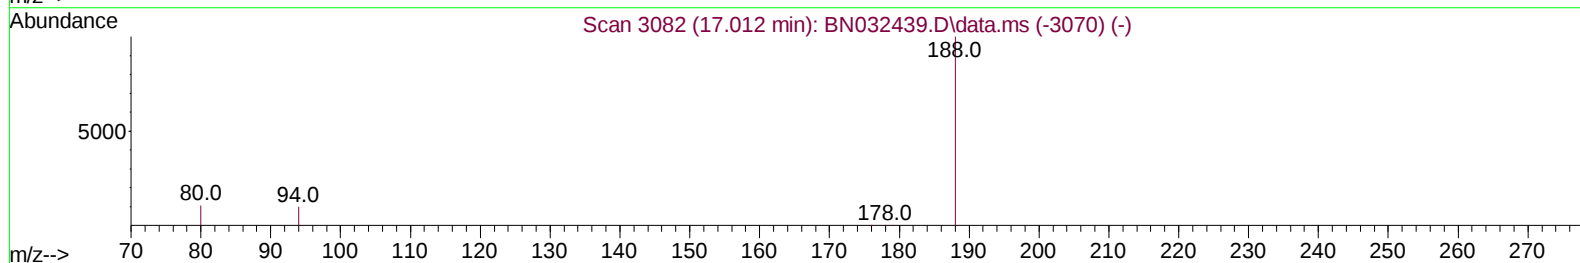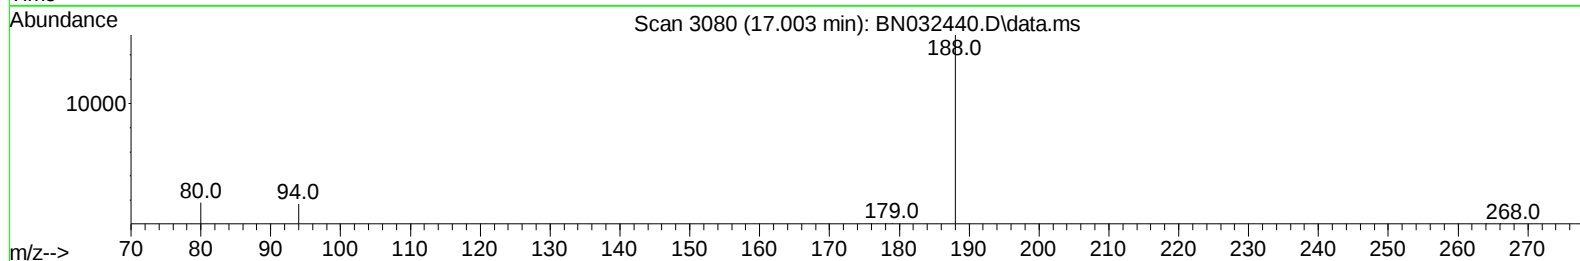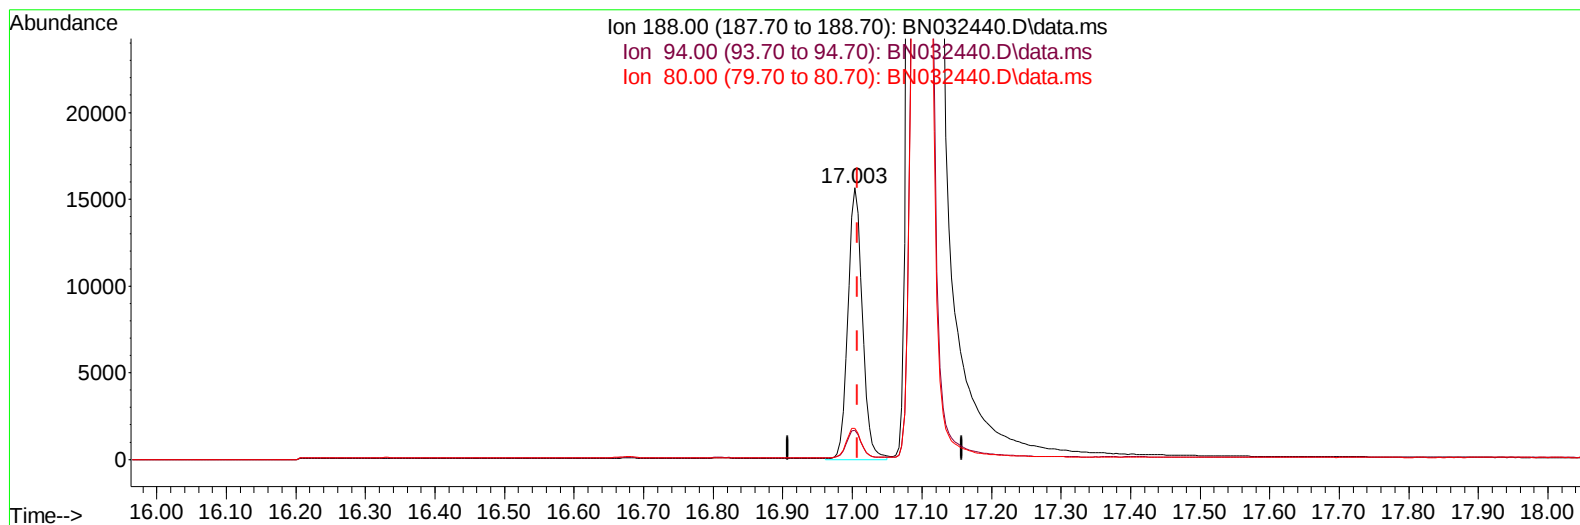

TIC: BN032440.D\data.ms

(13) Phenanthrene-d10 (I)

17.003min (-0.004) 0.40 ng/u1 m

response 22555

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	10.64
80.00	10.50	11.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032440.D
Acq On : 03 Jul 2024 17:34
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Quant Time: Jul 10 02:21:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

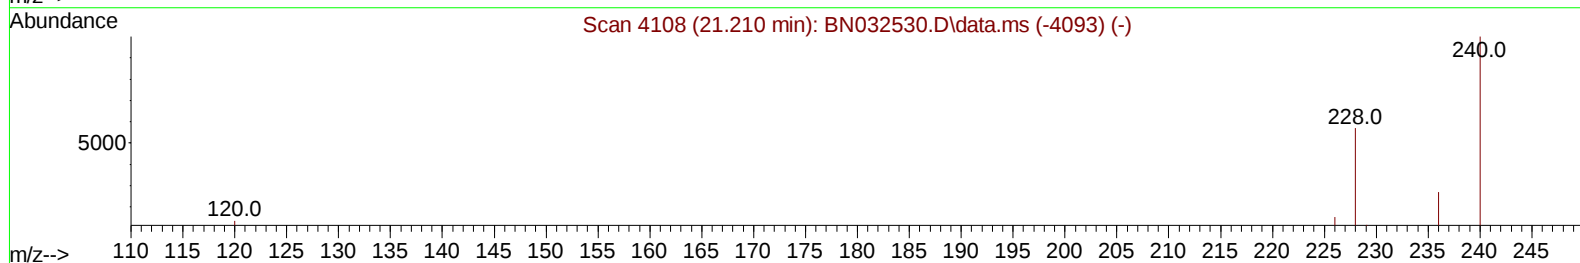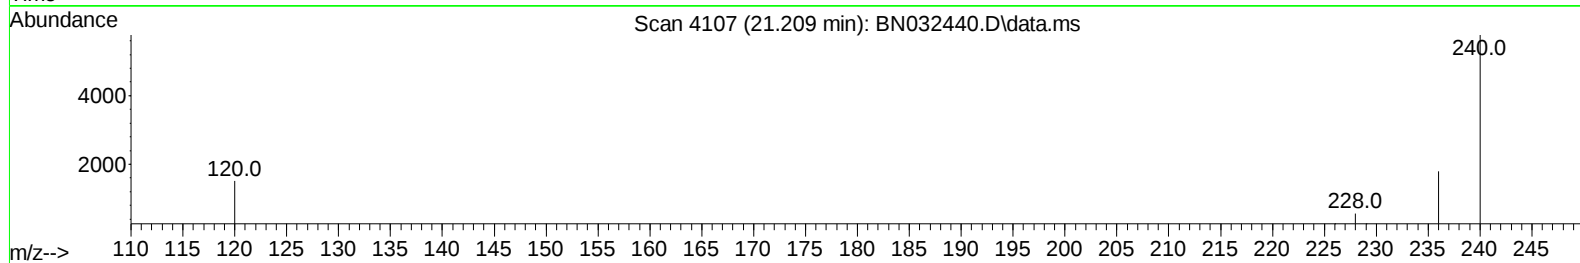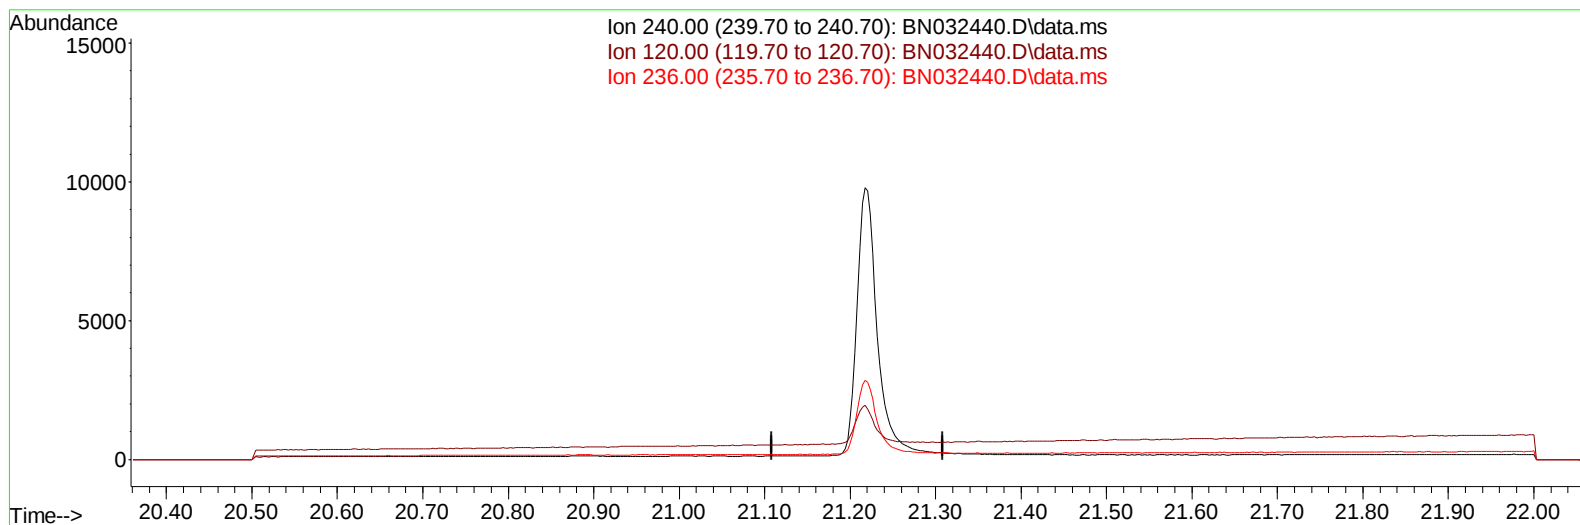

TIC: BN032440.D\data.ms

(17) Chrysene-d12

21.209min (-21.209) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.80	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032440.D
Acq On : 03 Jul 2024 17:34
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 03 18:01:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

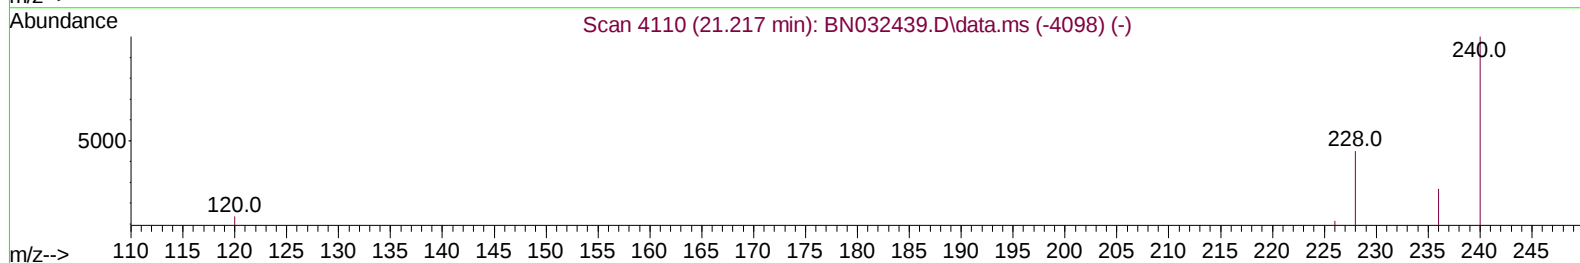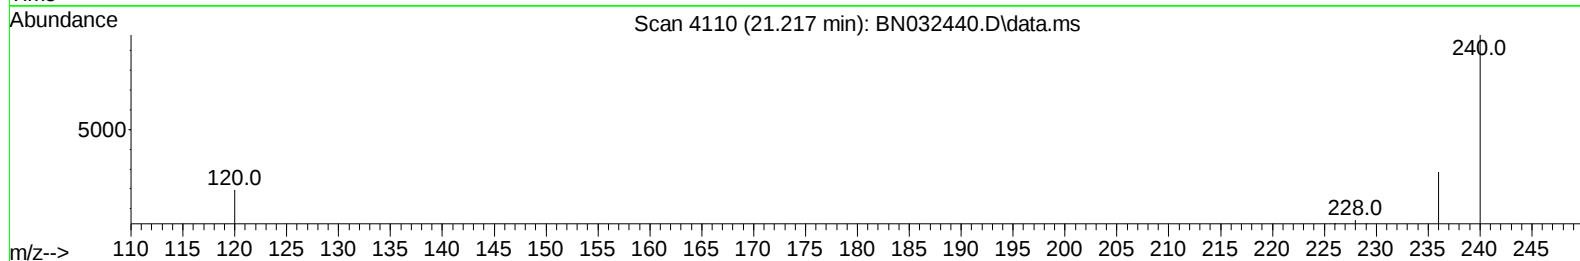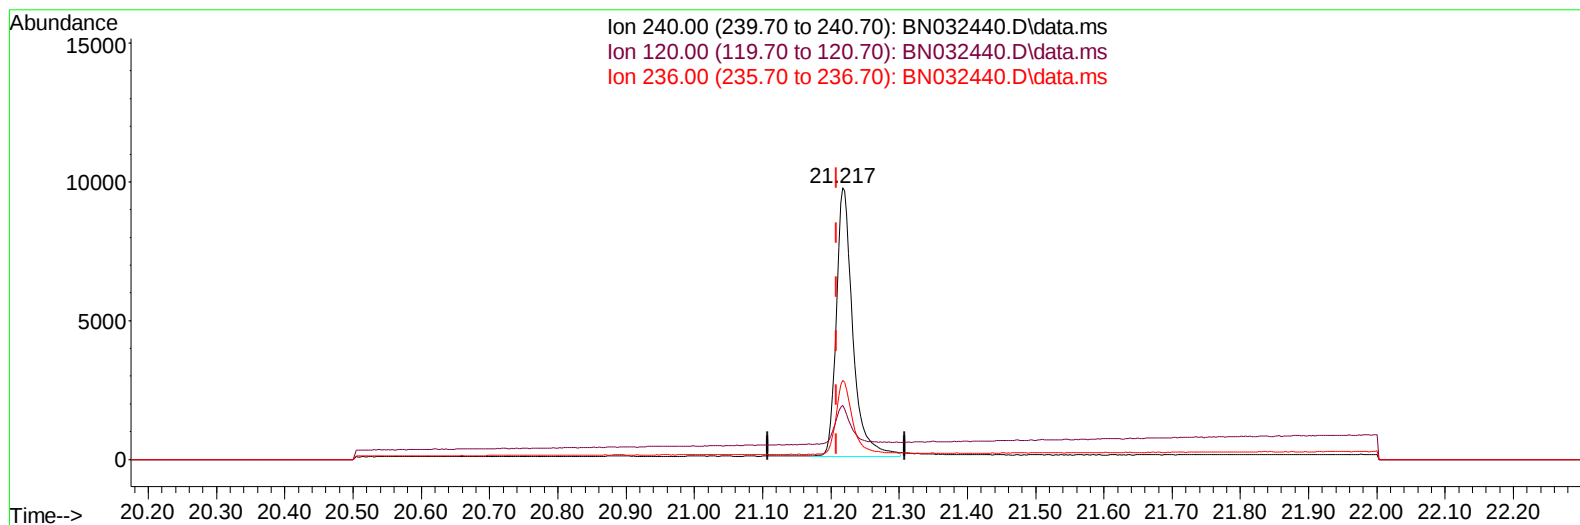

TIC: BN032440.D\data.ms

(17) Chrysene-d12

21.217min (+ 0.009) 0.40 ng/ul m

response 16281

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	19.90
236.00	28.40	29.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032440.D
Acq On : 03 Jul 2024 17:34
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 03 18:01:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

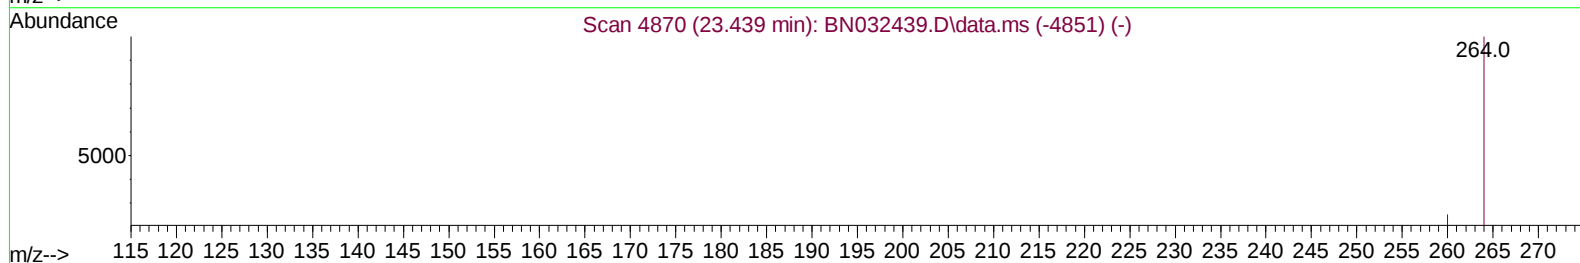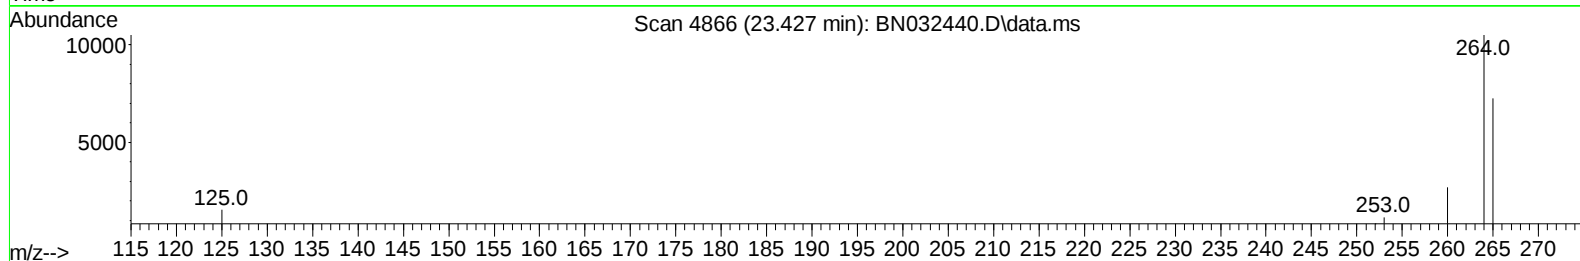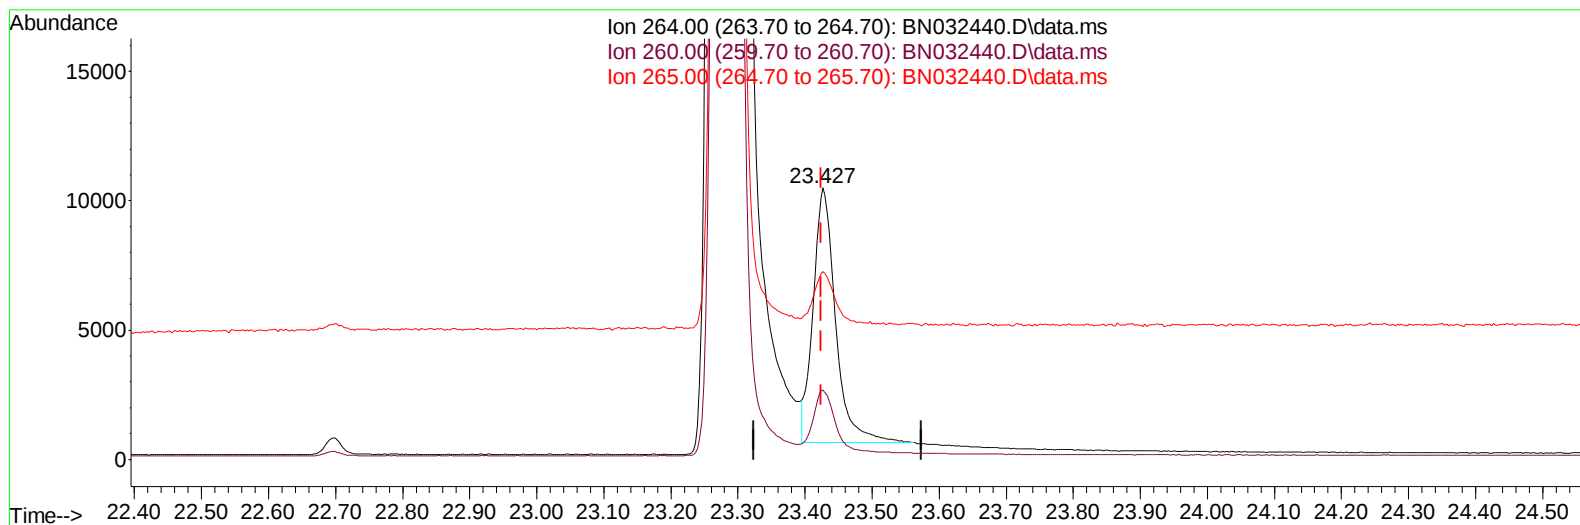

TIC: BN032440.D\data.ms

(23) Perylene-d12 (I)

23.427min (+ 0.003) 0.40 ng/u1

response 22845

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.71
265.00	67.20	69.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032440.D
Acq On : 03 Jul 2024 17:34
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 03 18:01:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

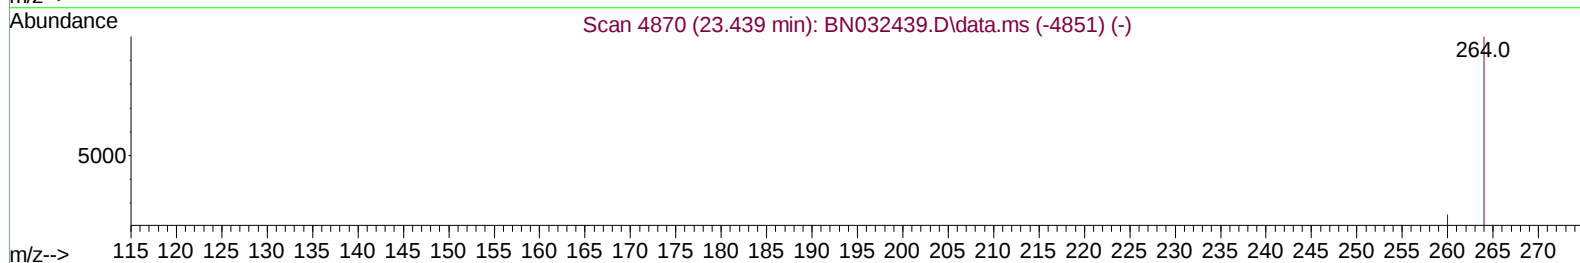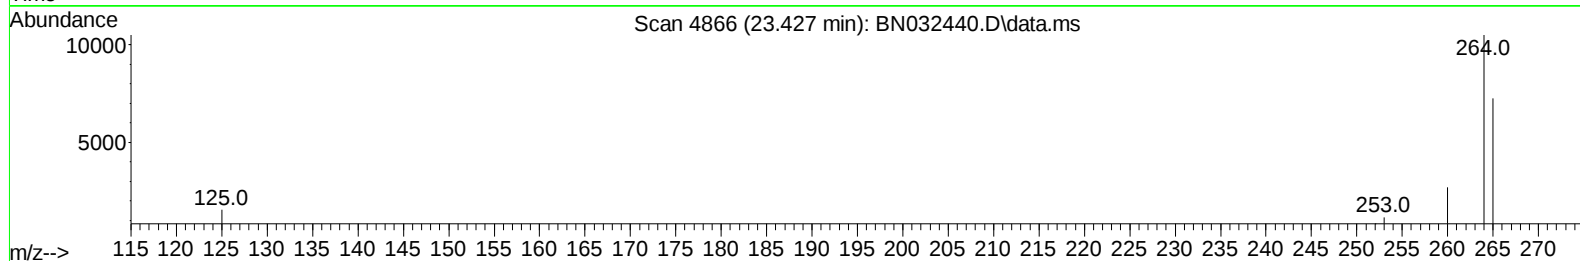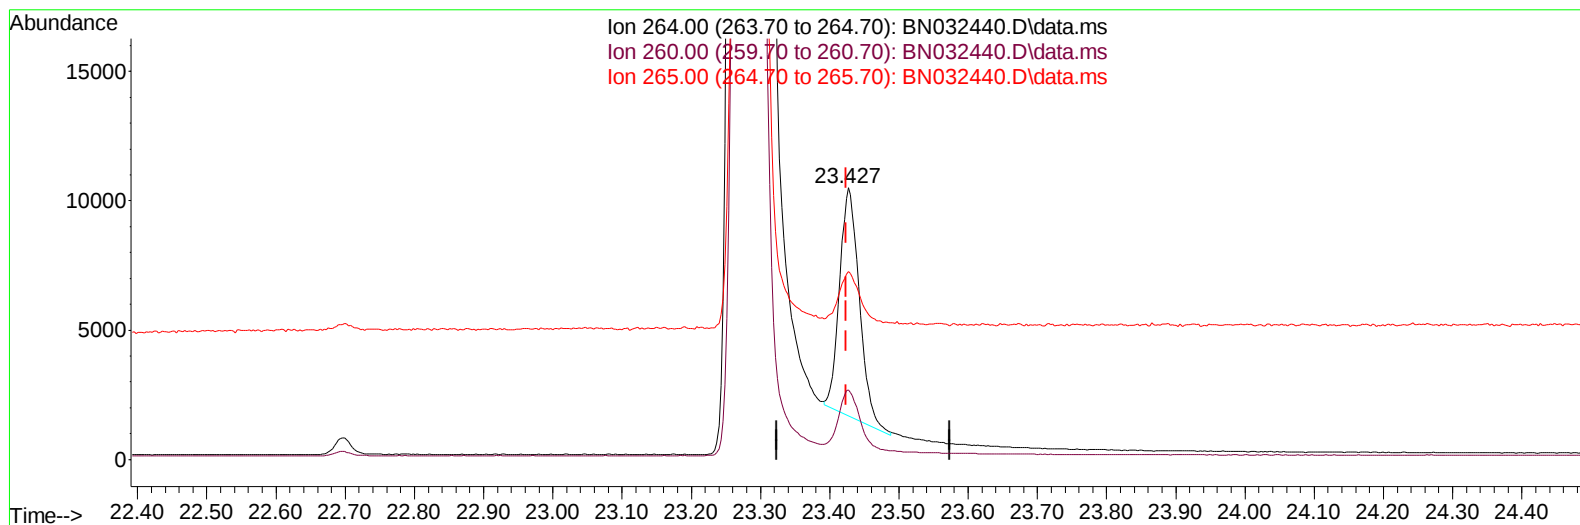

TIC: BN032440.D\data.ms

(23) Perylene-d12 (I)

23.427min (+ 0.003) 0.40 ng/ul m

response 17369

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.71
265.00	67.20	69.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
 Data File : BN032440.D
 Acq On : 03 Jul 2024 17:34
 Operator : MA/JU
 Sample : PB161653BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK653

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
 Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 03 18:01:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	6360	0.400	ng/ul	0.00
4) Naphthalene-d8	10.376	136	19852	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.249	164	11856	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.003	188	22555m	0.400	ng/ul	0.00
17) Chrysene-d12	21.217	240	16281m	0.400	ng/ul	0.00
23) Perylene-d12	23.427	264	17369m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.144	96	36600	5.177	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.982	152	7812	0.262	ng/ul	0.00
18) Fluoranthene-d10	19.045	212	14833	0.303	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032440.D
Acq On : 03 Jul 2024 17:34
Operator : MA/JU
Sample : PB161653BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK653

Manual IntegrationsAPPROVED

Quant Time: Jul 03 18:01:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

