




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032458.D
Acq On : 04 Jul 2024 04:58
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 04 05:26:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

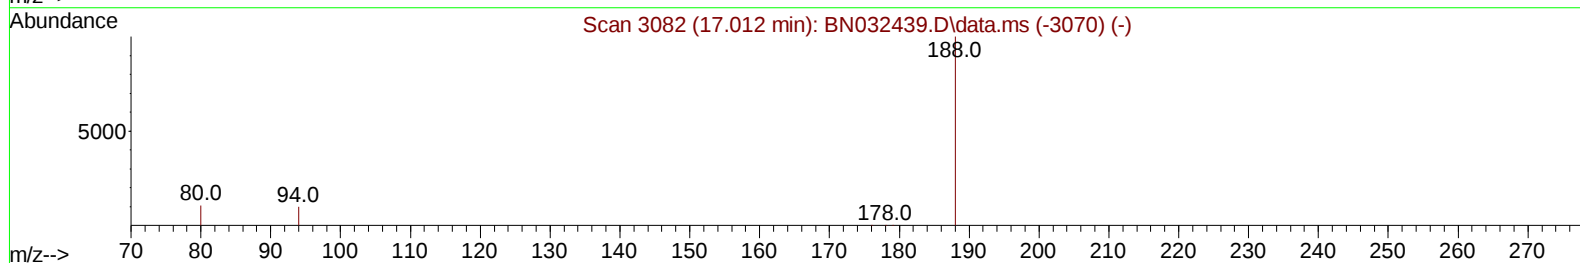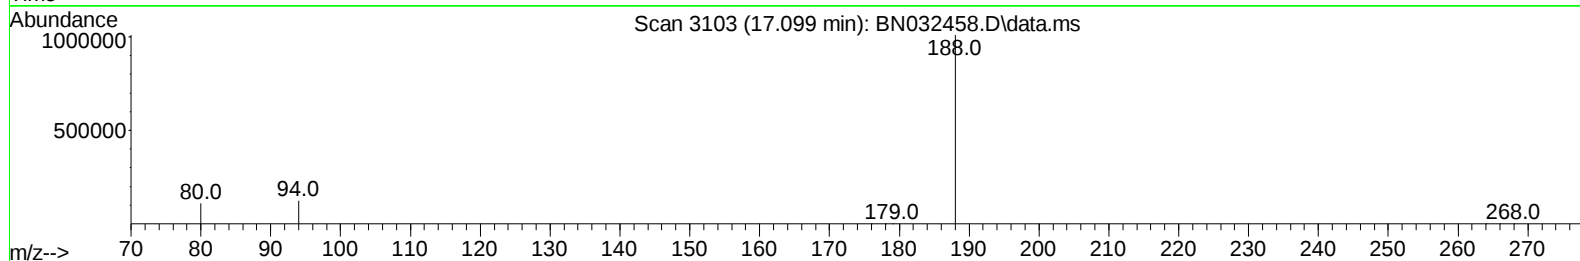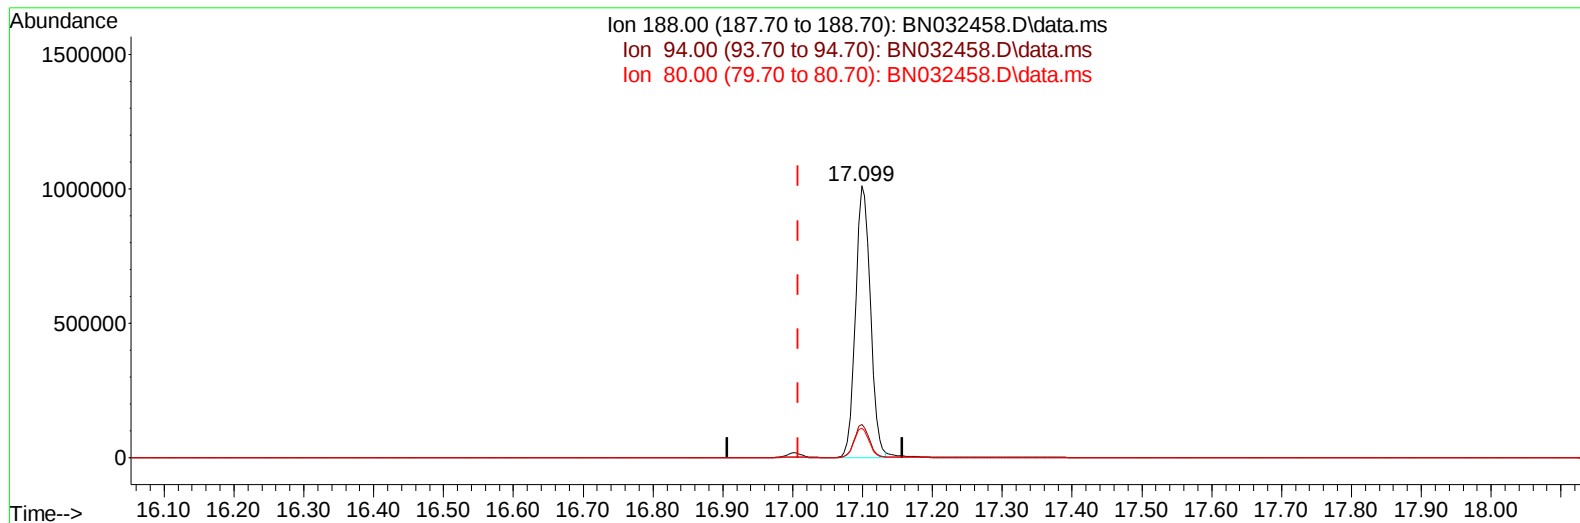

TIC: BN032458.D\data.ms

(13) Phenanthrene-d10 (I)

17.099min (+ 0.091) 0.40 ng/u1

response 1499057

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	12.20
80.00	10.50	10.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032458.D
Acq On : 04 Jul 2024 04:58
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 04 05:26:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

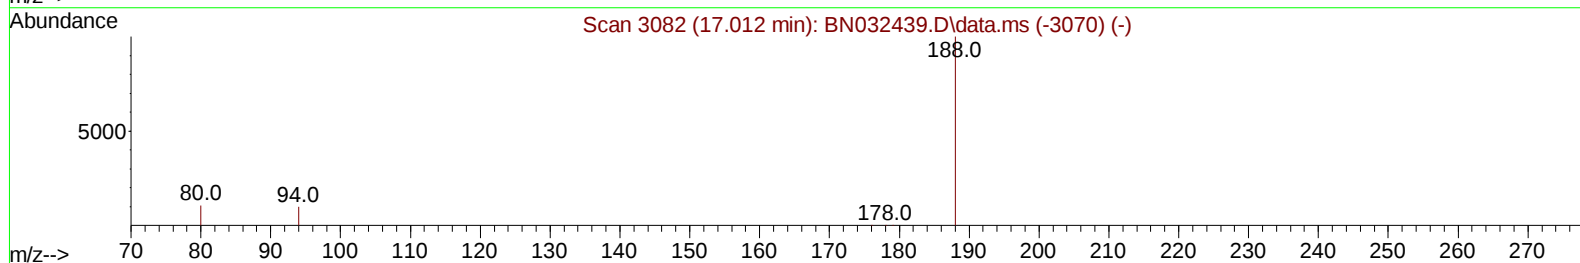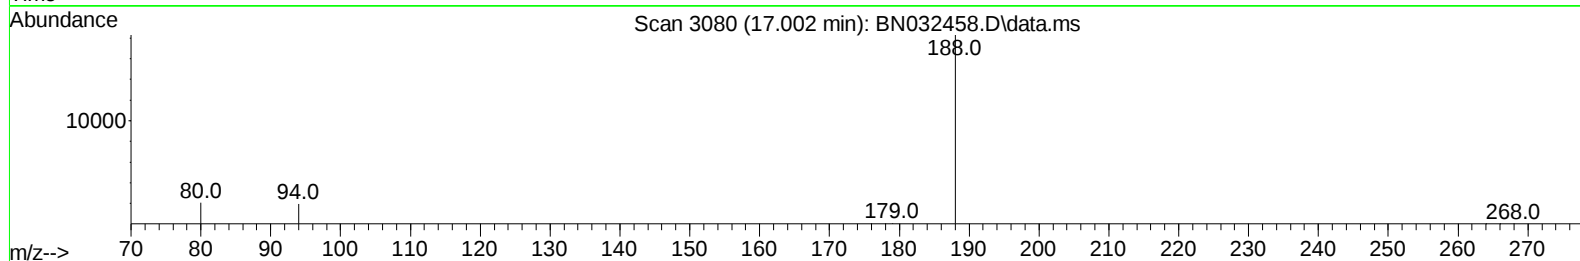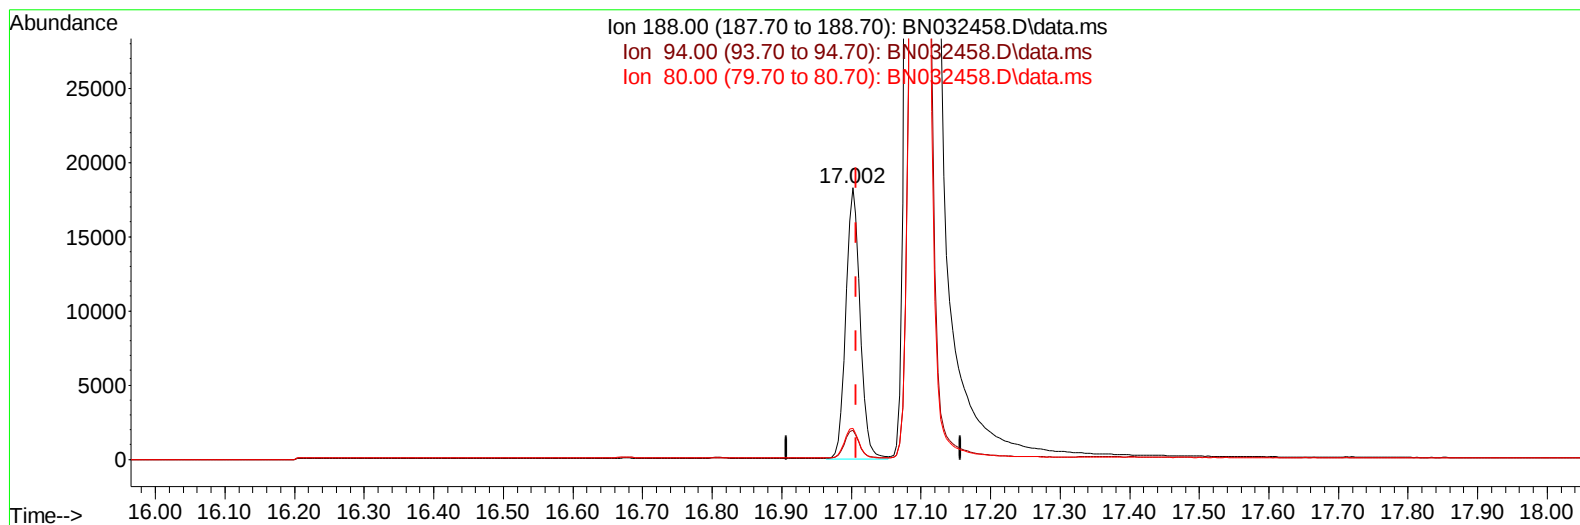

TIC: BN032458.D\data.ms

(13) Phenanthrene-d10 (I)

17.002min (-0.006) 0.40 ng/u1 m

response 25869

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	10.73
80.00	10.50	11.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032458.D
Acq On : 04 Jul 2024 04:58
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 04 05:26:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

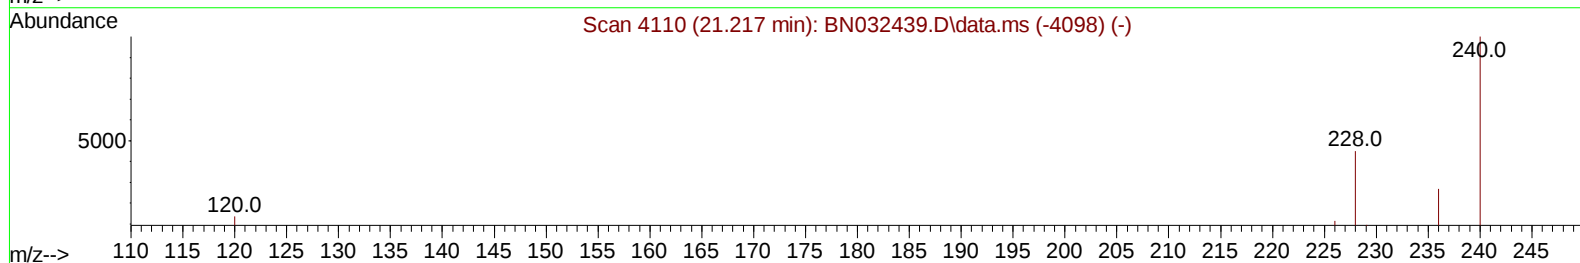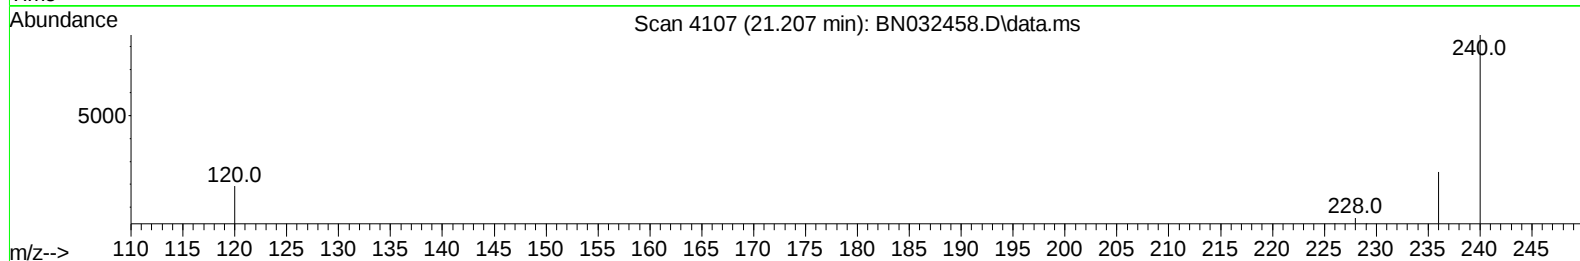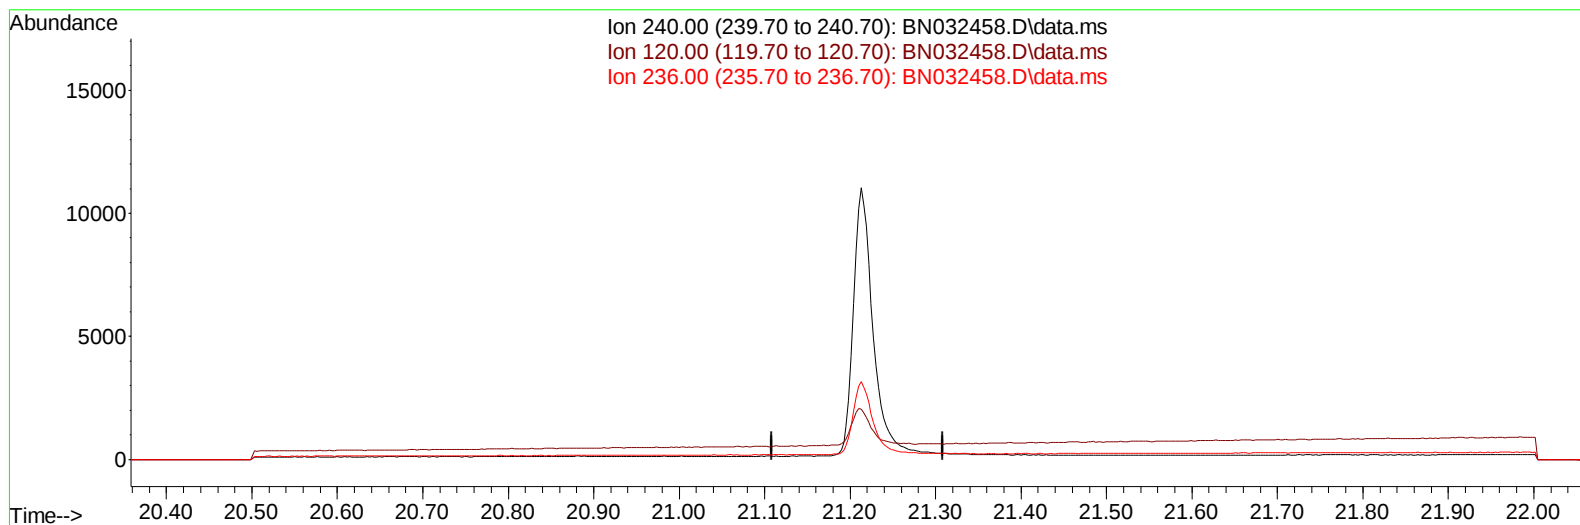

TIC: BN032458.D\data.ms

(17) Chrysene-d12

21.209min (-21.209) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.80	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032458.D
Acq On : 04 Jul 2024 04:58
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 04 05:26:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

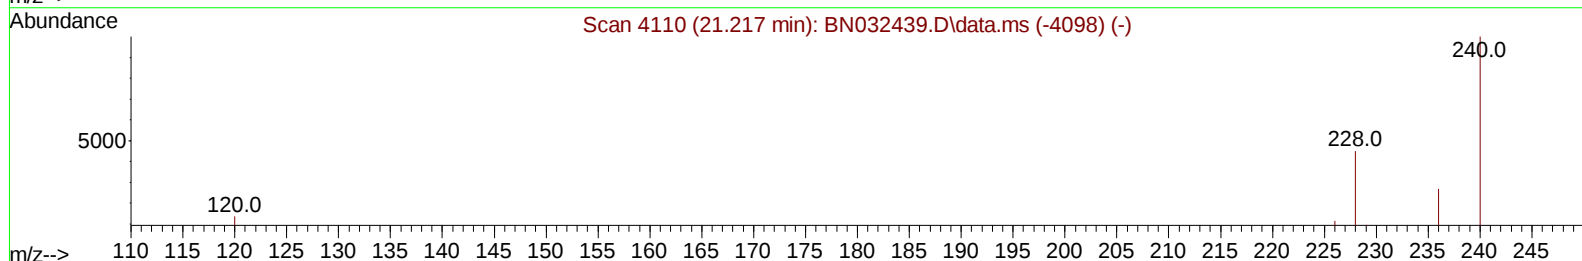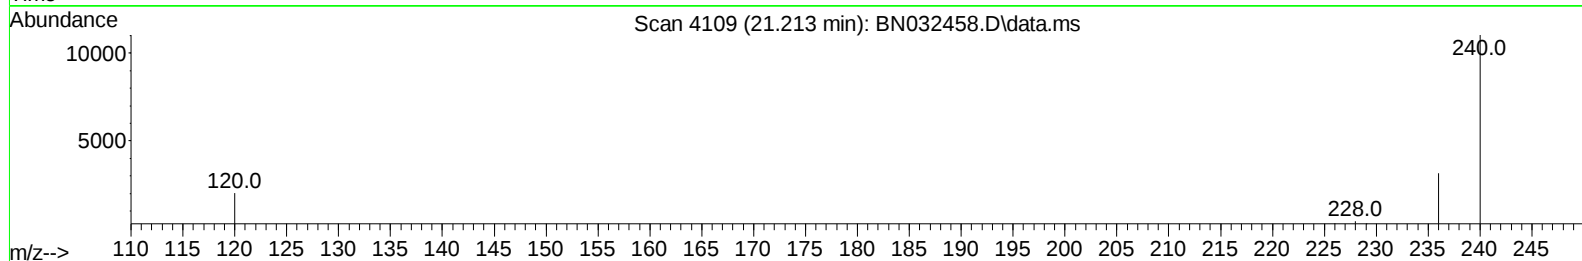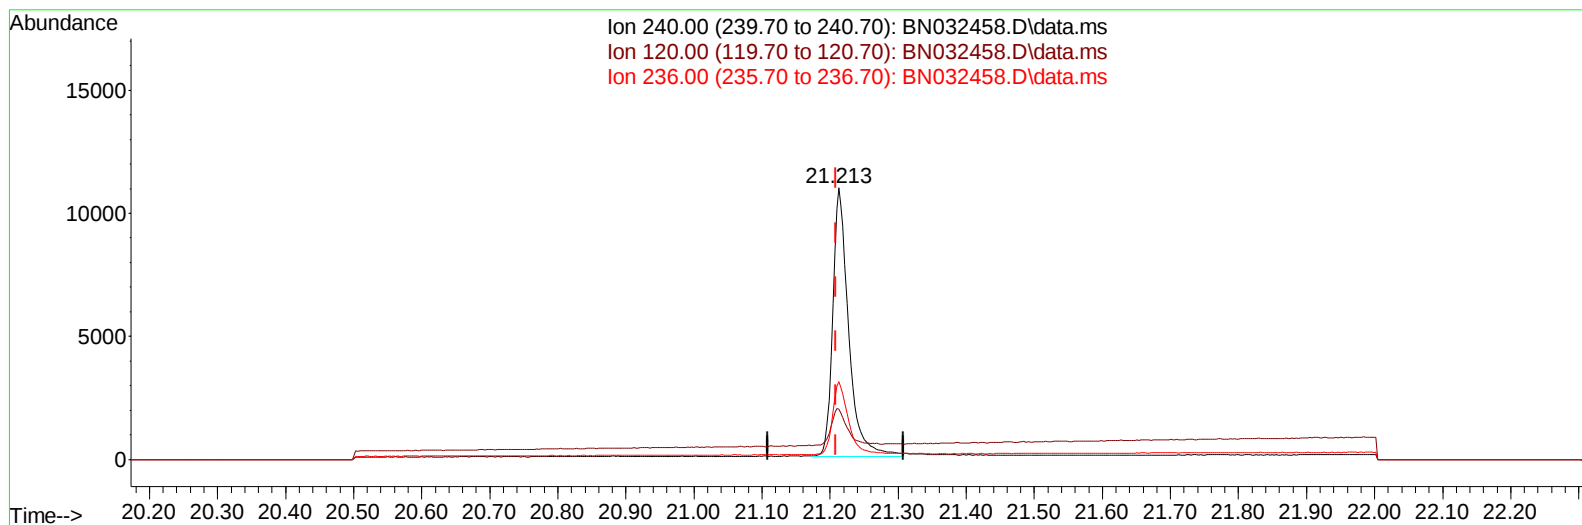

TIC: BN032458.D\data.ms

(17) Chrysene-d12

21.213min (+ 0.004) 0.40 ng/ul m

response 17794

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	18.43
236.00	28.40	28.75
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032458.D
Acq On : 04 Jul 2024 04:58
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 04 05:26:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

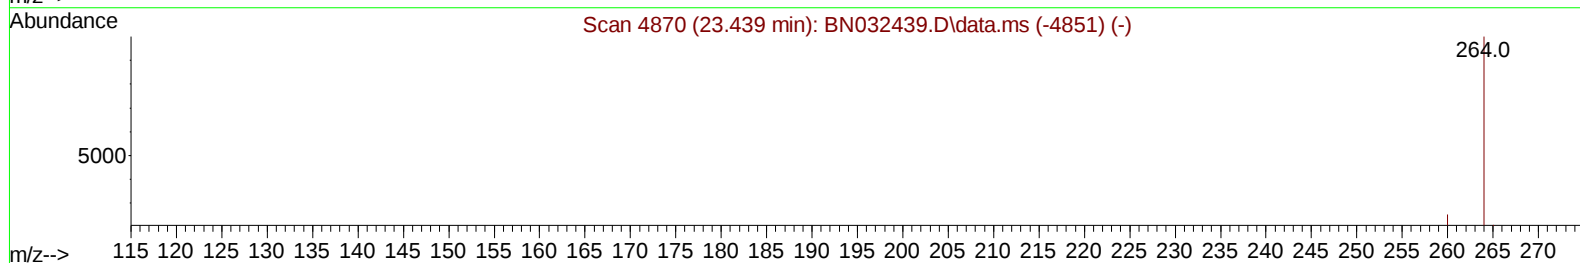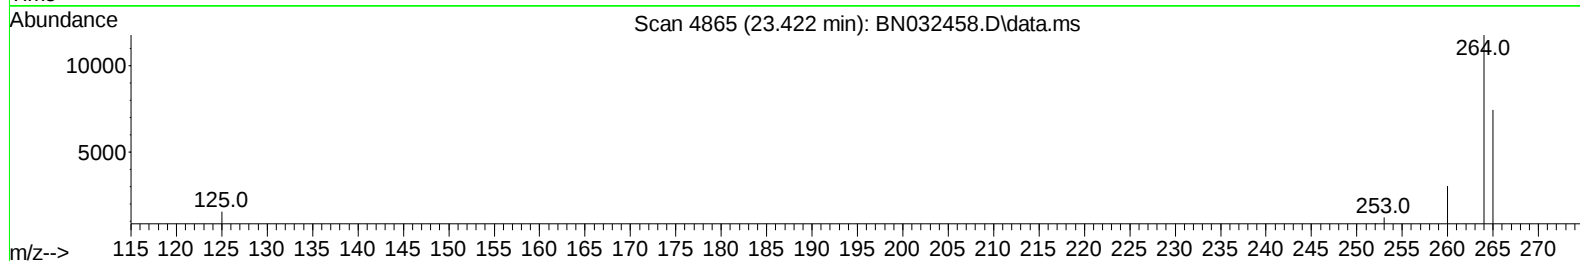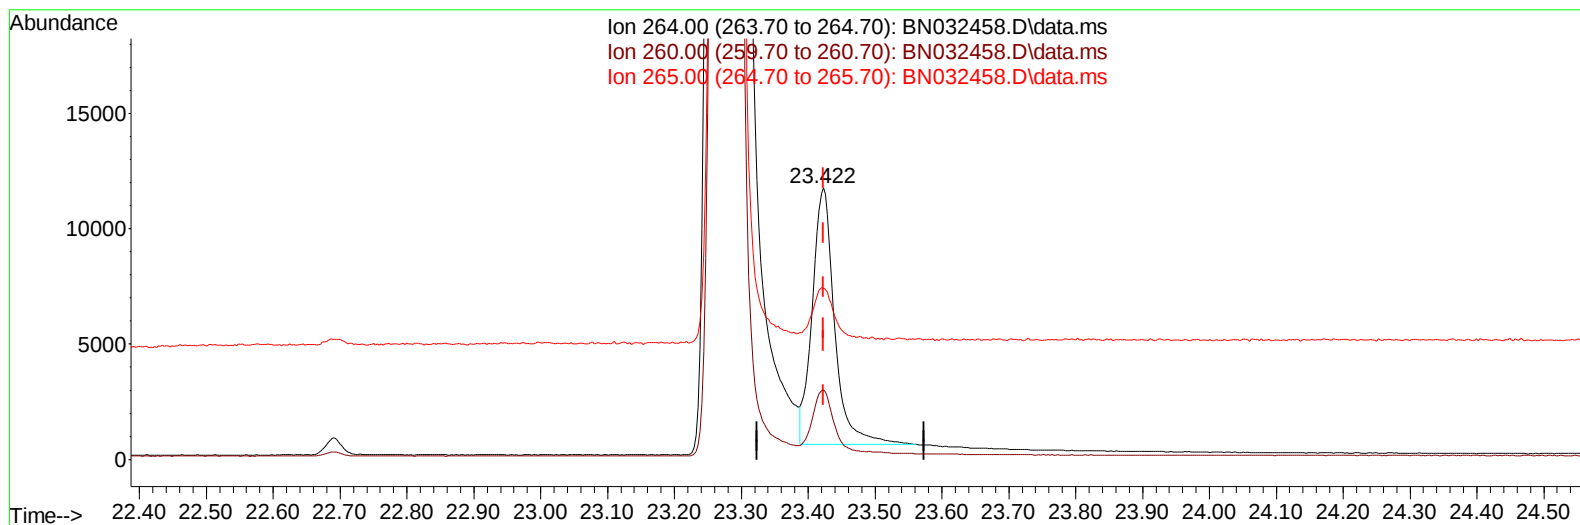

TIC: BN032458.D\data.ms

(23) Perylene-d12 (I)

23.422min (-0.001) 0.40 ng/u1

response 25680

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.69
265.00	67.20	63.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032458.D
Acq On : 04 Jul 2024 04:58
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 04 05:26:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

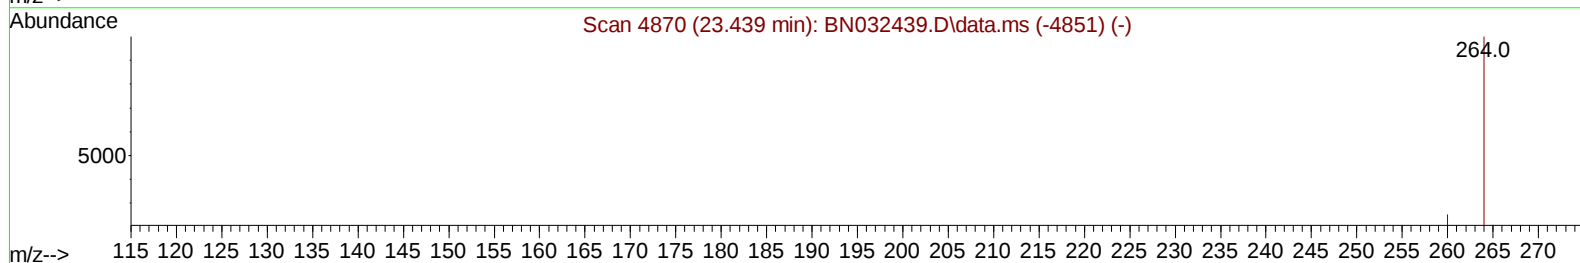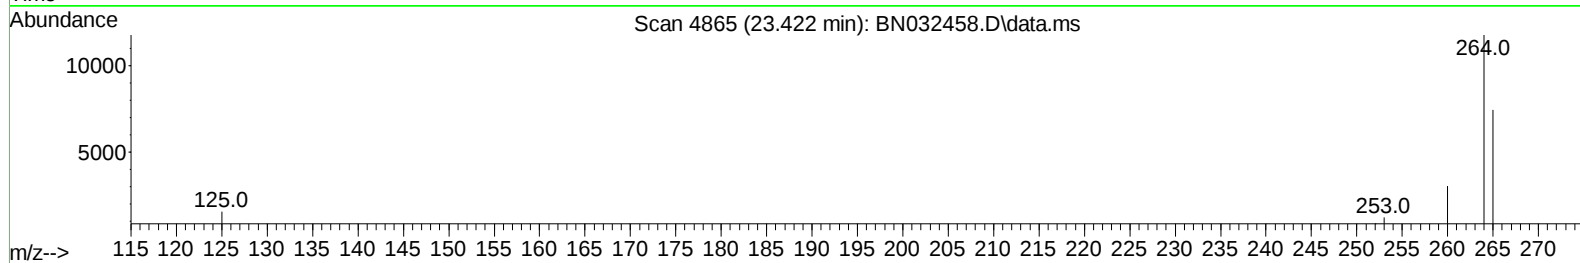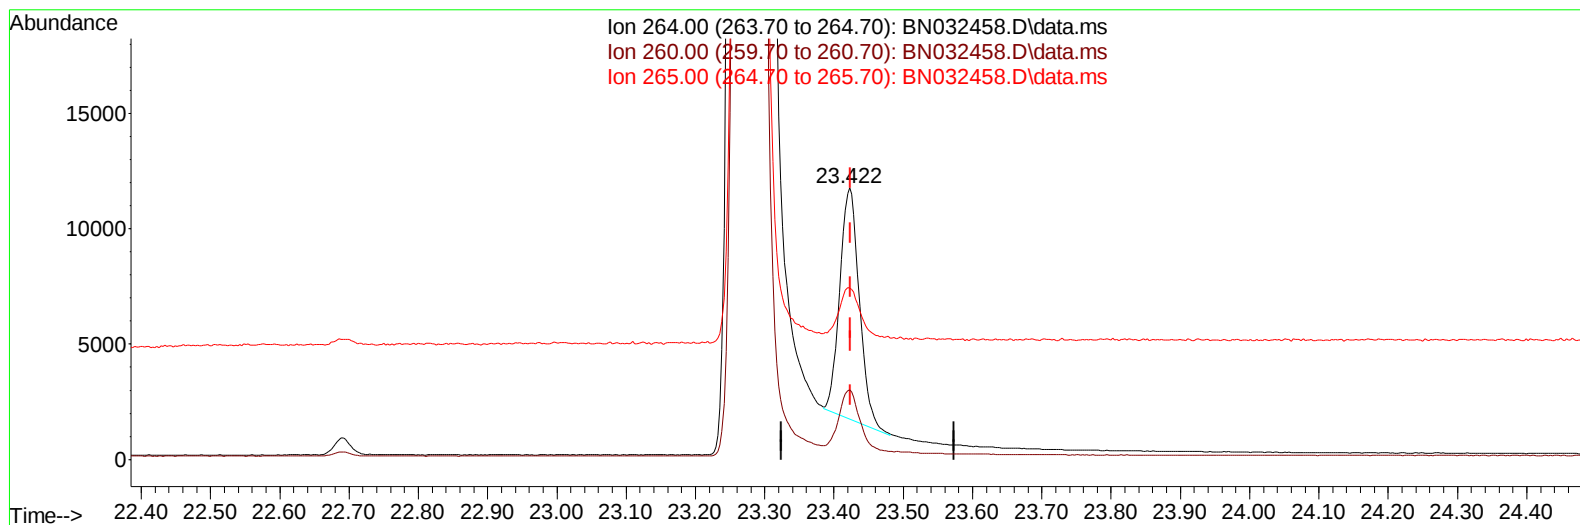

TIC: BN032458.D\data.ms

(23) Perylene-d12 (I)

23.422min (-0.001) 0.40 ng/ul m

response 19518

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.69
265.00	67.20	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
 Data File : BN032458.D
 Acq On : 04 Jul 2024 04:58
 Operator : MA/JU
 Sample : PB161629BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK629

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
 Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 04 05:26:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.599	152	8101	0.400	ng/ul	0.00
4) Naphthalene-d8	10.375	136	25478	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.247	164	14579	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.002	188	25869m	0.400	ng/ul	0.00
17) Chrysene-d12	21.213	240	17794m	0.400	ng/ul	0.00
23) Perylene-d12	23.422	264	19518m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	45033	5.001	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.981	152	10172	0.266	ng/ul	0.00
18) Fluoranthene-d10	19.039	212	16790	0.314	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032458.D
Acq On : 04 Jul 2024 04:58
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 04 05:26:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

